

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062019\
 Data File : P0057336.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2019 23:15
 Operator : SM/SJ
 Sample : K3448-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 M-3(0-10)

Manual Integrations
 APPROVED

Ankita
 6/21/2019 3:30:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:10:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.233	3.558	888804	729752	23.216	22.128
2) SA Decachlor...	9.791	8.481	847127	589277	17.259	16.526m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062019\
Data File : PO057336.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2019 23:15
Operator : SM/SJ
Sample : K3448-04
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
M-3(0-10)


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:10:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

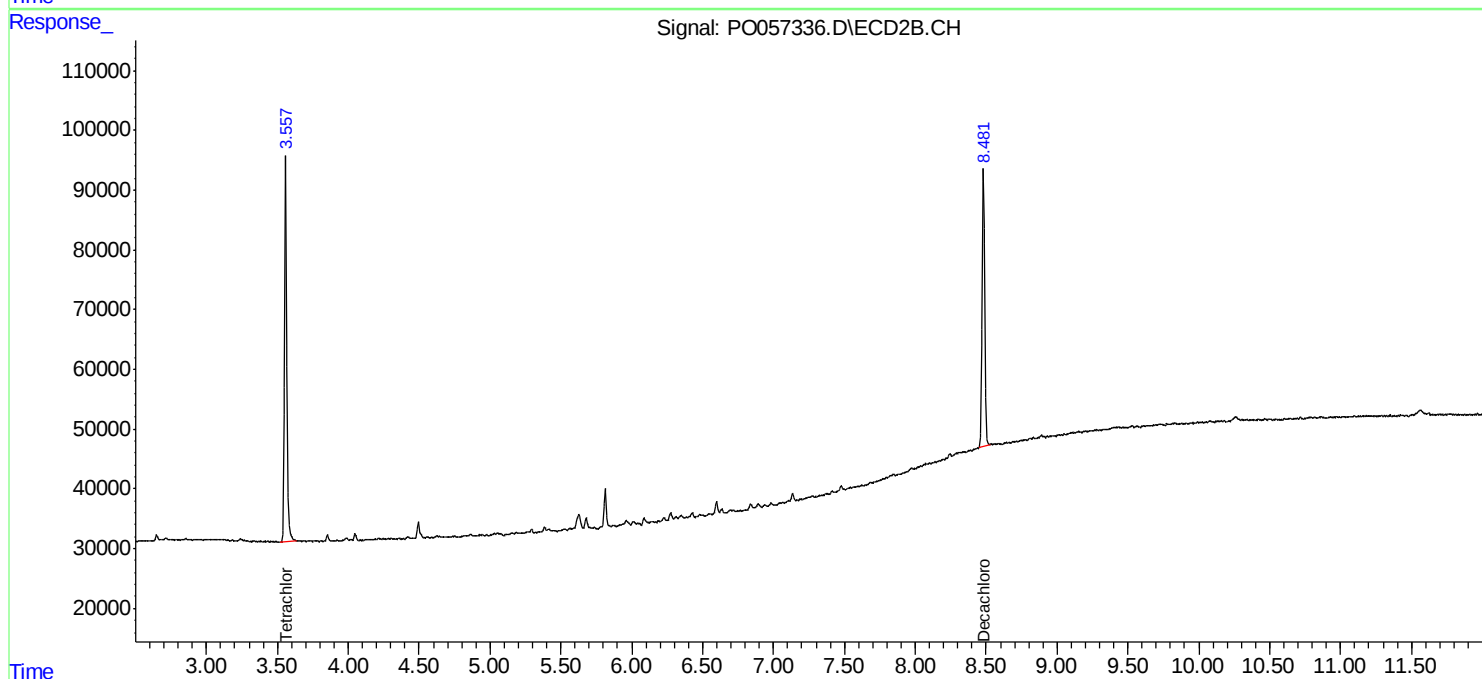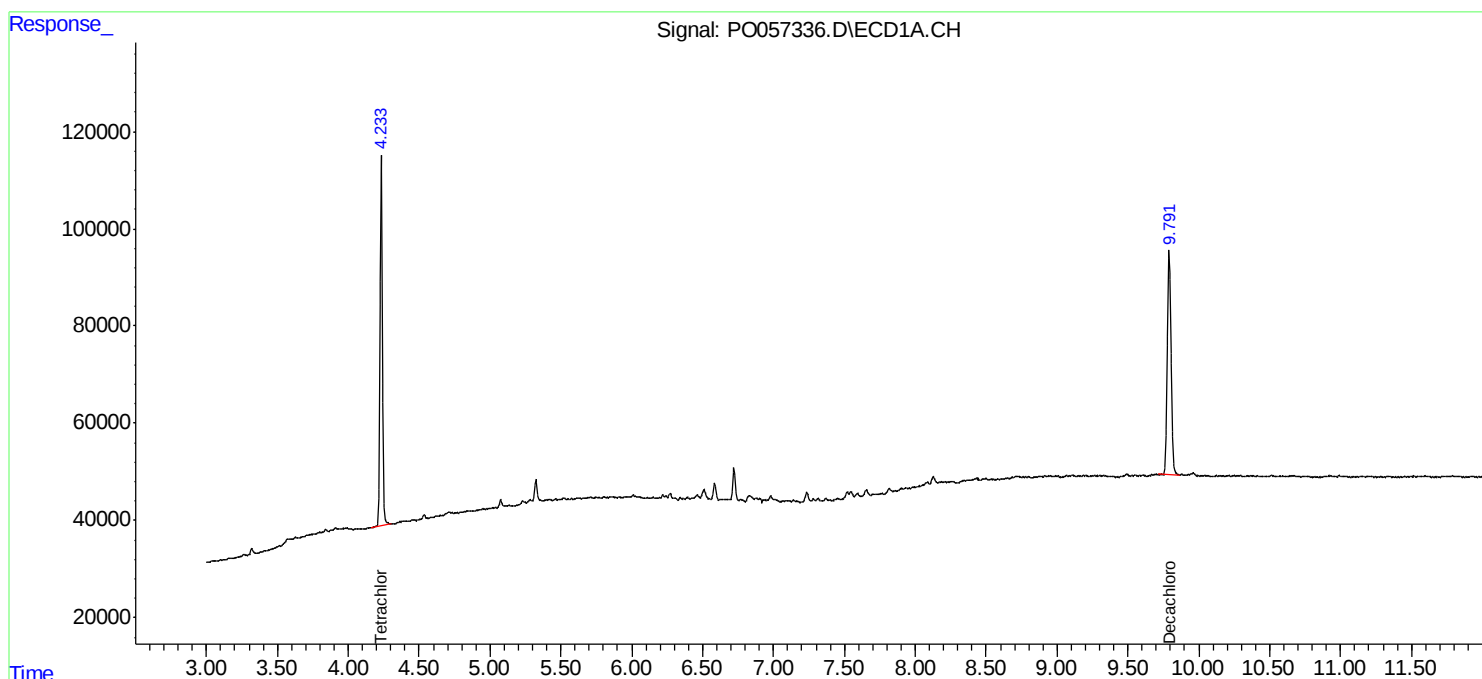

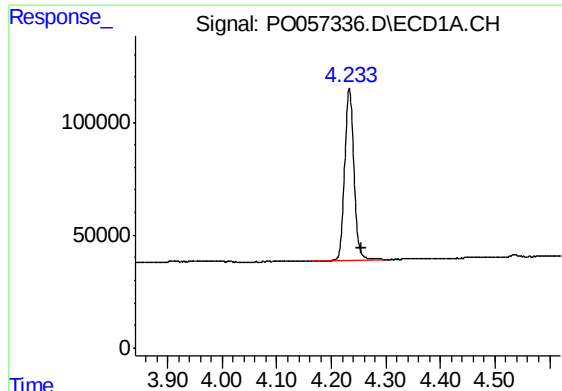


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.023 min
Response: 888804
Conc: 23.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
M-3(0-10)


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:36 PM

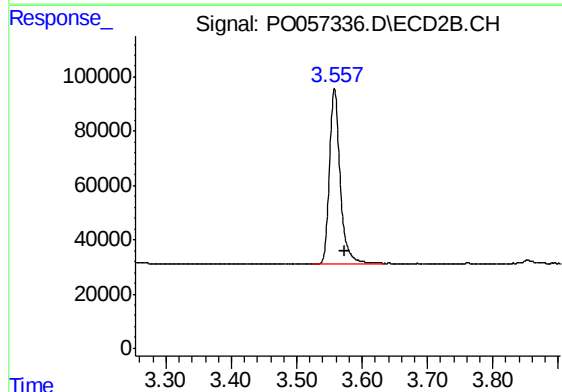


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: -0.015 min
Response: 729752
Conc: 22.13 ng/ml

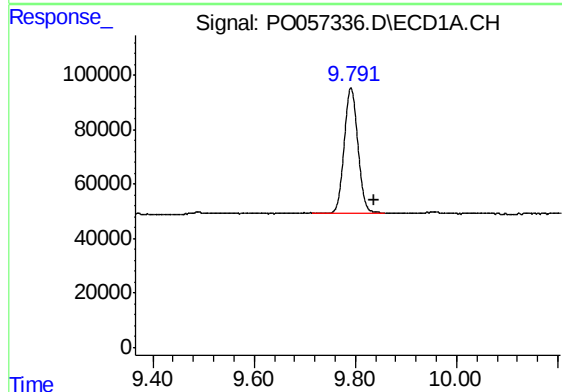

#2 Decachlorobiphenyl

R.T.: 9.791 min
Delta R.T.: -0.045 min
Response: 847127
Conc: 17.26 ng/ml

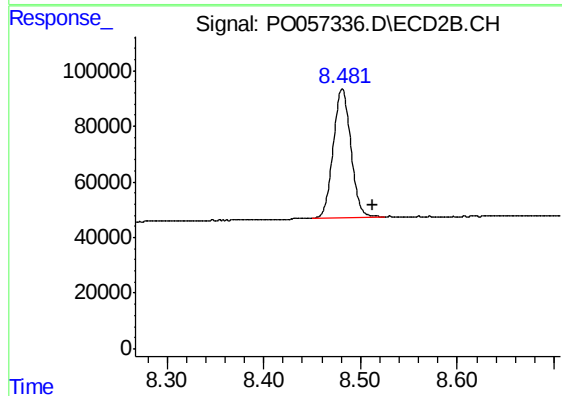

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.032 min
Response: 589277
Conc: 16.53 ng/ml m