

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062019\
 Data File : P0057345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 1:48
 Operator : SM/SJ
 Sample : K3455-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-5-DUCT-BANK

Manual Integrations
 APPROVED

Ankita
 6/21/2019 3:30:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 08:54:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.233	3.558	913748	736366	23.868	22.329
2)	SA Decachlor...	9.792	8.481	892274	600979	18.179	16.855m
Target Compounds							
26)	L6 AR-1254-1	6.238	5.414	208625	186311	75.788m	70.446
27)	L6 AR-1254-2	6.455	5.559	359687	216709	92.605	100.524m
28)	L6 AR-1254-3	6.821	5.958	444407	410805	107.777	112.209m
29)	L6 AR-1254-4	7.105	6.185	307361	213668	102.119m	97.257m
30)	L6 AR-1254-5	7.520	6.598	450967	424472	119.758m	133.893m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062019\
Data File : PO057345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 1:48
Operator : SM/SJ
Sample : K3455-09
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-5-DUCT-BANK


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 08:54:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

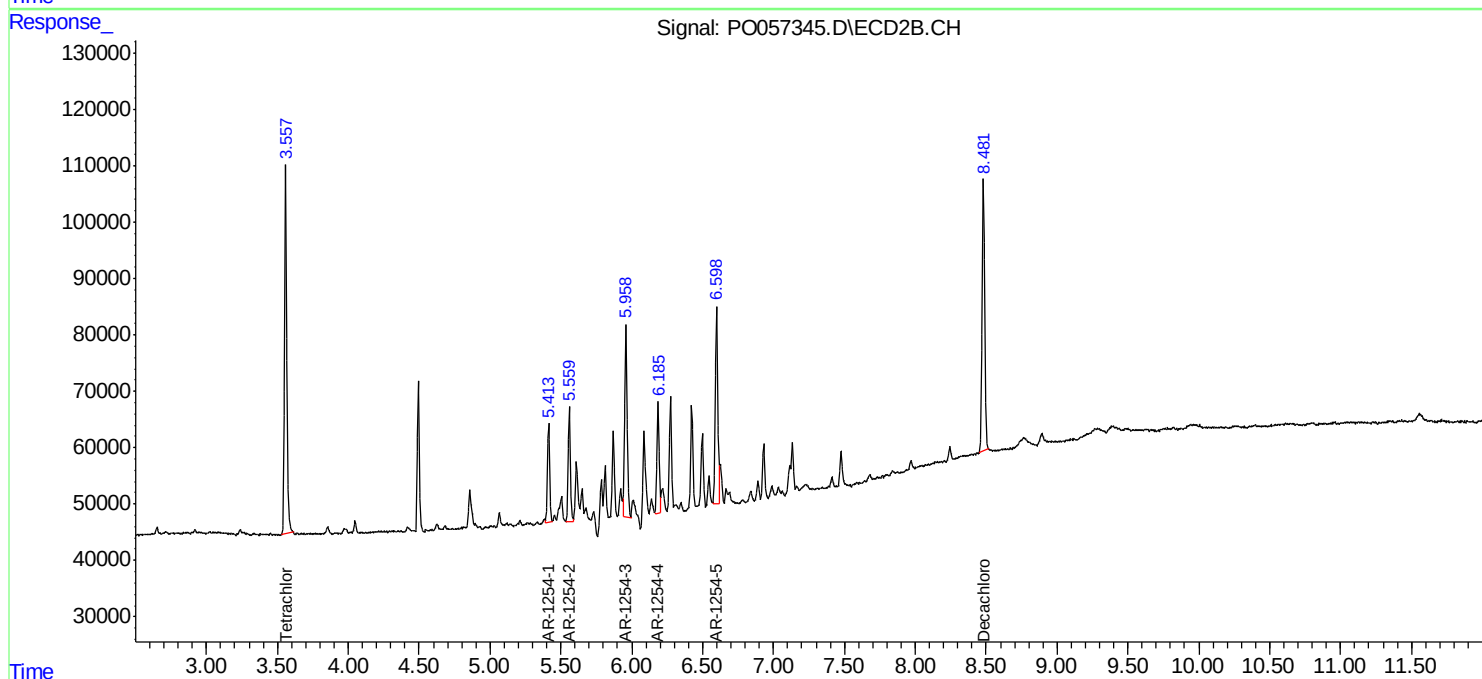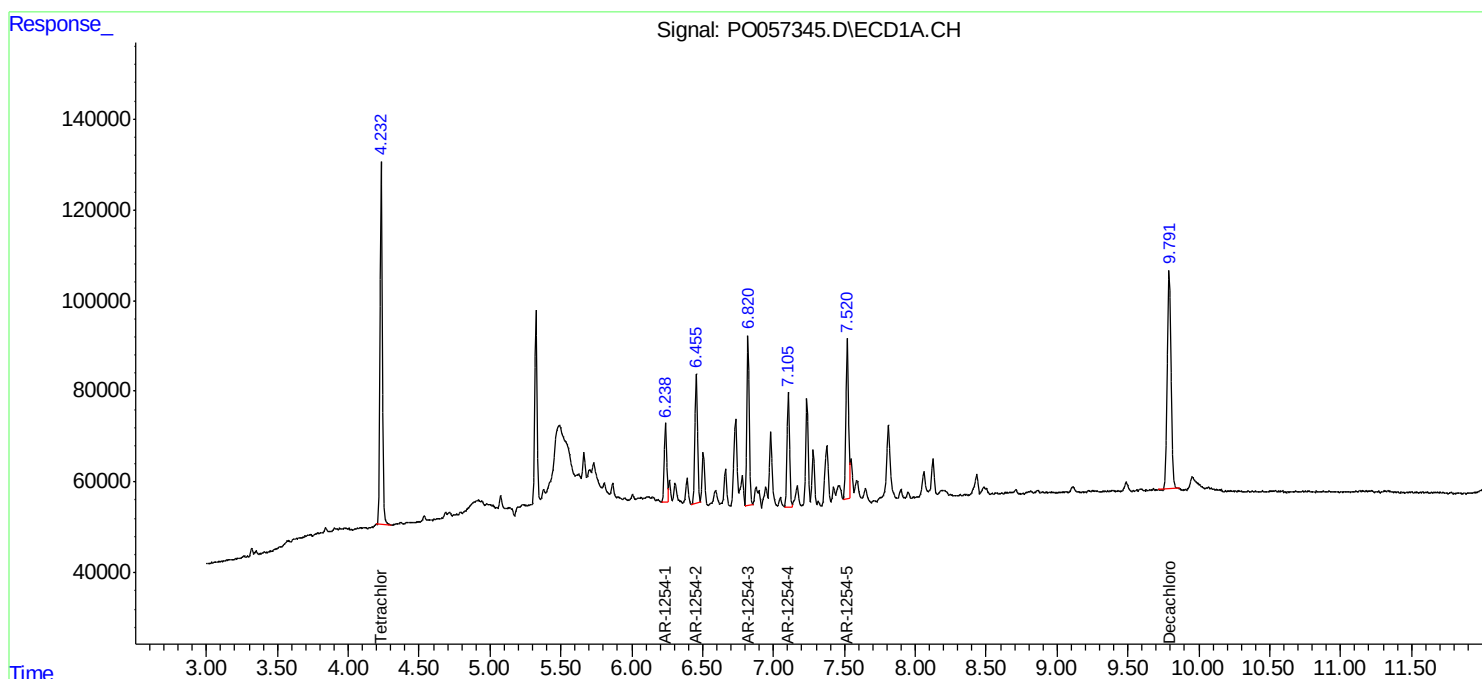

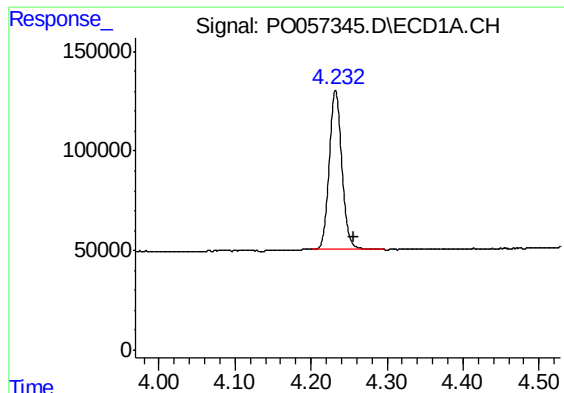


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.023 min
Response: 913748
Conc: 23.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-DUCT-BANK


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:53 PM

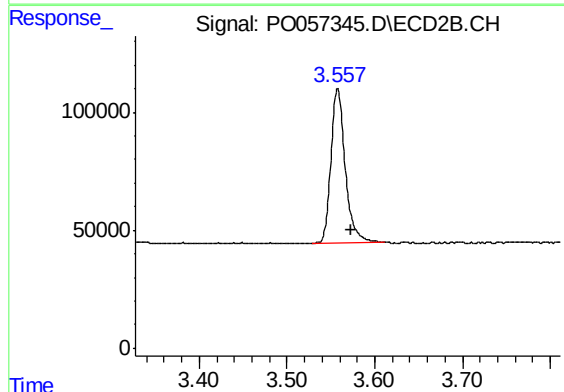


#1 Tetrachloro-m-xylene

R.T.: 3.558 min
Delta R.T.: -0.015 min
Response: 736366
Conc: 22.33 ng/ml

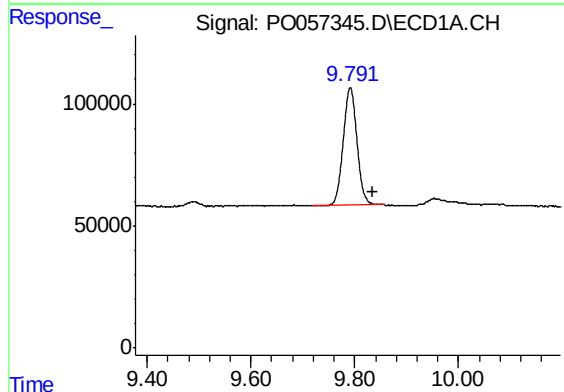


#2 Decachlorobiphenyl

R.T.: 9.792 min
Delta R.T.: -0.045 min
Response: 892274
Conc: 18.18 ng/ml

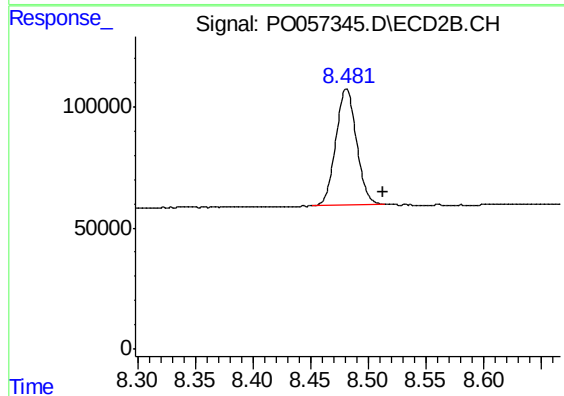

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.032 min
Response: 600979
Conc: 16.85 ng/ml m

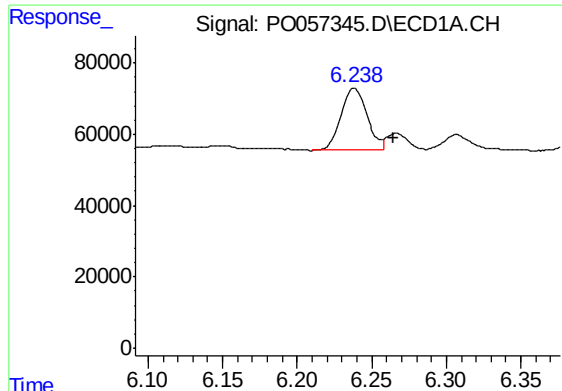


#26 AR-1254-1

R.T.: 6.238 min
Delta R.T.: -0.027 min
Response: 208625
Conc: 75.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-5-DUCT-BANK


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:53 PM

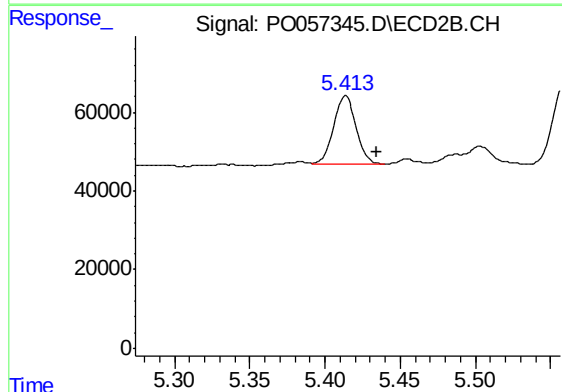


#26 AR-1254-1

R.T.: 5.414 min
Delta R.T.: -0.021 min
Response: 186311
Conc: 70.45 ng/ml

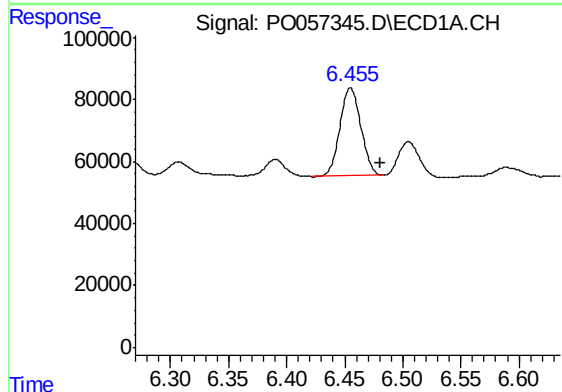


#27 AR-1254-2

R.T.: 6.455 min
Delta R.T.: -0.026 min
Response: 359687
Conc: 92.61 ng/ml

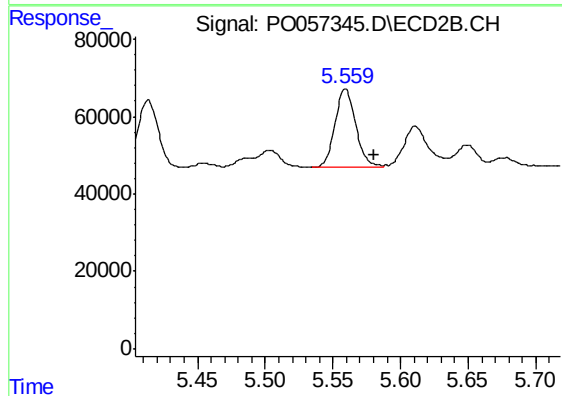

#27 AR-1254-2

R.T.: 5.559 min
Delta R.T.: -0.022 min
Response: 216709
Conc: 100.52 ng/ml m

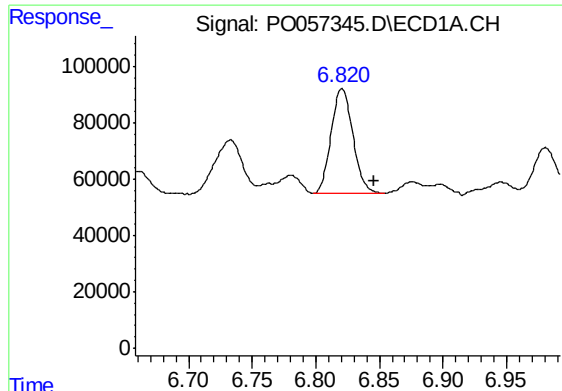


#28 AR-1254-3

R.T.: 6.821 min
Delta R.T.: -0.026 min
Response: 444407
Conc: 107.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-5-DUCT-BANK


Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:53 PM

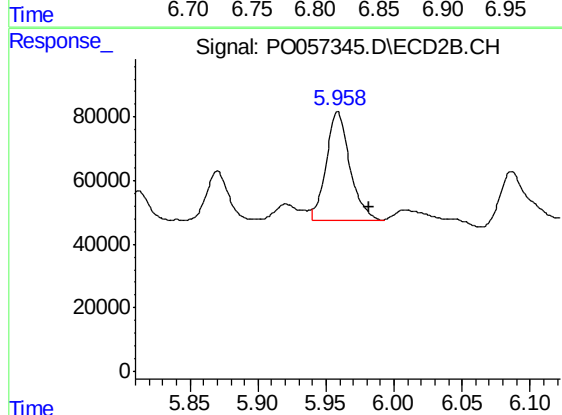


#28 AR-1254-3

R.T.: 5.958 min
Delta R.T.: -0.023 min
Response: 410805
Conc: 112.21 ng/ml m

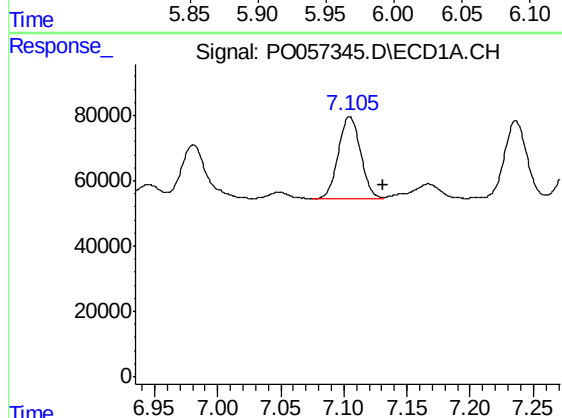


#29 AR-1254-4

R.T.: 7.105 min
Delta R.T.: -0.027 min
Response: 307361
Conc: 102.12 ng/ml m

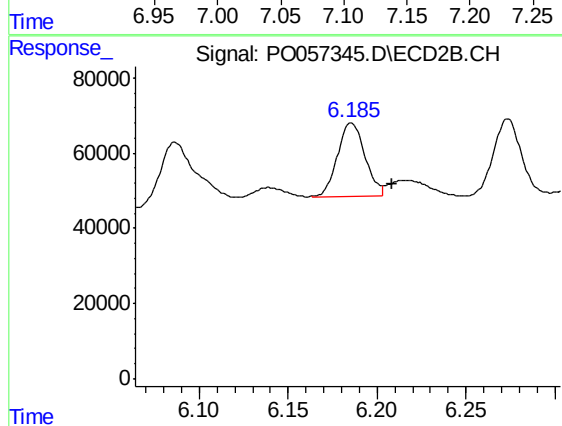

#29 AR-1254-4

R.T.: 6.185 min
Delta R.T.: -0.023 min
Response: 213668
Conc: 97.26 ng/ml m

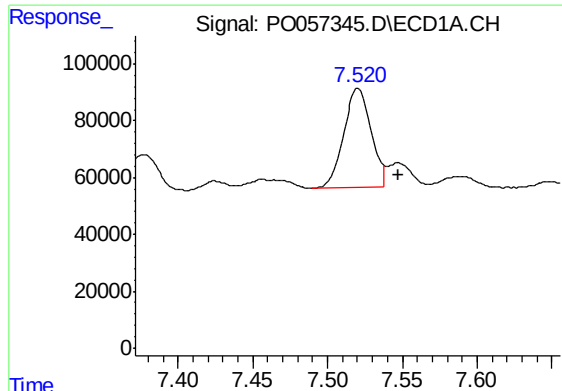


#30 AR-1254-5

R.T.: 7.520 min
Delta R.T.: -0.027 min
Response: 450967
Conc: 119.76 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-5-DUCT-BANK

Manual Integrations
APPROVED

Ankita
6/21/2019 3:30:53 PM

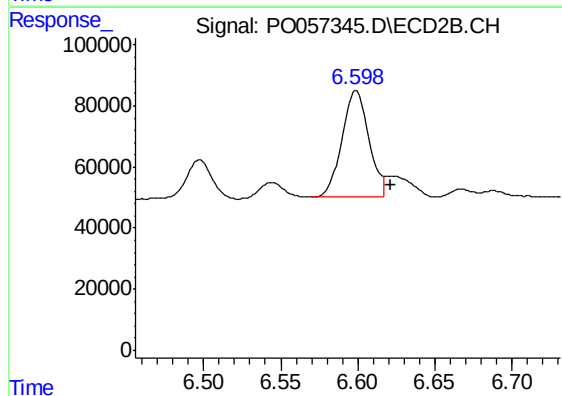

#30 AR-1254-5

R.T.: 6.598 min
Delta R.T.: -0.024 min
Response: 424472
Conc: 133.89 ng/ml m