

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062021\
 Data File : P0078953.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2021 11:03
 Operator : DD\AJ
 Sample : M2709-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-AMND-COMP-O(CL-24)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 05:24:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.329	3.606	1724124	645751	21.846	21.727
2)	SA Decachlor...	9.935	8.786	1277604	641843	20.457	21.539
Target Compounds							
5)	L1 AR-1016-3	5.715	0.000	67546	0	26.889	N.D. #
8)	L2 AR-1221-1	4.575	0.000	97636	0	117.443	N.D. #
9)	L2 AR-1221-2	4.670	3.926f	31103	7524	51.061	29.729 #
18)	L4 AR-1242-3	5.715	0.000	67546	0	36.498	N.D. #
24)	L5 AR-1248-4	6.555	0.000	113191	0	40.839	N.D. #
28)	L6 AR-1254-3	7.139f	6.245	37311	14636	8.378	6.580
29)	L6 AR-1254-4	7.420	0.000	34628	0	11.254	N.D. #
32)	L7 AR-1260-2	7.532f	0.000	33927	0	8.729	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062021\
Data File : PO078953.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2021 11:03
Operator : DD\AJ
Sample : M2709-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-O(CL-24)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 05:24:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

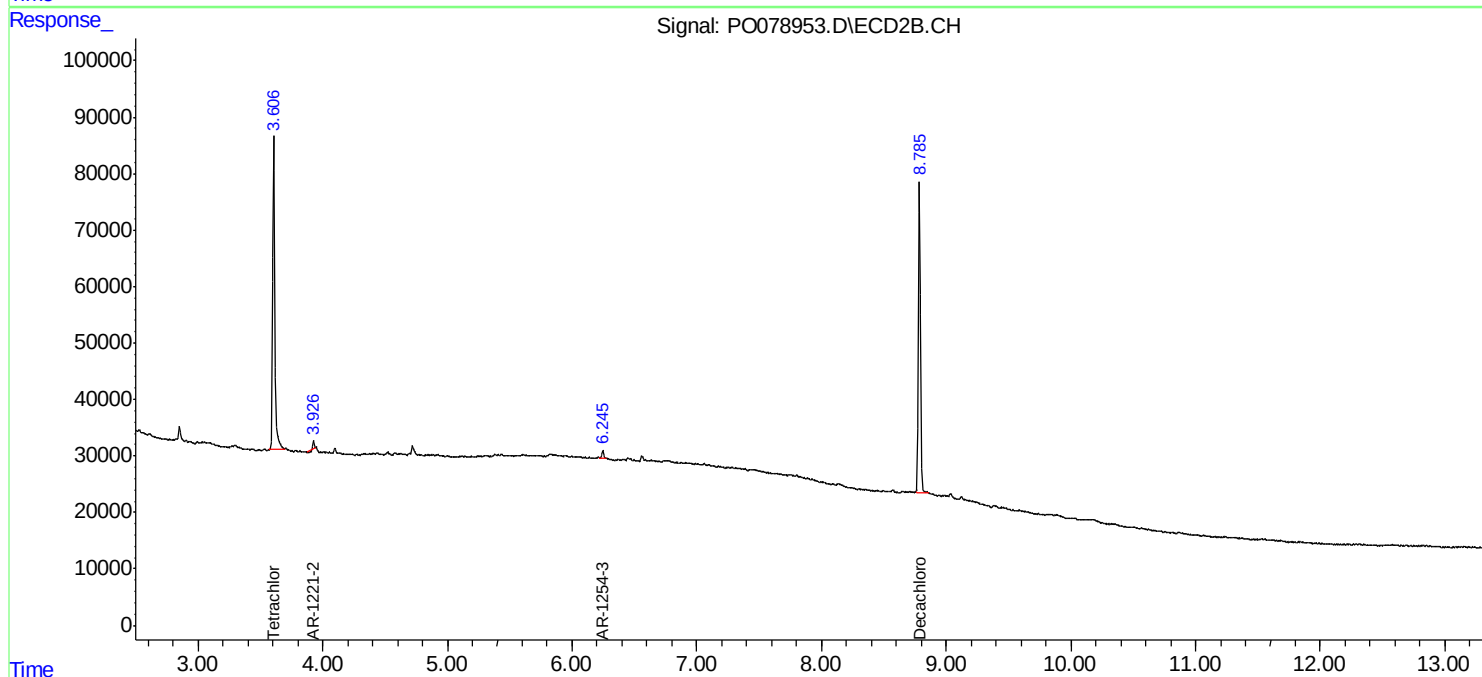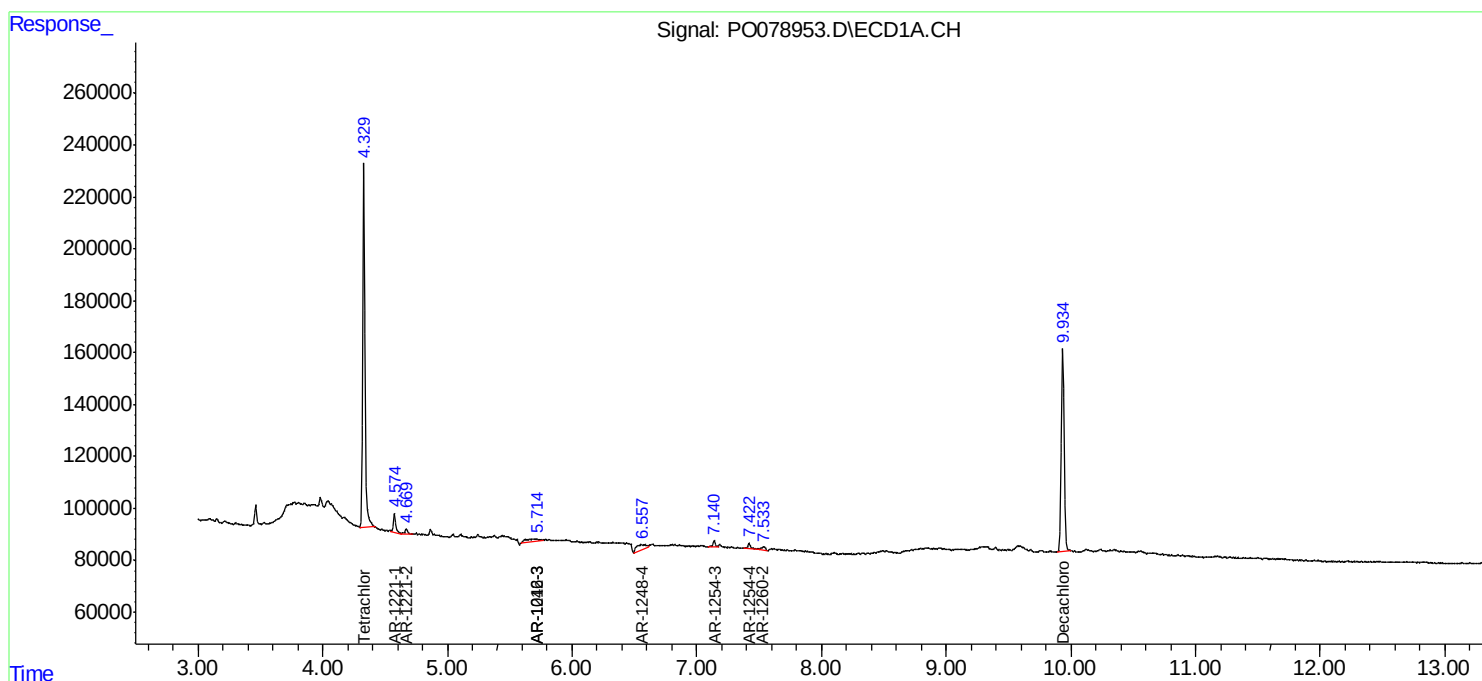


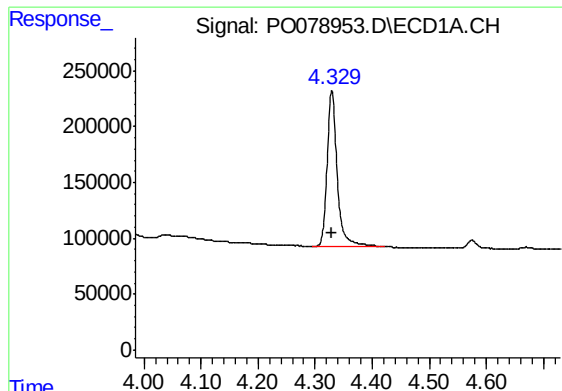

#1 Tetrachloro-m-xylene


R.T.: 4.329 min
Delta R.T.: 0.000 min
Response: 1724124
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-O(CL-24)

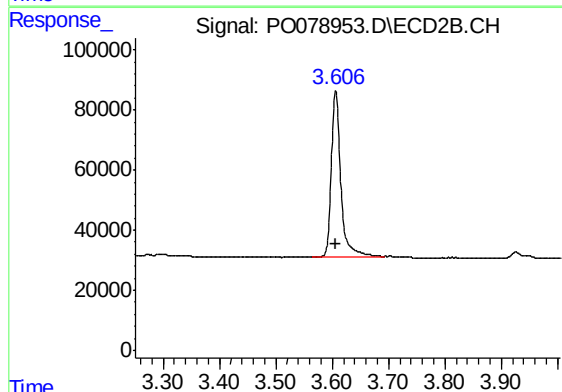


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 645751
Conc: 21.73 ng/ml

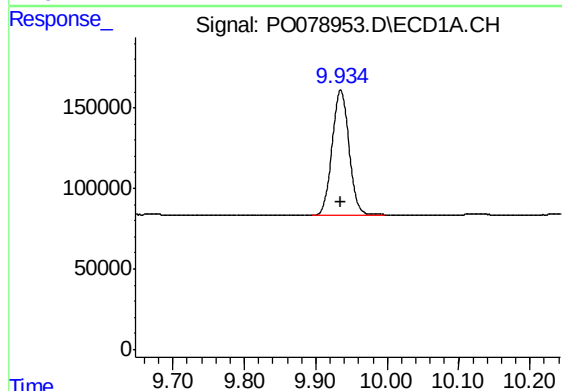


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: 0.000 min
Response: 1277604
Conc: 20.46 ng/ml

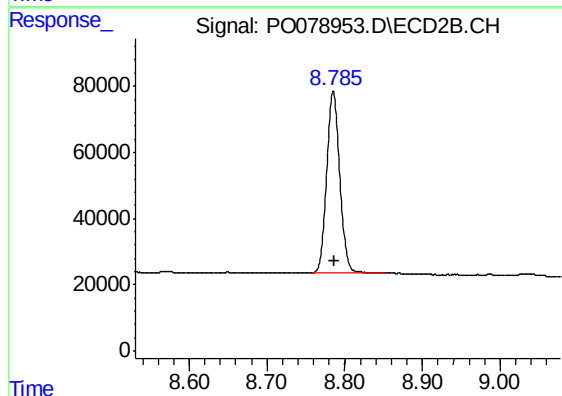

#2 Decachlorobiphenyl


R.T.: 8.786 min
Delta R.T.: -0.001 min
Response: 641843
Conc: 21.54 ng/ml

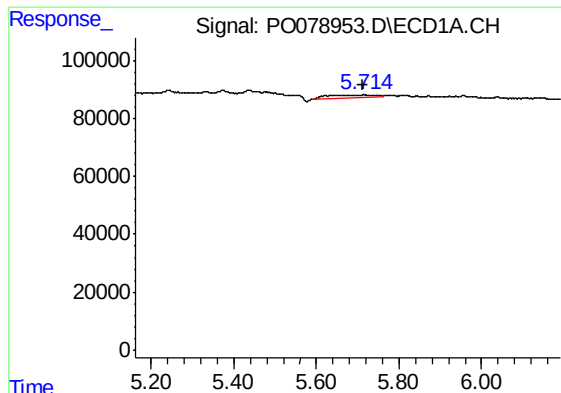

#5 AR-1016-3


R.T.: 5.715 min
Delta R.T.: 0.002 min
Response: 67546
Conc: 26.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-O(CL-24)

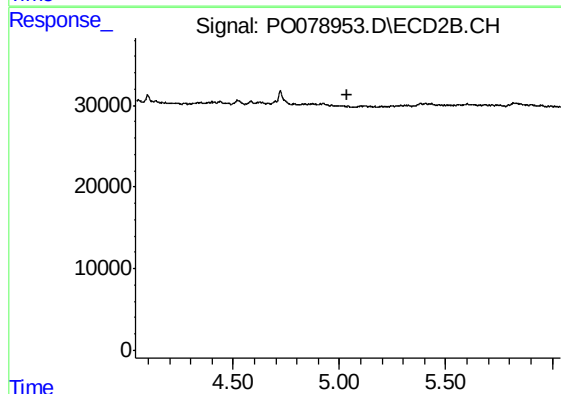


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

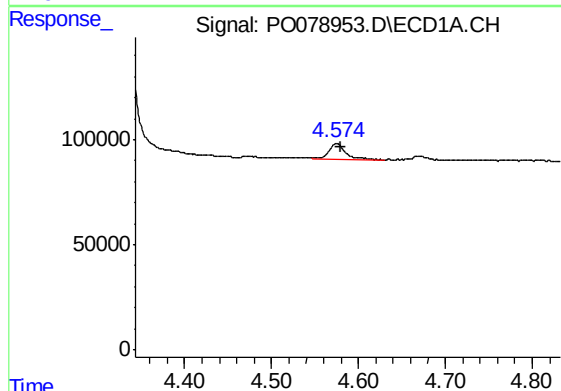


#8 AR-1221-1

R.T.: 4.575 min
Delta R.T.: -0.006 min
Response: 97636
Conc: 117.44 ng/ml

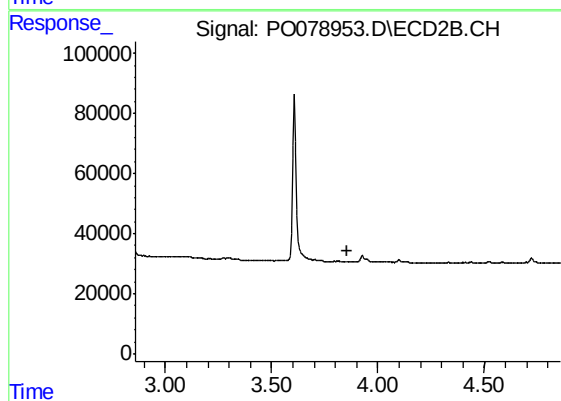

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.858 min
Response: 0
Conc: N.D.

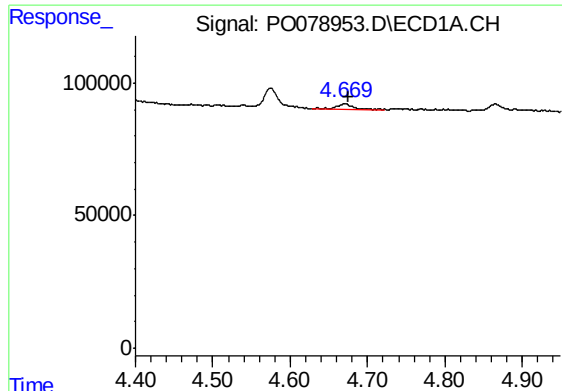

#9 AR-1221-2


R.T.: 4.670 min
Delta R.T.: -0.006 min
Response: 31103
Conc: 51.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-O(CL-24)

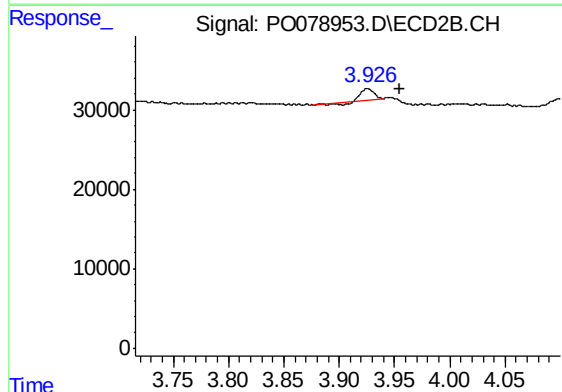


#9 AR-1221-2

R.T.: 3.926 min
Delta R.T.: -0.029 min
Response: 7524
Conc: 29.73 ng/ml

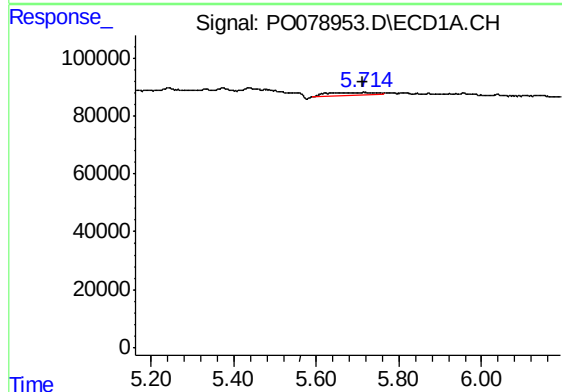


#18 AR-1242-3

R.T.: 5.715 min
Delta R.T.: 0.003 min
Response: 67546
Conc: 36.50 ng/ml

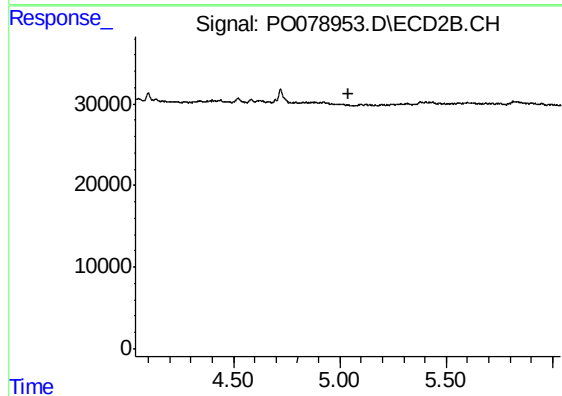

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.038 min
Response: 0
Conc: N.D.

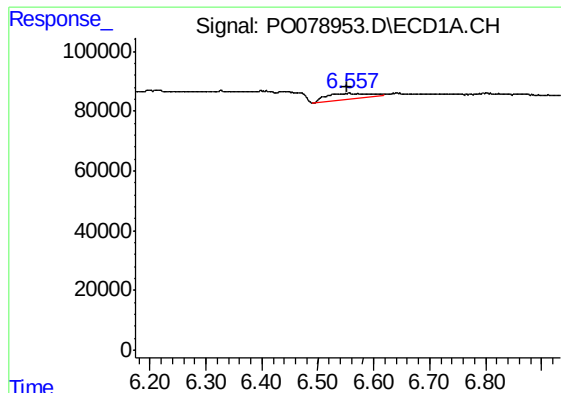

#24 AR-1248-4


R.T.: 6.555 min
Delta R.T.: 0.003 min
Response: 113191
Conc: 40.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-O(CL-24)

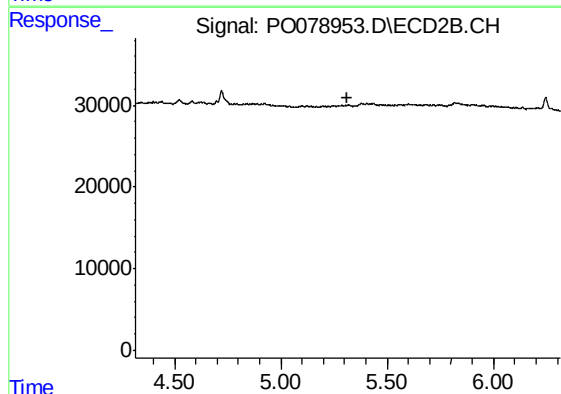


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.315 min
Response: 0
Conc: N.D.

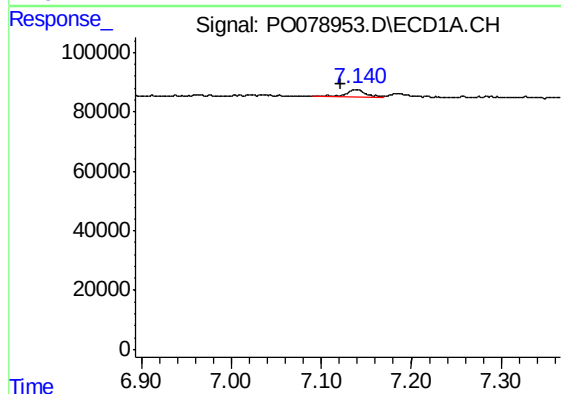


#28 AR-1254-3

R.T.: 7.139 min
Delta R.T.: 0.017 min
Response: 37311
Conc: 8.38 ng/ml

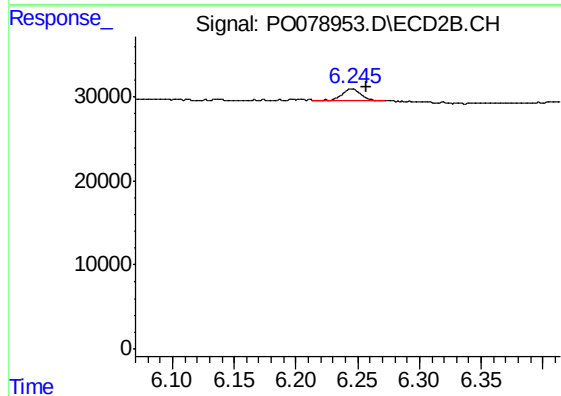

#28 AR-1254-3


R.T.: 6.245 min
Delta R.T.: -0.012 min
Response: 14636
Conc: 6.58 ng/ml

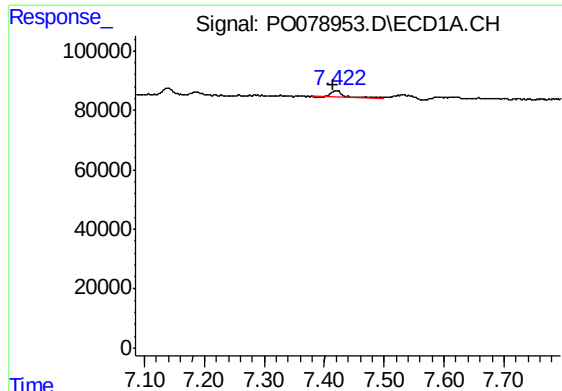

#29 AR-1254-4


R.T.: 7.420 min
Delta R.T.: 0.005 min
Response: 34628
Conc: 11.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-O(CL-24)

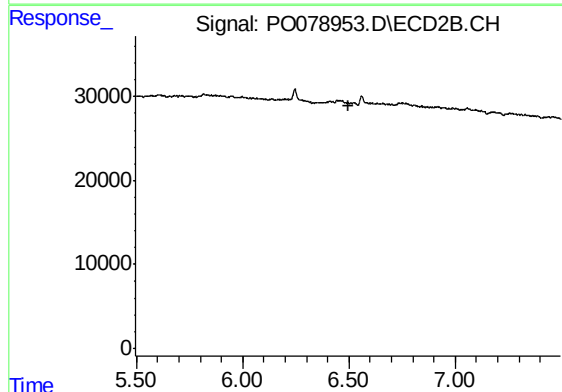


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.495 min
Response: 0
Conc: N.D.

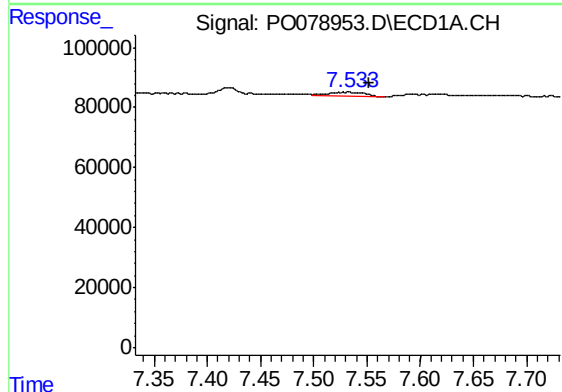

#32 AR-1260-2

R.T.: 7.532 min
Delta R.T.: -0.020 min
Response: 33927
Conc: 8.73 ng/ml

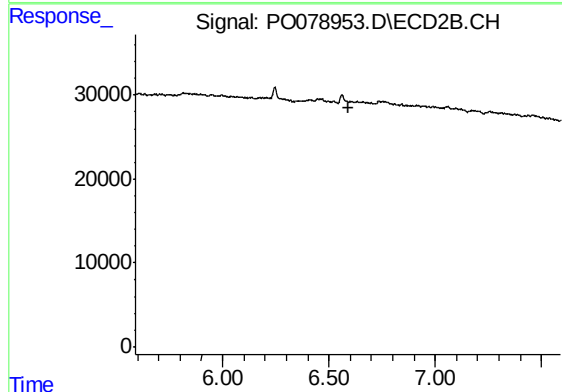

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.590 min
Response: 0
Conc: N.D.