

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062021\
 Data File : P0078951.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2021 10:29
 Operator : DD\AJ
 Sample : M2709-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-AMND-COMP-N(CL-22)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 05:23:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.330	3.607	1693299	648828	21.455	21.831
2) SA Decachlor...	9.936	8.786	1191122	614182	19.072	20.611

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062021\
Data File : PO078951.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2021 10:29
Operator : DD\AJ
Sample : M2709-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 05:23:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

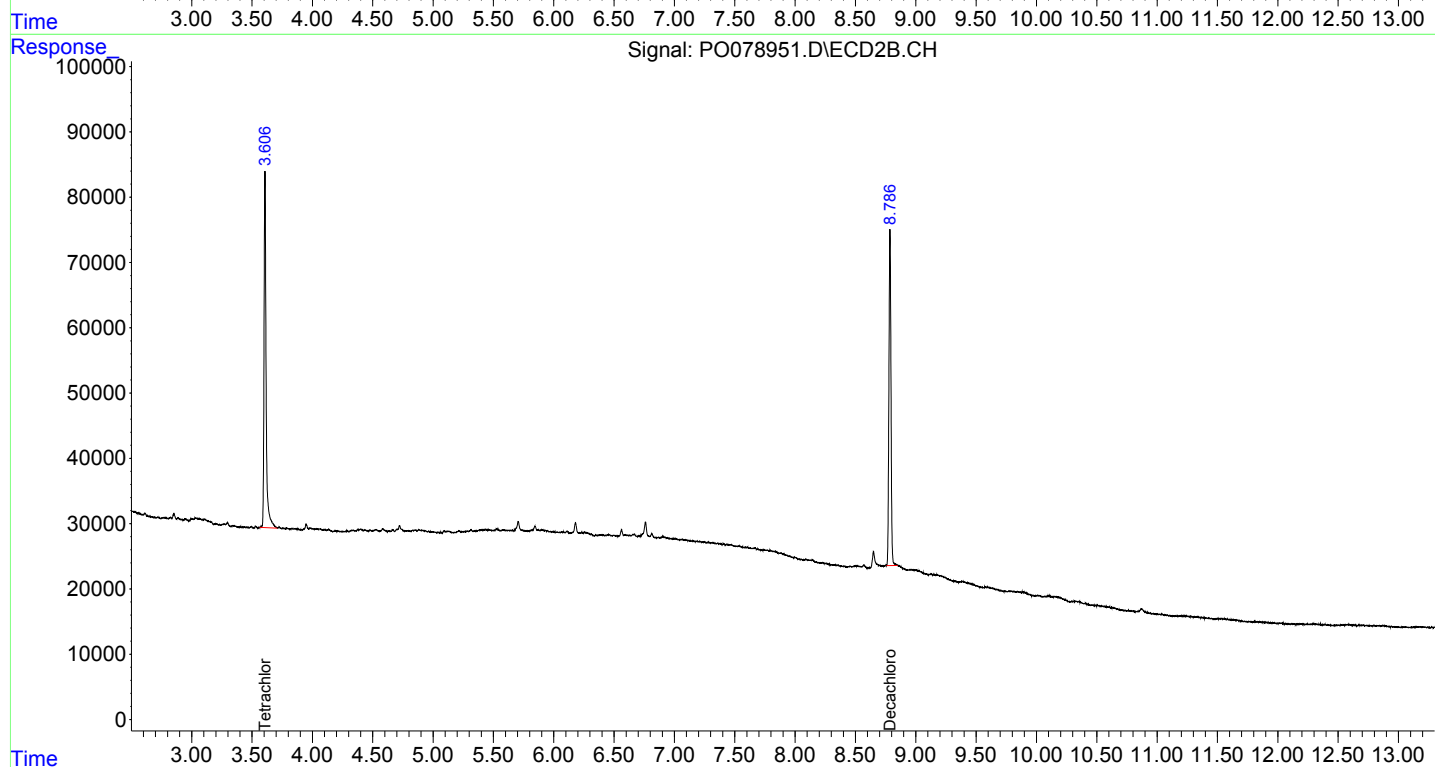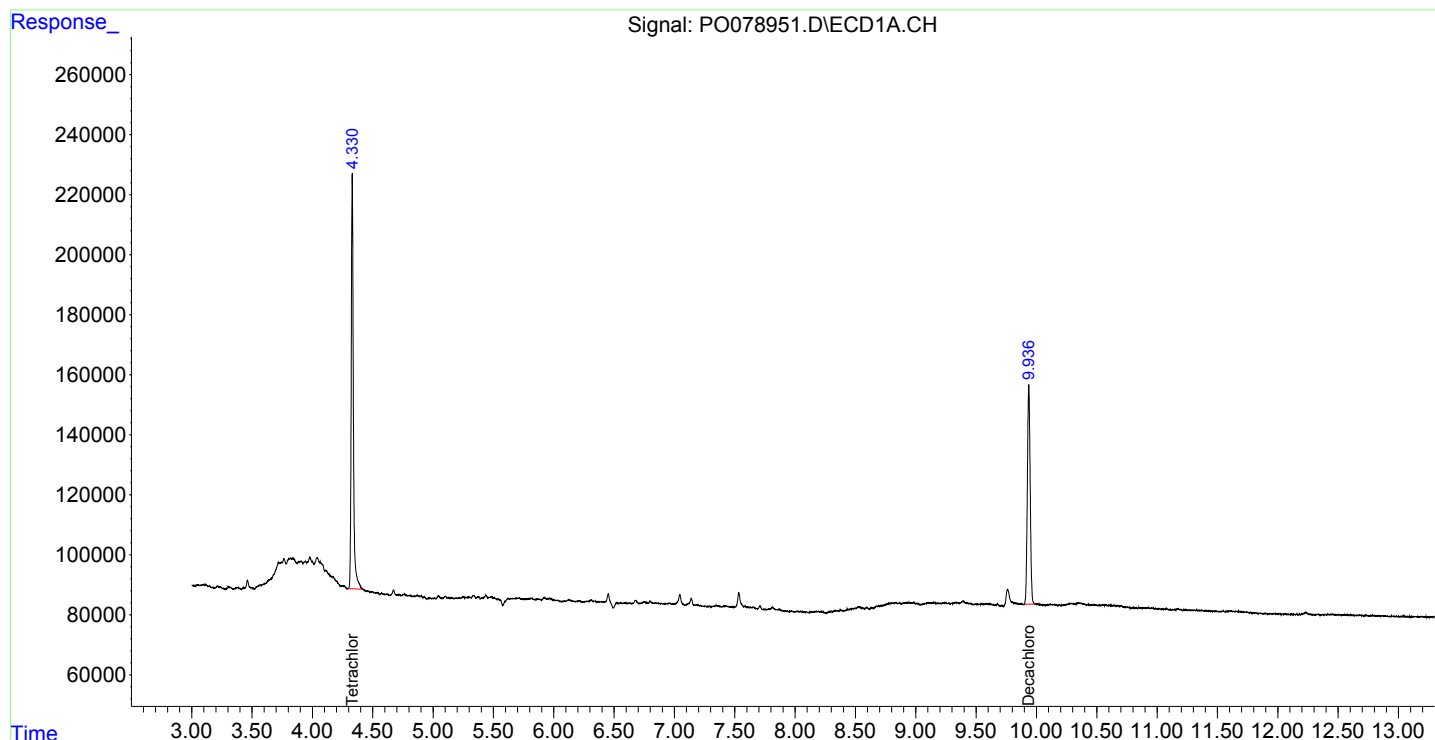


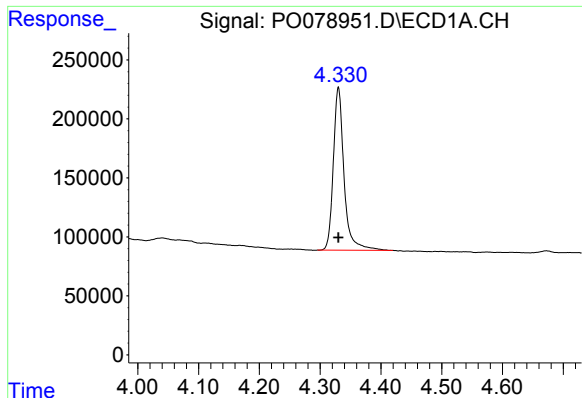

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 1693299
Conc: 21.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-AMND-COMP-N(CL-22)

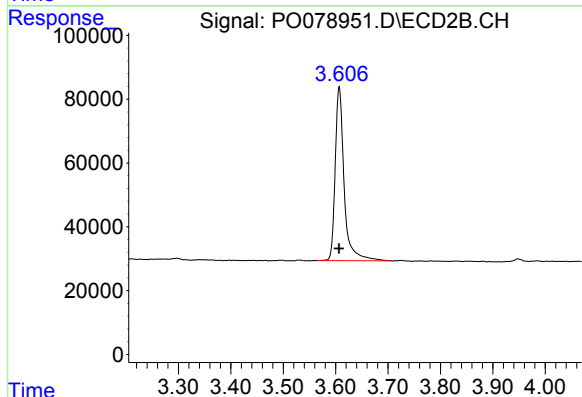


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 648828
Conc: 21.83 ng/ml

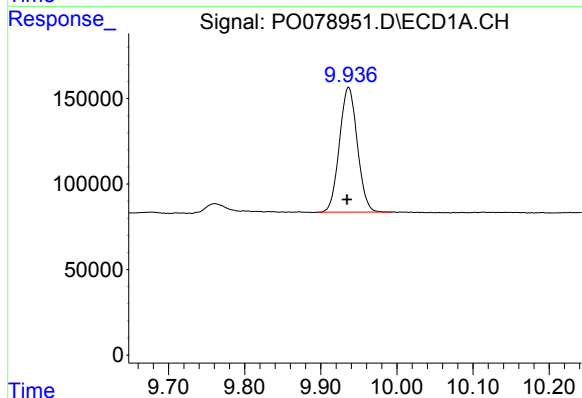

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.002 min
Response: 1191122
Conc: 19.07 ng/ml

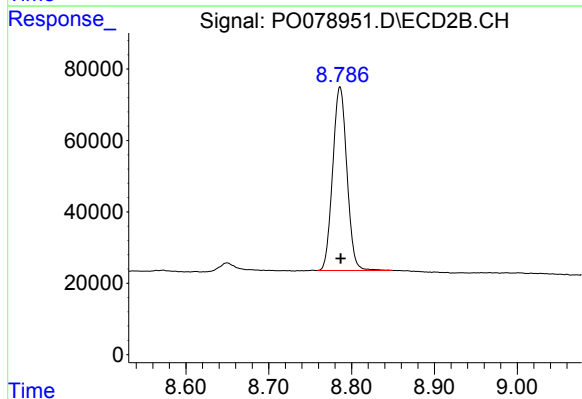

#2 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 614182
Conc: 20.61 ng/ml