

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062025\
 Data File : P0111746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 10:16
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:01:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.677	3.673	130.1E6	113.3E6	22.583	20.176
2)	SA Decachlor...	8.713	8.661	116.6E6	37928790	22.206	21.336
Target Compounds							
3)	L1 AR-1016-1	4.765	4.749	6948541	6109947	29.128	31.052
4)	L1 AR-1016-2	4.784	4.768	8965132	8311147	26.943	29.174
5)	L1 AR-1016-3	4.841	4.944	6937466	3733084	30.144	24.848
6)	L1 AR-1016-4	4.960	4.985	5522163	3777828	29.775	31.020
7)	L1 AR-1016-5	5.217	5.199	6654322	4306250	35.653	27.050
8)	L2 AR-1221-1	3.895	3.880	1060365	212570	12.177	2.847 #
9)	L2 AR-1221-2	3.959	3.953	10878782	8688550	169.537	155.294
10)	L2 AR-1221-3	4.051	4.042	3047793	2560420	15.627	14.901
11)	L3 AR-1232-1	4.051	4.042	3047793	2560420	20.084	19.253
12)	L3 AR-1232-2	4.543	4.768	5308682	8311147	61.571	63.063
13)	L3 AR-1232-3	4.784	4.944	8965132	3733084	55.041	54.010
14)	L3 AR-1232-4	4.960	5.027	5522163	4111216	63.459	67.972
15)	L3 AR-1232-5	5.004	5.199	5001250	4306250	88.392	64.839 #
16)	L4 AR-1242-1	4.765	4.749	6948541	6109947	34.494	37.540
17)	L4 AR-1242-2	4.784	4.768	8965132	8311147	31.818	35.208
18)	L4 AR-1242-3	4.841	4.944	6937466	3733084	34.893	29.725
19)	L4 AR-1242-4	4.960	5.027	5522163	4111216	34.907	33.545
20)	L4 AR-1242-5	5.616	5.548	4770236	5781178	28.527	38.570 #
21)	L5 AR-1248-1	4.765	4.749	6948541	6109947	43.088	45.841
22)	L5 AR-1248-2	5.004	4.985	5001250	3777828	23.196	21.205
23)	L5 AR-1248-3	5.217	5.027	6654322	4111216	24.670	21.702
24)	L5 AR-1248-4	5.571	5.199	14649849	4306250	36.643	18.860 #
25)	L5 AR-1248-5	5.616	5.591	4770236	3150552	16.987	14.468
26)	L6 AR-1254-1	5.571	5.548	14649849	5781178	34.465	17.898 #
27)	L6 AR-1254-2	5.720	5.695	16668210	7779841	43.918	27.853 #
28)	L6 AR-1254-3	6.141	6.113	25407299	13776599	44.469	32.876 #
29)	L6 AR-1254-4	6.342	6.310	14606182	3507936	41.866	15.399 #
30)	L6 AR-1254-5	6.772	6.741	15815139	7465981	30.881	22.931 #
31)	L7 AR-1260-1	6.257	6.227	48643263	19234050	136.899	76.655 #
32)	L7 AR-1260-2	6.446	6.416	41801186	14833592	88.473	50.452 #
33)	L7 AR-1260-3	6.812	6.568	17112351	6904806	40.295	25.843 #
34)	L7 AR-1260-4	7.073	7.037	17997698	5209937	57.236	27.407 #
35)	L7 AR-1260-5	7.315	7.279	29734338	10983925	36.097	25.843 #
36)	L8 AR-1262-1	6.812	6.780	17112351	7941441	28.059	23.519
37)	L8 AR-1262-2	7.315	7.279	29734338	10983925	31.585	23.582 #
38)	L8 AR-1262-3	7.599	7.562	6477806	2994326	16.332	18.007
39)	L8 AR-1262-4	7.662	7.624	13488175	6839730	20.530	24.686
40)	L8 AR-1262-5	8.159	8.118	4745425	1747526	15.576	17.197
41)	L9 AR-1268-1	7.599	7.562	6477806	2994326	5.750	6.259

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
Data File : P0111746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 10:16
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:01:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.662	7.624	13488175	6839730	13.802	16.422
43)	L9 AR-1268-3	7.865	7.830	347155	146465	0.424	0.462
44)	L9 AR-1268-4	8.159	8.118	4745425	1747526	13.796	15.110
45)	L9 AR-1268-5	8.454	8.404	2059922	579371	0.928	0.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062025\
Data File : PO111746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 10:16
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1660 LOD 25 PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:01:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

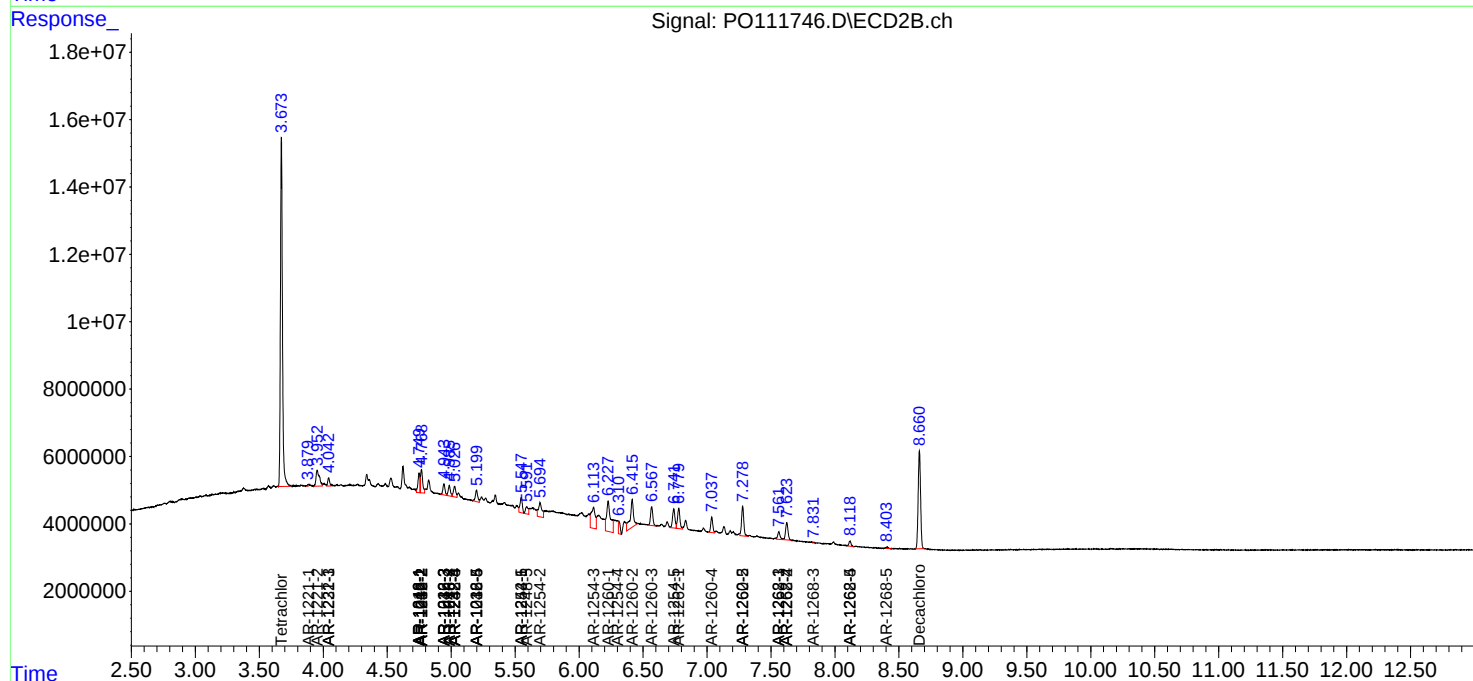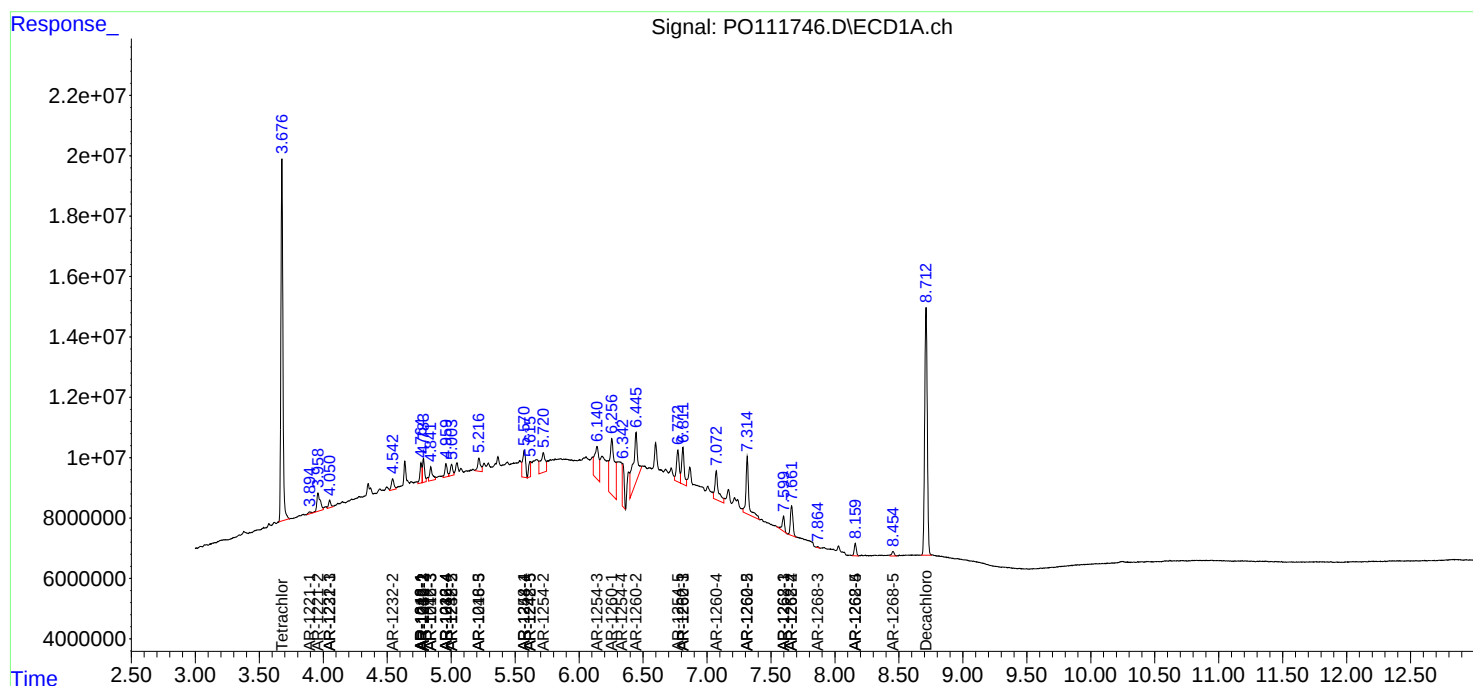


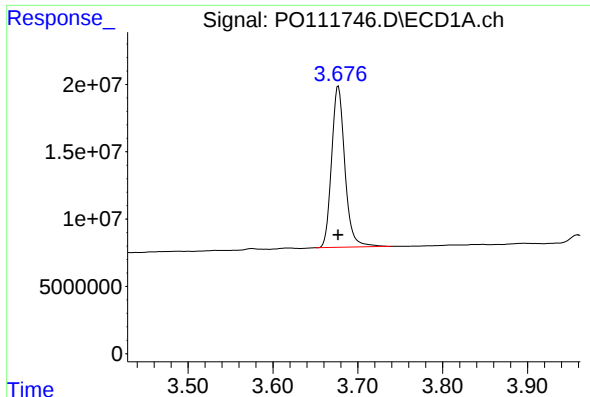

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 130064834
Conc: 22.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

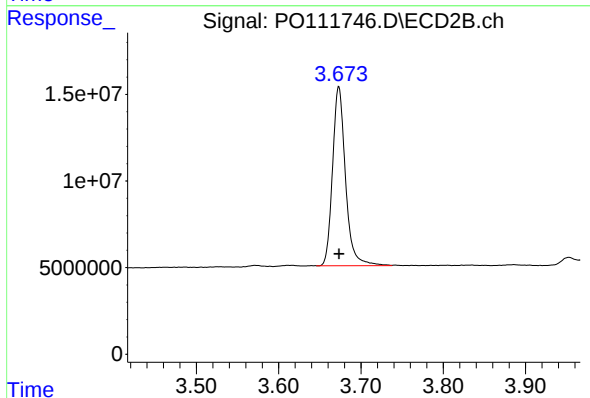


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 113332306
Conc: 20.18 ng/ml

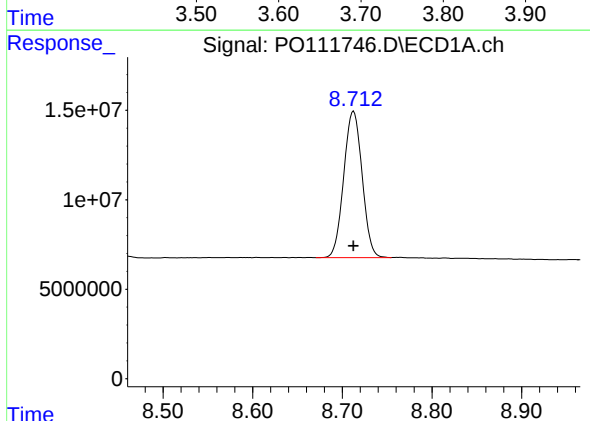


#2 Decachlorobiphenyl

R.T.: 8.713 min
Delta R.T.: 0.000 min
Response: 116564350
Conc: 22.21 ng/ml

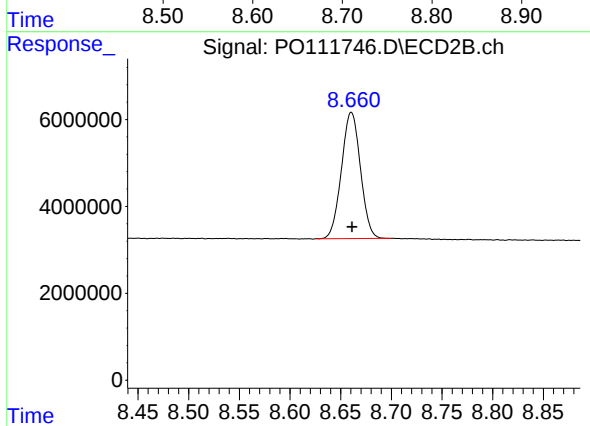

#2 Decachlorobiphenyl


R.T.: 8.661 min
Delta R.T.: 0.000 min
Response: 37928790
Conc: 21.34 ng/ml

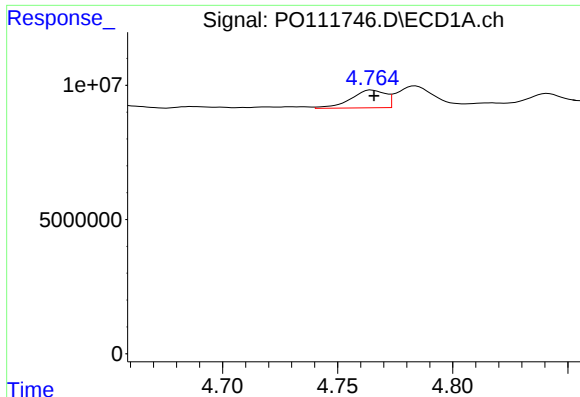

#3 AR-1016-1


R.T.: 4.765 min
Delta R.T.: -0.001 min
Response: 6948541
Conc: 29.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

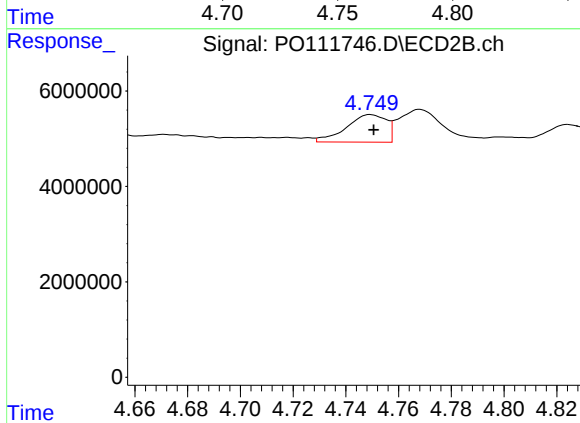


#3 AR-1016-1

R.T.: 4.749 min
Delta R.T.: -0.001 min
Response: 6109947
Conc: 31.05 ng/ml

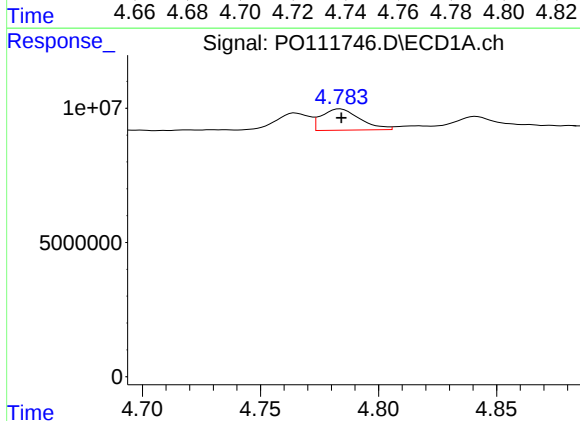


#4 AR-1016-2

R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 8965132
Conc: 26.94 ng/ml

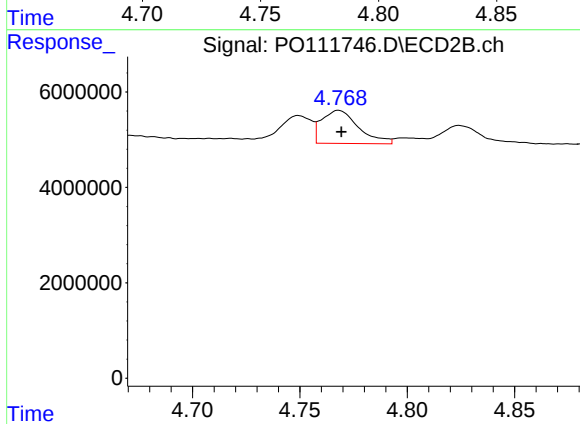

#4 AR-1016-2


R.T.: 4.768 min
Delta R.T.: -0.001 min
Response: 8311147
Conc: 29.17 ng/ml

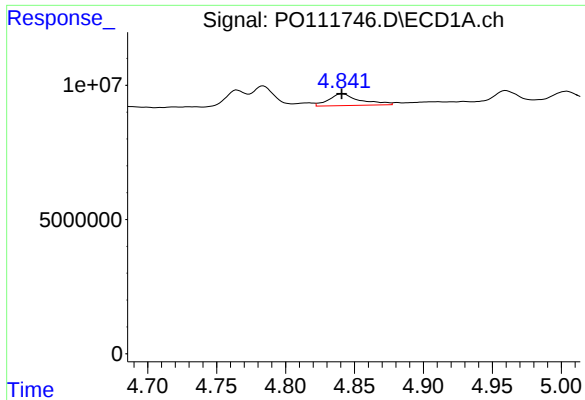

#5 AR-1016-3


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 6937466
Conc: 30.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

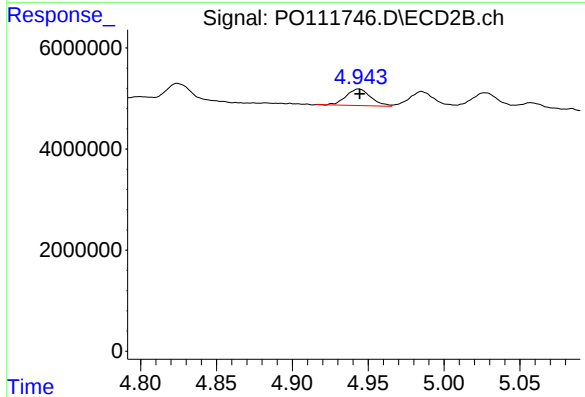


#5 AR-1016-3

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 3733084
Conc: 24.85 ng/ml

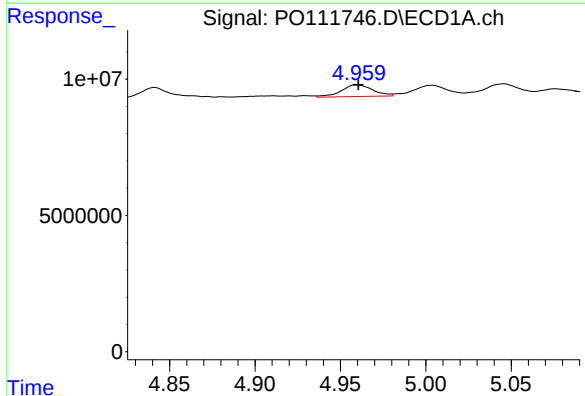


#6 AR-1016-4

R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 5522163
Conc: 29.78 ng/ml

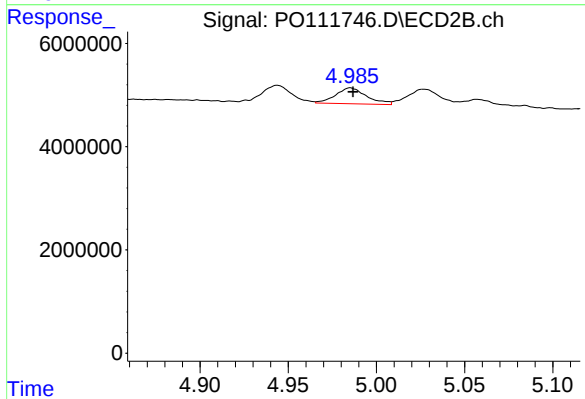

#6 AR-1016-4


R.T.: 4.985 min
Delta R.T.: -0.002 min
Response: 3777828
Conc: 31.02 ng/ml

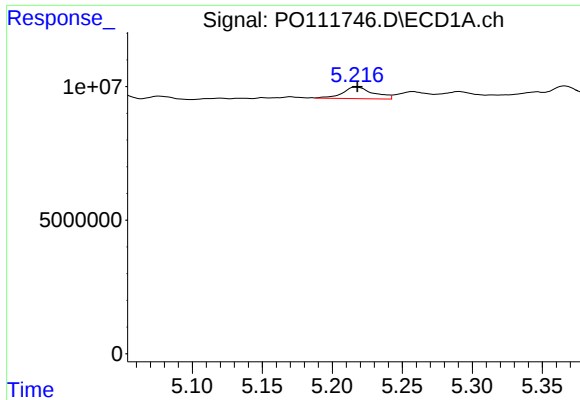

#7 AR-1016-5


R.T.: 5.217 min
Delta R.T.: -0.001 min
Response: 6654322
Conc: 35.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

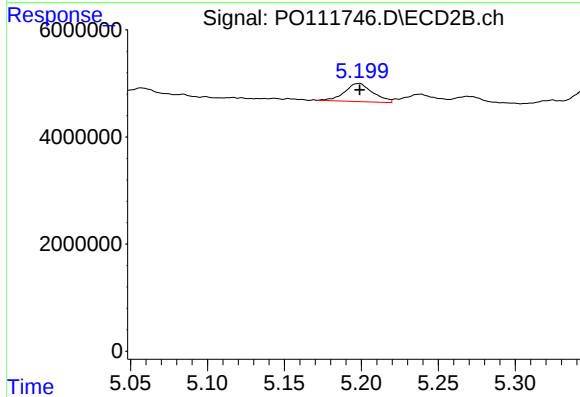


#7 AR-1016-5

R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 4306250
Conc: 27.05 ng/ml

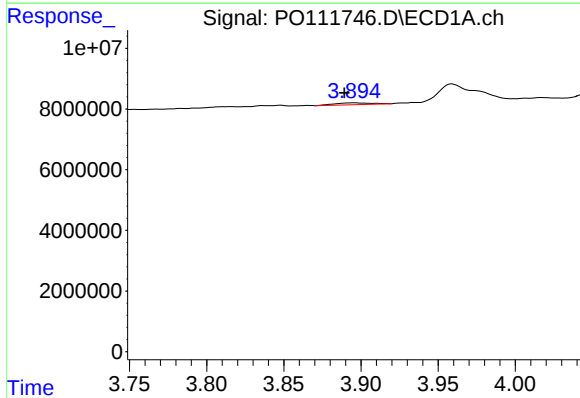


#8 AR-1221-1

R.T.: 3.895 min
Delta R.T.: 0.006 min
Response: 1060365
Conc: 12.18 ng/ml

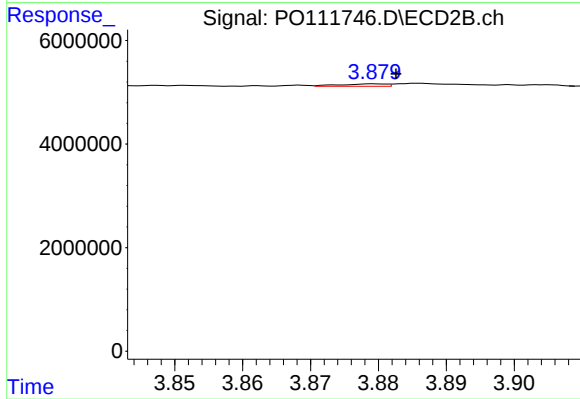

#8 AR-1221-1


R.T.: 3.880 min
Delta R.T.: -0.003 min
Response: 212570
Conc: 2.85 ng/ml

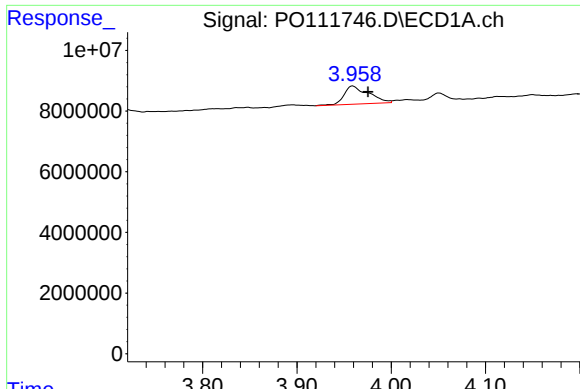

#9 AR-1221-2


R.T.: 3.959 min
Delta R.T.: -0.016 min
Response: 10878782
Conc: 169.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

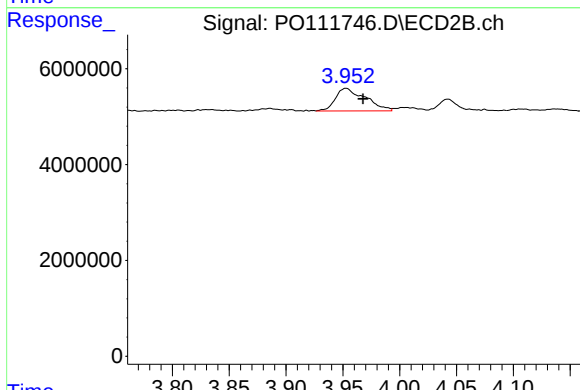


#9 AR-1221-2

R.T.: 3.953 min
Delta R.T.: -0.015 min
Response: 8688550
Conc: 155.29 ng/ml

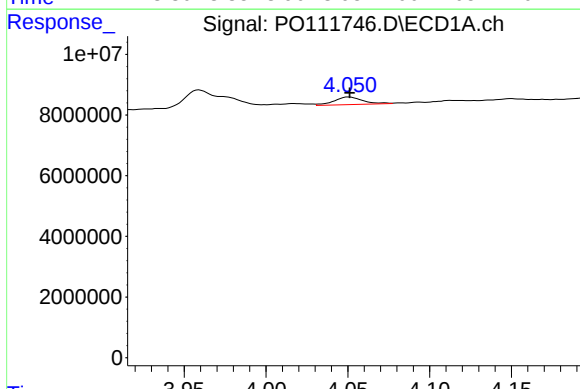


#10 AR-1221-3

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 3047793
Conc: 15.63 ng/ml

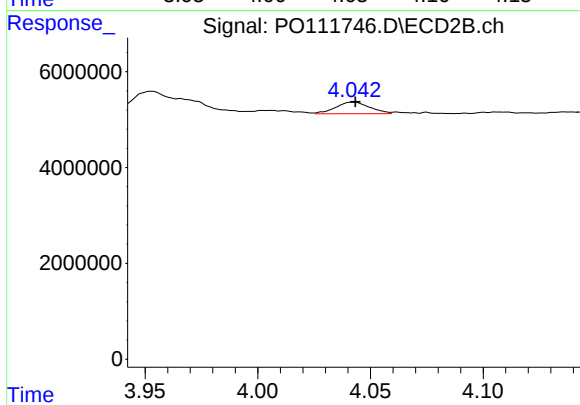

#10 AR-1221-3


R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 2560420
Conc: 14.90 ng/ml

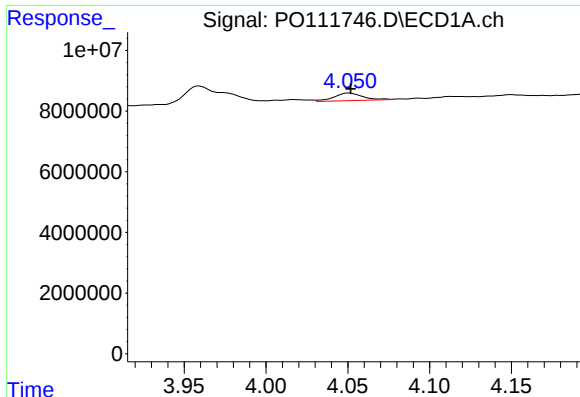

#11 AR-1232-1


R.T.: 4.051 min
Delta R.T.: -0.001 min
Response: 3047793
Conc: 20.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

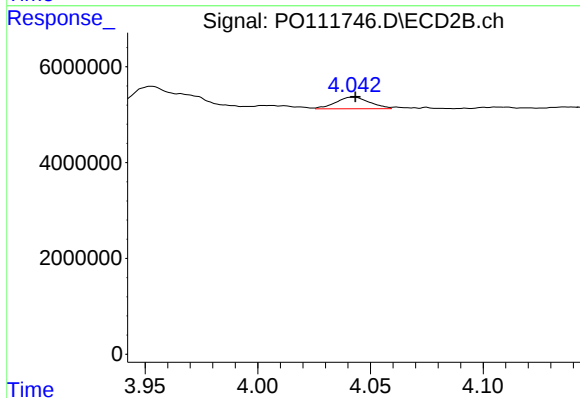


#11 AR-1232-1

R.T.: 4.042 min
Delta R.T.: 0.000 min
Response: 2560420
Conc: 19.25 ng/ml

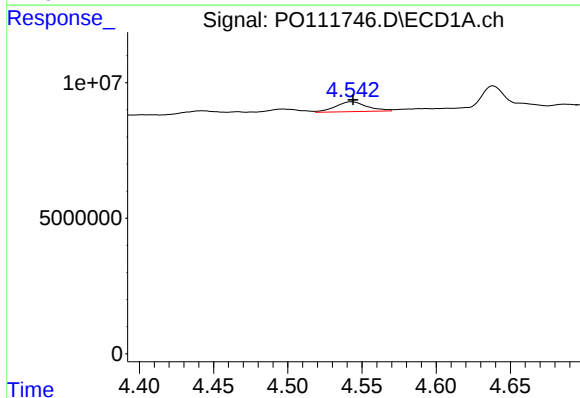


#12 AR-1232-2

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 5308682
Conc: 61.57 ng/ml

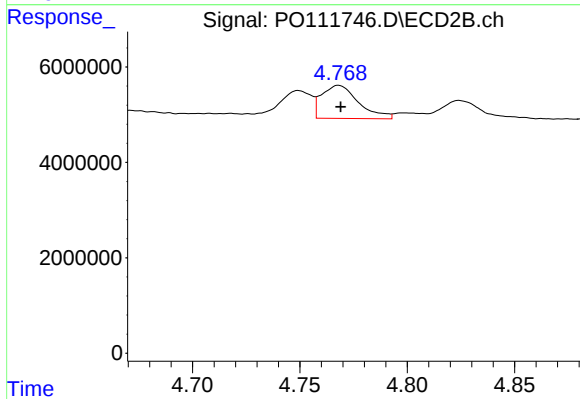

#12 AR-1232-2


R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 8311147
Conc: 63.06 ng/ml

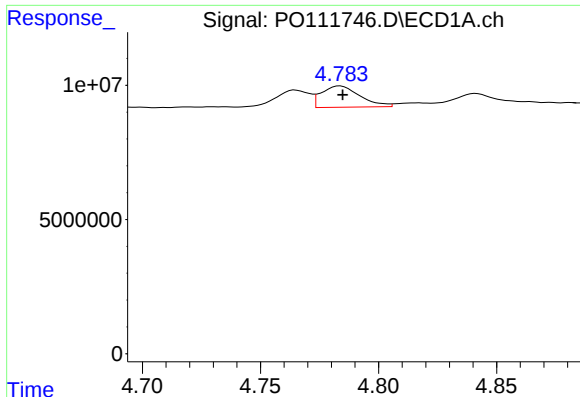

#13 AR-1232-3


R.T.: 4.784 min
Delta R.T.: -0.001 min
Response: 8965132
Conc: 55.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

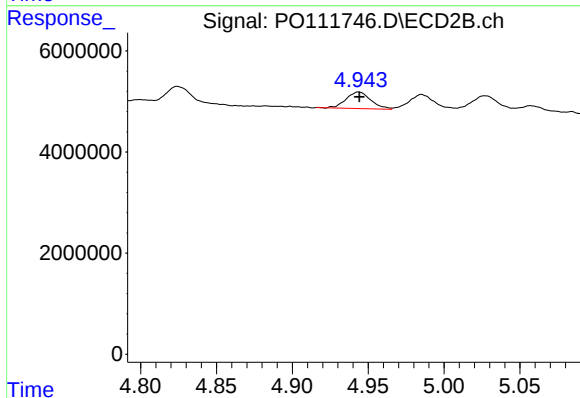


#13 AR-1232-3

R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 3733084
Conc: 54.01 ng/ml

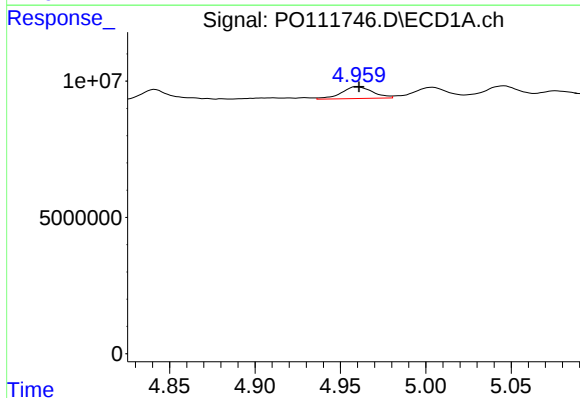


#14 AR-1232-4

R.T.: 4.960 min
Delta R.T.: -0.001 min
Response: 5522163
Conc: 63.46 ng/ml

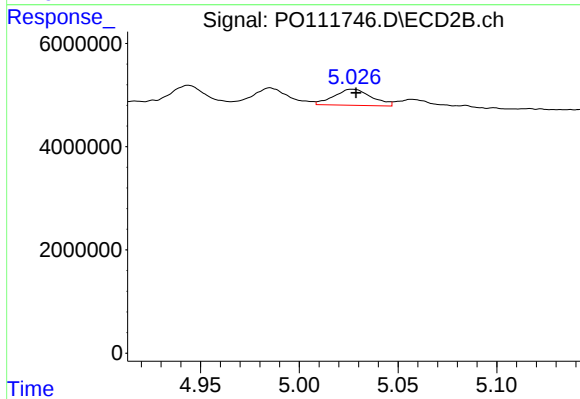

#14 AR-1232-4


R.T.: 5.027 min
Delta R.T.: -0.002 min
Response: 4111216
Conc: 67.97 ng/ml

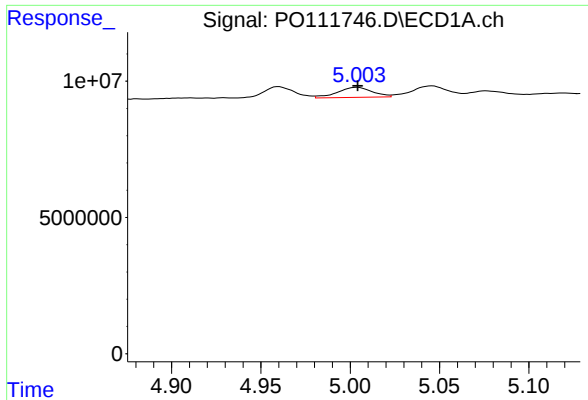

#15 AR-1232-5


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 5001250
Conc: 88.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

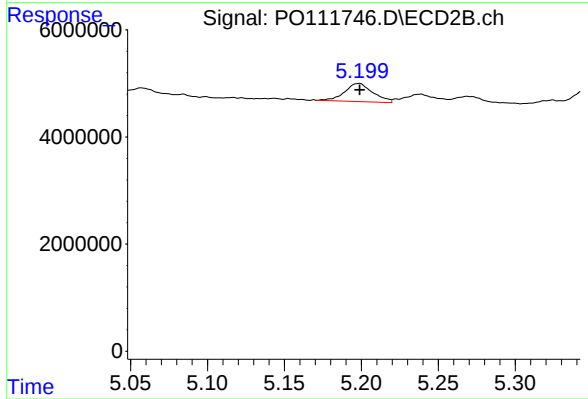


#15 AR-1232-5

R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 4306250
Conc: 64.84 ng/ml

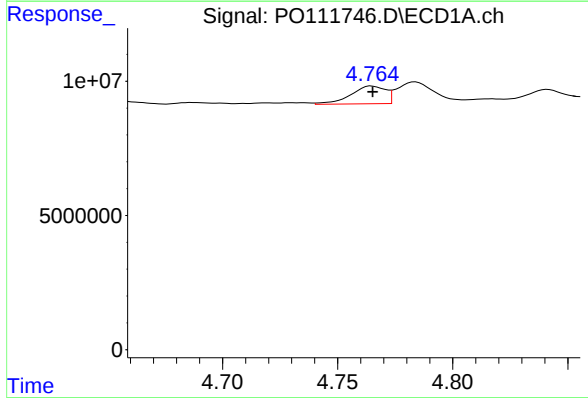


#16 AR-1242-1

R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 6948541
Conc: 34.49 ng/ml

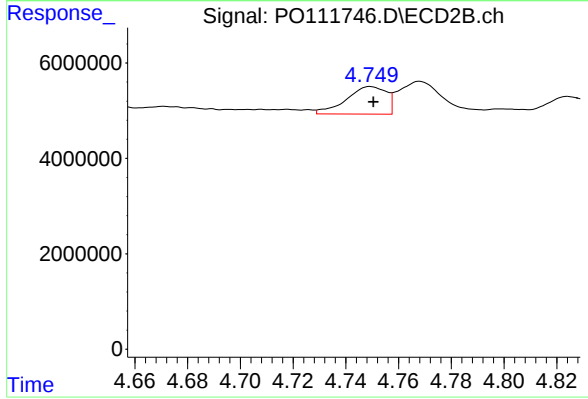

#16 AR-1242-1


R.T.: 4.749 min
Delta R.T.: -0.001 min
Response: 6109947
Conc: 37.54 ng/ml

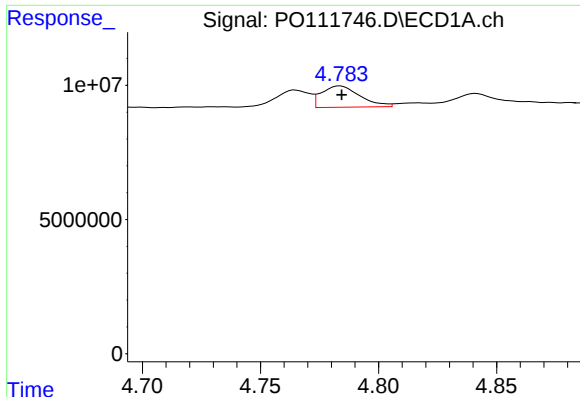

#17 AR-1242-2


R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 8965132
Conc: 31.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

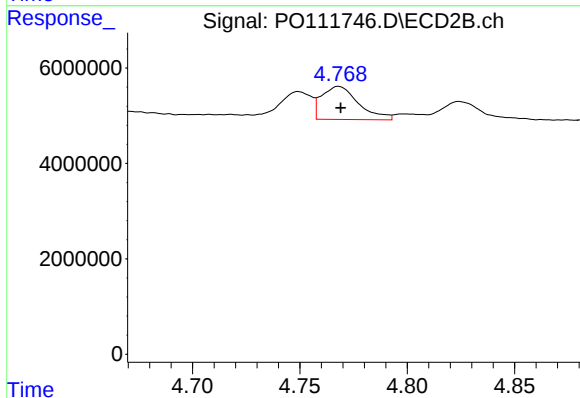


#17 AR-1242-2

R.T.: 4.768 min
Delta R.T.: -0.001 min
Response: 8311147
Conc: 35.21 ng/ml

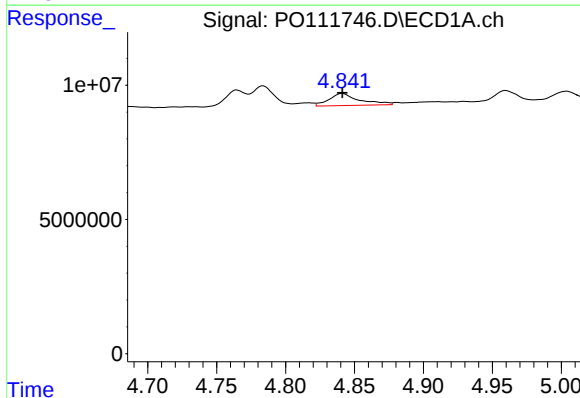


#18 AR-1242-3

R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 6937466
Conc: 34.89 ng/ml

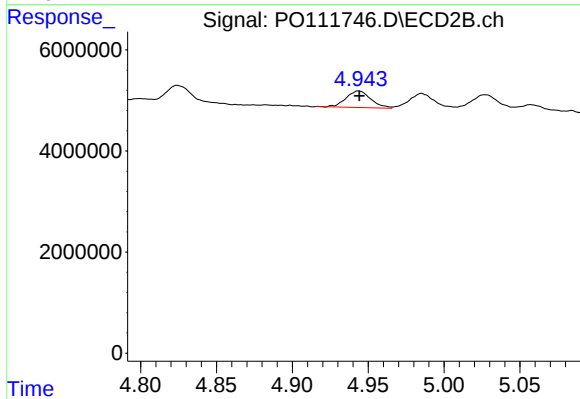

#18 AR-1242-3


R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 3733084
Conc: 29.72 ng/ml

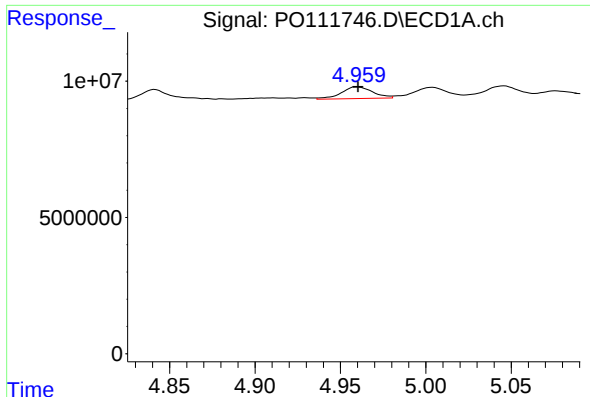

#19 AR-1242-4


R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 5522163
Conc: 34.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

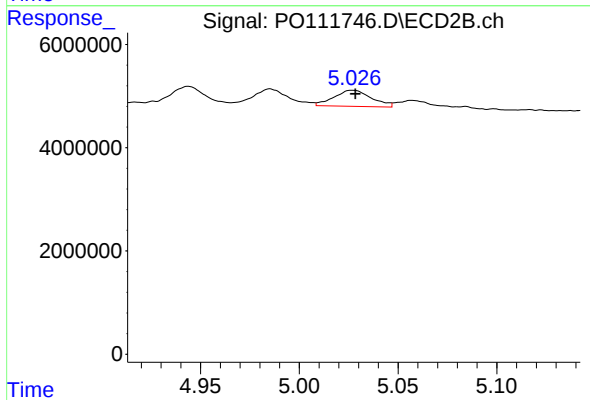


#19 AR-1242-4

R.T.: 5.027 min
Delta R.T.: -0.001 min
Response: 4111216
Conc: 33.54 ng/ml

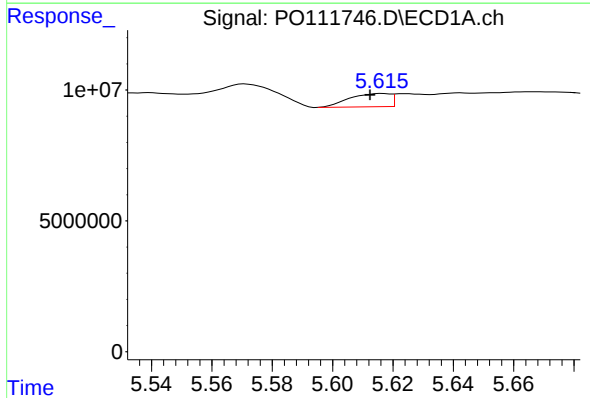


#20 AR-1242-5

R.T.: 5.616 min
Delta R.T.: 0.004 min
Response: 4770236
Conc: 28.53 ng/ml

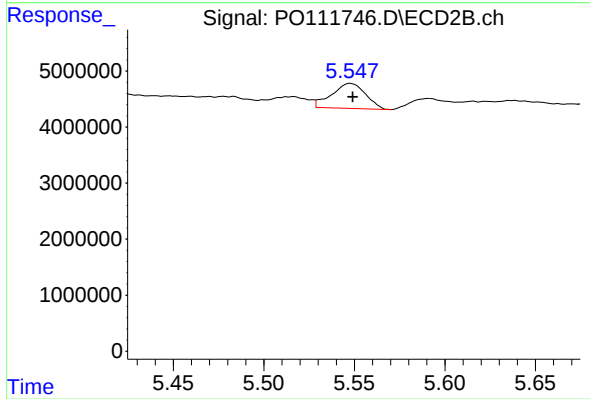

#20 AR-1242-5


R.T.: 5.548 min
Delta R.T.: -0.001 min
Response: 5781178
Conc: 38.57 ng/ml

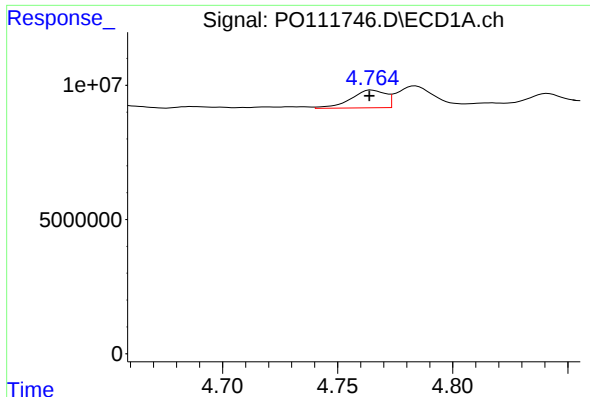

#21 AR-1248-1


R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 6948541
Conc: 43.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

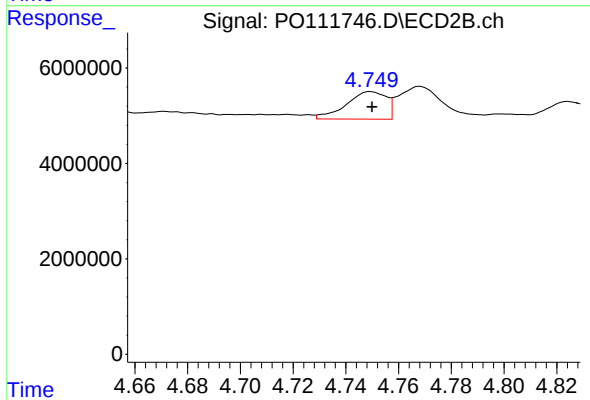


#21 AR-1248-1

R.T.: 4.749 min
Delta R.T.: 0.000 min
Response: 6109947
Conc: 45.84 ng/ml

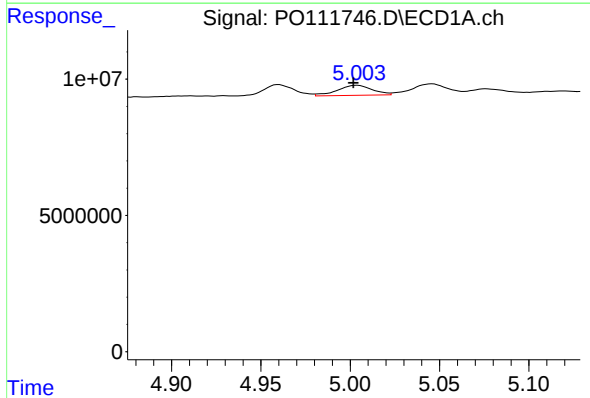


#22 AR-1248-2

R.T.: 5.004 min
Delta R.T.: 0.002 min
Response: 5001250
Conc: 23.20 ng/ml

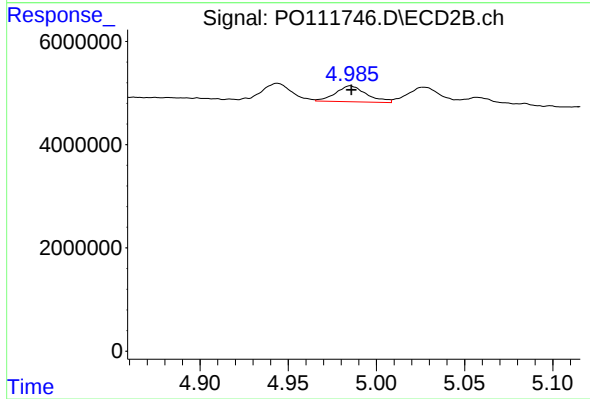

#22 AR-1248-2


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 3777828
Conc: 21.21 ng/ml

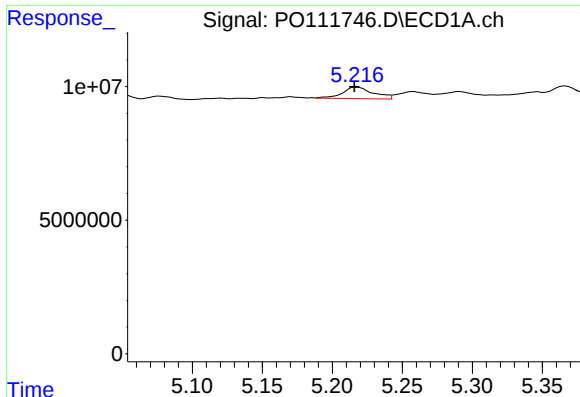

#23 AR-1248-3


R.T.: 5.217 min
Delta R.T.: 0.001 min
Response: 6654322
Conc: 24.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

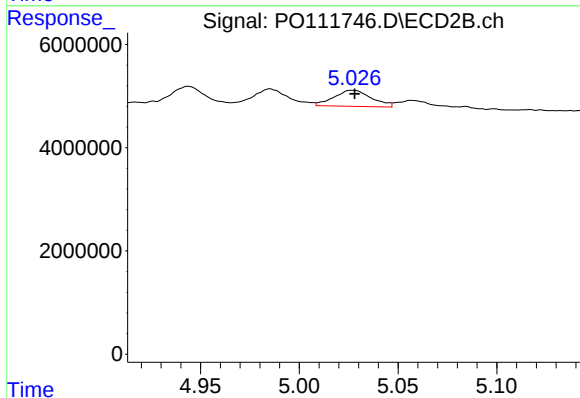


#23 AR-1248-3

R.T.: 5.027 min
Delta R.T.: -0.001 min
Response: 4111216
Conc: 21.70 ng/ml

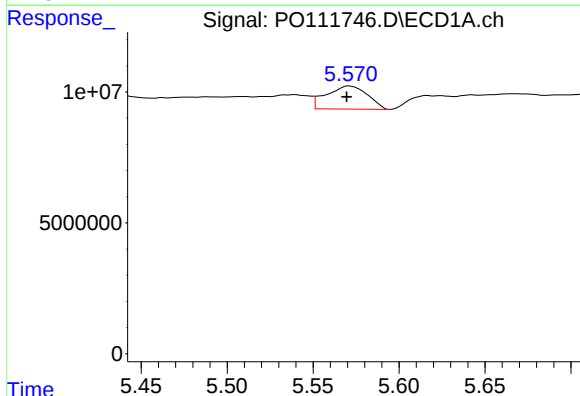


#24 AR-1248-4

R.T.: 5.571 min
Delta R.T.: 0.002 min
Response: 14649849
Conc: 36.64 ng/ml

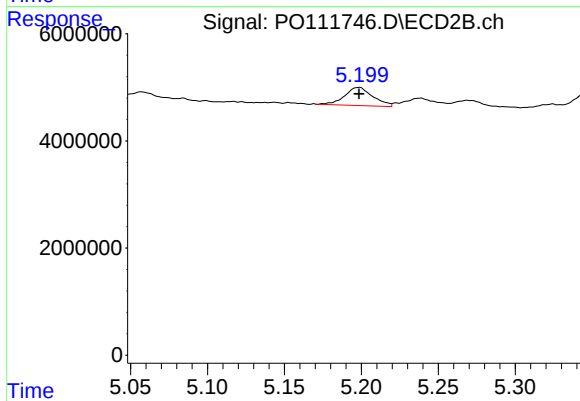

#24 AR-1248-4


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 4306250
Conc: 18.86 ng/ml

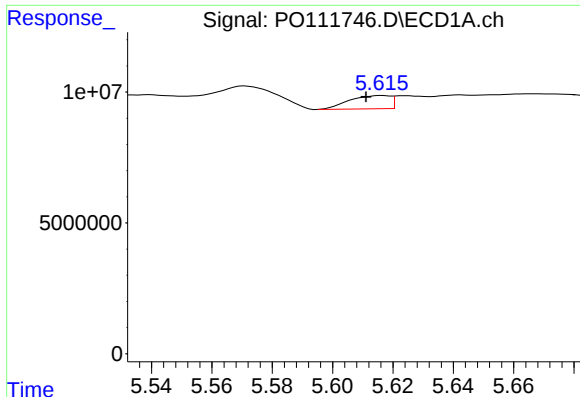

#25 AR-1248-5


R.T.: 5.616 min
Delta R.T.: 0.005 min
Response: 4770236
Conc: 16.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

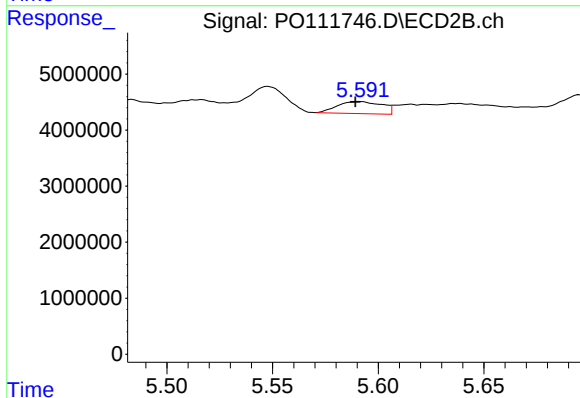


#25 AR-1248-5

R.T.: 5.591 min
Delta R.T.: 0.002 min
Response: 3150552
Conc: 14.47 ng/ml

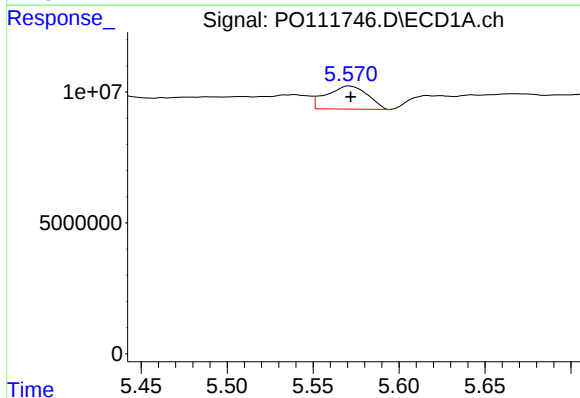


#26 AR-1254-1

R.T.: 5.571 min
Delta R.T.: 0.000 min
Response: 14649849
Conc: 34.46 ng/ml

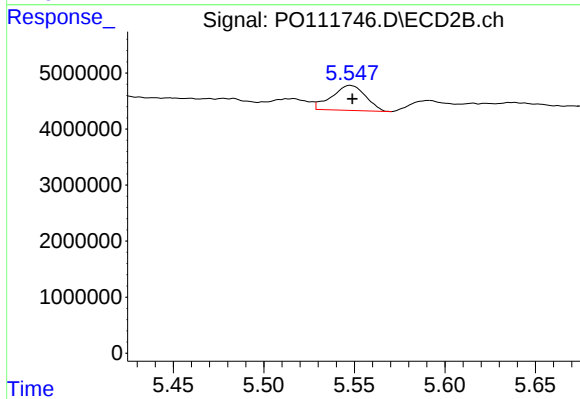

#26 AR-1254-1


R.T.: 5.548 min
Delta R.T.: -0.001 min
Response: 5781178
Conc: 17.90 ng/ml

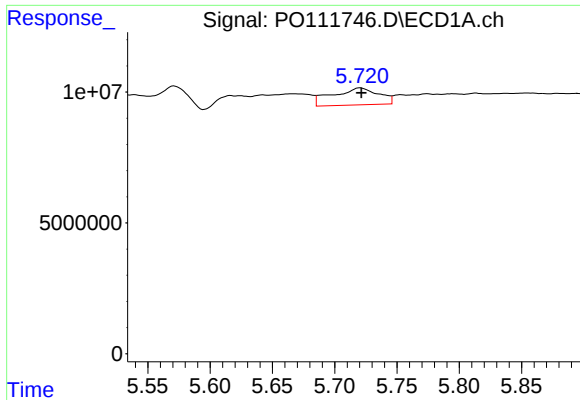

#27 AR-1254-2


R.T.: 5.720 min
Delta R.T.: -0.001 min
Response: 16668210
Conc: 43.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

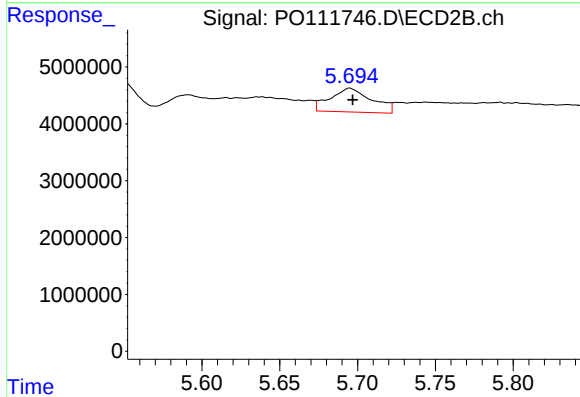


#27 AR-1254-2

R.T.: 5.695 min
Delta R.T.: -0.002 min
Response: 7779841
Conc: 27.85 ng/ml

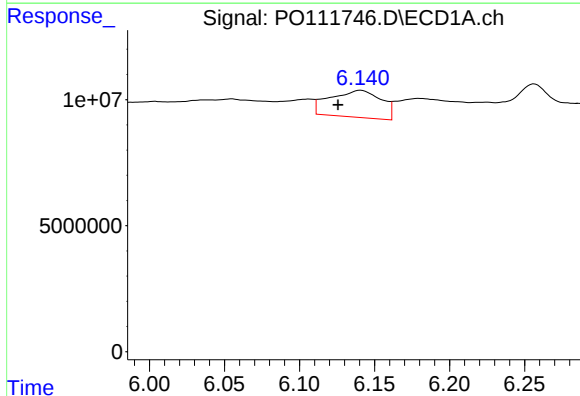


#28 AR-1254-3

R.T.: 6.141 min
Delta R.T.: 0.015 min
Response: 25407299
Conc: 44.47 ng/ml

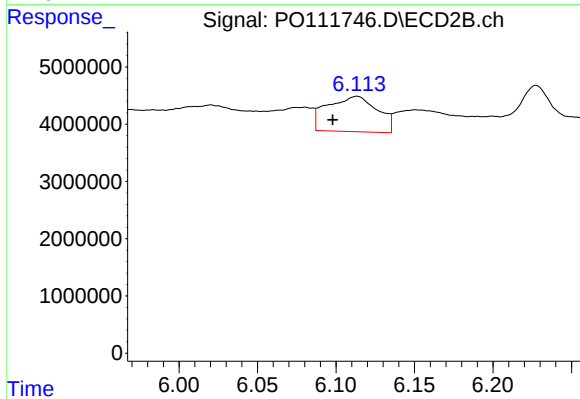

#28 AR-1254-3


R.T.: 6.113 min
Delta R.T.: 0.015 min
Response: 13776599
Conc: 32.88 ng/ml

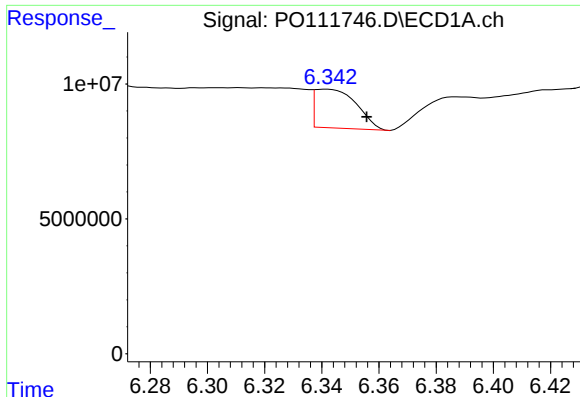

#29 AR-1254-4


R.T.: 6.342 min
Delta R.T.: -0.014 min
Response: 14606182
Conc: 41.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

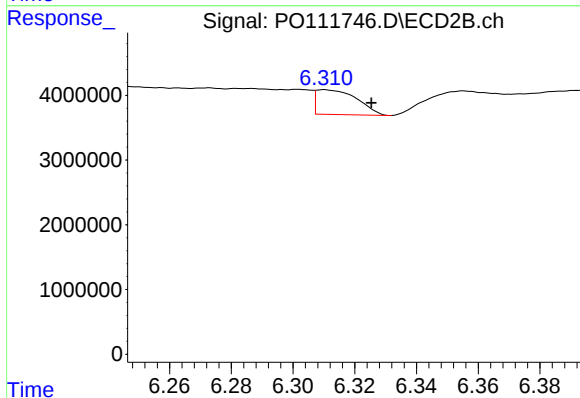


#29 AR-1254-4

R.T.: 6.310 min
Delta R.T.: -0.015 min
Response: 3507936
Conc: 15.40 ng/ml

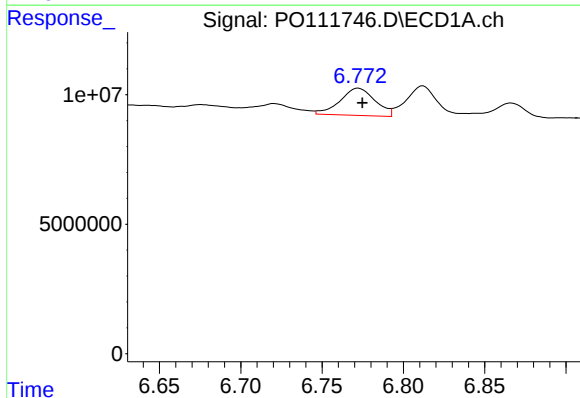


#30 AR-1254-5

R.T.: 6.772 min
Delta R.T.: -0.002 min
Response: 15815139
Conc: 30.88 ng/ml

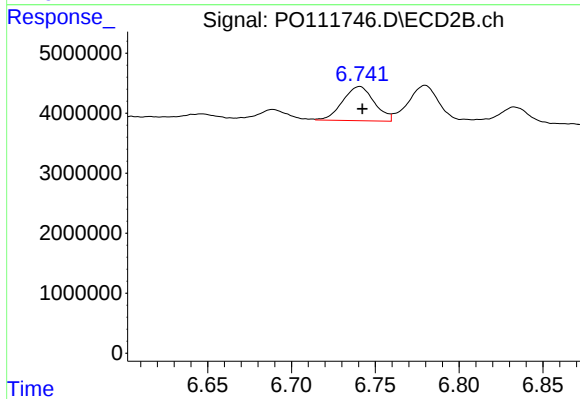

#30 AR-1254-5


R.T.: 6.741 min
Delta R.T.: -0.001 min
Response: 7465981
Conc: 22.93 ng/ml

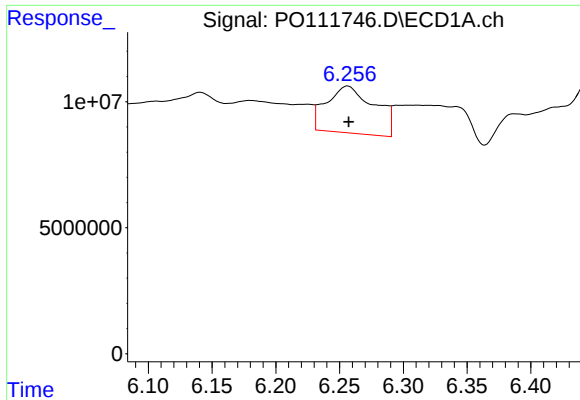

#31 AR-1260-1


R.T.: 6.257 min
Delta R.T.: 0.000 min
Response: 48643263
Conc: 136.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

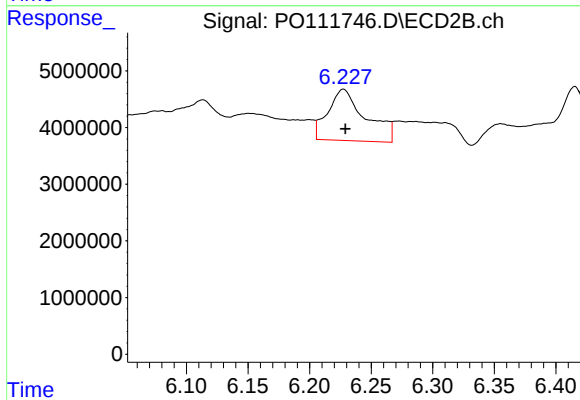


#31 AR-1260-1

R.T.: 6.227 min
Delta R.T.: -0.002 min
Response: 19234050
Conc: 76.66 ng/ml

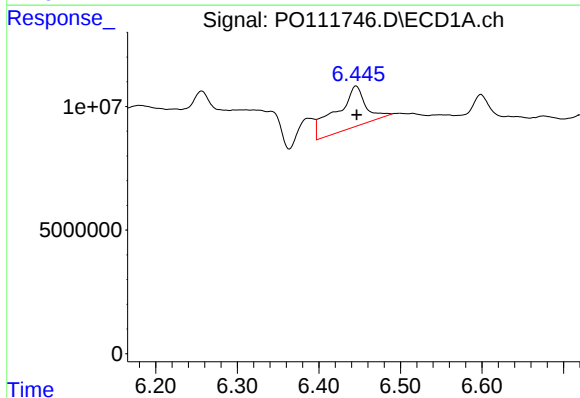


#32 AR-1260-2

R.T.: 6.446 min
Delta R.T.: 0.000 min
Response: 41801186
Conc: 88.47 ng/ml

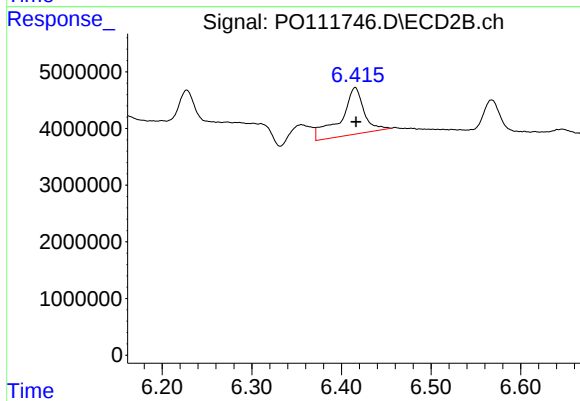

#32 AR-1260-2


R.T.: 6.416 min
Delta R.T.: 0.000 min
Response: 14833592
Conc: 50.45 ng/ml

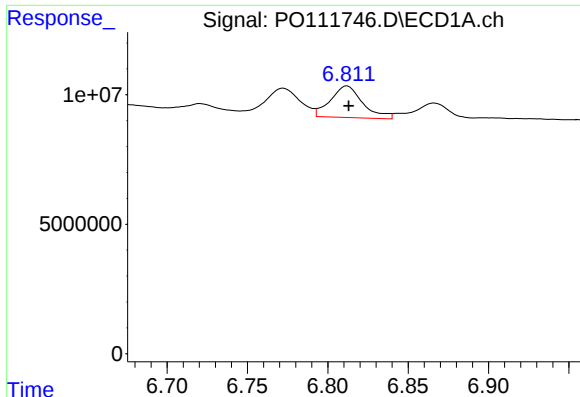

#33 AR-1260-3


R.T.: 6.812 min
Delta R.T.: 0.000 min
Response: 17112351
Conc: 40.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

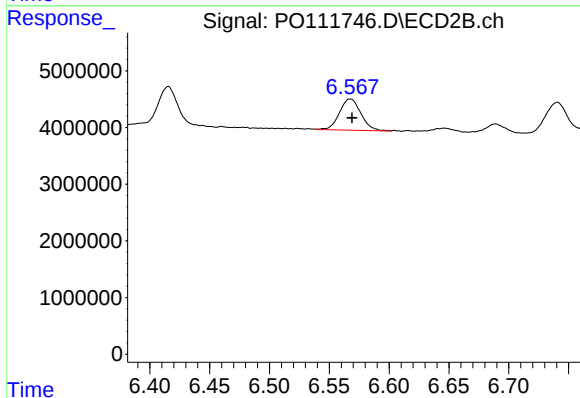


#33 AR-1260-3

R.T.: 6.568 min
Delta R.T.: -0.001 min
Response: 6904806
Conc: 25.84 ng/ml

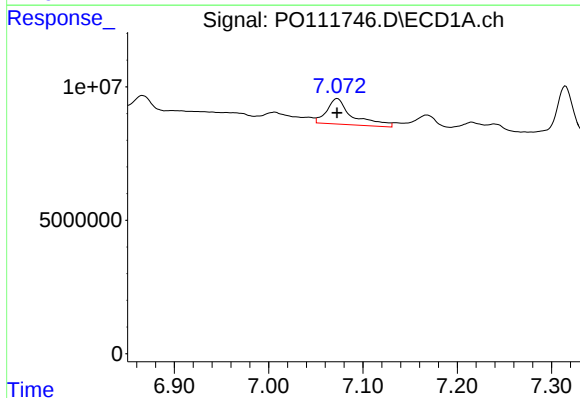


#34 AR-1260-4

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 17997698
Conc: 57.24 ng/ml

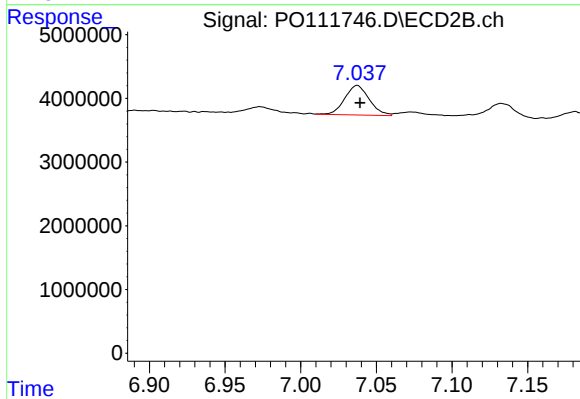

#34 AR-1260-4


R.T.: 7.037 min
Delta R.T.: -0.002 min
Response: 5209937
Conc: 27.41 ng/ml

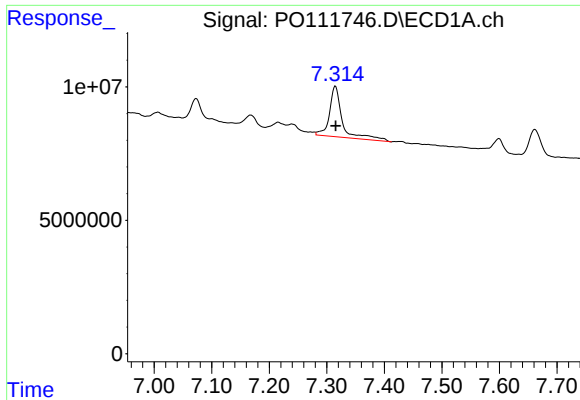

#35 AR-1260-5


R.T.: 7.315 min
Delta R.T.: 0.000 min
Response: 29734338
Conc: 36.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

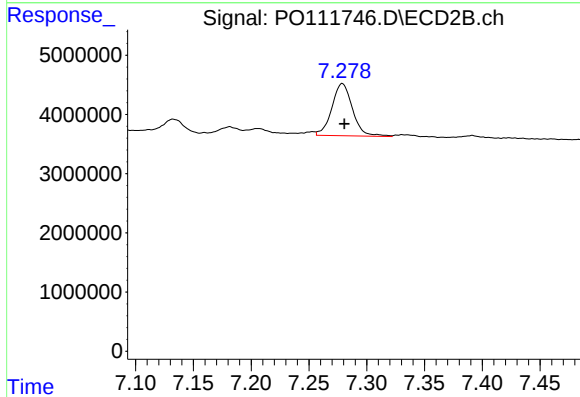


#35 AR-1260-5

R.T.: 7.279 min
Delta R.T.: -0.002 min
Response: 10983925
Conc: 25.84 ng/ml

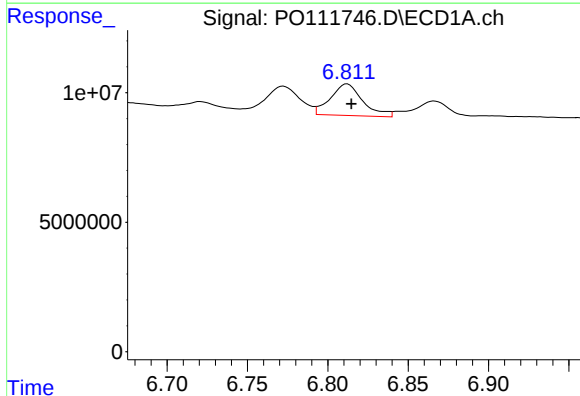


#36 AR-1262-1

R.T.: 6.812 min
Delta R.T.: -0.003 min
Response: 17112351
Conc: 28.06 ng/ml

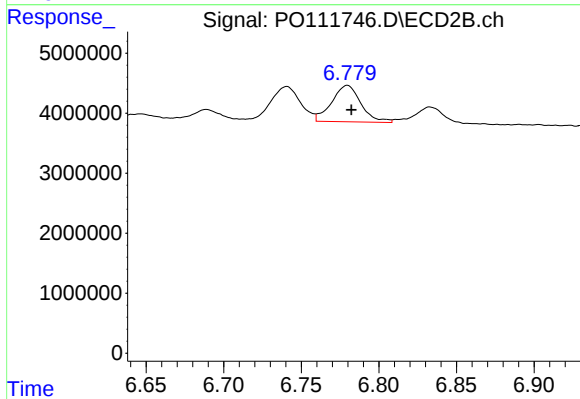

#36 AR-1262-1


R.T.: 6.780 min
Delta R.T.: -0.003 min
Response: 7941441
Conc: 23.52 ng/ml

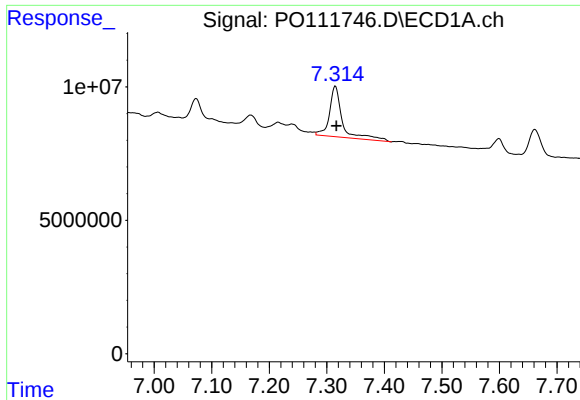

#37 AR-1262-2


R.T.: 7.315 min
Delta R.T.: -0.002 min
Response: 29734338
Conc: 31.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

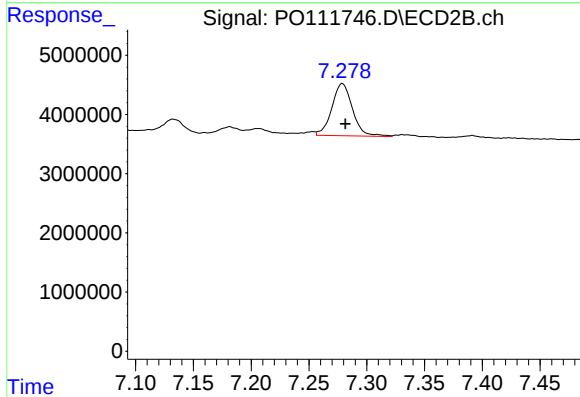


#37 AR-1262-2

R.T.: 7.279 min
Delta R.T.: -0.003 min
Response: 10983925
Conc: 23.58 ng/ml

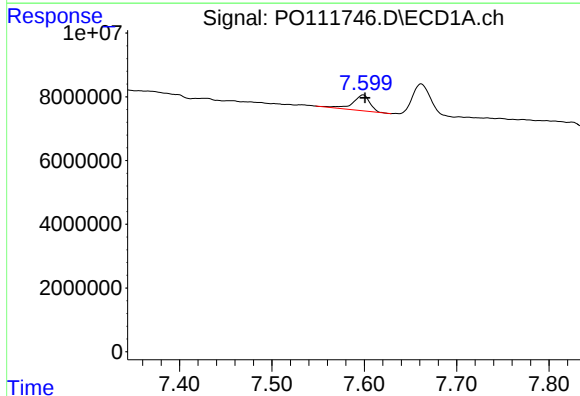


#38 AR-1262-3

R.T.: 7.599 min
Delta R.T.: -0.002 min
Response: 6477806
Conc: 16.33 ng/ml

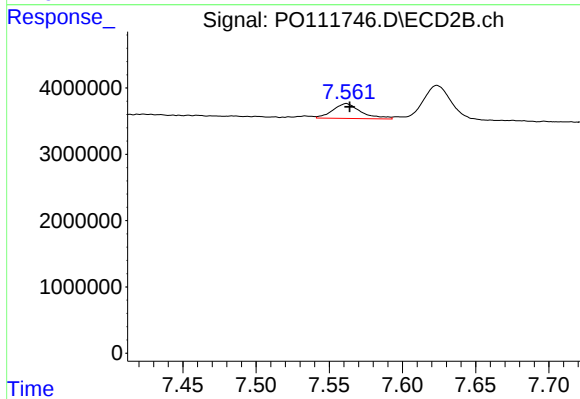

#38 AR-1262-3


R.T.: 7.562 min
Delta R.T.: -0.002 min
Response: 2994326
Conc: 18.01 ng/ml

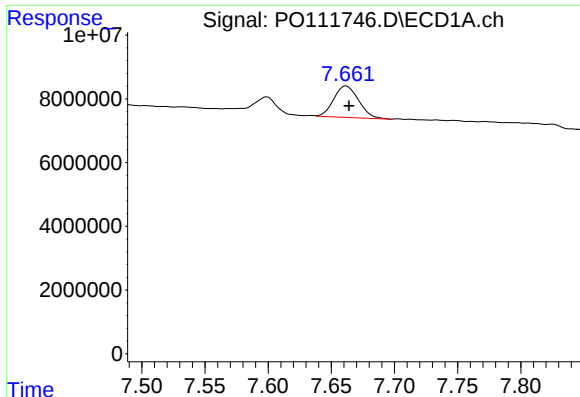

#39 AR-1262-4


R.T.: 7.662 min
Delta R.T.: -0.003 min
Response: 13488175
Conc: 20.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

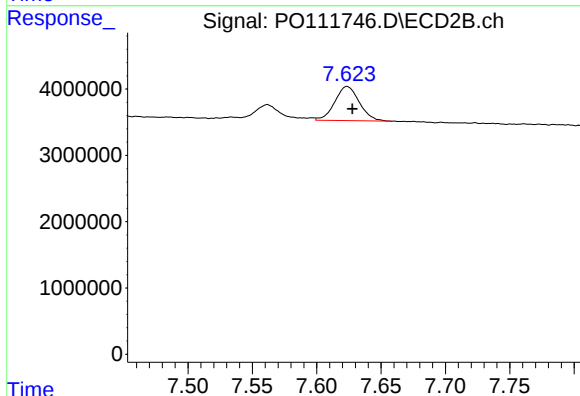


#39 AR-1262-4

R.T.: 7.624 min
Delta R.T.: -0.004 min
Response: 6839730
Conc: 24.69 ng/ml

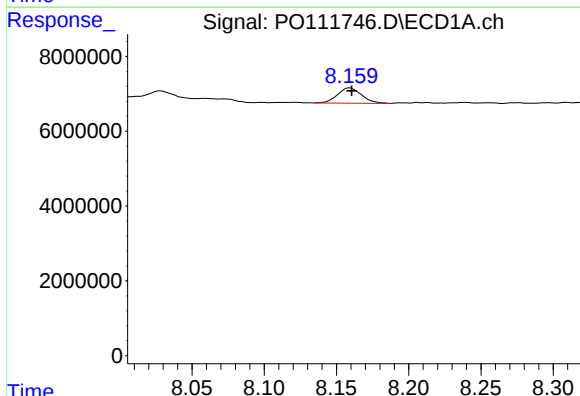


#40 AR-1262-5

R.T.: 8.159 min
Delta R.T.: -0.001 min
Response: 4745425
Conc: 15.58 ng/ml

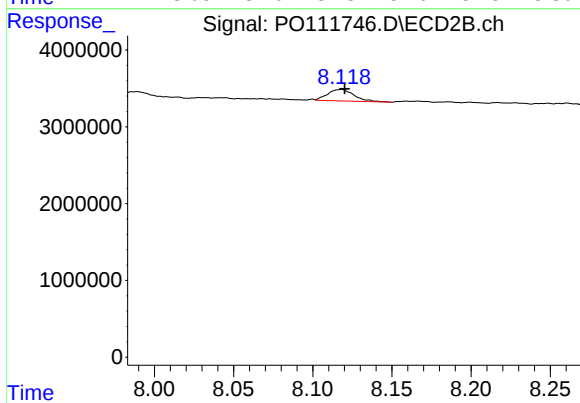

#40 AR-1262-5


R.T.: 8.118 min
Delta R.T.: -0.002 min
Response: 1747526
Conc: 17.20 ng/ml

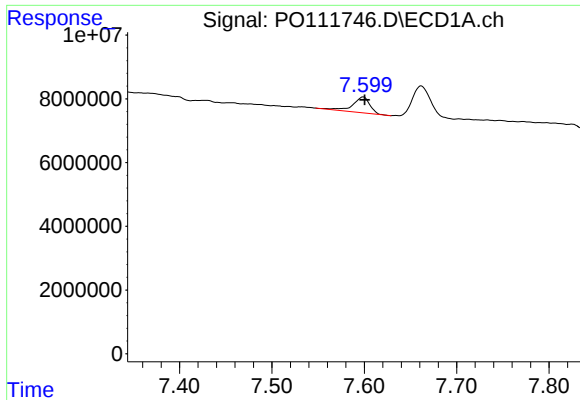

#41 AR-1268-1


R.T.: 7.599 min
Delta R.T.: -0.001 min
Response: 6477806
Conc: 5.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

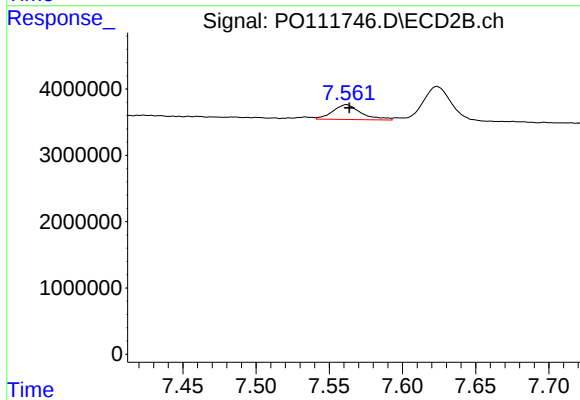


#41 AR-1268-1

R.T.: 7.562 min
Delta R.T.: -0.002 min
Response: 2994326
Conc: 6.26 ng/ml

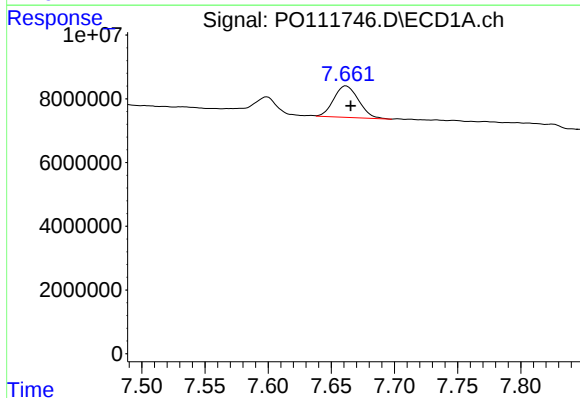


#42 AR-1268-2

R.T.: 7.662 min
Delta R.T.: -0.004 min
Response: 13488175
Conc: 13.80 ng/ml

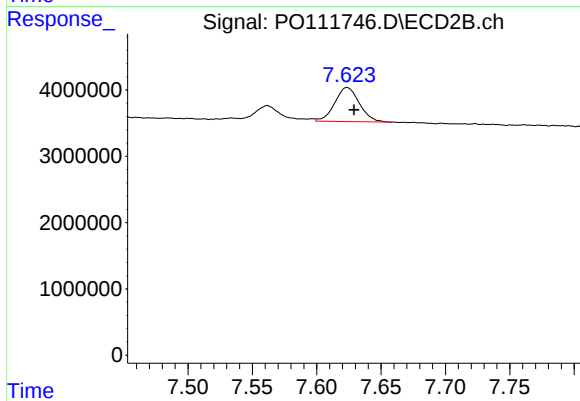

#42 AR-1268-2


R.T.: 7.624 min
Delta R.T.: -0.006 min
Response: 6839730
Conc: 16.42 ng/ml

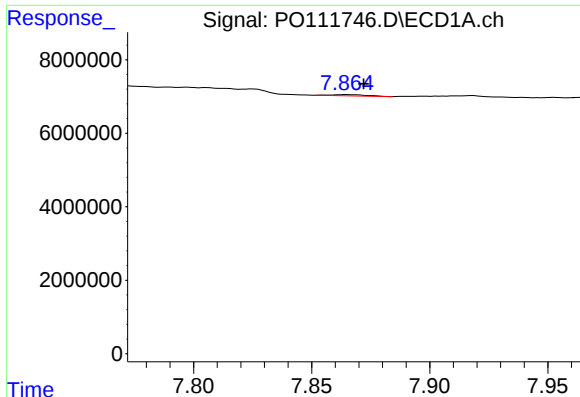

#43 AR-1268-3


R.T.: 7.865 min
Delta R.T.: -0.007 min
Response: 347155
Conc: 0.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

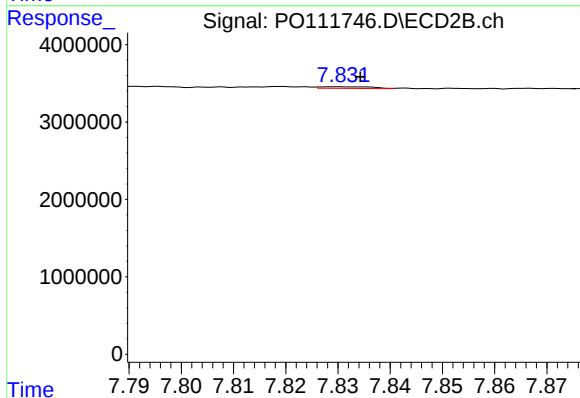


#43 AR-1268-3

R.T.: 7.830 min
Delta R.T.: -0.004 min
Response: 146465
Conc: 0.46 ng/ml

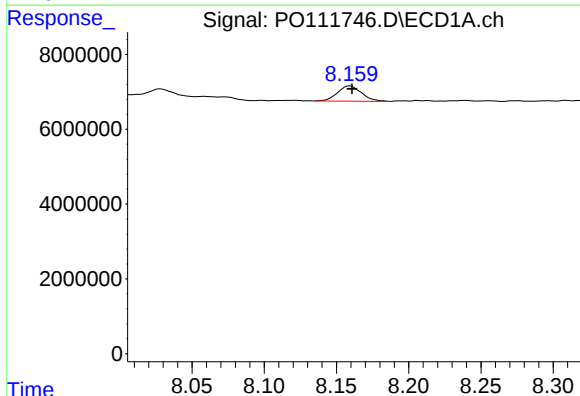


#44 AR-1268-4

R.T.: 8.159 min
Delta R.T.: -0.001 min
Response: 4745425
Conc: 13.80 ng/ml

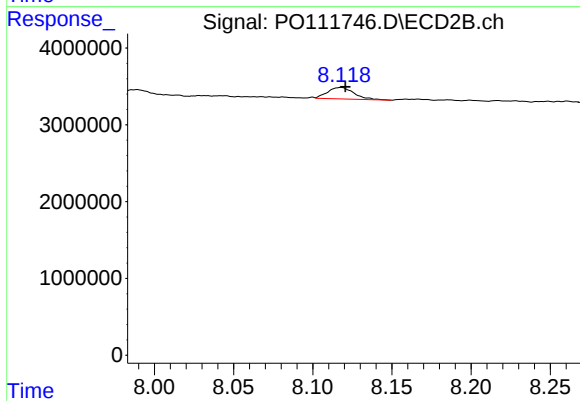

#44 AR-1268-4


R.T.: 8.118 min
Delta R.T.: -0.002 min
Response: 1747526
Conc: 15.11 ng/ml

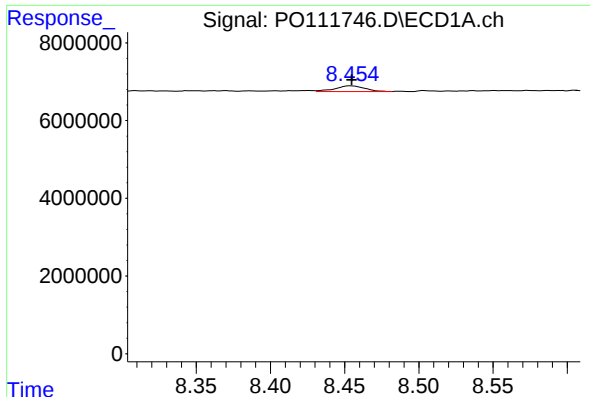

#45 AR-1268-5

R.T.: 8.454 min
Delta R.T.: 0.000 min
Response: 2059922
Conc: 0.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

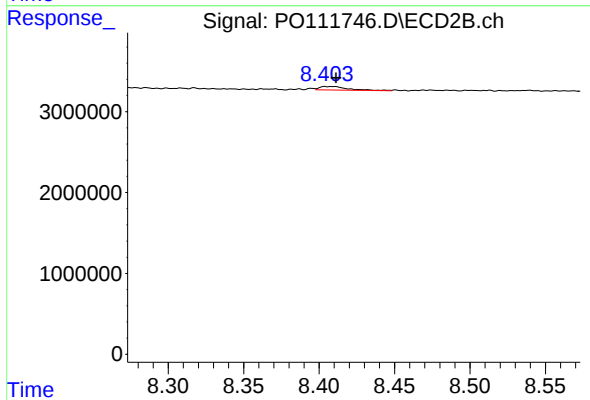

#45 AR-1268-5

R.T.: 8.404 min
Delta R.T.: -0.008 min
Response: 579371
Conc: 0.80 ng/ml