

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
 Data File : P0111747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 10:34
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:02:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.678	3.673	129.8E6	112.4E6	22.542	20.011
2)	SA Decachlor...	8.712	8.660	114.0E6	37450807	21.722	21.067
Target Compounds							
3)	L1 AR-1016-1	4.770	4.749	1565050	1558398	6.561	7.920
4)	L1 AR-1016-2	4.786	4.768	954138	1623474	2.867	5.699 #
5)	L1 AR-1016-3	4.842	4.942	1537113	527076	6.679	3.508 #
6)	L1 AR-1016-4	4.959	4.978	1003075	639841	5.409	5.254
7)	L1 AR-1016-5	5.214	5.199	784101	209122	4.201	1.314 #
8)	L2 AR-1221-1	3.891	3.883	1948756	1789341	22.379	23.962
9)	L2 AR-1221-2	3.977	3.969	3502899	2906948	54.590	51.957
10)	L2 AR-1221-3	4.051	4.043	4466701	3784502	22.902	22.025
11)	L3 AR-1232-1	4.051	4.043	4466701	3784502	29.435	28.457
12)	L3 AR-1232-2	4.542	4.768	769011	1623474	8.919	12.319 #
13)	L3 AR-1232-3	4.786	4.942	954138	527076	5.858	7.626 #
14)	L3 AR-1232-4	4.959	5.029	1003075	553751	11.527	9.155
15)	L3 AR-1232-5	5.006	5.199	874762	209122	15.460	3.149 #
16)	L4 AR-1242-1	4.770	4.749	1565050	1558398	7.769	9.575
17)	L4 AR-1242-2	4.786	4.768	954138	1623474	3.386	6.877 #
18)	L4 AR-1242-3	4.842	4.942	1537113	527076	7.731	4.197 #
19)	L4 AR-1242-4	4.959	5.029	1003075	553751	6.341	4.518 #
20)	L4 AR-1242-5	5.626	5.547	3600806	731428	21.534	4.880 #
21)	L5 AR-1248-1	4.770	4.749	1565050	1558398	9.705	11.692
22)	L5 AR-1248-2	5.006	4.978	874762	639841	4.057	3.591
23)	L5 AR-1248-3	5.214	5.029	784101	553751	2.907	2.923
24)	L5 AR-1248-4	5.576	5.199	3124638	209122	7.815	0.916 #
25)	L5 AR-1248-5	5.626	5.592	3600806	1555337	12.823	7.142 #
26)	L6 AR-1254-1	5.576	5.547	3124638	731428	7.351	2.264 #
27)	L6 AR-1254-2	5.722	5.700	2526288	1875631	6.656	6.715
28)	L6 AR-1254-3	6.119	6.162f	3348379	1600646	5.860	3.820 #
29)	L6 AR-1254-4	6.333	6.348	12506847	774344	35.848	3.399 #
30)	L6 AR-1254-5	6.755	6.750	932502	89112	1.821	0.274 #
31)	L7 AR-1260-1	6.251	6.229	8450404	1788634	23.782	7.128 #
32)	L7 AR-1260-2	6.439	6.389	3953637	3418725	8.368	11.628 #
33)	L7 AR-1260-3	6.813	6.598	8229490	220327	19.378	0.825 #
34)	L7 AR-1260-4	7.070	7.032	2286864	582390	7.273	3.064 #
35)	L7 AR-1260-5	7.324	7.280	2673075	1697385	3.245	3.994
36)	L8 AR-1262-1	6.813	6.777	8229490	1692068	13.494	5.011 #
37)	L8 AR-1262-2	7.324	7.280	2673075	1697385	2.839	3.644 #
38)	L8 AR-1262-3	7.609	7.565	-683577	423182	N.D.	2.545 #
40)	L8 AR-1262-5	8.165	8.150	38189	27619	0.125	0.272 #
41)	L9 AR-1268-1	7.609	7.565	-683577	423182	N.D.	0.885 #
43)	L9 AR-1268-3	7.868	7.824	304682	182870	0.372	0.577 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
Data File : P0111747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 10:34
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:02:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	8.165	8.150	38189	27619	0.111	0.239 #
45)	L9 AR-1268-5	8.453	8.408	670743	210383	0.302	0.290


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062025\
Data File : PO111747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 10:34
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:02:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

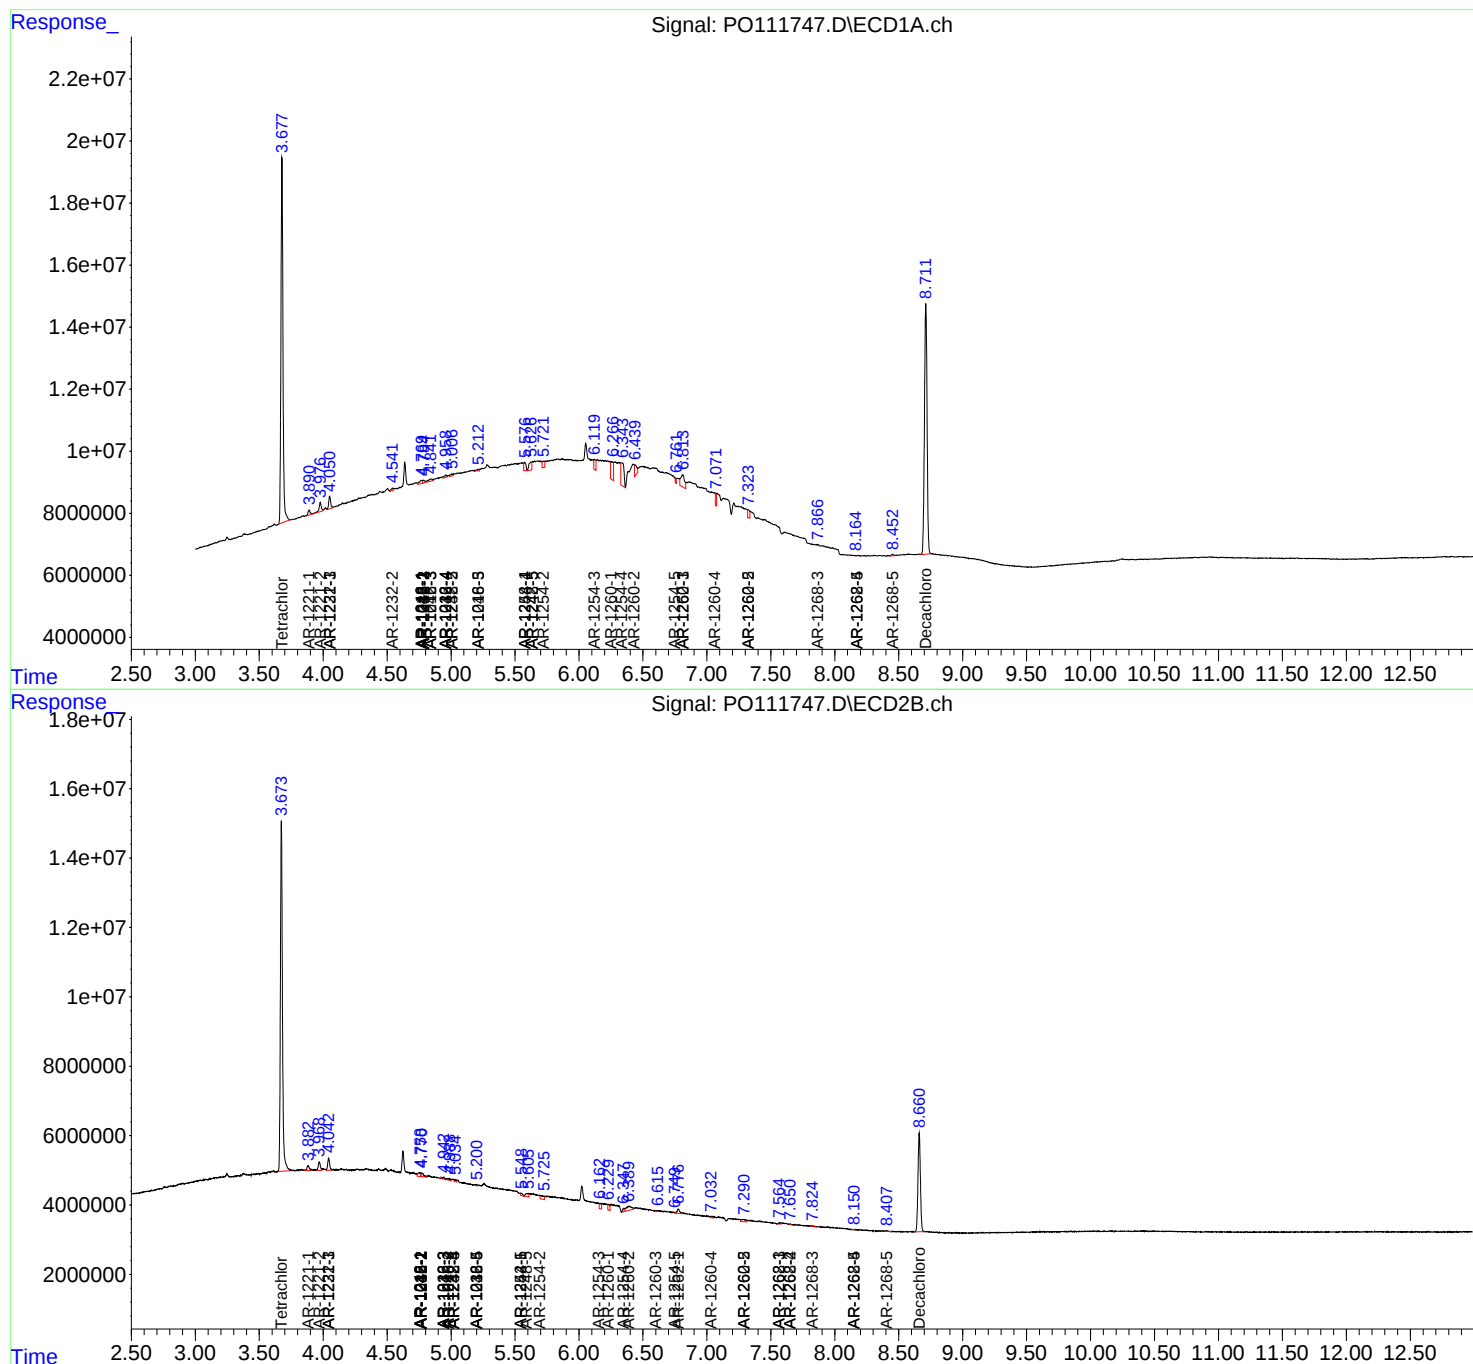


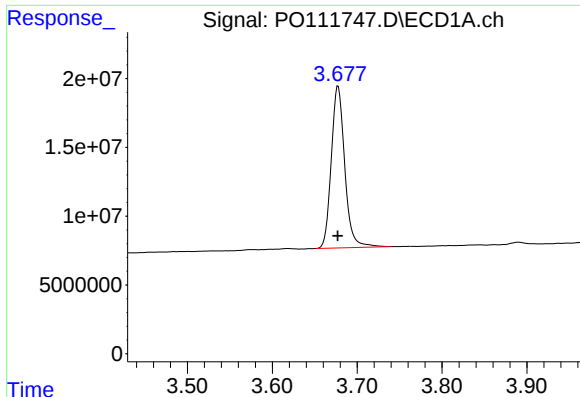

#1 Tetrachloro-m-xylene


R.T.: 3.678 min
Delta R.T.: 0.000 min
Response: 129827811
Conc: 22.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

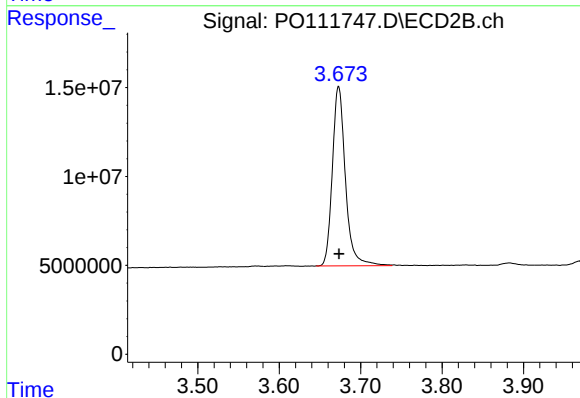


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 112405272
Conc: 20.01 ng/ml

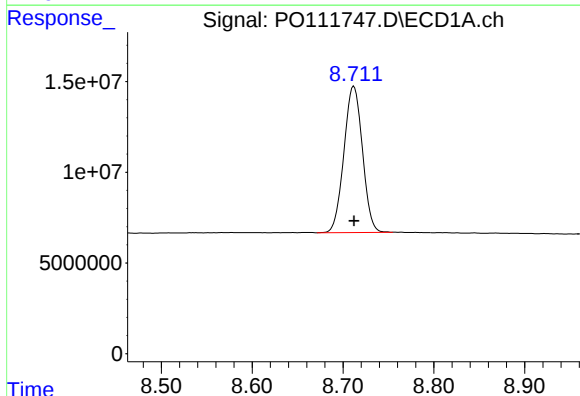


#2 Decachlorobiphenyl

R.T.: 8.712 min
Delta R.T.: 0.000 min
Response: 114026356
Conc: 21.72 ng/ml

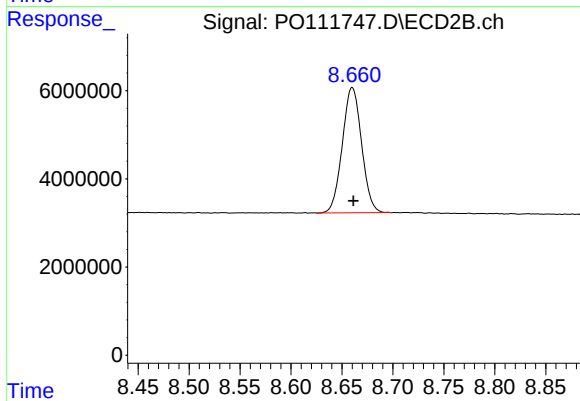

#2 Decachlorobiphenyl


R.T.: 8.660 min
Delta R.T.: -0.001 min
Response: 37450807
Conc: 21.07 ng/ml

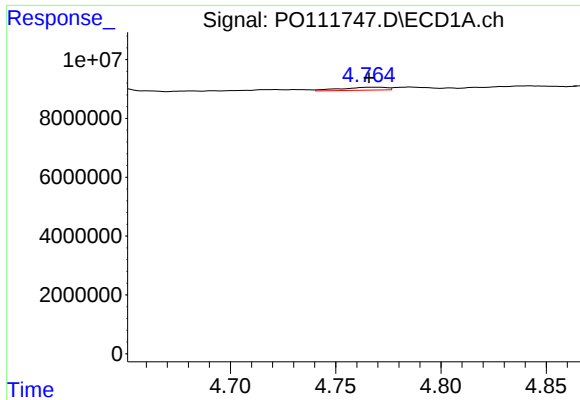

#3 AR-1016-1


R.T.: 4.770 min
Delta R.T.: 0.004 min
Response: 1565050
Conc: 6.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

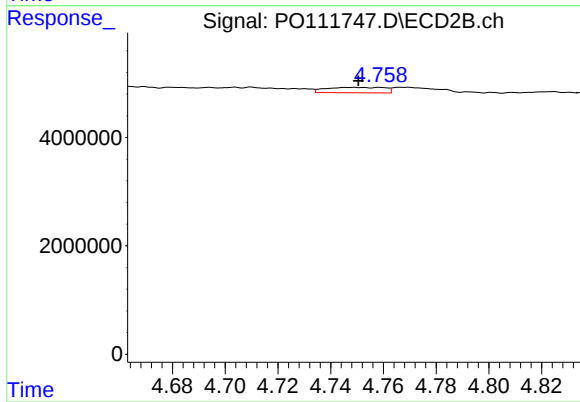


#3 AR-1016-1

R.T.: 4.749 min
Delta R.T.: -0.002 min
Response: 1558398
Conc: 7.92 ng/ml

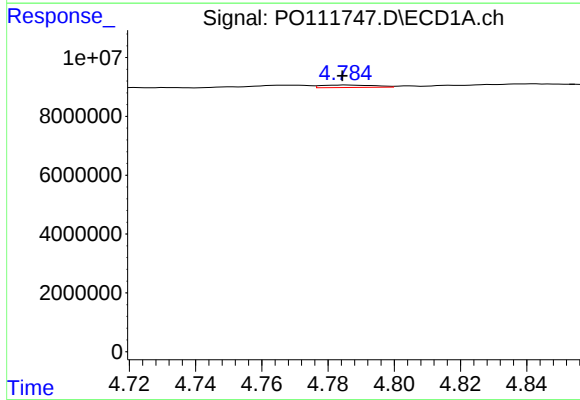


#4 AR-1016-2

R.T.: 4.786 min
Delta R.T.: 0.001 min
Response: 954138
Conc: 2.87 ng/ml

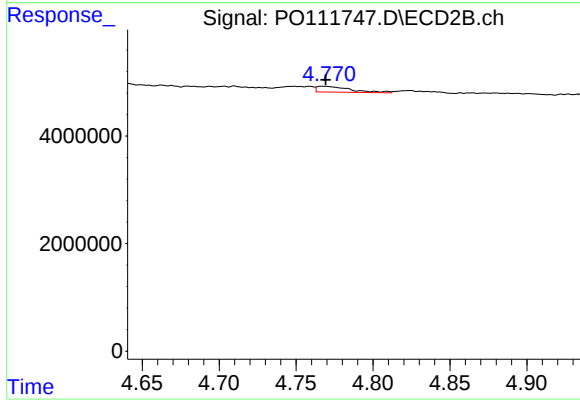

#4 AR-1016-2


R.T.: 4.768 min
Delta R.T.: -0.002 min
Response: 1623474
Conc: 5.70 ng/ml

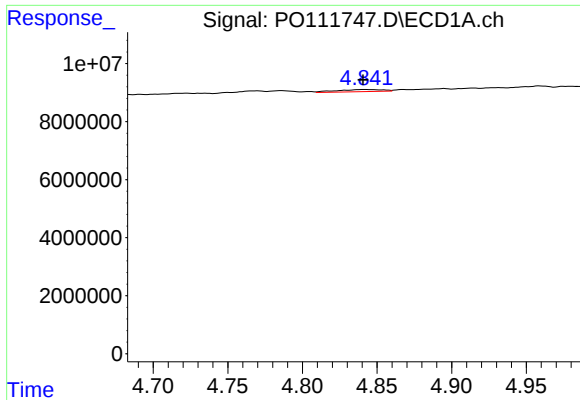

#5 AR-1016-3


R.T.: 4.842 min
Delta R.T.: 0.001 min
Response: 1537113
Conc: 6.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

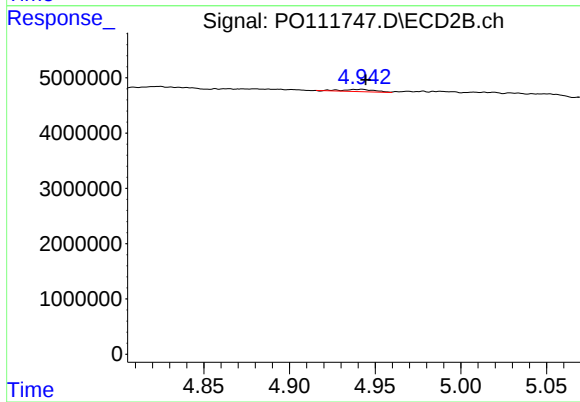


#5 AR-1016-3

R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 527076
Conc: 3.51 ng/ml

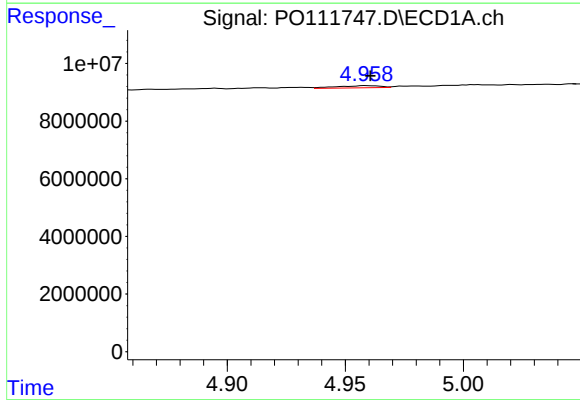


#6 AR-1016-4

R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 1003075
Conc: 5.41 ng/ml

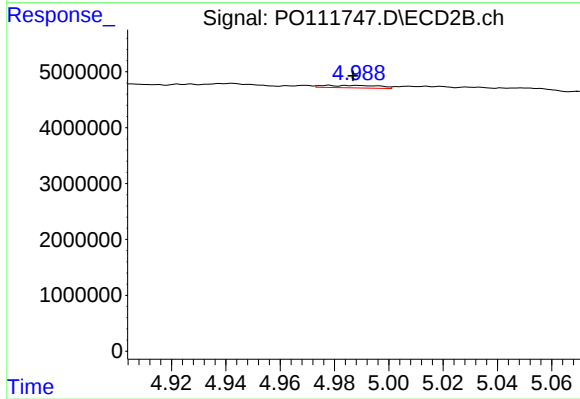

#6 AR-1016-4


R.T.: 4.978 min
Delta R.T.: -0.009 min
Response: 639841
Conc: 5.25 ng/ml

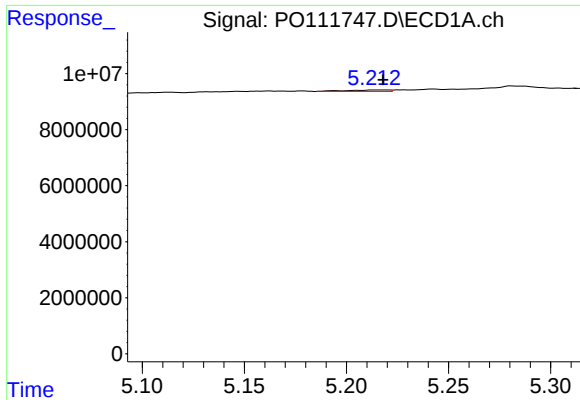

#7 AR-1016-5


R.T.: 5.214 min
Delta R.T.: -0.004 min
Response: 784101
Conc: 4.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

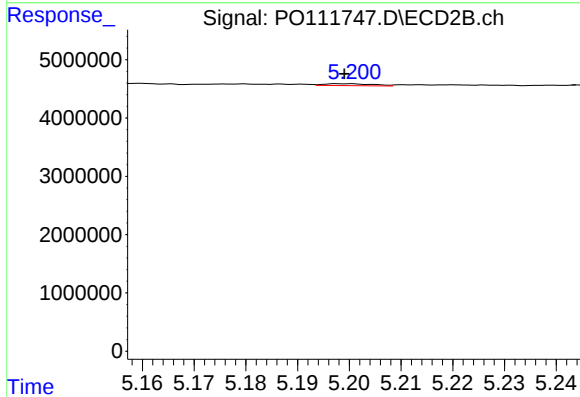


#7 AR-1016-5

R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 209122
Conc: 1.31 ng/ml

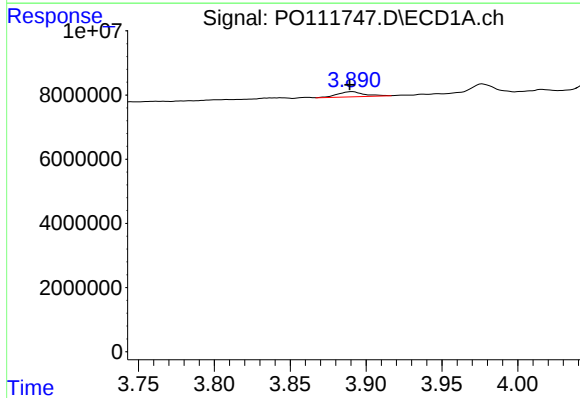


#8 AR-1221-1

R.T.: 3.891 min
Delta R.T.: 0.002 min
Response: 1948756
Conc: 22.38 ng/ml

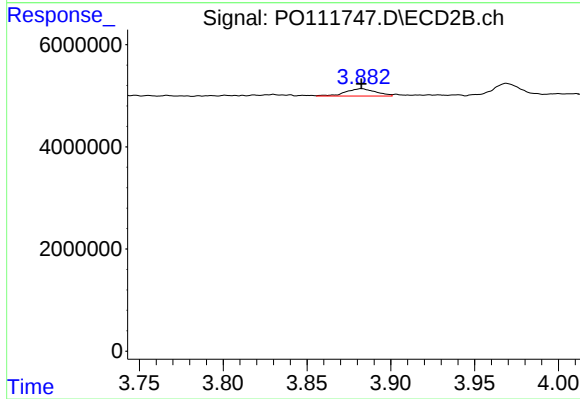

#8 AR-1221-1


R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 1789341
Conc: 23.96 ng/ml

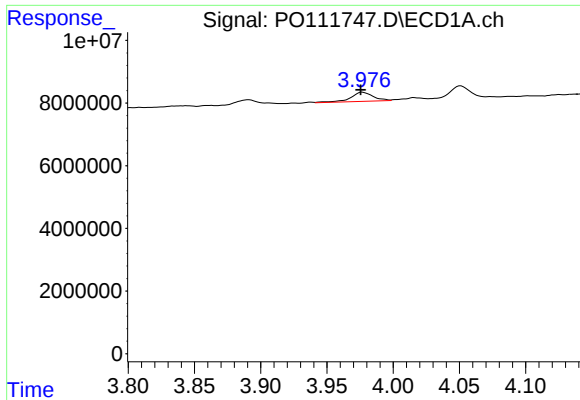

#9 AR-1221-2


R.T.: 3.977 min
Delta R.T.: 0.001 min
Response: 3502899
Conc: 54.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

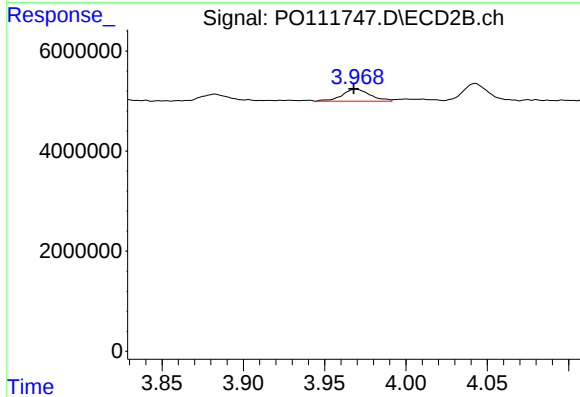


#9 AR-1221-2

R.T.: 3.969 min
Delta R.T.: 0.001 min
Response: 2906948
Conc: 51.96 ng/ml

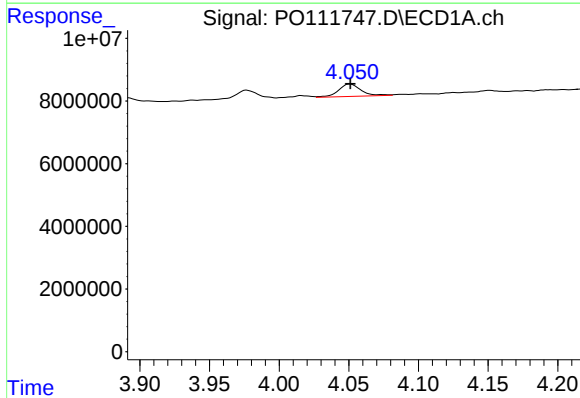


#10 AR-1221-3

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 4466701
Conc: 22.90 ng/ml

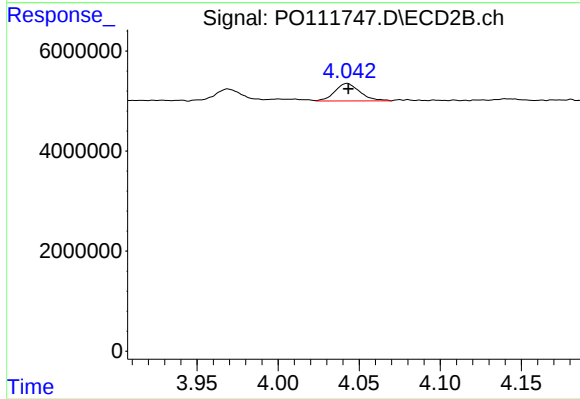

#10 AR-1221-3


R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 3784502
Conc: 22.02 ng/ml

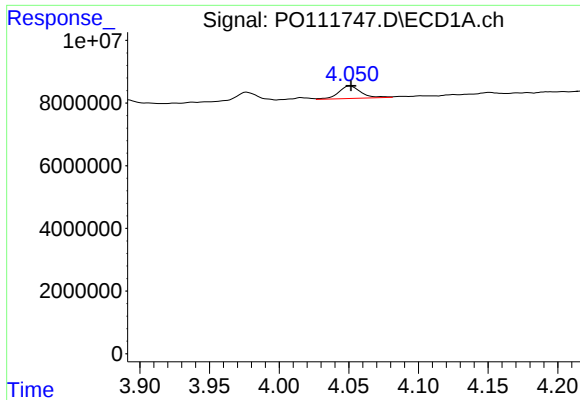

#11 AR-1232-1


R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 4466701
Conc: 29.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

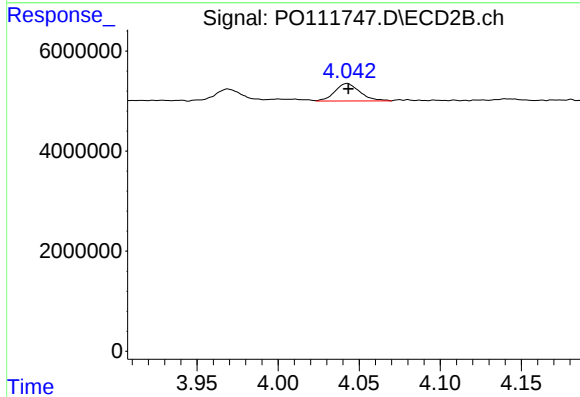


#11 AR-1232-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 3784502
Conc: 28.46 ng/ml

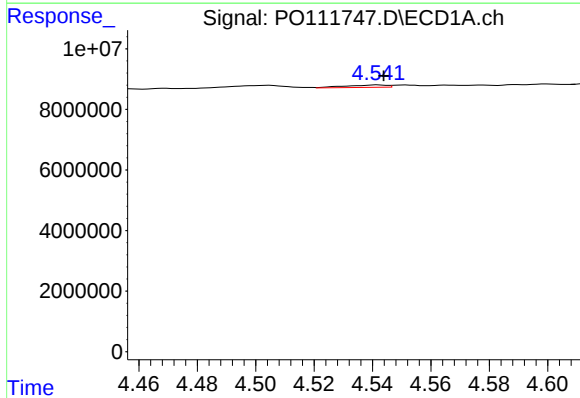


#12 AR-1232-2

R.T.: 4.542 min
Delta R.T.: -0.002 min
Response: 769011
Conc: 8.92 ng/ml

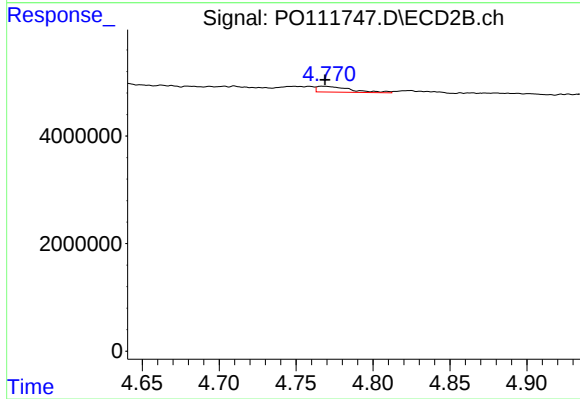

#12 AR-1232-2


R.T.: 4.768 min
Delta R.T.: -0.001 min
Response: 1623474
Conc: 12.32 ng/ml

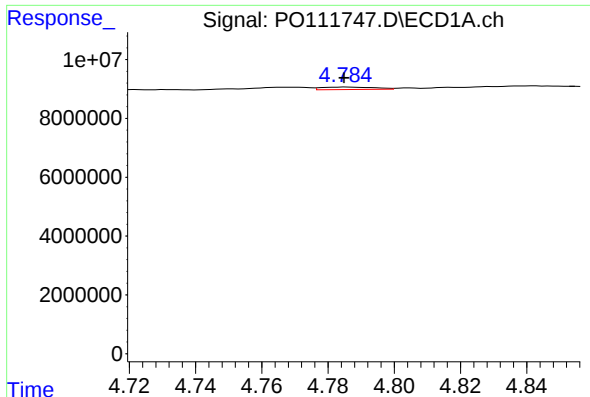

#13 AR-1232-3


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 954138
Conc: 5.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

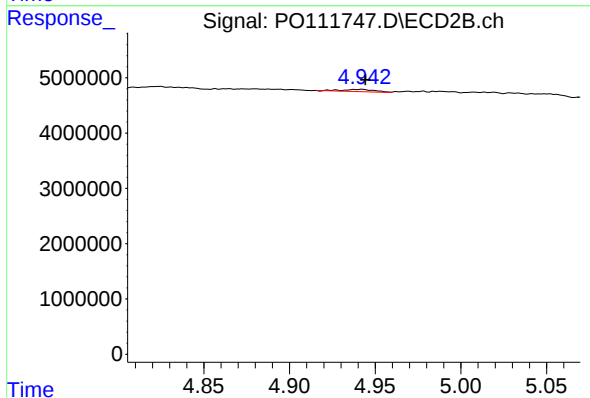


#13 AR-1232-3

R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 527076
Conc: 7.63 ng/ml

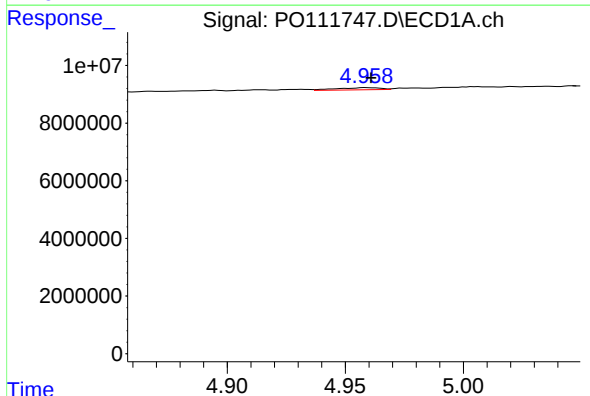


#14 AR-1232-4

R.T.: 4.959 min
Delta R.T.: -0.002 min
Response: 1003075
Conc: 11.53 ng/ml

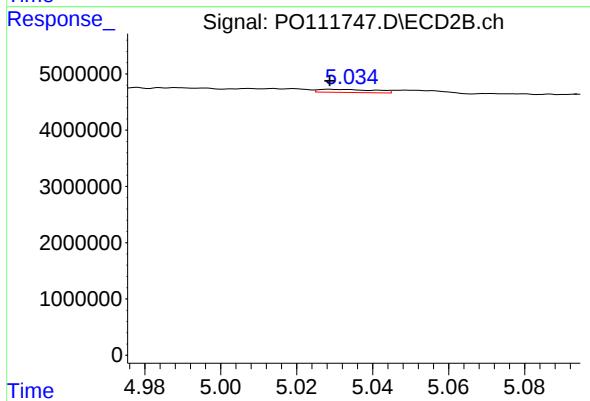

#14 AR-1232-4


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 553751
Conc: 9.16 ng/ml

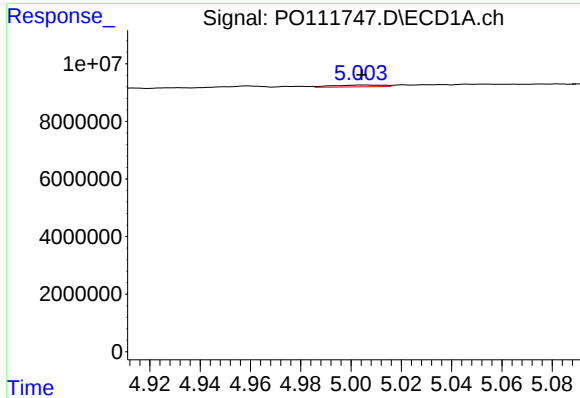

#15 AR-1232-5


R.T.: 5.006 min
Delta R.T.: 0.001 min
Response: 874762
Conc: 15.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

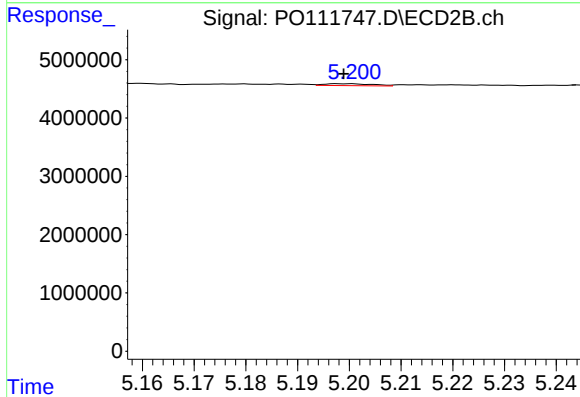


#15 AR-1232-5

R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 209122
Conc: 3.15 ng/ml

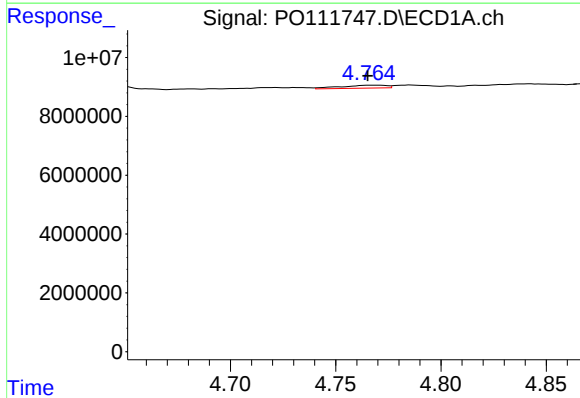


#16 AR-1242-1

R.T.: 4.770 min
Delta R.T.: 0.005 min
Response: 1565050
Conc: 7.77 ng/ml

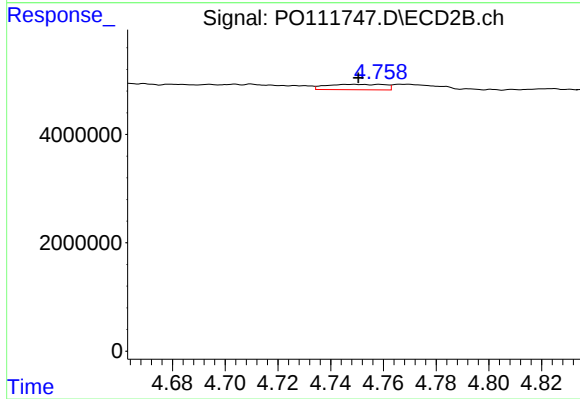

#16 AR-1242-1


R.T.: 4.749 min
Delta R.T.: -0.002 min
Response: 1558398
Conc: 9.57 ng/ml

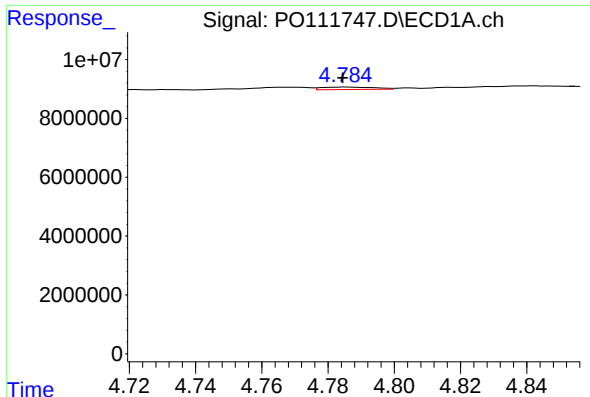

#17 AR-1242-2


R.T.: 4.786 min
Delta R.T.: 0.001 min
Response: 954138
Conc: 3.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

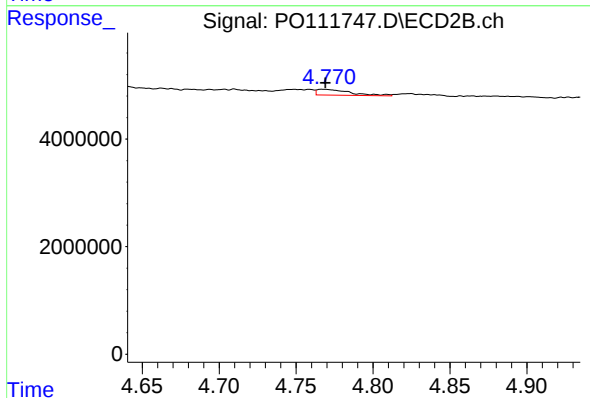


#17 AR-1242-2

R.T.: 4.768 min
Delta R.T.: -0.001 min
Response: 1623474
Conc: 6.88 ng/ml

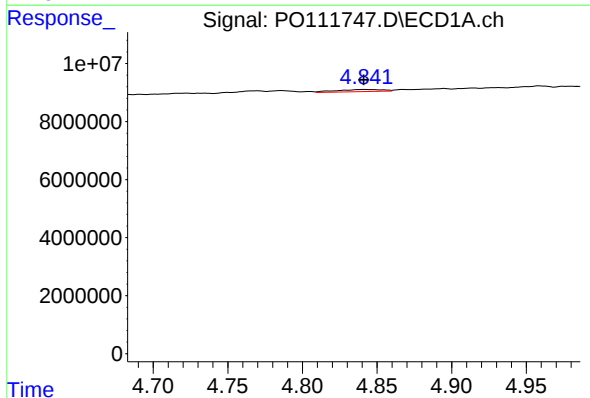


#18 AR-1242-3

R.T.: 4.842 min
Delta R.T.: 0.000 min
Response: 1537113
Conc: 7.73 ng/ml

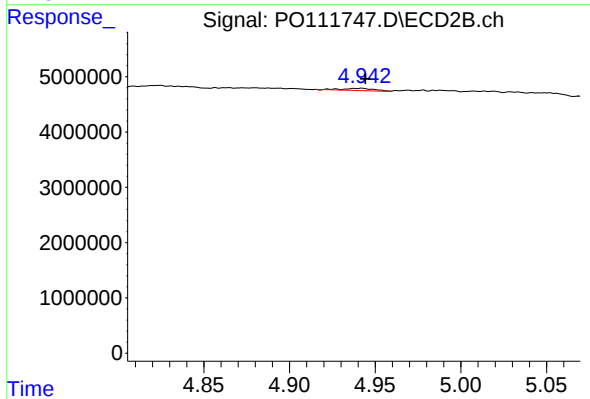

#18 AR-1242-3


R.T.: 4.942 min
Delta R.T.: -0.002 min
Response: 527076
Conc: 4.20 ng/ml

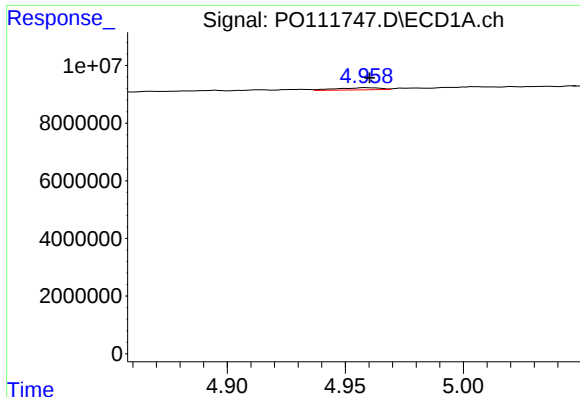

#19 AR-1242-4


R.T.: 4.959 min
Delta R.T.: -0.001 min
Response: 1003075
Conc: 6.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

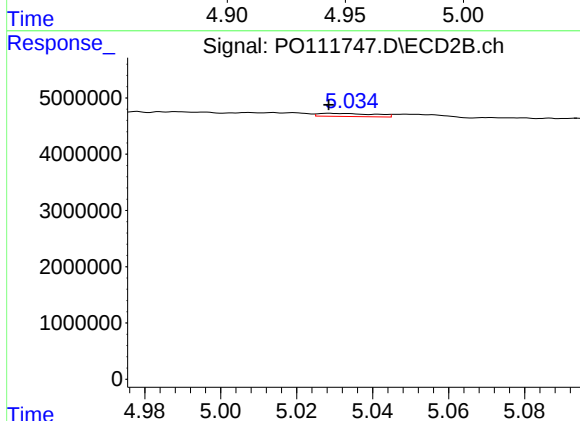


#19 AR-1242-4

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 553751
Conc: 4.52 ng/ml

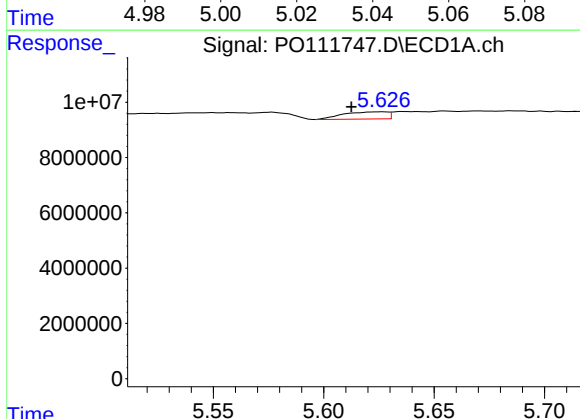


#20 AR-1242-5

R.T.: 5.626 min
Delta R.T.: 0.014 min
Response: 3600806
Conc: 21.53 ng/ml

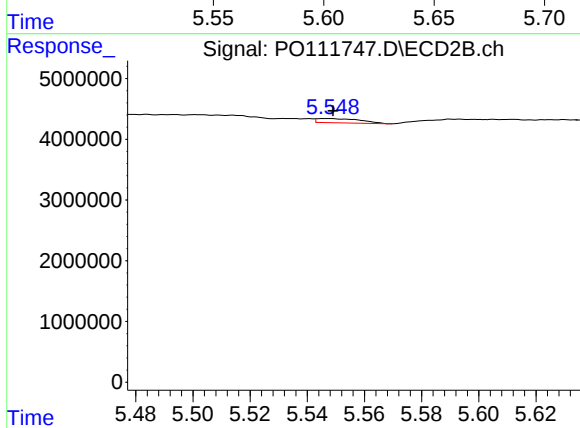

#20 AR-1242-5


R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 731428
Conc: 4.88 ng/ml

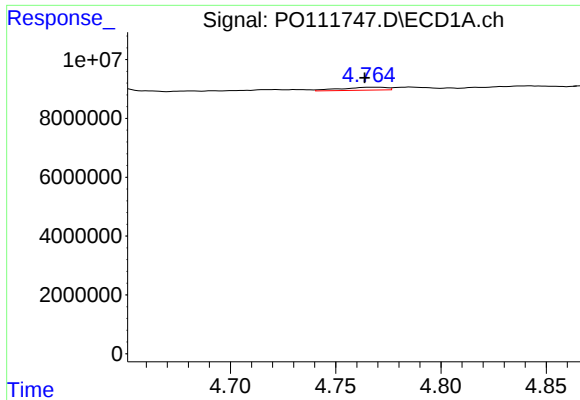

#21 AR-1248-1


R.T.: 4.770 min
Delta R.T.: 0.006 min
Response: 1565050
Conc: 9.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

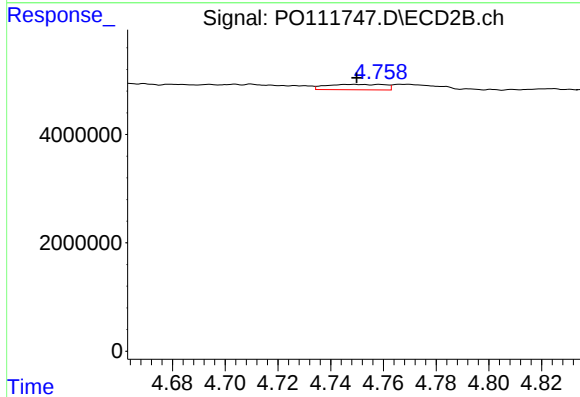


#21 AR-1248-1

R.T.: 4.749 min
Delta R.T.: -0.001 min
Response: 1558398
Conc: 11.69 ng/ml

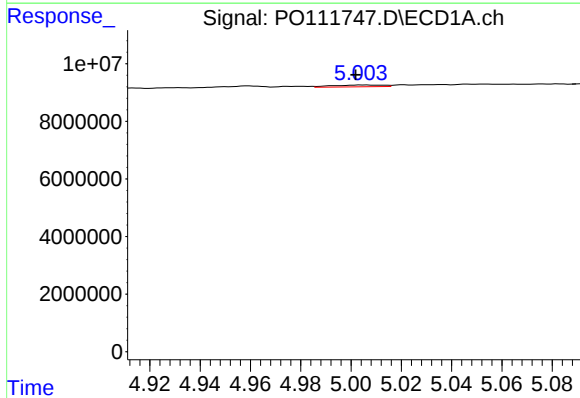


#22 AR-1248-2

R.T.: 5.006 min
Delta R.T.: 0.004 min
Response: 874762
Conc: 4.06 ng/ml

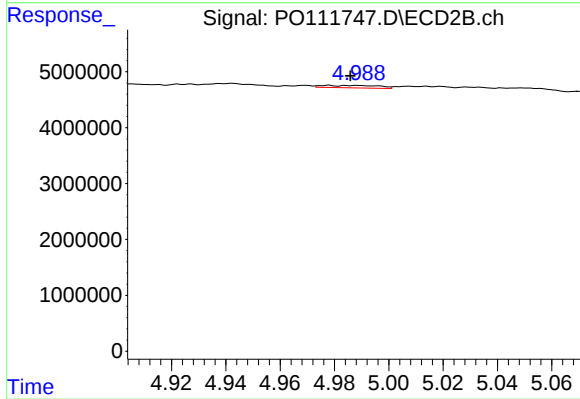

#22 AR-1248-2


R.T.: 4.978 min
Delta R.T.: -0.008 min
Response: 639841
Conc: 3.59 ng/ml

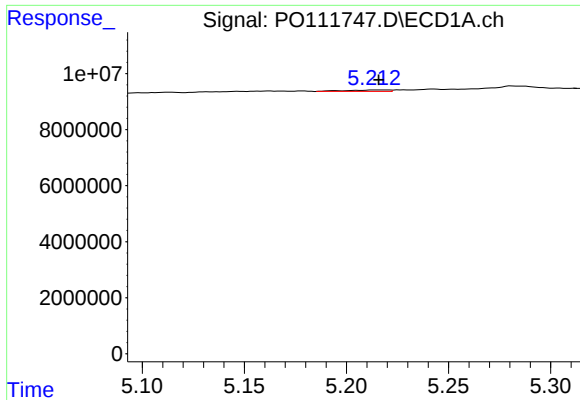

#23 AR-1248-3


R.T.: 5.214 min
Delta R.T.: -0.002 min
Response: 784101
Conc: 2.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

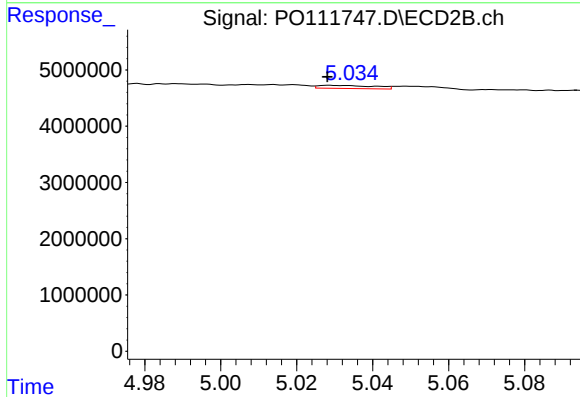


#23 AR-1248-3

R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 553751
Conc: 2.92 ng/ml

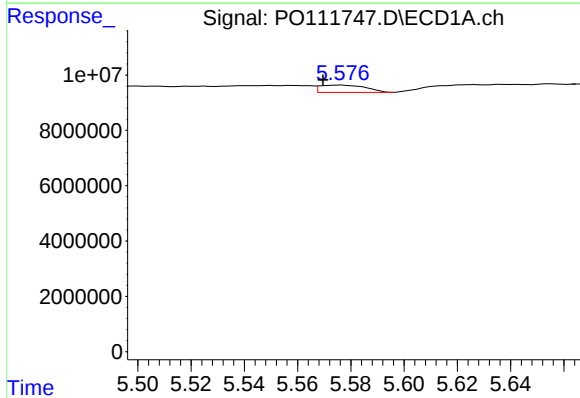


#24 AR-1248-4

R.T.: 5.576 min
Delta R.T.: 0.007 min
Response: 3124638
Conc: 7.82 ng/ml

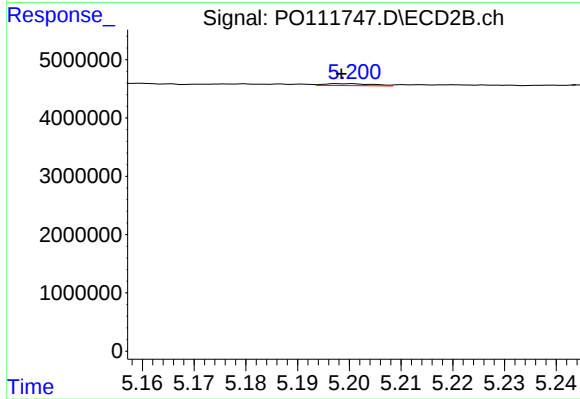

#24 AR-1248-4


R.T.: 5.199 min
Delta R.T.: 0.000 min
Response: 209122
Conc: 0.92 ng/ml

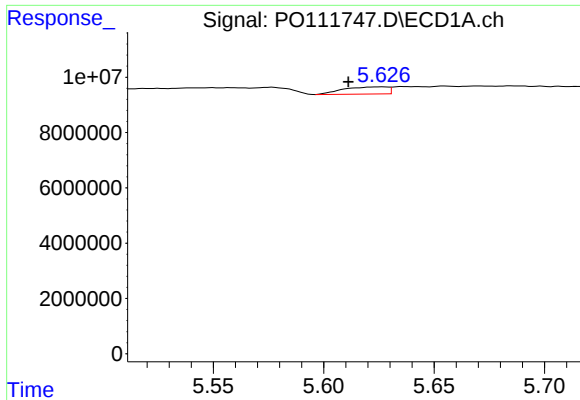

#25 AR-1248-5


R.T.: 5.626 min
Delta R.T.: 0.015 min
Response: 3600806
Conc: 12.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

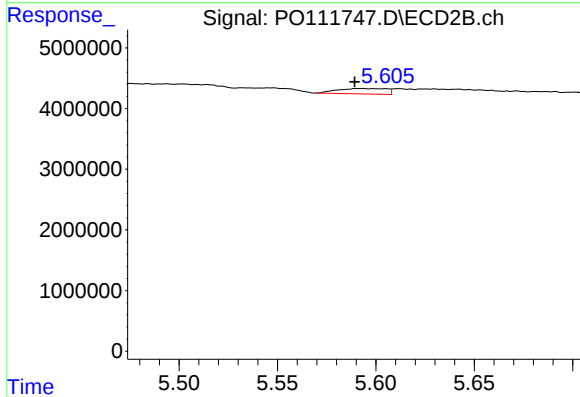


#25 AR-1248-5

R.T.: 5.592 min
Delta R.T.: 0.003 min
Response: 1555337
Conc: 7.14 ng/ml

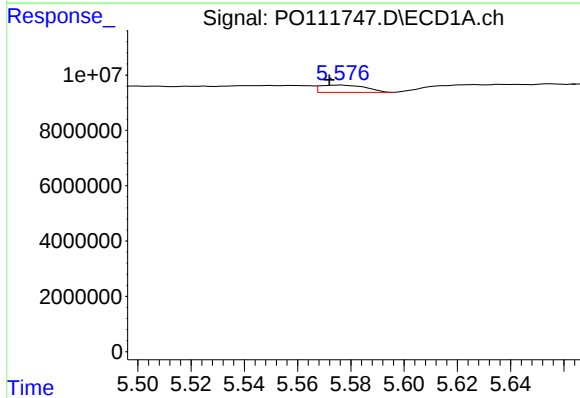


#26 AR-1254-1

R.T.: 5.576 min
Delta R.T.: 0.004 min
Response: 3124638
Conc: 7.35 ng/ml

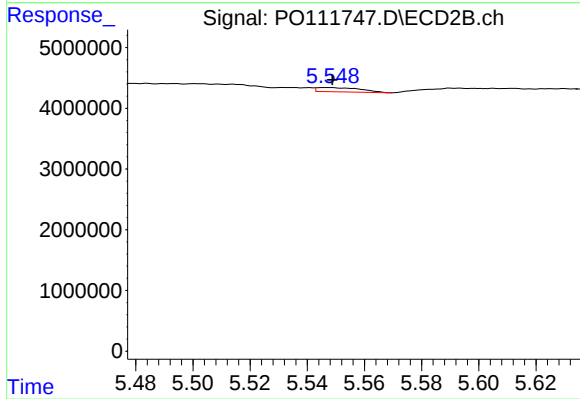

#26 AR-1254-1


R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 731428
Conc: 2.26 ng/ml

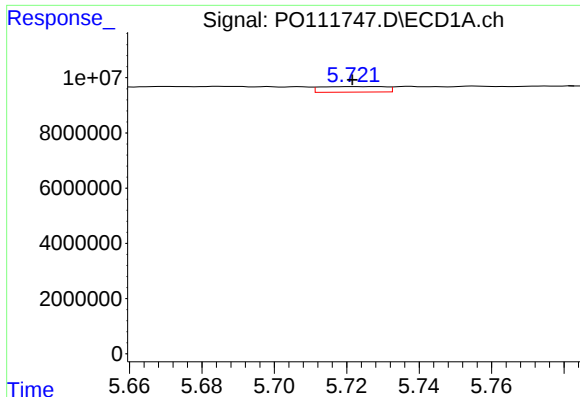

#27 AR-1254-2


R.T.: 5.722 min
Delta R.T.: 0.000 min
Response: 2526288
Conc: 6.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

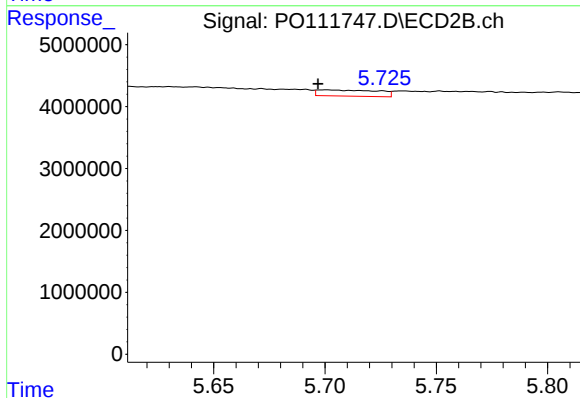


#27 AR-1254-2

R.T.: 5.700 min
Delta R.T.: 0.004 min
Response: 1875631
Conc: 6.72 ng/ml

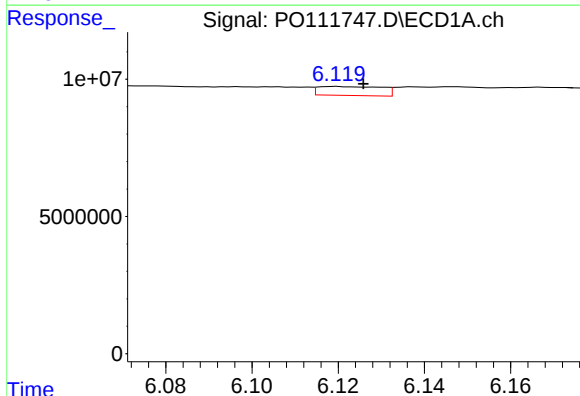


#28 AR-1254-3

R.T.: 6.119 min
Delta R.T.: -0.006 min
Response: 3348379
Conc: 5.86 ng/ml

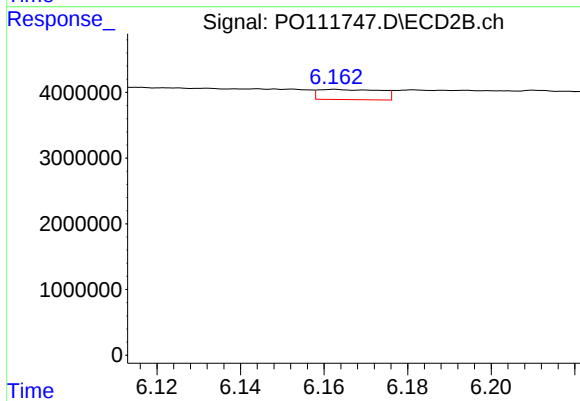

#28 AR-1254-3


R.T.: 6.162 min
Delta R.T.: 0.064 min
Response: 1600646
Conc: 3.82 ng/ml

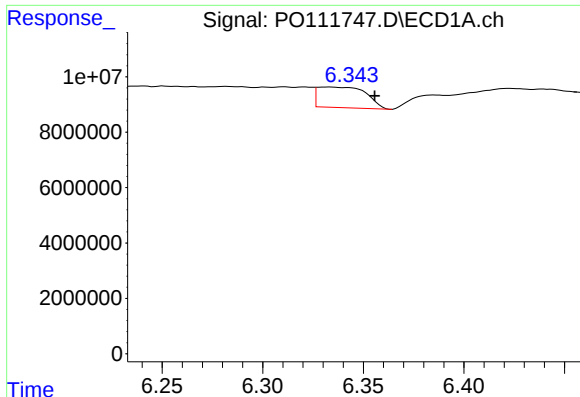

#29 AR-1254-4


R.T.: 6.333 min
Delta R.T.: -0.023 min
Response: 12506847
Conc: 35.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

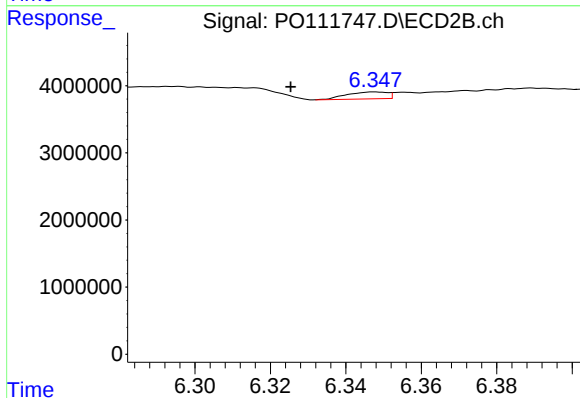


#29 AR-1254-4

R.T.: 6.348 min
Delta R.T.: 0.023 min
Response: 774344
Conc: 3.40 ng/ml

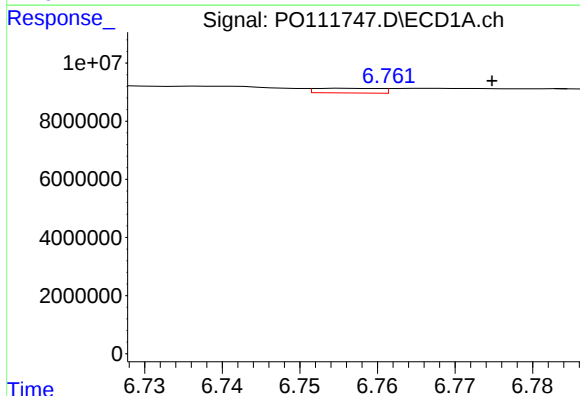


#30 AR-1254-5

R.T.: 6.755 min
Delta R.T.: -0.019 min
Response: 932502
Conc: 1.82 ng/ml

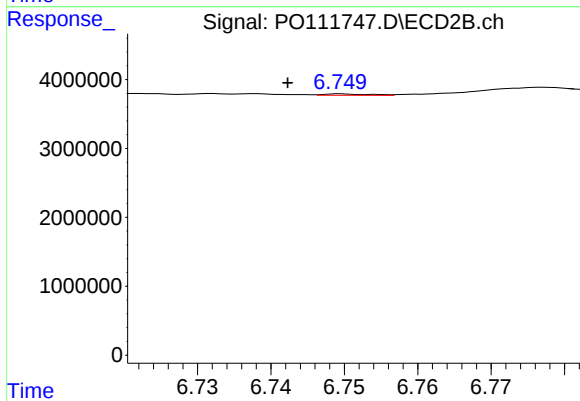

#30 AR-1254-5


R.T.: 6.750 min
Delta R.T.: 0.007 min
Response: 89112
Conc: 0.27 ng/ml

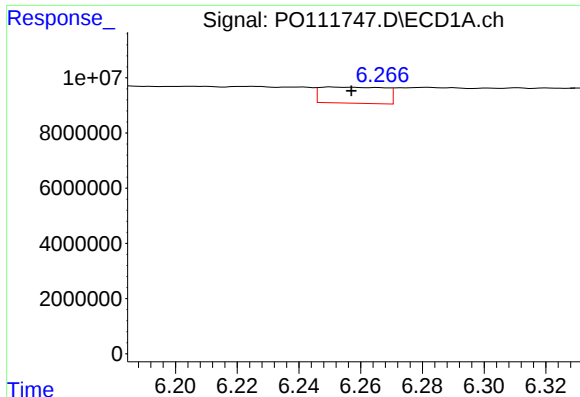

#31 AR-1260-1


R.T.: 6.251 min
Delta R.T.: -0.006 min
Response: 8450404
Conc: 23.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

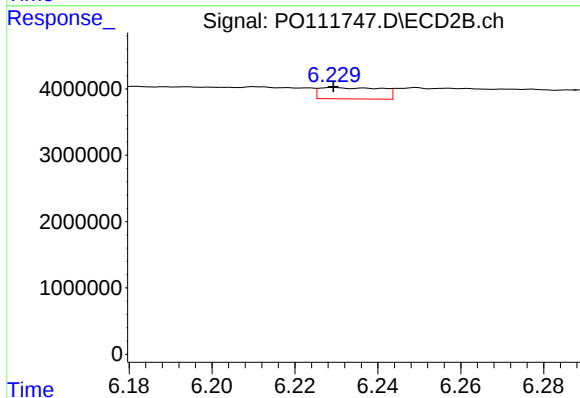


#31 AR-1260-1

R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 1788634
Conc: 7.13 ng/ml

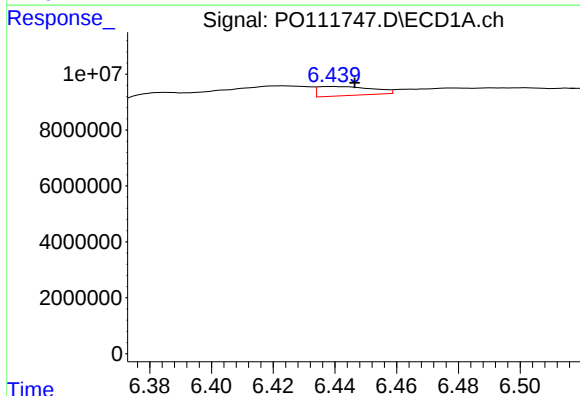


#32 AR-1260-2

R.T.: 6.439 min
Delta R.T.: -0.008 min
Response: 3953637
Conc: 8.37 ng/ml

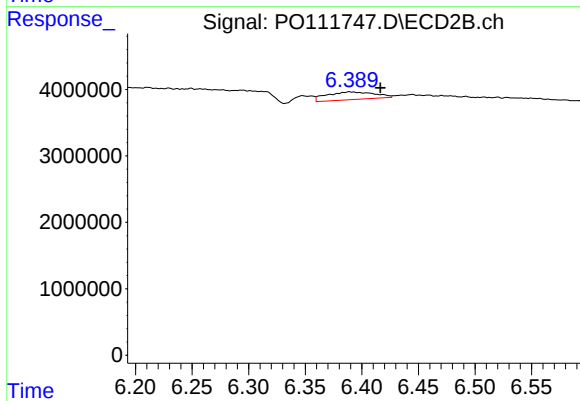

#32 AR-1260-2


R.T.: 6.389 min
Delta R.T.: -0.027 min
Response: 3418725
Conc: 11.63 ng/ml

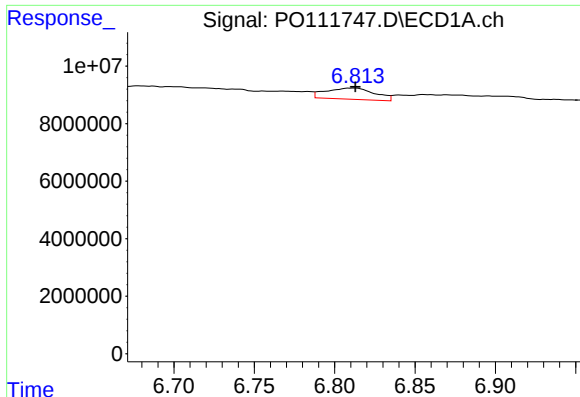

#33 AR-1260-3


R.T.: 6.813 min
Delta R.T.: 0.000 min
Response: 8229490
Conc: 19.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

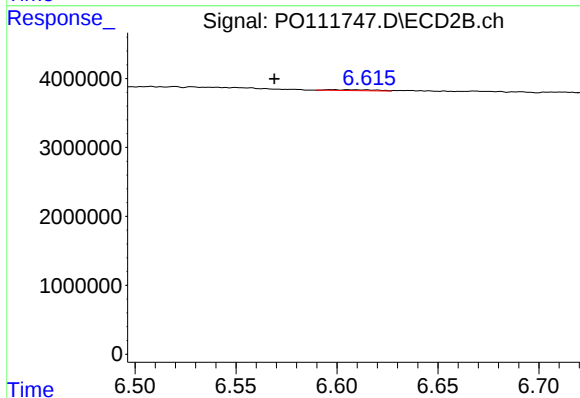


#33 AR-1260-3

R.T.: 6.598 min
Delta R.T.: 0.029 min
Response: 220327
Conc: 0.82 ng/ml

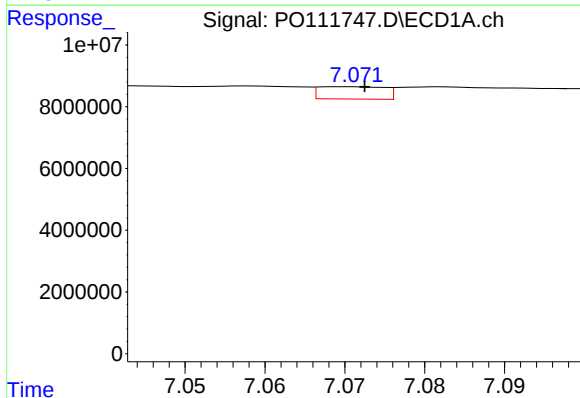


#34 AR-1260-4

R.T.: 7.070 min
Delta R.T.: -0.003 min
Response: 2286864
Conc: 7.27 ng/ml

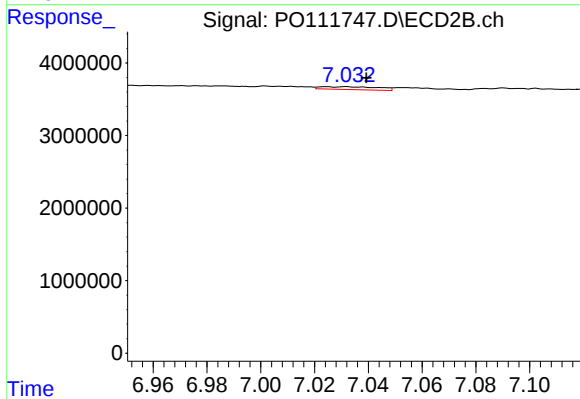

#34 AR-1260-4


R.T.: 7.032 min
Delta R.T.: -0.008 min
Response: 582390
Conc: 3.06 ng/ml

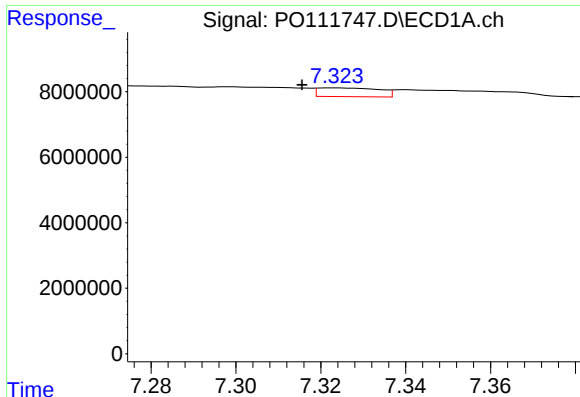

#35 AR-1260-5


R.T.: 7.324 min
Delta R.T.: 0.008 min
Response: 2673075
Conc: 3.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

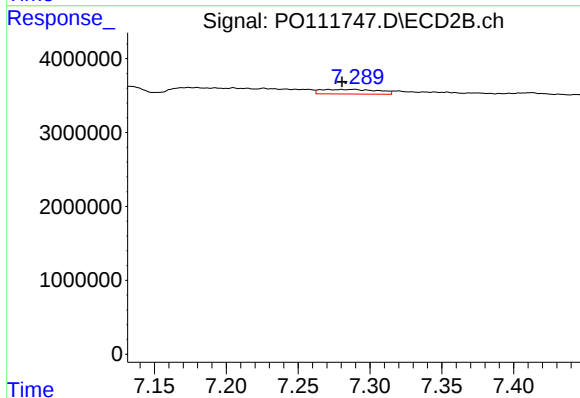


#35 AR-1260-5

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 1697385
Conc: 3.99 ng/ml

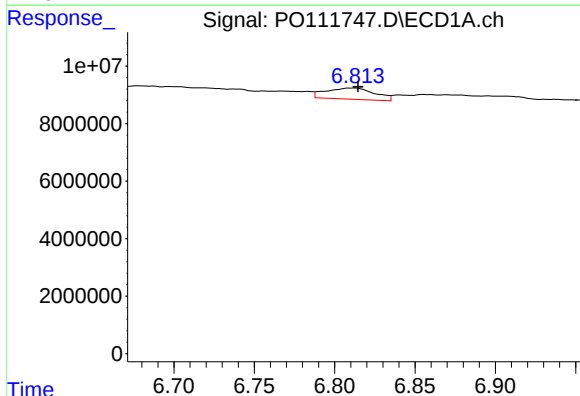


#36 AR-1262-1

R.T.: 6.813 min
Delta R.T.: -0.002 min
Response: 8229490
Conc: 13.49 ng/ml

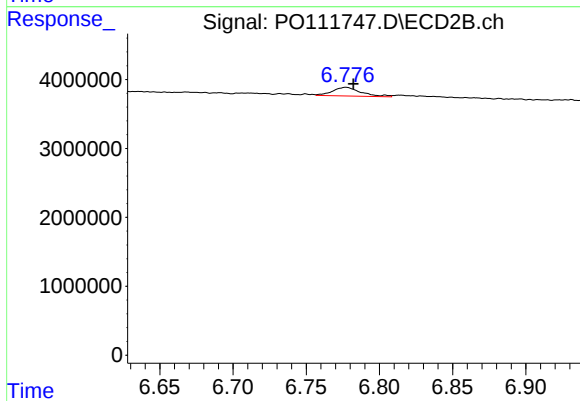

#36 AR-1262-1


R.T.: 6.777 min
Delta R.T.: -0.005 min
Response: 1692068
Conc: 5.01 ng/ml

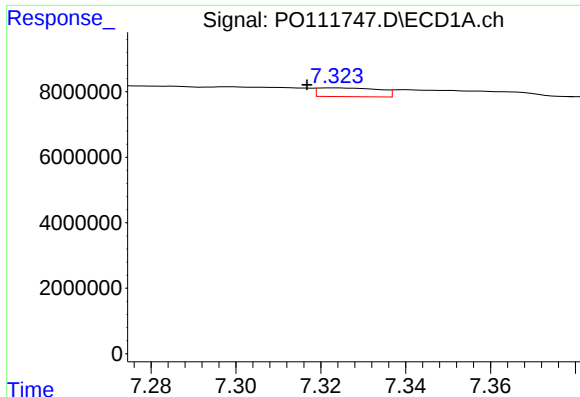

#37 AR-1262-2


R.T.: 7.324 min
Delta R.T.: 0.007 min
Response: 2673075
Conc: 2.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

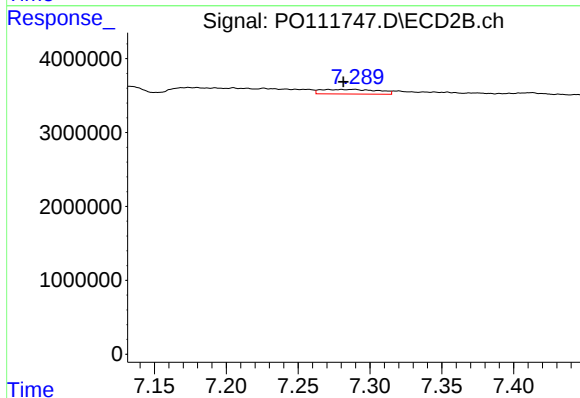


#37 AR-1262-2

R.T.: 7.280 min
Delta R.T.: -0.001 min
Response: 1697385
Conc: 3.64 ng/ml

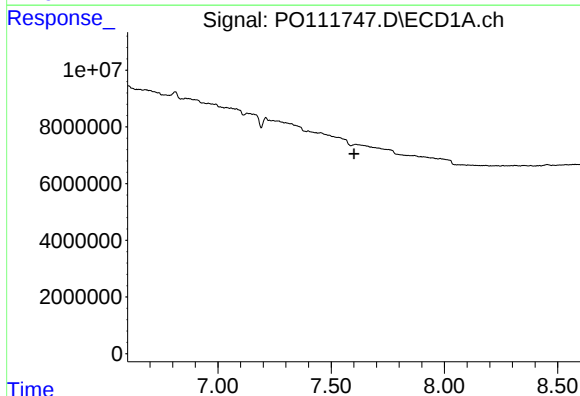


#38 AR-1262-3

R.T.: 7.609 min
Delta R.T.: 0.008 min
Response: -683577
Conc: N.D.

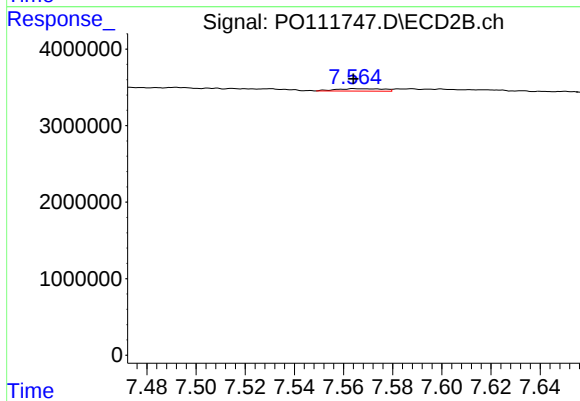

#38 AR-1262-3


R.T.: 7.565 min
Delta R.T.: 0.000 min
Response: 423182
Conc: 2.54 ng/ml

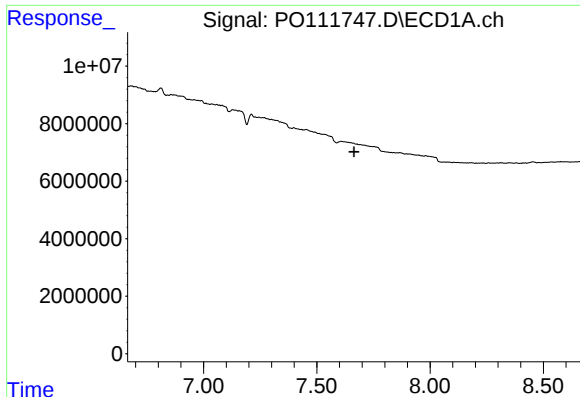

#39 AR-1262-4


R.T.: 7.609 min
Delta R.T.: -0.055 min
Response: -683577
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

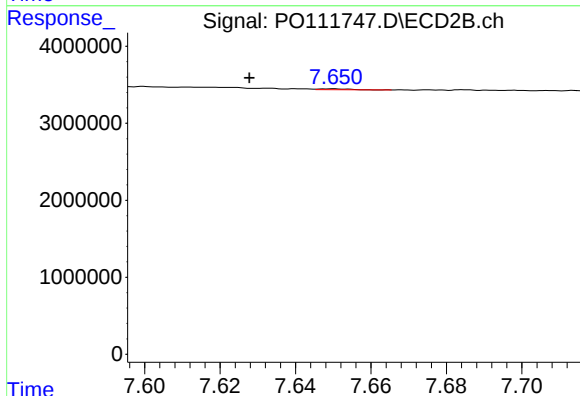


#39 AR-1262-4

R.T.: 7.650 min
Delta R.T.: 0.022 min
Response: 43335
Conc: 0.16 ng/ml

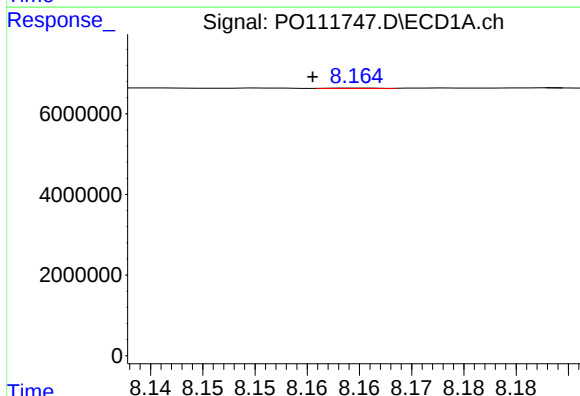


#40 AR-1262-5

R.T.: 8.165 min
Delta R.T.: 0.004 min
Response: 38189
Conc: 0.13 ng/ml

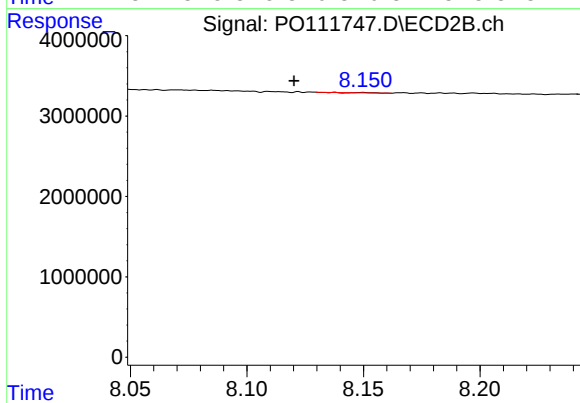

#40 AR-1262-5


R.T.: 8.150 min
Delta R.T.: 0.030 min
Response: 27619
Conc: 0.27 ng/ml

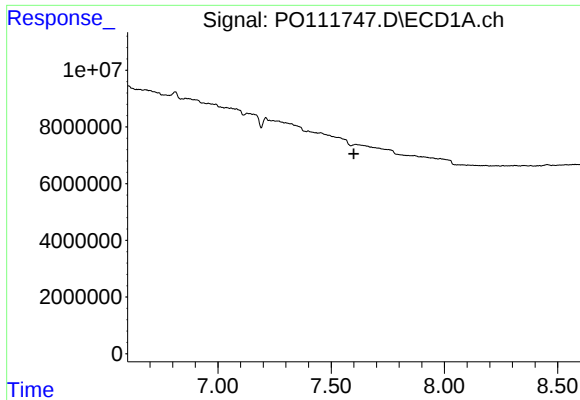

#41 AR-1268-1


R.T.: 7.609 min
Delta R.T.: 0.009 min
Response: -683577
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

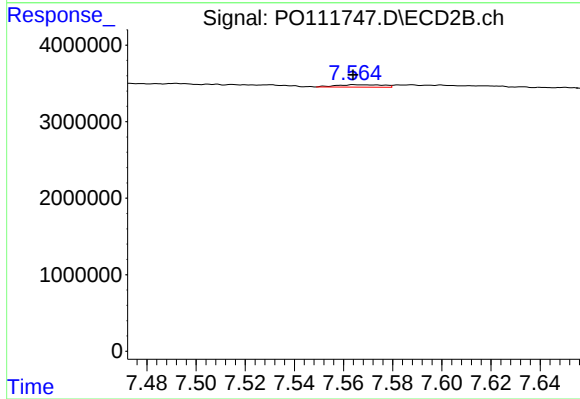


#41 AR-1268-1

R.T.: 7.565 min
Delta R.T.: 0.000 min
Response: 423182
Conc: 0.88 ng/ml

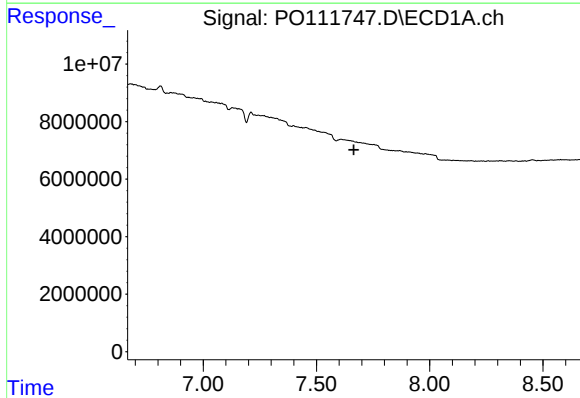


#42 AR-1268-2

R.T.: 7.609 min
Delta R.T.: -0.056 min
Response: -683577
Conc: N.D.

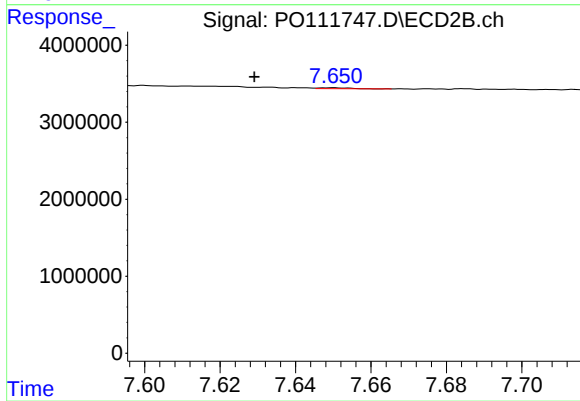

#42 AR-1268-2


R.T.: 7.650 min
Delta R.T.: 0.021 min
Response: 43335
Conc: 0.10 ng/ml

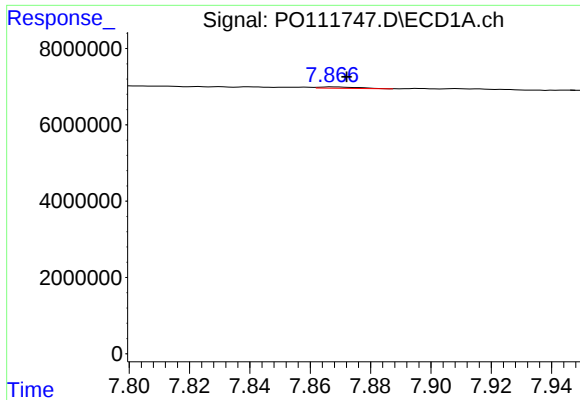

#43 AR-1268-3


R.T.: 7.868 min
Delta R.T.: -0.005 min
Response: 304682
Conc: 0.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

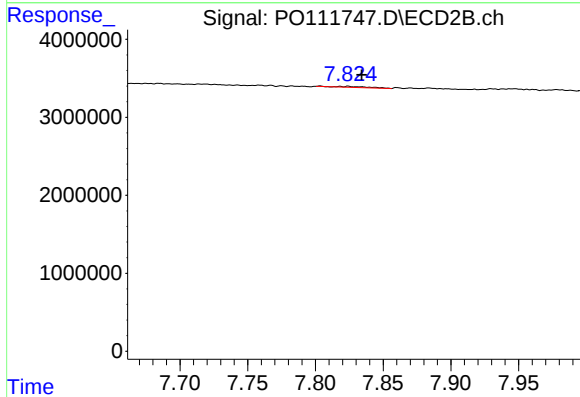


#43 AR-1268-3

R.T.: 7.824 min
Delta R.T.: -0.010 min
Response: 182870
Conc: 0.58 ng/ml

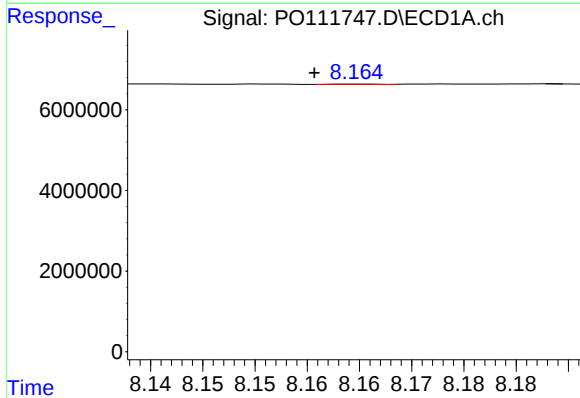


#44 AR-1268-4

R.T.: 8.165 min
Delta R.T.: 0.004 min
Response: 38189
Conc: 0.11 ng/ml

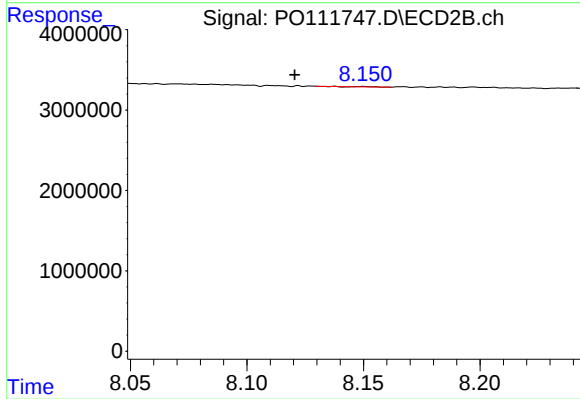

#44 AR-1268-4


R.T.: 8.150 min
Delta R.T.: 0.029 min
Response: 27619
Conc: 0.24 ng/ml

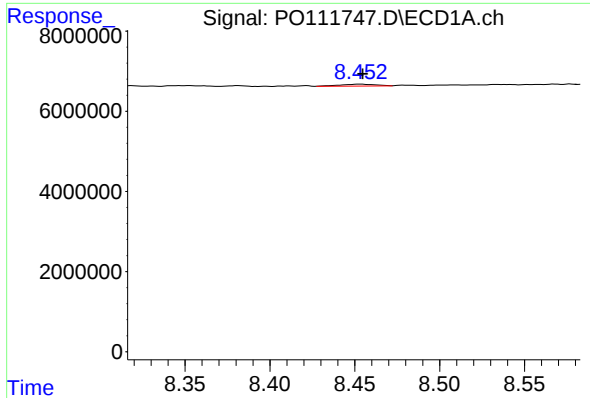

#45 AR-1268-5

R.T.: 8.453 min
Delta R.T.: -0.002 min
Response: 670743
Conc: 0.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

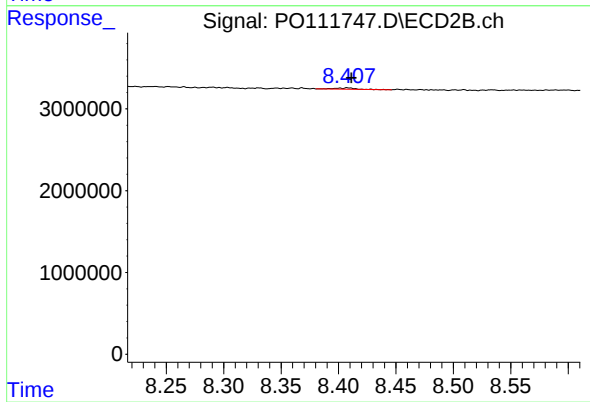

#45 AR-1268-5

R.T.: 8.408 min
Delta R.T.: -0.003 min
Response: 210383
Conc: 0.29 ng/ml