

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
 Data File : P0111757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 14:33
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:04:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.677	3.673	130.1E6	113.4E6	22.583	20.181
2)	SA Decachlor...	8.713	8.660	113.5E6	39037213	21.624	21.960
Target Compounds							
3)	L1 AR-1016-1	4.767	4.748	1201452	1516745	5.036	7.708 #
4)	L1 AR-1016-2	4.784	4.768	1610217	1752274	4.839	6.151 #
5)	L1 AR-1016-3	4.846	4.945	1897518	776994	8.245	5.172 #
6)	L1 AR-1016-4	4.962	4.984	1337351	632972	7.211	5.197 #
7)	L1 AR-1016-5	5.214	5.200	662960	243836	3.552	1.532 #
8)	L2 AR-1221-1	3.889	3.882	3297460	2690456	37.868	36.029
9)	L2 AR-1221-2	3.977	3.970	4593875	3578323	71.592	63.957
10)	L2 AR-1221-3	4.051	4.043	6871016	6356741	35.229	36.994
11)	L3 AR-1232-1	4.051	4.043	6871016	6356741	45.279	47.799
12)	L3 AR-1232-2	4.546	4.768	1129882	1752274	13.104	13.296
13)	L3 AR-1232-3	4.784	4.945	1610217	776994	9.886	11.242
14)	L3 AR-1232-4	4.962	5.026	1337351	513385	15.368	8.488 #
15)	L3 AR-1232-5	5.005	5.200	1712806	243836	30.272	3.671 #
16)	L4 AR-1242-1	4.767	4.748	1201452	1516745	5.964	9.319 #
17)	L4 AR-1242-2	4.784	4.768	1610217	1752274	5.715	7.423 #
18)	L4 AR-1242-3	4.846	4.945	1897518	776994	9.544	6.187 #
19)	L4 AR-1242-4	4.962	5.026	1337351	513385	8.454	4.189 #
20)	L4 AR-1242-5	5.643	5.547	6735370	506317	40.279	3.378 #
21)	L5 AR-1248-1	4.767	4.748	1201452	1516745	7.450	11.380 #
22)	L5 AR-1248-2	5.005	4.984	1712806	632972	7.944	3.553 #
23)	L5 AR-1248-3	5.214	5.026	662960	513385	2.458	2.710
24)	L5 AR-1248-4	5.574	5.200	3650470	243836	9.131	1.068 #
25)	L5 AR-1248-5	5.643	5.589	6735370	924115	23.985	4.244 #
26)	L6 AR-1254-1	5.574	5.547	3650470	506317	8.588	1.568 #
27)	L6 AR-1254-2	5.719	5.699	1079109	483489	2.843	1.731 #
28)	L6 AR-1254-3	6.132	6.100	4331293	1214334	7.581	2.898 #
29)	L6 AR-1254-4	6.329	6.301	16801778	3601291	48.159	15.809 #
30)	L6 AR-1254-5	6.783	6.743	1712024	104772	3.343	0.322 #
31)	L7 AR-1260-1	6.251	6.226	8582002	1355598	24.153	5.403 #
32)	L7 AR-1260-2	6.443	6.423	3736527	263704	7.908	0.897 #
33)	L7 AR-1260-3	6.809	6.558	9094300	82525	21.415	0.309 #
34)	L7 AR-1260-4	7.073	7.044	4427603	156772	14.081	0.825 #
35)	L7 AR-1260-5	7.334	7.279	2016415	377976	2.448	0.889 #
36)	L8 AR-1262-1	6.809	6.777	9094300	1459699	14.912	4.323 #
37)	L8 AR-1262-2	7.334	7.279	2016415	377976	2.142	0.811 #
38)	L8 AR-1262-3	7.598	7.561	694438	128260	1.751	0.771 #
39)	L8 AR-1262-4	7.623f	7.624	7095364	91049	10.800	0.329 #
40)	L8 AR-1262-5	8.162	8.117	525708	35508	1.726	0.349 #
41)	L9 AR-1268-1	7.598	7.561	694438	128260	0.616	0.268 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
Data File : P0111757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 14:33
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:04:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.623f	7.624	7095364	91049	7.261	0.219 #
43)	L9 AR-1268-3	7.903	7.835	14738	104135	0.018	0.329 #
44)	L9 AR-1268-4	8.162	8.117	525708	35508	1.528	0.307 #
45)	L9 AR-1268-5	8.454	8.411	405619	138631	0.183	0.191


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

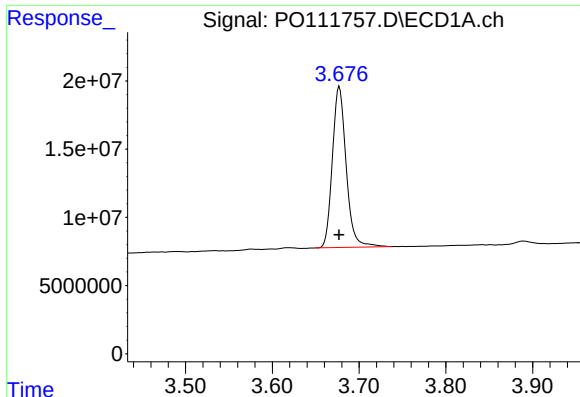

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 130066821
Conc: 22.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

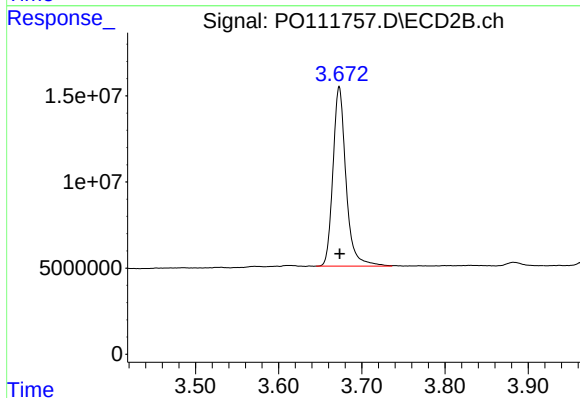


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 113364054
Conc: 20.18 ng/ml

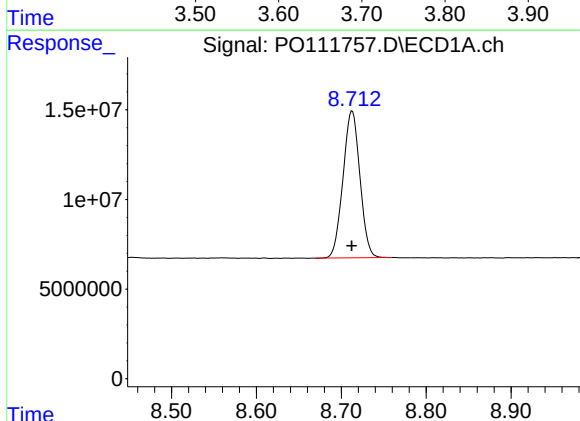


#2 Decachlorobiphenyl

R.T.: 8.713 min
Delta R.T.: 0.000 min
Response: 113512282
Conc: 21.62 ng/ml

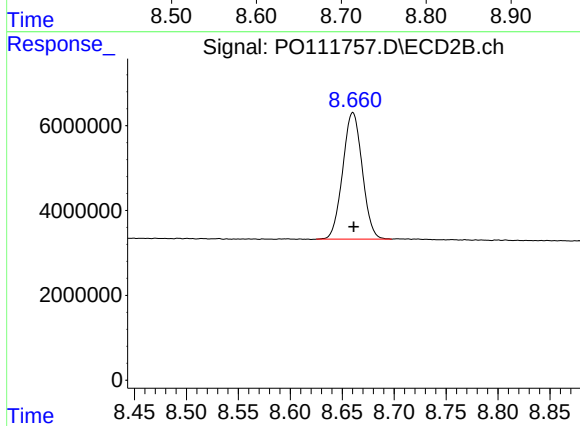

#2 Decachlorobiphenyl


R.T.: 8.660 min
Delta R.T.: 0.000 min
Response: 39037213
Conc: 21.96 ng/ml

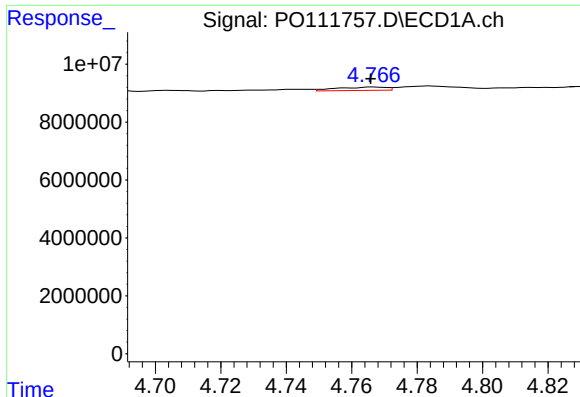

#3 AR-1016-1


R.T.: 4.767 min
Delta R.T.: 0.000 min
Response: 1201452
Conc: 5.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

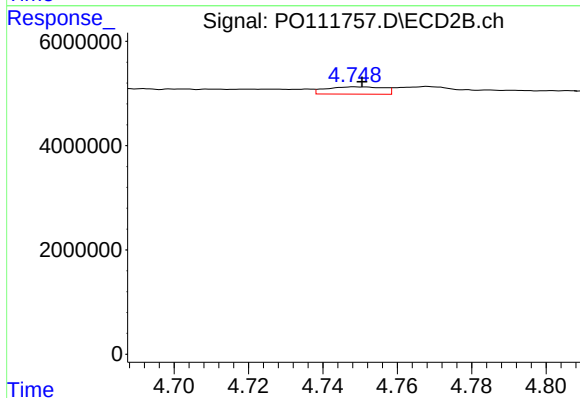


#3 AR-1016-1

R.T.: 4.748 min
Delta R.T.: -0.002 min
Response: 1516745
Conc: 7.71 ng/ml

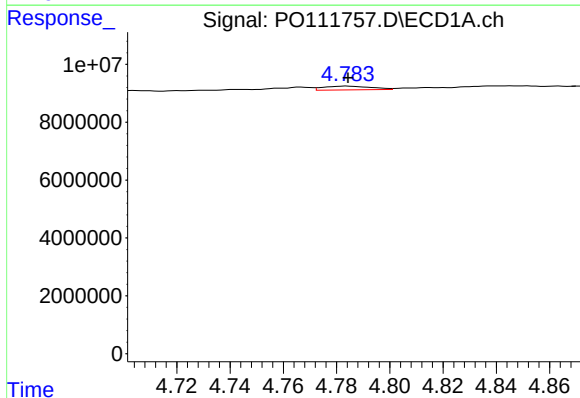


#4 AR-1016-2

R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 1610217
Conc: 4.84 ng/ml

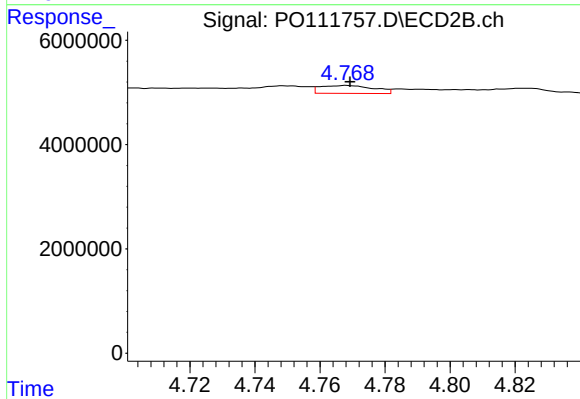

#4 AR-1016-2


R.T.: 4.768 min
Delta R.T.: -0.001 min
Response: 1752274
Conc: 6.15 ng/ml

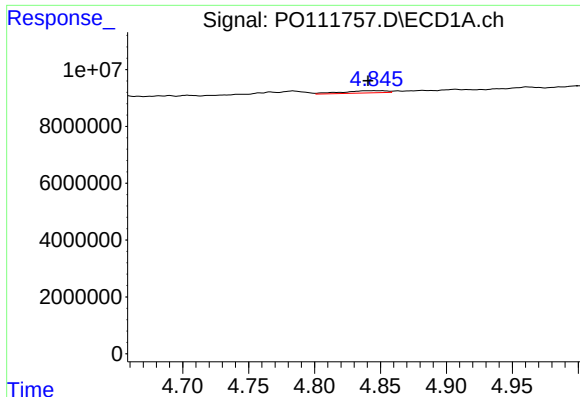

#5 AR-1016-3


R.T.: 4.846 min
Delta R.T.: 0.005 min
Response: 1897518
Conc: 8.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

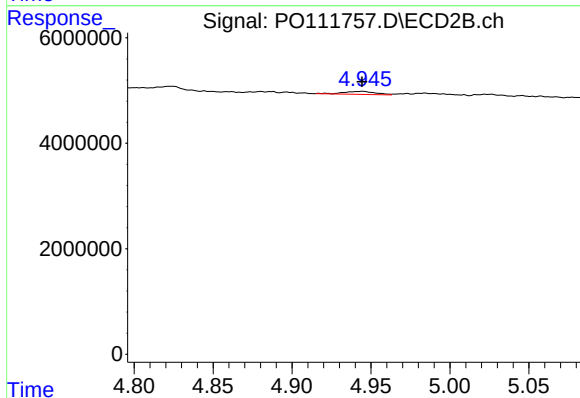


#5 AR-1016-3

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 776994
Conc: 5.17 ng/ml

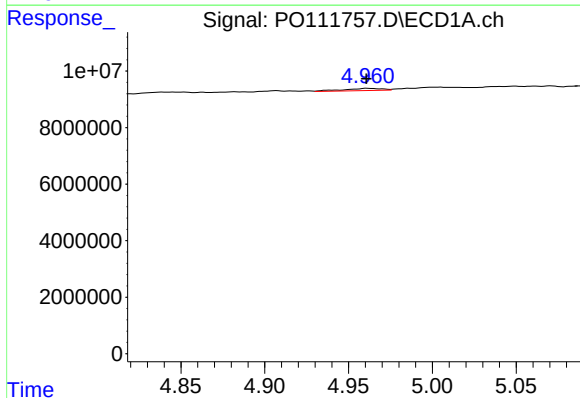


#6 AR-1016-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 1337351
Conc: 7.21 ng/ml

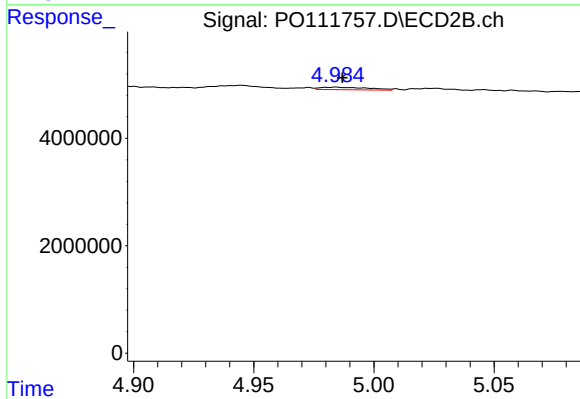

#6 AR-1016-4


R.T.: 4.984 min
Delta R.T.: -0.003 min
Response: 632972
Conc: 5.20 ng/ml

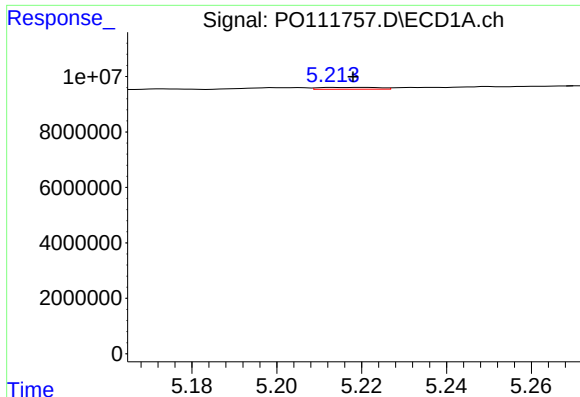

#7 AR-1016-5


R.T.: 5.214 min
Delta R.T.: -0.004 min
Response: 662960
Conc: 3.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

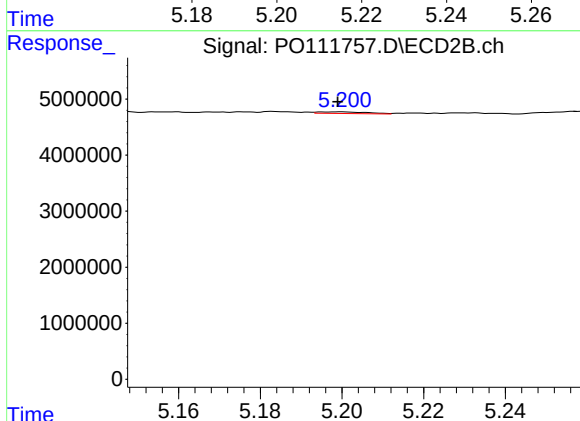


#7 AR-1016-5

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 243836
Conc: 1.53 ng/ml

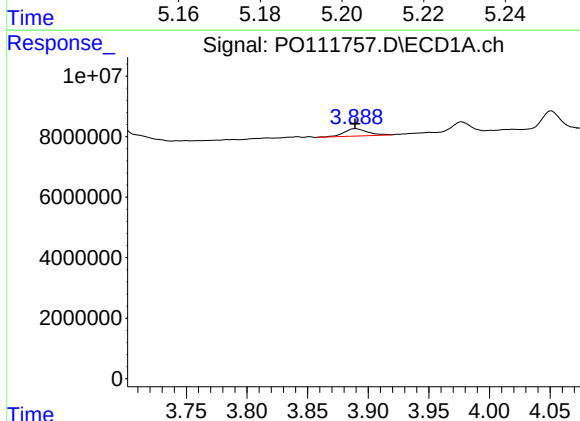


#8 AR-1221-1

R.T.: 3.889 min
Delta R.T.: 0.000 min
Response: 3297460
Conc: 37.87 ng/ml

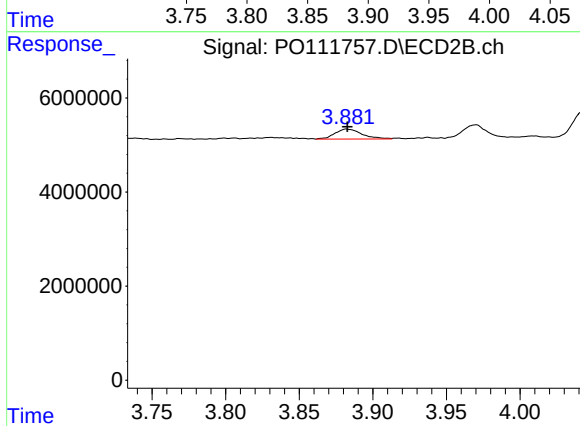

#8 AR-1221-1


R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 2690456
Conc: 36.03 ng/ml

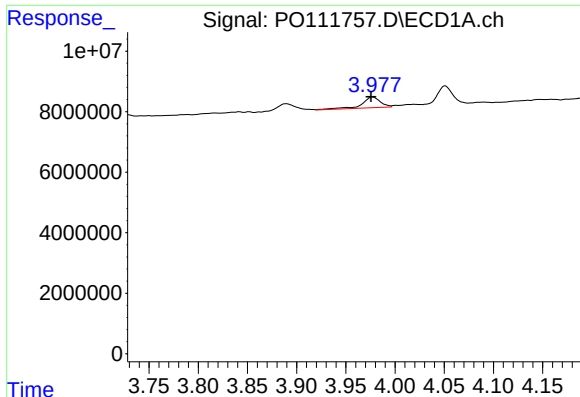

#9 AR-1221-2


R.T.: 3.977 min
Delta R.T.: 0.002 min
Response: 4593875
Conc: 71.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

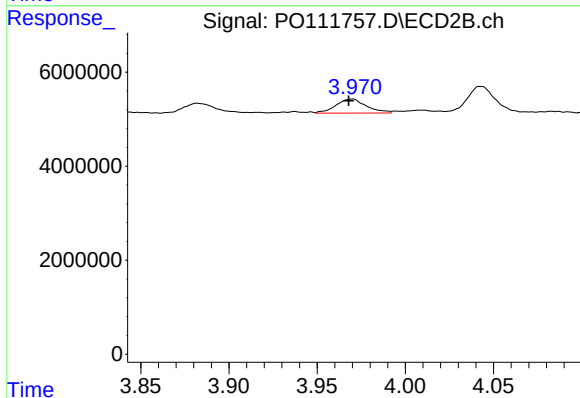


#9 AR-1221-2

R.T.: 3.970 min
Delta R.T.: 0.002 min
Response: 3578323
Conc: 63.96 ng/ml

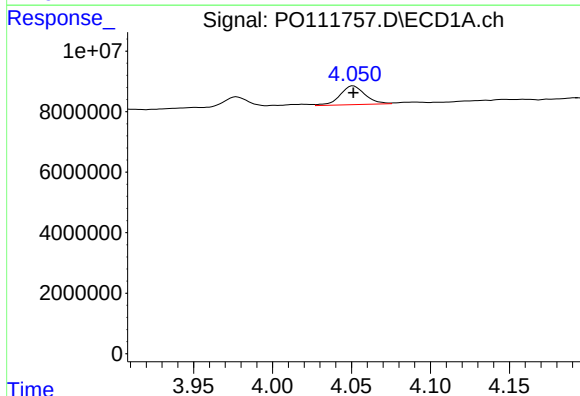


#10 AR-1221-3

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 6871016
Conc: 35.23 ng/ml

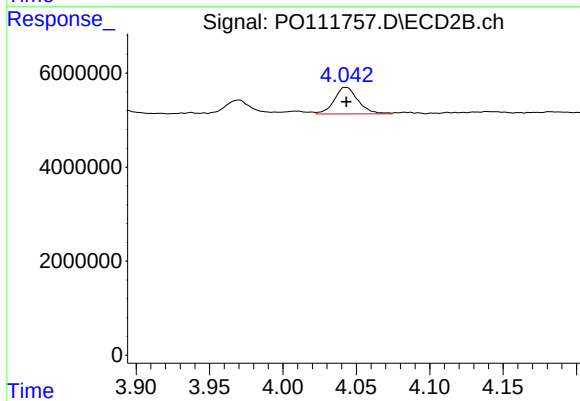

#10 AR-1221-3


R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 6356741
Conc: 36.99 ng/ml

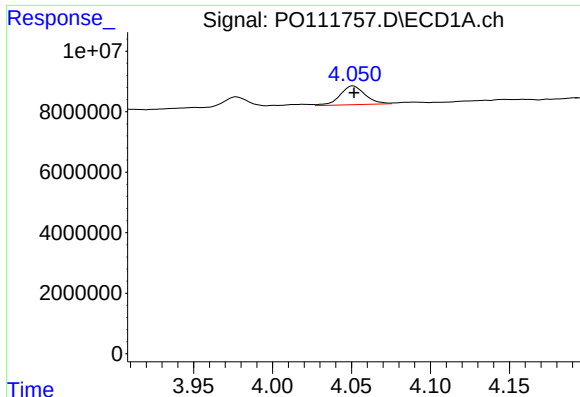

#11 AR-1232-1


R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 6871016
Conc: 45.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

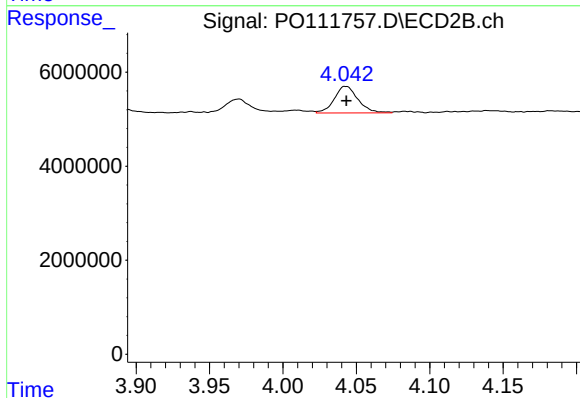


#11 AR-1232-1

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 6356741
Conc: 47.80 ng/ml

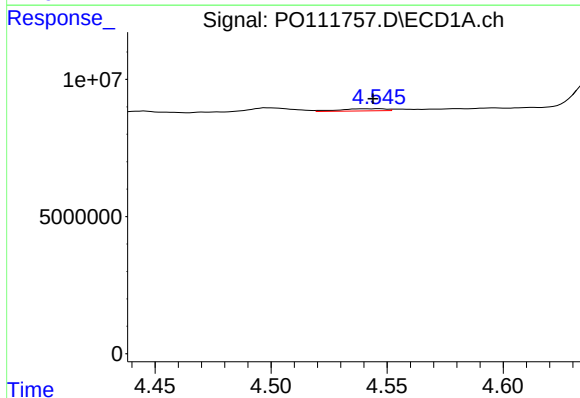


#12 AR-1232-2

R.T.: 4.546 min
Delta R.T.: 0.002 min
Response: 1129882
Conc: 13.10 ng/ml

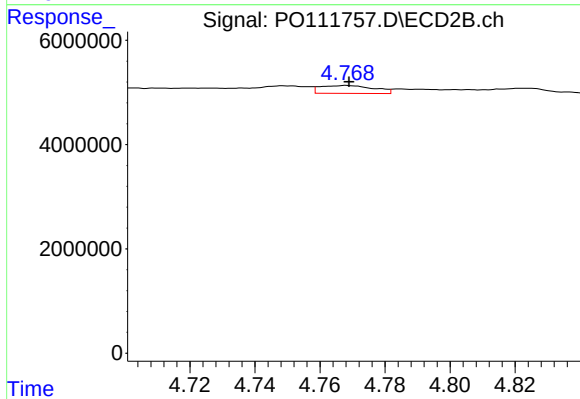

#12 AR-1232-2


R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 1752274
Conc: 13.30 ng/ml

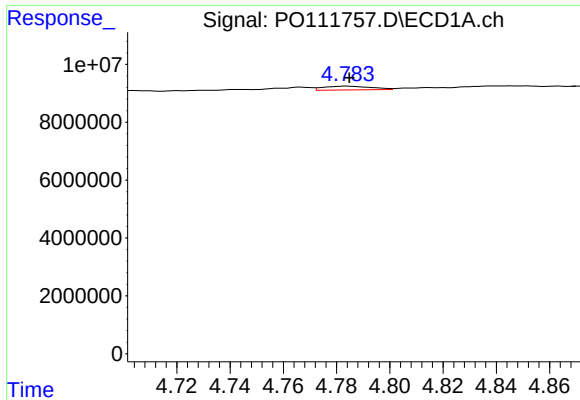

#13 AR-1232-3


R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 1610217
Conc: 9.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

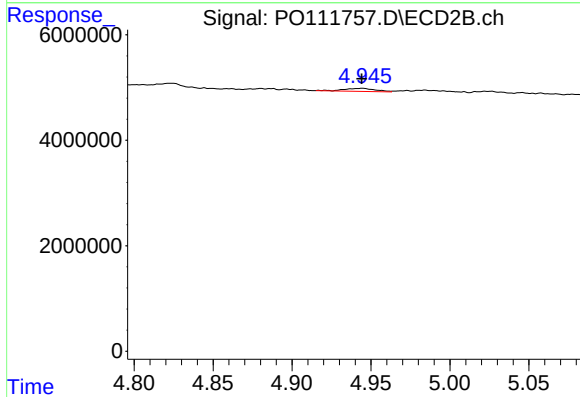


#13 AR-1232-3

R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 776994
Conc: 11.24 ng/ml

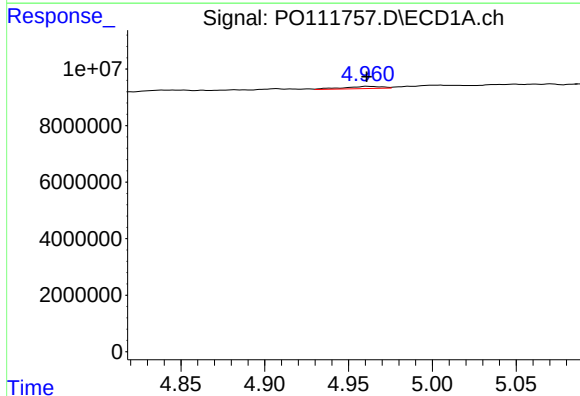


#14 AR-1232-4

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 1337351
Conc: 15.37 ng/ml

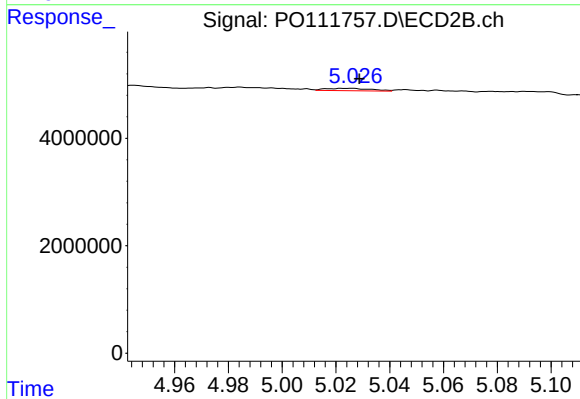

#14 AR-1232-4


R.T.: 5.026 min
Delta R.T.: -0.002 min
Response: 513385
Conc: 8.49 ng/ml

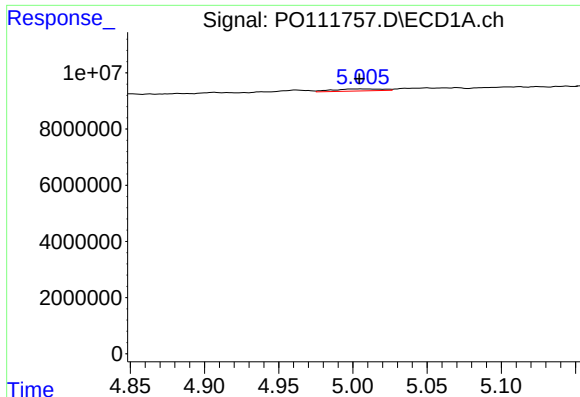

#15 AR-1232-5


R.T.: 5.005 min
Delta R.T.: 0.001 min
Response: 1712806
Conc: 30.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

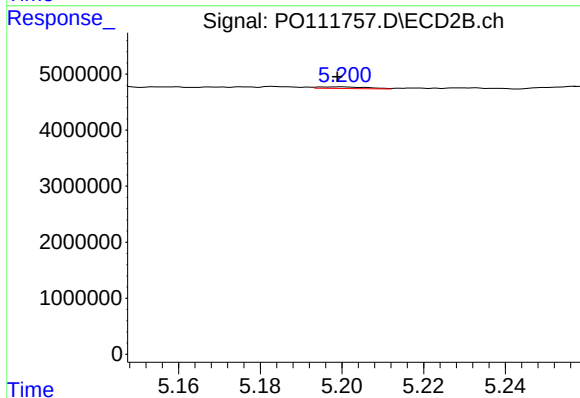


#15 AR-1232-5

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 243836
Conc: 3.67 ng/ml

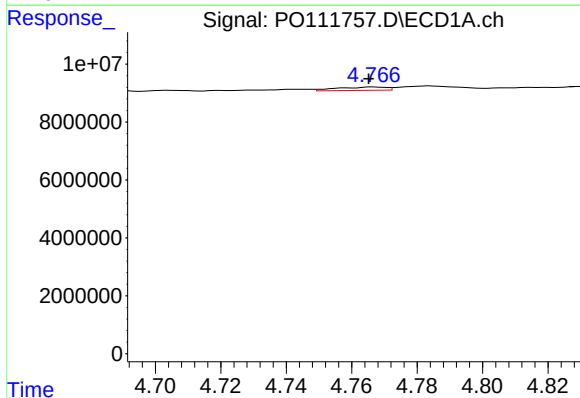


#16 AR-1242-1

R.T.: 4.767 min
Delta R.T.: 0.002 min
Response: 1201452
Conc: 5.96 ng/ml

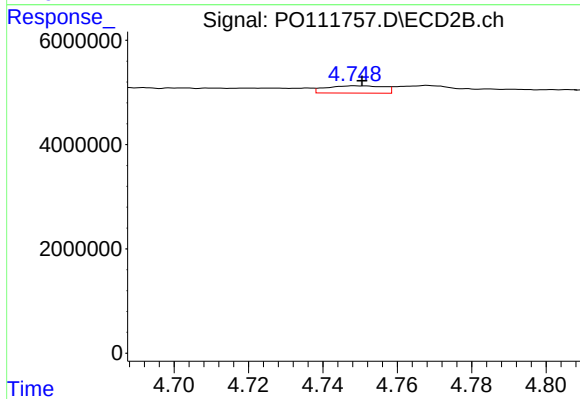

#16 AR-1242-1


R.T.: 4.748 min
Delta R.T.: -0.002 min
Response: 1516745
Conc: 9.32 ng/ml

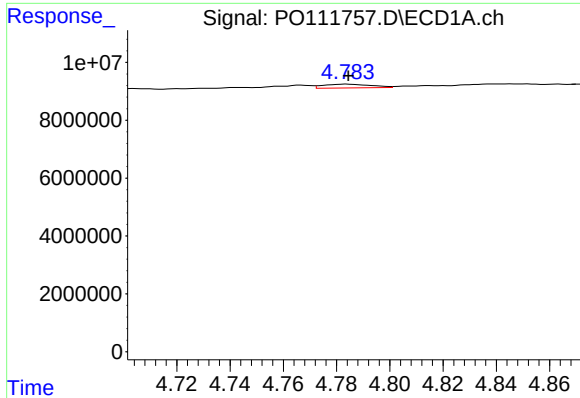

#17 AR-1242-2


R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 1610217
Conc: 5.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

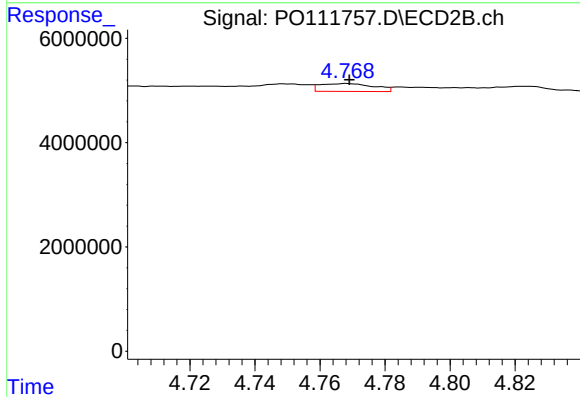


#17 AR-1242-2

R.T.: 4.768 min
Delta R.T.: 0.000 min
Response: 1752274
Conc: 7.42 ng/ml

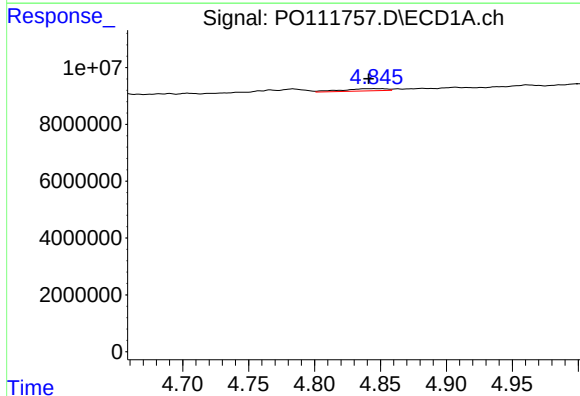


#18 AR-1242-3

R.T.: 4.846 min
Delta R.T.: 0.004 min
Response: 1897518
Conc: 9.54 ng/ml

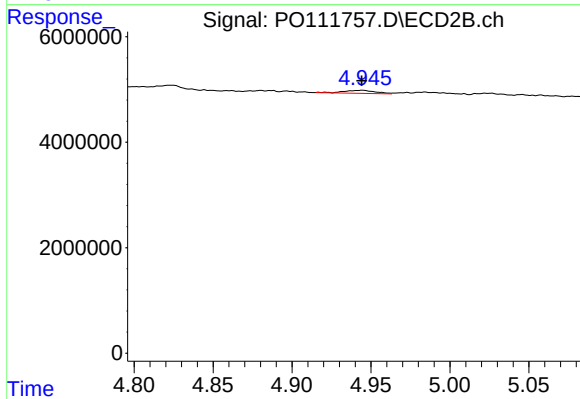

#18 AR-1242-3


R.T.: 4.945 min
Delta R.T.: 0.000 min
Response: 776994
Conc: 6.19 ng/ml

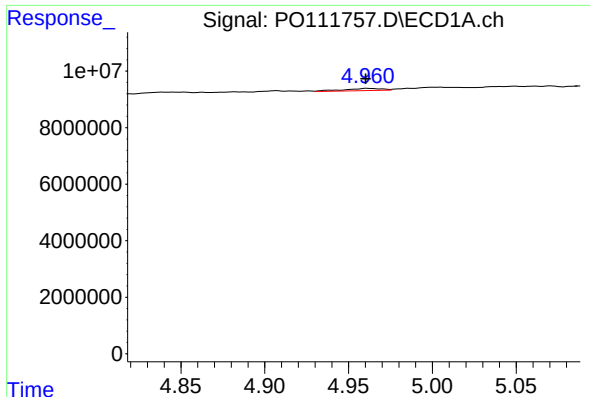

#19 AR-1242-4


R.T.: 4.962 min
Delta R.T.: 0.001 min
Response: 1337351
Conc: 8.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

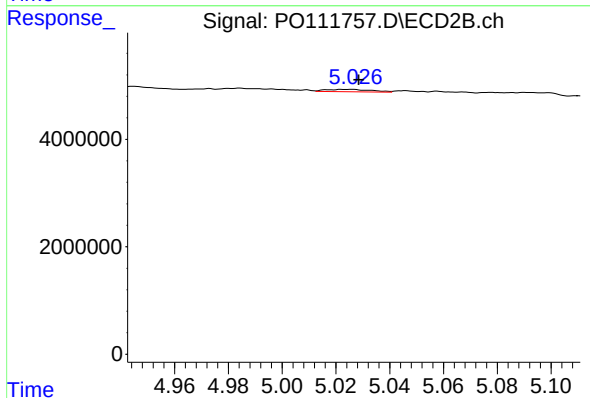


#19 AR-1242-4

R.T.: 5.026 min
Delta R.T.: -0.002 min
Response: 513385
Conc: 4.19 ng/ml

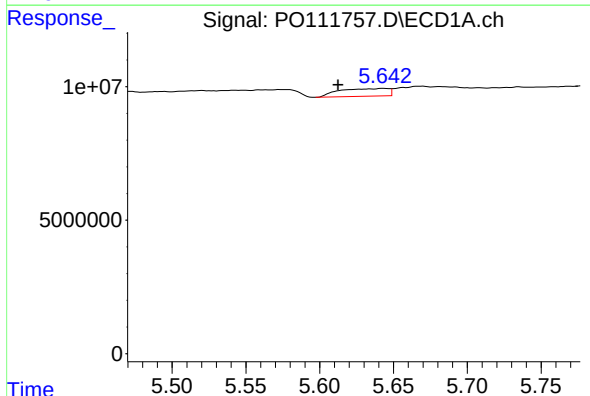


#20 AR-1242-5

R.T.: 5.643 min
Delta R.T.: 0.031 min
Response: 6735370
Conc: 40.28 ng/ml

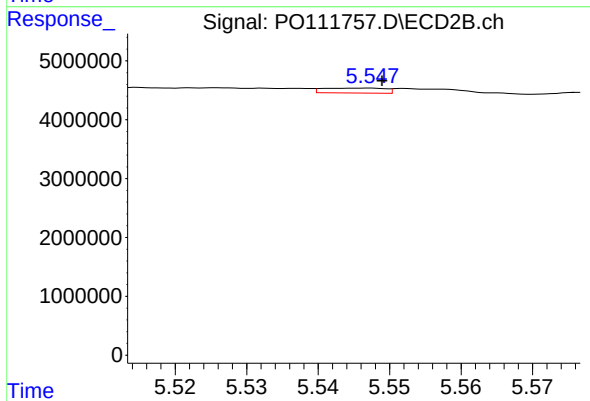

#20 AR-1242-5


R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 506317
Conc: 3.38 ng/ml

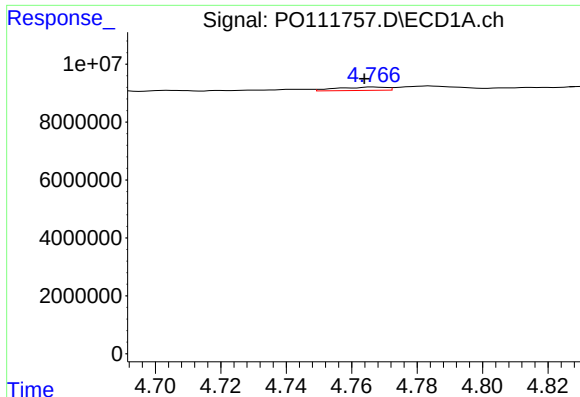

#21 AR-1248-1


R.T.: 4.767 min
Delta R.T.: 0.003 min
Response: 1201452
Conc: 7.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

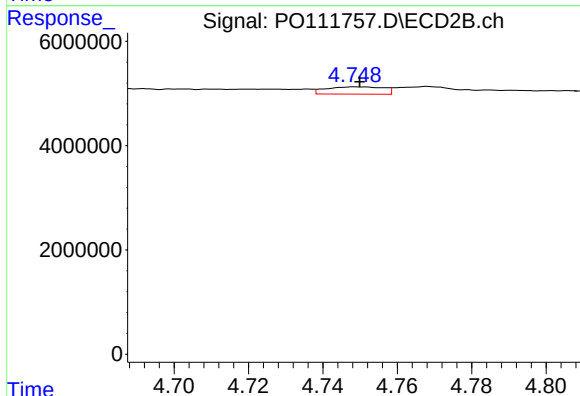


#21 AR-1248-1

R.T.: 4.748 min
Delta R.T.: -0.001 min
Response: 1516745
Conc: 11.38 ng/ml

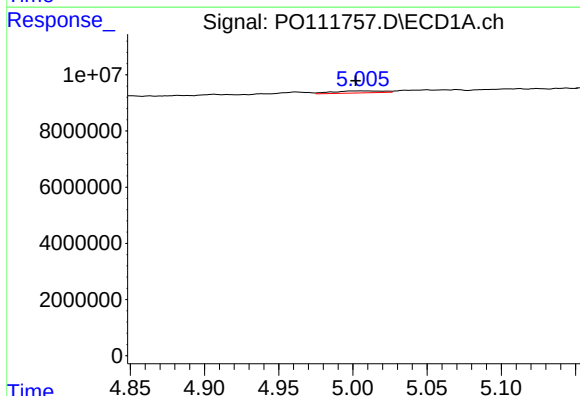


#22 AR-1248-2

R.T.: 5.005 min
Delta R.T.: 0.003 min
Response: 1712806
Conc: 7.94 ng/ml

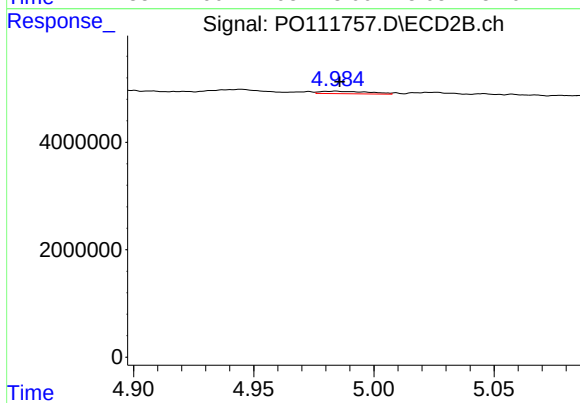

#22 AR-1248-2


R.T.: 4.984 min
Delta R.T.: -0.001 min
Response: 632972
Conc: 3.55 ng/ml

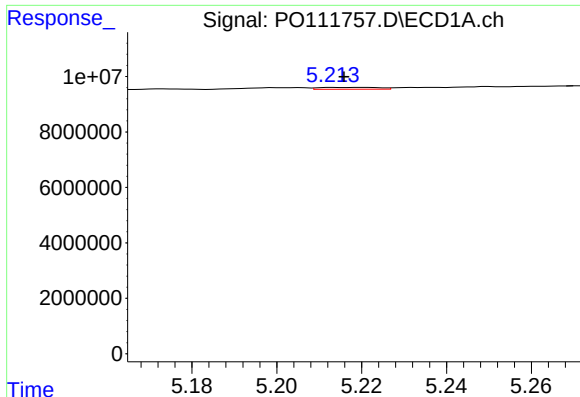

#23 AR-1248-3


R.T.: 5.214 min
Delta R.T.: -0.002 min
Response: 662960
Conc: 2.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

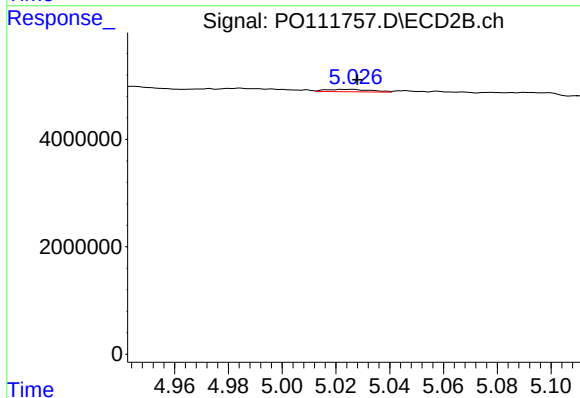


#23 AR-1248-3

R.T.: 5.026 min
Delta R.T.: -0.002 min
Response: 513385
Conc: 2.71 ng/ml

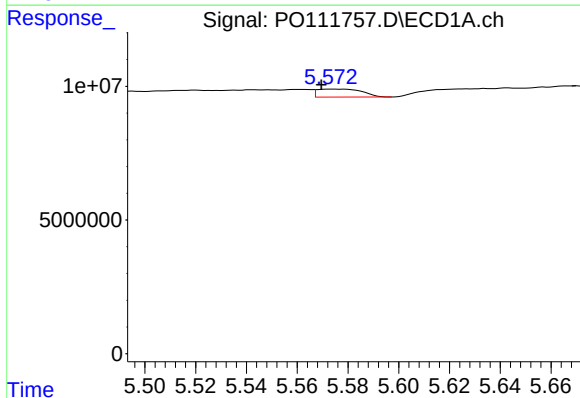


#24 AR-1248-4

R.T.: 5.574 min
Delta R.T.: 0.004 min
Response: 3650470
Conc: 9.13 ng/ml

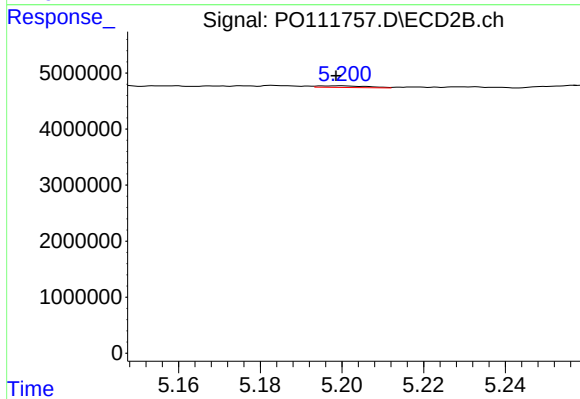

#24 AR-1248-4


R.T.: 5.200 min
Delta R.T.: 0.001 min
Response: 243836
Conc: 1.07 ng/ml

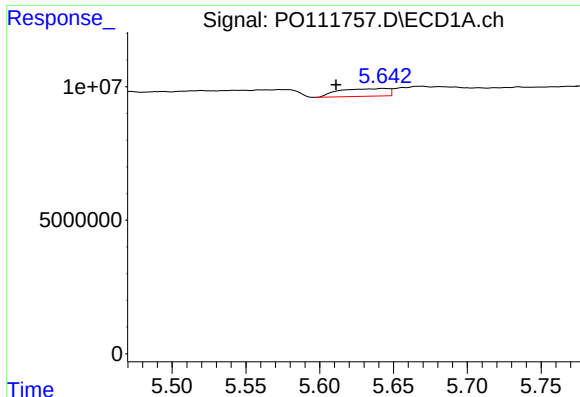

#25 AR-1248-5


R.T.: 5.643 min
Delta R.T.: 0.032 min
Response: 6735370
Conc: 23.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

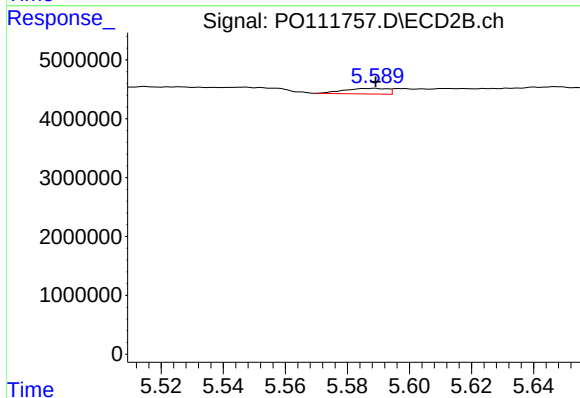


#25 AR-1248-5

R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 924115
Conc: 4.24 ng/ml

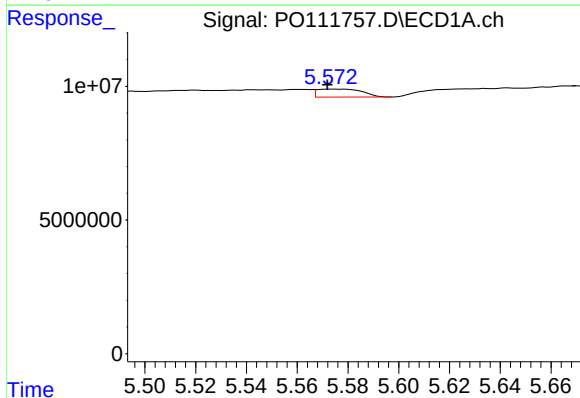


#26 AR-1254-1

R.T.: 5.574 min
Delta R.T.: 0.002 min
Response: 3650470
Conc: 8.59 ng/ml

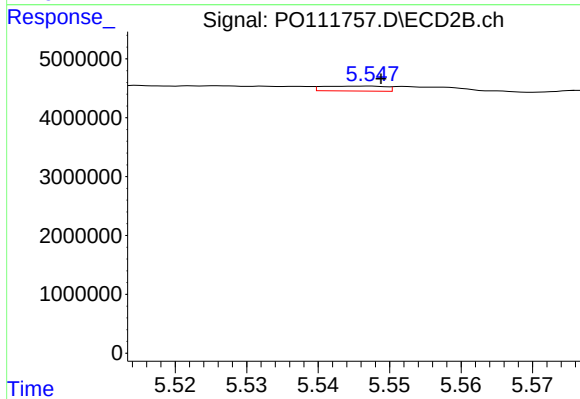

#26 AR-1254-1


R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 506317
Conc: 1.57 ng/ml

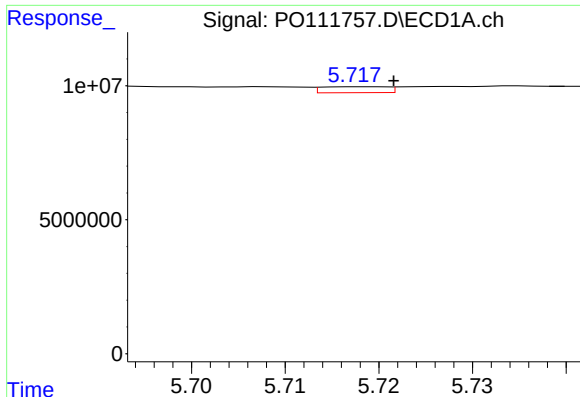

#27 AR-1254-2


R.T.: 5.719 min
Delta R.T.: -0.003 min
Response: 1079109
Conc: 2.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

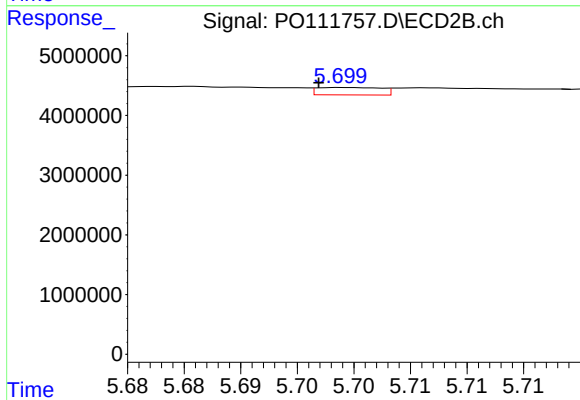


#27 AR-1254-2

R.T.: 5.699 min
Delta R.T.: 0.002 min
Response: 483489
Conc: 1.73 ng/ml

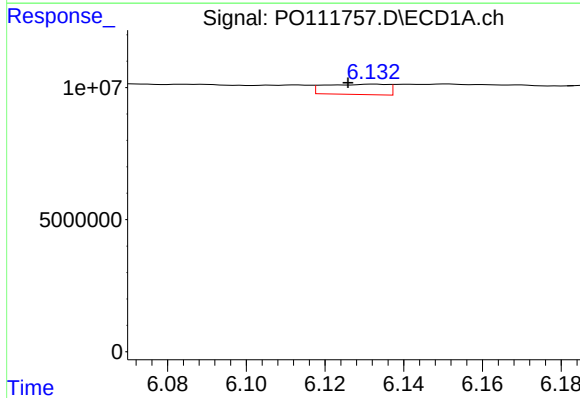


#28 AR-1254-3

R.T.: 6.132 min
Delta R.T.: 0.007 min
Response: 4331293
Conc: 7.58 ng/ml

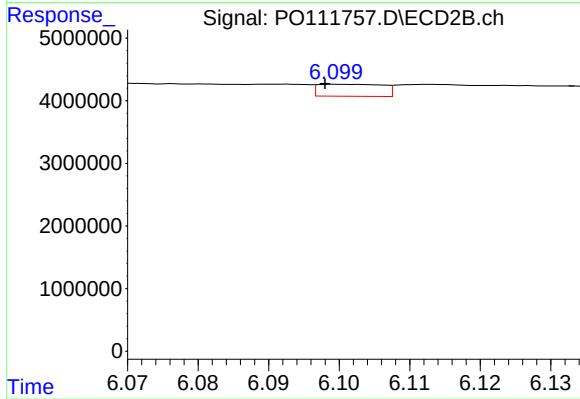

#28 AR-1254-3


R.T.: 6.100 min
Delta R.T.: 0.002 min
Response: 1214334
Conc: 2.90 ng/ml

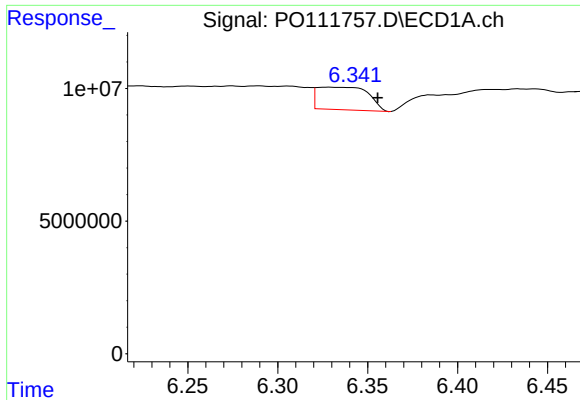

#29 AR-1254-4


R.T.: 6.329 min
Delta R.T.: -0.027 min
Response: 16801778
Conc: 48.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

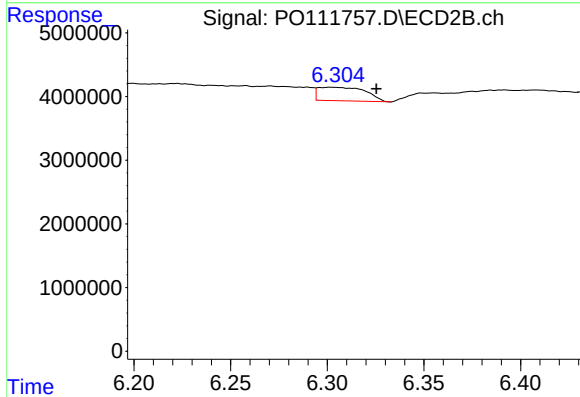


#29 AR-1254-4

R.T.: 6.301 min
Delta R.T.: -0.024 min
Response: 3601291
Conc: 15.81 ng/ml

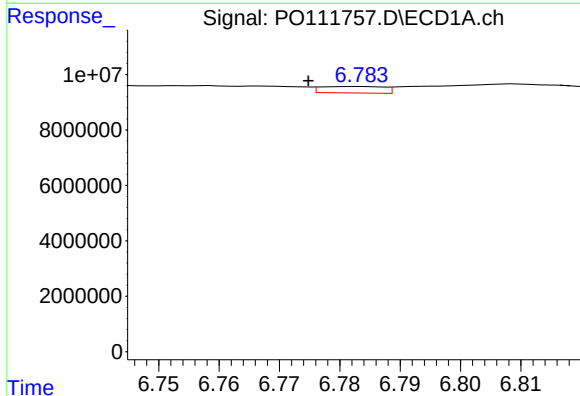


#30 AR-1254-5

R.T.: 6.783 min
Delta R.T.: 0.008 min
Response: 1712024
Conc: 3.34 ng/ml

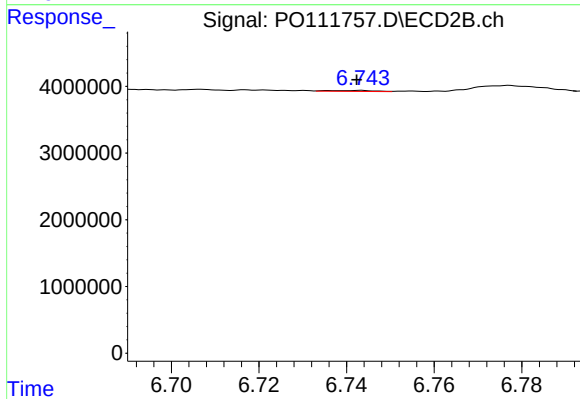

#30 AR-1254-5


R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 104772
Conc: 0.32 ng/ml

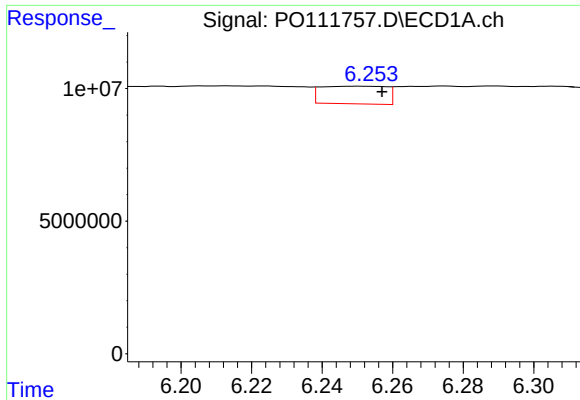

#31 AR-1260-1


R.T.: 6.251 min
Delta R.T.: -0.006 min
Response: 8582002
Conc: 24.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

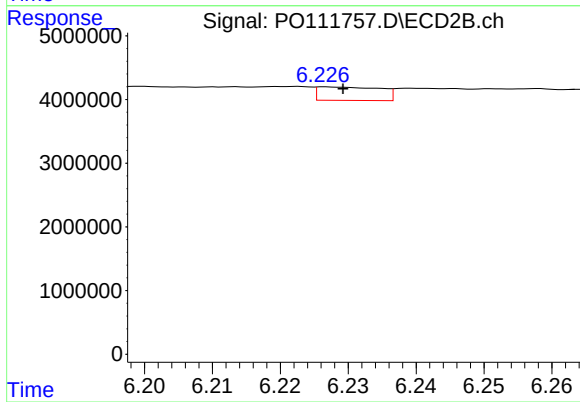


#31 AR-1260-1

R.T.: 6.226 min
Delta R.T.: -0.003 min
Response: 1355598
Conc: 5.40 ng/ml

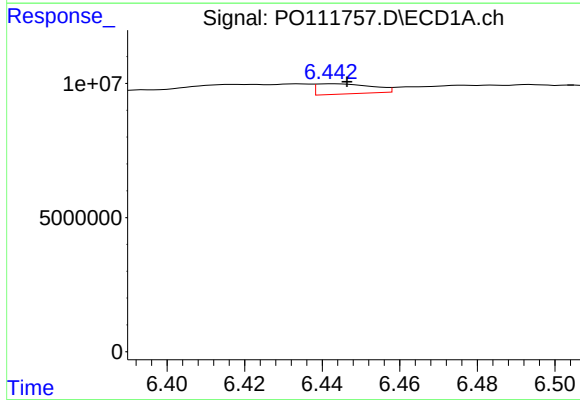


#32 AR-1260-2

R.T.: 6.443 min
Delta R.T.: -0.004 min
Response: 3736527
Conc: 7.91 ng/ml

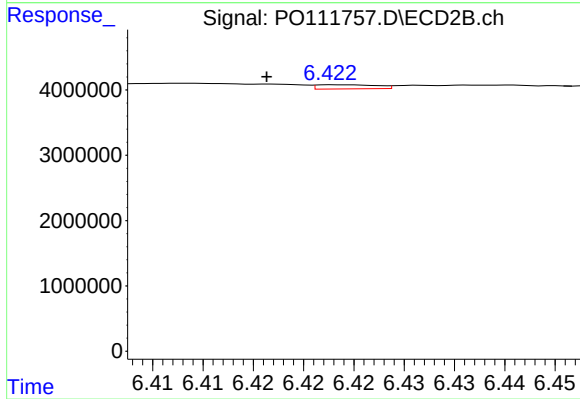

#32 AR-1260-2


R.T.: 6.423 min
Delta R.T.: 0.007 min
Response: 263704
Conc: 0.90 ng/ml

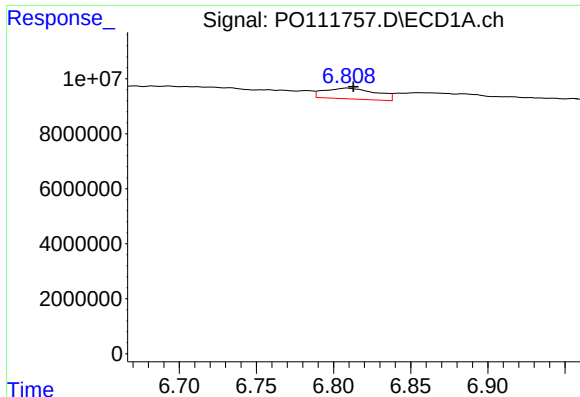

#33 AR-1260-3


R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 9094300
Conc: 21.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

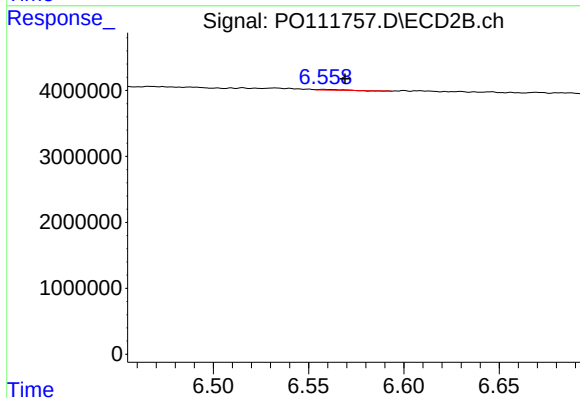


#33 AR-1260-3

R.T.: 6.558 min
Delta R.T.: -0.011 min
Response: 82525
Conc: 0.31 ng/ml

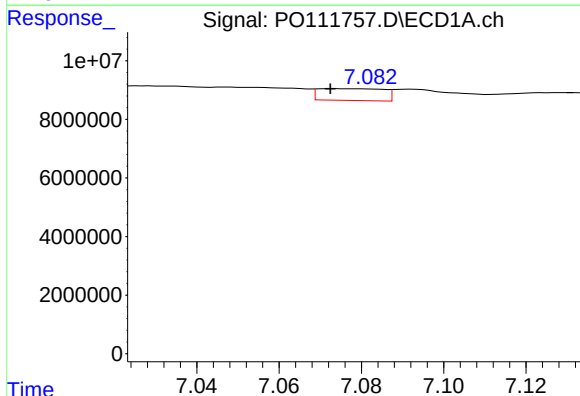


#34 AR-1260-4

R.T.: 7.073 min
Delta R.T.: 0.000 min
Response: 4427603
Conc: 14.08 ng/ml

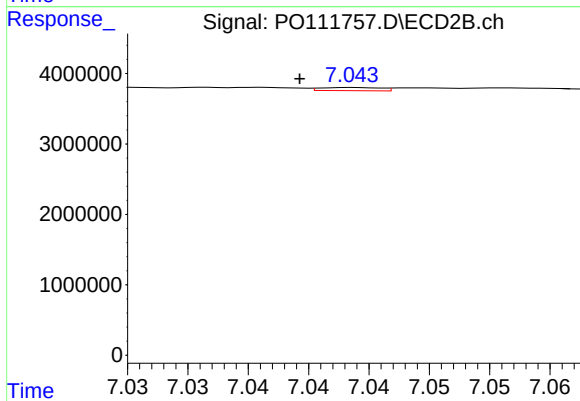

#34 AR-1260-4


R.T.: 7.044 min
Delta R.T.: 0.005 min
Response: 156772
Conc: 0.82 ng/ml

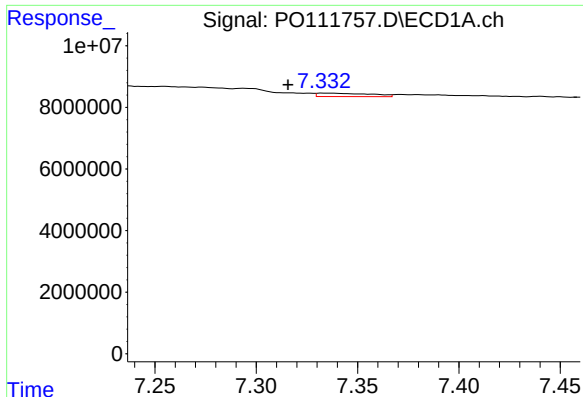

#35 AR-1260-5


R.T.: 7.334 min
Delta R.T.: 0.018 min
Response: 2016415
Conc: 2.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

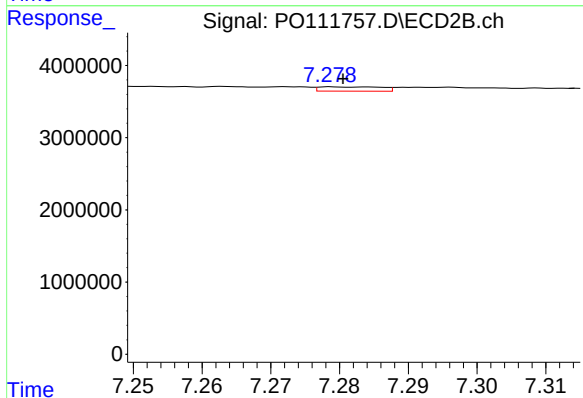


#35 AR-1260-5

R.T.: 7.279 min
Delta R.T.: -0.002 min
Response: 377976
Conc: 0.89 ng/ml

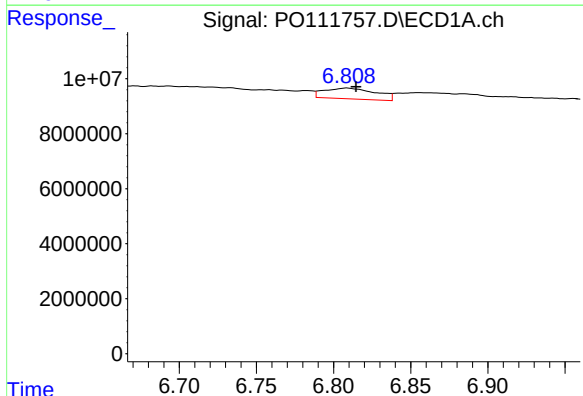


#36 AR-1262-1

R.T.: 6.809 min
Delta R.T.: -0.006 min
Response: 9094300
Conc: 14.91 ng/ml

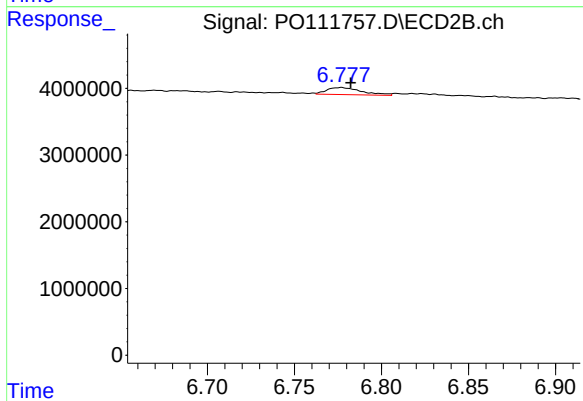

#36 AR-1262-1


R.T.: 6.777 min
Delta R.T.: -0.005 min
Response: 1459699
Conc: 4.32 ng/ml

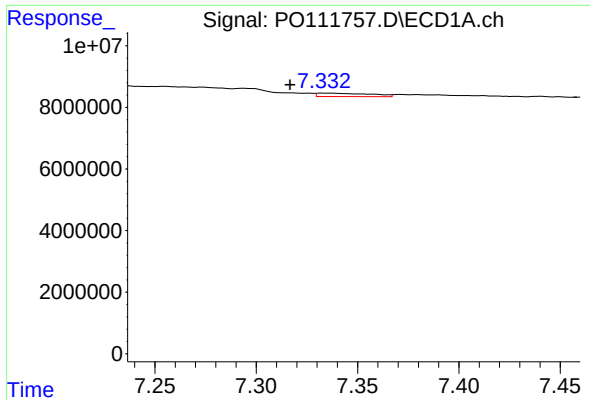

#37 AR-1262-2


R.T.: 7.334 min
Delta R.T.: 0.017 min
Response: 2016415
Conc: 2.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

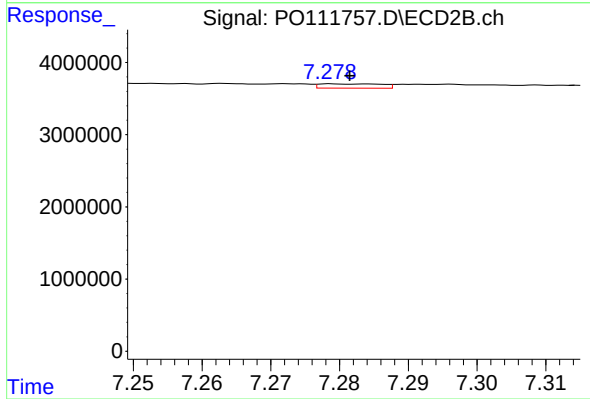


#37 AR-1262-2

R.T.: 7.279 min
Delta R.T.: -0.003 min
Response: 377976
Conc: 0.81 ng/ml

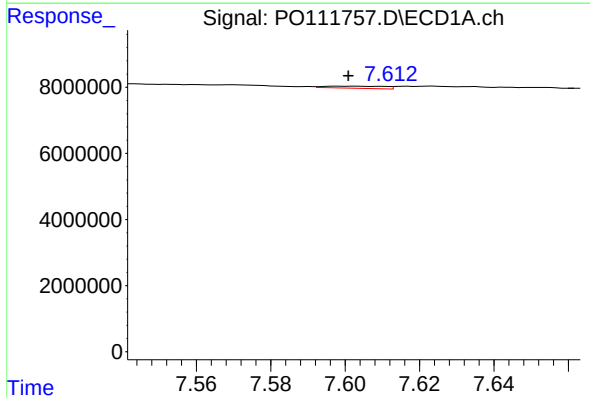


#38 AR-1262-3

R.T.: 7.598 min
Delta R.T.: -0.003 min
Response: 694438
Conc: 1.75 ng/ml

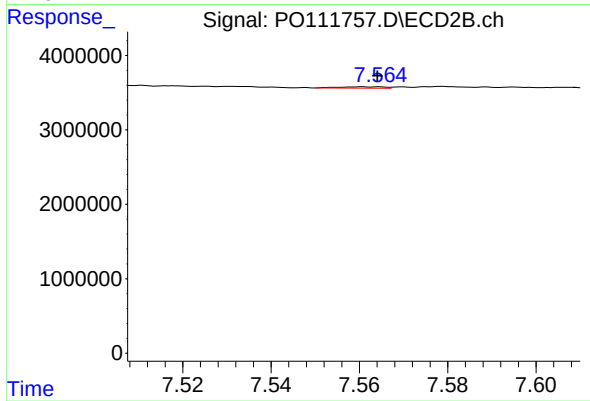

#38 AR-1262-3


R.T.: 7.561 min
Delta R.T.: -0.003 min
Response: 128260
Conc: 0.77 ng/ml

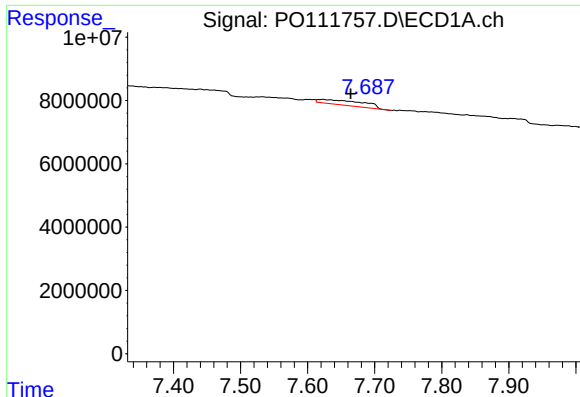

#39 AR-1262-4


R.T.: 7.623 min
Delta R.T.: -0.041 min
Response: 7095364
Conc: 10.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

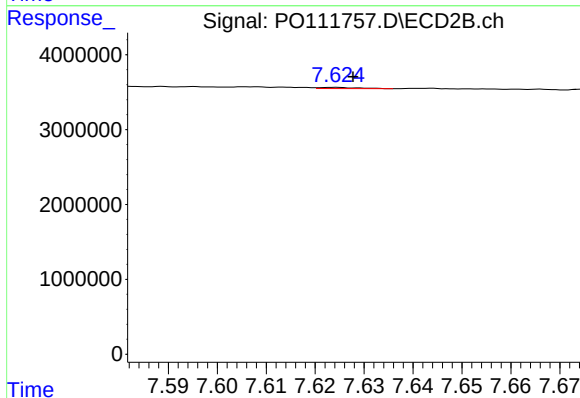


#39 AR-1262-4

R.T.: 7.624 min
Delta R.T.: -0.003 min
Response: 91049
Conc: 0.33 ng/ml

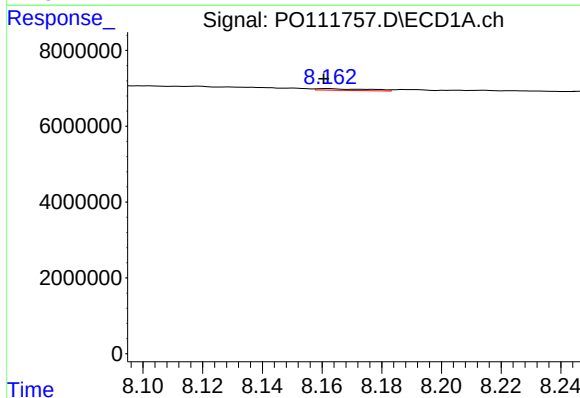


#40 AR-1262-5

R.T.: 8.162 min
Delta R.T.: 0.002 min
Response: 525708
Conc: 1.73 ng/ml

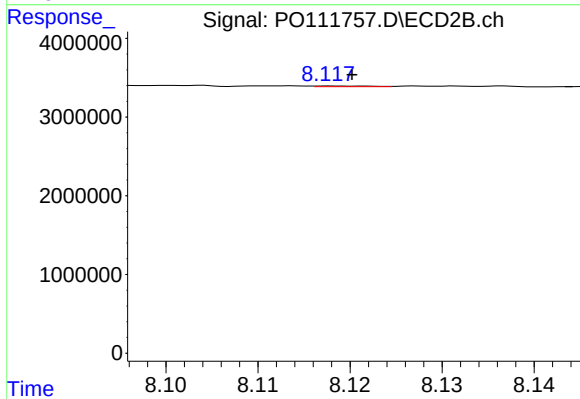

#40 AR-1262-5


R.T.: 8.117 min
Delta R.T.: -0.003 min
Response: 35508
Conc: 0.35 ng/ml

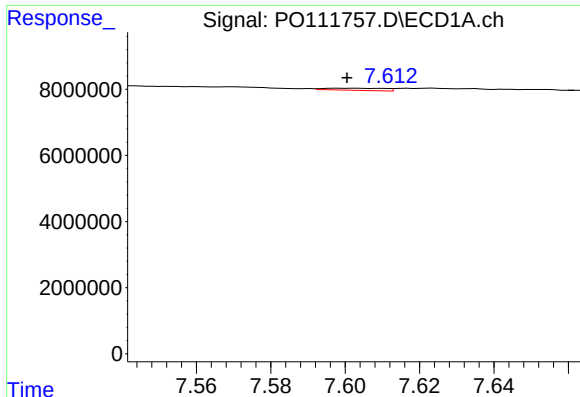

#41 AR-1268-1


R.T.: 7.598 min
Delta R.T.: -0.002 min
Response: 694438
Conc: 0.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

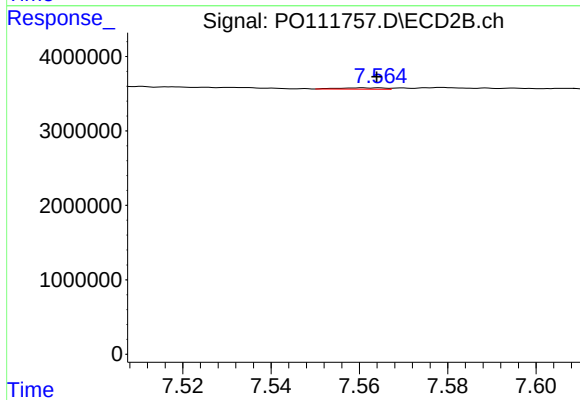


#41 AR-1268-1

R.T.: 7.561 min
Delta R.T.: -0.003 min
Response: 128260
Conc: 0.27 ng/ml

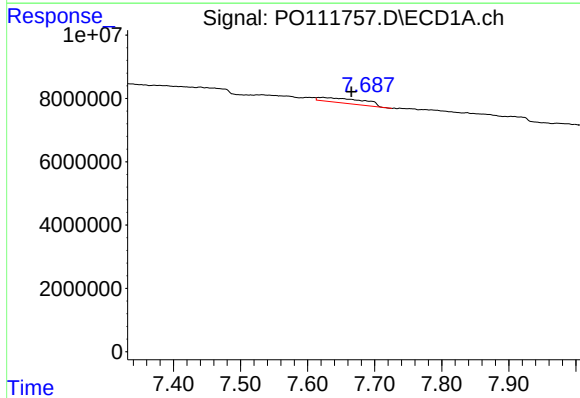


#42 AR-1268-2

R.T.: 7.623 min
Delta R.T.: -0.042 min
Response: 7095364
Conc: 7.26 ng/ml

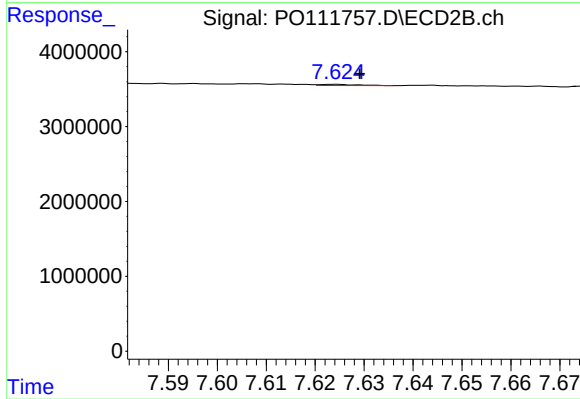

#42 AR-1268-2


R.T.: 7.624 min
Delta R.T.: -0.005 min
Response: 91049
Conc: 0.22 ng/ml

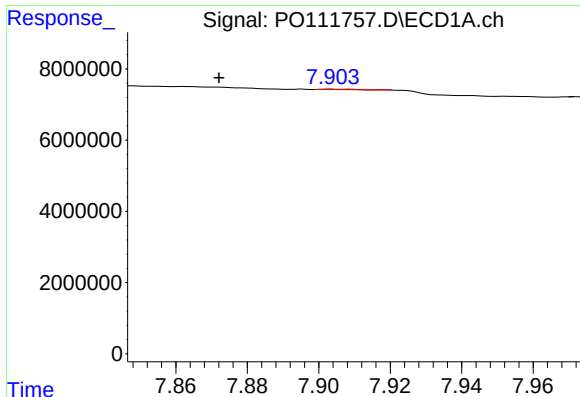

#43 AR-1268-3


R.T.: 7.903 min
Delta R.T.: 0.031 min
Response: 14738
Conc: 0.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

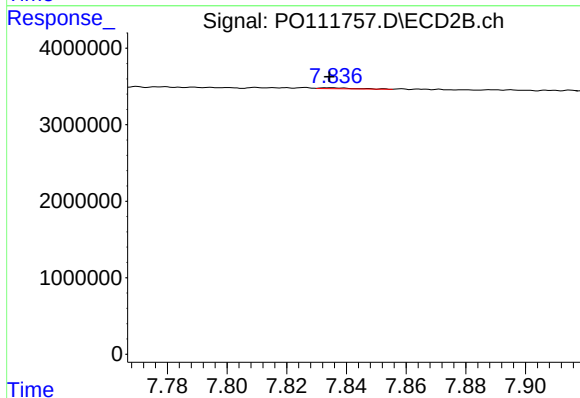


#43 AR-1268-3

R.T.: 7.835 min
Delta R.T.: 0.000 min
Response: 104135
Conc: 0.33 ng/ml

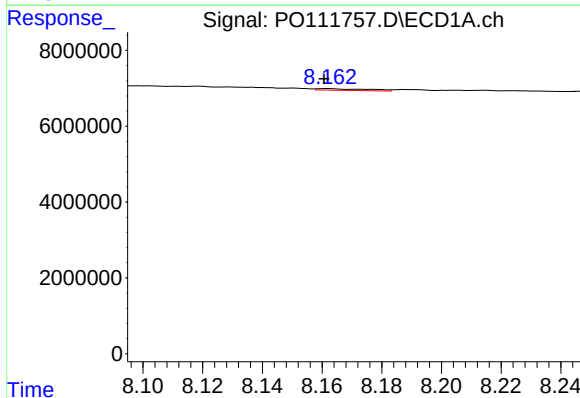


#44 AR-1268-4

R.T.: 8.162 min
Delta R.T.: 0.002 min
Response: 525708
Conc: 1.53 ng/ml

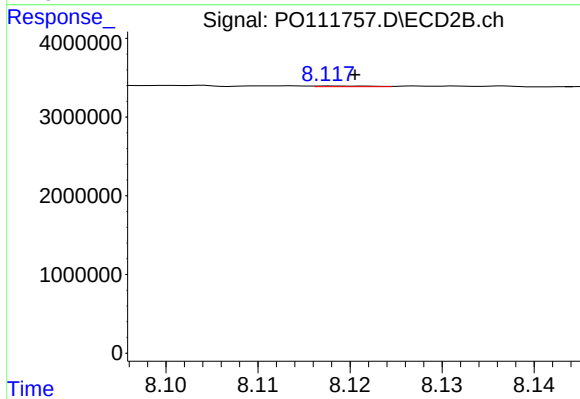

#44 AR-1268-4


R.T.: 8.117 min
Delta R.T.: -0.003 min
Response: 35508
Conc: 0.31 ng/ml

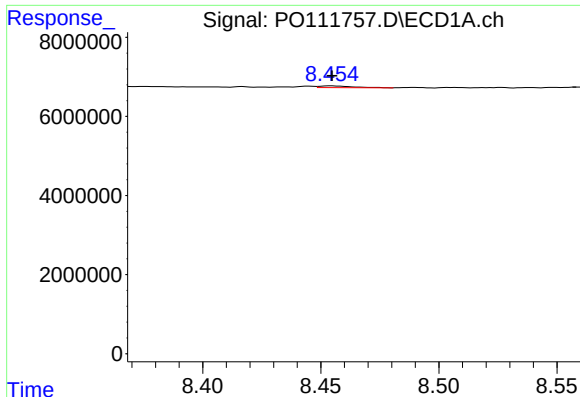

#45 AR-1268-5

R.T.: 8.454 min
Delta R.T.: 0.000 min
Response: 405619
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

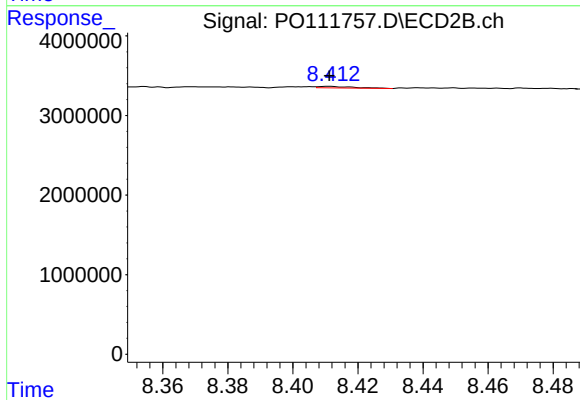

#45 AR-1268-5

R.T.: 8.411 min
Delta R.T.: 0.000 min
Response: 138631
Conc: 0.19 ng/ml