

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
 Data File : P0111762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 16:03
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:05:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.675	3.673	119.7E6	105.9E6	20.779	18.850
2)	SA Decachlor...	8.710	8.659	104.7E6	36691059	19.945	20.640
Target Compounds							
3)	L1 AR-1016-1	4.764	4.749	1126066	1140326	4.720	5.795
4)	L1 AR-1016-2	4.787	4.766	325451	1491549	0.978	5.236 #
5)	L1 AR-1016-3	4.843	4.946	676549	179943	2.940	1.198 #
6)	L1 AR-1016-4	4.957	4.985	1275701	391023	6.878	3.211 #
7)	L1 AR-1016-5	5.221	5.198	1678396	114457	8.993	0.719 #
8)	L2 AR-1221-1	3.901	3.884	339185	155780	3.895	2.086 #
9)	L2 AR-1221-2	3.978	3.970	2258233	2027834	35.193	36.244
10)	L2 AR-1221-3	4.017	4.041	779247	107151	3.995	0.624 #
11)	L3 AR-1232-1	4.017	4.041	779247	107151	5.135	0.806 #
12)	L3 AR-1232-2	4.555	4.766	903173	1491549	10.475	11.318
13)	L3 AR-1232-3	4.787	4.946	325451	179943	1.998	2.603 #
14)	L3 AR-1232-4	4.957	5.031	1275701	86634	14.660	1.432 #
15)	L3 AR-1232-5	5.003	5.198	1038572	114457	18.356	1.723 #
16)	L4 AR-1242-1	4.764	4.749	1126066	1140326	5.590	7.006 #
17)	L4 AR-1242-2	4.787	4.766	325451	1491549	1.155	6.318 #
18)	L4 AR-1242-3	4.843	4.946	676549	179943	3.403	1.433 #
19)	L4 AR-1242-4	4.957	5.031	1275701	86634	8.064	0.707 #
20)	L4 AR-1242-5	5.632	5.547	6550124	2685473	39.172	17.916 #
21)	L5 AR-1248-1	4.764	4.749	1126066	1140326	6.983	8.556
22)	L5 AR-1248-2	5.003	4.985	1038572	391023	4.817	2.195 #
23)	L5 AR-1248-3	5.221	5.025	1678396	130790	6.222	0.690 #
24)	L5 AR-1248-4	5.570	5.198	8235021	114457	20.598	0.501 #
25)	L5 AR-1248-5	5.632	5.597	6550124	1471328	23.326	6.757 #
26)	L6 AR-1254-1	5.570	5.547	8235021	2685473	19.373	8.314 #
27)	L6 AR-1254-2	5.720	5.695	9321075	3257102	24.560	11.661 #
28)	L6 AR-1254-3	6.140	6.112	20006774	9843436	35.017	23.490 #
29)	L6 AR-1254-4	6.383	6.300	8980318	854027	25.740	3.749 #
30)	L6 AR-1254-5	6.769	6.740	15928082	5972073	31.102	18.342 #
31)	L7 AR-1260-1	6.254	6.227	35733022	14711203	100.565	58.630 #
32)	L7 AR-1260-2	6.443	6.415	32478406	11234924	68.741	38.212 #
33)	L7 AR-1260-3	6.811	6.569	34055000	8186507	80.191	30.640 #
34)	L7 AR-1260-4	7.070	7.037	34916309	12153706	111.040	63.934 #
35)	L7 AR-1260-5	7.313	7.279	47025798	19273982	57.089	45.348
36)	L8 AR-1262-1	6.811	6.779	34055000	14119480	55.839	41.815 #
37)	L8 AR-1262-2	7.313	7.279	47025798	19273982	49.953	41.381
38)	L8 AR-1262-3	7.598	7.560	14529512	5666698	36.633	34.078
39)	L8 AR-1262-4	7.662	7.624	26490168	10281568	40.320	37.108
40)	L8 AR-1262-5	8.157	8.117	9899798	3482969	32.494	34.275
41)	L9 AR-1268-1	7.598	7.560	14529512	5666698	12.897	11.845

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
 Data File : P0111762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 16:03
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:05:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.662	7.624	26490168	10281568	27.107	24.686
43) L9	AR-1268-3	7.857	7.832	1111906	628662	1.357	1.983 #
44) L9	AR-1268-4	8.157	8.117	9899798	3482969	28.780	30.115
45) L9	AR-1268-5	8.452	8.407	3764510	1479028	1.695	2.041



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062025\
Data File : PO111762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 16:03
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:05:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

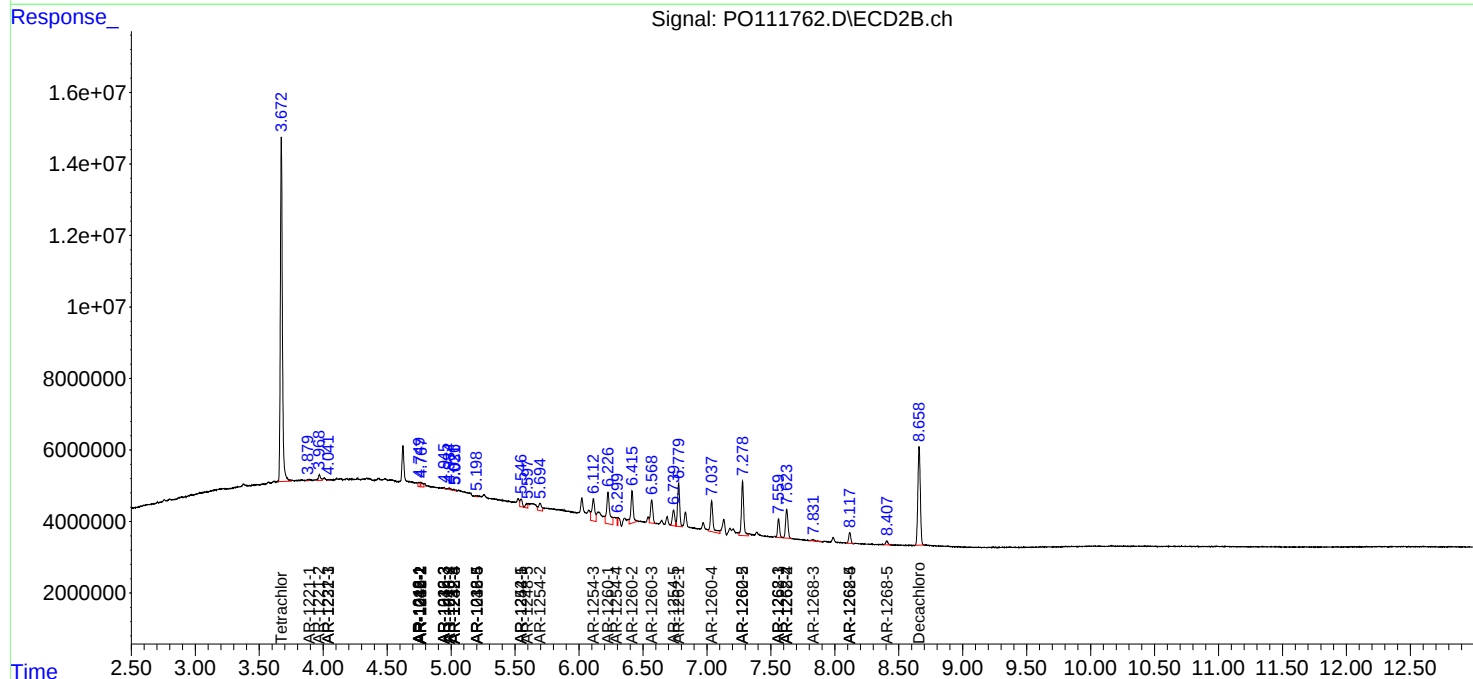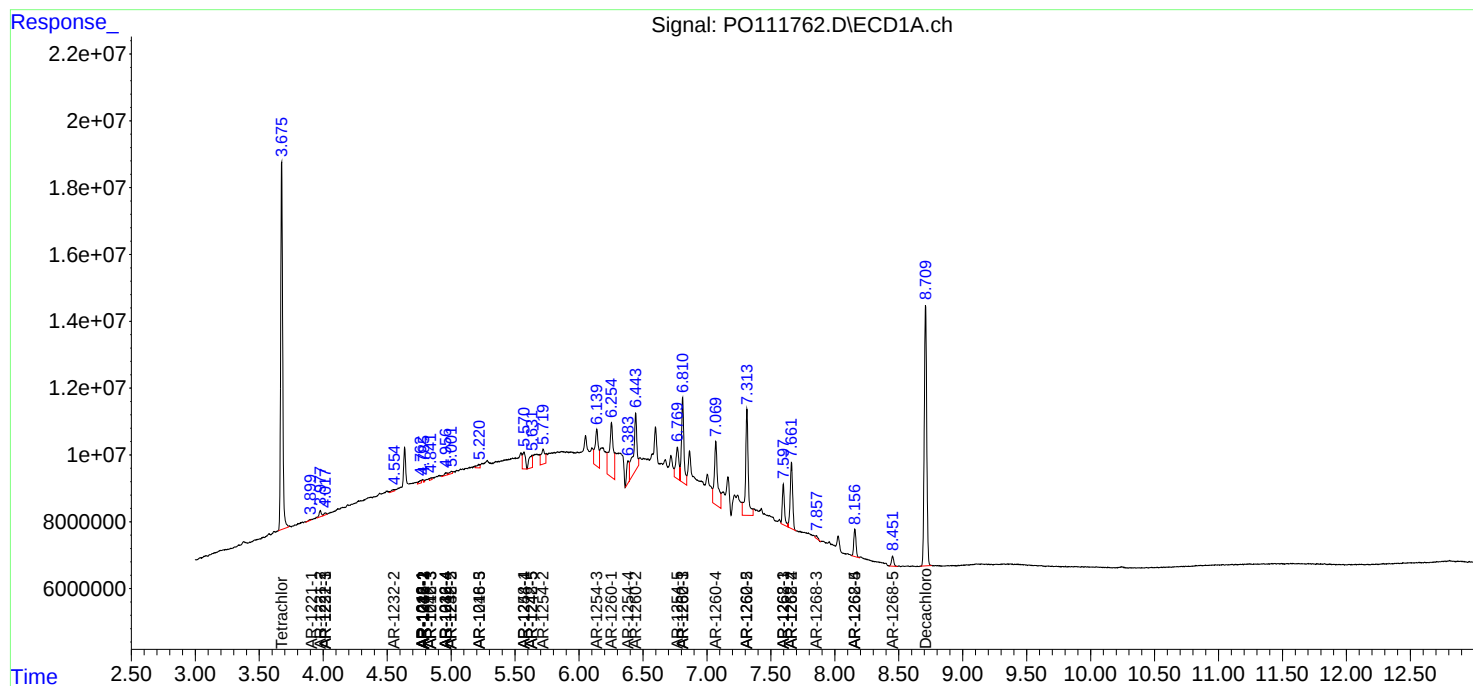


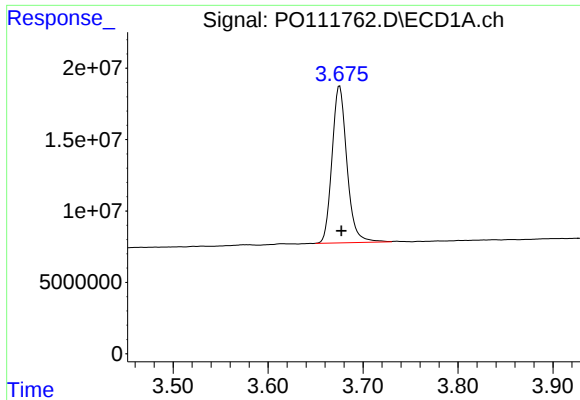

#1 Tetrachloro-m-xylene


R.T.: 3.675 min
Delta R.T.: -0.002 min
Response: 119677201
Conc: 20.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

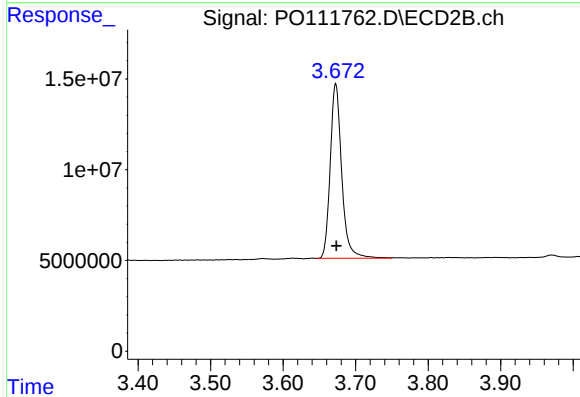


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 105883608
Conc: 18.85 ng/ml

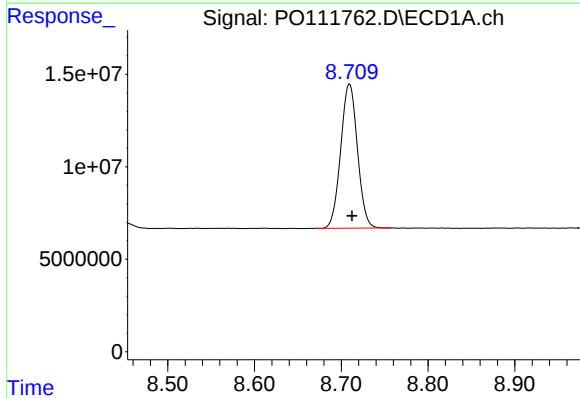


#2 Decachlorobiphenyl

R.T.: 8.710 min
Delta R.T.: -0.003 min
Response: 104694680
Conc: 19.94 ng/ml

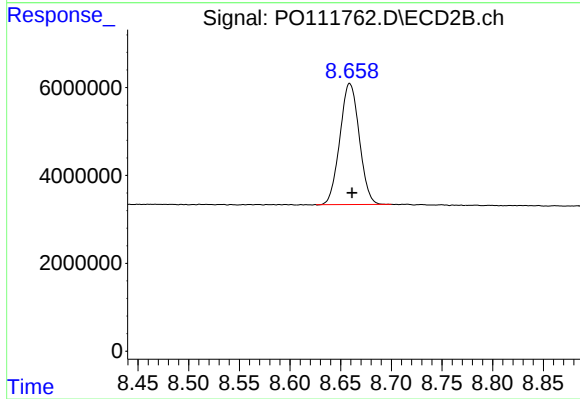

#2 Decachlorobiphenyl


R.T.: 8.659 min
Delta R.T.: -0.002 min
Response: 36691059
Conc: 20.64 ng/ml

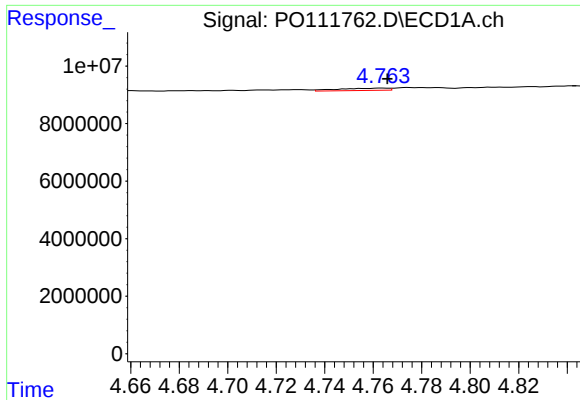

#3 AR-1016-1


R.T.: 4.764 min
Delta R.T.: -0.002 min
Response: 1126066
Conc: 4.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

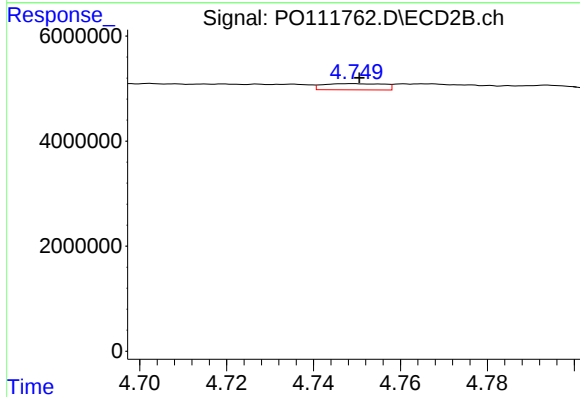


#3 AR-1016-1

R.T.: 4.749 min
Delta R.T.: -0.001 min
Response: 1140326
Conc: 5.80 ng/ml

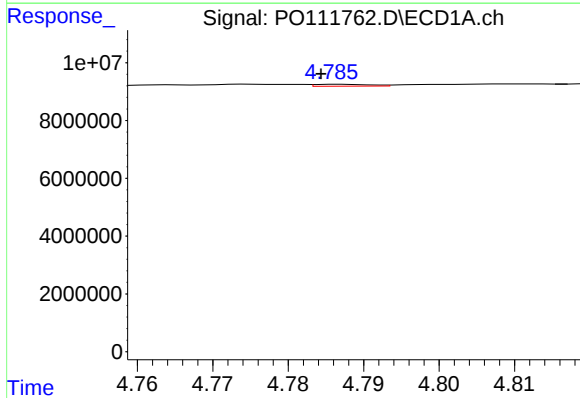


#4 AR-1016-2

R.T.: 4.787 min
Delta R.T.: 0.002 min
Response: 325451
Conc: 0.98 ng/ml

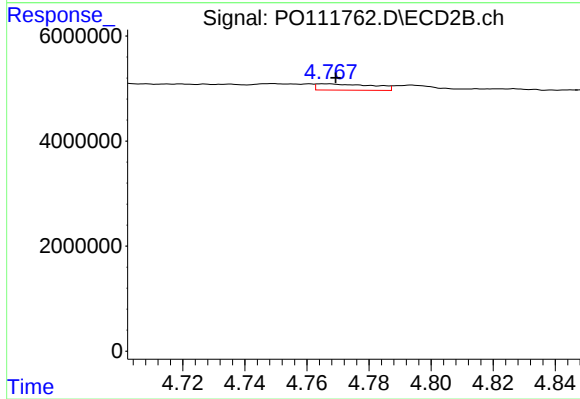

#4 AR-1016-2


R.T.: 4.766 min
Delta R.T.: -0.003 min
Response: 1491549
Conc: 5.24 ng/ml

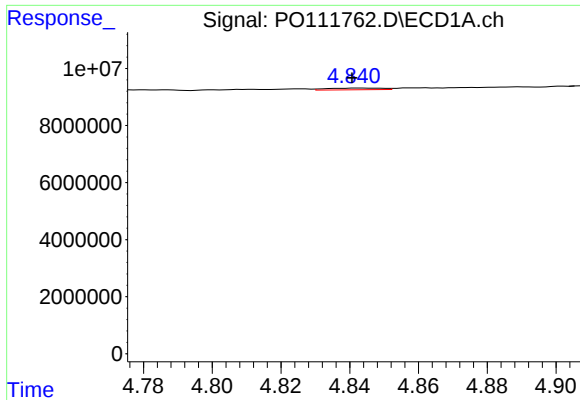

#5 AR-1016-3


R.T.: 4.843 min
Delta R.T.: 0.002 min
Response: 676549
Conc: 2.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

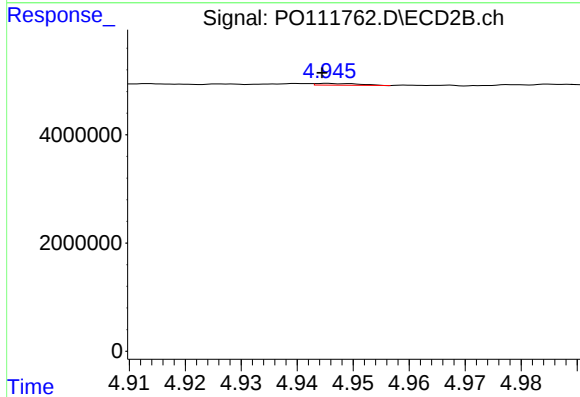


#5 AR-1016-3

R.T.: 4.946 min
Delta R.T.: 0.001 min
Response: 179943
Conc: 1.20 ng/ml

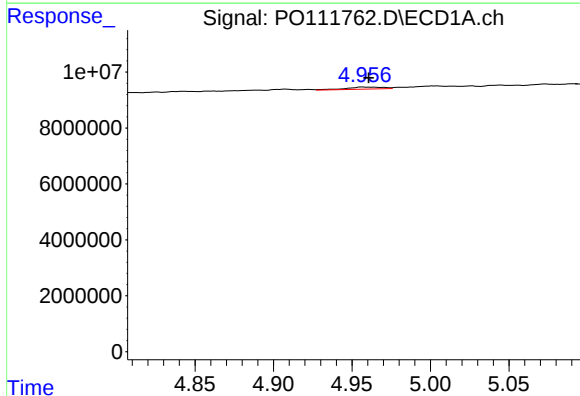


#6 AR-1016-4

R.T.: 4.957 min
Delta R.T.: -0.004 min
Response: 1275701
Conc: 6.88 ng/ml

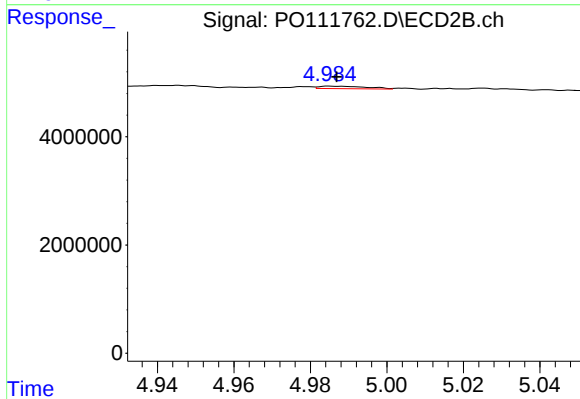

#6 AR-1016-4


R.T.: 4.985 min
Delta R.T.: -0.002 min
Response: 391023
Conc: 3.21 ng/ml

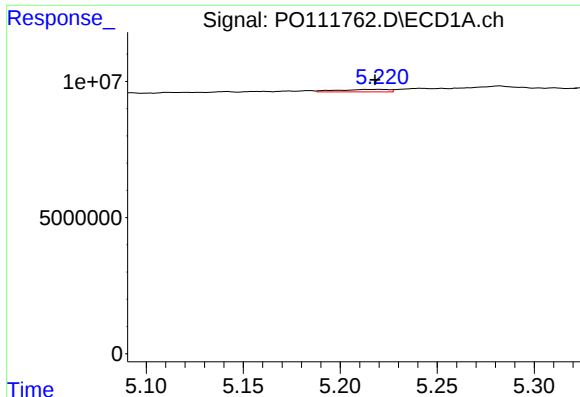

#7 AR-1016-5


R.T.: 5.221 min
Delta R.T.: 0.003 min
Response: 1678396
Conc: 8.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

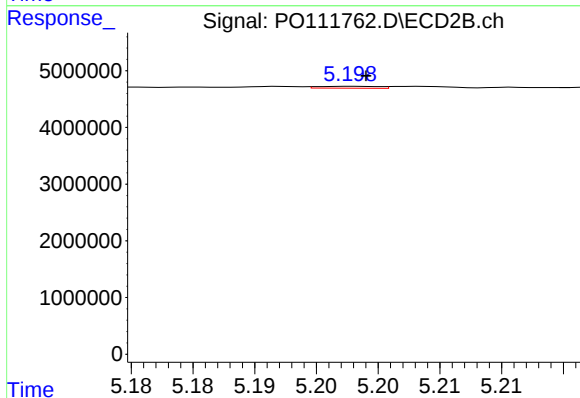


#7 AR-1016-5

R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 114457
Conc: 0.72 ng/ml

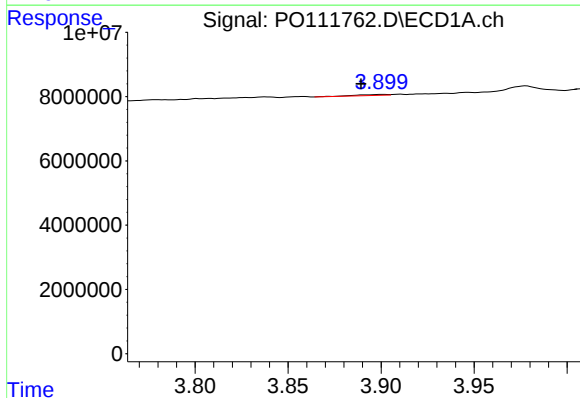


#8 AR-1221-1

R.T.: 3.901 min
Delta R.T.: 0.011 min
Response: 339185
Conc: 3.90 ng/ml

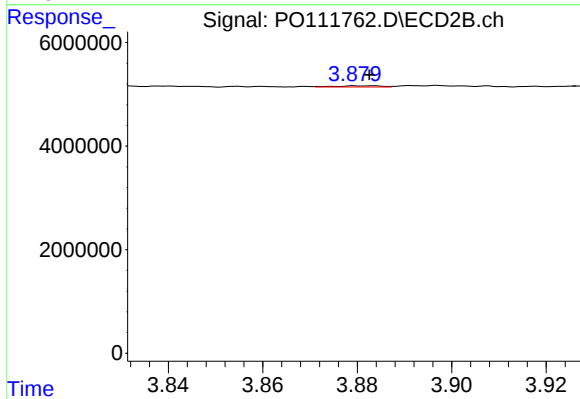

#8 AR-1221-1


R.T.: 3.884 min
Delta R.T.: 0.001 min
Response: 155780
Conc: 2.09 ng/ml

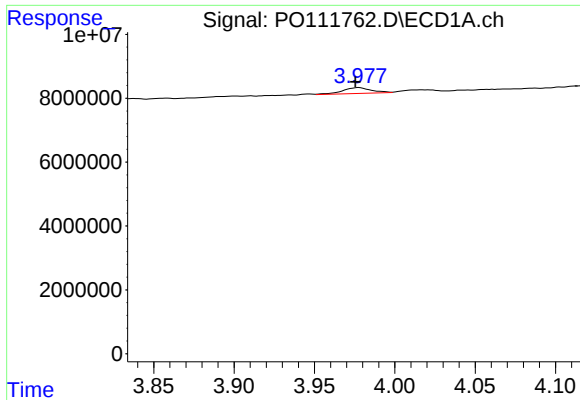

#9 AR-1221-2


R.T.: 3.978 min
Delta R.T.: 0.002 min
Response: 2258233
Conc: 35.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

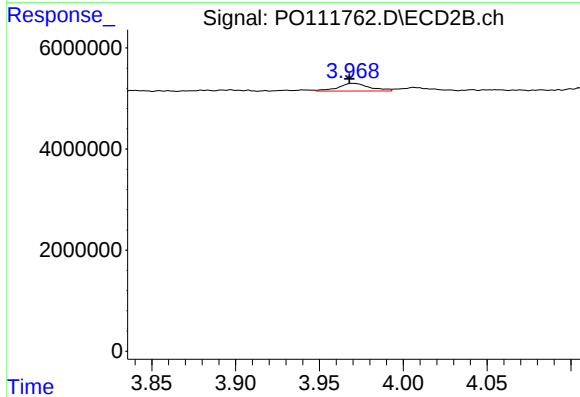


#9 AR-1221-2

R.T.: 3.970 min
Delta R.T.: 0.002 min
Response: 2027834
Conc: 36.24 ng/ml

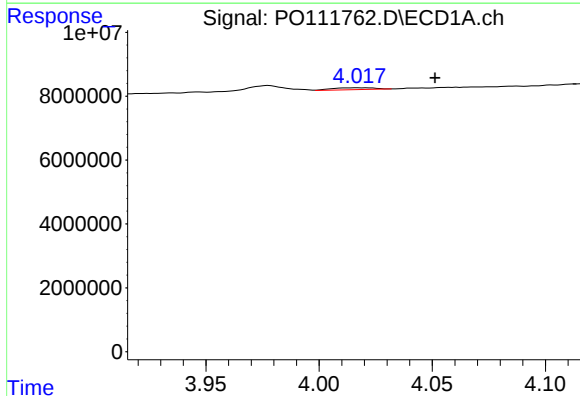


#10 AR-1221-3

R.T.: 4.017 min
Delta R.T.: -0.034 min
Response: 779247
Conc: 4.00 ng/ml

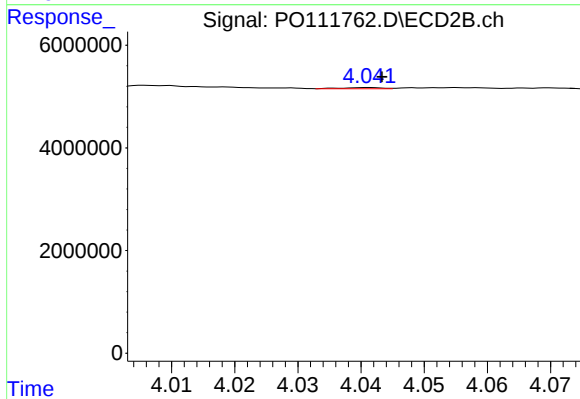

#10 AR-1221-3


R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 107151
Conc: 0.62 ng/ml

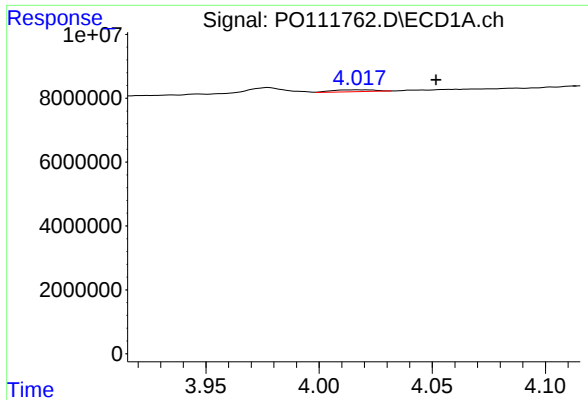

#11 AR-1232-1


R.T.: 4.017 min
Delta R.T.: -0.035 min
Response: 779247
Conc: 5.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

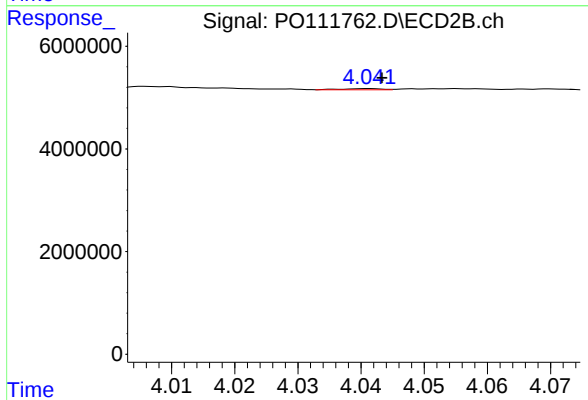


#11 AR-1232-1

R.T.: 4.041 min
Delta R.T.: -0.002 min
Response: 107151
Conc: 0.81 ng/ml

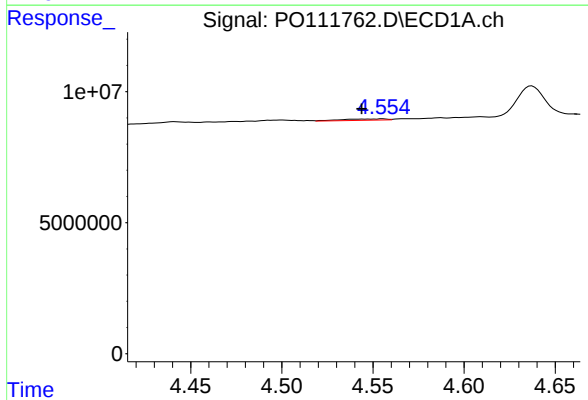


#12 AR-1232-2

R.T.: 4.555 min
Delta R.T.: 0.012 min
Response: 903173
Conc: 10.48 ng/ml

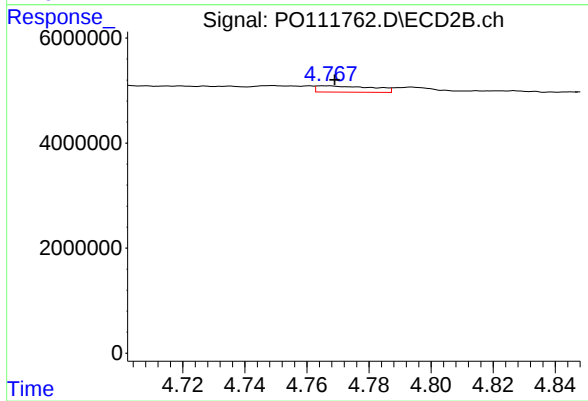

#12 AR-1232-2


R.T.: 4.766 min
Delta R.T.: -0.003 min
Response: 1491549
Conc: 11.32 ng/ml

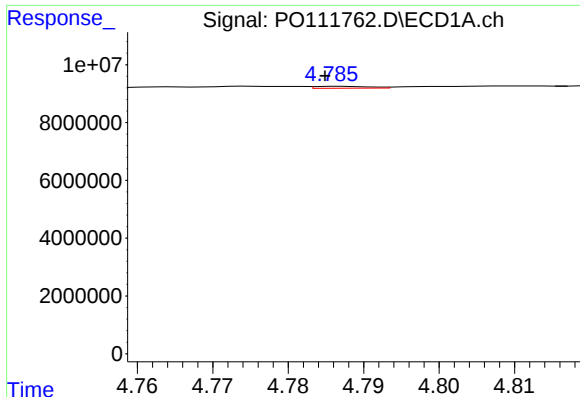

#13 AR-1232-3


R.T.: 4.787 min
Delta R.T.: 0.002 min
Response: 325451
Conc: 2.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

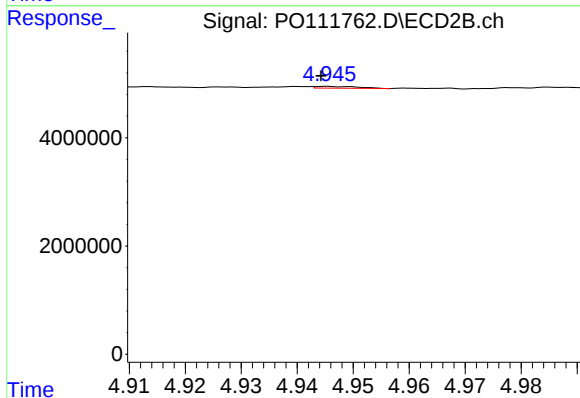


#13 AR-1232-3

R.T.: 4.946 min
Delta R.T.: 0.001 min
Response: 179943
Conc: 2.60 ng/ml

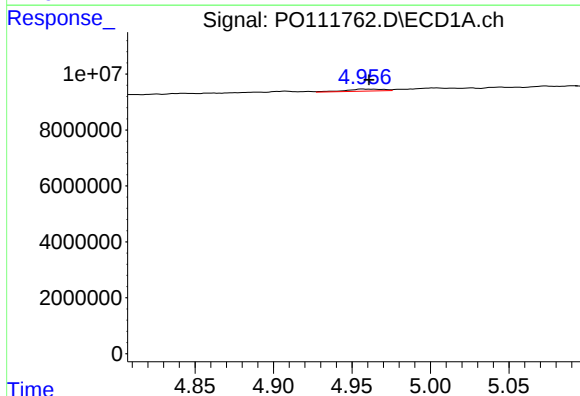


#14 AR-1232-4

R.T.: 4.957 min
Delta R.T.: -0.004 min
Response: 1275701
Conc: 14.66 ng/ml

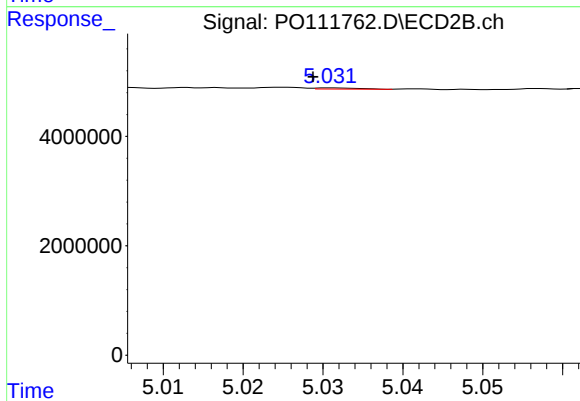

#14 AR-1232-4


R.T.: 5.031 min
Delta R.T.: 0.002 min
Response: 86634
Conc: 1.43 ng/ml

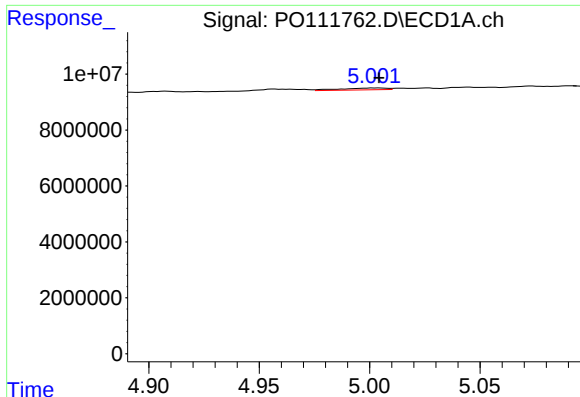

#15 AR-1232-5


R.T.: 5.003 min
Delta R.T.: -0.001 min
Response: 1038572
Conc: 18.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

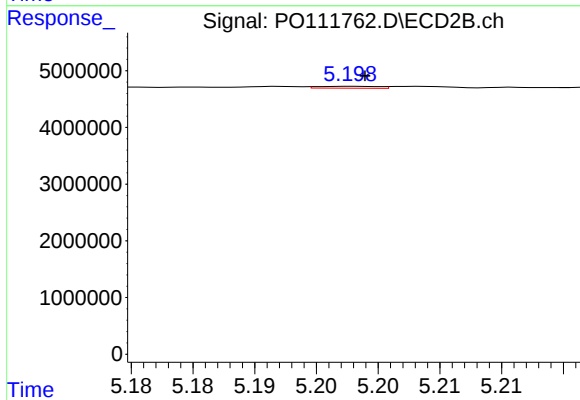


#15 AR-1232-5

R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 114457
Conc: 1.72 ng/ml

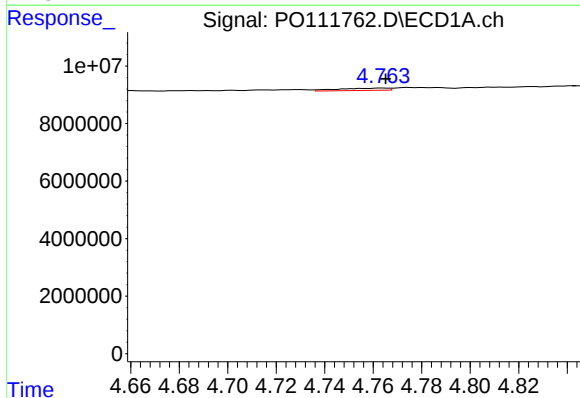


#16 AR-1242-1

R.T.: 4.764 min
Delta R.T.: -0.001 min
Response: 1126066
Conc: 5.59 ng/ml

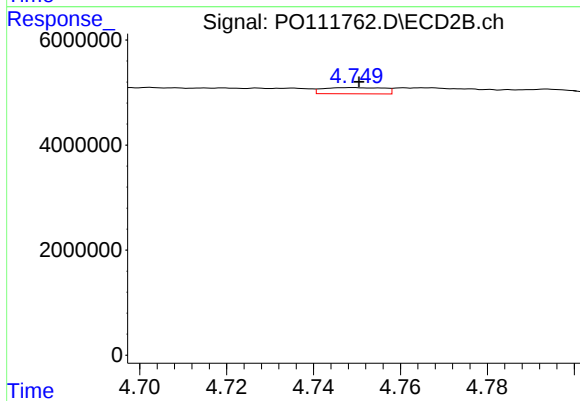

#16 AR-1242-1


R.T.: 4.749 min
Delta R.T.: -0.001 min
Response: 1140326
Conc: 7.01 ng/ml

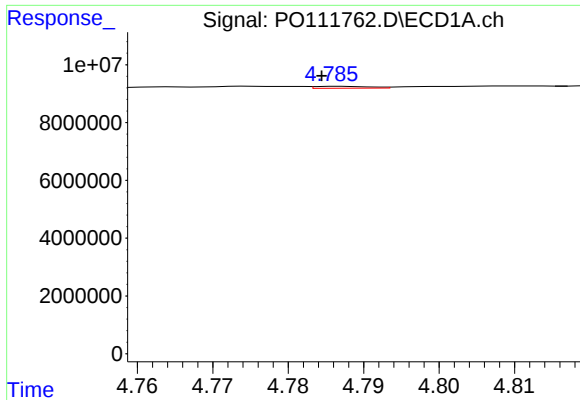

#17 AR-1242-2


R.T.: 4.787 min
Delta R.T.: 0.002 min
Response: 325451
Conc: 1.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

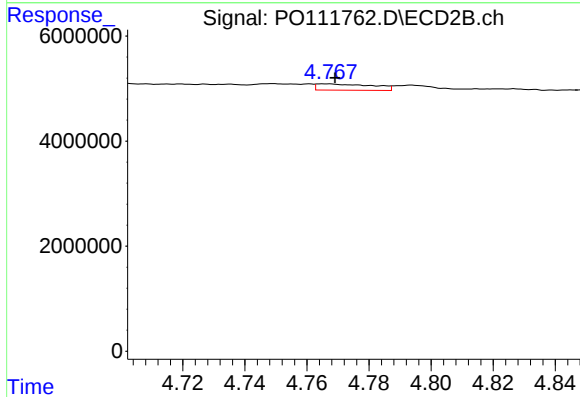


#17 AR-1242-2

R.T.: 4.766 min
Delta R.T.: -0.003 min
Response: 1491549
Conc: 6.32 ng/ml

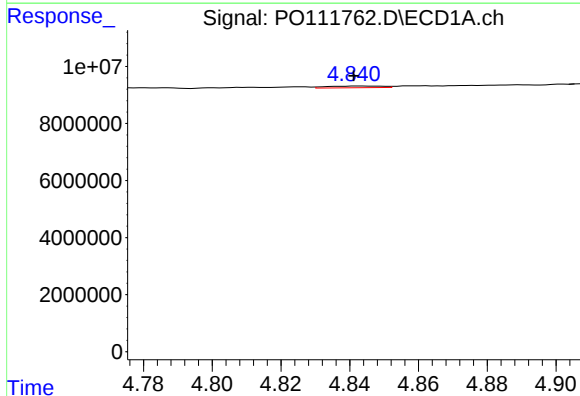


#18 AR-1242-3

R.T.: 4.843 min
Delta R.T.: 0.002 min
Response: 676549
Conc: 3.40 ng/ml

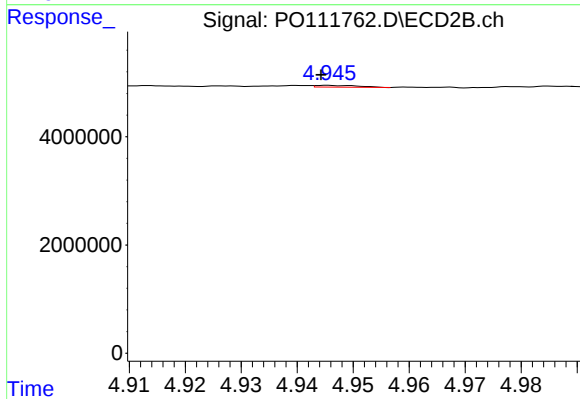

#18 AR-1242-3


R.T.: 4.946 min
Delta R.T.: 0.001 min
Response: 179943
Conc: 1.43 ng/ml

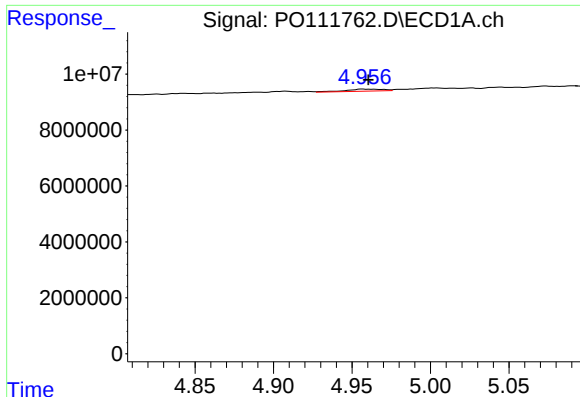

#19 AR-1242-4


R.T.: 4.957 min
Delta R.T.: -0.004 min
Response: 1275701
Conc: 8.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

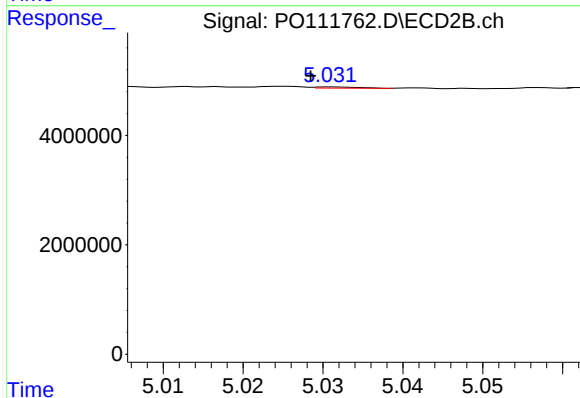


#19 AR-1242-4

R.T.: 5.031 min
Delta R.T.: 0.003 min
Response: 86634
Conc: 0.71 ng/ml

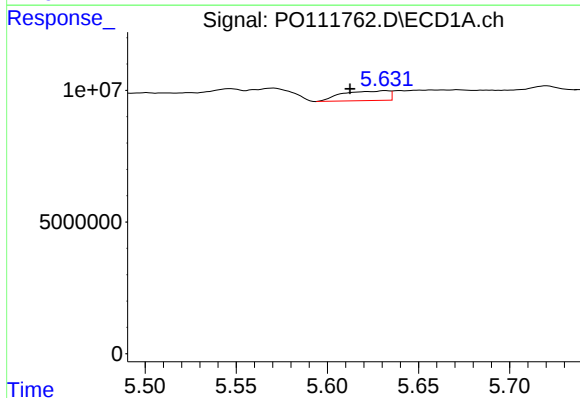


#20 AR-1242-5

R.T.: 5.632 min
Delta R.T.: 0.019 min
Response: 6550124
Conc: 39.17 ng/ml

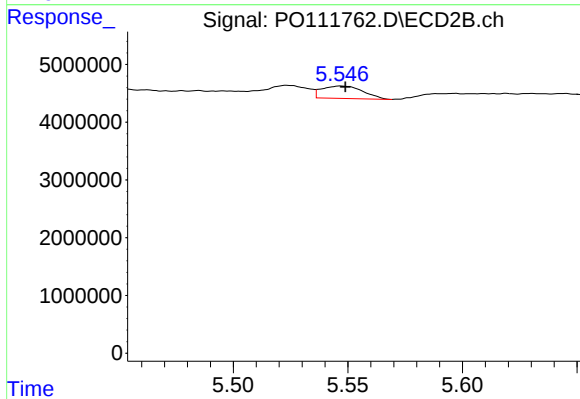

#20 AR-1242-5


R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 2685473
Conc: 17.92 ng/ml

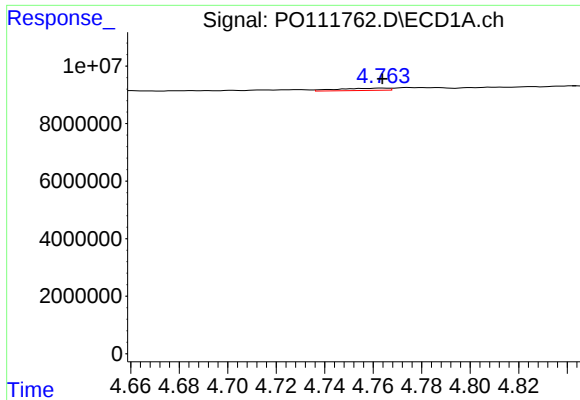

#21 AR-1248-1


R.T.: 4.764 min
Delta R.T.: 0.000 min
Response: 1126066
Conc: 6.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

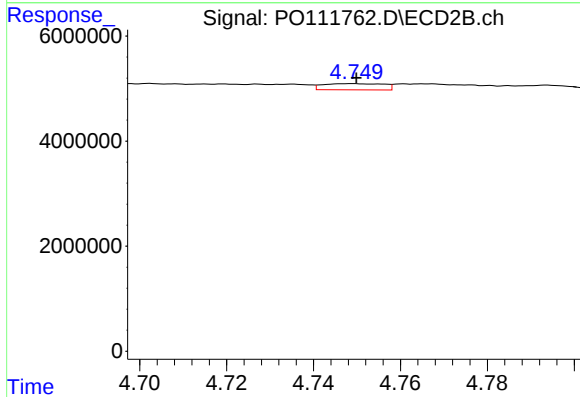


#21 AR-1248-1

R.T.: 4.749 min
Delta R.T.: 0.000 min
Response: 1140326
Conc: 8.56 ng/ml

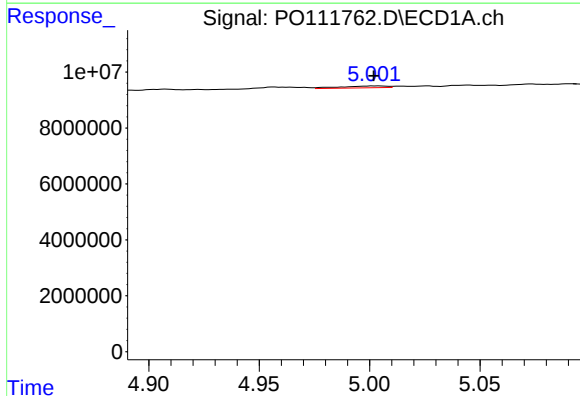


#22 AR-1248-2

R.T.: 5.003 min
Delta R.T.: 0.001 min
Response: 1038572
Conc: 4.82 ng/ml

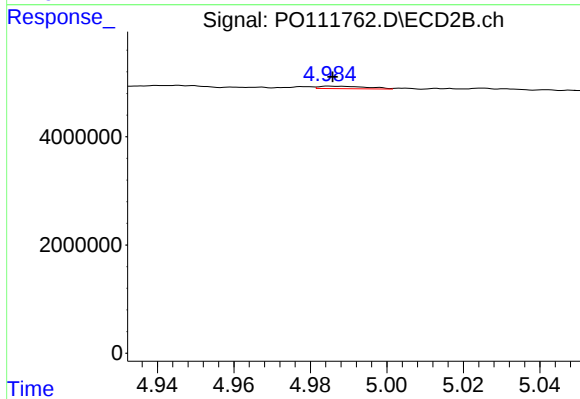

#22 AR-1248-2


R.T.: 4.985 min
Delta R.T.: 0.000 min
Response: 391023
Conc: 2.19 ng/ml

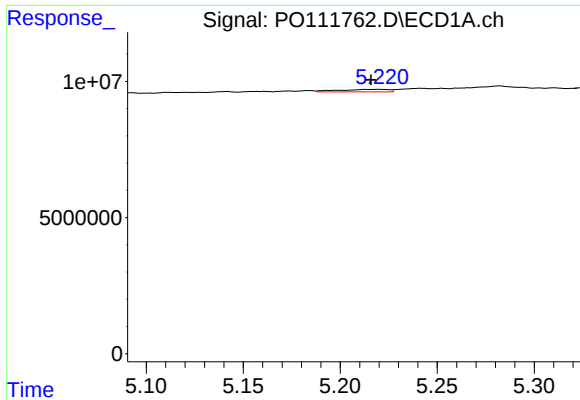

#23 AR-1248-3


R.T.: 5.221 min
Delta R.T.: 0.005 min
Response: 1678396
Conc: 6.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

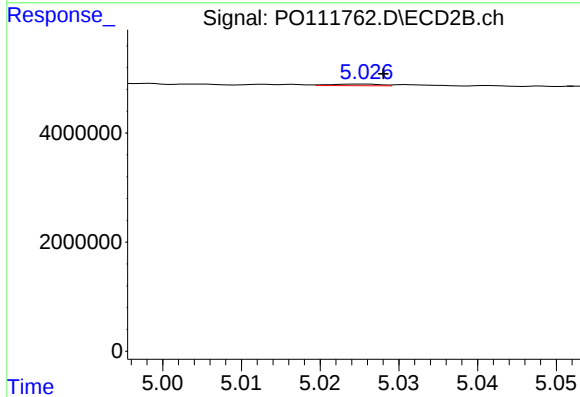


#23 AR-1248-3

R.T.: 5.025 min
Delta R.T.: -0.003 min
Response: 130790
Conc: 0.69 ng/ml

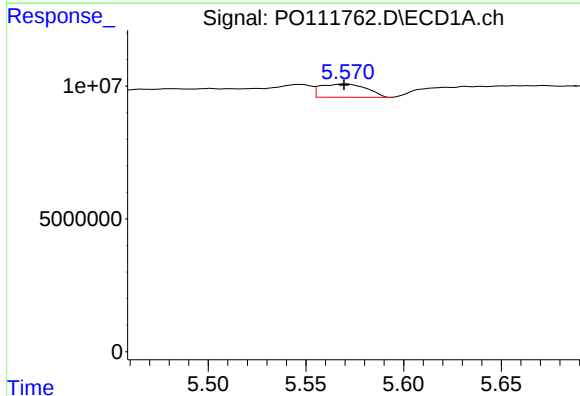


#24 AR-1248-4

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 8235021
Conc: 20.60 ng/ml

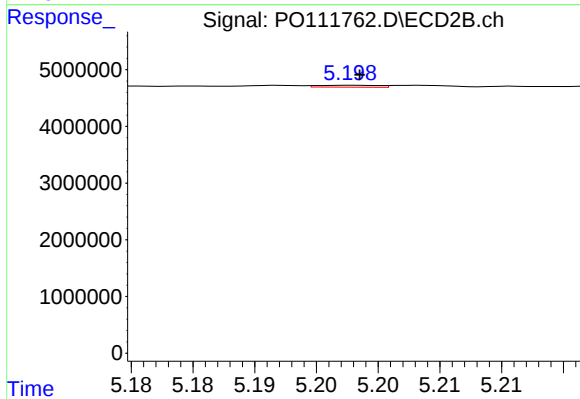

#24 AR-1248-4


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 114457
Conc: 0.50 ng/ml

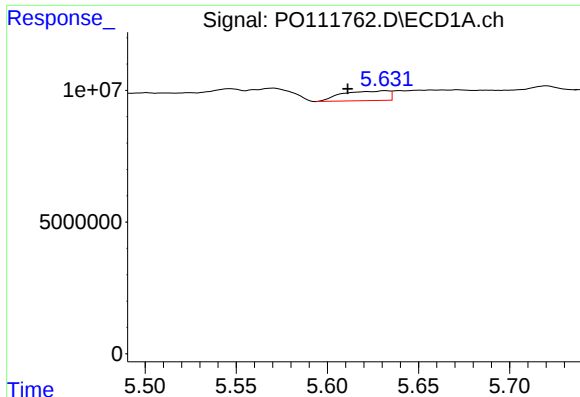

#25 AR-1248-5


R.T.: 5.632 min
Delta R.T.: 0.021 min
Response: 6550124
Conc: 23.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

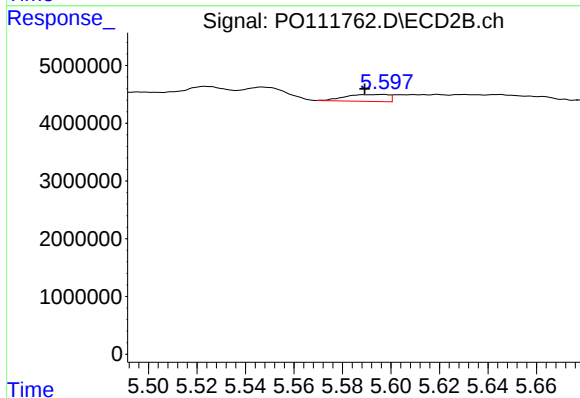


#25 AR-1248-5

R.T.: 5.597 min
Delta R.T.: 0.008 min
Response: 1471328
Conc: 6.76 ng/ml

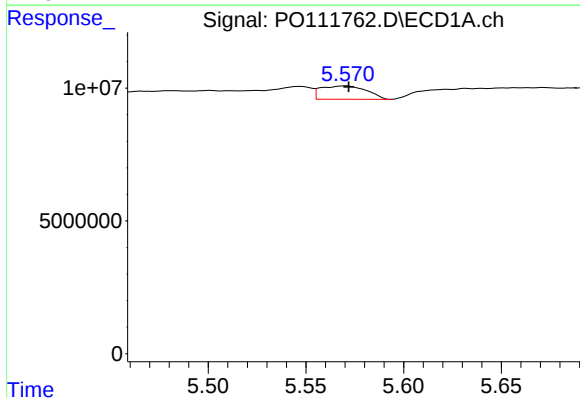


#26 AR-1254-1

R.T.: 5.570 min
Delta R.T.: -0.002 min
Response: 8235021
Conc: 19.37 ng/ml

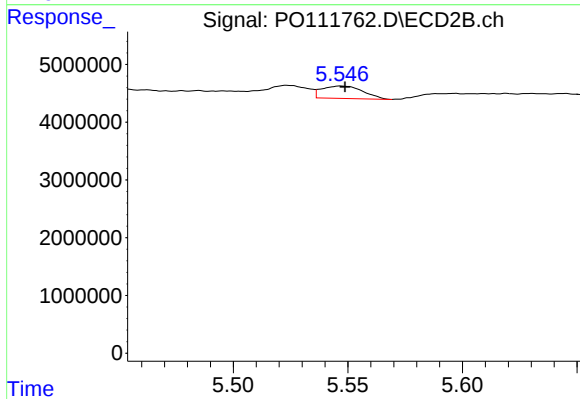

#26 AR-1254-1


R.T.: 5.547 min
Delta R.T.: -0.002 min
Response: 2685473
Conc: 8.31 ng/ml

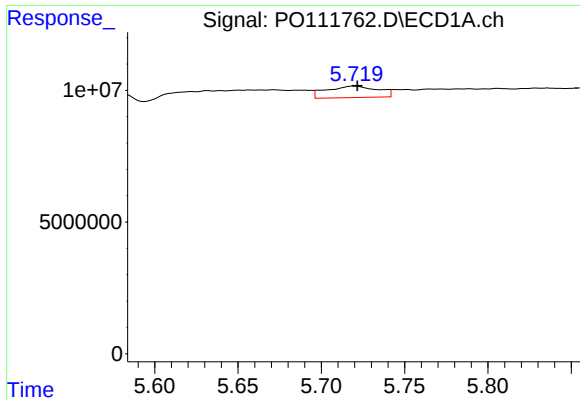

#27 AR-1254-2


R.T.: 5.720 min
Delta R.T.: -0.001 min
Response: 9321075
Conc: 24.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

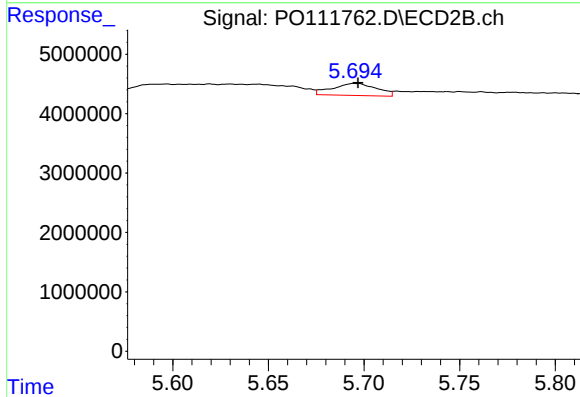


#27 AR-1254-2

R.T.: 5.695 min
Delta R.T.: -0.002 min
Response: 3257102
Conc: 11.66 ng/ml

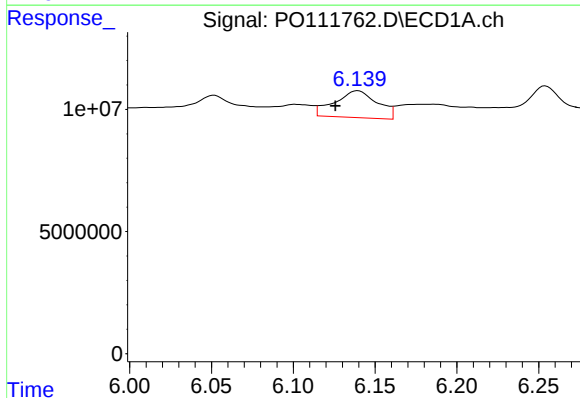


#28 AR-1254-3

R.T.: 6.140 min
Delta R.T.: 0.014 min
Response: 20006774
Conc: 35.02 ng/ml

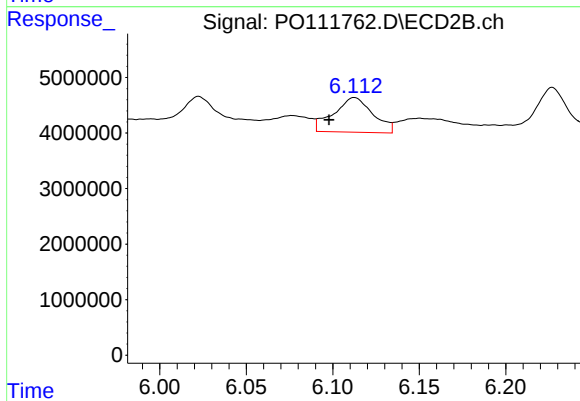

#28 AR-1254-3


R.T.: 6.112 min
Delta R.T.: 0.014 min
Response: 9843436
Conc: 23.49 ng/ml

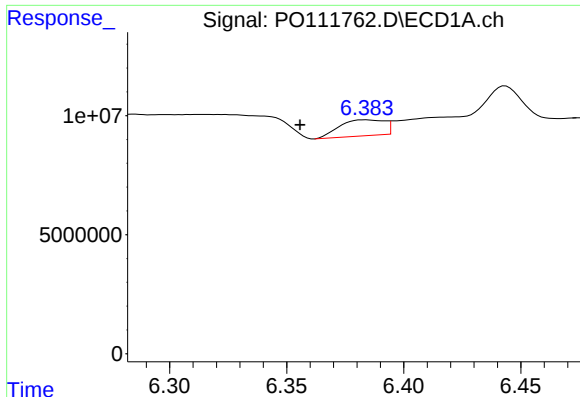

#29 AR-1254-4


R.T.: 6.383 min
Delta R.T.: 0.028 min
Response: 8980318
Conc: 25.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

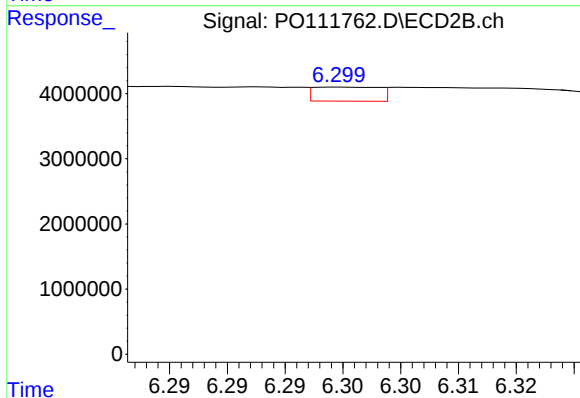


#29 AR-1254-4

R.T.: 6.300 min
Delta R.T.: -0.026 min
Response: 854027
Conc: 3.75 ng/ml

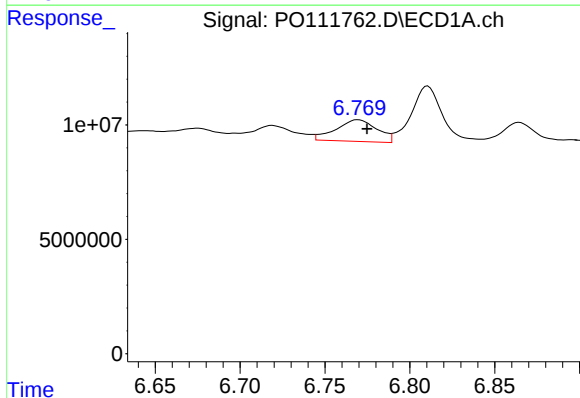


#30 AR-1254-5

R.T.: 6.769 min
Delta R.T.: -0.005 min
Response: 15928082
Conc: 31.10 ng/ml

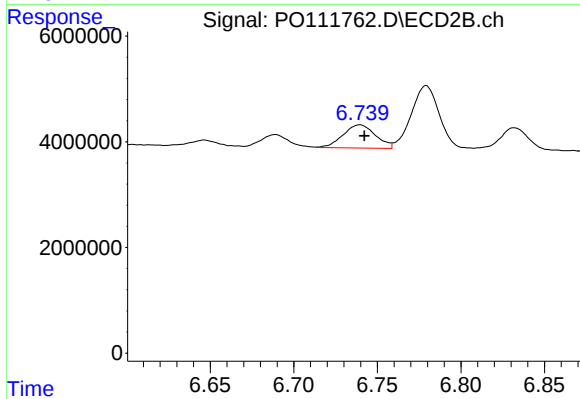

#30 AR-1254-5


R.T.: 6.740 min
Delta R.T.: -0.003 min
Response: 5972073
Conc: 18.34 ng/ml

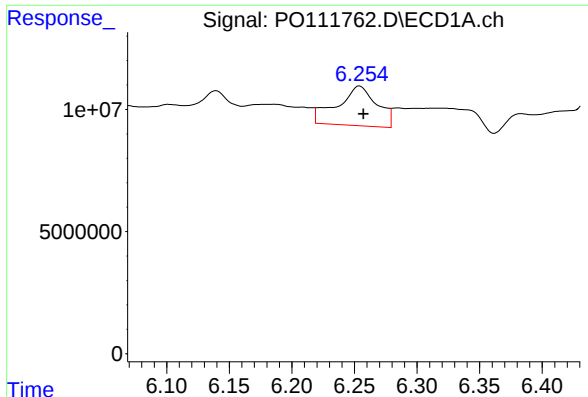

#31 AR-1260-1


R.T.: 6.254 min
Delta R.T.: -0.003 min
Response: 35733022
Conc: 100.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

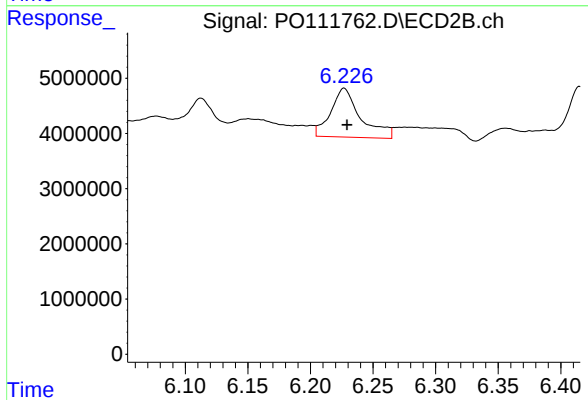


#31 AR-1260-1

R.T.: 6.227 min
Delta R.T.: -0.002 min
Response: 14711203
Conc: 58.63 ng/ml

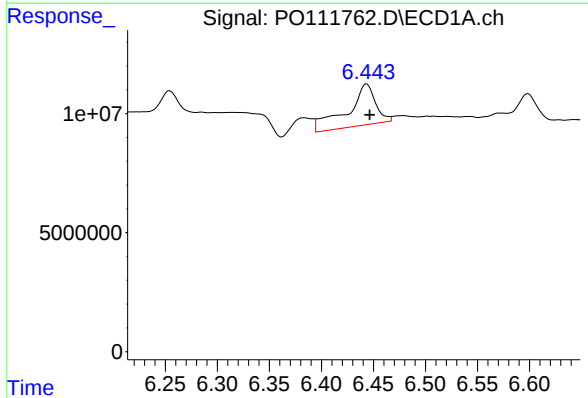


#32 AR-1260-2

R.T.: 6.443 min
Delta R.T.: -0.003 min
Response: 32478406
Conc: 68.74 ng/ml

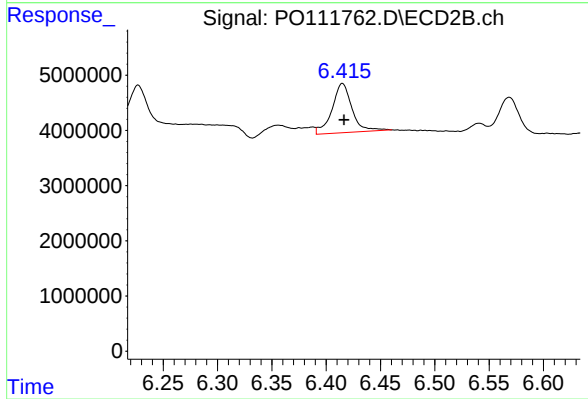

#32 AR-1260-2


R.T.: 6.415 min
Delta R.T.: -0.001 min
Response: 11234924
Conc: 38.21 ng/ml

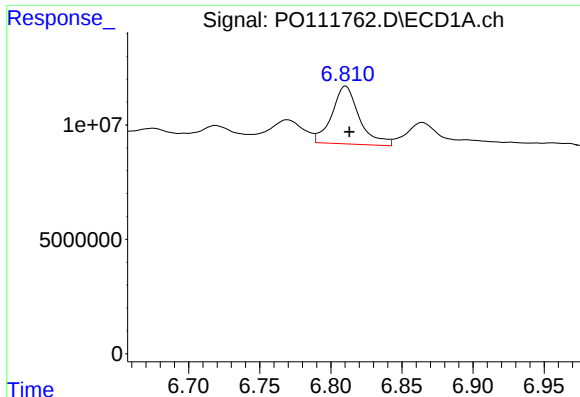

#33 AR-1260-3


R.T.: 6.811 min
Delta R.T.: -0.002 min
Response: 34055000
Conc: 80.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

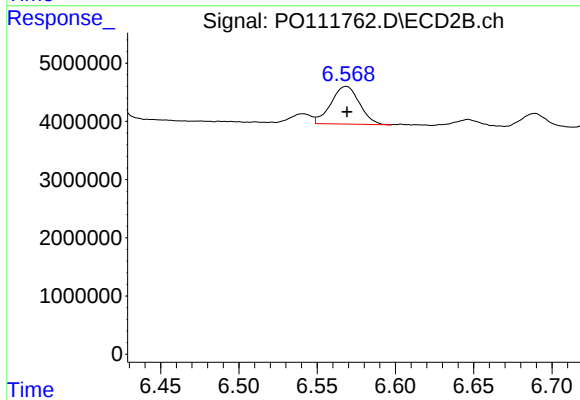


#33 AR-1260-3

R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 8186507
Conc: 30.64 ng/ml

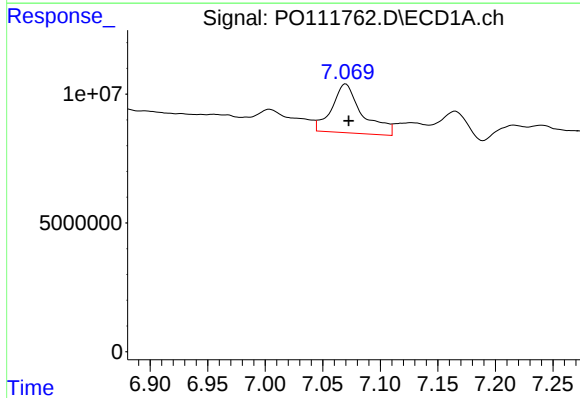


#34 AR-1260-4

R.T.: 7.070 min
Delta R.T.: -0.003 min
Response: 34916309
Conc: 111.04 ng/ml

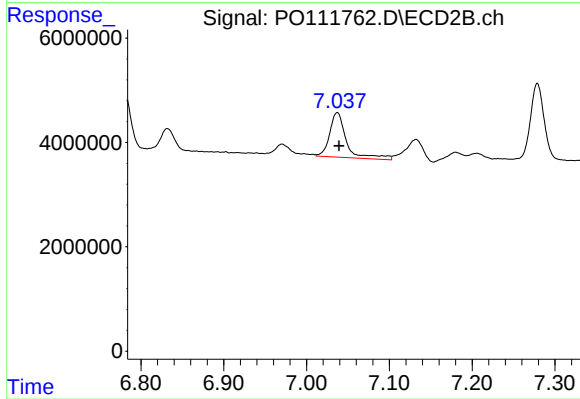

#34 AR-1260-4


R.T.: 7.037 min
Delta R.T.: -0.002 min
Response: 12153706
Conc: 63.93 ng/ml

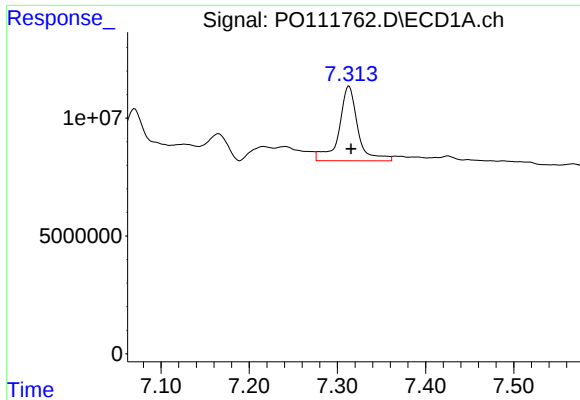

#35 AR-1260-5


R.T.: 7.313 min
Delta R.T.: -0.002 min
Response: 47025798
Conc: 57.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

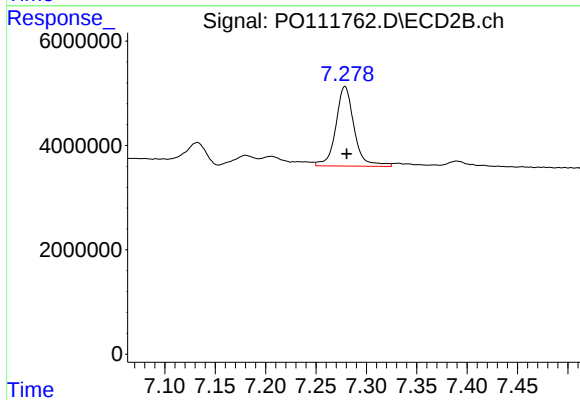


#35 AR-1260-5

R.T.: 7.279 min
Delta R.T.: -0.002 min
Response: 19273982
Conc: 45.35 ng/ml

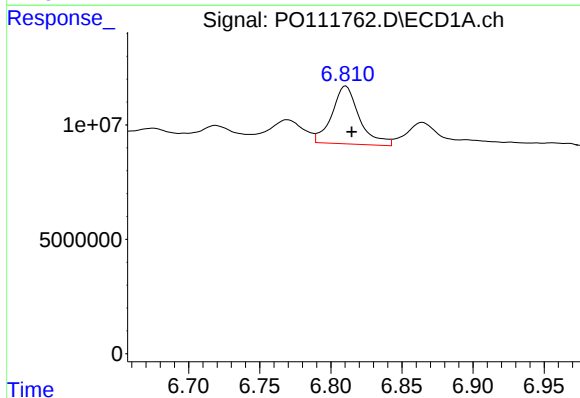


#36 AR-1262-1

R.T.: 6.811 min
Delta R.T.: -0.004 min
Response: 34055000
Conc: 55.84 ng/ml

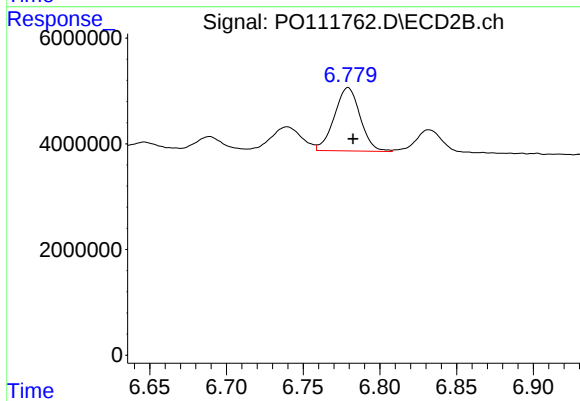

#36 AR-1262-1


R.T.: 6.779 min
Delta R.T.: -0.003 min
Response: 14119480
Conc: 41.82 ng/ml

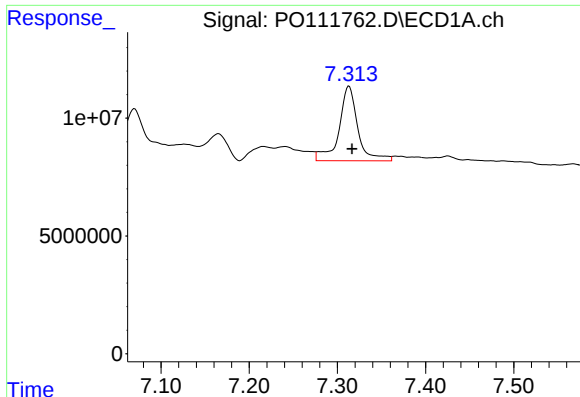

#37 AR-1262-2


R.T.: 7.313 min
Delta R.T.: -0.004 min
Response: 47025798
Conc: 49.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

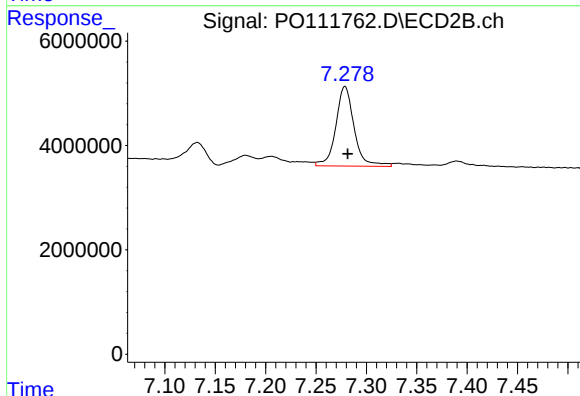


#37 AR-1262-2

R.T.: 7.279 min
Delta R.T.: -0.003 min
Response: 19273982
Conc: 41.38 ng/ml

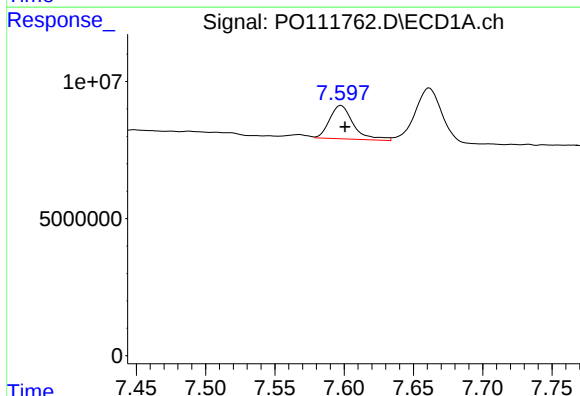


#38 AR-1262-3

R.T.: 7.598 min
Delta R.T.: -0.003 min
Response: 14529512
Conc: 36.63 ng/ml

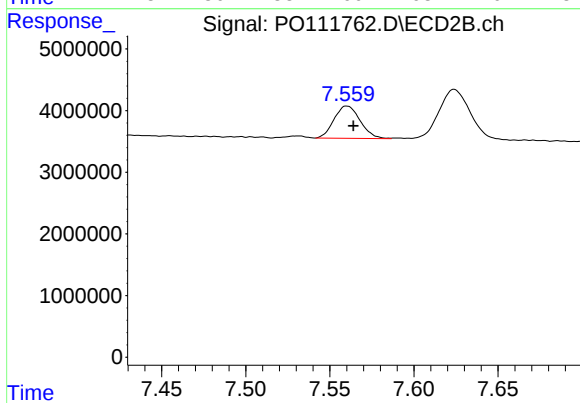

#38 AR-1262-3


R.T.: 7.560 min
Delta R.T.: -0.004 min
Response: 5666698
Conc: 34.08 ng/ml

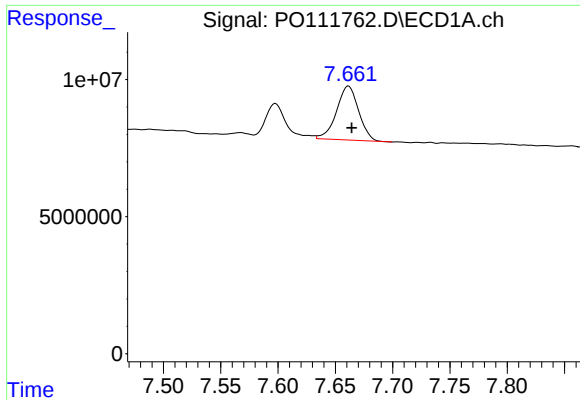

#39 AR-1262-4


R.T.: 7.662 min
Delta R.T.: -0.003 min
Response: 26490168
Conc: 40.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

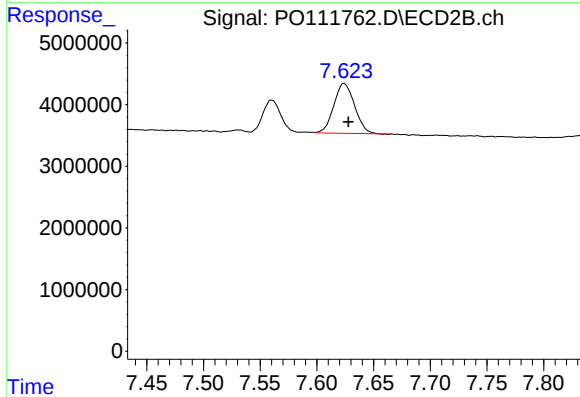


#39 AR-1262-4

R.T.: 7.624 min
Delta R.T.: -0.004 min
Response: 10281568
Conc: 37.11 ng/ml

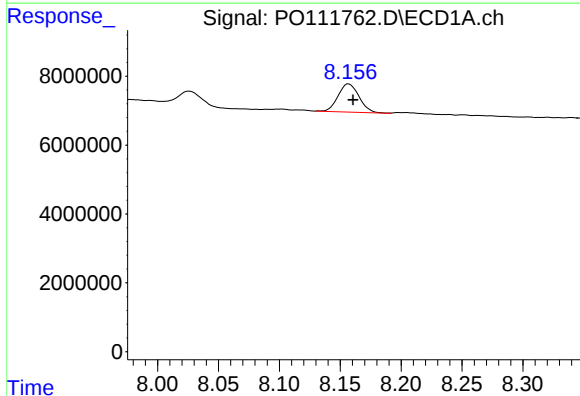


#40 AR-1262-5

R.T.: 8.157 min
Delta R.T.: -0.004 min
Response: 9899798
Conc: 32.49 ng/ml

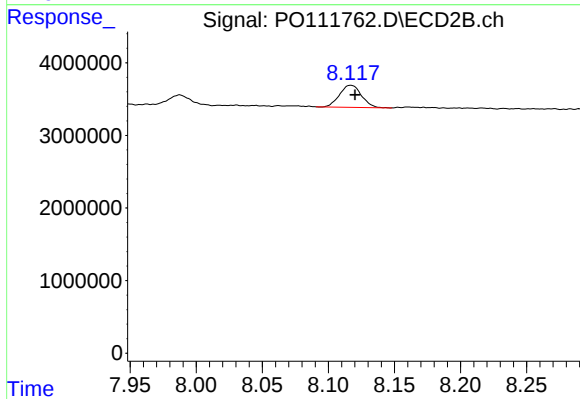

#40 AR-1262-5


R.T.: 8.117 min
Delta R.T.: -0.003 min
Response: 3482969
Conc: 34.27 ng/ml

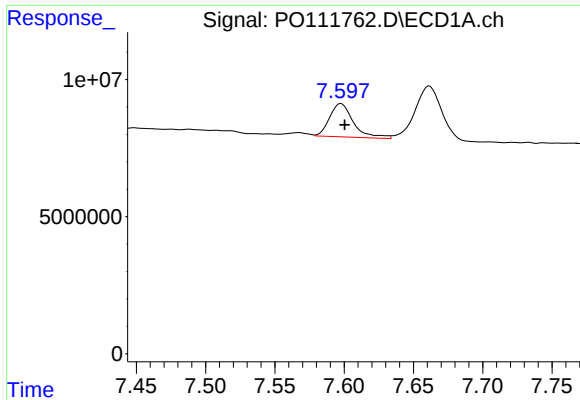

#41 AR-1268-1


R.T.: 7.598 min
Delta R.T.: -0.003 min
Response: 14529512
Conc: 12.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

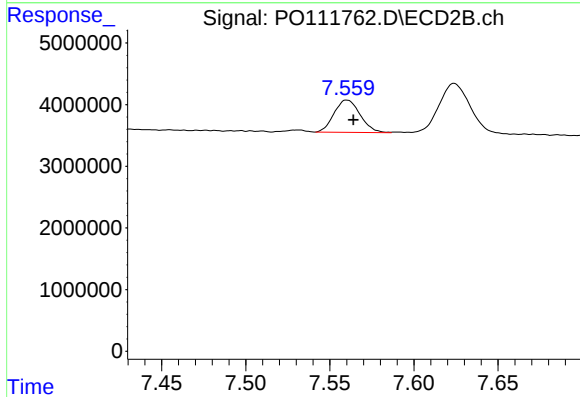


#41 AR-1268-1

R.T.: 7.560 min
Delta R.T.: -0.004 min
Response: 5666698
Conc: 11.84 ng/ml

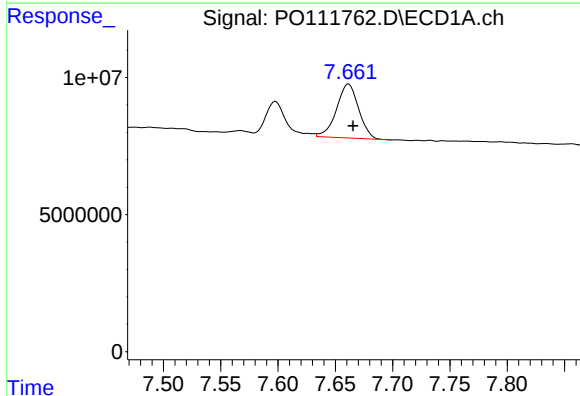


#42 AR-1268-2

R.T.: 7.662 min
Delta R.T.: -0.004 min
Response: 26490168
Conc: 27.11 ng/ml

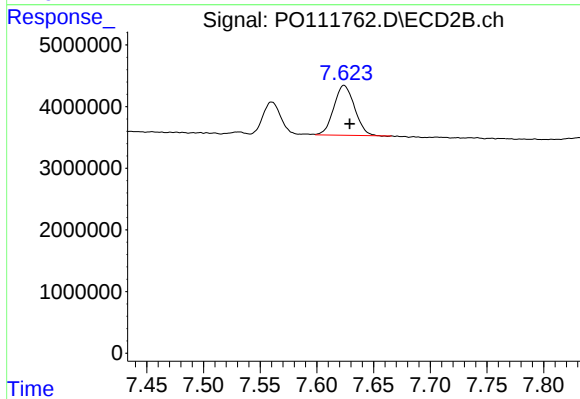

#42 AR-1268-2


R.T.: 7.624 min
Delta R.T.: -0.005 min
Response: 10281568
Conc: 24.69 ng/ml

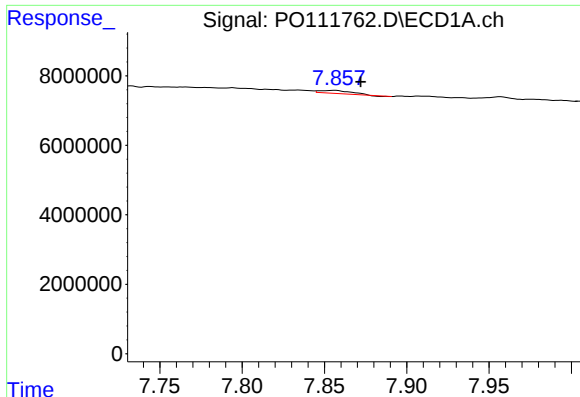

#43 AR-1268-3


R.T.: 7.857 min
Delta R.T.: -0.016 min
Response: 1111906
Conc: 1.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

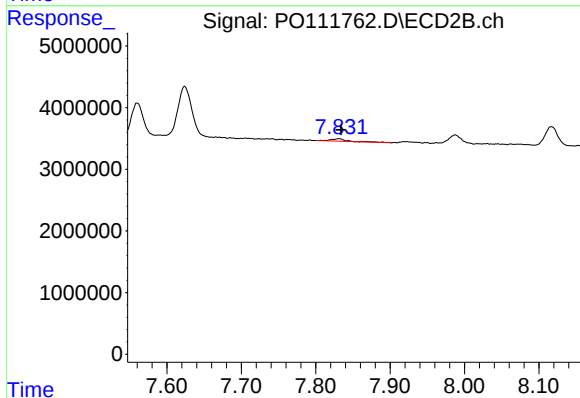


#43 AR-1268-3

R.T.: 7.832 min
Delta R.T.: -0.003 min
Response: 628662
Conc: 1.98 ng/ml

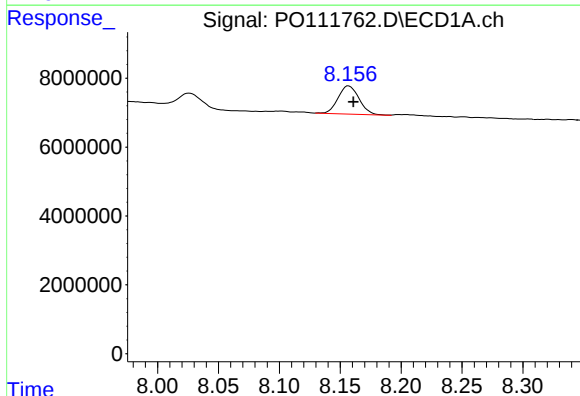


#44 AR-1268-4

R.T.: 8.157 min
Delta R.T.: -0.004 min
Response: 9899798
Conc: 28.78 ng/ml

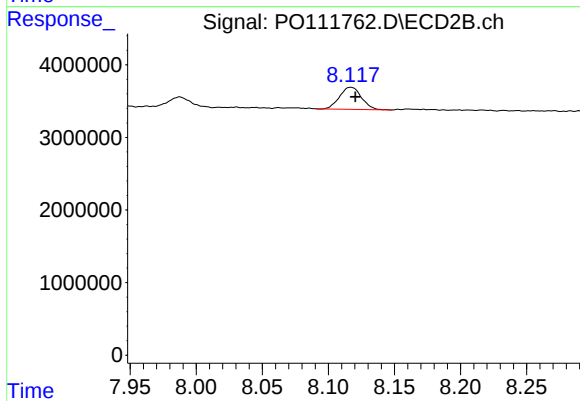

#44 AR-1268-4


R.T.: 8.117 min
Delta R.T.: -0.004 min
Response: 3482969
Conc: 30.11 ng/ml

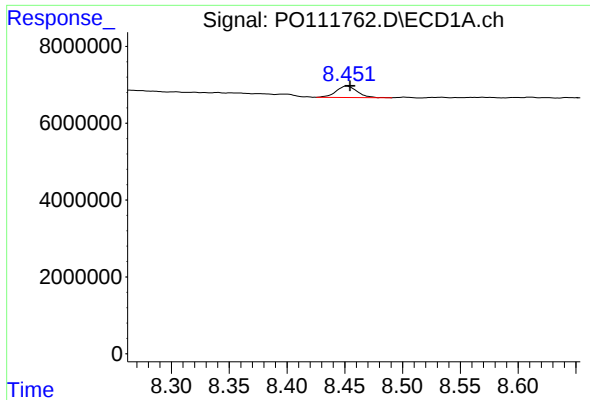

#45 AR-1268-5

R.T.: 8.452 min
Delta R.T.: -0.003 min
Response: 3764510
Conc: 1.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

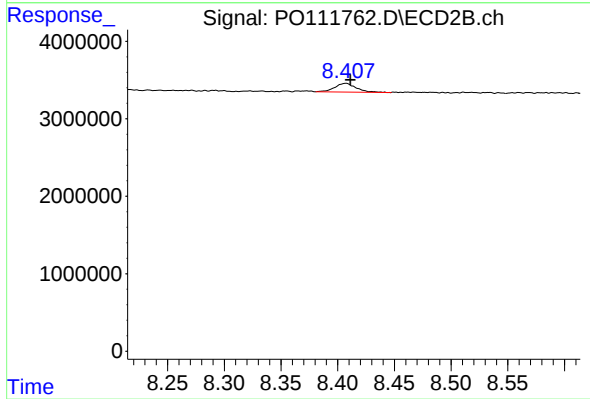

#45 AR-1268-5

R.T.: 8.407 min
Delta R.T.: -0.004 min
Response: 1479028
Conc: 2.04 ng/ml