

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
 Data File : P0111763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 16:21
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1268 LOD 40 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 04:08:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.678	3.673	111.9E6	97601901	19.421	17.375
2)	SA Decachlor...	8.711	8.659	109.1E6	38097640	20.790	21.431
Target Compounds							
3)	L1 AR-1016-1	4.775	4.751	1383085	1034897	5.798	5.259
4)	L1 AR-1016-2	4.775	4.771	1383085	338818	4.157	1.189 #
5)	L1 AR-1016-3	4.849	4.940	828268	141159	3.599	0.940 #
6)	L1 AR-1016-4	4.958	4.979	1417229	839162	7.642	6.890
7)	L1 AR-1016-5	5.227	5.261f	966208	1122391	5.177	7.050 #
8)	L2 AR-1221-1	3.902	3.885	499096	252012	5.732	3.375 #
9)	L2 AR-1221-2	3.979	3.972	2246112	1851699	35.004	33.096
10)	L2 AR-1221-3	4.050	4.039	118705	52641	0.609	0.306 #
11)	L3 AR-1232-1	4.050	4.039	118705	52641	0.782	0.396 #
12)	L3 AR-1232-2	4.543	4.771	1044235	338818	12.111	2.571 #
13)	L3 AR-1232-3	4.775	4.940	1383085	141159	8.491	2.042 #
14)	L3 AR-1232-4	4.958	5.054	1417229	42212	16.286	0.698 #
15)	L3 AR-1232-5	5.011	5.261f	783530	1122391	13.848	16.900
16)	L4 AR-1242-1	4.775	4.751	1383085	1034897	6.866	6.358
17)	L4 AR-1242-2	4.775	4.771	1383085	338818	4.909	1.435 #
18)	L4 AR-1242-3	4.849	4.940	828268	141159	4.166	1.124 #
19)	L4 AR-1242-4	4.958	5.054	1417229	42212	8.959	0.344 #
20)	L4 AR-1242-5	5.635	5.546	5814785	1218313	34.774	8.128 #
21)	L5 AR-1248-1	4.775	4.751	1383085	1034897	8.576	7.765
22)	L5 AR-1248-2	4.995	4.979	642006	839162	2.978	4.710 #
23)	L5 AR-1248-3	5.227	5.054	966208	42212	3.582	0.223 #
24)	L5 AR-1248-4	5.565	5.261f	2306309	1122391	5.769	4.916
25)	L5 AR-1248-5	5.635	5.594	5814785	929392	20.707	4.268 #
26)	L6 AR-1254-1	5.577	5.546	2785025	1218313	6.552	3.772 #
27)	L6 AR-1254-2	5.735	5.685	4642670	2511320	12.233	8.991 #
28)	L6 AR-1254-3	6.120	6.114	2350154	4987327	4.113	11.901 #
29)	L6 AR-1254-4	6.333	6.306	14810281	2794751	42.451	12.268 #
30)	L6 AR-1254-5	6.777	6.727	2752997	183617	5.376	0.564 #
31)	L7 AR-1260-1	6.243	6.210	11221497	6315851	31.581	25.171
32)	L7 AR-1260-2	6.443	6.411	27554718	5092830	58.320	17.322 #
33)	L7 AR-1260-3	6.812	6.542	17026604	1196625	40.093	4.479 #
34)	L7 AR-1260-4	7.069	7.034	24535130	5977672	78.026	31.445 #
35)	L7 AR-1260-5	7.314	7.278	11247933	3432251	13.655	8.076 #
36)	L8 AR-1262-1	6.812	6.778	17026604	5059418	27.918	14.984 #
37)	L8 AR-1262-2	7.314	7.278	11247933	3432251	11.948	7.369 #
38)	L8 AR-1262-3	7.598	7.561	34983286	14296753	88.203	85.977
39)	L8 AR-1262-4	7.663	7.626	29900722	12731956	45.511	45.952
40)	L8 AR-1262-5	8.158	8.117	10401226	3264969	34.140	32.129
41)	L9 AR-1268-1	7.598	7.561	34983286	14296753	31.053	29.884

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
Data File : P0111763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 16:21
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1268 LOD 40 PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 04:08:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.663	7.626	29900722	12731956	30.597	30.569
43)	L9 AR-1268-3	7.869	7.830	24277997	9618205	29.621	30.346
44)	L9 AR-1268-4	8.158	8.117	10401226	3264969	30.238	28.230
45)	L9 AR-1268-5	8.454	8.407	62056622	21554160	27.948	29.744



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062025\
Data File : PO111763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 16:21
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1268 LOD 40 PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 04:08:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

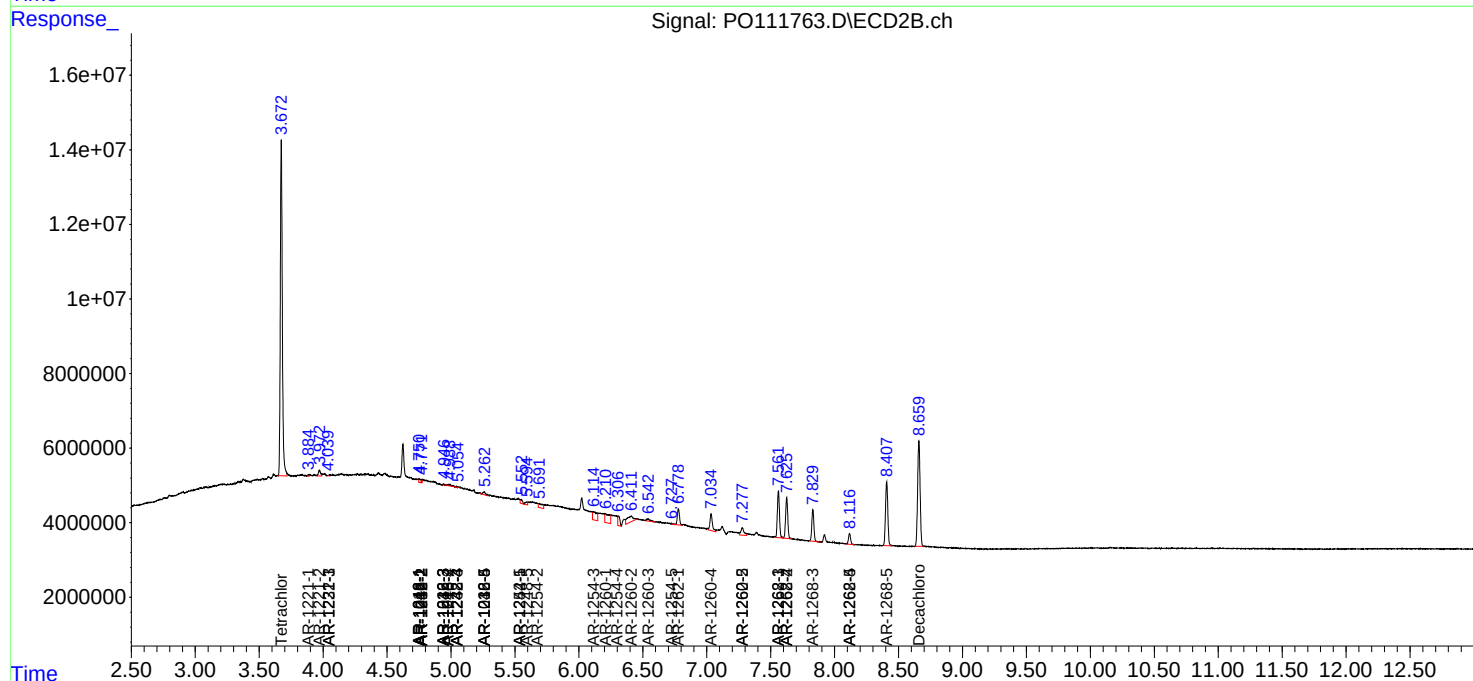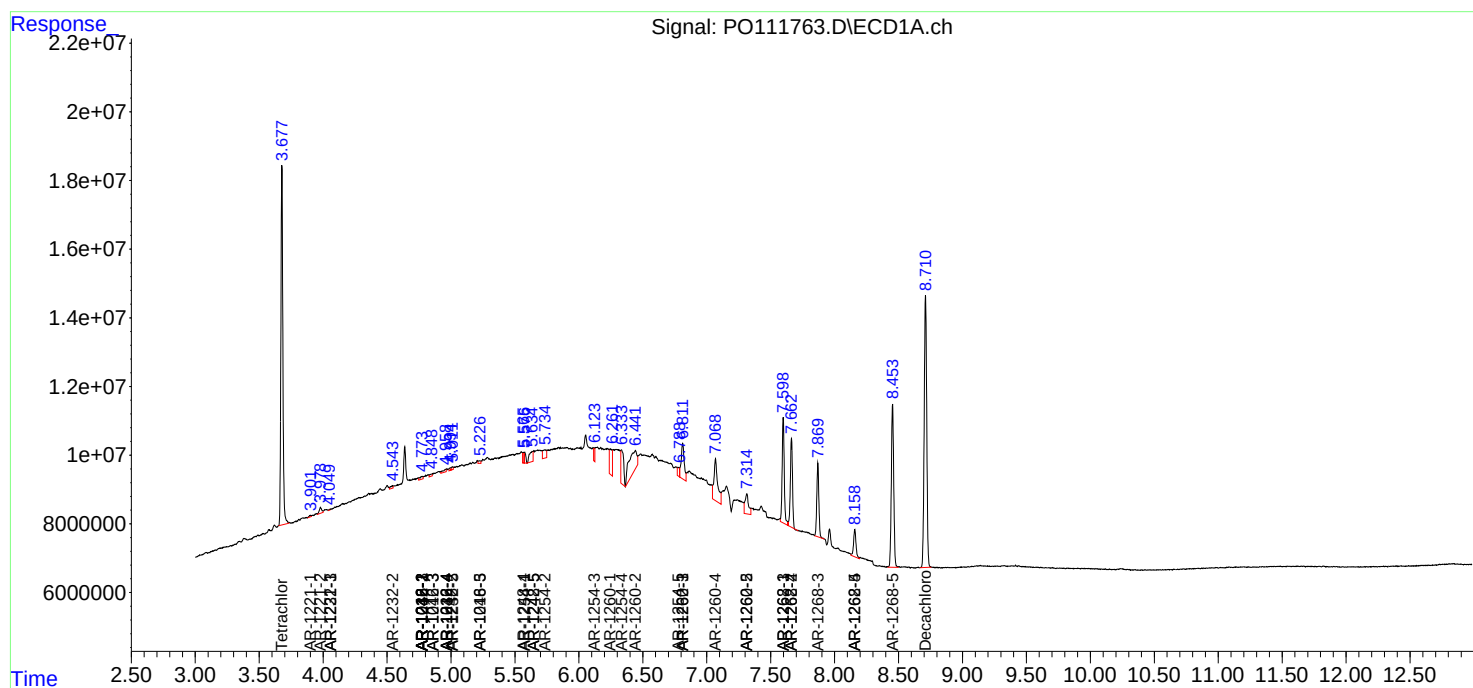


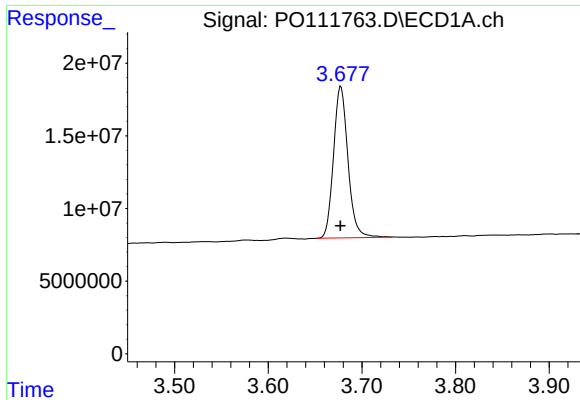

#1 Tetrachloro-m-xylene


R.T.: 3.678 min
Delta R.T.: 0.000 min
Response: 111850861
Conc: 19.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

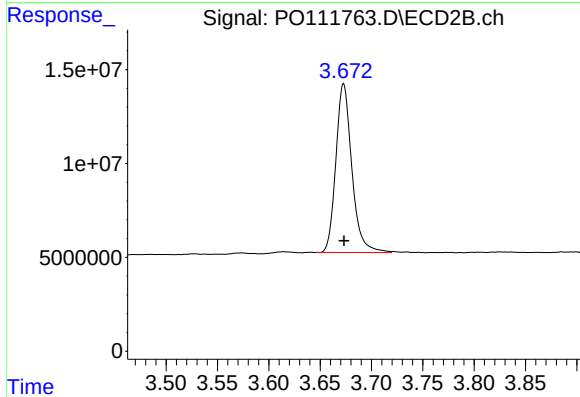


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 97601901
Conc: 17.38 ng/ml

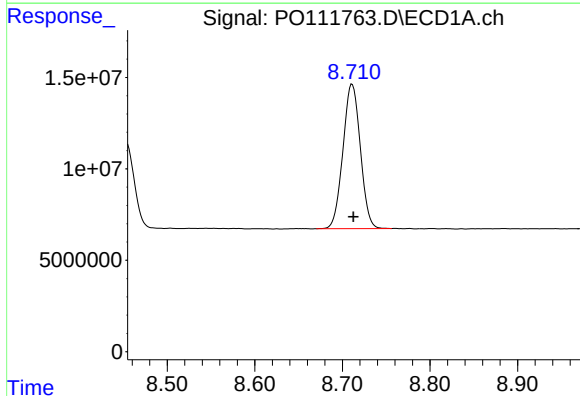


#2 Decachlorobiphenyl

R.T.: 8.711 min
Delta R.T.: -0.001 min
Response: 109134048
Conc: 20.79 ng/ml

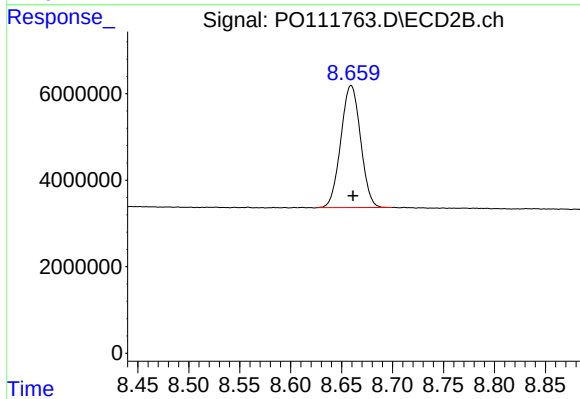

#2 Decachlorobiphenyl


R.T.: 8.659 min
Delta R.T.: -0.002 min
Response: 38097640
Conc: 21.43 ng/ml

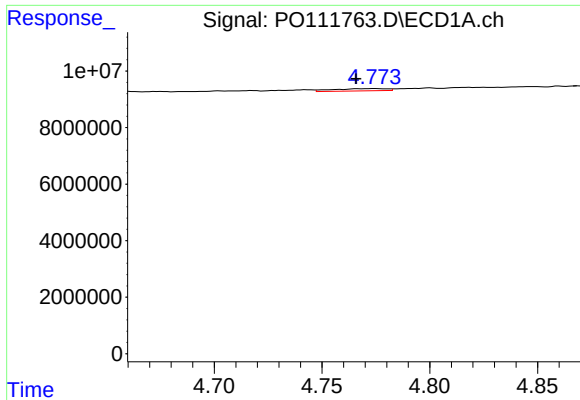

#3 AR-1016-1


R.T.: 4.775 min
Delta R.T.: 0.009 min
Response: 1383085
Conc: 5.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

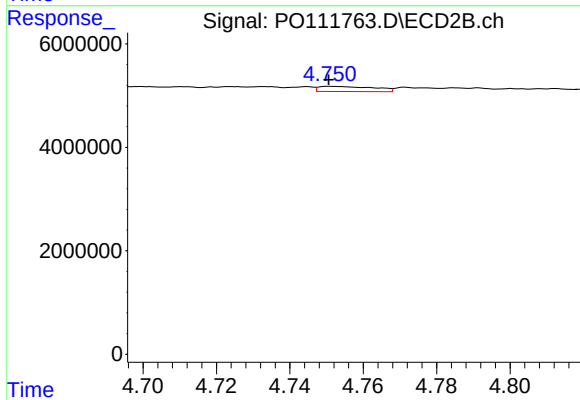


#3 AR-1016-1

R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 1034897
Conc: 5.26 ng/ml

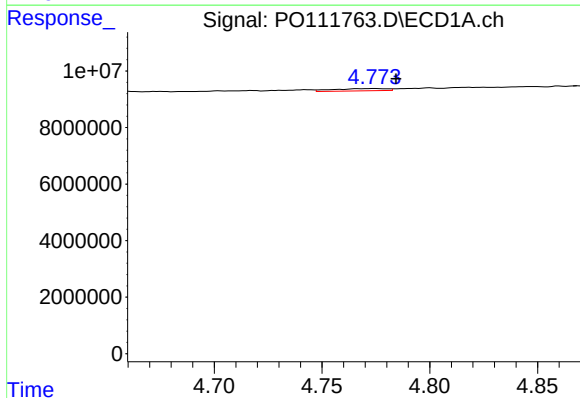


#4 AR-1016-2

R.T.: 4.775 min
Delta R.T.: -0.010 min
Response: 1383085
Conc: 4.16 ng/ml

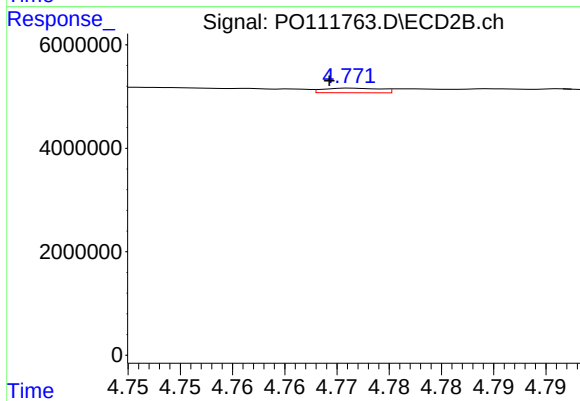

#4 AR-1016-2


R.T.: 4.771 min
Delta R.T.: 0.002 min
Response: 338818
Conc: 1.19 ng/ml

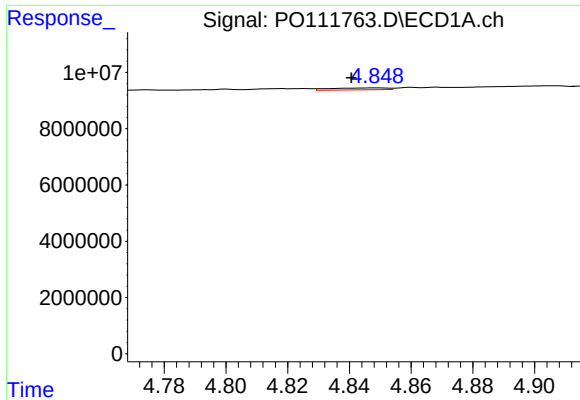

#5 AR-1016-3


R.T.: 4.849 min
Delta R.T.: 0.008 min
Response: 828268
Conc: 3.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

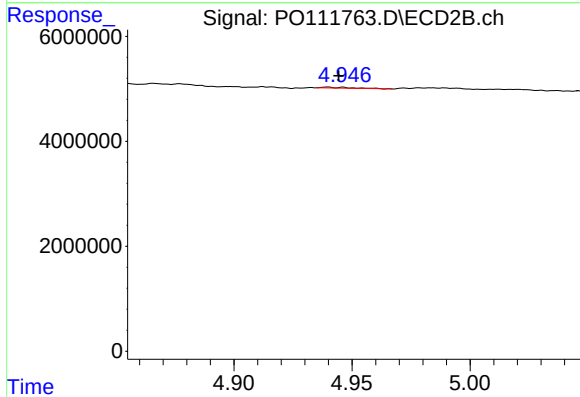


#5 AR-1016-3

R.T.: 4.940 min
Delta R.T.: -0.005 min
Response: 141159
Conc: 0.94 ng/ml

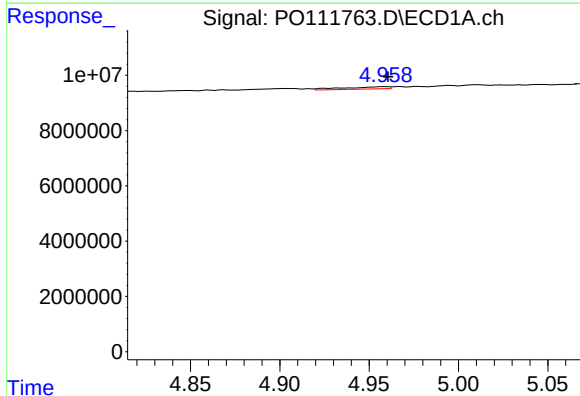


#6 AR-1016-4

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 1417229
Conc: 7.64 ng/ml

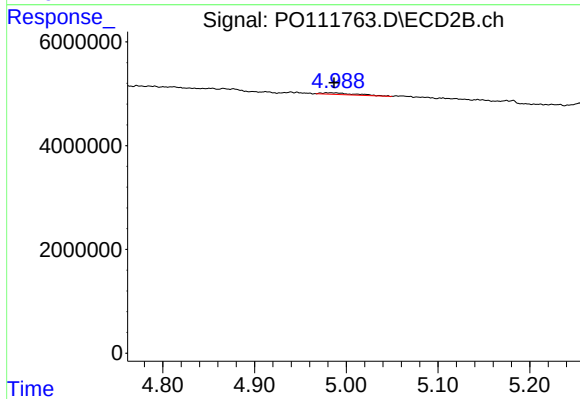

#6 AR-1016-4


R.T.: 4.979 min
Delta R.T.: -0.008 min
Response: 839162
Conc: 6.89 ng/ml

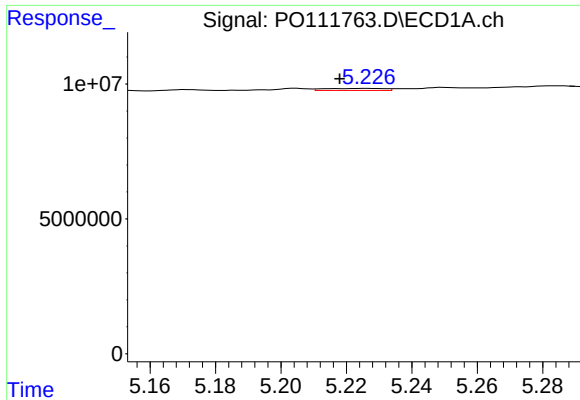

#7 AR-1016-5


R.T.: 5.227 min
Delta R.T.: 0.009 min
Response: 966208
Conc: 5.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

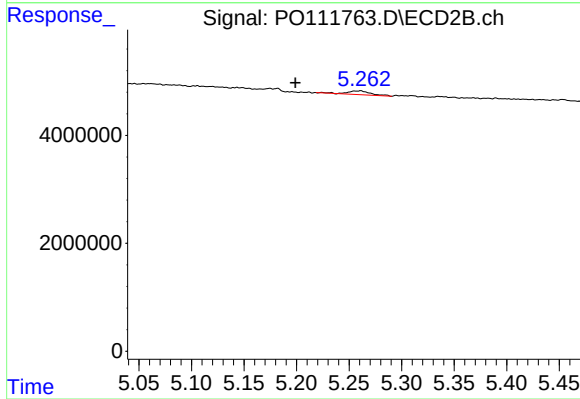


#7 AR-1016-5

R.T.: 5.261 min
Delta R.T.: 0.062 min
Response: 1122391
Conc: 7.05 ng/ml

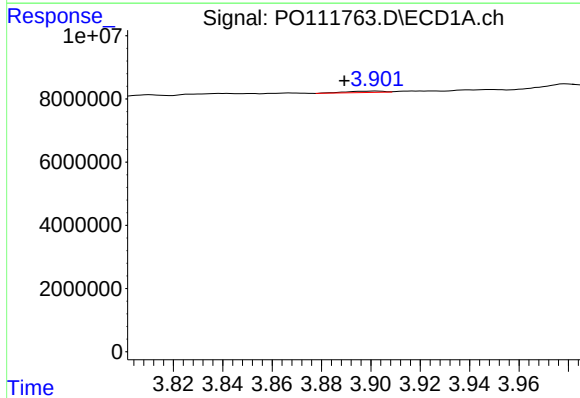


#8 AR-1221-1

R.T.: 3.902 min
Delta R.T.: 0.013 min
Response: 499096
Conc: 5.73 ng/ml

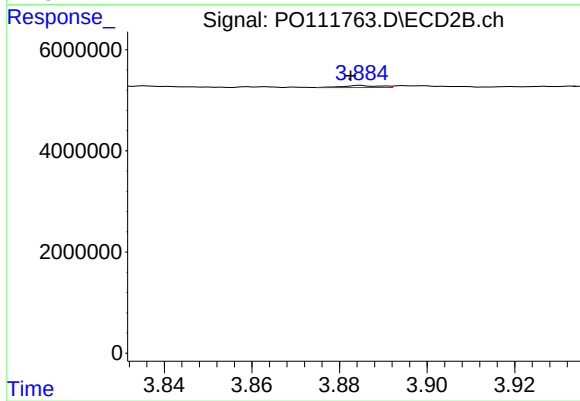

#8 AR-1221-1


R.T.: 3.885 min
Delta R.T.: 0.002 min
Response: 252012
Conc: 3.37 ng/ml

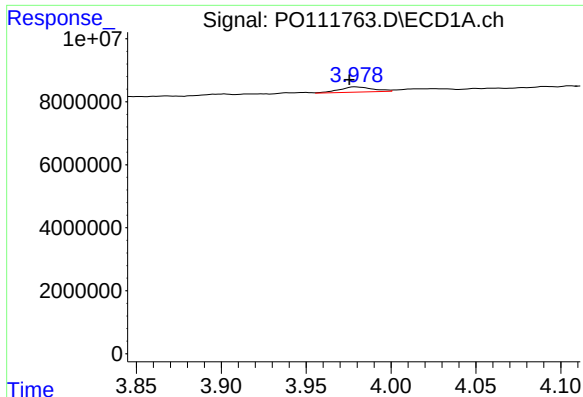

#9 AR-1221-2


R.T.: 3.979 min
Delta R.T.: 0.004 min
Response: 2246112
Conc: 35.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

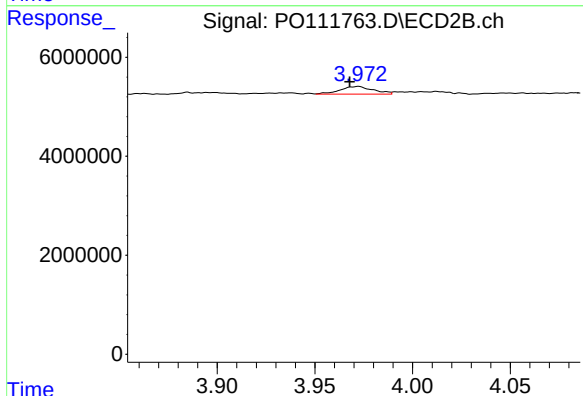


#9 AR-1221-2

R.T.: 3.972 min
Delta R.T.: 0.005 min
Response: 1851699
Conc: 33.10 ng/ml

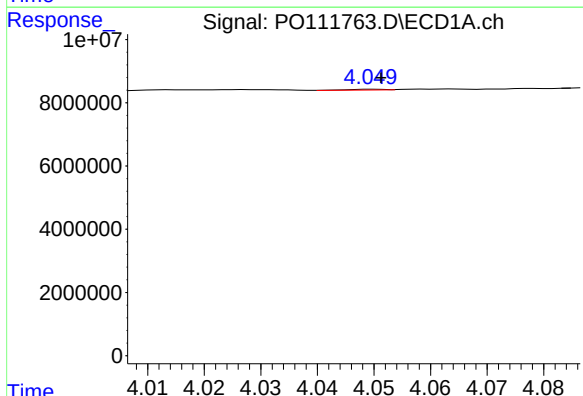


#10 AR-1221-3

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 118705
Conc: 0.61 ng/ml

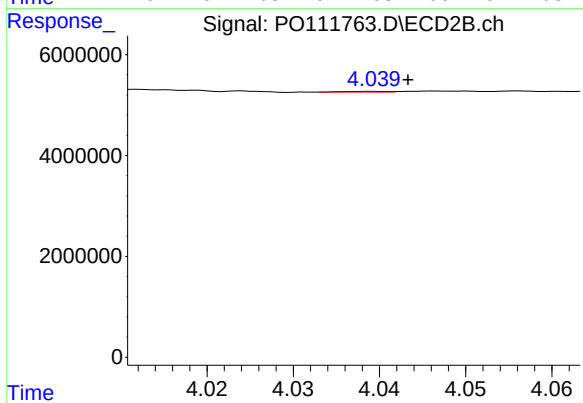

#10 AR-1221-3


R.T.: 4.039 min
Delta R.T.: -0.004 min
Response: 52641
Conc: 0.31 ng/ml

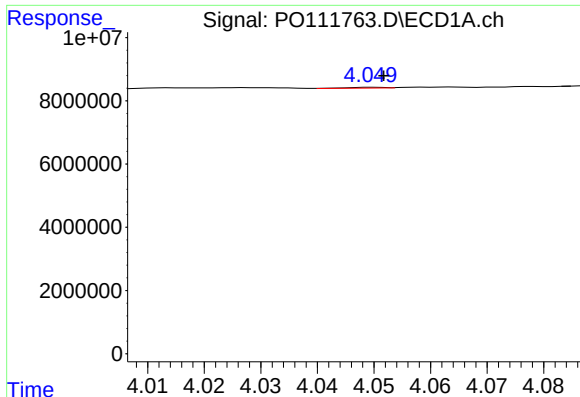

#11 AR-1232-1


R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 118705
Conc: 0.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

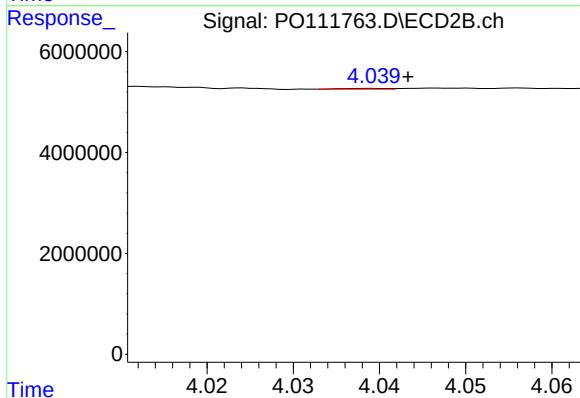


#11 AR-1232-1

R.T.: 4.039 min
Delta R.T.: -0.004 min
Response: 52641
Conc: 0.40 ng/ml

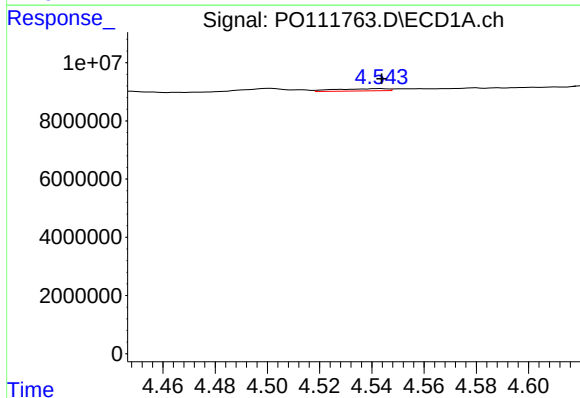


#12 AR-1232-2

R.T.: 4.543 min
Delta R.T.: 0.000 min
Response: 1044235
Conc: 12.11 ng/ml

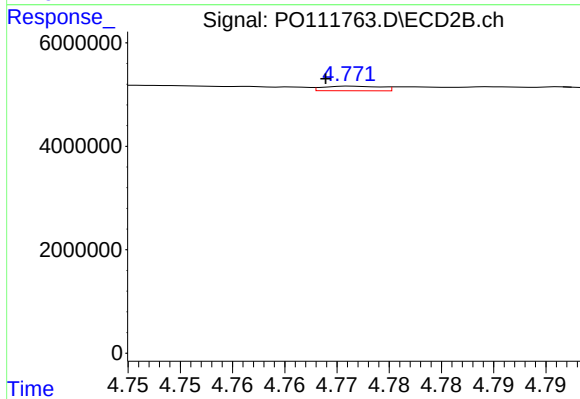

#12 AR-1232-2


R.T.: 4.771 min
Delta R.T.: 0.003 min
Response: 338818
Conc: 2.57 ng/ml

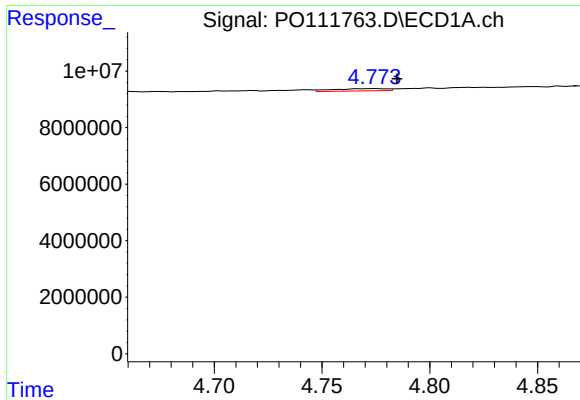

#13 AR-1232-3


R.T.: 4.775 min
Delta R.T.: -0.010 min
Response: 1383085
Conc: 8.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

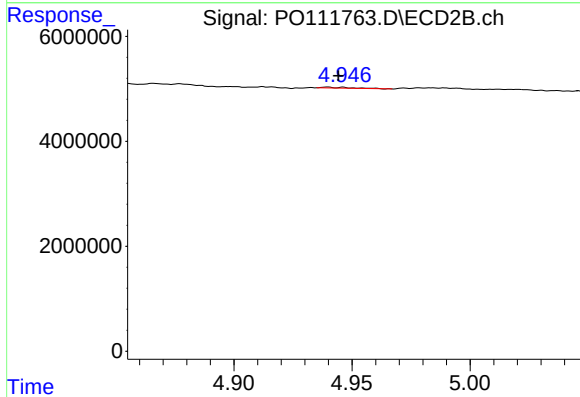


#13 AR-1232-3

R.T.: 4.940 min
Delta R.T.: -0.005 min
Response: 141159
Conc: 2.04 ng/ml

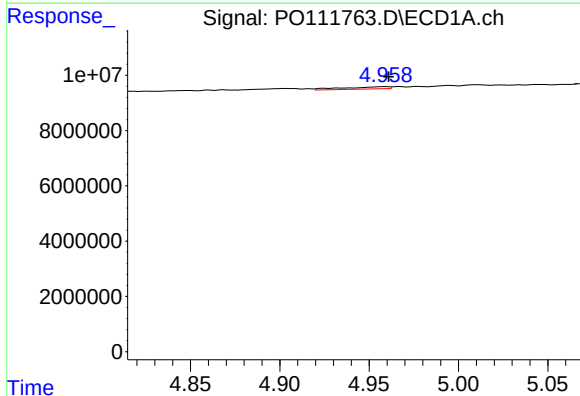


#14 AR-1232-4

R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 1417229
Conc: 16.29 ng/ml

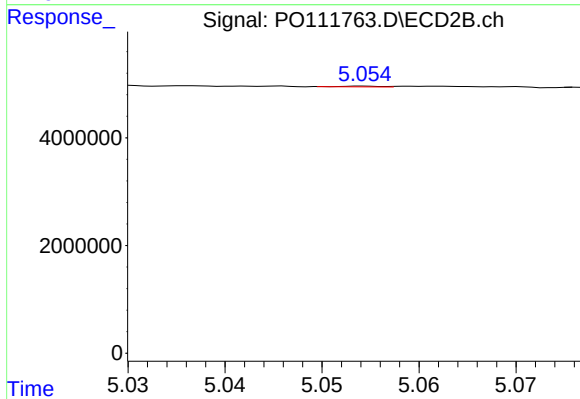

#14 AR-1232-4


R.T.: 5.054 min
Delta R.T.: 0.026 min
Response: 42212
Conc: 0.70 ng/ml

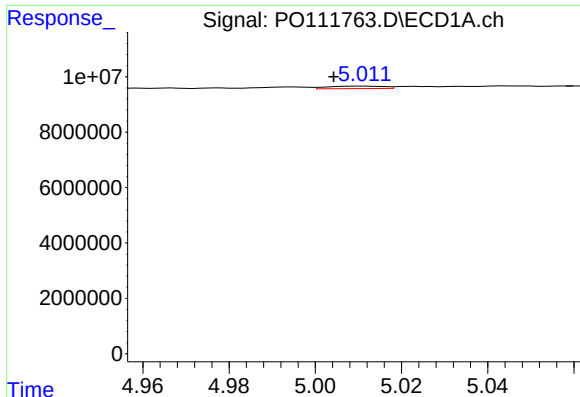

#15 AR-1232-5


R.T.: 5.011 min
Delta R.T.: 0.006 min
Response: 783530
Conc: 13.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

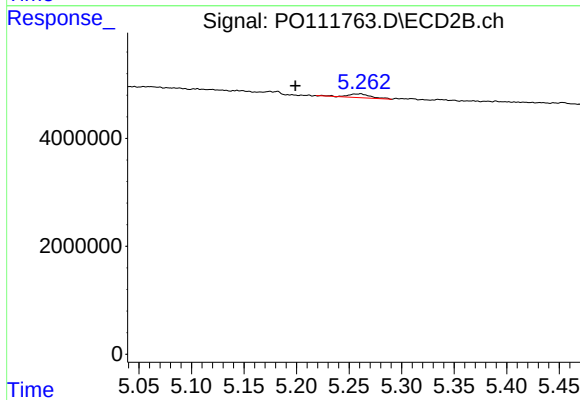


#15 AR-1232-5

R.T.: 5.261 min
Delta R.T.: 0.062 min
Response: 1122391
Conc: 16.90 ng/ml

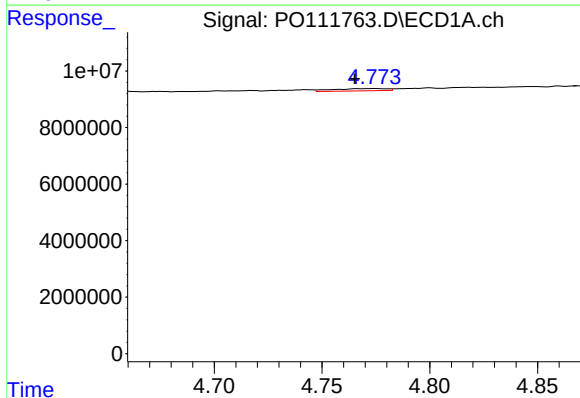


#16 AR-1242-1

R.T.: 4.775 min
Delta R.T.: 0.009 min
Response: 1383085
Conc: 6.87 ng/ml

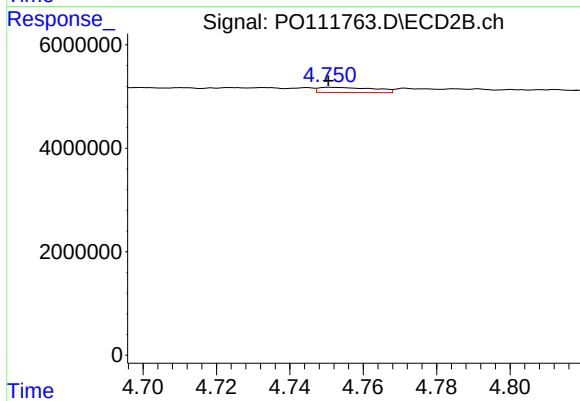

#16 AR-1242-1


R.T.: 4.751 min
Delta R.T.: 0.000 min
Response: 1034897
Conc: 6.36 ng/ml

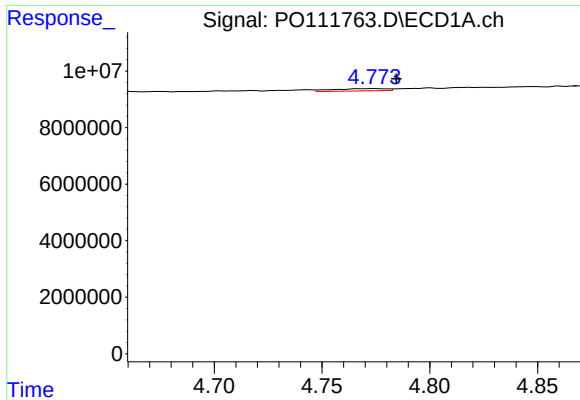

#17 AR-1242-2


R.T.: 4.775 min
Delta R.T.: -0.010 min
Response: 1383085
Conc: 4.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

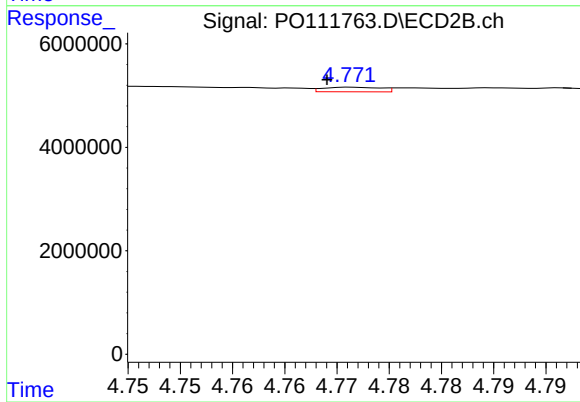


#17 AR-1242-2

R.T.: 4.771 min
Delta R.T.: 0.002 min
Response: 338818
Conc: 1.44 ng/ml

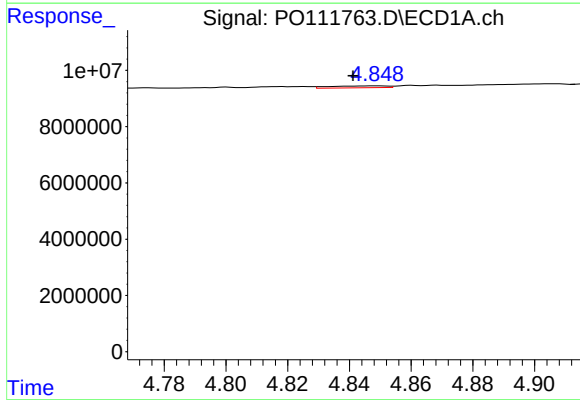


#18 AR-1242-3

R.T.: 4.849 min
Delta R.T.: 0.007 min
Response: 828268
Conc: 4.17 ng/ml

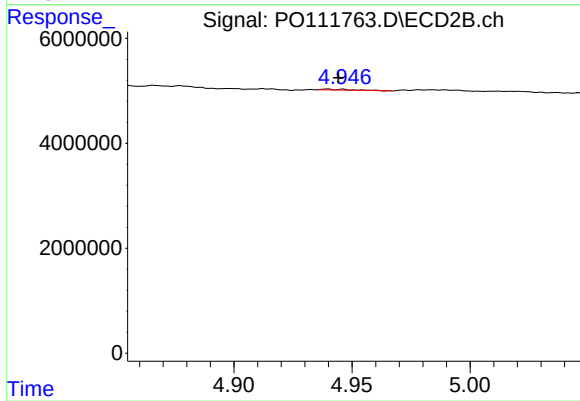

#18 AR-1242-3


R.T.: 4.940 min
Delta R.T.: -0.005 min
Response: 141159
Conc: 1.12 ng/ml

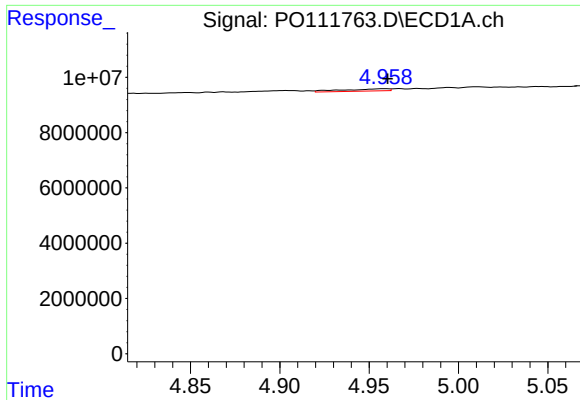

#19 AR-1242-4


R.T.: 4.958 min
Delta R.T.: -0.002 min
Response: 1417229
Conc: 8.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

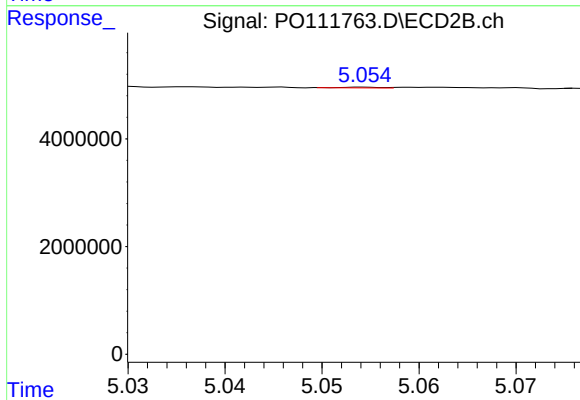


#19 AR-1242-4

R.T.: 5.054 min
Delta R.T.: 0.026 min
Response: 42212
Conc: 0.34 ng/ml

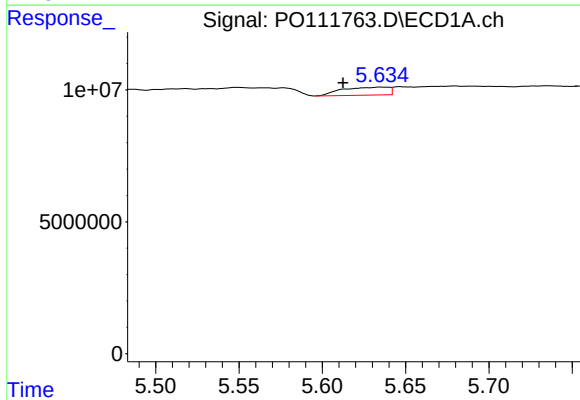


#20 AR-1242-5

R.T.: 5.635 min
Delta R.T.: 0.023 min
Response: 5814785
Conc: 34.77 ng/ml

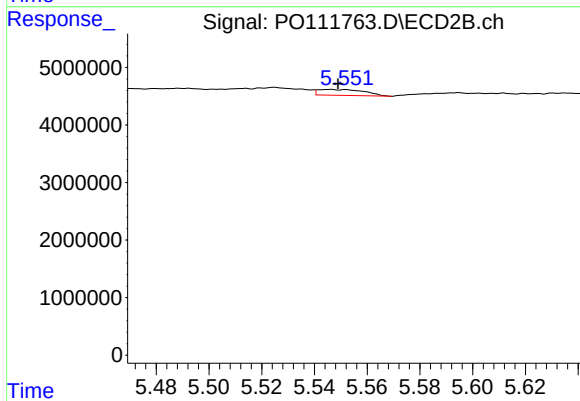

#20 AR-1242-5


R.T.: 5.546 min
Delta R.T.: -0.003 min
Response: 1218313
Conc: 8.13 ng/ml

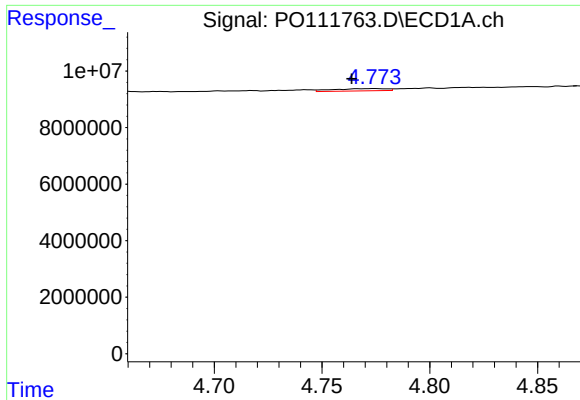

#21 AR-1248-1


R.T.: 4.775 min
Delta R.T.: 0.011 min
Response: 1383085
Conc: 8.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

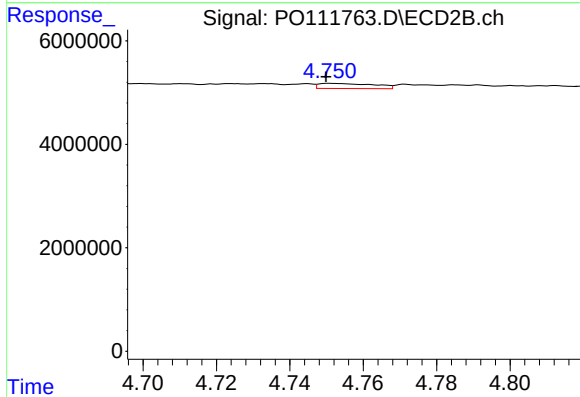


#21 AR-1248-1

R.T.: 4.751 min
Delta R.T.: 0.001 min
Response: 1034897
Conc: 7.76 ng/ml

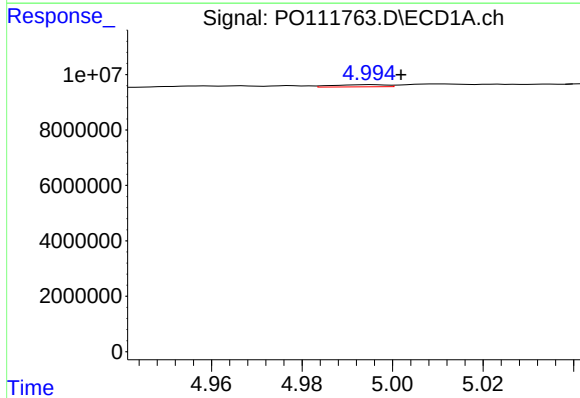


#22 AR-1248-2

R.T.: 4.995 min
Delta R.T.: -0.007 min
Response: 642006
Conc: 2.98 ng/ml

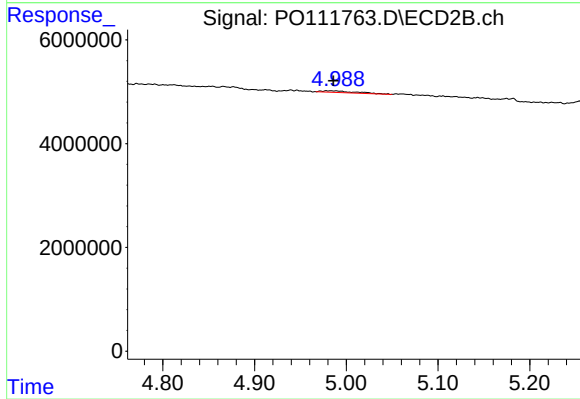

#22 AR-1248-2


R.T.: 4.979 min
Delta R.T.: -0.007 min
Response: 839162
Conc: 4.71 ng/ml

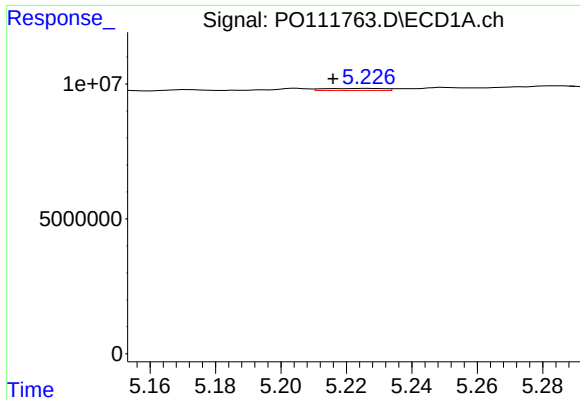

#23 AR-1248-3


R.T.: 5.227 min
Delta R.T.: 0.011 min
Response: 966208
Conc: 3.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

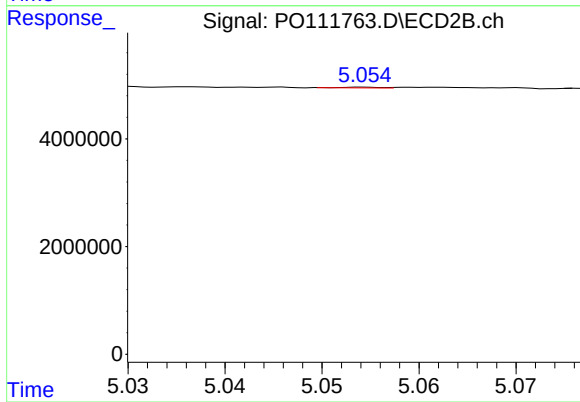


#23 AR-1248-3

R.T.: 5.054 min
Delta R.T.: 0.026 min
Response: 42212
Conc: 0.22 ng/ml

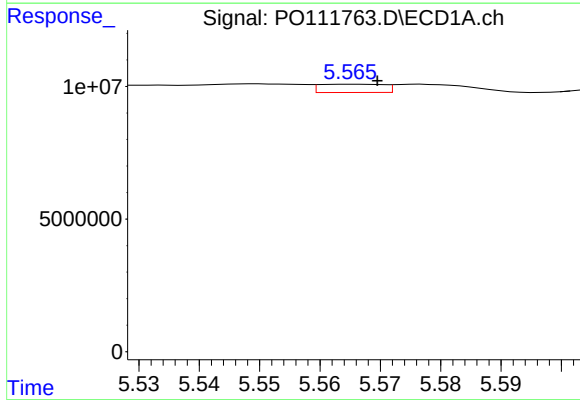


#24 AR-1248-4

R.T.: 5.565 min
Delta R.T.: -0.004 min
Response: 2306309
Conc: 5.77 ng/ml

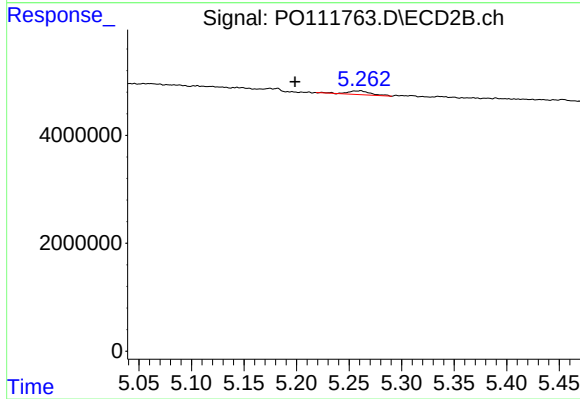

#24 AR-1248-4


R.T.: 5.261 min
Delta R.T.: 0.062 min
Response: 1122391
Conc: 4.92 ng/ml

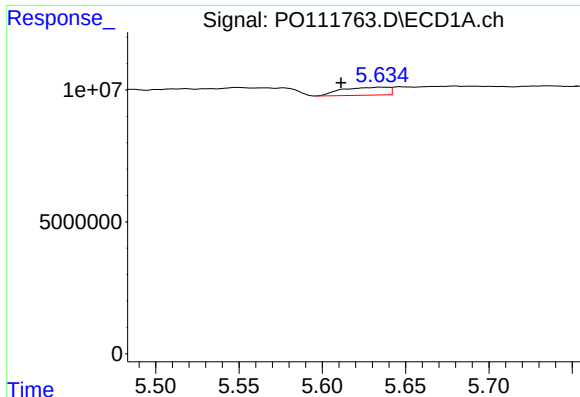

#25 AR-1248-5


R.T.: 5.635 min
Delta R.T.: 0.024 min
Response: 5814785
Conc: 20.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

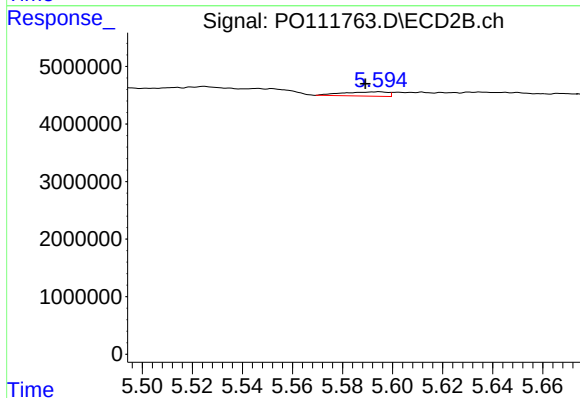


#25 AR-1248-5

R.T.: 5.594 min
Delta R.T.: 0.005 min
Response: 929392
Conc: 4.27 ng/ml

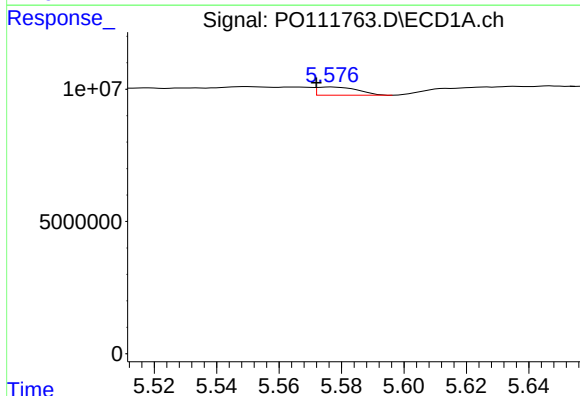


#26 AR-1254-1

R.T.: 5.577 min
Delta R.T.: 0.005 min
Response: 2785025
Conc: 6.55 ng/ml

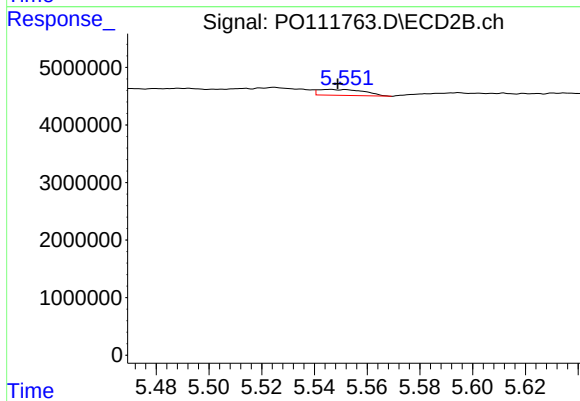

#26 AR-1254-1


R.T.: 5.546 min
Delta R.T.: -0.003 min
Response: 1218313
Conc: 3.77 ng/ml

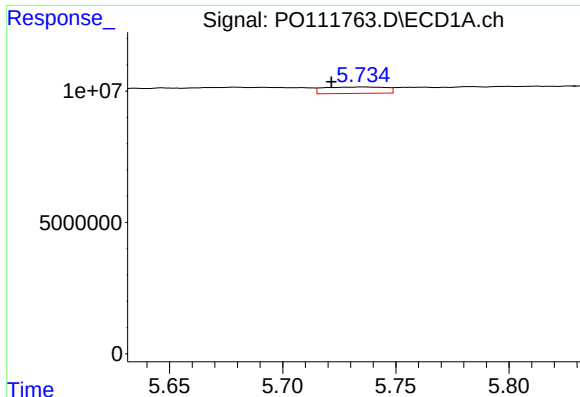

#27 AR-1254-2


R.T.: 5.735 min
Delta R.T.: 0.014 min
Response: 4642670
Conc: 12.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

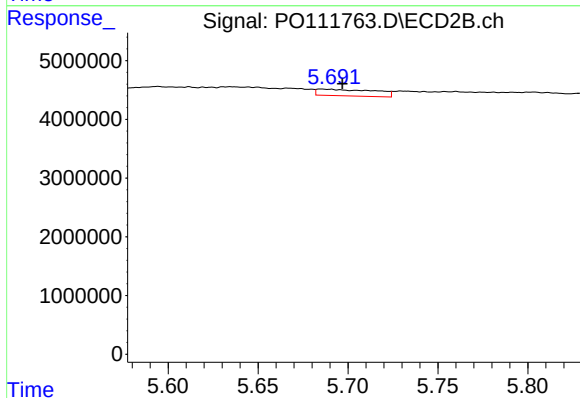


#27 AR-1254-2

R.T.: 5.685 min
Delta R.T.: -0.012 min
Response: 2511320
Conc: 8.99 ng/ml

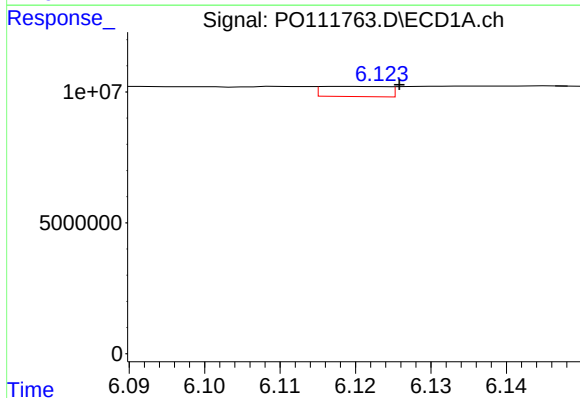


#28 AR-1254-3

R.T.: 6.120 min
Delta R.T.: -0.006 min
Response: 2350154
Conc: 4.11 ng/ml

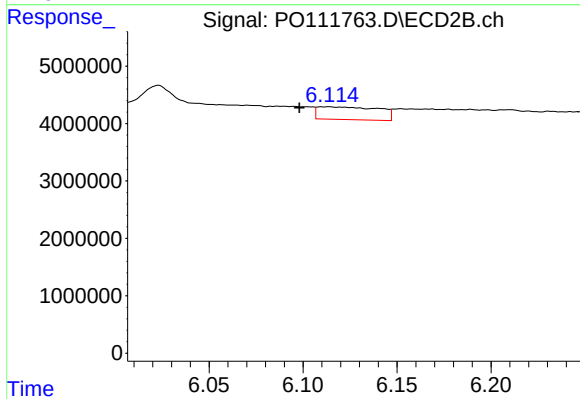

#28 AR-1254-3


R.T.: 6.114 min
Delta R.T.: 0.016 min
Response: 4987327
Conc: 11.90 ng/ml

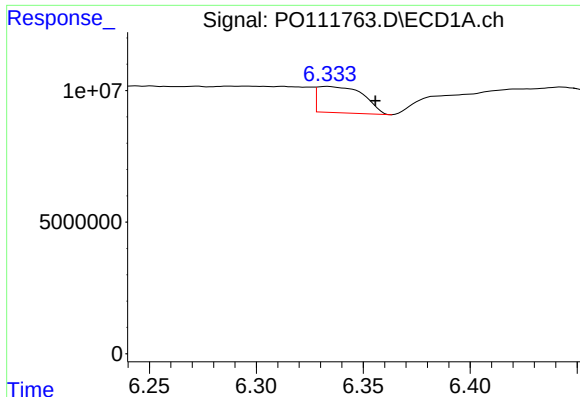

#29 AR-1254-4


R.T.: 6.333 min
Delta R.T.: -0.022 min
Response: 14810281
Conc: 42.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

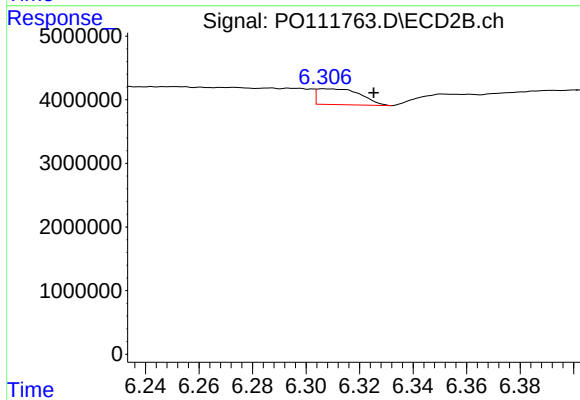


#29 AR-1254-4

R.T.: 6.306 min
Delta R.T.: -0.019 min
Response: 2794751
Conc: 12.27 ng/ml

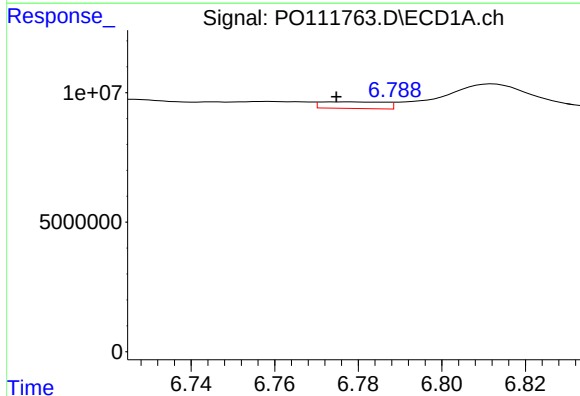


#30 AR-1254-5

R.T.: 6.777 min
Delta R.T.: 0.002 min
Response: 2752997
Conc: 5.38 ng/ml

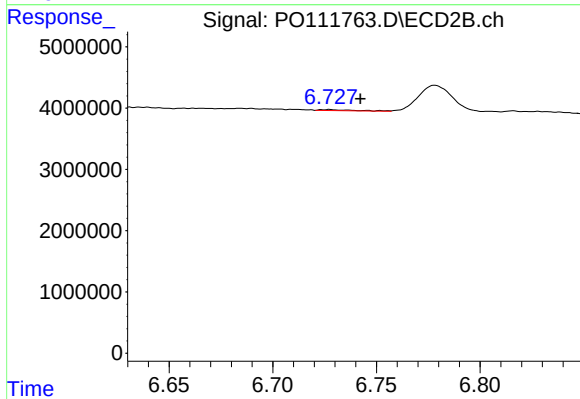

#30 AR-1254-5


R.T.: 6.727 min
Delta R.T.: -0.015 min
Response: 183617
Conc: 0.56 ng/ml

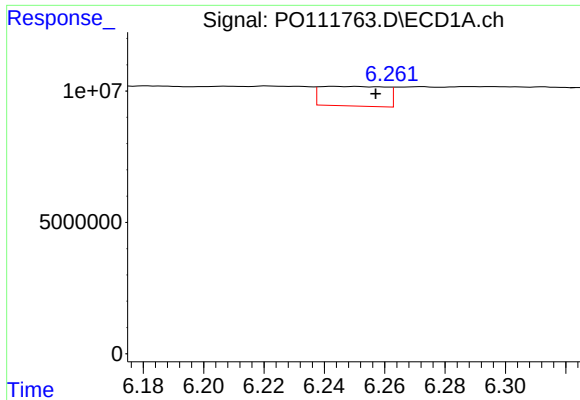

#31 AR-1260-1


R.T.: 6.243 min
Delta R.T.: -0.014 min
Response: 11221497
Conc: 31.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

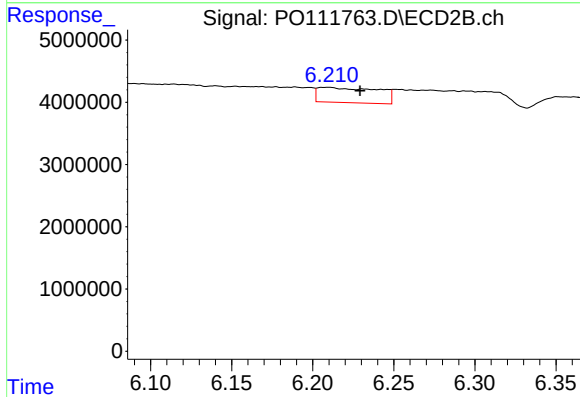


#31 AR-1260-1

R.T.: 6.210 min
Delta R.T.: -0.020 min
Response: 6315851
Conc: 25.17 ng/ml

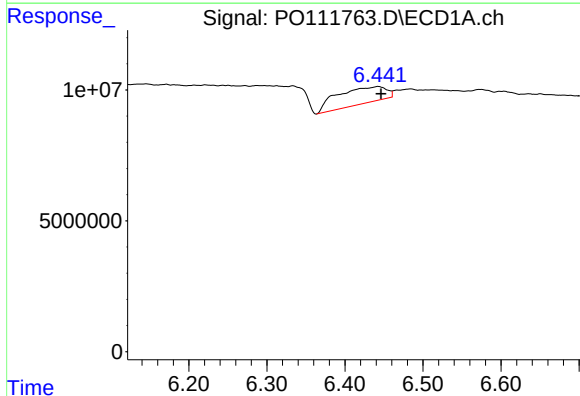


#32 AR-1260-2

R.T.: 6.443 min
Delta R.T.: -0.004 min
Response: 27554718
Conc: 58.32 ng/ml

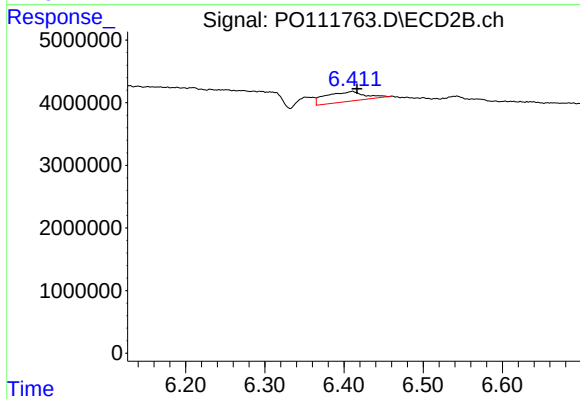

#32 AR-1260-2


R.T.: 6.411 min
Delta R.T.: -0.006 min
Response: 5092830
Conc: 17.32 ng/ml

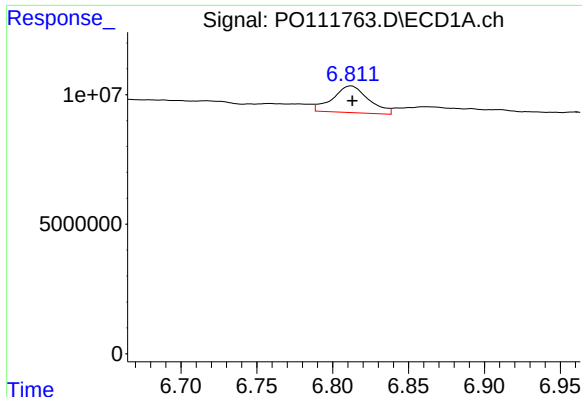

#33 AR-1260-3


R.T.: 6.812 min
Delta R.T.: 0.000 min
Response: 17026604
Conc: 40.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

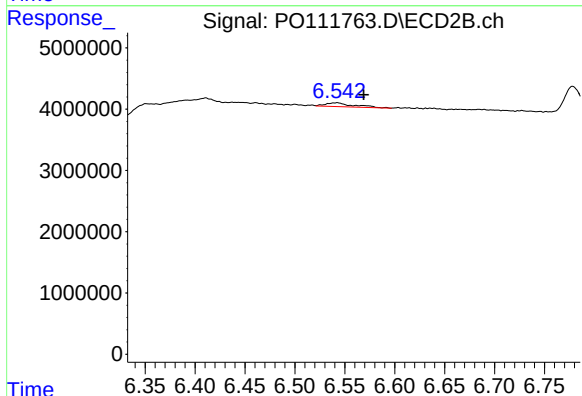


#33 AR-1260-3

R.T.: 6.542 min
Delta R.T.: -0.027 min
Response: 1196625
Conc: 4.48 ng/ml

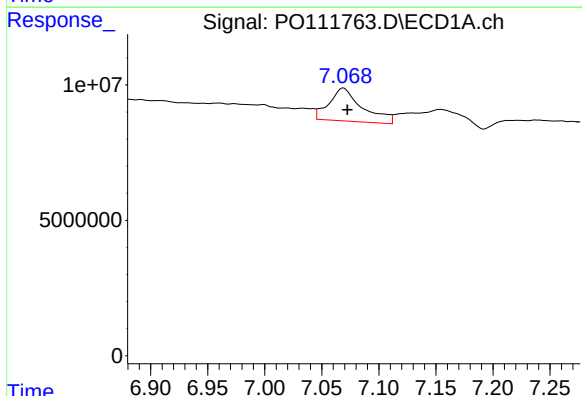


#34 AR-1260-4

R.T.: 7.069 min
Delta R.T.: -0.003 min
Response: 24535130
Conc: 78.03 ng/ml

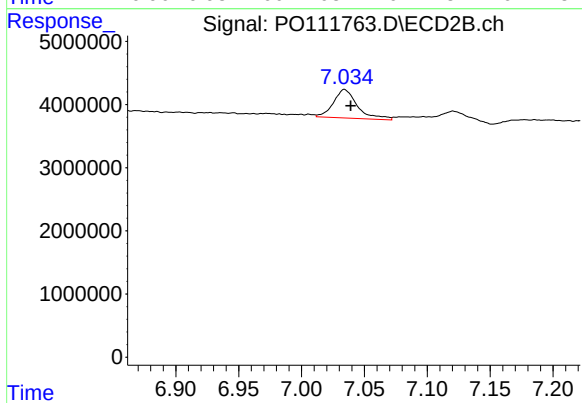

#34 AR-1260-4


R.T.: 7.034 min
Delta R.T.: -0.005 min
Response: 5977672
Conc: 31.45 ng/ml

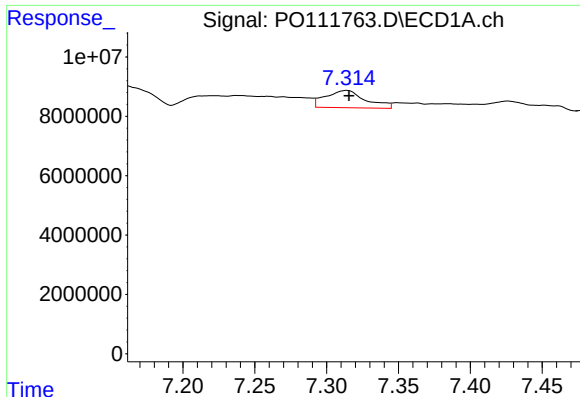

#35 AR-1260-5


R.T.: 7.314 min
Delta R.T.: -0.001 min
Response: 11247933
Conc: 13.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

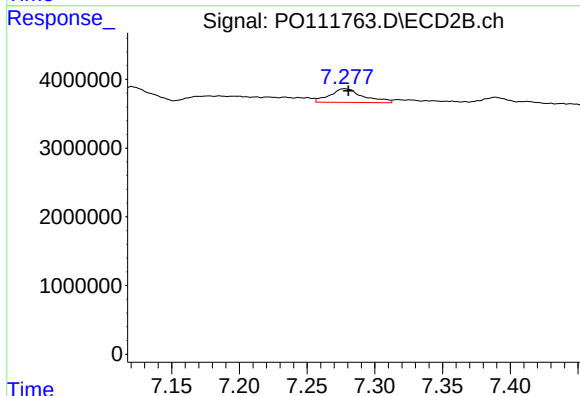


#35 AR-1260-5

R.T.: 7.278 min
Delta R.T.: -0.003 min
Response: 3432251
Conc: 8.08 ng/ml

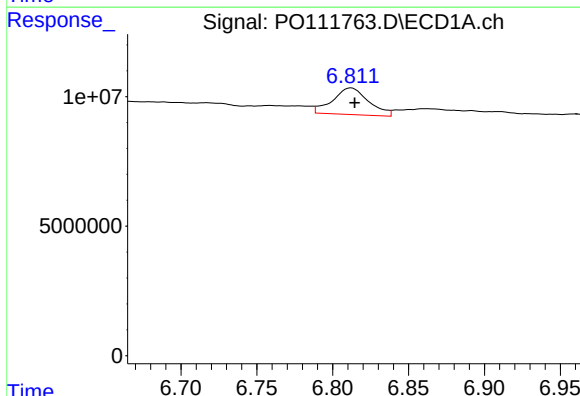


#36 AR-1262-1

R.T.: 6.812 min
Delta R.T.: -0.002 min
Response: 17026604
Conc: 27.92 ng/ml

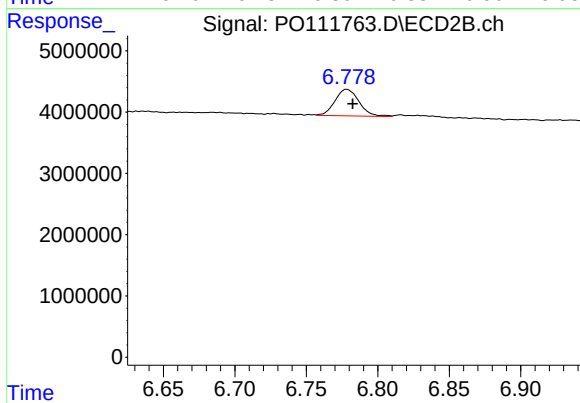

#36 AR-1262-1


R.T.: 6.778 min
Delta R.T.: -0.004 min
Response: 5059418
Conc: 14.98 ng/ml

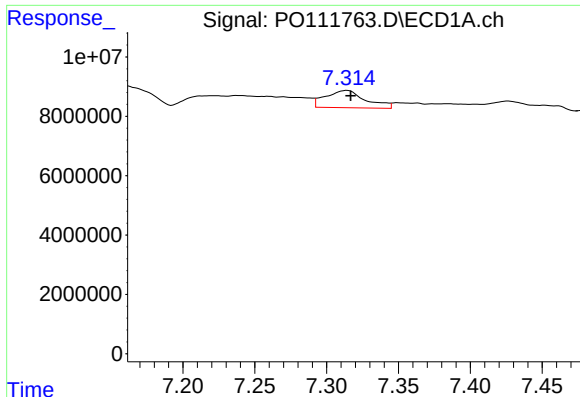

#37 AR-1262-2


R.T.: 7.314 min
Delta R.T.: -0.002 min
Response: 11247933
Conc: 11.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

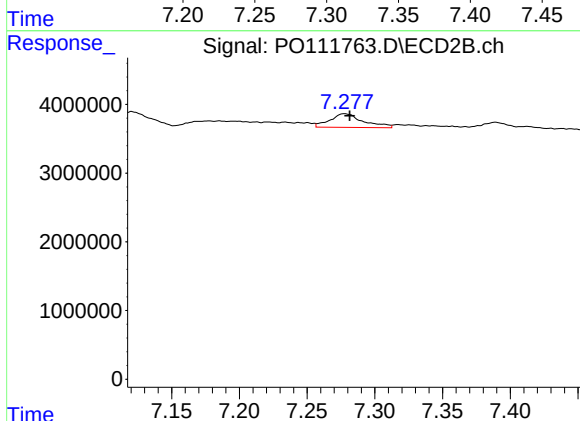


#37 AR-1262-2

R.T.: 7.278 min
Delta R.T.: -0.004 min
Response: 3432251
Conc: 7.37 ng/ml

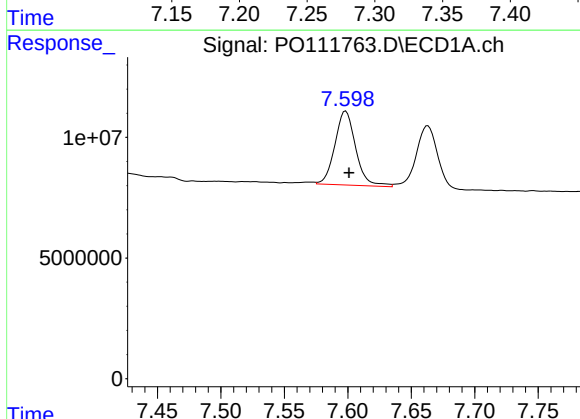


#38 AR-1262-3

R.T.: 7.598 min
Delta R.T.: -0.002 min
Response: 34983286
Conc: 88.20 ng/ml

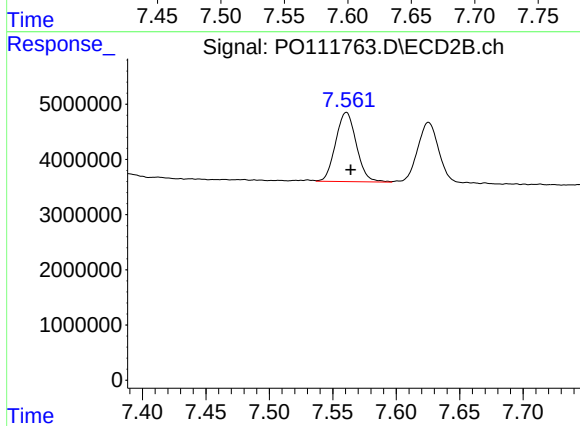

#38 AR-1262-3


R.T.: 7.561 min
Delta R.T.: -0.003 min
Response: 14296753
Conc: 85.98 ng/ml

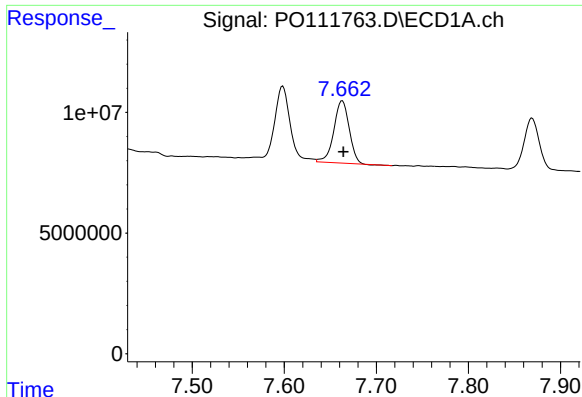

#39 AR-1262-4


R.T.: 7.663 min
Delta R.T.: -0.001 min
Response: 29900722
Conc: 45.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

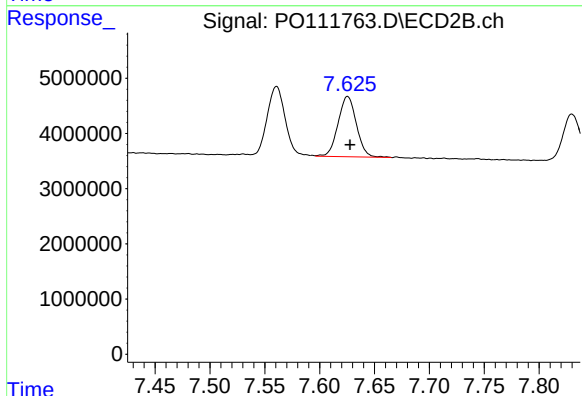


#39 AR-1262-4

R.T.: 7.626 min
Delta R.T.: -0.002 min
Response: 12731956
Conc: 45.95 ng/ml

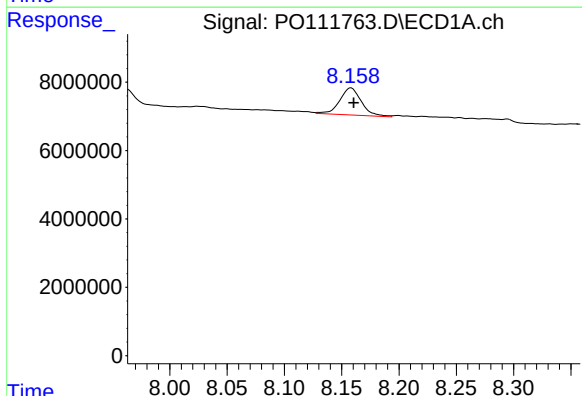


#40 AR-1262-5

R.T.: 8.158 min
Delta R.T.: -0.002 min
Response: 10401226
Conc: 34.14 ng/ml

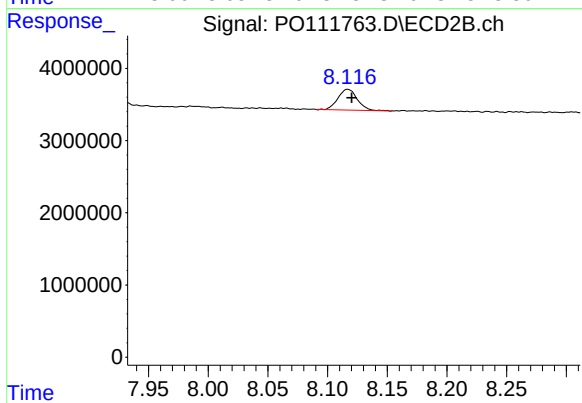

#40 AR-1262-5


R.T.: 8.117 min
Delta R.T.: -0.003 min
Response: 3264969
Conc: 32.13 ng/ml

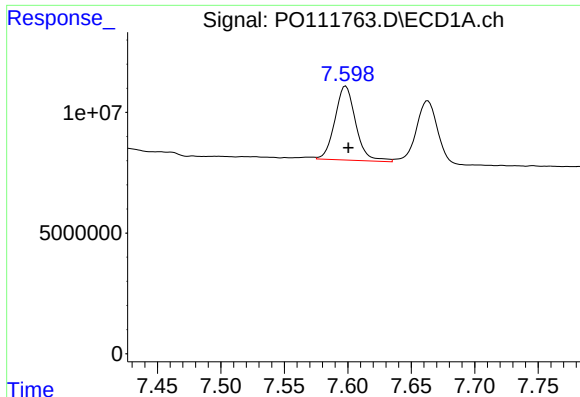

#41 AR-1268-1


R.T.: 7.598 min
Delta R.T.: -0.002 min
Response: 34983286
Conc: 31.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

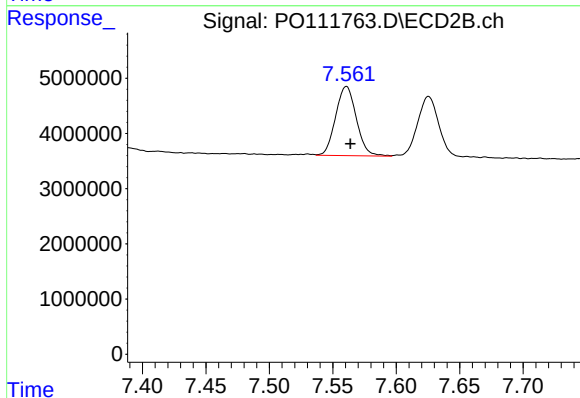


#41 AR-1268-1

R.T.: 7.561 min
Delta R.T.: -0.003 min
Response: 14296753
Conc: 29.88 ng/ml

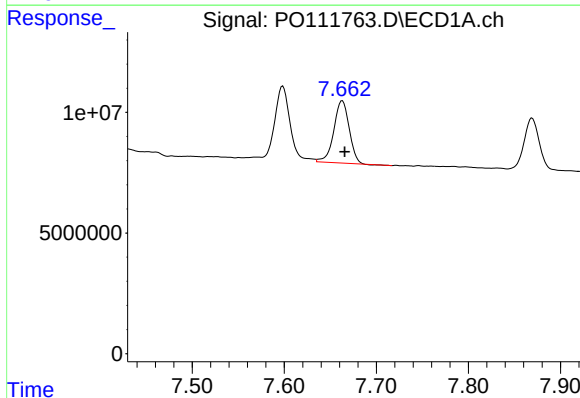


#42 AR-1268-2

R.T.: 7.663 min
Delta R.T.: -0.002 min
Response: 29900722
Conc: 30.60 ng/ml

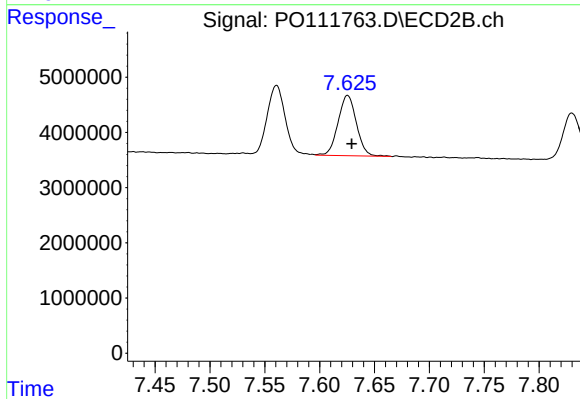

#42 AR-1268-2


R.T.: 7.626 min
Delta R.T.: -0.004 min
Response: 12731956
Conc: 30.57 ng/ml

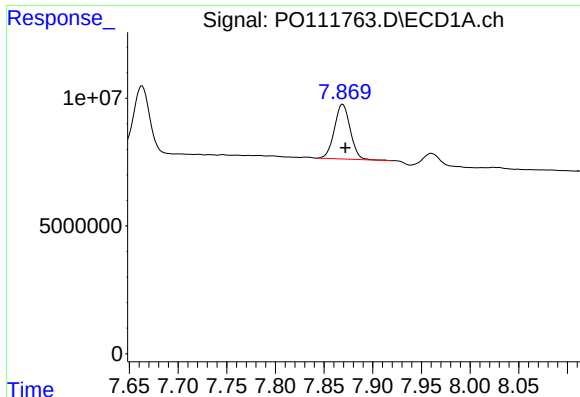

#43 AR-1268-3


R.T.: 7.869 min
Delta R.T.: -0.003 min
Response: 24277997
Conc: 29.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

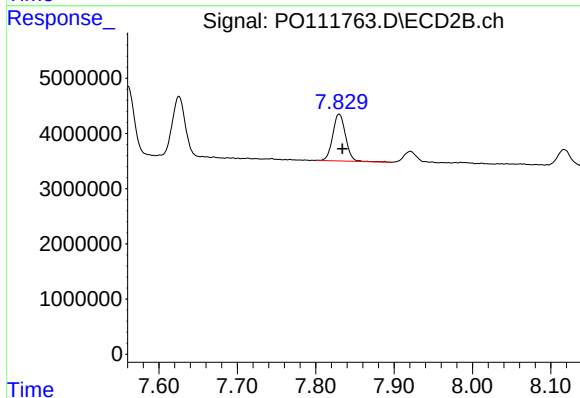


#43 AR-1268-3

R.T.: 7.830 min
Delta R.T.: -0.004 min
Response: 9618205
Conc: 30.35 ng/ml

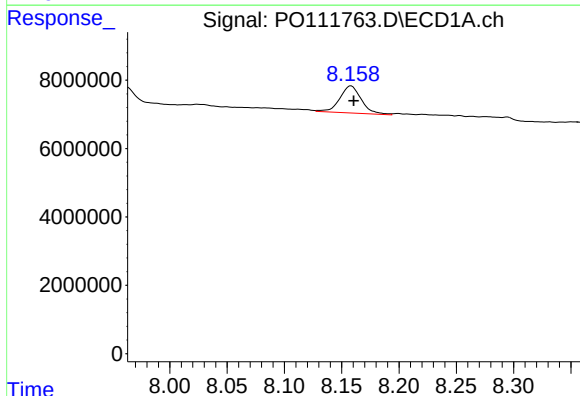


#44 AR-1268-4

R.T.: 8.158 min
Delta R.T.: -0.002 min
Response: 10401226
Conc: 30.24 ng/ml

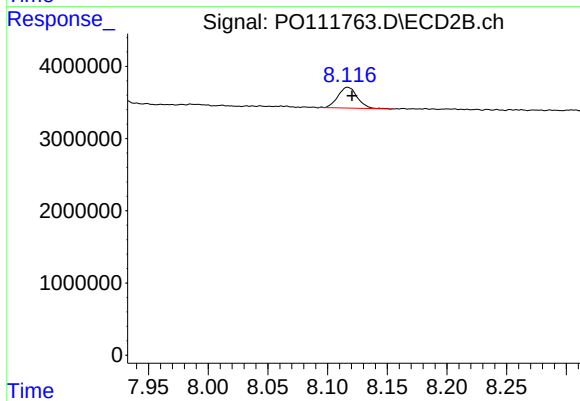

#44 AR-1268-4


R.T.: 8.117 min
Delta R.T.: -0.004 min
Response: 3264969
Conc: 28.23 ng/ml

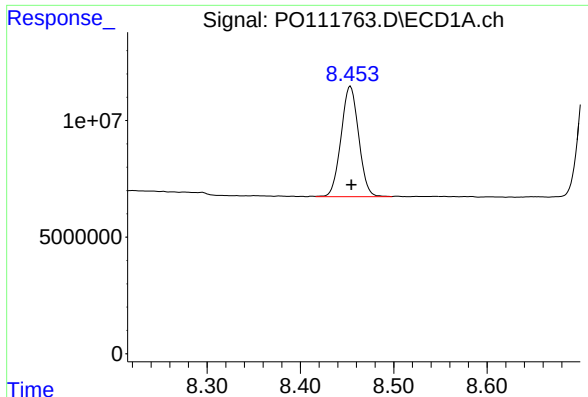

#45 AR-1268-5

R.T.: 8.454 min
Delta R.T.: -0.001 min
Response: 62056622
Conc: 27.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

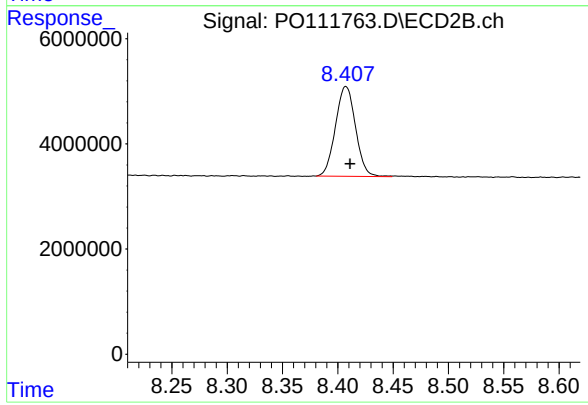

#45 AR-1268-5

R.T.: 8.407 min
Delta R.T.: -0.004 min
Response: 21554160
Conc: 29.74 ng/ml