

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
 Data File : P0111747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2025 10:34
 Operator : YP/AJ
 Sample : Q2126-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/23/2025
 Supervised By :mohammad ahmed 06/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 00:02:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.678	3.673	129.8E6	112.4E6	22.542	20.011
2) SA Decachlor...	8.712	8.660	114.0E6	37450807	21.722	21.067
Target Compounds						
8) L2 AR-1221-1	3.891	3.883	1948756	1789341	22.379	23.962
9) L2 AR-1221-2	3.976	3.968	2185977	2032636	34.067m	36.330m
10) L2 AR-1221-3	4.051	4.043	4466701	3784502	22.902	22.025

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062025\
Data File : PO111747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2025 10:34
Operator : YP/AJ
Sample : Q2126-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2025
Supervised By :mohammad ahmed 06/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 00:02:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

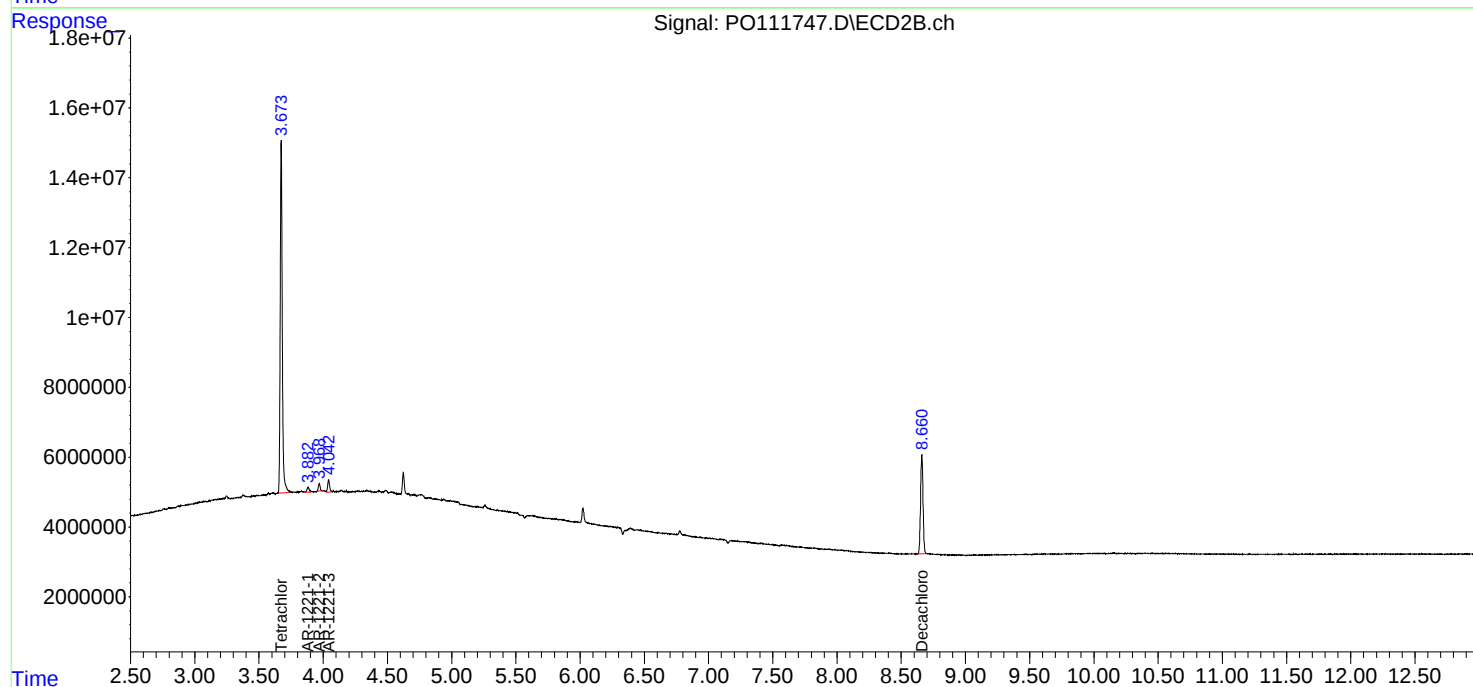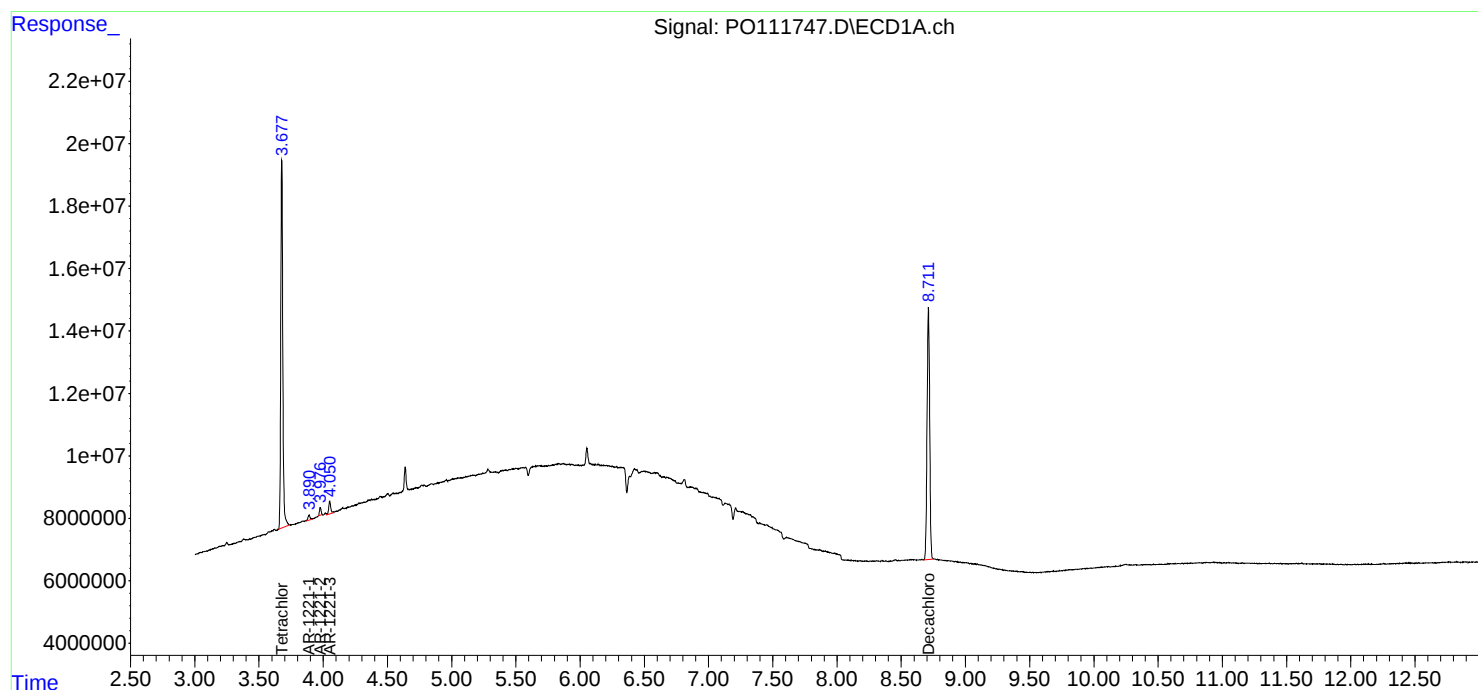

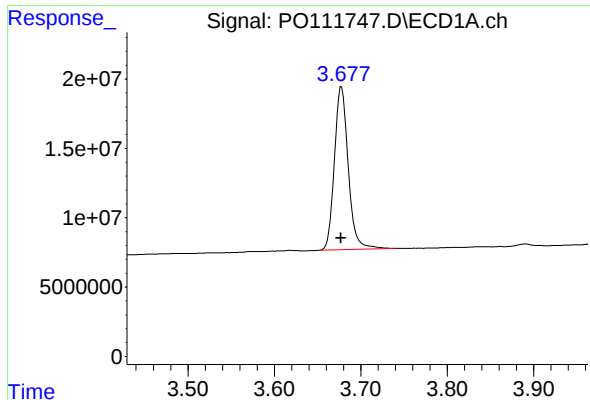


#1 Tetrachloro-m-xylene

R.T.: 3.678 min
Delta R.T.: 0.000 min
Response: 129827811
Conc: 22.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2025
Supervised By :mohammad ahmed 06/24/2025

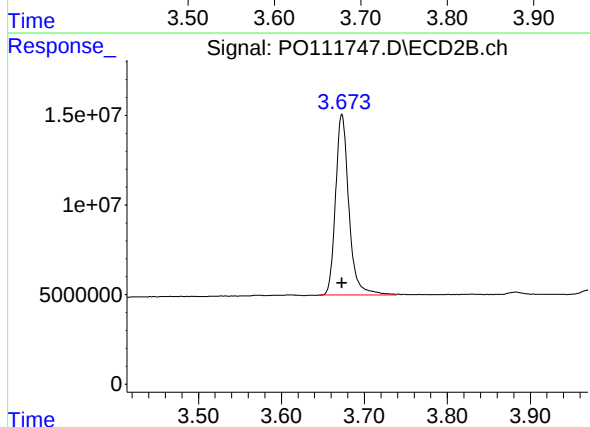


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.000 min
Response: 112405272
Conc: 20.01 ng/ml

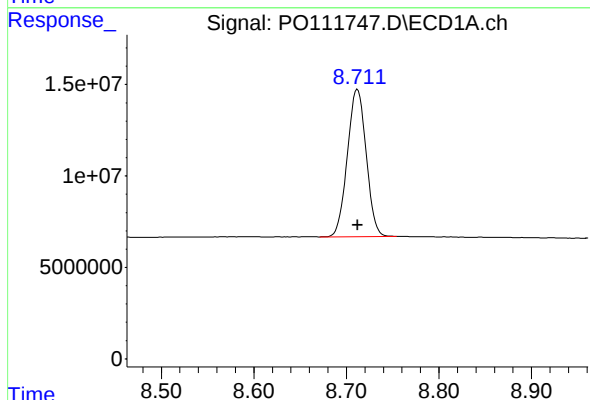


#2 Decachlorobiphenyl

R.T.: 8.712 min
Delta R.T.: 0.000 min
Response: 114026356
Conc: 21.72 ng/ml

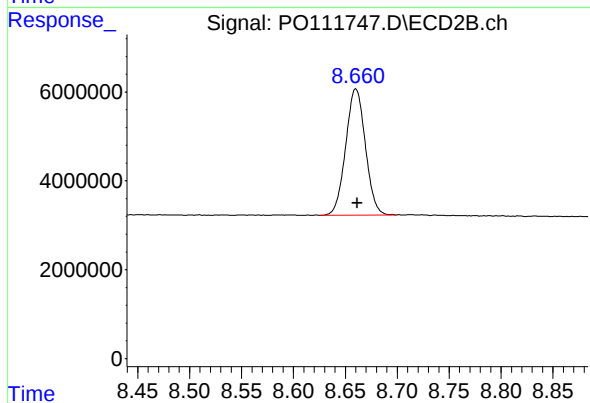

#2 Decachlorobiphenyl

R.T.: 8.660 min
Delta R.T.: -0.001 min
Response: 37450807
Conc: 21.07 ng/ml

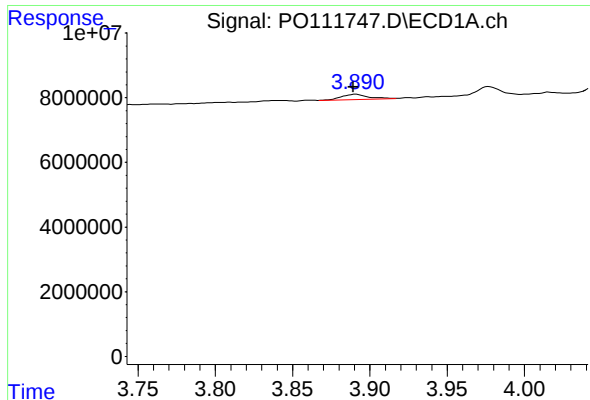


#8 AR-1221-1

R.T.: 3.891 min
Delta R.T.: 0.002 min
Response: 1948756
Conc: 22.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2025
Supervised By :mohammad ahmed 06/24/2025

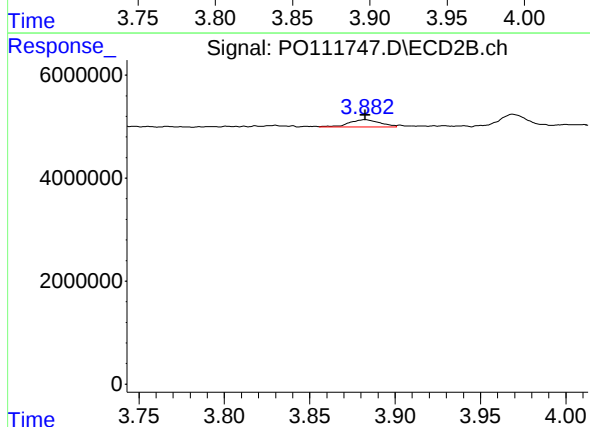


#8 AR-1221-1

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 1789341
Conc: 23.96 ng/ml

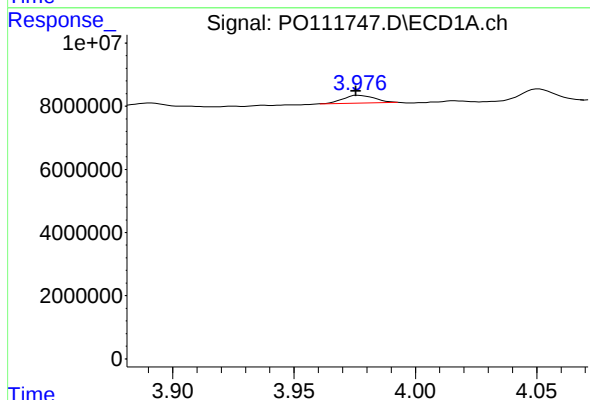


#9 AR-1221-2

R.T.: 3.976 min
Delta R.T.: 0.000 min
Response: 2185977
Conc: 34.07 ng/ml m

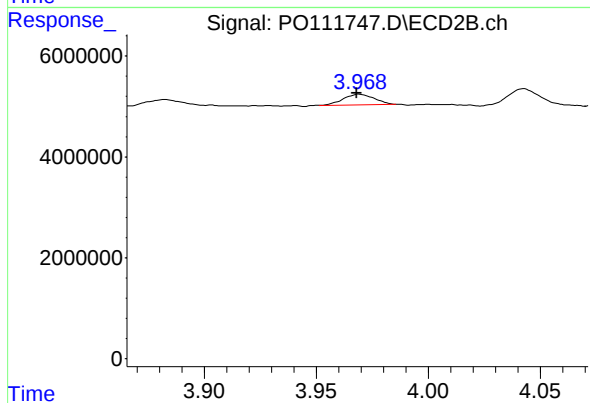

#9 AR-1221-2

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 2032636
Conc: 36.33 ng/ml m

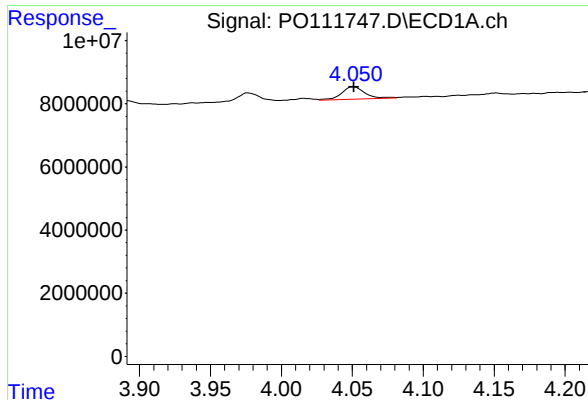


#10 AR-1221-3

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 4466701
Conc: 22.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT2-2025

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2025
Supervised By :mohammad ahmed 06/24/2025

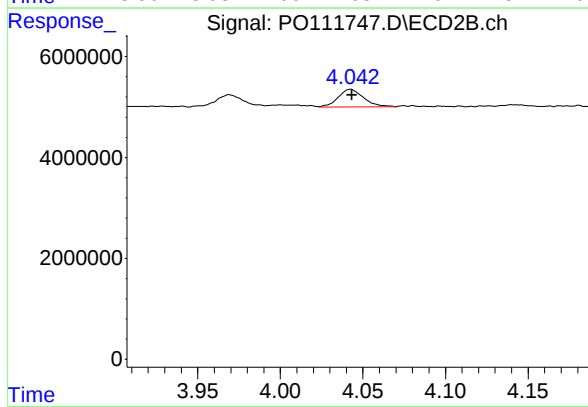

#10 AR-1221-3

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 3784502
Conc: 22.02 ng/ml