

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062025\
Data File : P0111785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2025 01:42
Operator : YP/AJ
Sample : DDT ANALOGUE
Misc : AR1268 LOD 40 PPB
ALS Vial : 100 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 08:51:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

30) L6	AR-1254-5	6.772	6.739	2446.6E6	1693.9E6	4777.270	5202.667
--------	-----------	-------	-------	----------	----------	----------	----------



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062025\
Data File : PO111785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2025 01:42
Operator : YP/AJ
Sample : DDT ANALOGUE
Misc : AR1268 LOD 40 PPB
ALS Vial : 100 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOGUE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 08:51:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

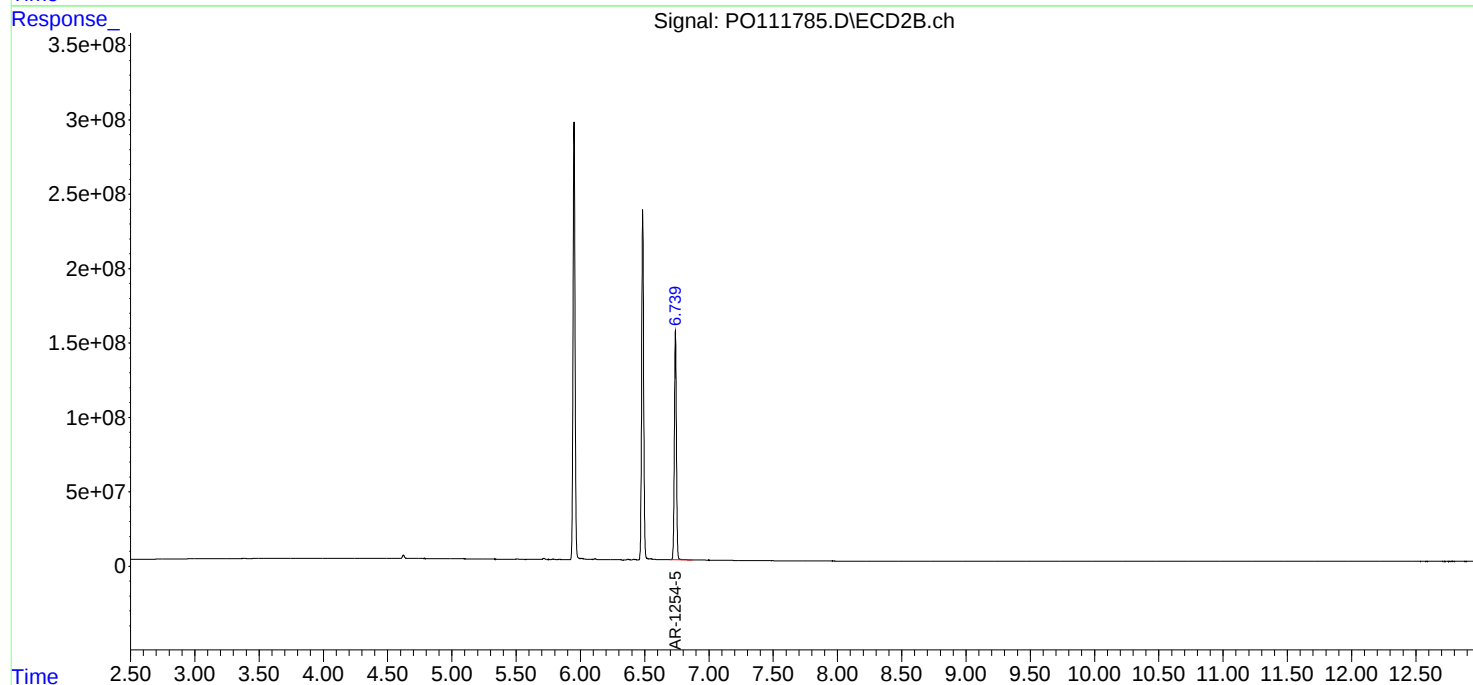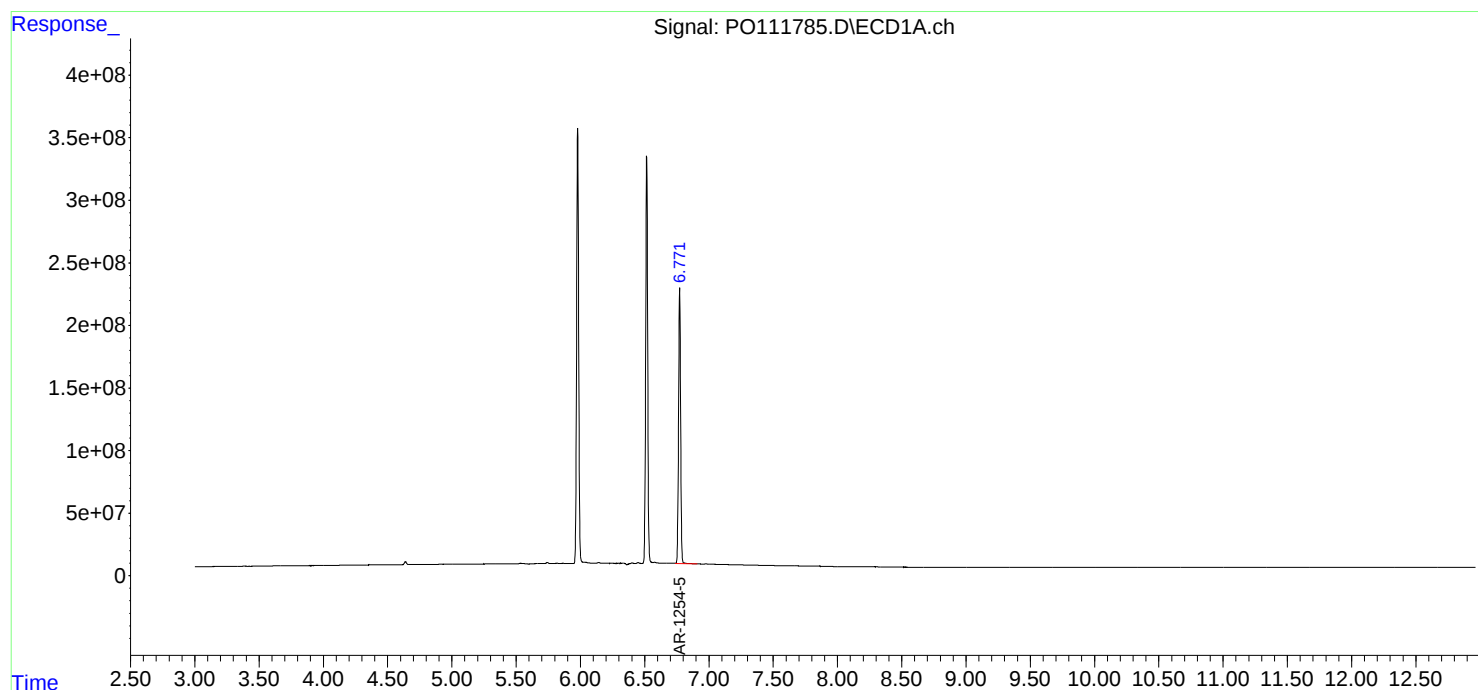


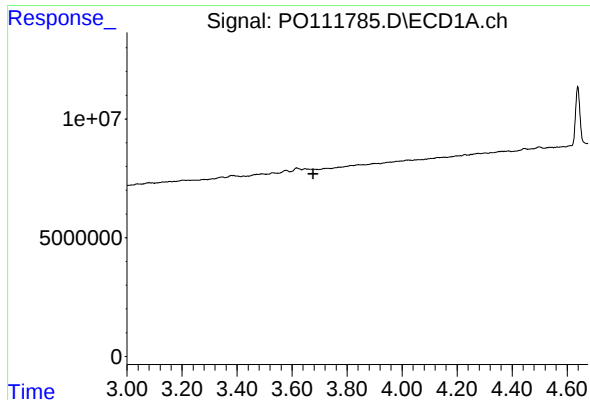

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOGUE

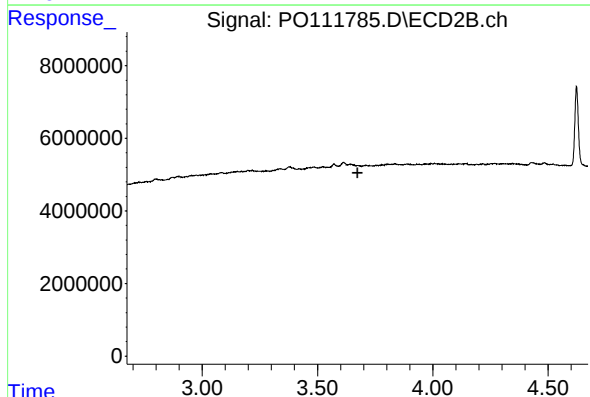


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.673 min
Response: 0
Conc: N.D.

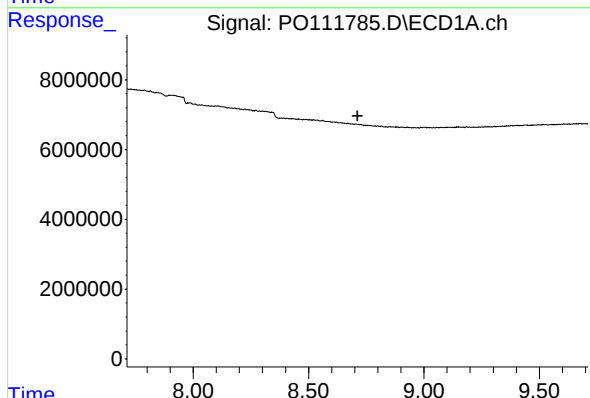


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

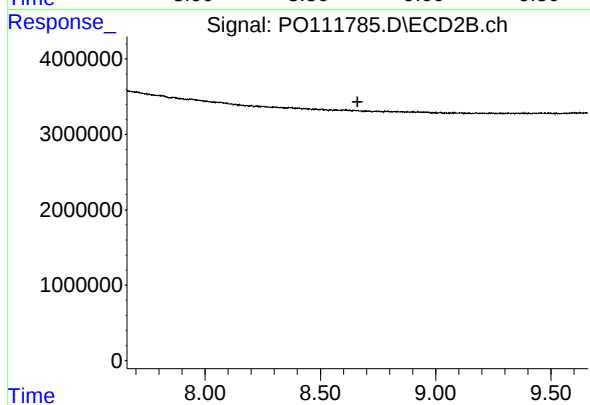

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T.: 8.661 min
Response: 0
Conc: N.D.

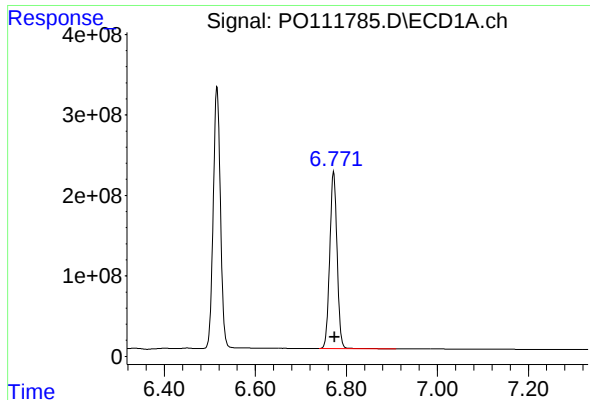

#30 AR-1254-5

R.T.: 6.772 min
Delta R.T.: -0.003 min
Response: 2446583174
Conc: 4777.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOGUE

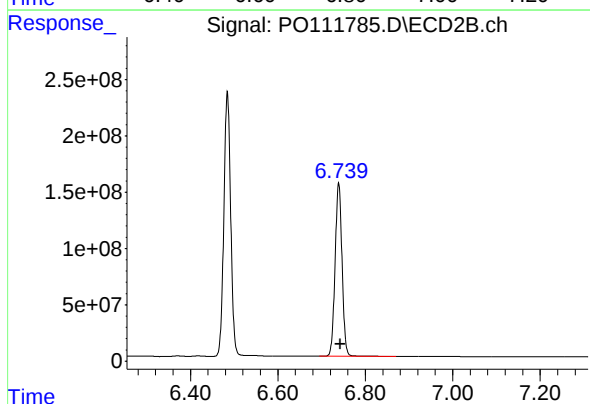

#30 AR-1254-5

R.T.: 6.739 min
Delta R.T.: -0.003 min
Response: 1693938610
Conc: 5202.67 ng/ml