

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
 Data File : PL067664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2021 15:58
 Operator : AR\AJ
 Sample : PB137227BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 04:19:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	5.529	10382401	19004936	18.884	20.159
28)	SA Decachlor...	10.220	11.428	13770699	20369360	19.431	20.450
Target Compounds							
3)	MA gamma-BHC...	5.588	0.000	666065	0	0.889	N.D. #
6)	B beta-BHC	5.962f	0.000	202735	0	0.567	N.D. #
7)	B delta-BHC	0.000	7.003f	0	1082568	N.D.	0.921 #
15)	B Endosulfa...	0.000	9.178f	0	705961	N.D.	0.885 #
23)	Chlordane-1	0.000	6.937f	0	871077	N.D.	30.848 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062121\
Data File : PL067664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2021 15:58
Operator : AR\AJ
Sample : PB137227BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 04:19:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

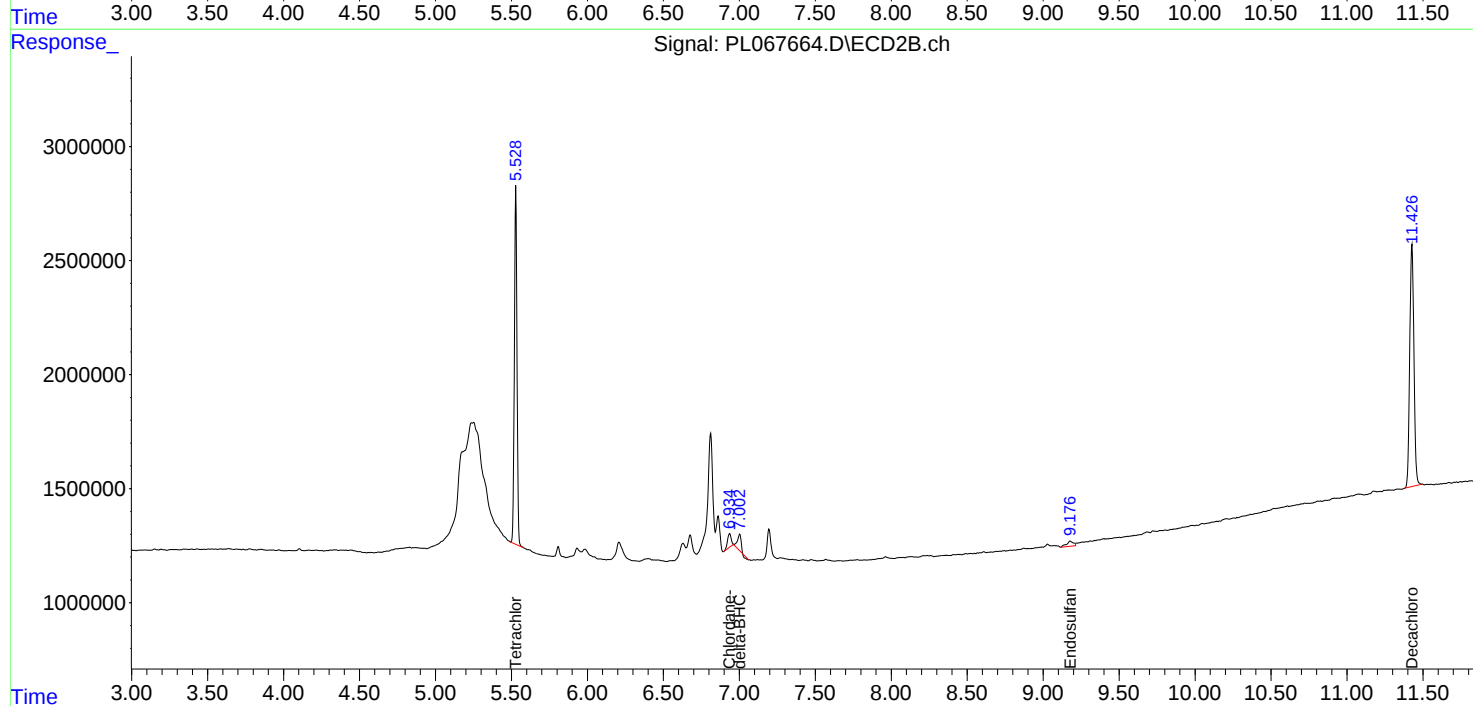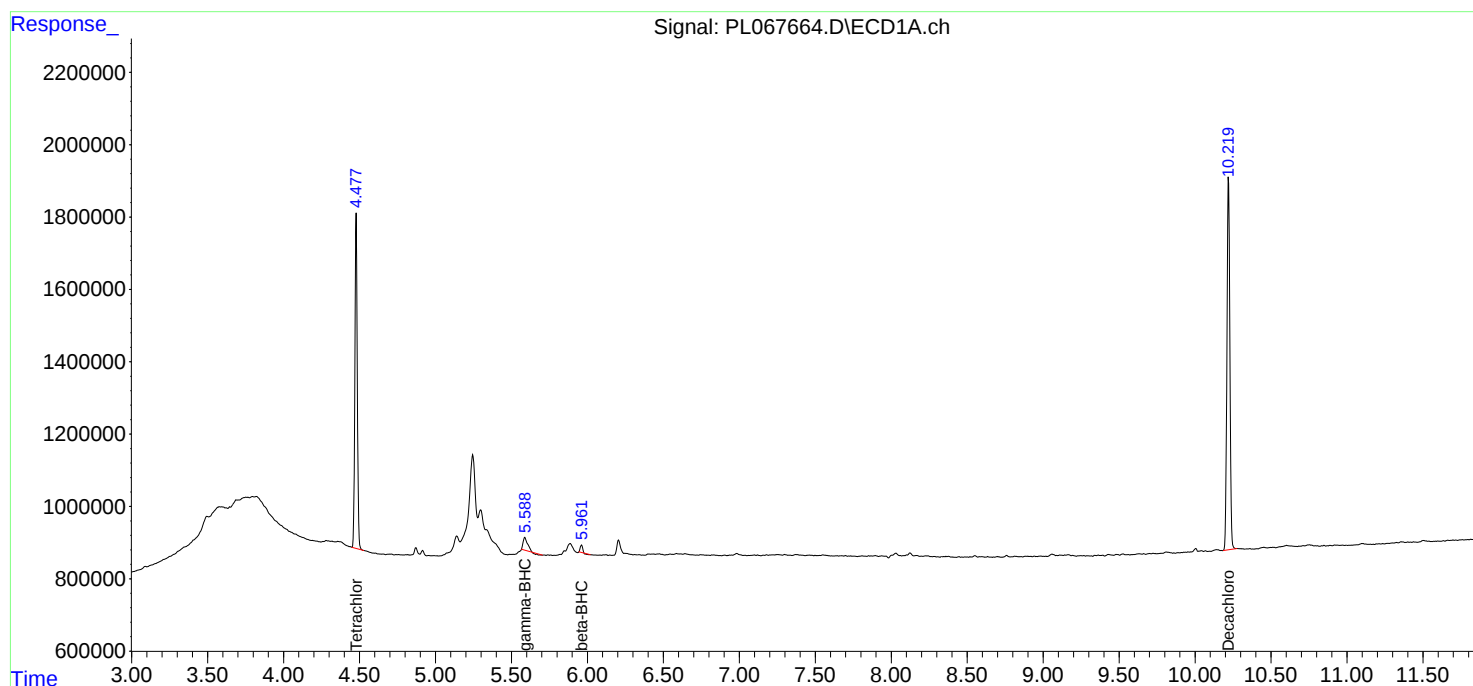


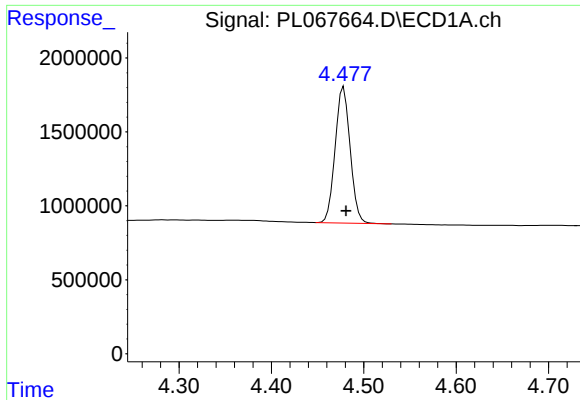

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: -0.003 min
Response: 10382401
Conc: 18.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

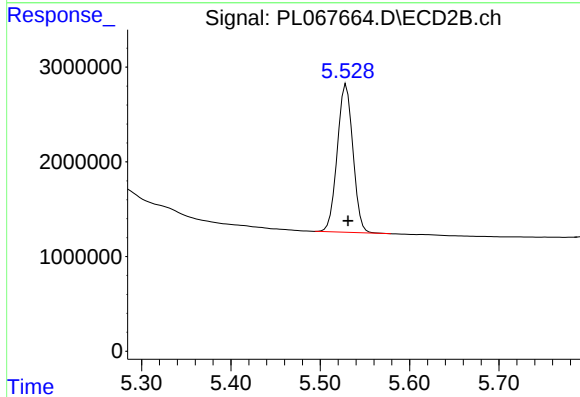


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 19004936
Conc: 20.16 ng/ml

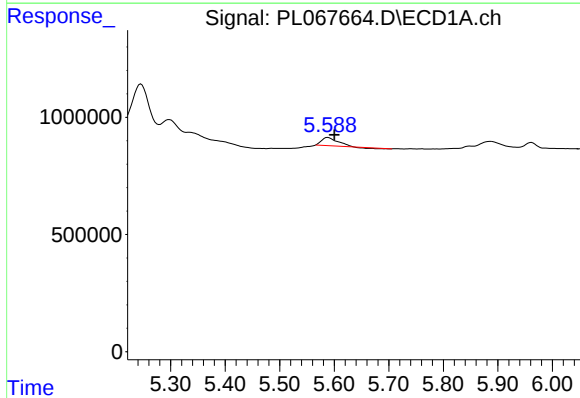


#3 gamma-BHC (Lindane)

R.T.: 5.588 min
Delta R.T.: -0.012 min
Response: 666065
Conc: 0.89 ng/ml

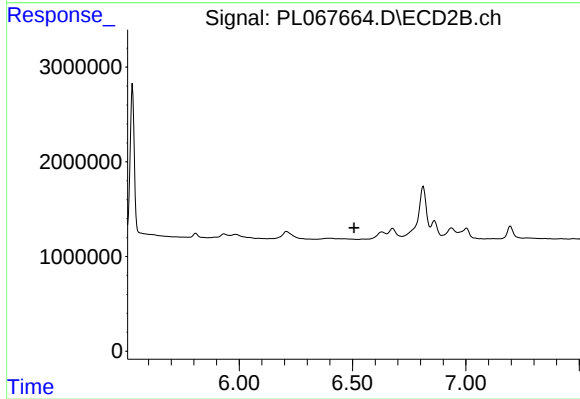

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

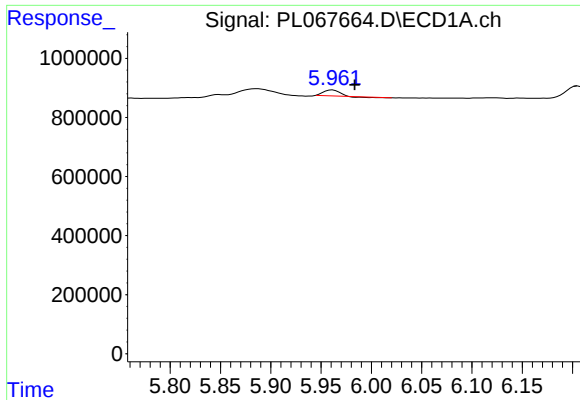

#6 beta-BHC


R.T.: 5.962 min
Delta R.T.: -0.022 min
Response: 202735
Conc: 0.57 ng/ml

Instrument :
ECD_O
ClientSampleId :

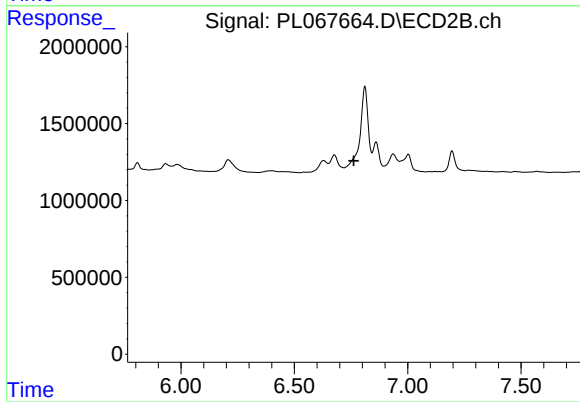


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.762 min
Response: 0
Conc: N.D.

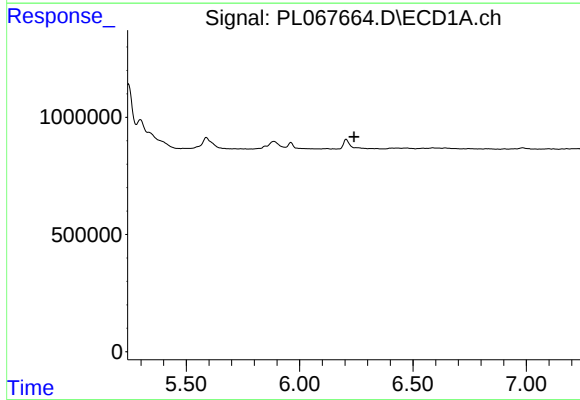


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.241 min
Response: 0
Conc: N.D.

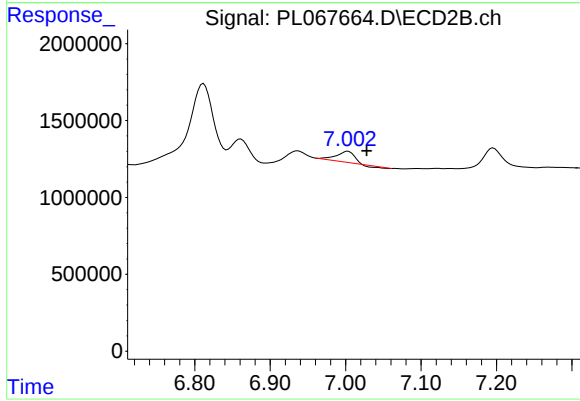

#7 delta-BHC


R.T.: 7.003 min
Delta R.T.: -0.025 min
Response: 1082568
Conc: 0.92 ng/ml

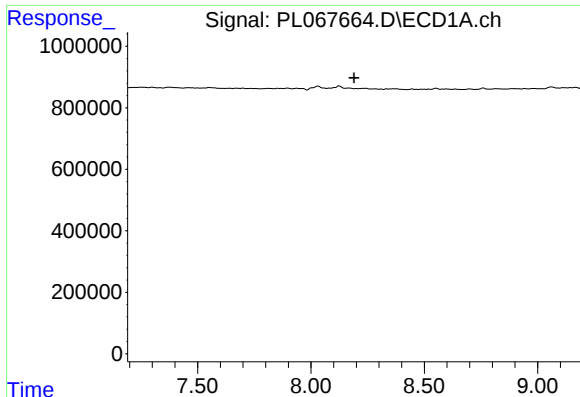

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

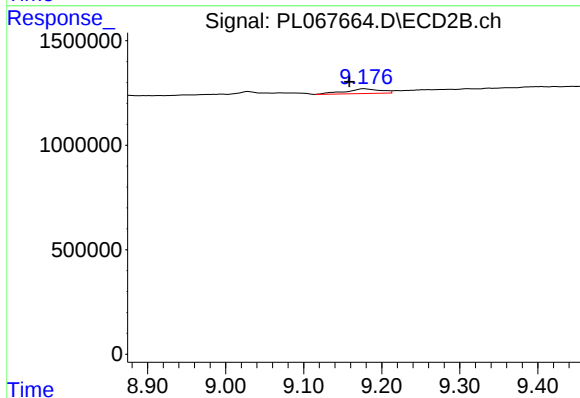


#15 Endosulfan II

R.T.: 9.178 min
Delta R.T.: 0.020 min
Response: 705961
Conc: 0.89 ng/ml

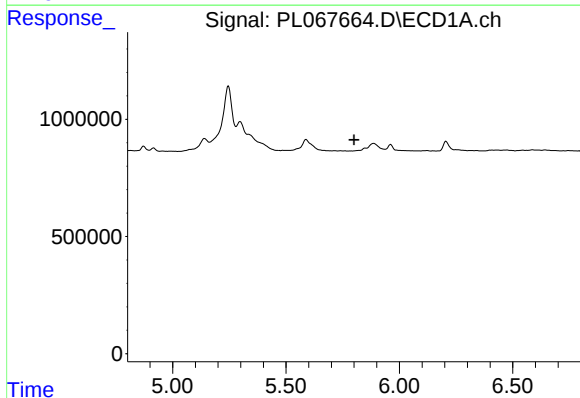


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.800 min
Response: 0
Conc: N.D.

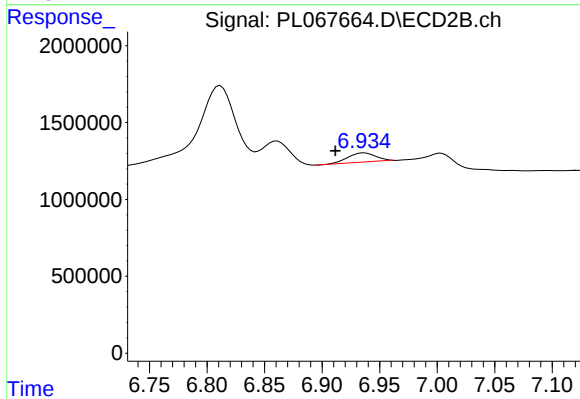

#23 Chlordane-1


R.T.: 6.937 min
Delta R.T.: 0.025 min
Response: 871077
Conc: 30.85 ng/ml

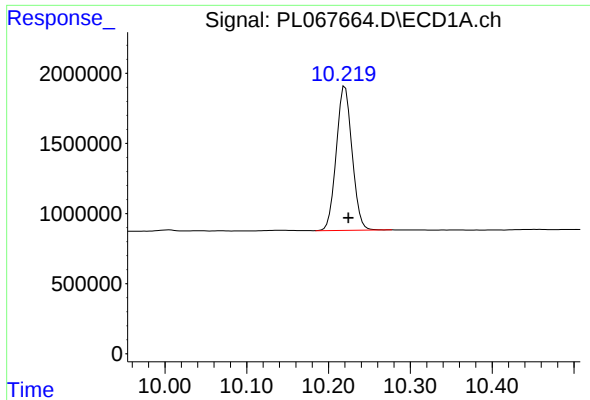

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 13770699
Conc: 19.43 ng/ml

Instrument :
ECD_O
ClientSampleId :

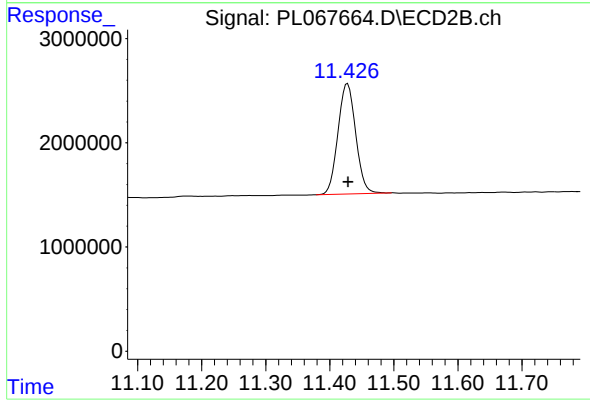

#28 Decachlorobiphenyl

R.T.: 11.428 min
Delta R.T.: 0.000 min
Response: 20369360
Conc: 20.45 ng/ml