

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078971.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 9:27
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:06:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.329	3.605	1734679	657782	21.979	22.132
2)	SA Decachlor...	9.936	8.786	1304876	654357	20.893	21.959
Target Compounds							
5)	L1 AR-1016-3	5.709	0.000	49503	0	19.707	N.D. #
8)	L2 AR-1221-1	4.575	0.000	35470	0	42.666	N.D. #
9)	L2 AR-1221-2	4.670	0.000	19517	0	32.042	N.D. #
18)	L4 AR-1242-3	5.709	0.000	49503	0	26.749	N.D. #
28)	L6 AR-1254-3	7.139f	0.000	96366	0	21.638	N.D. #
32)	L7 AR-1260-2	0.000	6.560f	0	42661	N.D.	22.016 #
39)	L8 AR-1262-4	8.797	0.000	31620	0	8.495	N.D. #
42)	L9 AR-1268-2	8.797	0.000	31620	0	4.229	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
Data File : P0078971.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 9:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:06:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

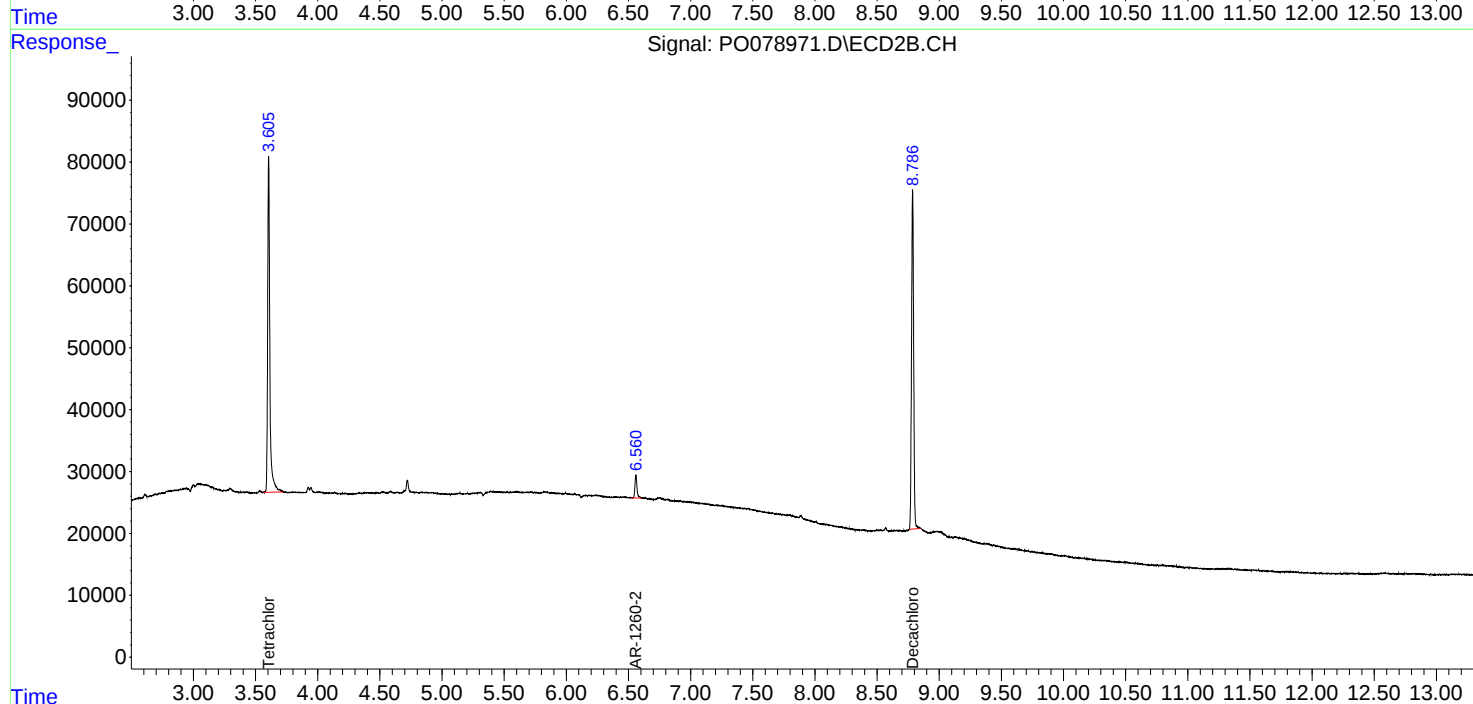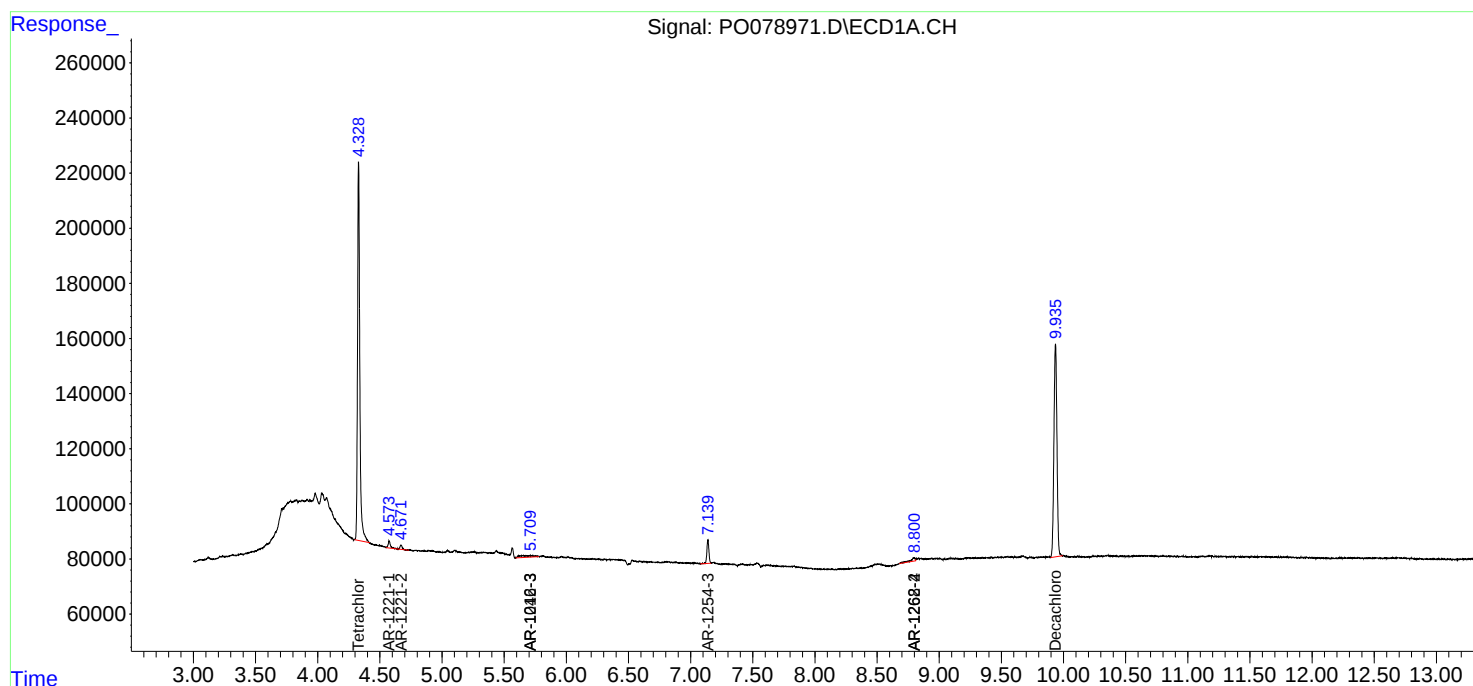


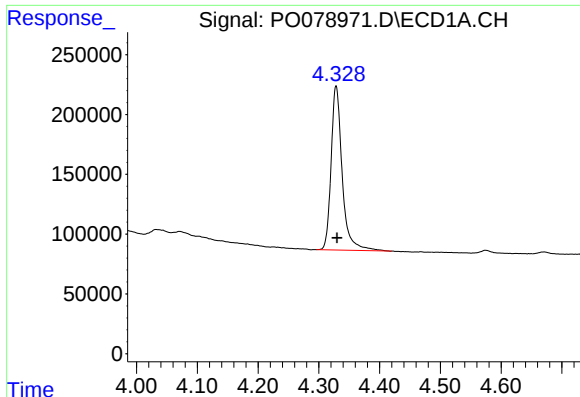

#1 Tetrachloro-m-xylene


R.T.: 4.329 min
Delta R.T.: -0.001 min
Response: 1734679
Conc: 21.98 ng/ml

Instrument :
ECD_O
ClientSampleId :

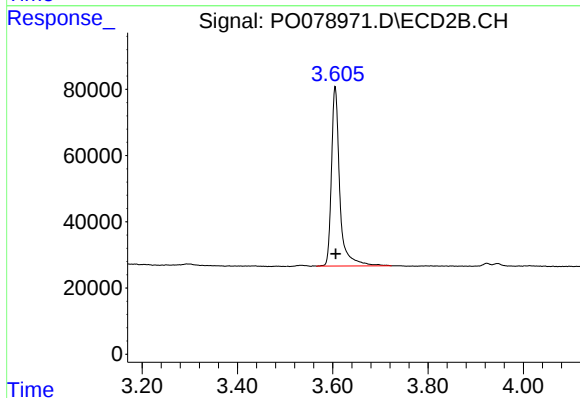


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: 0.000 min
Response: 657782
Conc: 22.13 ng/ml

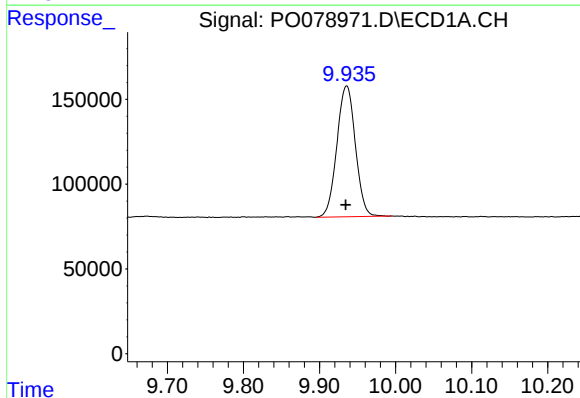


#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.000 min
Response: 1304876
Conc: 20.89 ng/ml

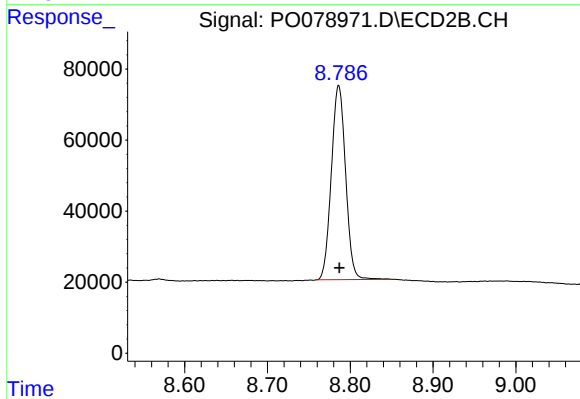

#2 Decachlorobiphenyl


R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 654357
Conc: 21.96 ng/ml

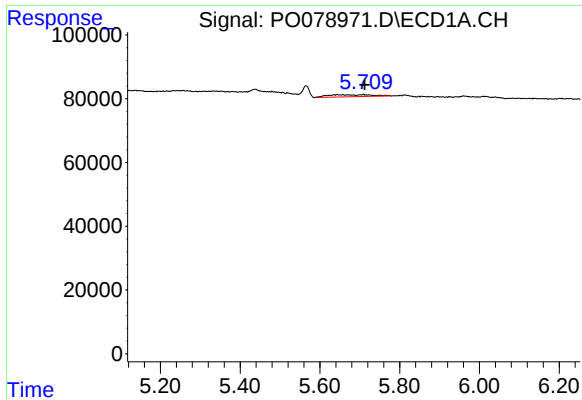

#5 AR-1016-3


R.T.: 5.709 min
Delta R.T.: -0.003 min
Response: 49503
Conc: 19.71 ng/ml

Instrument :
ECD_O
ClientSampleId :

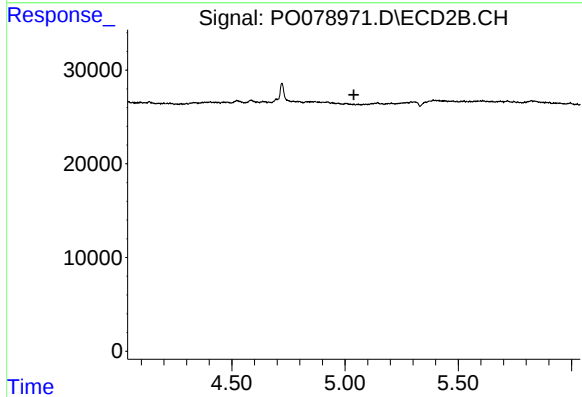


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

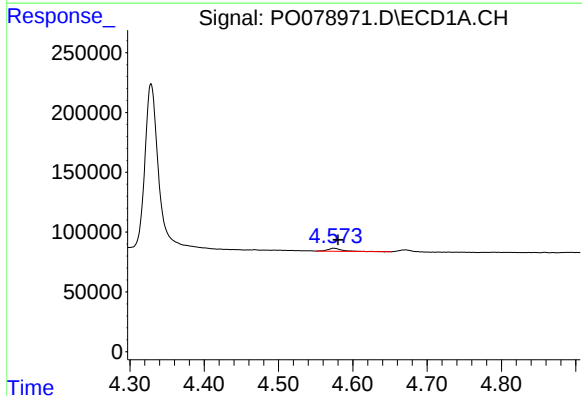


#8 AR-1221-1

R.T.: 4.575 min
Delta R.T.: -0.006 min
Response: 35470
Conc: 42.67 ng/ml

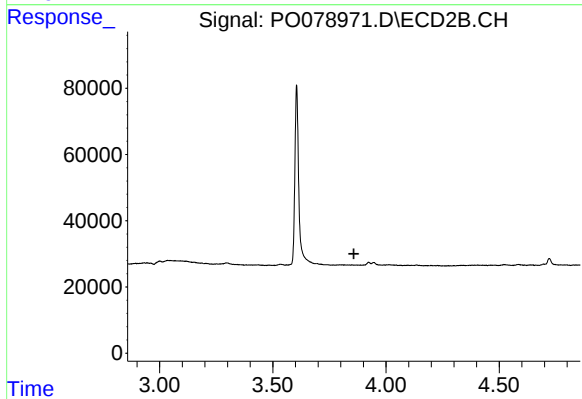

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.858 min
Response: 0
Conc: N.D.

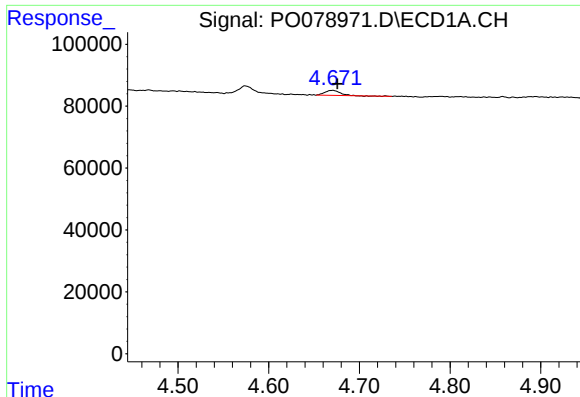

#9 AR-1221-2


R.T.: 4.670 min
Delta R.T.: -0.006 min
Response: 19517
Conc: 32.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

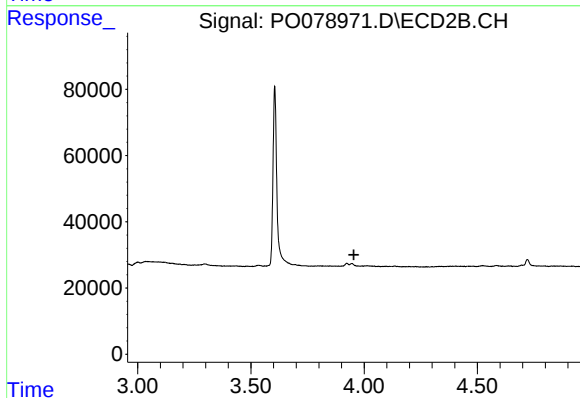


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.955 min
Response: 0
Conc: N.D.

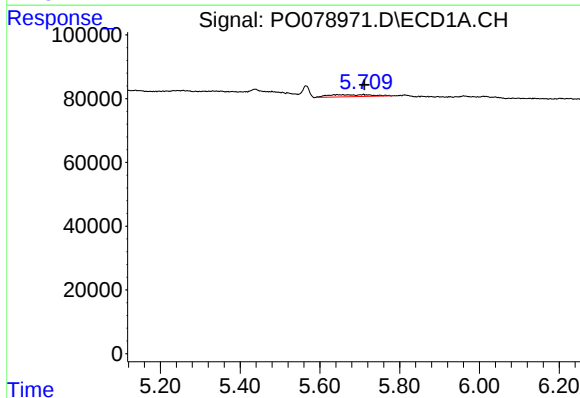


#18 AR-1242-3

R.T.: 5.709 min
Delta R.T.: -0.002 min
Response: 49503
Conc: 26.75 ng/ml

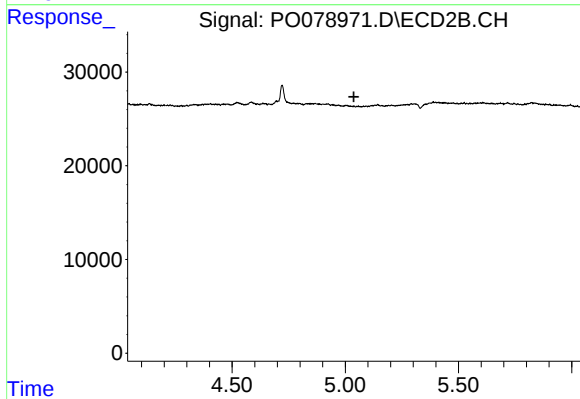

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.038 min
Response: 0
Conc: N.D.

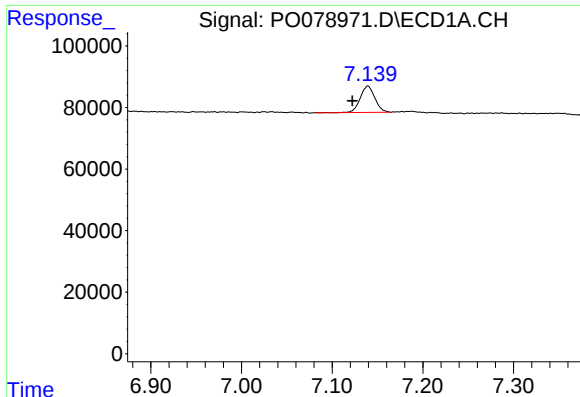

#28 AR-1254-3


R.T.: 7.139 min
Delta R.T.: 0.017 min
Response: 96366
Conc: 21.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

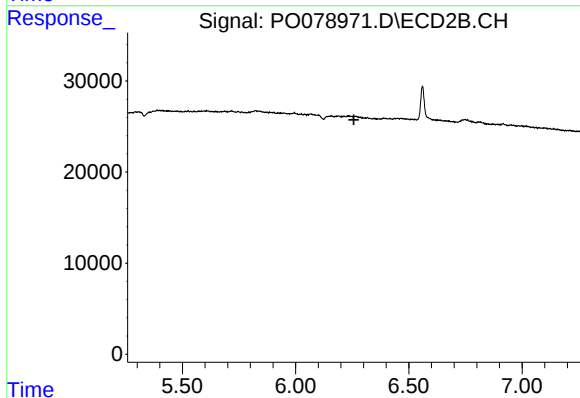


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.

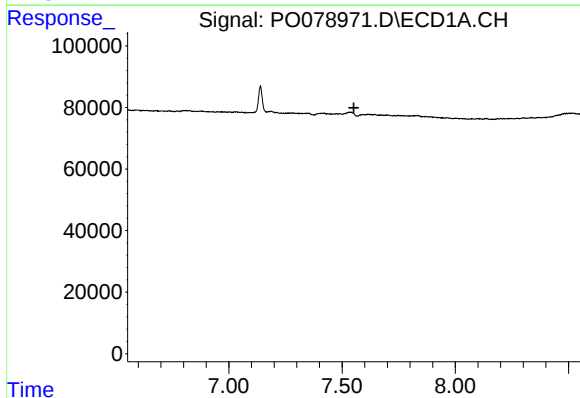


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.552 min
Response: 0
Conc: N.D.

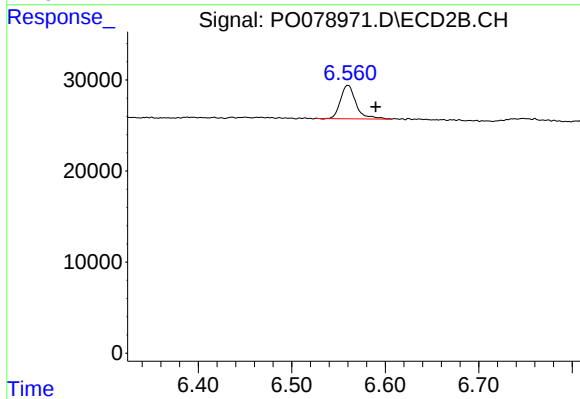

#32 AR-1260-2


R.T.: 6.560 min
Delta R.T.: -0.030 min
Response: 42661
Conc: 22.02 ng/ml

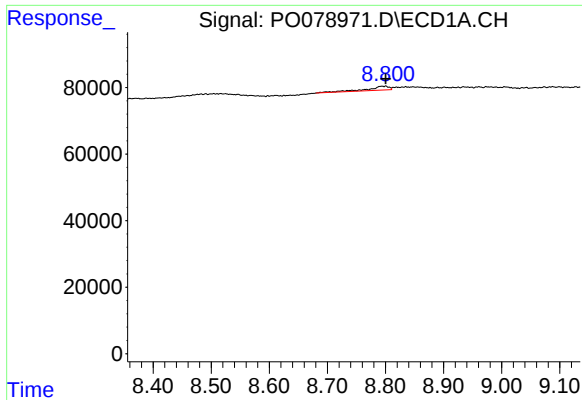

#39 AR-1262-4


R.T.: 8.797 min
Delta R.T.: -0.004 min
Response: 31620
Conc: 8.49 ng/ml

Instrument :
ECD_O
ClientSampleId :

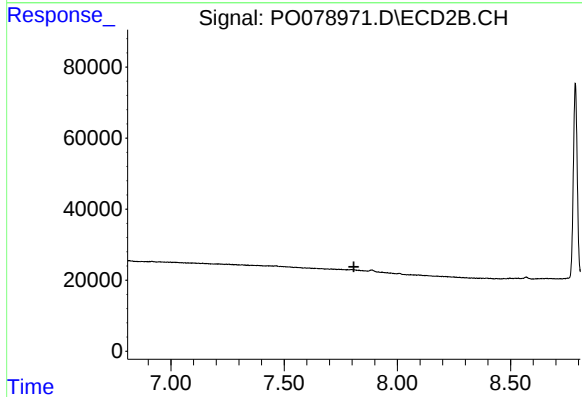


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.808 min
Response: 0
Conc: N.D.

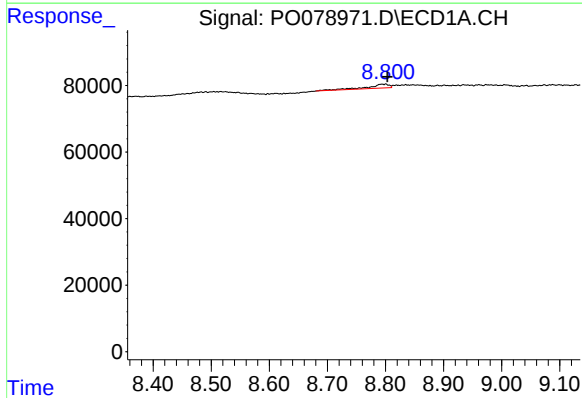

#42 AR-1268-2

R.T.: 8.797 min
Delta R.T.: -0.006 min
Response: 31620
Conc: 4.23 ng/ml

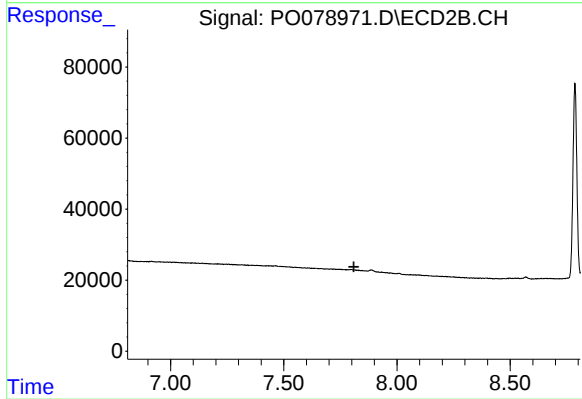

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.810 min
Response: 0
Conc: N.D.