

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078972.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 9:44
 Operator : DD\AJ
 Sample : M2756-07 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:06:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.606	384324	71855	4.870m	2.418 #
2) SA Decachlor...	9.936	8.787	184771	84289	2.958m	2.829

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 HEF317G-N-1

Manual Integrations
 APPROVED

Ankita
 6/22/2021 12:20:16 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062121\
Data File : PO078972.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 9:44
Operator : DD\AJ
Sample : M2756-07 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:06:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleId :
HEF317G-N-1

Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:16 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

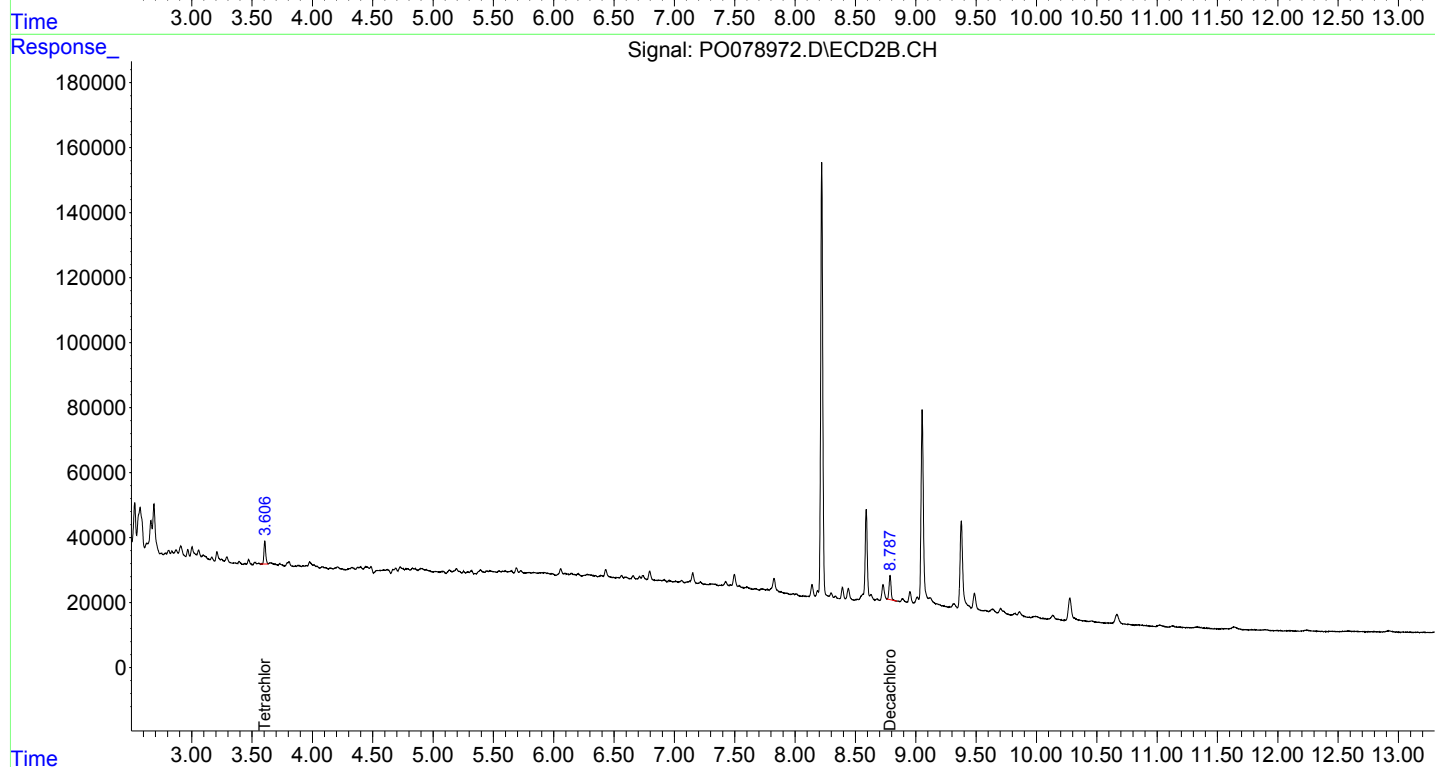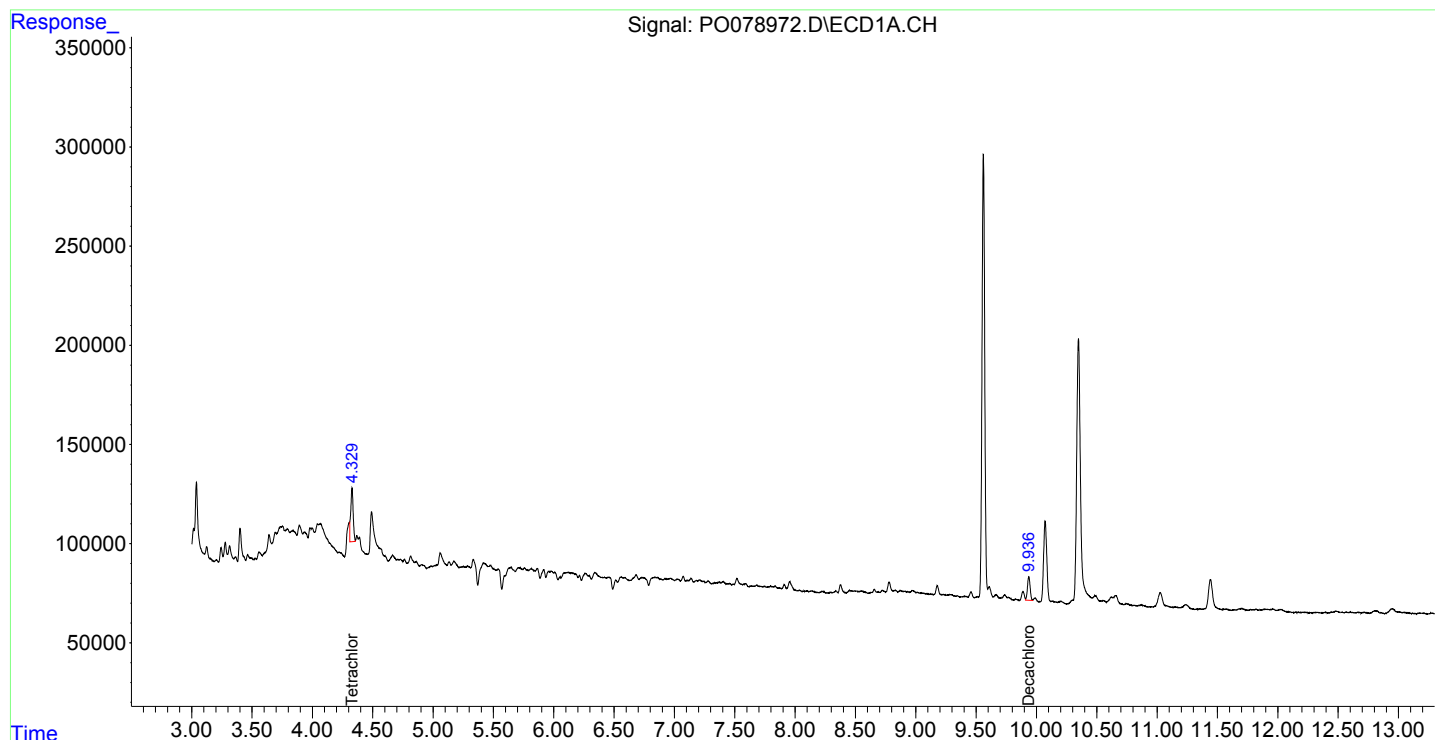

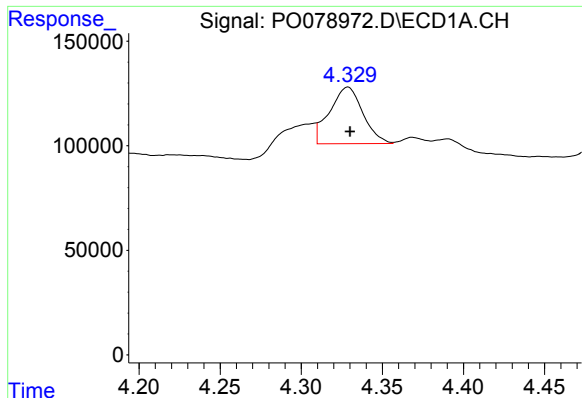

#1 Tetrachloro-m-xylene

R.T.: 4.329 min

Delta R.T.: -0.001 min


Response: 384324

Conc: 4.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HEF317G-N-1

Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:16 PM

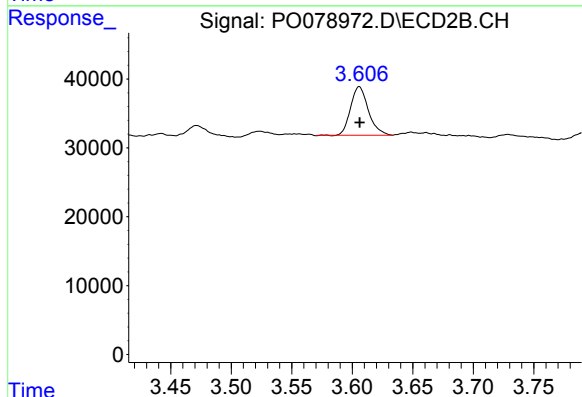


#1 Tetrachloro-m-xylene

R.T.: 3.606 min

Delta R.T.: 0.000 min

Response: 71855

Conc: 2.42 ng/ml

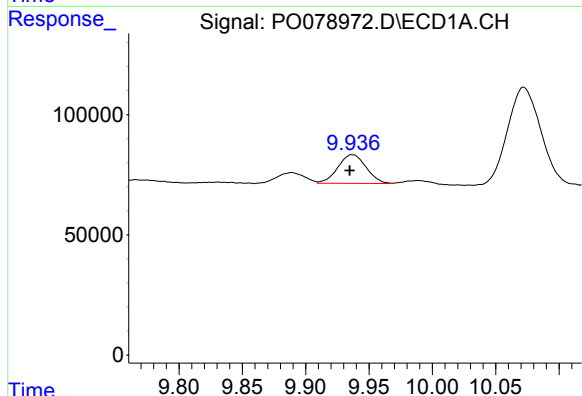


#2 Decachlorobiphenyl

R.T.: 9.936 min

Delta R.T.: 0.000 min

Response: 184771

Conc: 2.96 ng/ml m

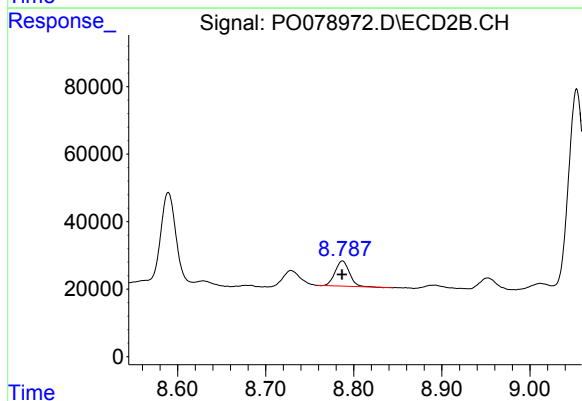

#2 Decachlorobiphenyl

R.T.: 8.787 min

Delta R.T.: 0.000 min

Response: 84289

Conc: 2.83 ng/ml