

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078976.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 10:53
 Operator : DD\AJ
 Sample : M2757-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:08:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.606	808297	2937258	10.242m	98.828 #
2) SA Decachlor...	9.939	8.788	916240	456210	14.671m	15.310

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 JEB542P-N-1

Manual Integrations
 APPROVED

Ankita
 6/22/2021 12:20:19 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
Data File : P0078976.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 10:53
Operator : DD\AJ
Sample : M2757-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:08:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Instrument :

ECD_O

ClientSampled :



JEB542P-N-1


Manual Integrations
APPROVED

Ankita

6/22/2021 12:20:19 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

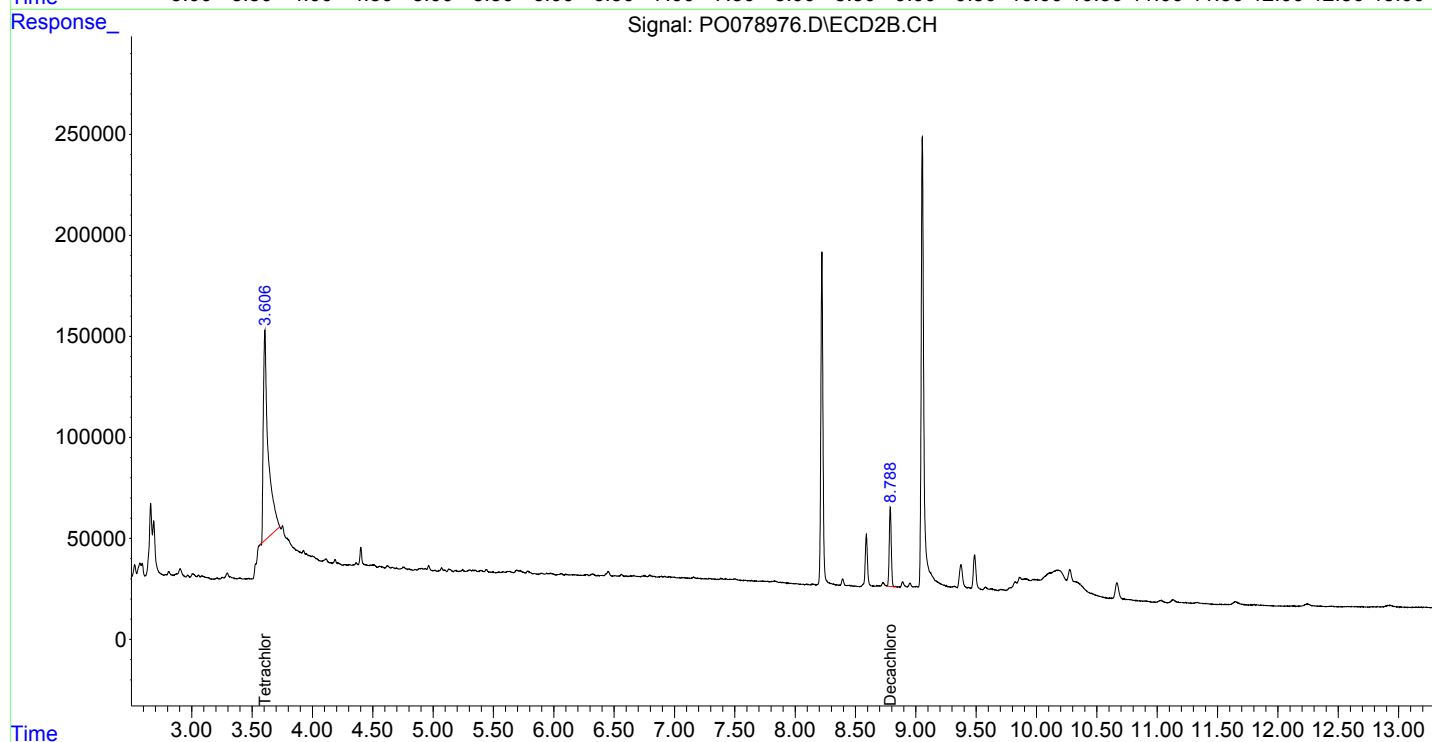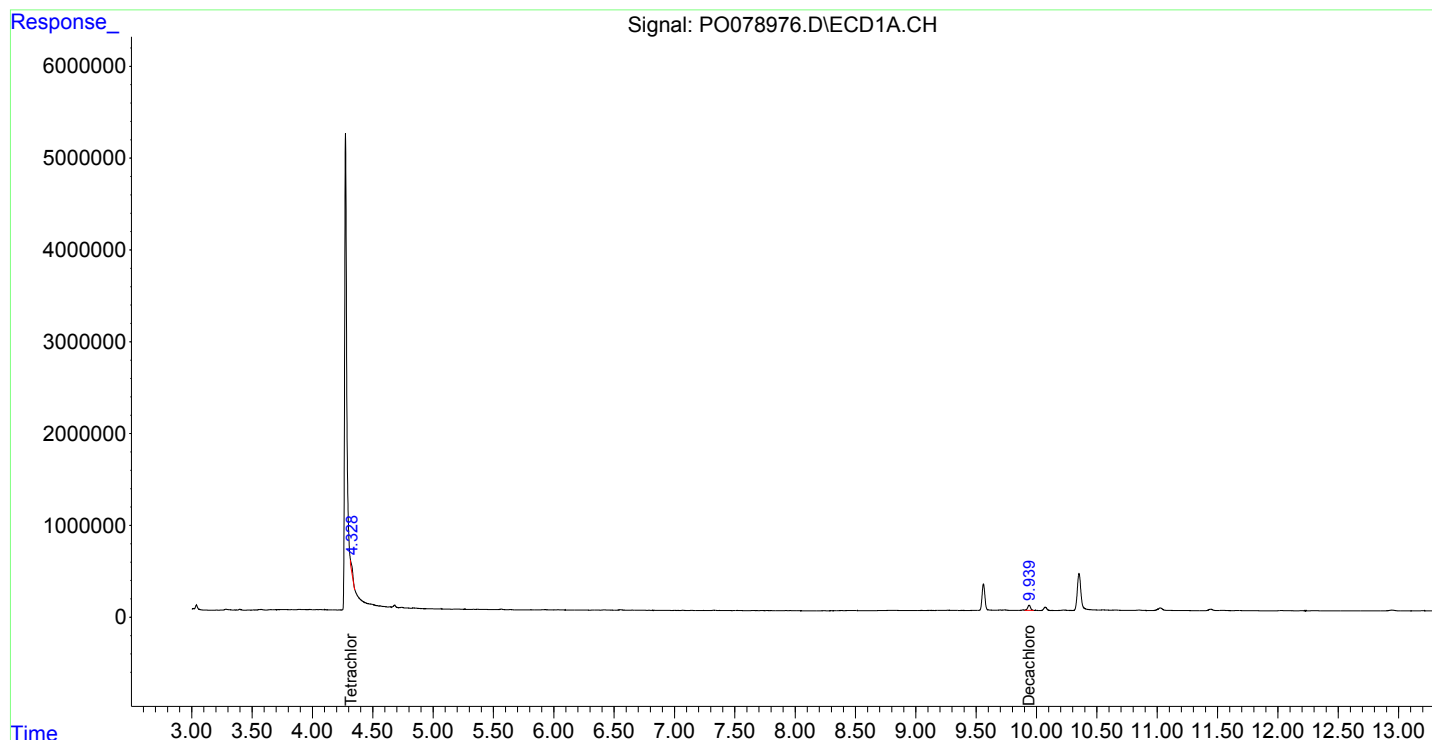

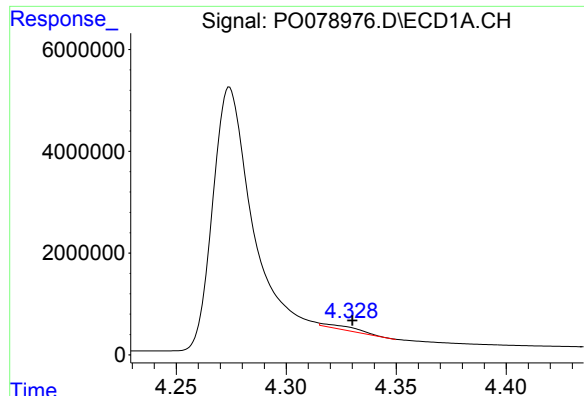


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.002 min
Response: 808297
Conc: 10.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
JEB542P-N-1


Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:19 PM

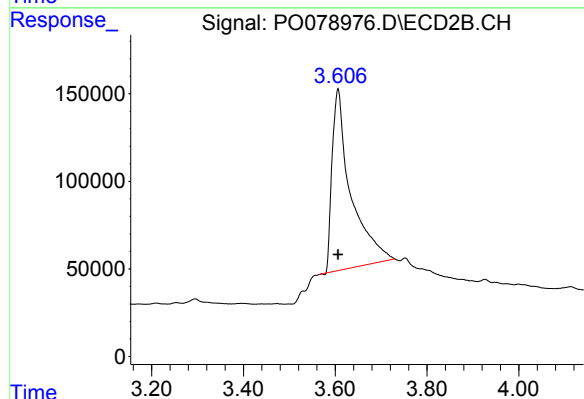


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 2937258
Conc: 98.83 ng/ml

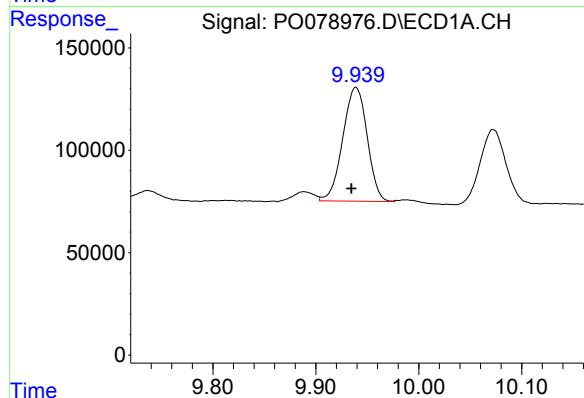

#2 Decachlorobiphenyl

R.T.: 9.939 min
Delta R.T.: 0.004 min
Response: 916240
Conc: 14.67 ng/ml m

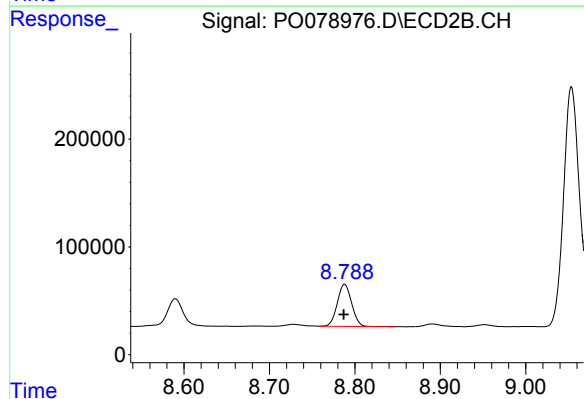

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: 0.001 min
Response: 456210
Conc: 15.31 ng/ml