

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078977.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 11:10
 Operator : DD\AJ
 Sample : M2757-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:08:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.330	3.606	749326	3013940	9.494m	101.408 #
2) SA Decachlor...	9.937	8.789	953785	464240	15.272m	15.579

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 JEB542P-N-2

Manual Integrations
 APPROVED

Ankita
 6/22/2021 12:20:20 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062121\
Data File : PO078977.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 11:10
Operator : DD\AJ
Sample : M2757-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:08:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Instrument :



ECD_O


ClientSampleId :

JEB542P-N-2

Manual Integrations
APPROVEDAnkita
6/22/2021 12:20:20 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

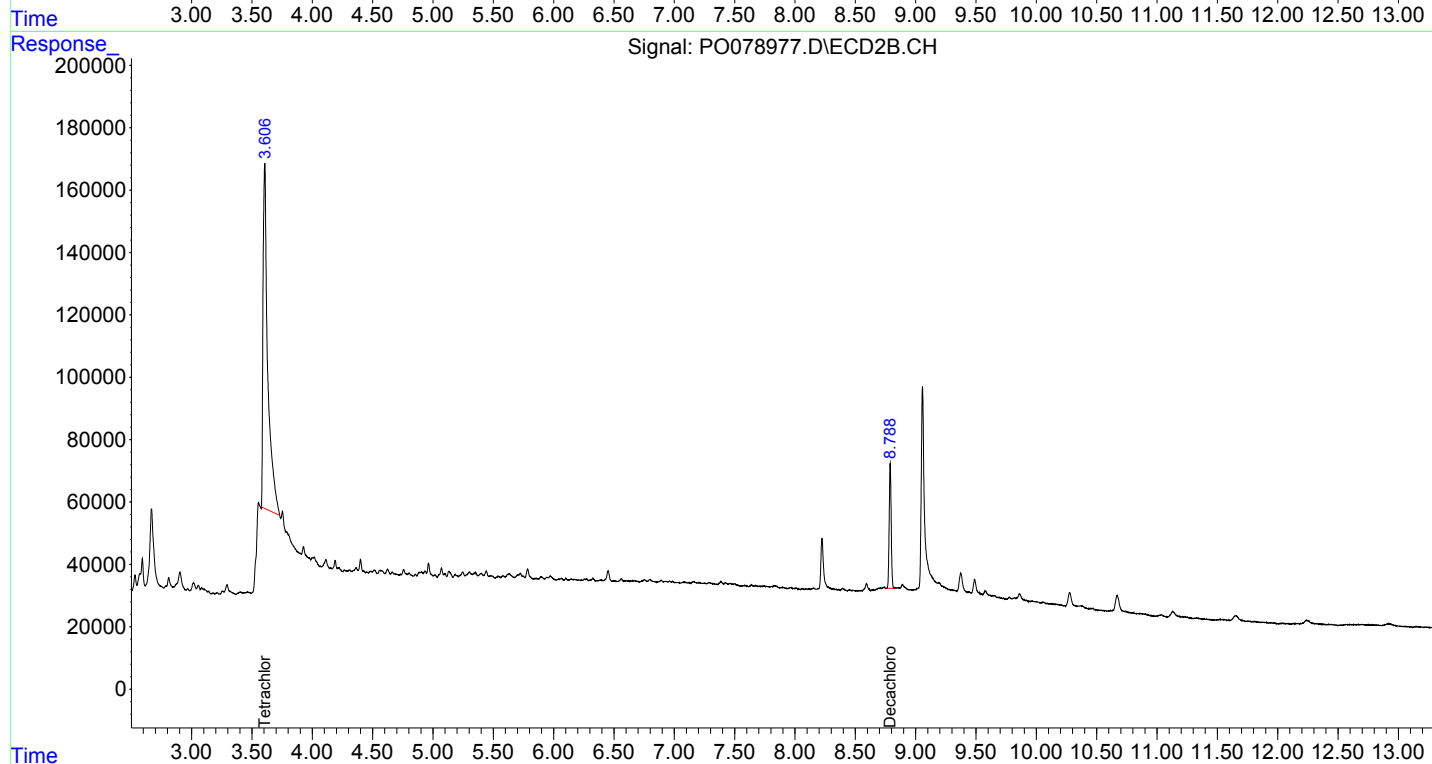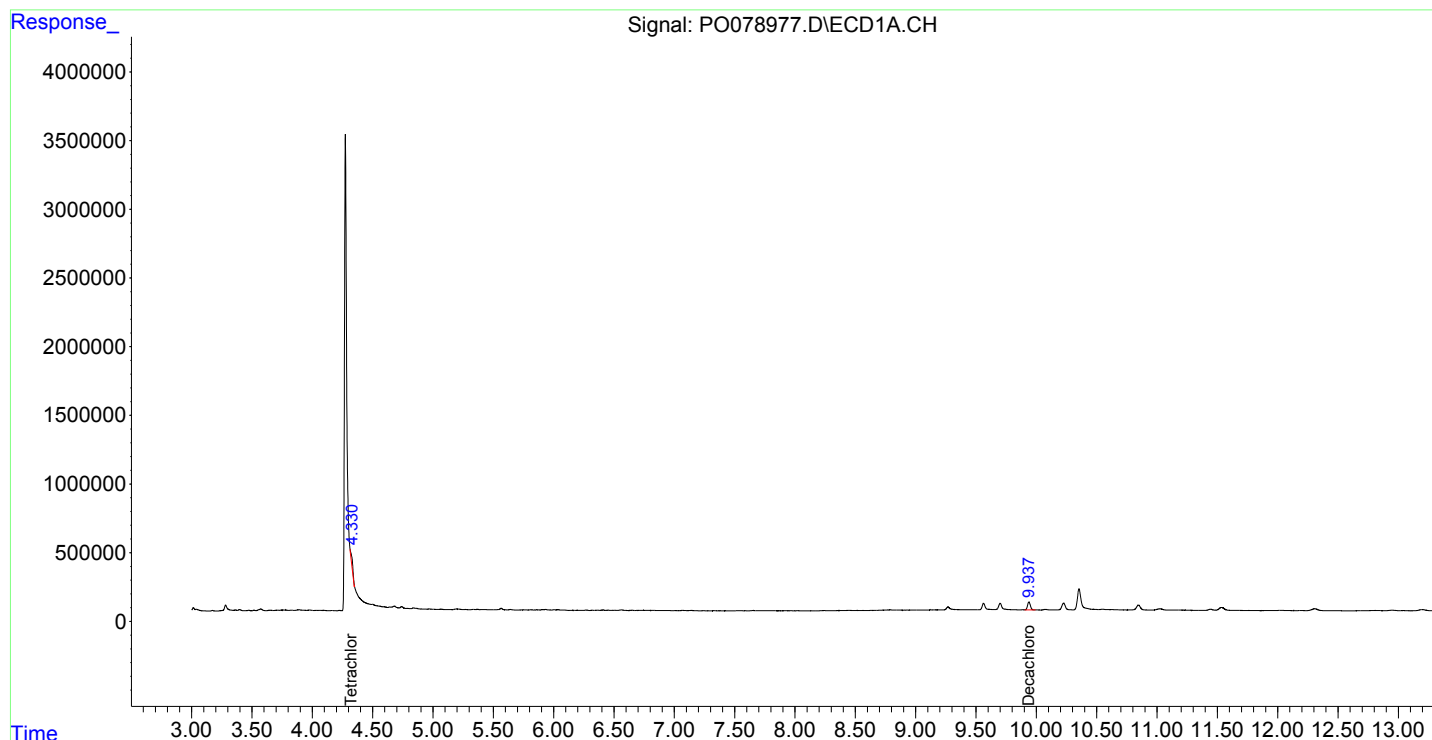

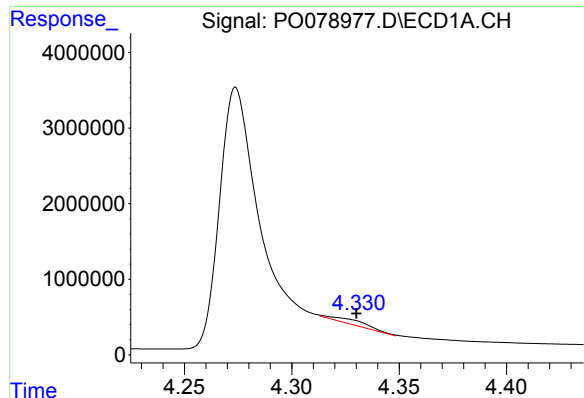


#1 Tetrachloro-m-xylene

R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 749326
Conc: 9.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
JEB542P-N-2


Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:20 PM

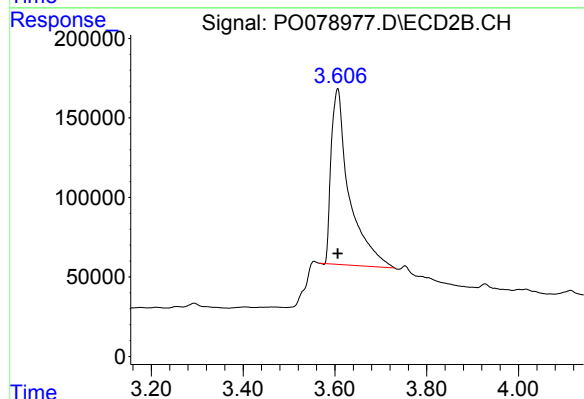


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.000 min
Response: 3013940
Conc: 101.41 ng/ml

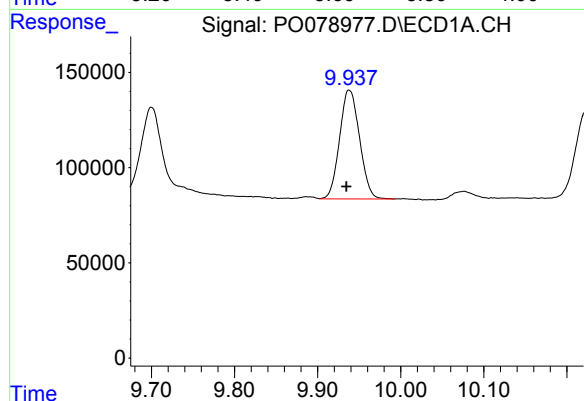

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: 0.002 min
Response: 953785
Conc: 15.27 ng/ml m

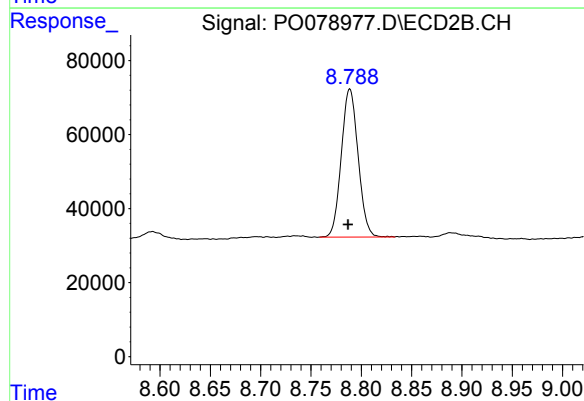

#2 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: 0.002 min
Response: 464240
Conc: 15.58 ng/ml