

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078985.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 16:30
 Operator : DD\AJ
 Sample : M2768-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-061721

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:13:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.604	1573772	629618	19.941	21.184
2) SA Decachlor...	9.936	8.786	997934	503402	15.979	16.893

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
Data File : P0078985.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 16:30
Operator : DD\AJ
Sample : M2768-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-01-061721

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:13:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

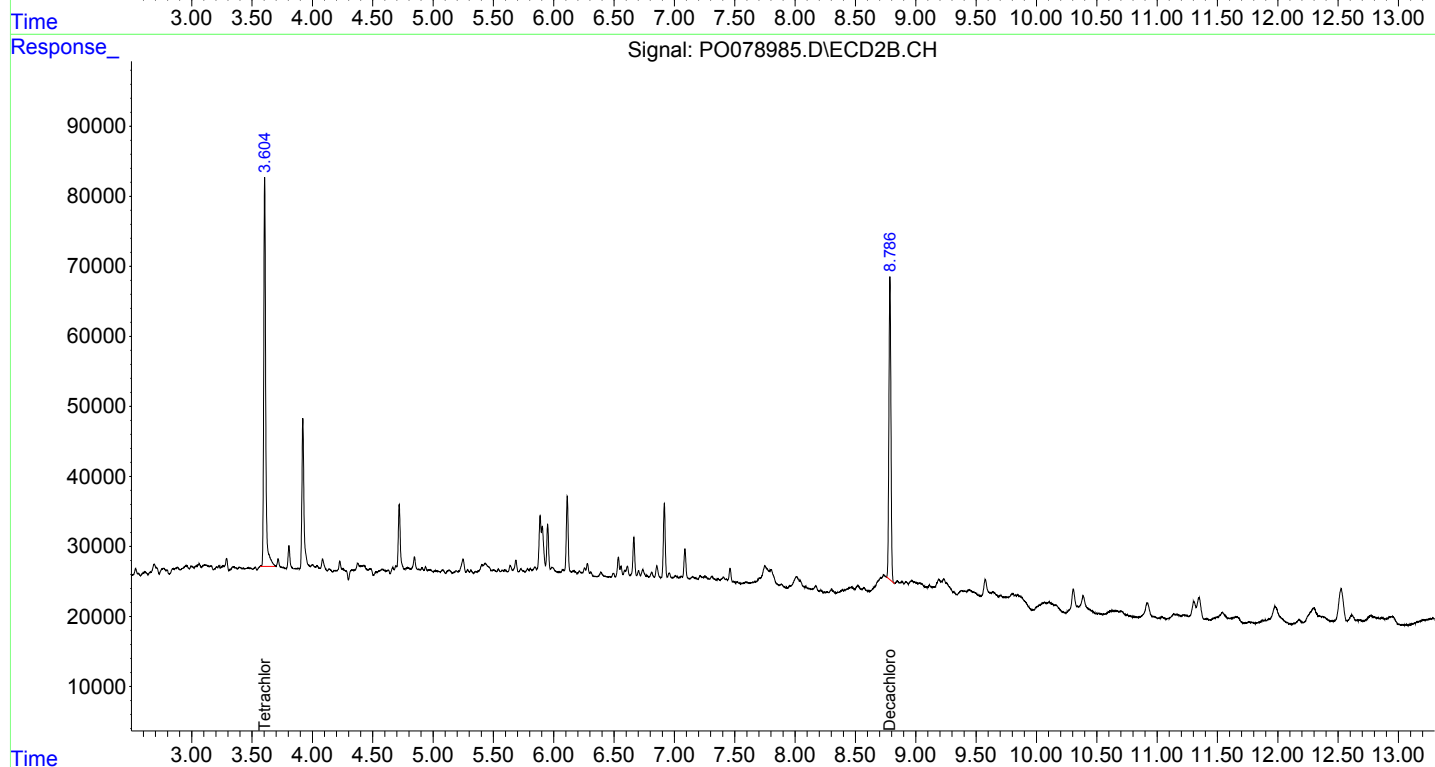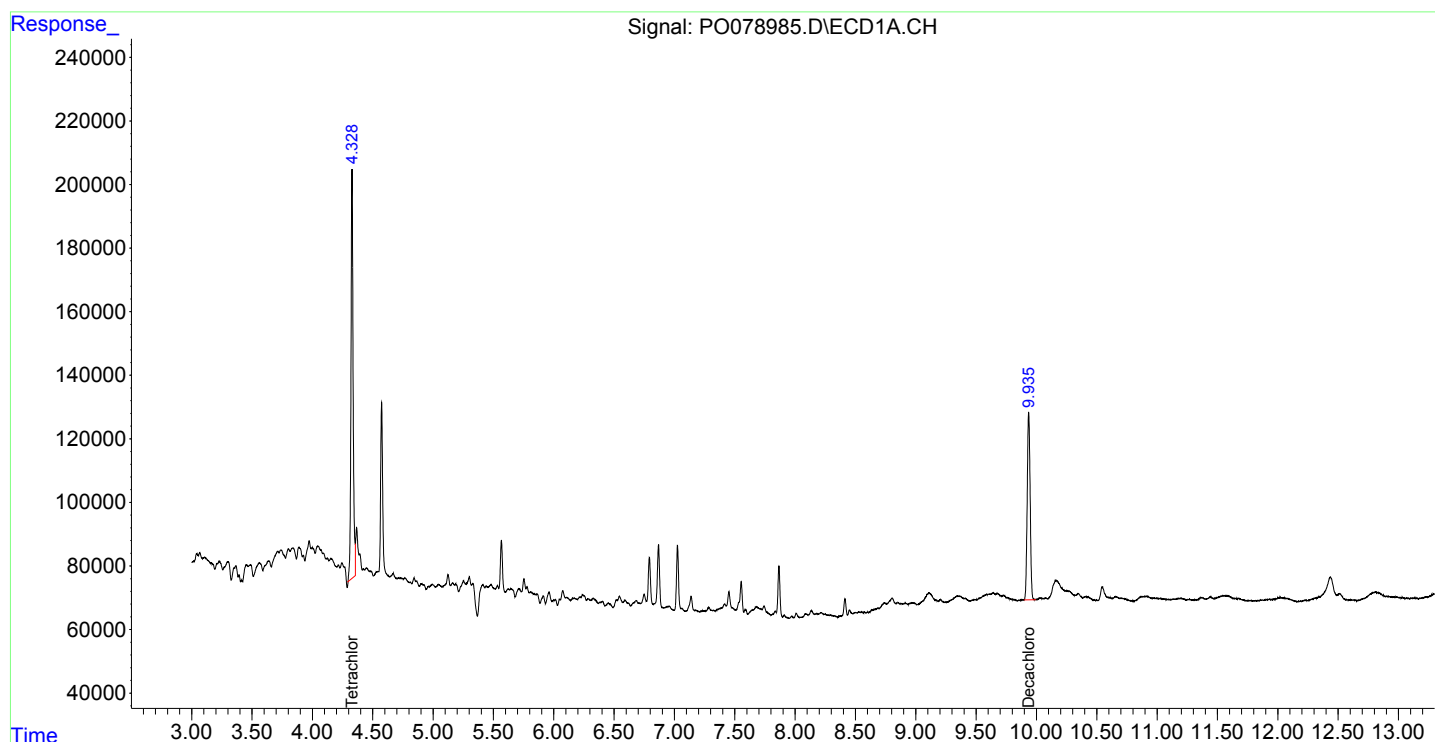


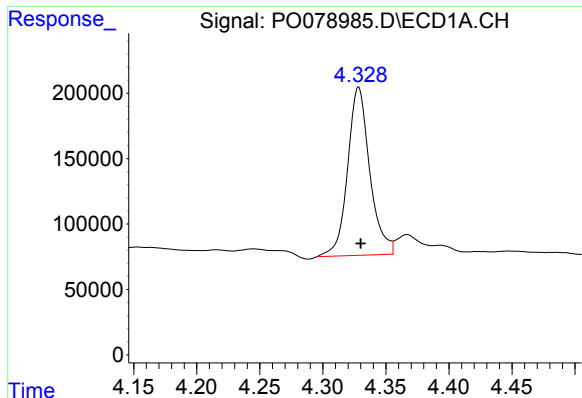

#1 Tetrachloro-m-xylene


R.T.: 4.328 min
Delta R.T.: -0.002 min
Response: 1573772
Conc: 19.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-061721

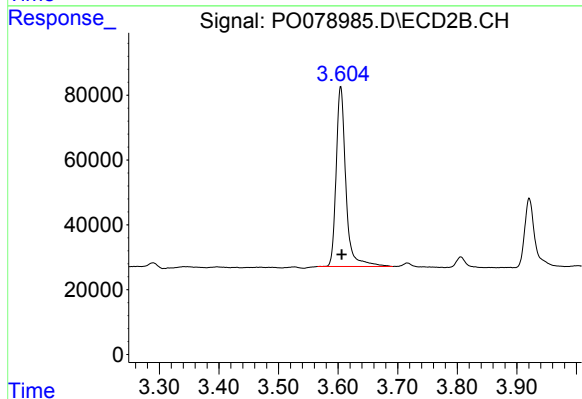


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.002 min
Response: 629618
Conc: 21.18 ng/ml

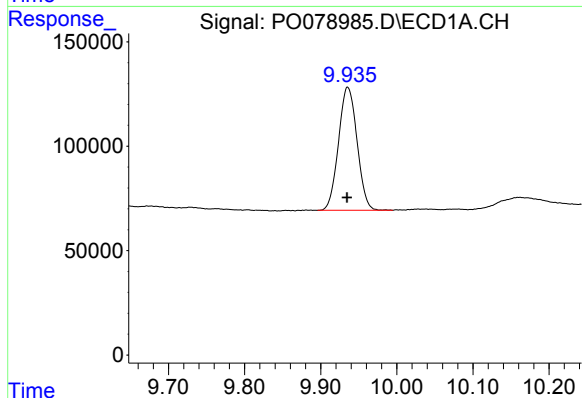

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.000 min
Response: 997934
Conc: 15.98 ng/ml

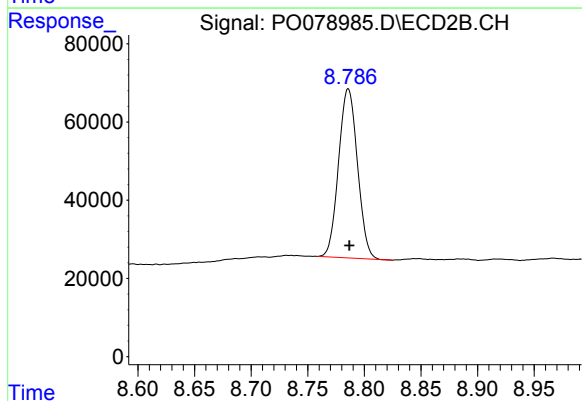

#2 Decachlorobiphenyl

R.T.: 8.786 min
Delta R.T.: -0.001 min
Response: 503402
Conc: 16.89 ng/ml