

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078993.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 18:49
 Operator : DD\AJ
 Sample : M2776-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0339-DISCRETE-CORE-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:17:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.330	3.605	1151696	608777	14.593	20.483 #
2) SA Decachlor...	9.938	8.788	411492	256290	6.589	8.601 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062121\
Data File : PO078993.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 18:49
Operator : DD\AJ
Sample : M2776-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0339-DISCRETE-CORE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:17:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

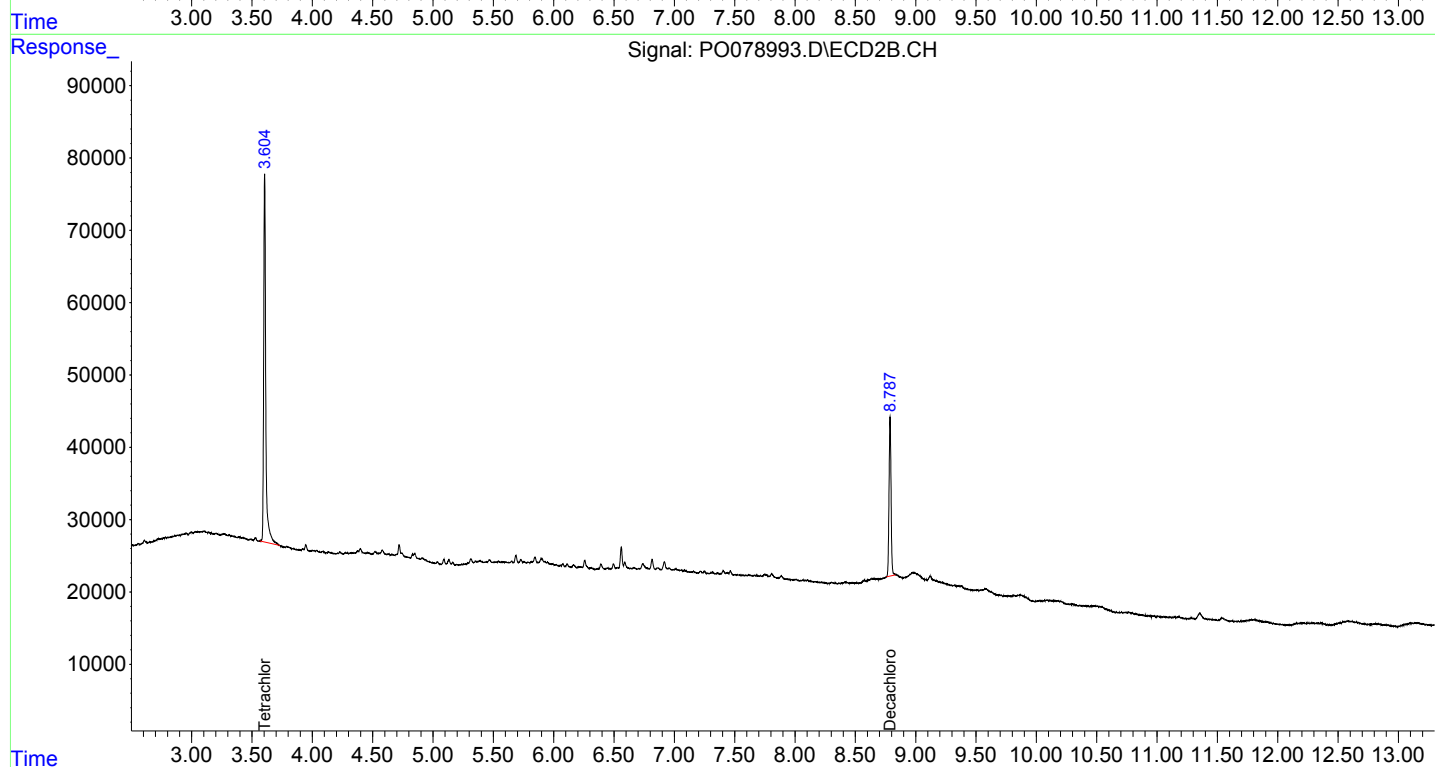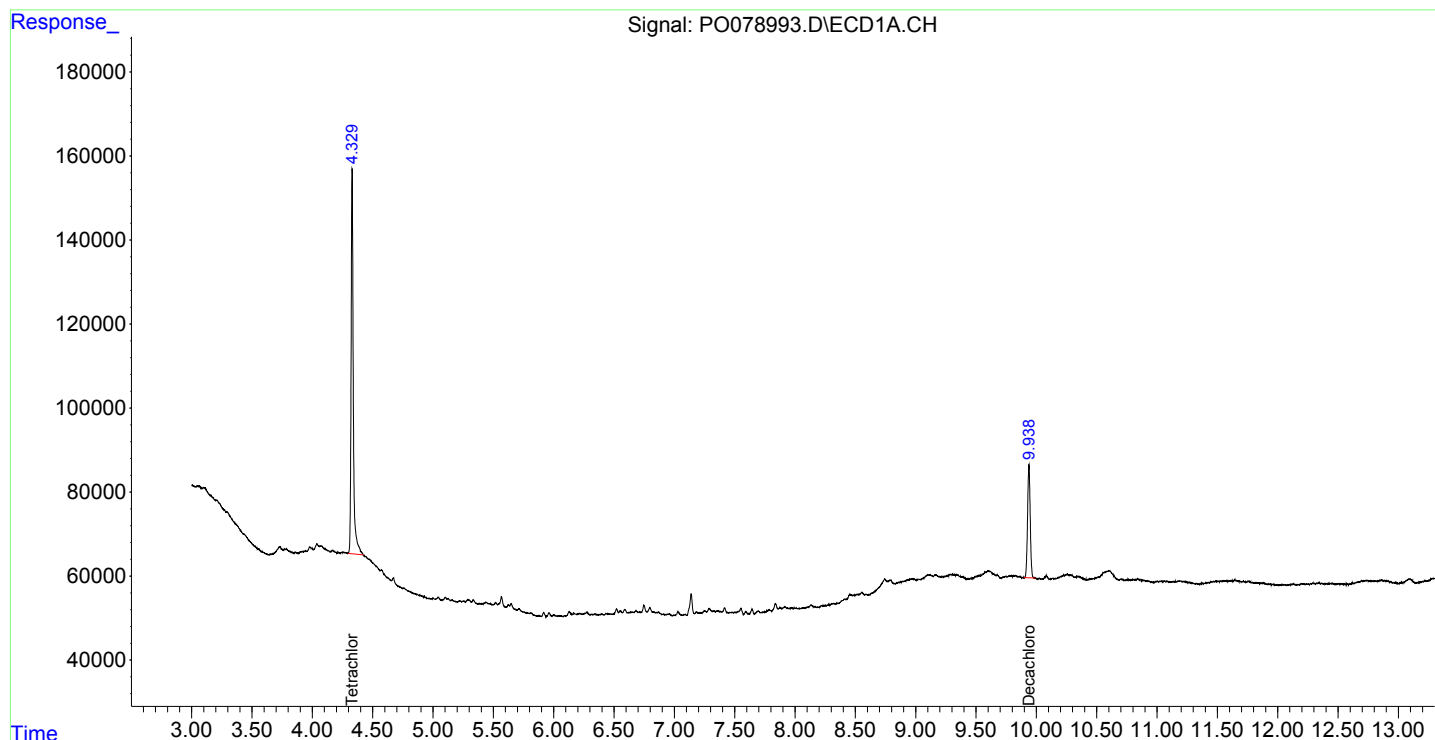


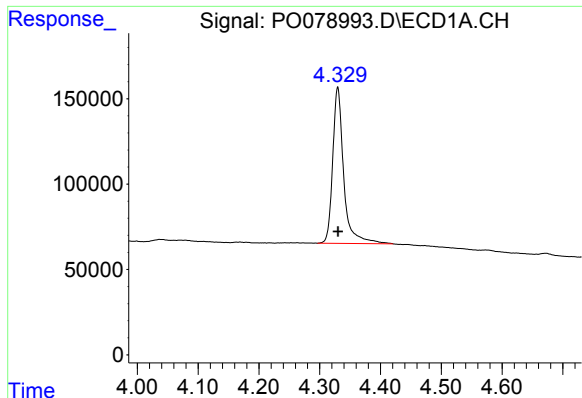

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 1151696
Conc: 14.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
0339-DISCRETE-CORE-1

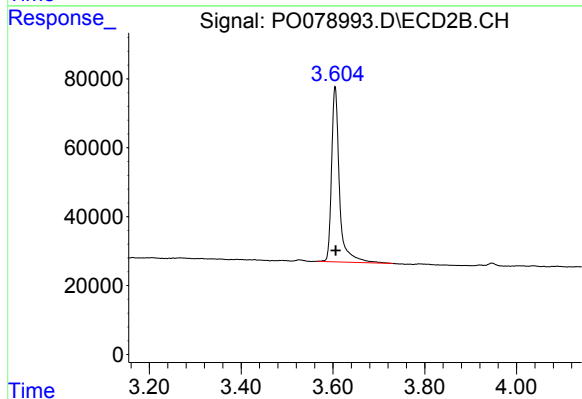


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.001 min
Response: 608777
Conc: 20.48 ng/ml

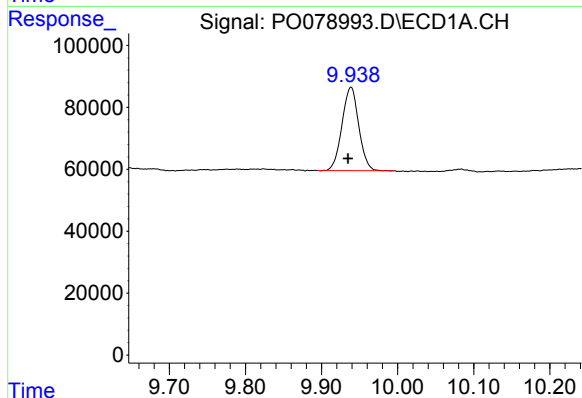

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.004 min
Response: 411492
Conc: 6.59 ng/ml

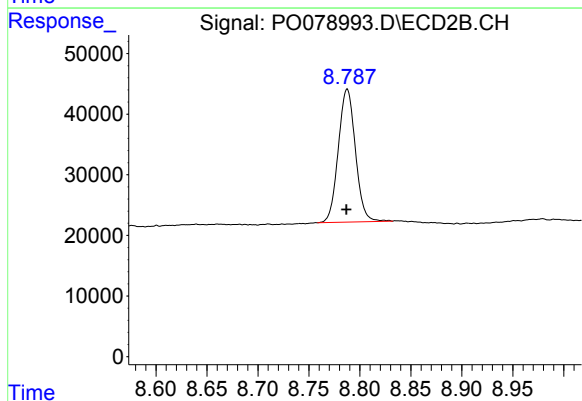

#2 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: 0.000 min
Response: 256290
Conc: 8.60 ng/ml