

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
 Data File : P0078996.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2021 20:17
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:18:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.604	4863703	1860551	61.626	62.601
2) SA Decachlor...	9.936	8.785	2528961	1374119	40.493	46.114
Target Compounds						
26) L6 AR-1254-1	6.518	5.685	1389023	962917	515.687	579.586
27) L6 AR-1254-2	6.745	5.843	1991972	847476	474.911	575.062
28) L6 AR-1254-3	7.121	6.256	2081587	1293539	467.396	581.570
29) L6 AR-1254-4	7.415	6.494	1402484	801445	455.800	589.434 #
30) L6 AR-1254-5	7.837	6.916	1473962	1122844	451.535m	563.914

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 6/22/2021 12:20:32 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062121\
Data File : P0078996.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2021 20:17
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:18:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleID :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:32 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

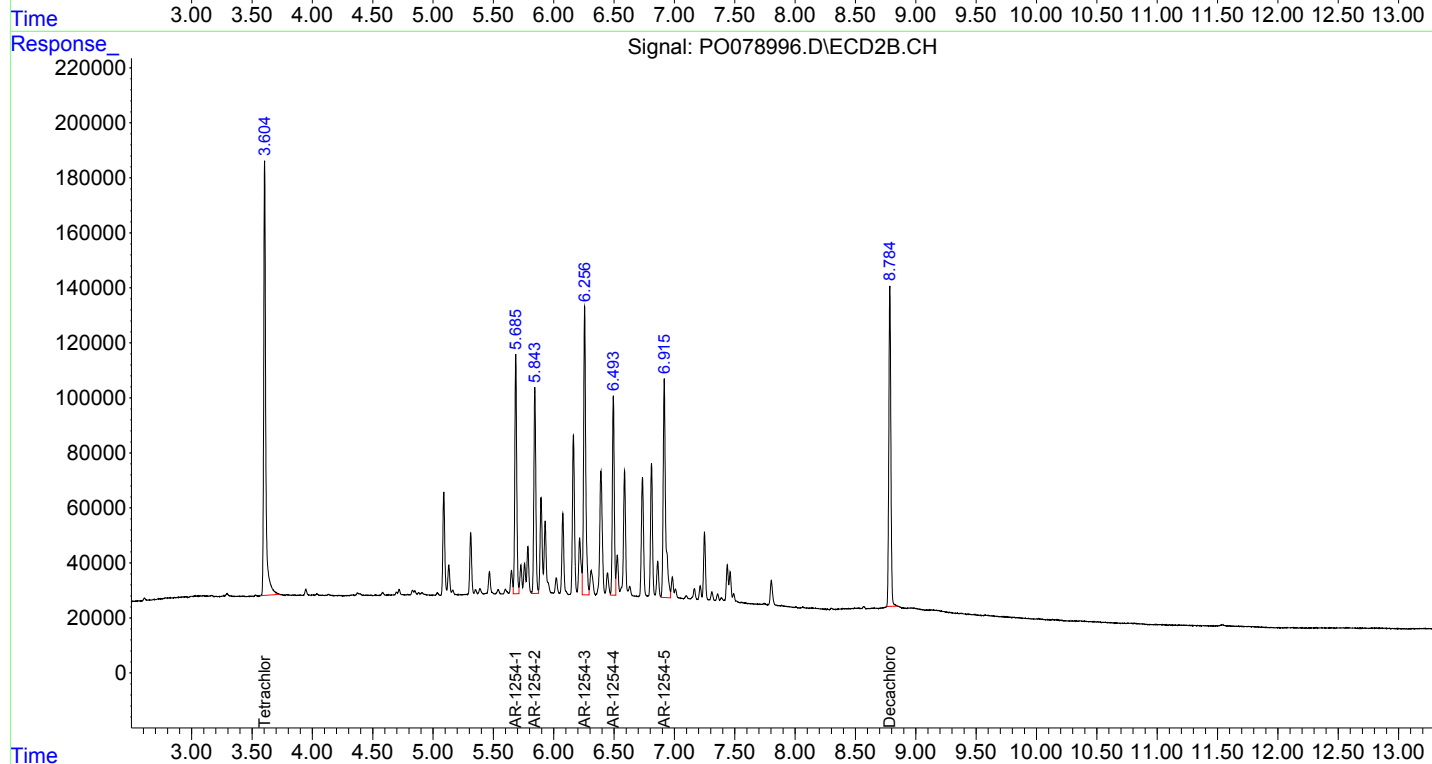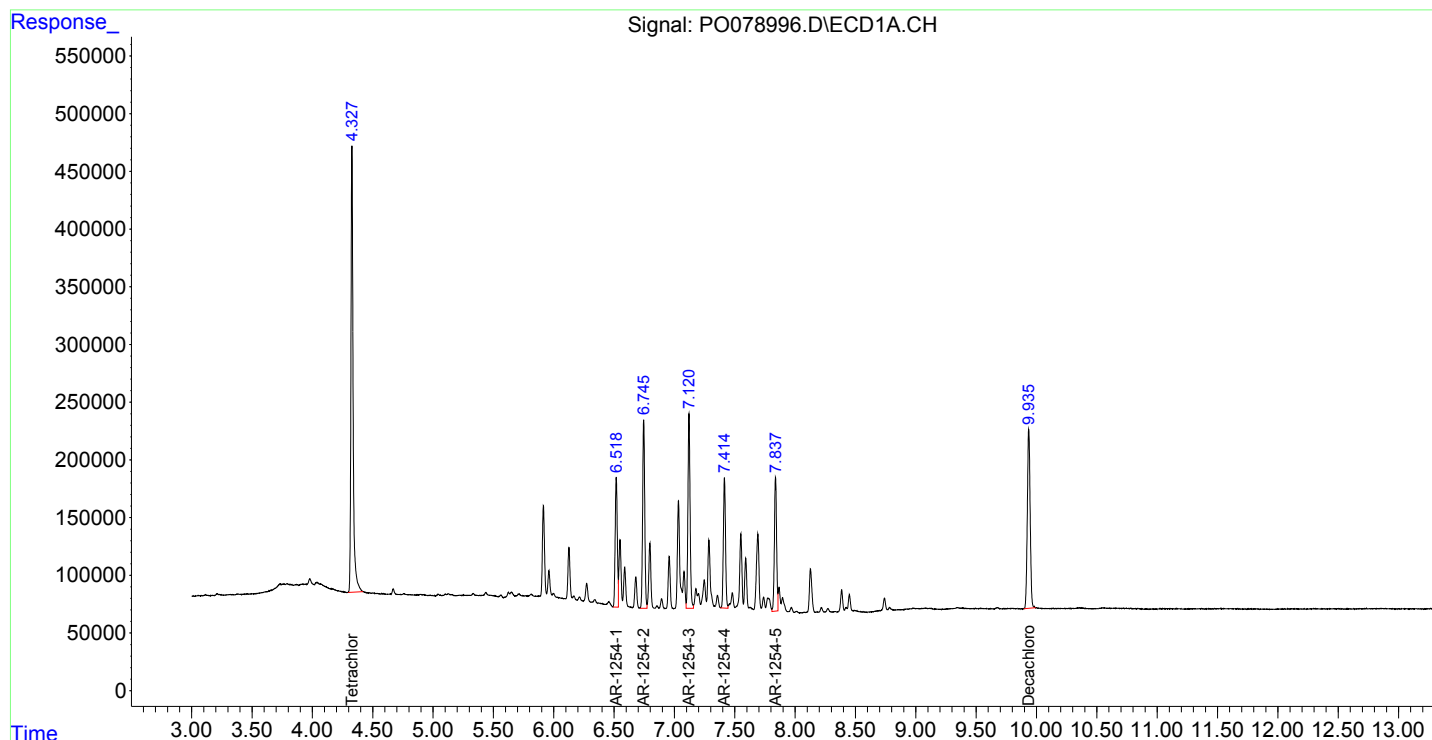

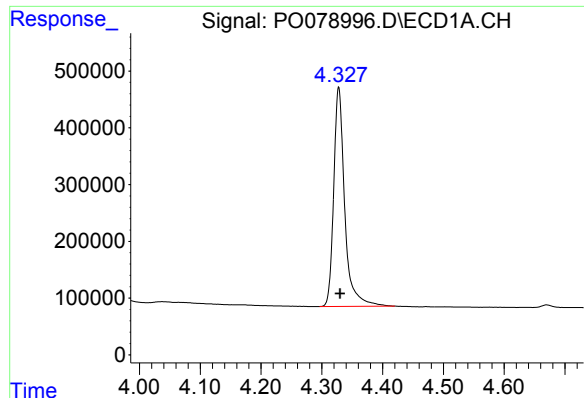


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.002 min
Response: 4863703
Conc: 61.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:32 PM

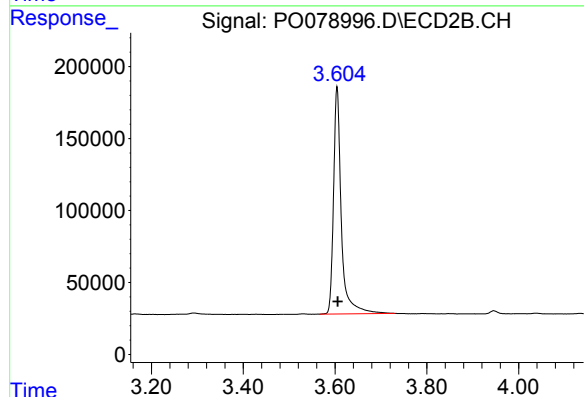


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.002 min
Response: 1860551
Conc: 62.60 ng/ml

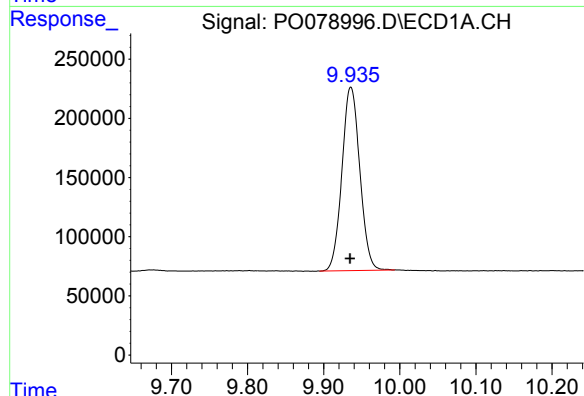


#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.000 min
Response: 2528961
Conc: 40.49 ng/ml

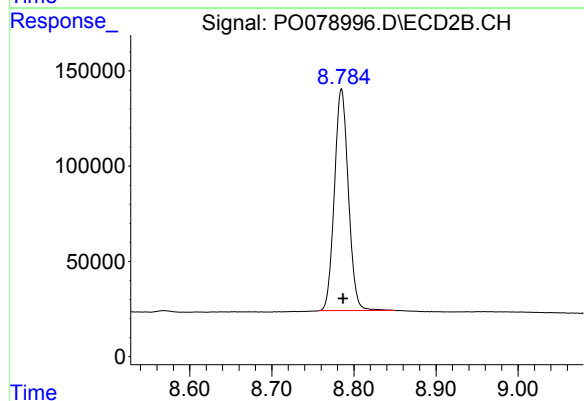

#2 Decachlorobiphenyl

R.T.: 8.785 min
Delta R.T.: -0.002 min
Response: 1374119
Conc: 46.11 ng/ml

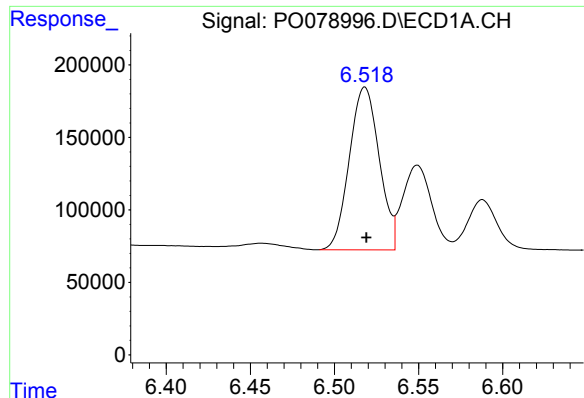


#26 AR-1254-1

R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 1389023
Conc: 515.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:32 PM

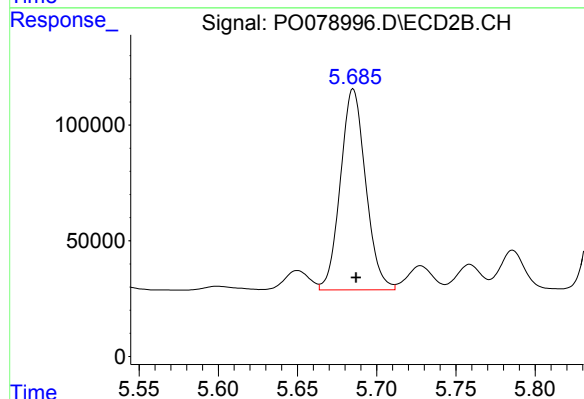


#26 AR-1254-1

R.T.: 5.685 min
Delta R.T.: -0.002 min
Response: 962917
Conc: 579.59 ng/ml

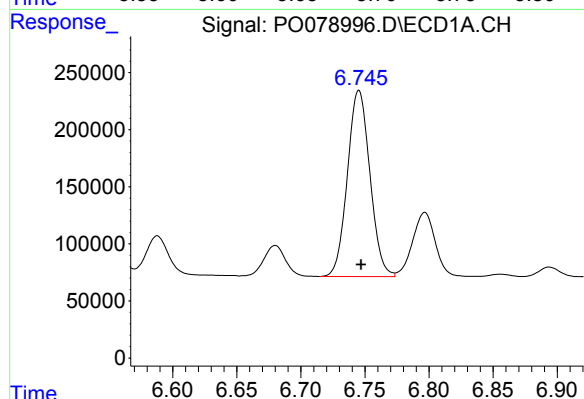


#27 AR-1254-2

R.T.: 6.745 min
Delta R.T.: -0.002 min
Response: 1991972
Conc: 474.91 ng/ml

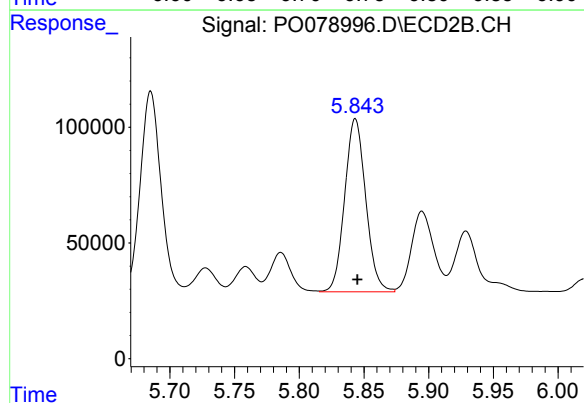

#27 AR-1254-2

R.T.: 5.843 min
Delta R.T.: -0.002 min
Response: 847476
Conc: 575.06 ng/ml

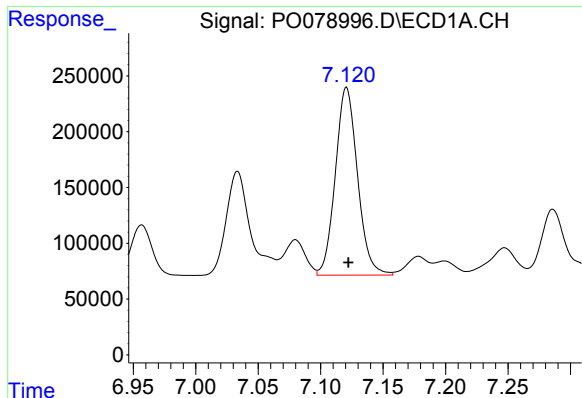


#28 AR-1254-3

R.T.: 7.121 min
Delta R.T.: -0.002 min
Response: 2081587
Conc: 467.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:32 PM

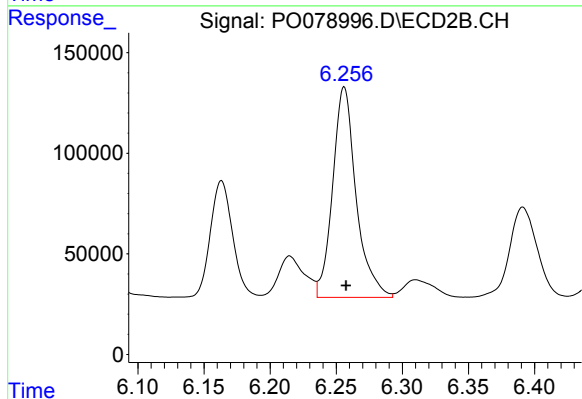


#28 AR-1254-3

R.T.: 6.256 min
Delta R.T.: -0.001 min
Response: 1293539
Conc: 581.57 ng/ml

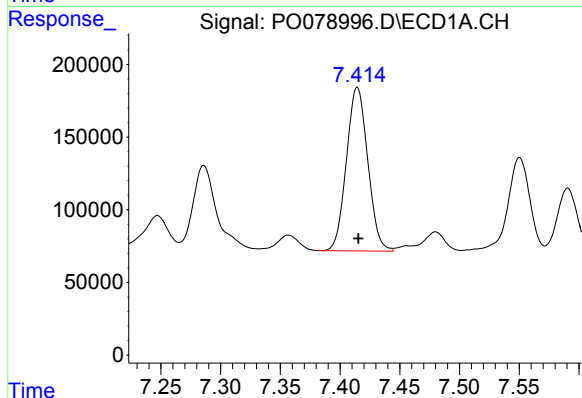


#29 AR-1254-4

R.T.: 7.415 min
Delta R.T.: 0.000 min
Response: 1402484
Conc: 455.80 ng/ml

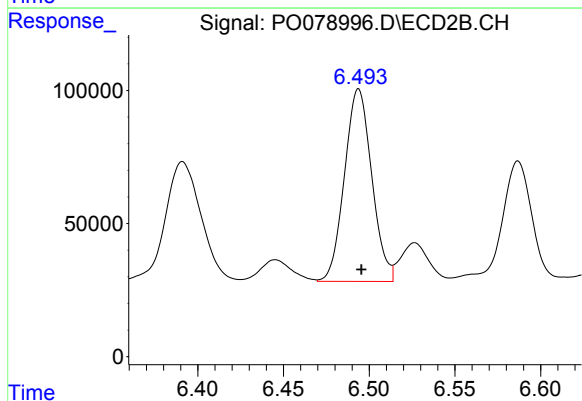

#29 AR-1254-4


R.T.: 6.494 min
Delta R.T.: -0.002 min
Response: 801445
Conc: 589.43 ng/ml

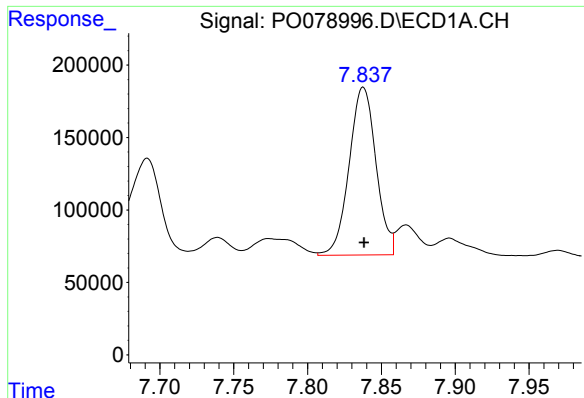

#30 AR-1254-5

R.T.: 7.837 min
Delta R.T.: -0.001 min
Response: 1473962
Conc: 451.54 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

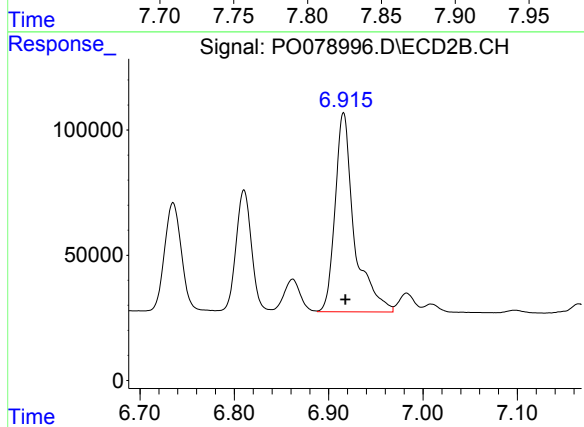

#30 AR-1254-5

R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 1122844
Conc: 563.91 ng/ml

Manual Integrations
APPROVED

Ankita
6/22/2021 12:20:32 PM