

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 15:06
 Operator : DD\AJ
 Sample : M2797-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:40:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.328	3.604	1931020	723625	24.467	24.347
2)	SA Decachlor...	9.934	8.784	1191000	595425	19.070	19.982
Target Compounds							
5)	L1 AR-1016-3	5.713	0.000	81319	0	32.372	N.D. #
8)	L2 AR-1221-1	4.574	0.000	76957	0	92.569	N.D. #
9)	L2 AR-1221-2	4.670	0.000	31070	0	51.007	N.D. #
18)	L4 AR-1242-3	5.713	0.000	81319	0	43.941	N.D. #
20)	L4 AR-1242-5	6.584	0.000	227036	0	146.951	N.D. #
25)	L5 AR-1248-5	6.584	0.000	227036	0	83.100	N.D. #
28)	L6 AR-1254-3	7.138f	0.000	165932	0	37.258	N.D. #
32)	L7 AR-1260-2	7.530f	0.000	37682	0	9.695	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
Data File : P0079017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 15:06
Operator : DD\AJ
Sample : M2797-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:40:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

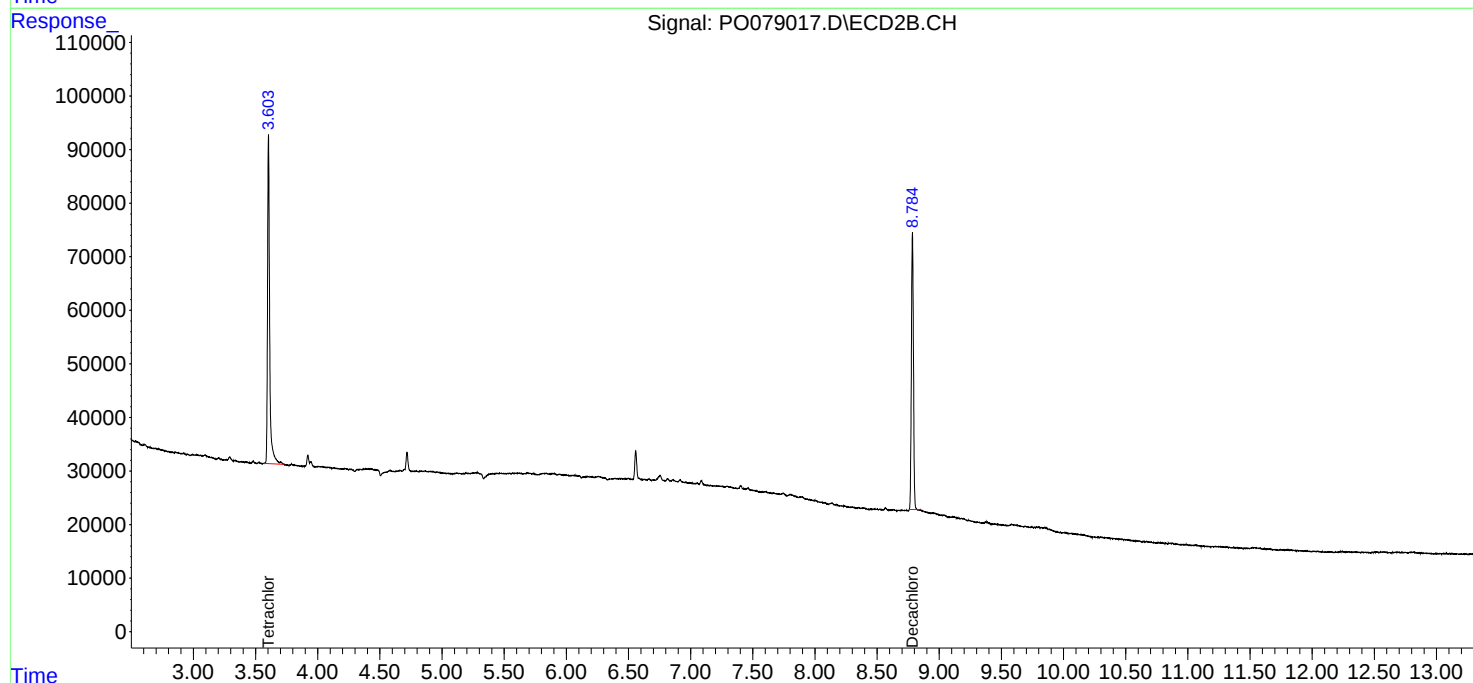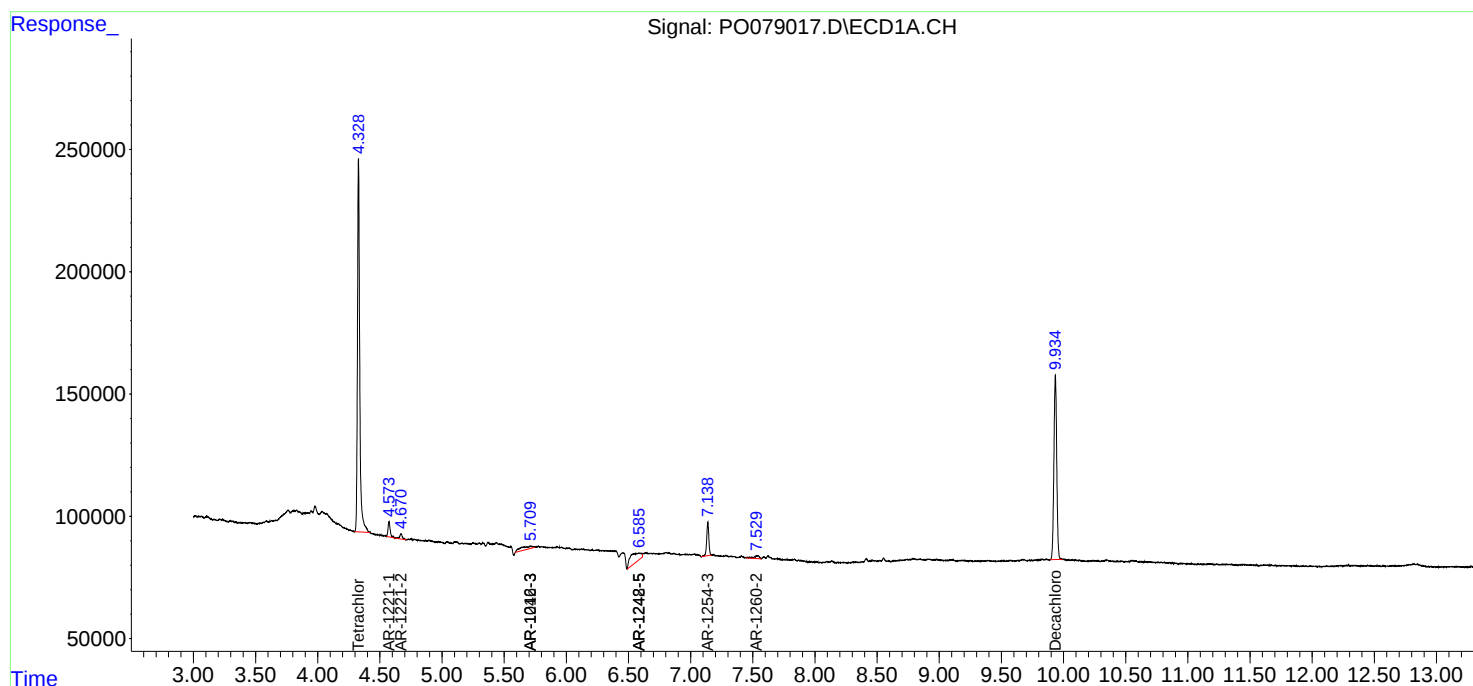


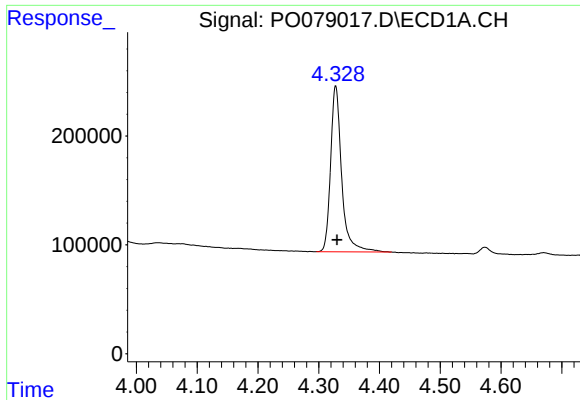

#1 Tetrachloro-m-xylene


R.T.: 4.328 min
Delta R.T.: -0.002 min
Response: 1931020
Conc: 24.47 ng/ml

Instrument :
ECD_O
ClientSampleId :

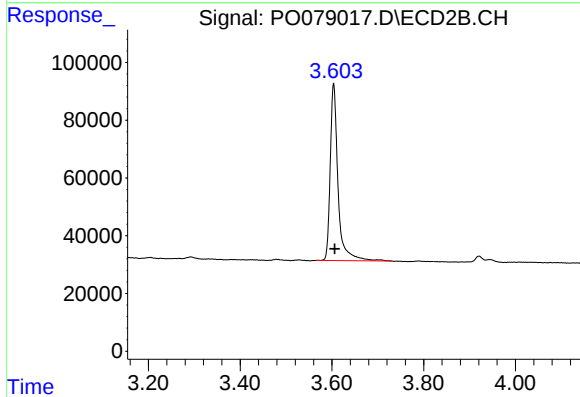


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.002 min
Response: 723625
Conc: 24.35 ng/ml

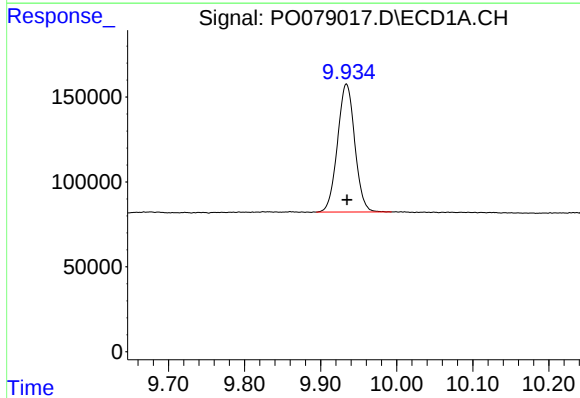


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.000 min
Response: 1191000
Conc: 19.07 ng/ml

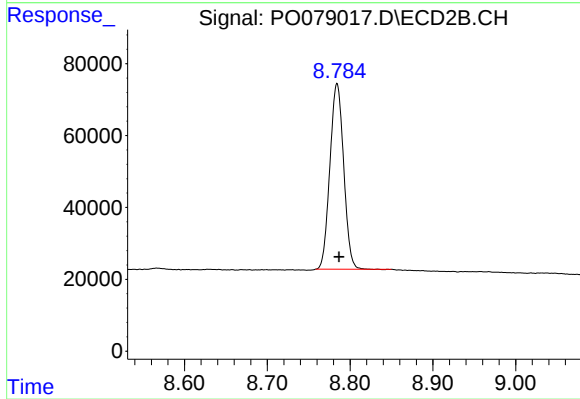

#2 Decachlorobiphenyl


R.T.: 8.784 min
Delta R.T.: -0.003 min
Response: 595425
Conc: 19.98 ng/ml

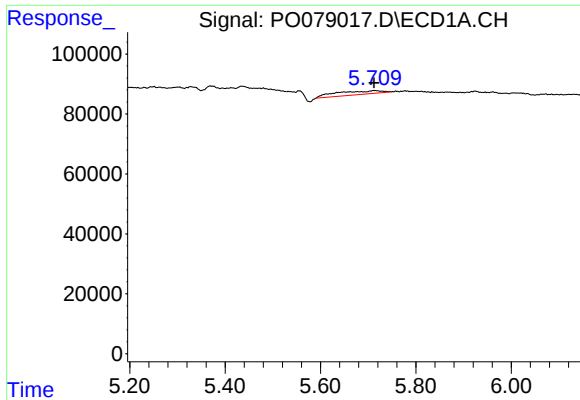

#5 AR-1016-3


R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 81319
Conc: 32.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

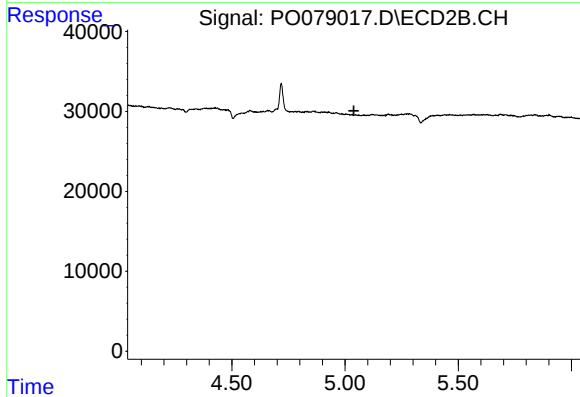


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

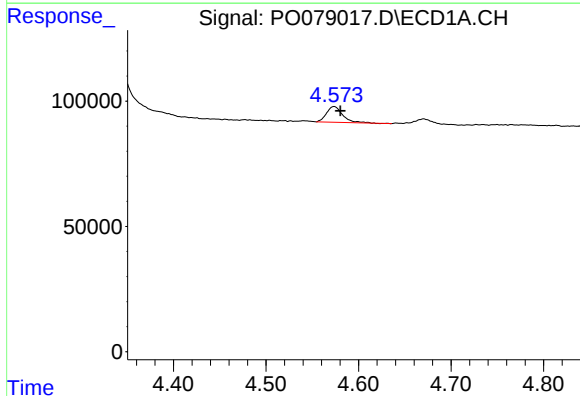


#8 AR-1221-1

R.T.: 4.574 min
Delta R.T.: -0.007 min
Response: 76957
Conc: 92.57 ng/ml

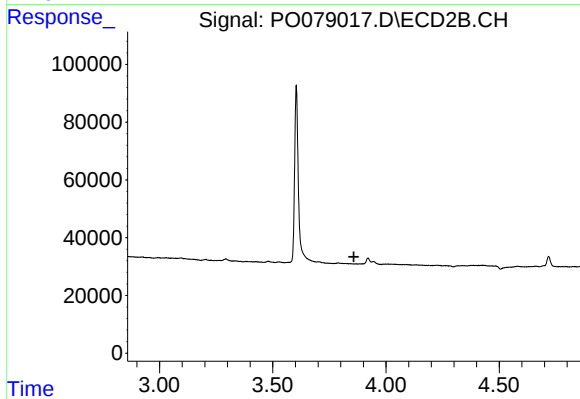

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.858 min
Response: 0
Conc: N.D.

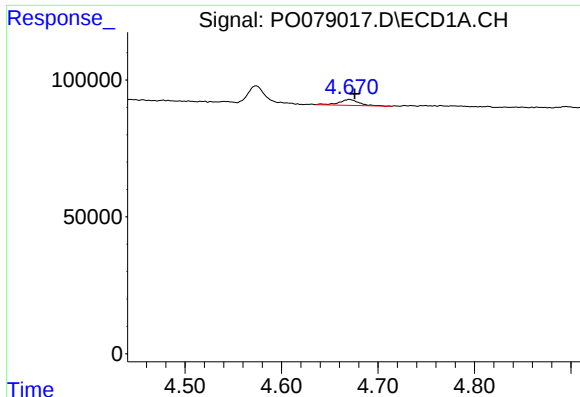

#9 AR-1221-2


R.T.: 4.670 min
Delta R.T.: -0.006 min
Response: 31070
Conc: 51.01 ng/ml

Instrument :
ECD_O
ClientSampleId :

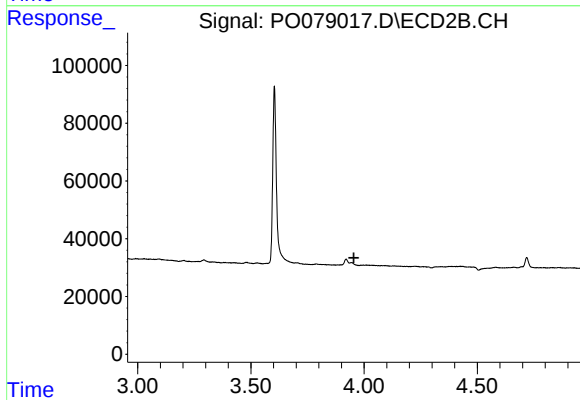


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.955 min
Response: 0
Conc: N.D.

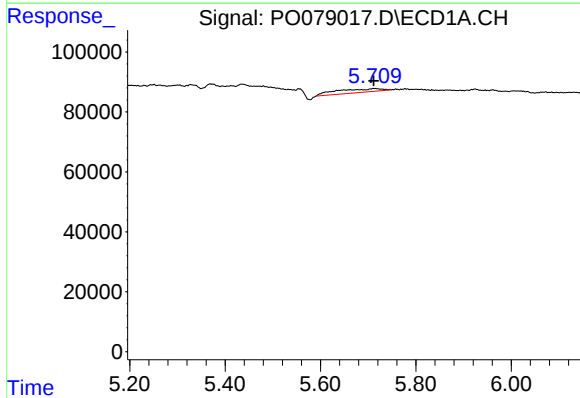


#18 AR-1242-3

R.T.: 5.713 min
Delta R.T.: 0.002 min
Response: 81319
Conc: 43.94 ng/ml

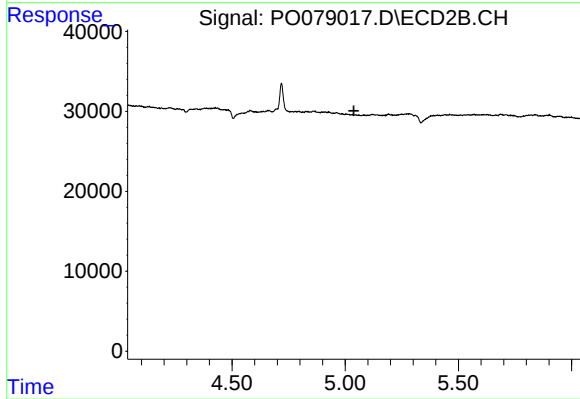

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.038 min
Response: 0
Conc: N.D.

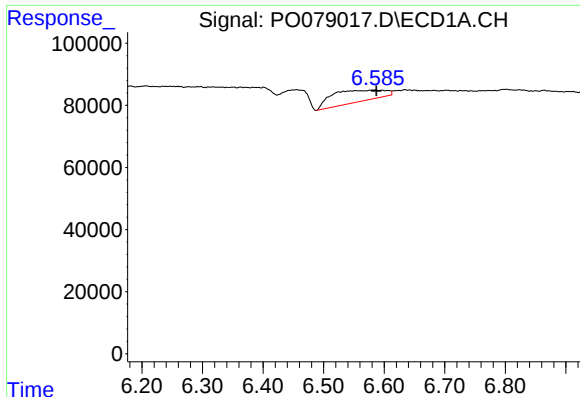

#20 AR-1242-5


R.T.: 6.584 min
Delta R.T.: -0.003 min
Response: 227036
Conc: 146.95 ng/ml

Instrument :
ECD_O
ClientSampleId :

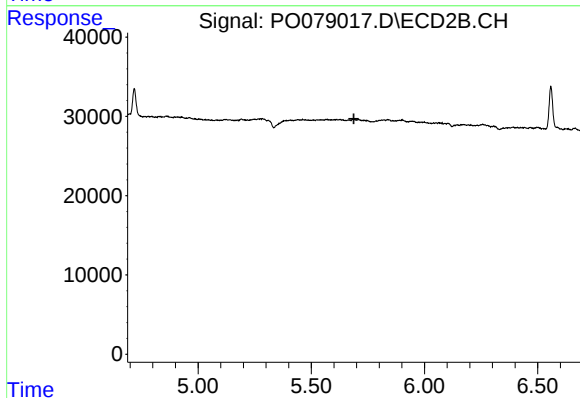


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

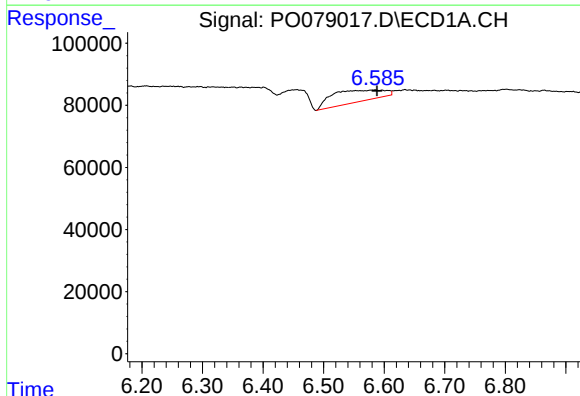


#25 AR-1248-5

R.T.: 6.584 min
Delta R.T.: -0.005 min
Response: 227036
Conc: 83.10 ng/ml

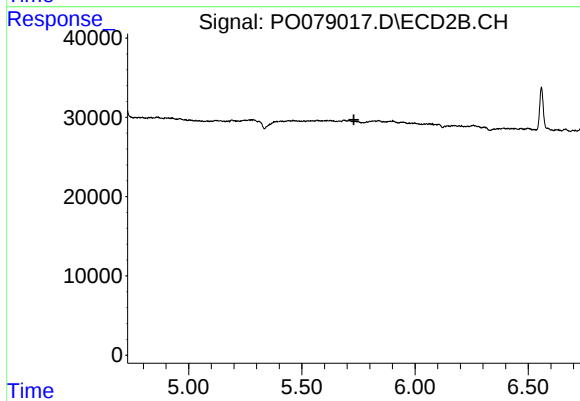

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.730 min
Response: 0
Conc: N.D.

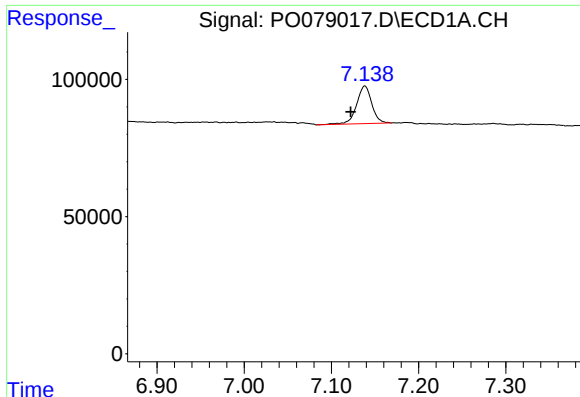

#28 AR-1254-3


R.T.: 7.138 min
Delta R.T.: 0.016 min
Response: 165932
Conc: 37.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

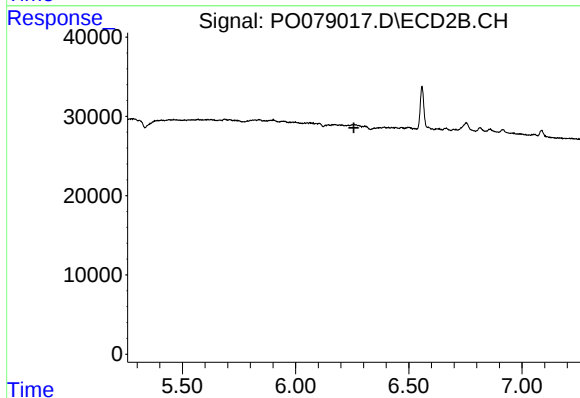


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.

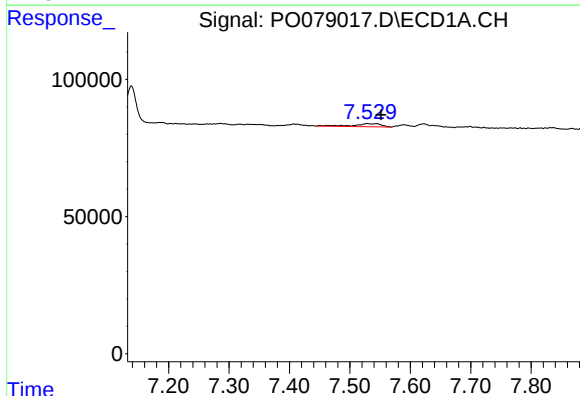

#32 AR-1260-2

R.T.: 7.530 min
Delta R.T.: -0.022 min
Response: 37682
Conc: 9.70 ng/ml

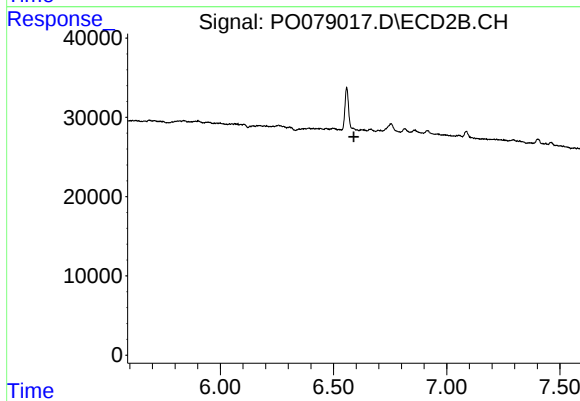

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.590 min
Response: 0
Conc: N.D.