

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 16:40
 Operator : DD\AJ
 Sample : M2797-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:43:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.333	3.604	1799390	661683	22.799	22.263
2)	SA Decachlor...	9.938	8.785	963352	497256	15.425	16.687
Target Compounds							
5)	L1 AR-1016-3	5.718	0.000	41151	0	16.382	N.D. #
8)	L2 AR-1221-1	4.579	0.000	216781	0	260.758	N.D. #
9)	L2 AR-1221-2	4.675	0.000	27505	0	45.156	N.D. #
18)	L4 AR-1242-3	5.718	0.000	41151	0	22.236	N.D. #
20)	L4 AR-1242-5	6.569f	0.000	81580	0	52.804	N.D. #
24)	L5 AR-1248-4	6.569f	0.000	81580	0	29.434	N.D. #
25)	L5 AR-1248-5	6.569f	0.000	81580	0	29.860	N.D. #
28)	L6 AR-1254-3	7.142f	0.000	63845	0	14.336	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
Data File : P0079022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 16:40
Operator : DD\AJ
Sample : M2797-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:43:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

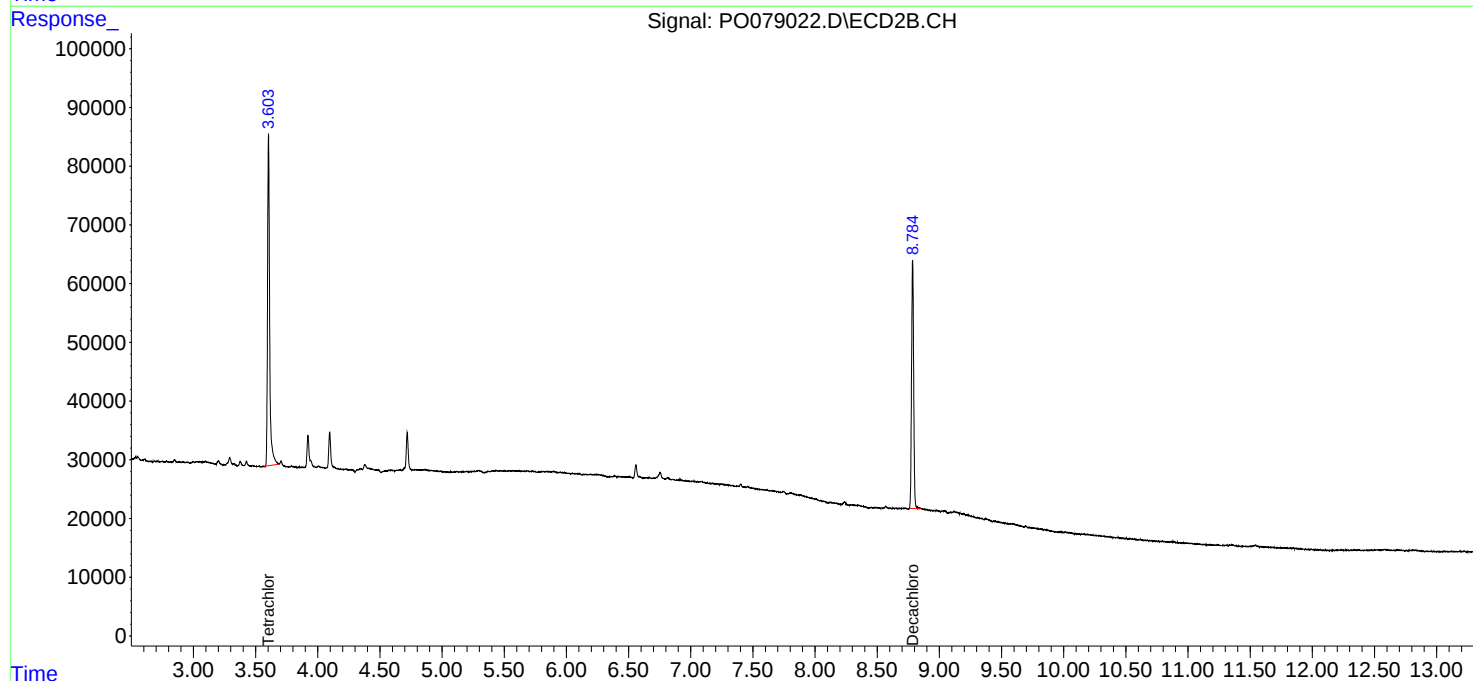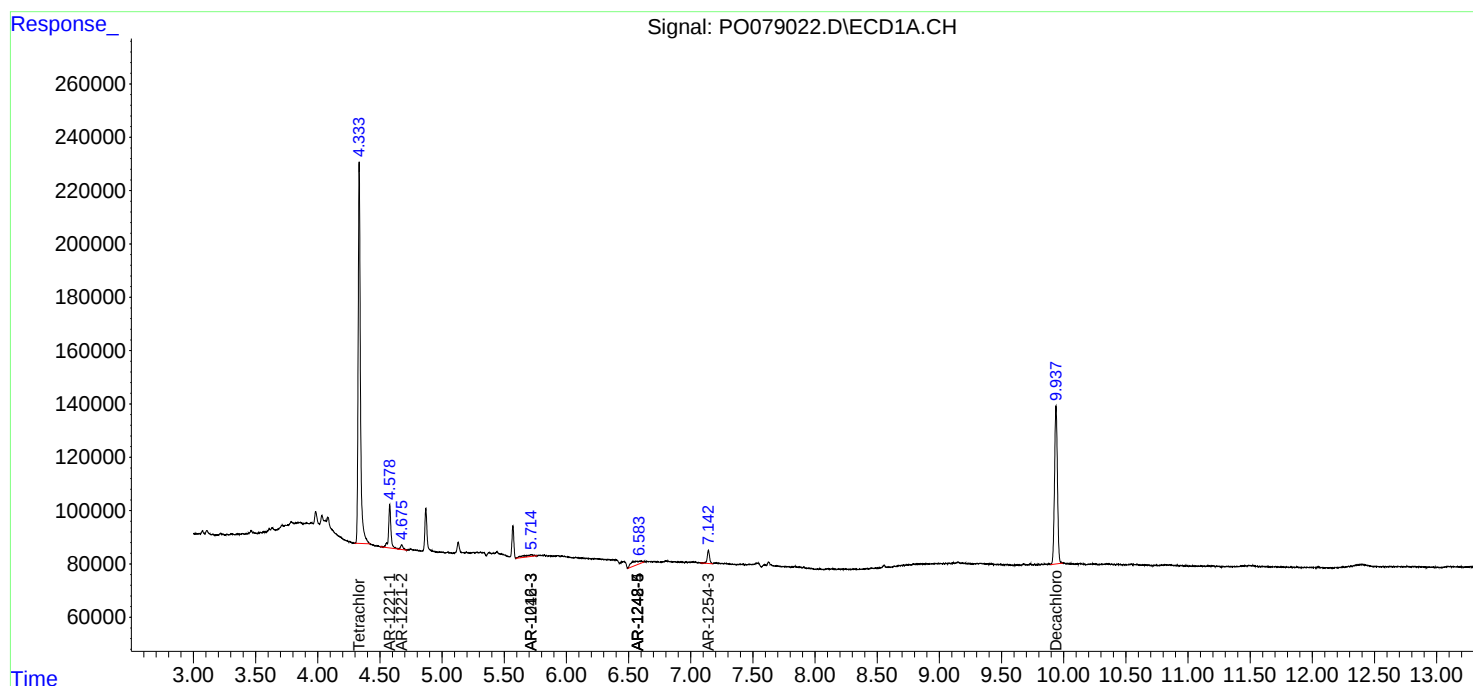


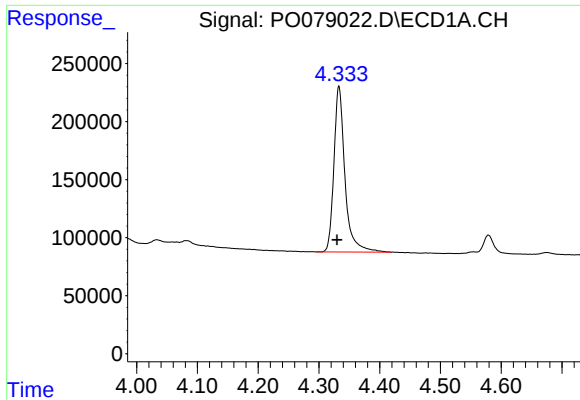

#1 Tetrachloro-m-xylene


R.T.: 4.333 min
Delta R.T.: 0.003 min
Response: 1799390
Conc: 22.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

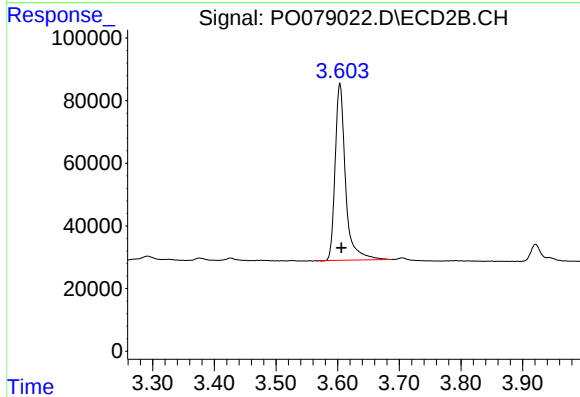


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.002 min
Response: 661683
Conc: 22.26 ng/ml

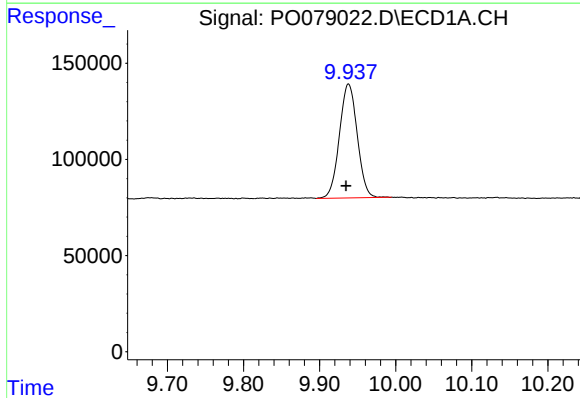


#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.003 min
Response: 963352
Conc: 15.42 ng/ml

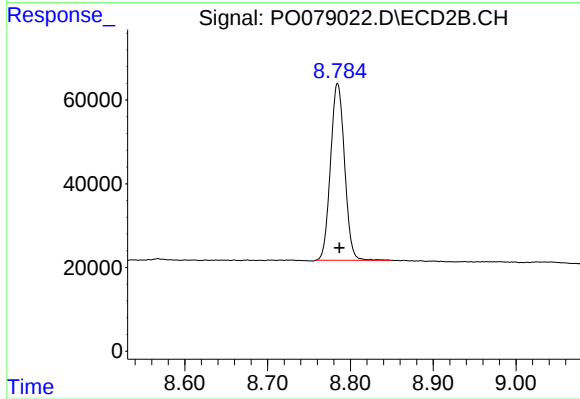

#2 Decachlorobiphenyl


R.T.: 8.785 min
Delta R.T.: -0.002 min
Response: 497256
Conc: 16.69 ng/ml

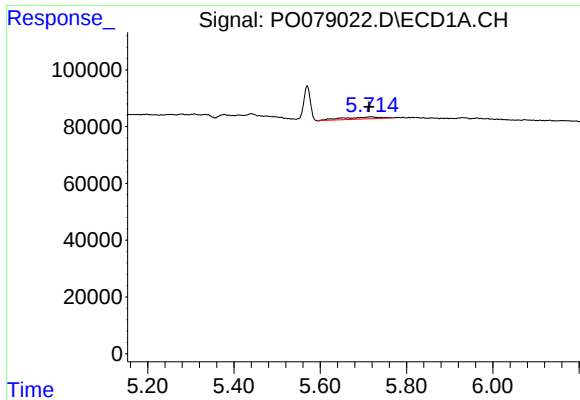

#5 AR-1016-3


R.T.: 5.718 min
Delta R.T.: 0.005 min
Response: 41151
Conc: 16.38 ng/ml

Instrument :
ECD_O
ClientSampleId :

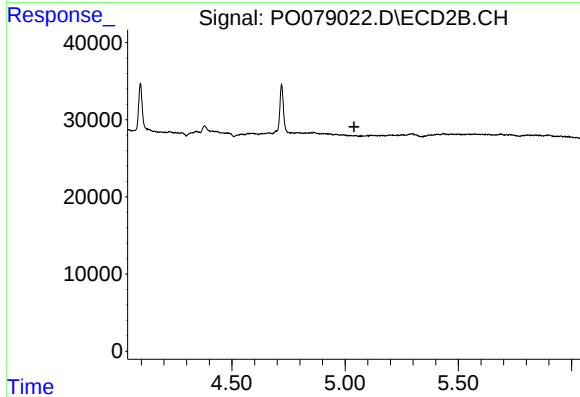


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

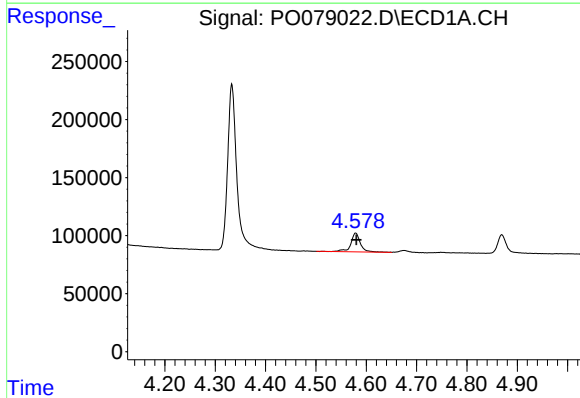


#8 AR-1221-1

R.T.: 4.579 min
Delta R.T.: -0.001 min
Response: 216781
Conc: 260.76 ng/ml

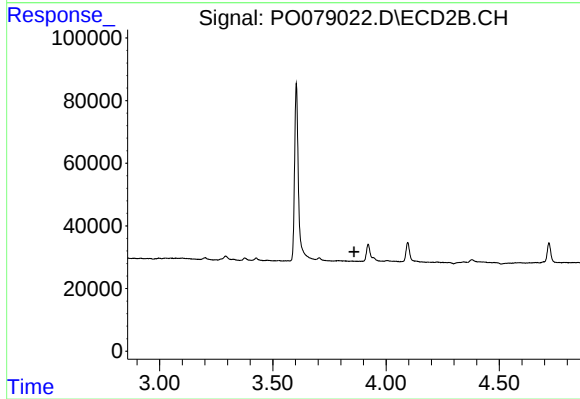

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.858 min
Response: 0
Conc: N.D.

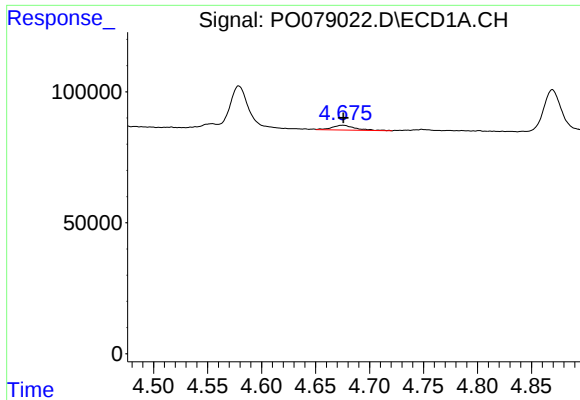

#9 AR-1221-2


R.T.: 4.675 min
Delta R.T.: 0.000 min
Response: 27505
Conc: 45.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

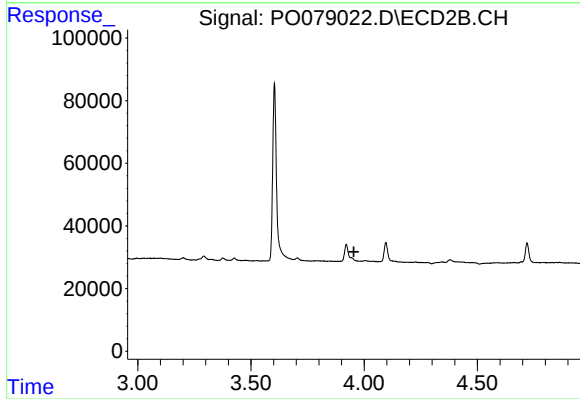


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.955 min
Response: 0
Conc: N.D.

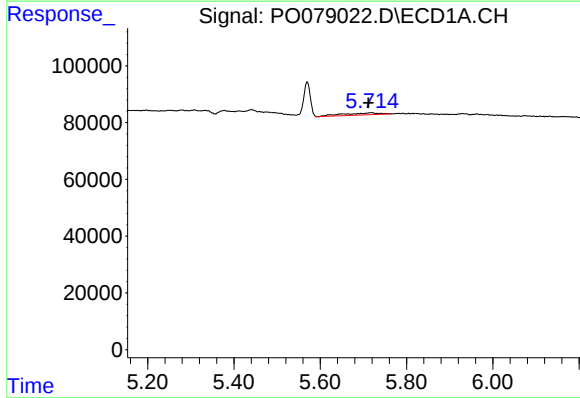


#18 AR-1242-3

R.T.: 5.718 min
Delta R.T.: 0.007 min
Response: 41151
Conc: 22.24 ng/ml

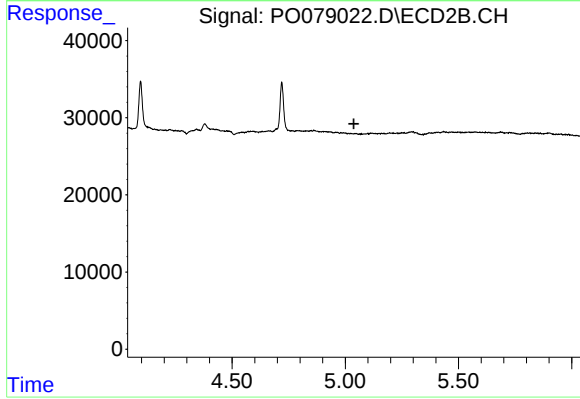

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.038 min
Response: 0
Conc: N.D.

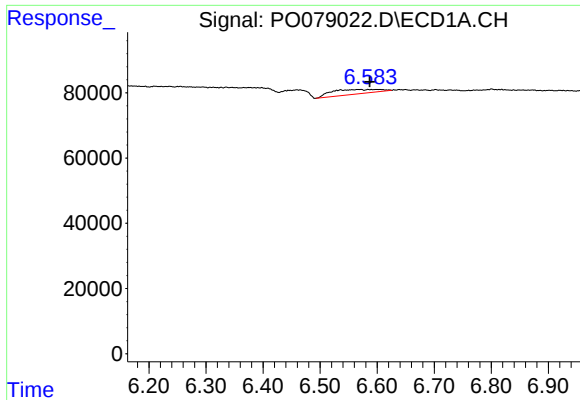

#20 AR-1242-5


R.T.: 6.569 min
Delta R.T.: -0.018 min
Response: 81580
Conc: 52.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

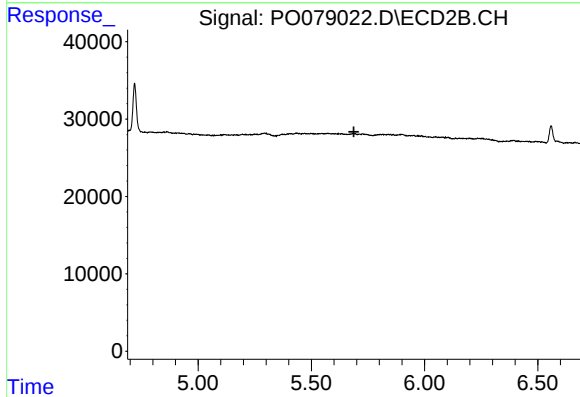


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.688 min
Response: 0
Conc: N.D.

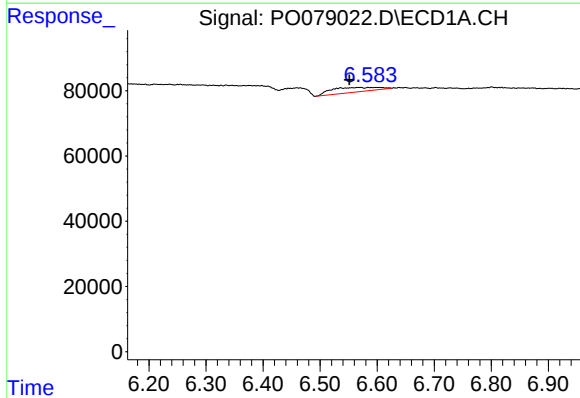


#24 AR-1248-4

R.T.: 6.569 min
Delta R.T.: 0.017 min
Response: 81580
Conc: 29.43 ng/ml

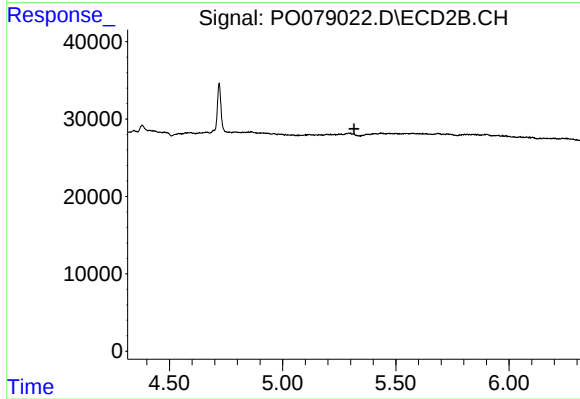

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.315 min
Response: 0
Conc: N.D.

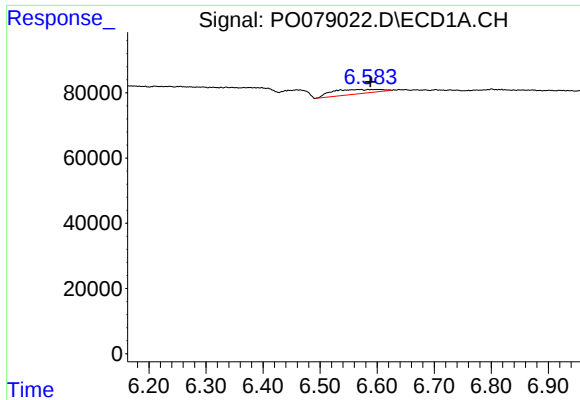

#25 AR-1248-5


R.T.: 6.569 min
Delta R.T.: -0.019 min
Response: 81580
Conc: 29.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

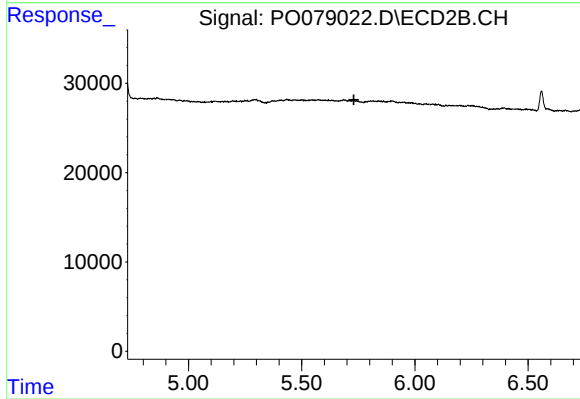


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.730 min
Response: 0
Conc: N.D.

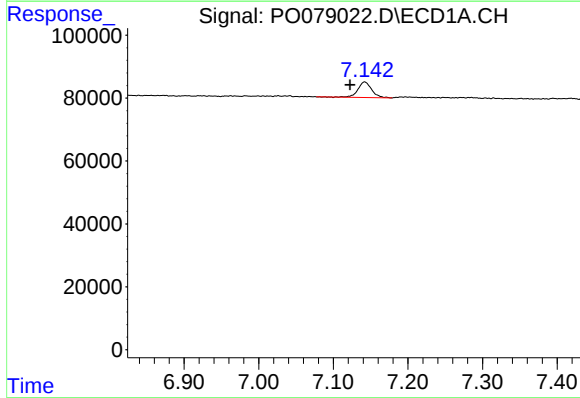

#28 AR-1254-3

R.T.: 7.142 min
Delta R.T.: 0.020 min
Response: 63845
Conc: 14.34 ng/ml

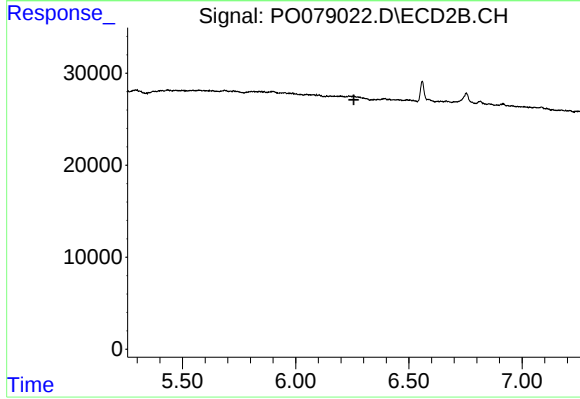

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.