

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079006.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 11:29
 Operator : DD\AJ
 Sample : M2794-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:32:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.603	1895420	722344	24.016	24.304
2) SA Decachlor...	9.933	8.784	1166052	582880	18.670	19.561
Target Compounds						
26) L6 AR-1254-1	6.529	5.683	64197	14356	23.834m	8.641 #
27) L6 AR-1254-2	6.743	5.842	73326	24978	17.482	16.949
28) L6 AR-1254-3	7.120	6.255	167161	59511	37.534m	26.756 #
29) L6 AR-1254-4	7.413	6.492	88183	29489	28.659	21.688
30) L6 AR-1254-5	7.835	6.915	148976	94308	45.638	47.363

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 15C-1

Manual Integrations
 APPROVED

Ankita
 6/23/2021 1:50:06 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
Data File : P0079006.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 11:29
Operator : DD\AJ
Sample : M2794-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:32:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleId :
15C-1

Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:06 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

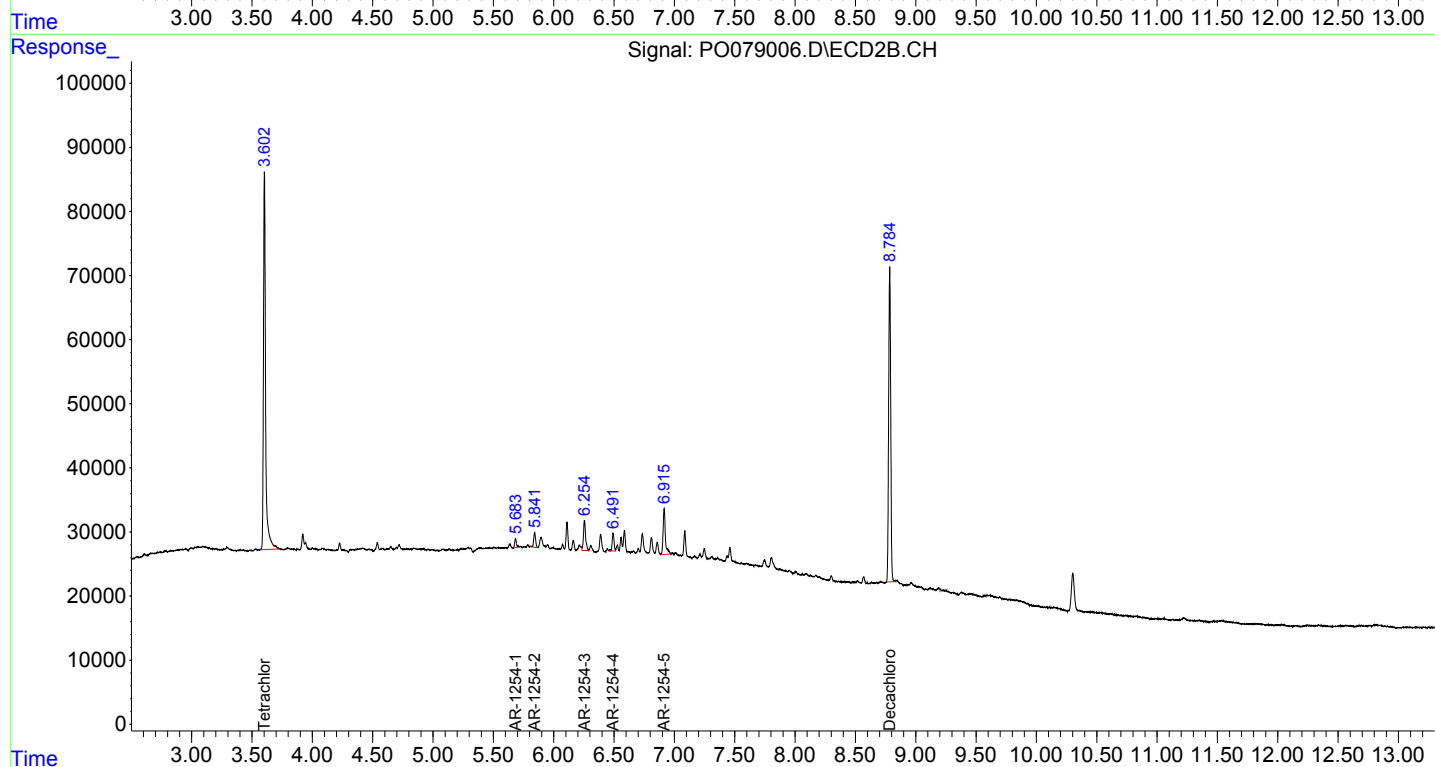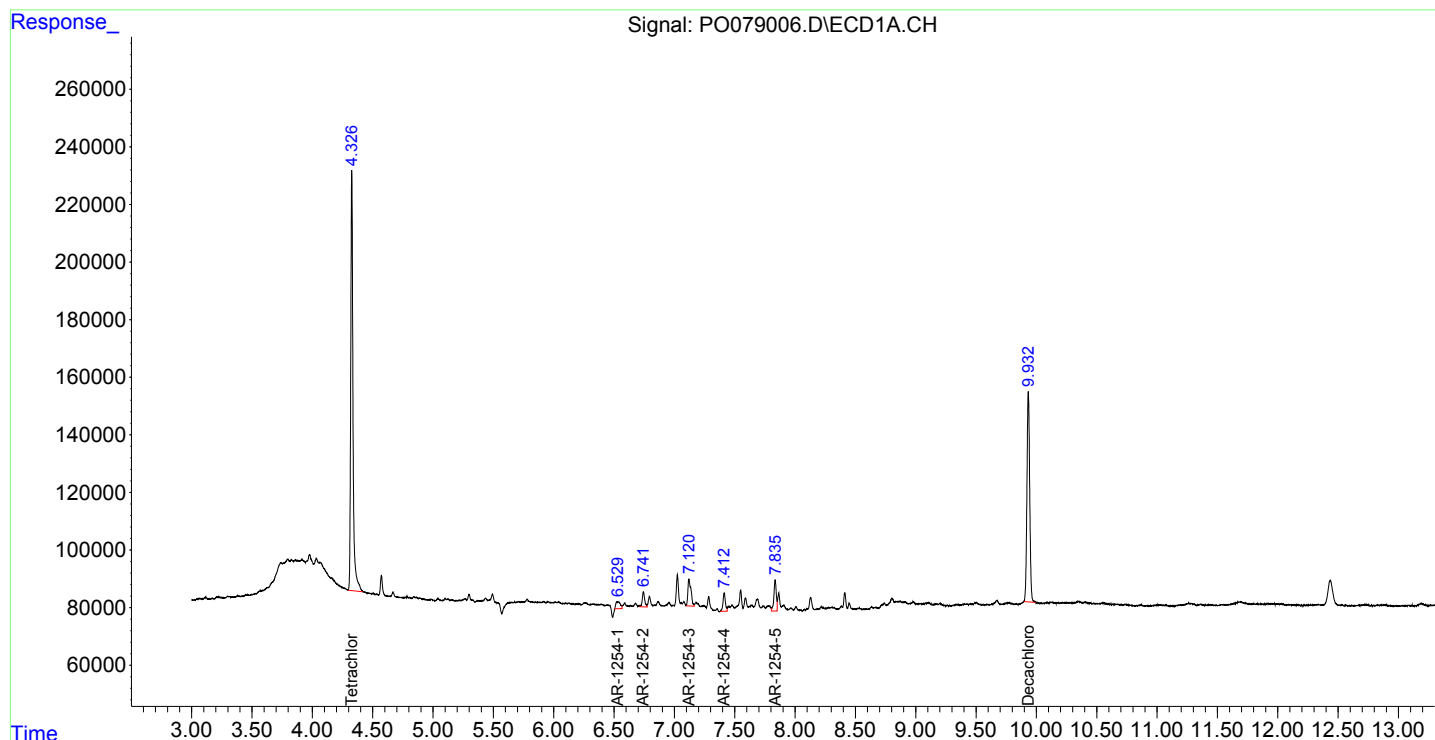

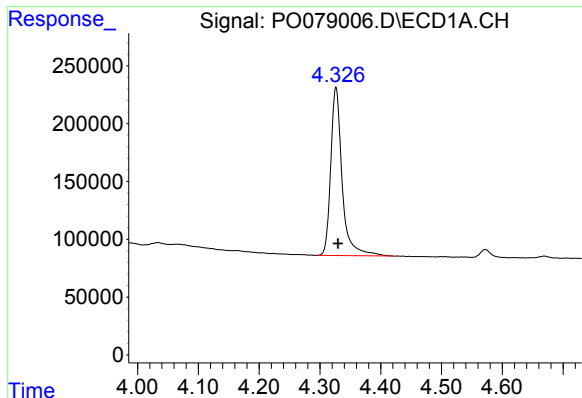


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: -0.004 min
Response: 1895420
Conc: 24.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
15C-1


Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:06 PM

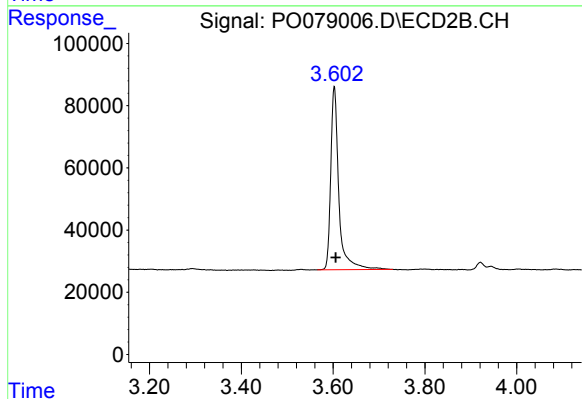


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.004 min
Response: 722344
Conc: 24.30 ng/ml

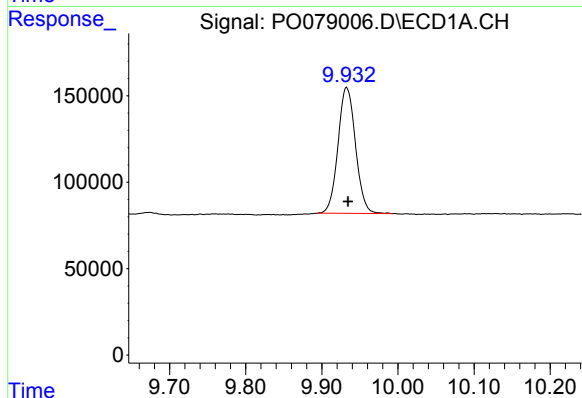


#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.002 min
Response: 1166052
Conc: 18.67 ng/ml

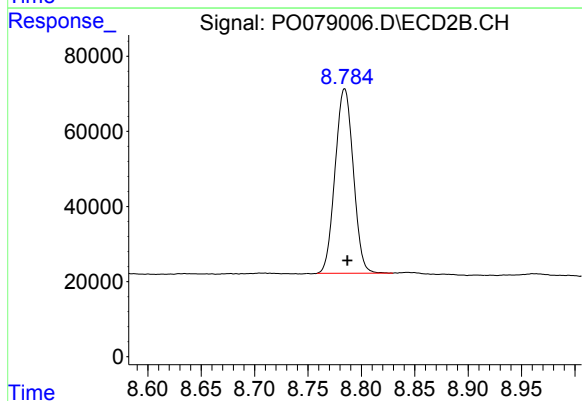

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: -0.002 min
Response: 582880
Conc: 19.56 ng/ml

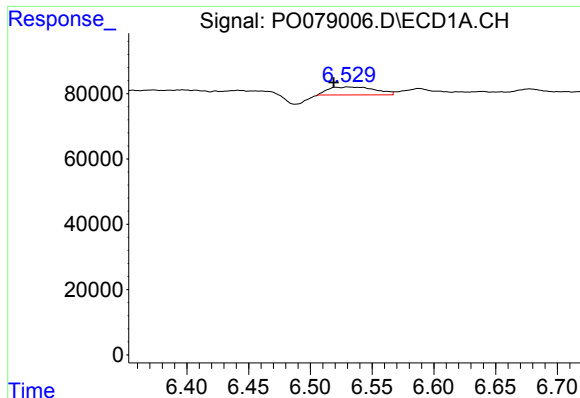


#26 AR-1254-1

R.T.: 6.529 min
Delta R.T.: 0.010 min
Response: 64197
Conc: 23.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
15C-1


Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:06 PM

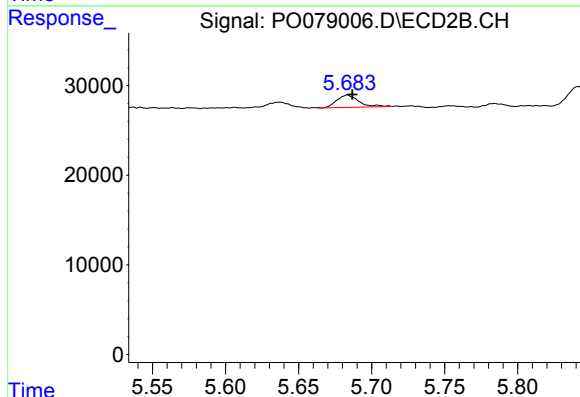


#26 AR-1254-1

R.T.: 5.683 min
Delta R.T.: -0.004 min
Response: 14356
Conc: 8.64 ng/ml

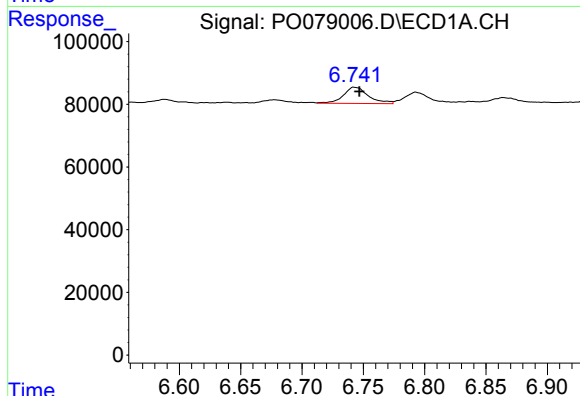


#27 AR-1254-2

R.T.: 6.743 min
Delta R.T.: -0.003 min
Response: 73326
Conc: 17.48 ng/ml

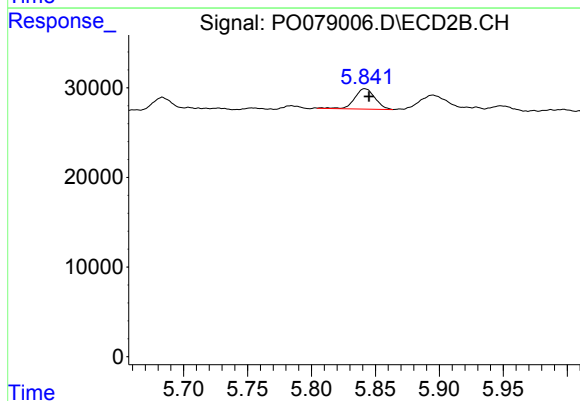

#27 AR-1254-2

R.T.: 5.842 min
Delta R.T.: -0.003 min
Response: 24978
Conc: 16.95 ng/ml

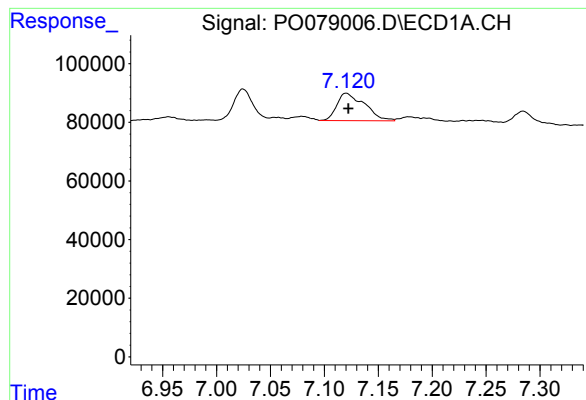


#28 AR-1254-3

R.T.: 7.120 min
Delta R.T.: -0.002 min
Response: 167161
Conc: 37.53 ng/ml m

Instrument :
ECD_O
ClientSampleId :
15C-1


Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:06 PM

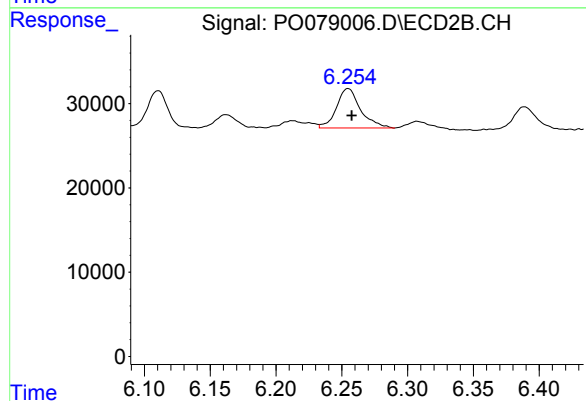


#28 AR-1254-3

R.T.: 6.255 min
Delta R.T.: -0.003 min
Response: 59511
Conc: 26.76 ng/ml

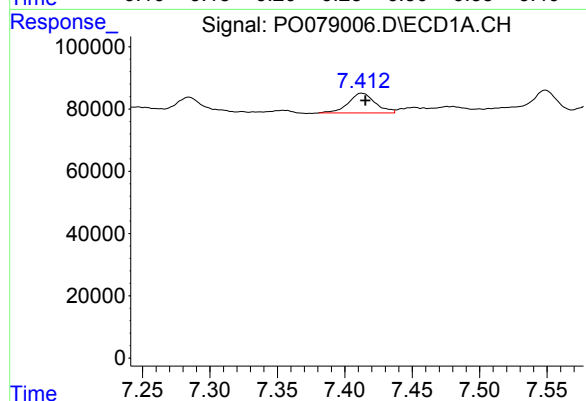


#29 AR-1254-4

R.T.: 7.413 min
Delta R.T.: -0.002 min
Response: 88183
Conc: 28.66 ng/ml

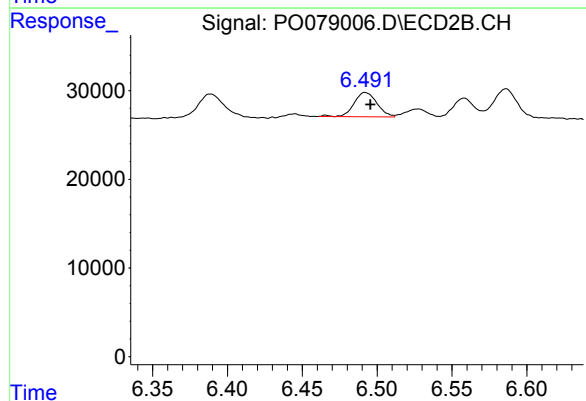


#29 AR-1254-4

R.T.: 6.492 min
Delta R.T.: -0.003 min
Response: 29489
Conc: 21.69 ng/ml

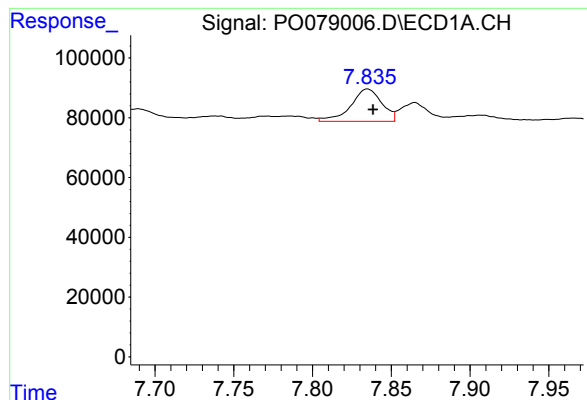

#30 AR-1254-5

R.T.: 7.835 min
Delta R.T.: -0.003 min
Response: 148976
Conc: 45.64 ng/ml

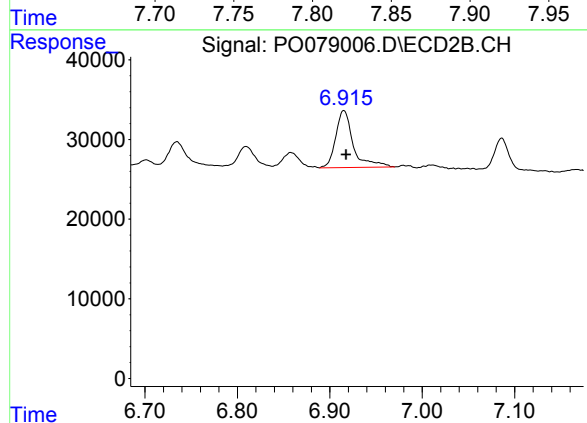

#30 AR-1254-5

R.T.: 6.915 min
Delta R.T.: -0.003 min
Response: 94308
Conc: 47.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
15C-1

Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:06 PM