

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079024.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 17:16
 Operator : DD\AJ
 Sample : M2791-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:44:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.328	3.604	1319827	583220	16.723m	19.623
2) SA Decachlor...	9.934	8.784	907826	466247	14.536	15.647

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 RW-1-20210618

Manual Integrations
 APPROVED

Ankita
 6/23/2021 4:15:55 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062221\
Data File : PO079024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 17:16
Operator : DD\AJ
Sample : M2791-08
Misc :
ALS Vial : 25 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:44:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleId :
RW-1-20210618

Manual Integrations
APPROVED

Ankita
6/23/2021 4:15:55 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

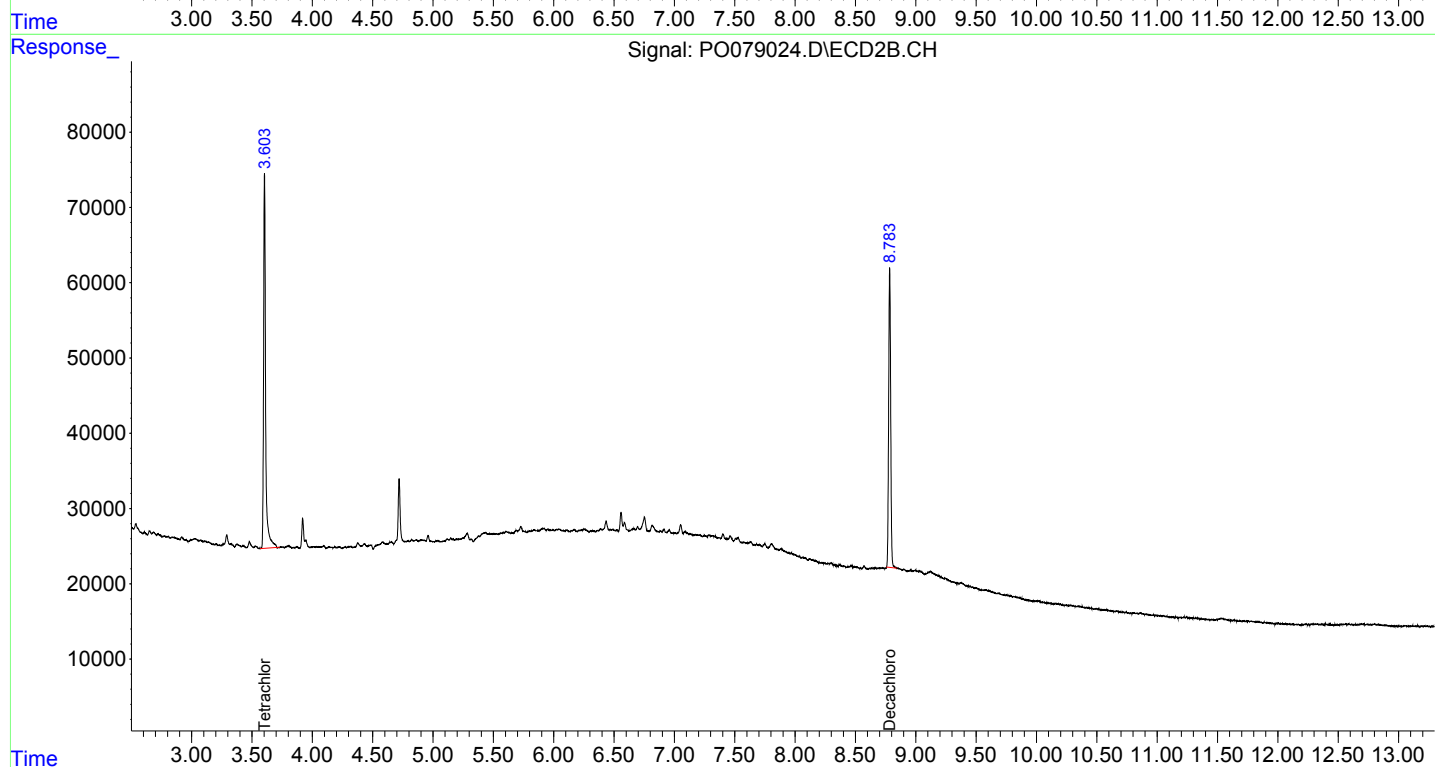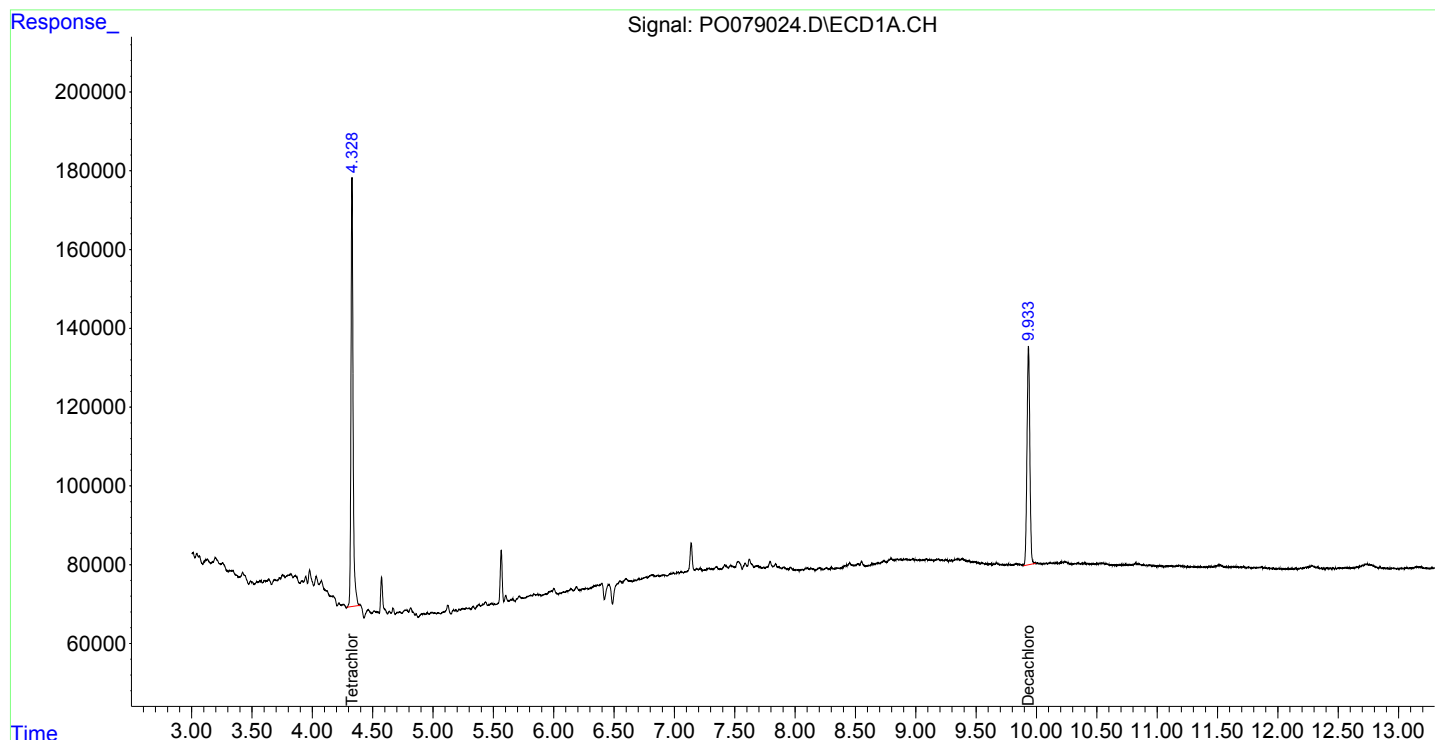

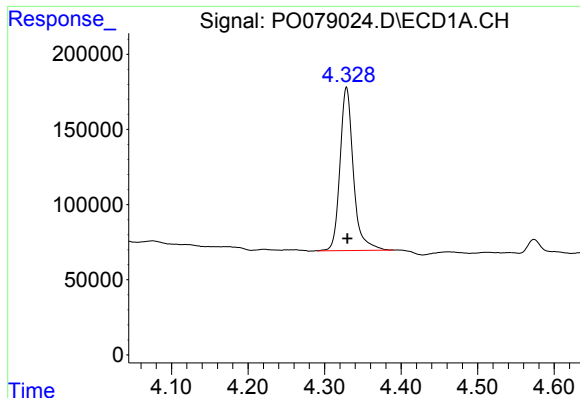


#1 Tetrachloro-m-xylene

R.T.: 4.328 min
Delta R.T.: -0.002 min
Response: 1319827
Conc: 16.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RW-1-20210618


Manual Integrations
APPROVED

Ankita
6/23/2021 4:15:55 PM

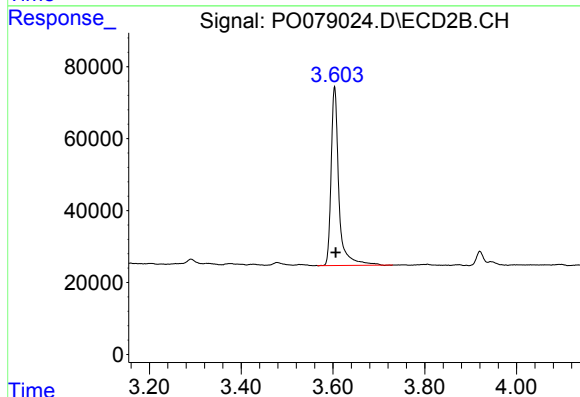


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.003 min
Response: 583220
Conc: 19.62 ng/ml

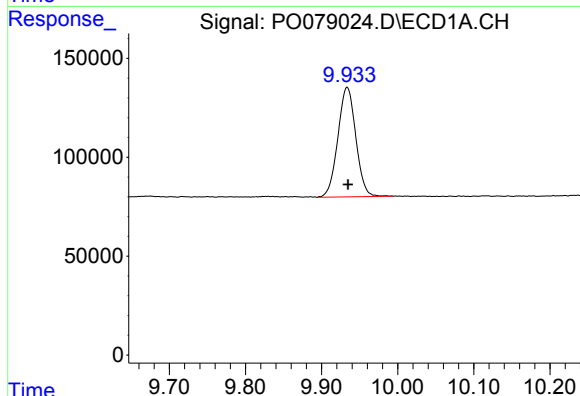

#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: -0.001 min
Response: 907826
Conc: 14.54 ng/ml

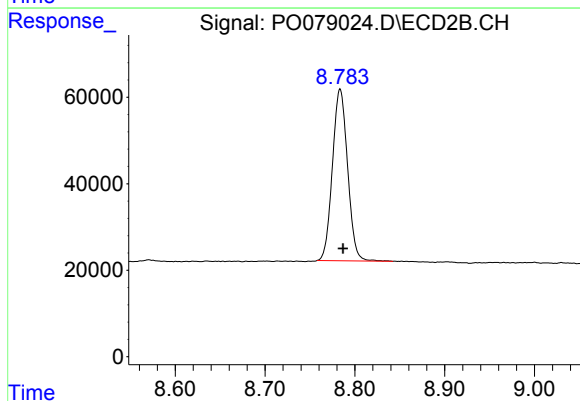

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: -0.003 min
Response: 466247
Conc: 15.65 ng/ml