

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079035.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 21:22
 Operator : DD\AJ
 Sample : M2771-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:52:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.602	1744159	677572	22.100m	22.798m
2) SA Decachlor...	9.930	8.783	637428	313758	10.206	10.529

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :

ECD_O

ClientSampleId :

0370-COMPOSITE-DC-21-MOD-F

Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:22 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062221\
Data File : PO079035.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 21:22
Operator : DD\AJ
Sample : M2771-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:52:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Instrument :

ECD_O



ClientSampleId :


0370-COMPOSITE-DC-21-MOD-F

Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:22 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

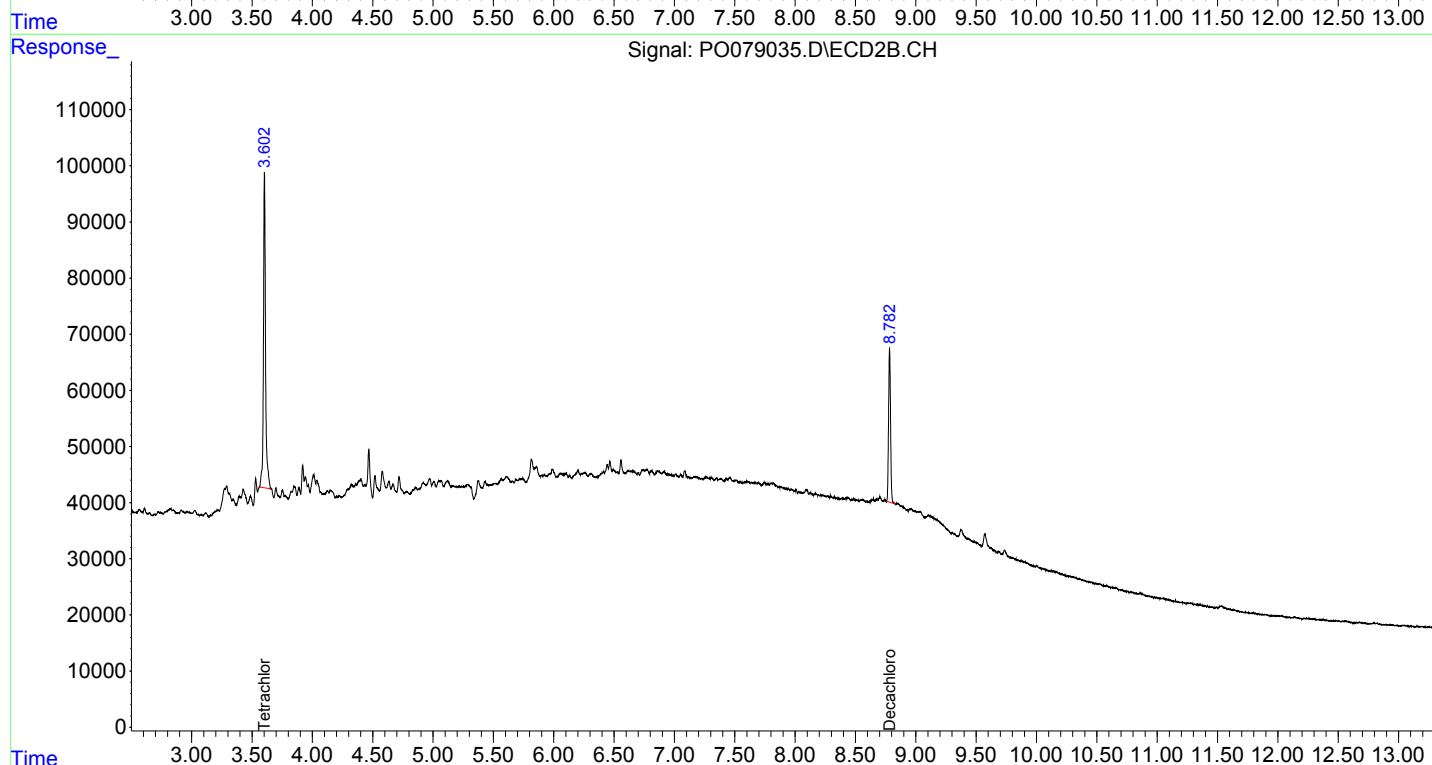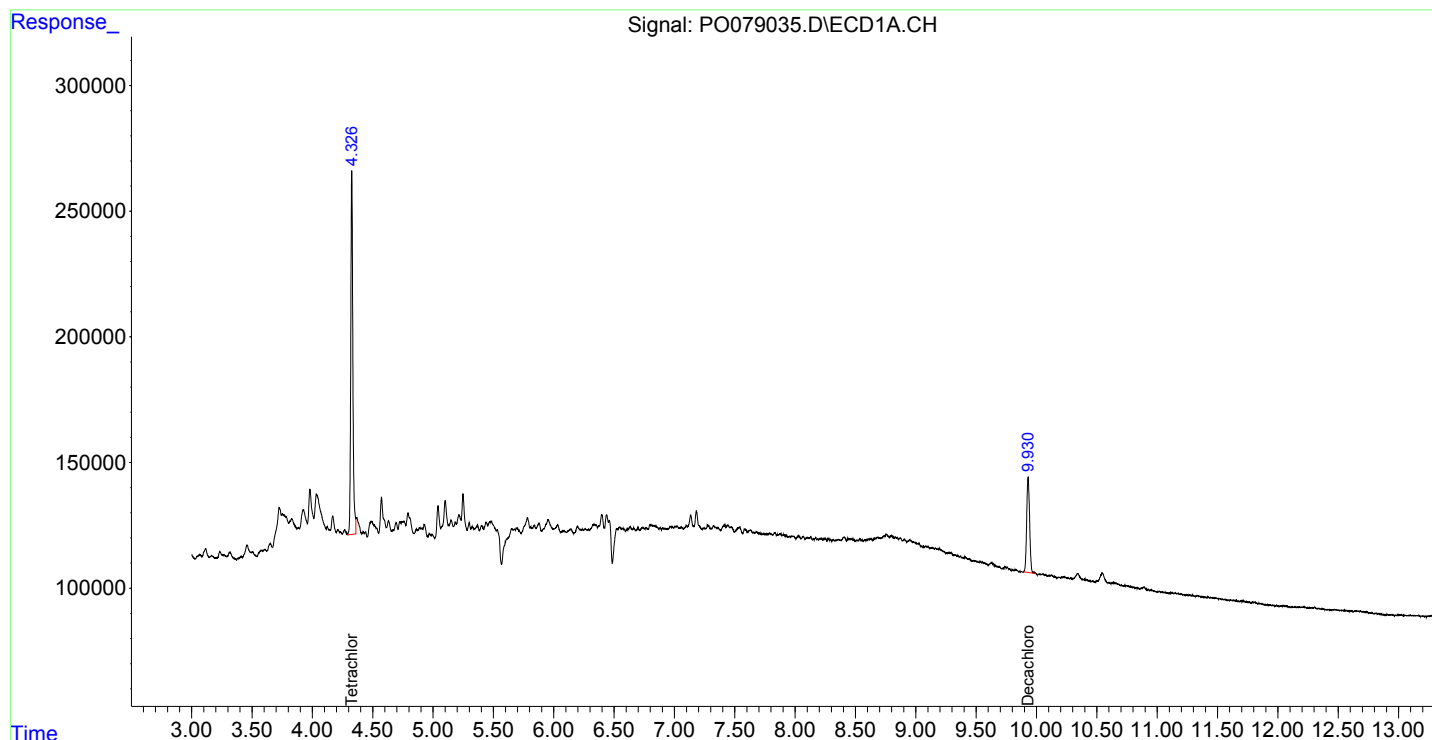

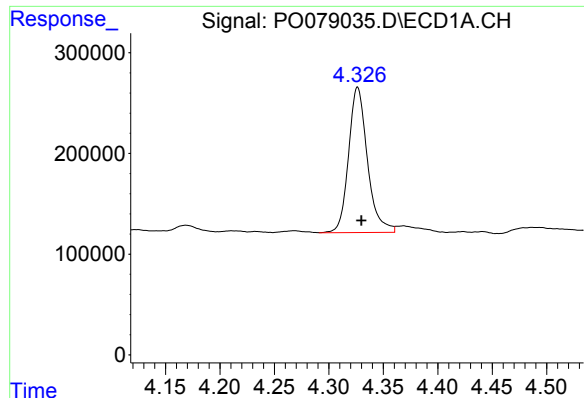


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: -0.004 min
Response: 1744159
Conc: 22.10 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0370-COMPOSITE-DC-21-MOD-E


Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:22 PM

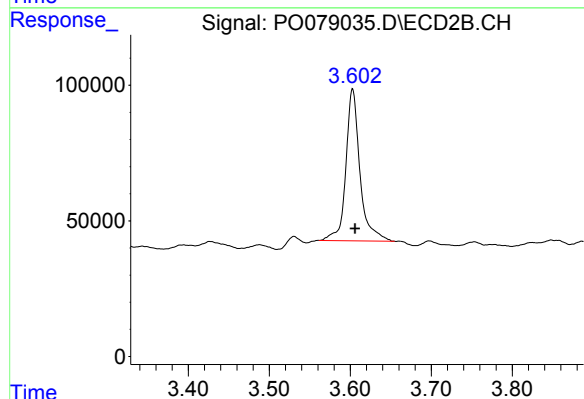


#1 Tetrachloro-m-xylene

R.T.: 3.602 min
Delta R.T.: -0.004 min
Response: 677572
Conc: 22.80 ng/ml m

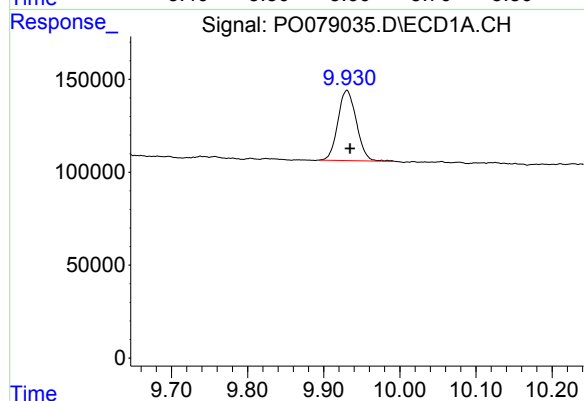

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.004 min
Response: 637428
Conc: 10.21 ng/ml

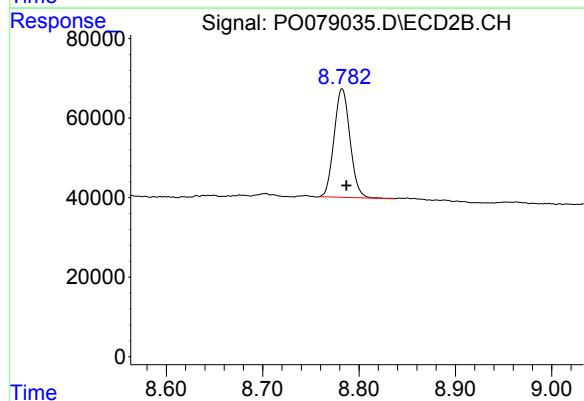

#2 Decachlorobiphenyl

R.T.: 8.783 min
Delta R.T.: -0.004 min
Response: 313758
Conc: 10.53 ng/ml