

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079036.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 21:40
 Operator : DD\AJ
 Sample : M2771-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0370-COMPOSITE-DC-21-MOD-F

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:53:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.327	3.603	1945633	699874	24.652	23.548
2) SA Decachlor...	9.931	8.782	696155	371824	11.147	12.478

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
Data File : P0079036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 21:40
Operator : DD\AJ
Sample : M2771-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :



ECD_O


ClientSampleId :

0370-COMPOSITE-DC-21-MOD-F

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:53:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

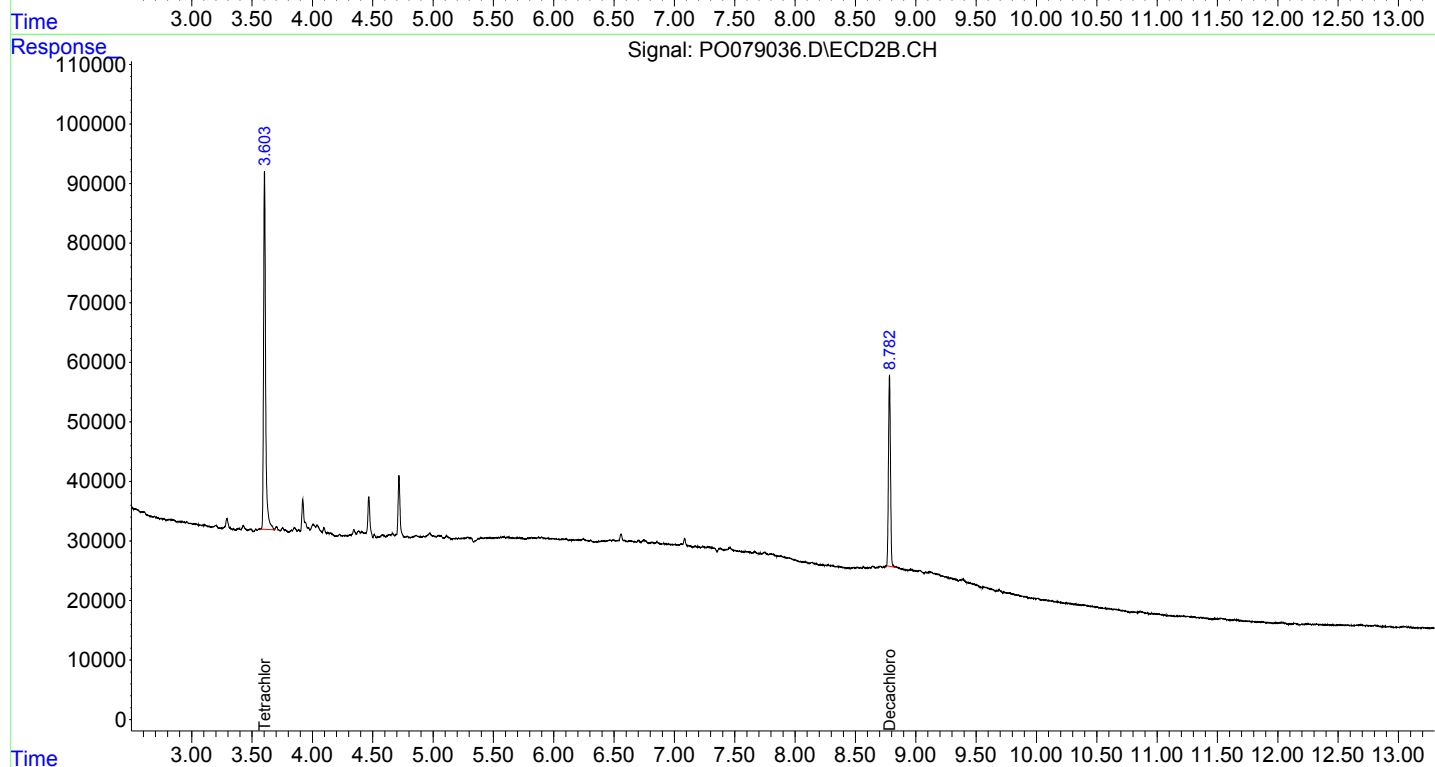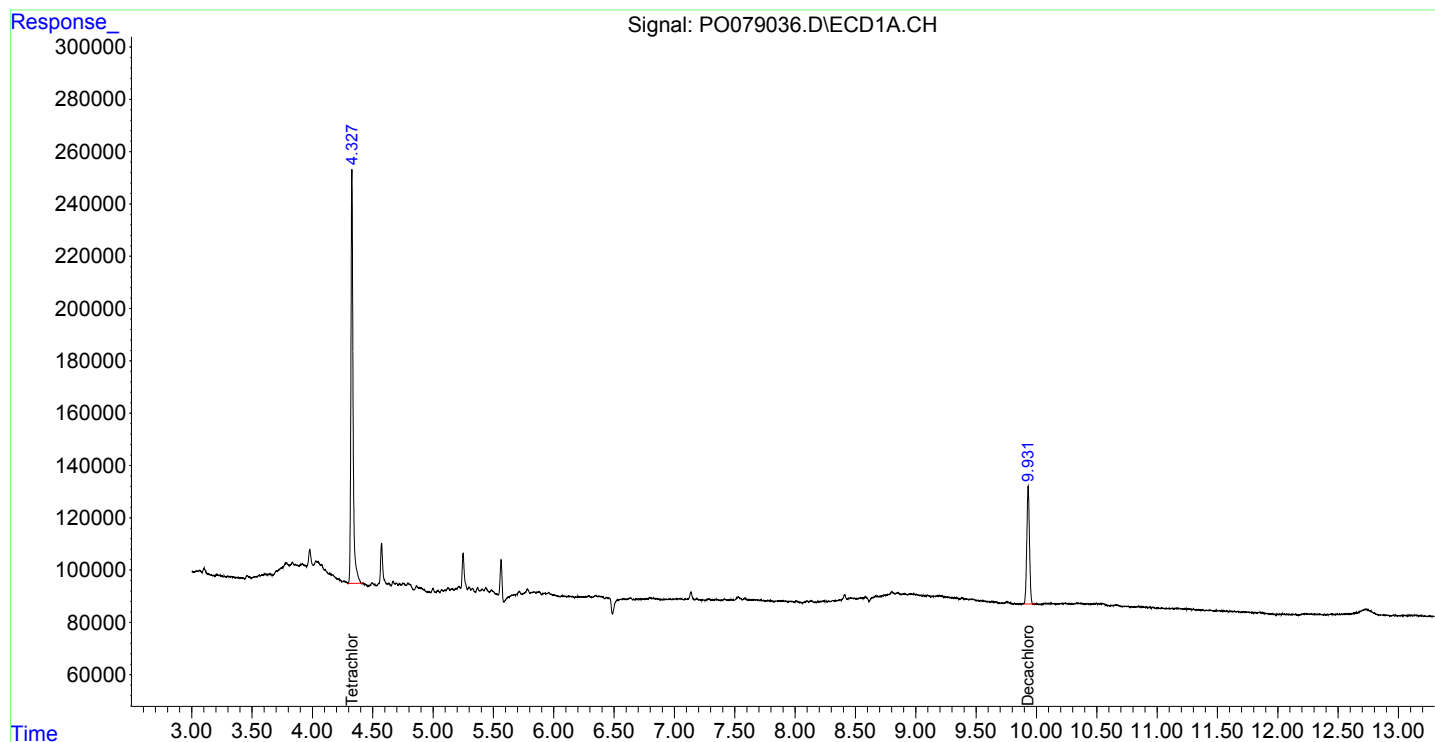


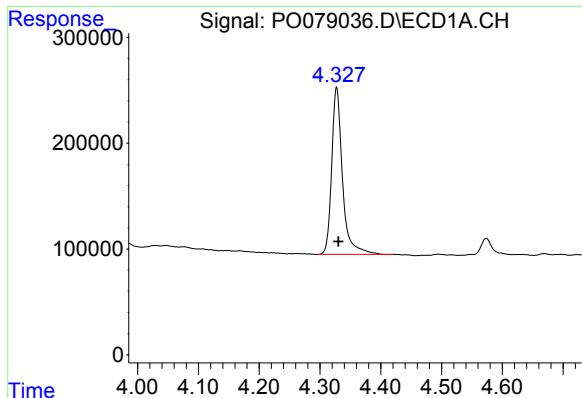

#1 Tetrachloro-m-xylene


R.T.: 4.327 min
Delta R.T.: -0.003 min
Response: 1945633
Conc: 24.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
0370-COMPOSITE-DC-21-MOD-F

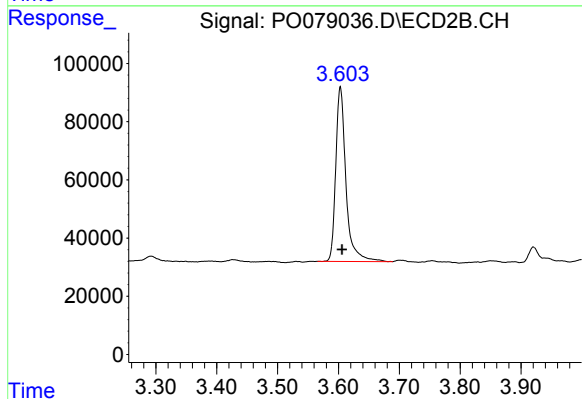


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.003 min
Response: 699874
Conc: 23.55 ng/ml

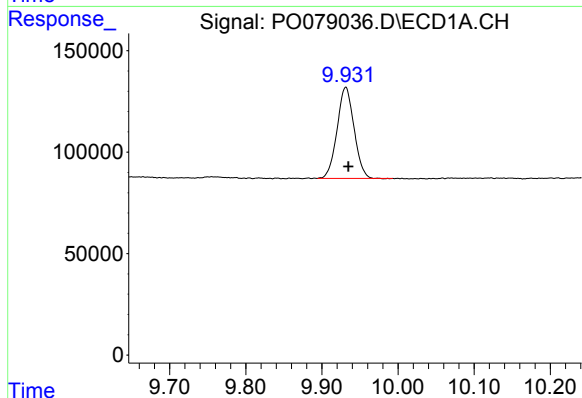

#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.003 min
Response: 696155
Conc: 11.15 ng/ml

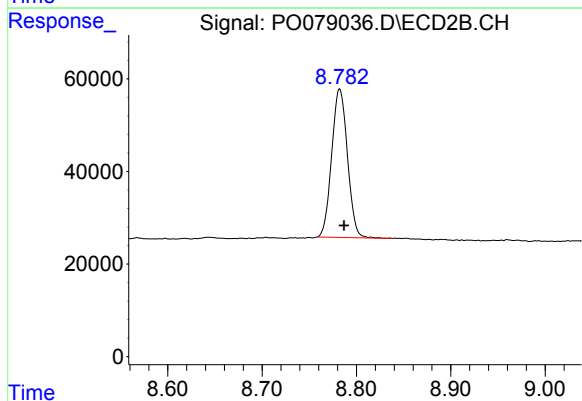

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: -0.005 min
Response: 371824
Conc: 12.48 ng/ml