

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062221\
 Data File : P0079037.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jun 2021 21:57
 Operator : DD\AJ
 Sample : M2787-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 03:53:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.603	1844608	719727	23.372m	24.216
2) SA Decachlor...	9.930	8.782	1007729	521543	16.135	17.502

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Instrument :
 ECD_O
 ClientSampleId :
 41216

Manual Integrations
 APPROVED

Ankita
 6/23/2021 1:50:24 PM

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062221\
Data File : PO079037.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jun 2021 21:57
Operator : DD\AJ
Sample : M2787-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 03:53:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Instrument :
ECD_O
ClientSampleId :
41216

Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:24 PM

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

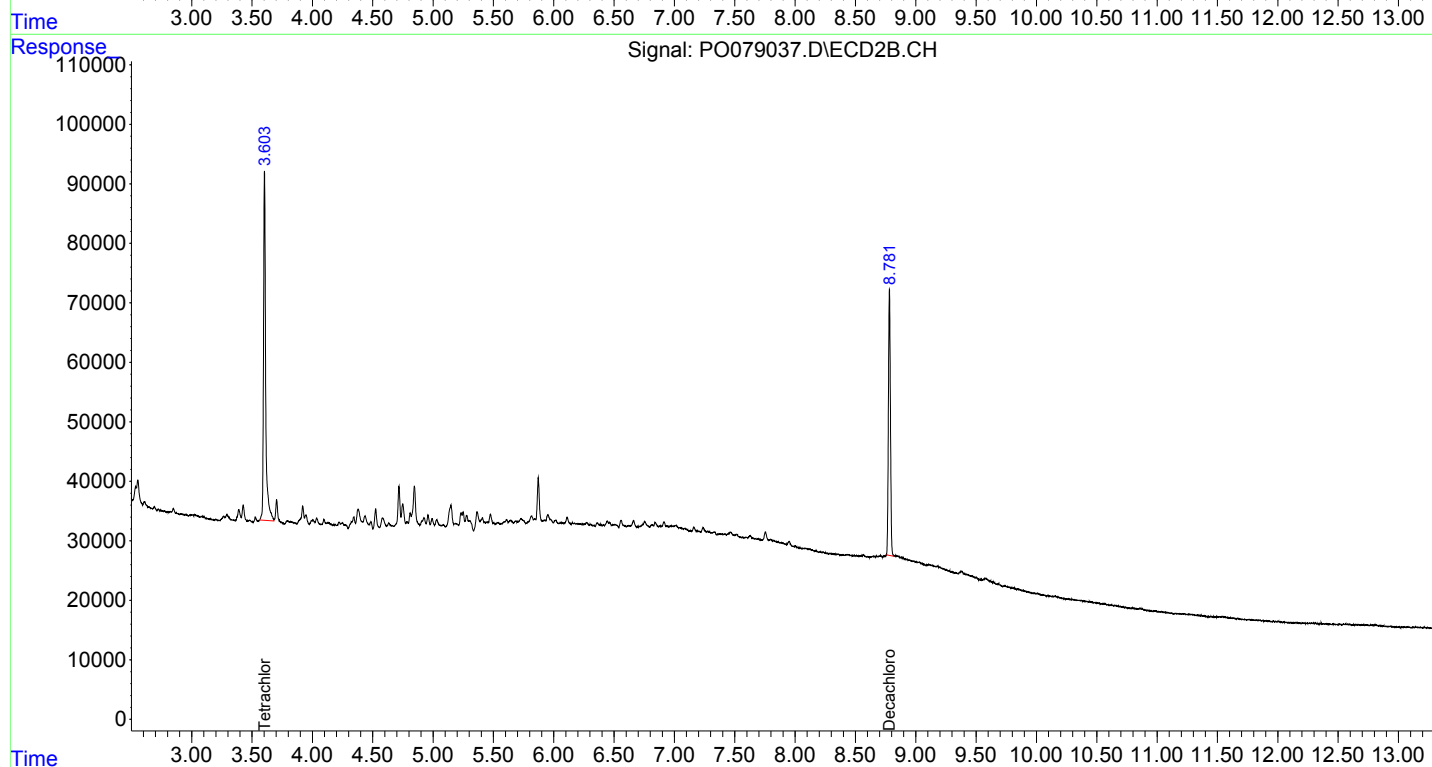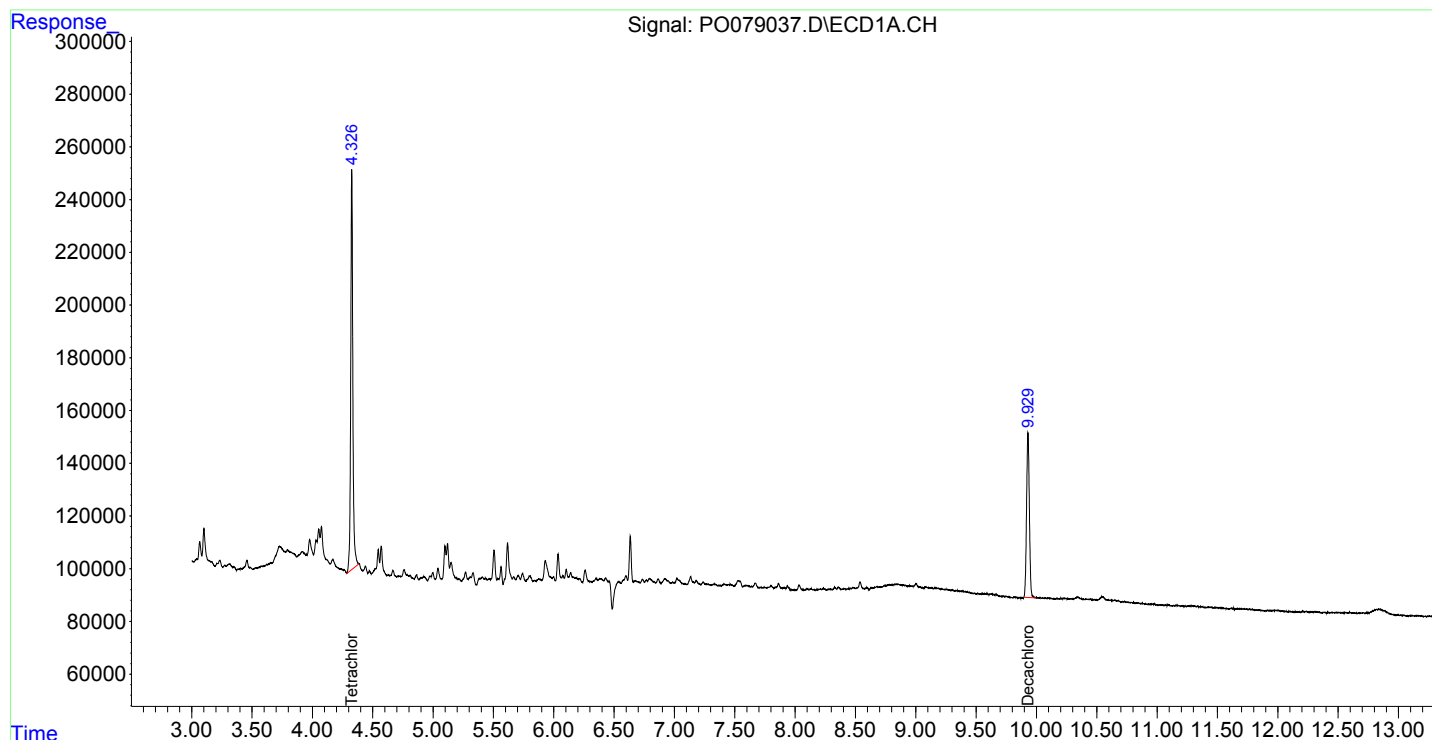

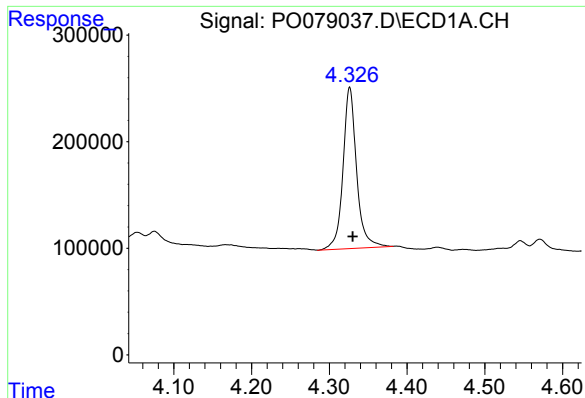


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: -0.004 min
Response: 1844608
Conc: 23.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
41216


Manual Integrations
APPROVED

Ankita
6/23/2021 1:50:24 PM

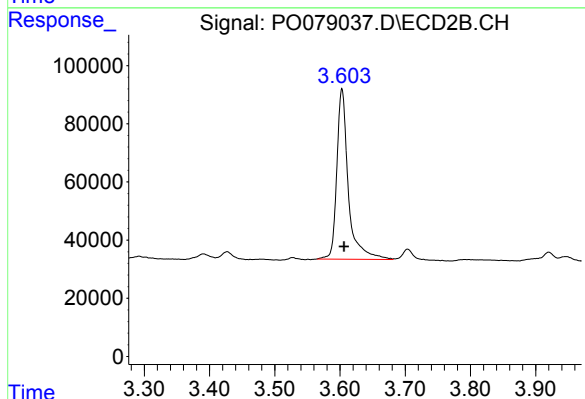


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.003 min
Response: 719727
Conc: 24.22 ng/ml

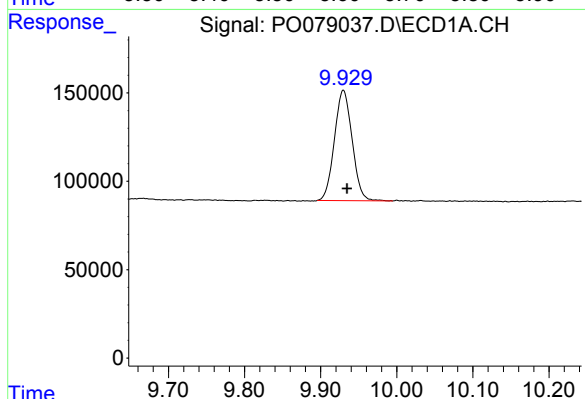

#2 Decachlorobiphenyl

R.T.: 9.930 min
Delta R.T.: -0.005 min
Response: 1007729
Conc: 16.14 ng/ml

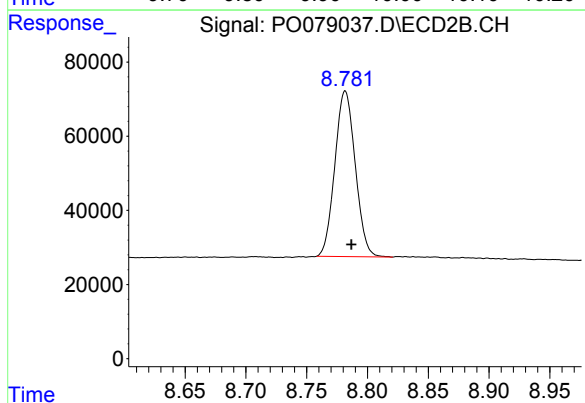

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: -0.005 min
Response: 521543
Conc: 17.50 ng/ml