

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062222\
 Data File : P0087254.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 11:37
 Operator : YP/AJ
 Sample : N3421-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-3-0-2-20220620

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/23/2022
 Supervised By :Ankita Jodhani 06/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 12:41:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.640	43318513	21788376	18.536	19.352
2) SA Decachlor...	10.349	8.644	23616048	9806510	12.833	12.473m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062222\
Data File : PO087254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 11:37
Operator : YP/AJ
Sample : N3421-04
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-3-0-2-20220620


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 12:41:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

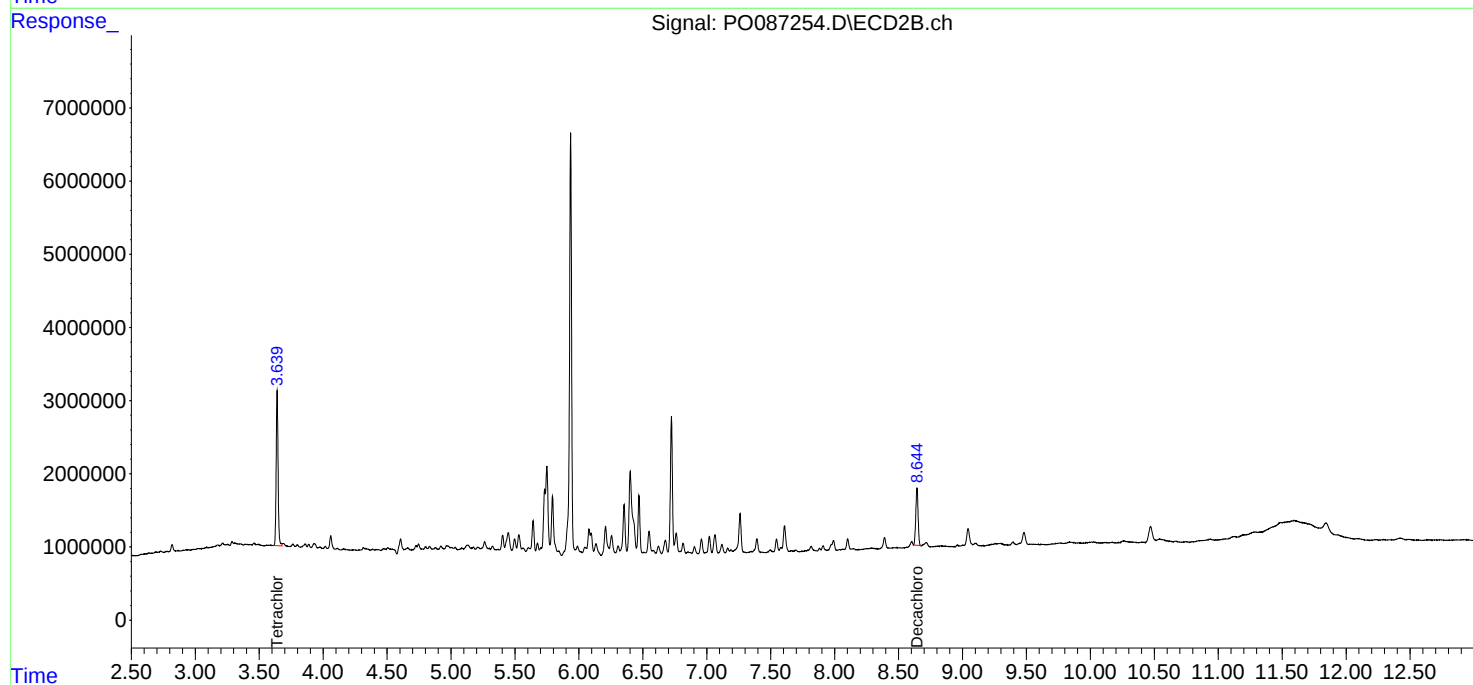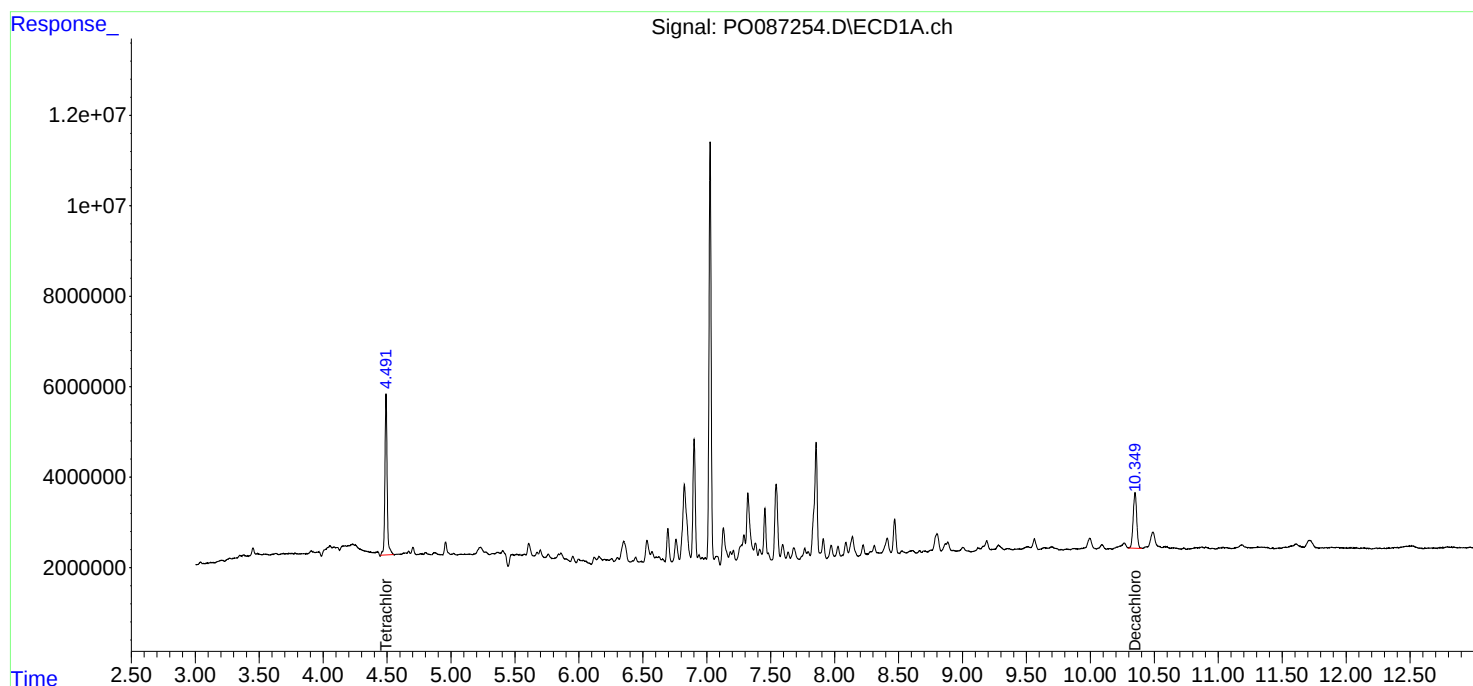

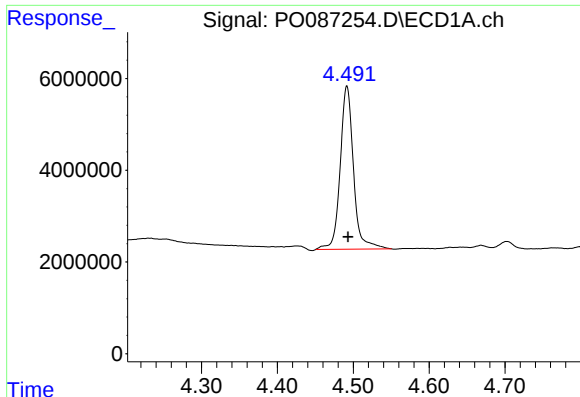


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: -0.001 min
Response: 43318513
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-3-0-2-20220620


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

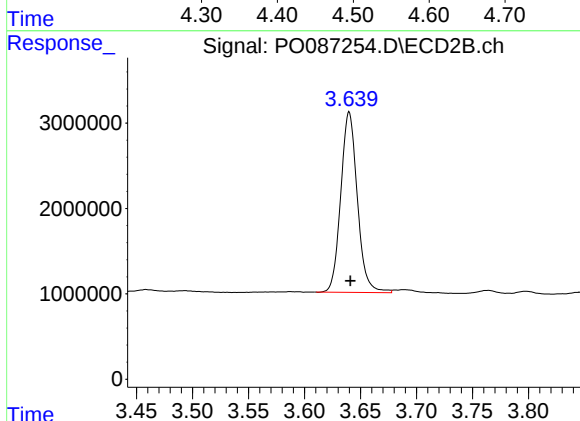


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.001 min
Response: 21788376
Conc: 19.35 ng/ml

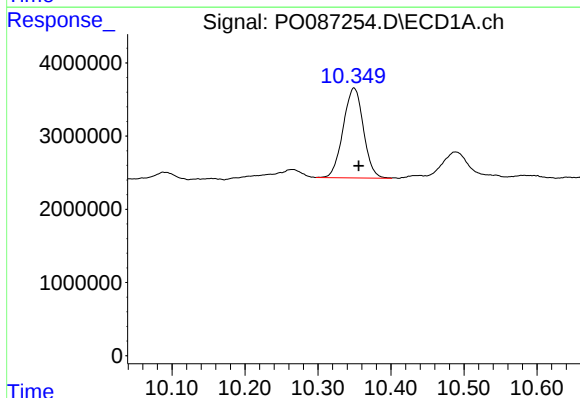

#2 Decachlorobiphenyl

R.T.: 10.349 min
Delta R.T.: -0.006 min
Response: 23616048
Conc: 12.83 ng/ml

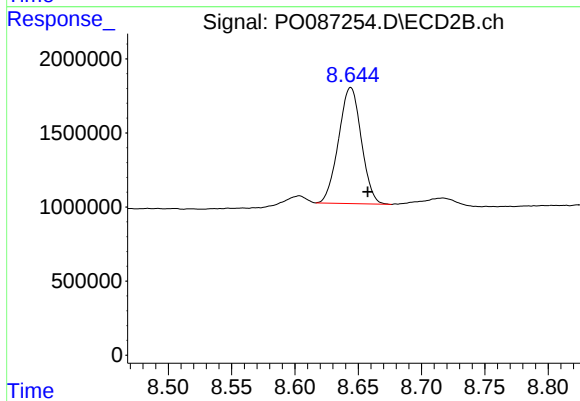

#2 Decachlorobiphenyl

R.T.: 8.644 min
Delta R.T.: -0.014 min
Response: 9806510
Conc: 12.47 ng/ml m