

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062222\
 Data File : P0087300.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 04:28
 Operator : YP/AJ
 Sample : N3445-04 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC204970-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/23/2022
 Supervised By :Ankita Jodhani 06/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 07:49:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.638	3264223	1918915	1.397	1.704
2) SA Decachlor...	10.351	8.648	2903037	1071065	1.577m	1.362

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062222\
Data File : PO087300.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 04:28
Operator : YP/AJ
Sample : N3445-04 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC204970-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 07:49:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

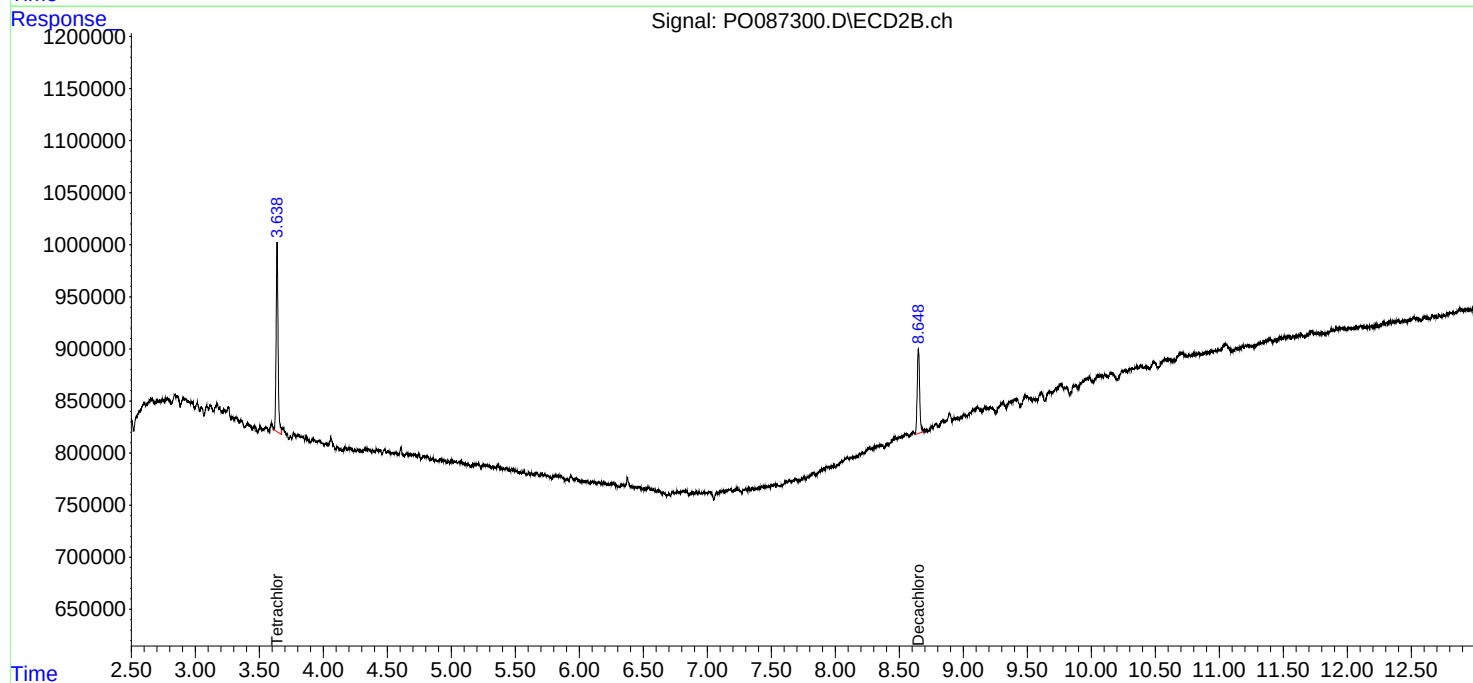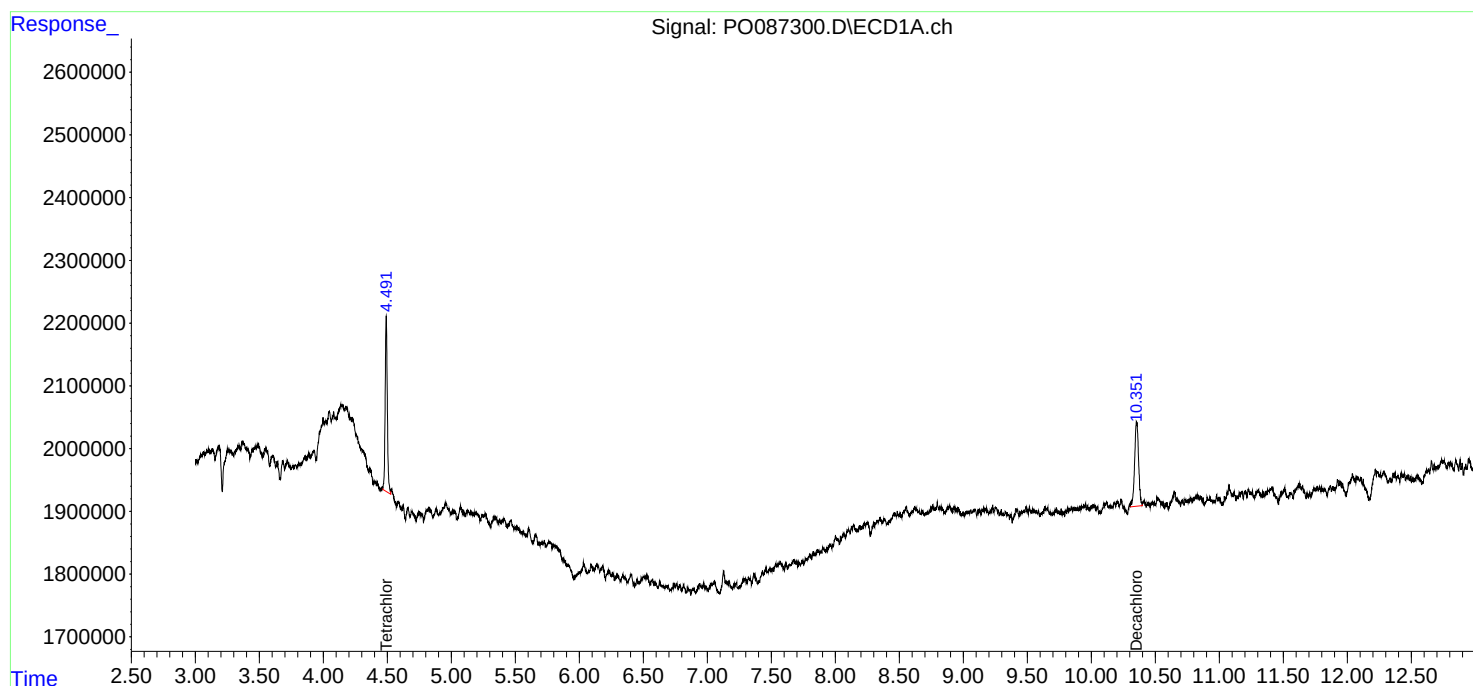

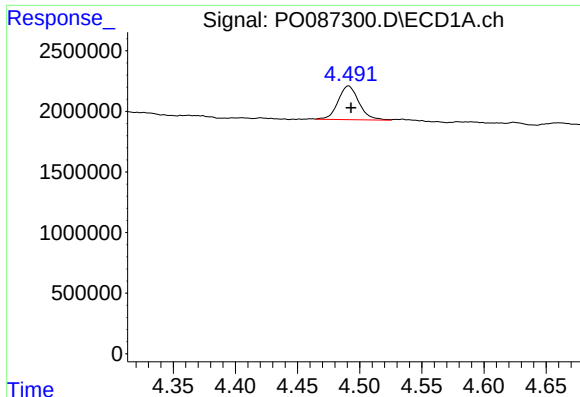


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: -0.002 min
Response: 3264223
Conc: 1.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC204970-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

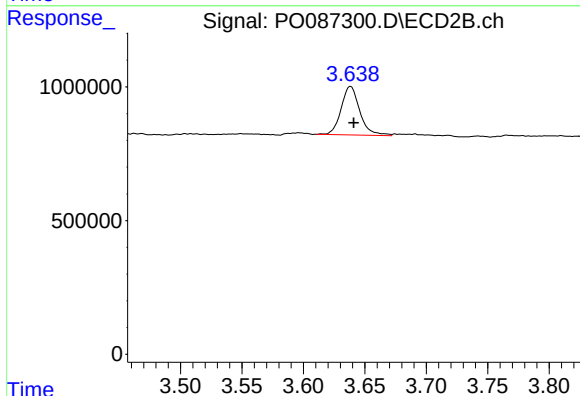


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 1918915
Conc: 1.70 ng/ml

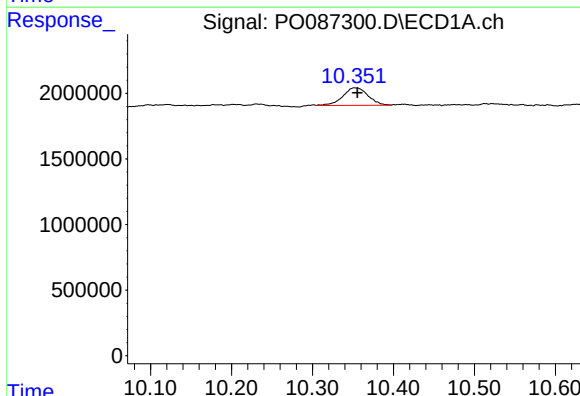

#2 Decachlorobiphenyl

R.T.: 10.351 min
Delta R.T.: -0.004 min
Response: 2903037
Conc: 1.58 ng/ml m

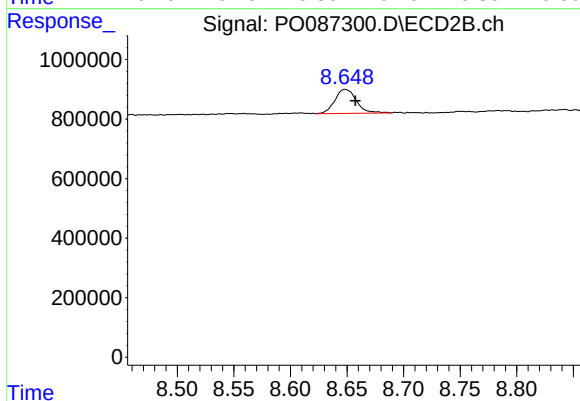

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.009 min
Response: 1071065
Conc: 1.36 ng/ml