

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062223\
 Data File : P0095874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 17:12
 Operator : YP/AJ
 Sample : 03344-04 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC260371-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/23/2023
 Supervised By :Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:34:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.634	4333415	1916504	1.489	1.412
2) SA Decachlor...	10.231	8.671	4499847	1994596	2.172	1.627m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062223\
Data File : PO095874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 17:12
Operator : YP/AJ
Sample : 03344-04 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC260371-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:34:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

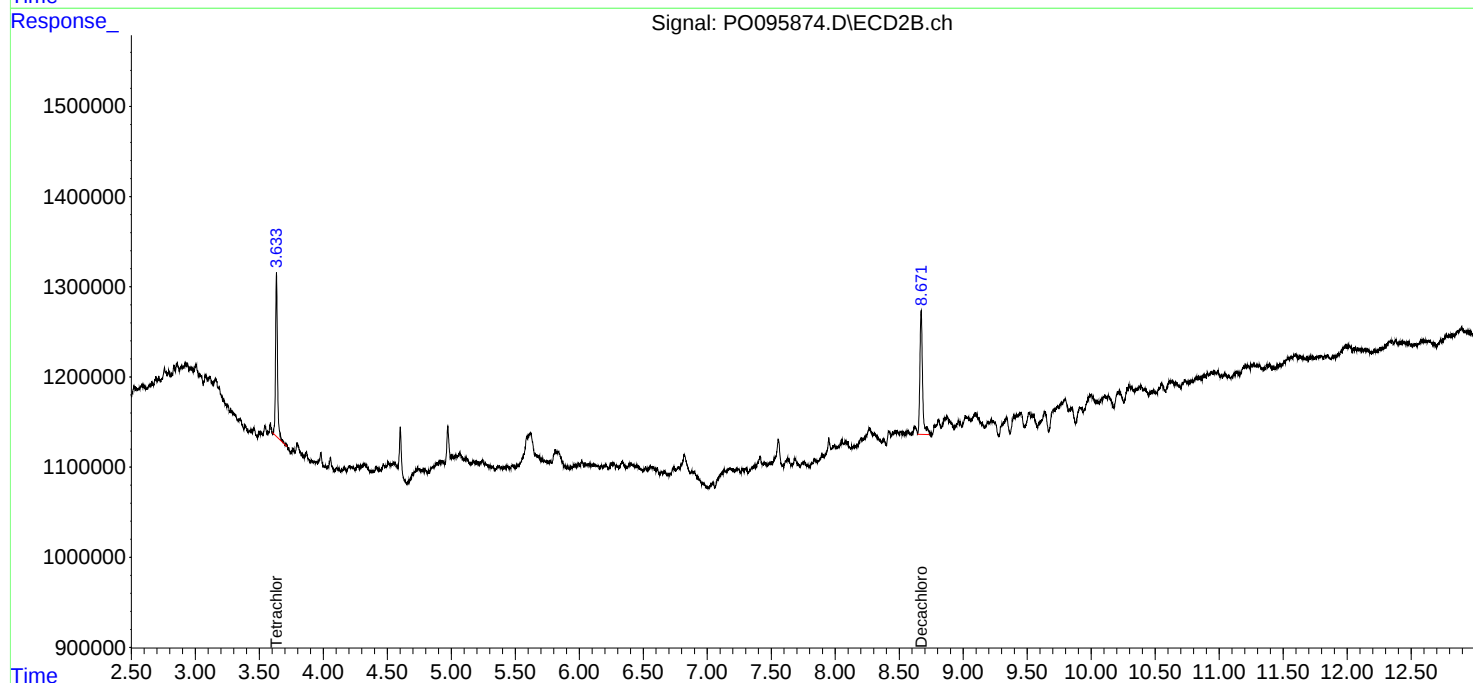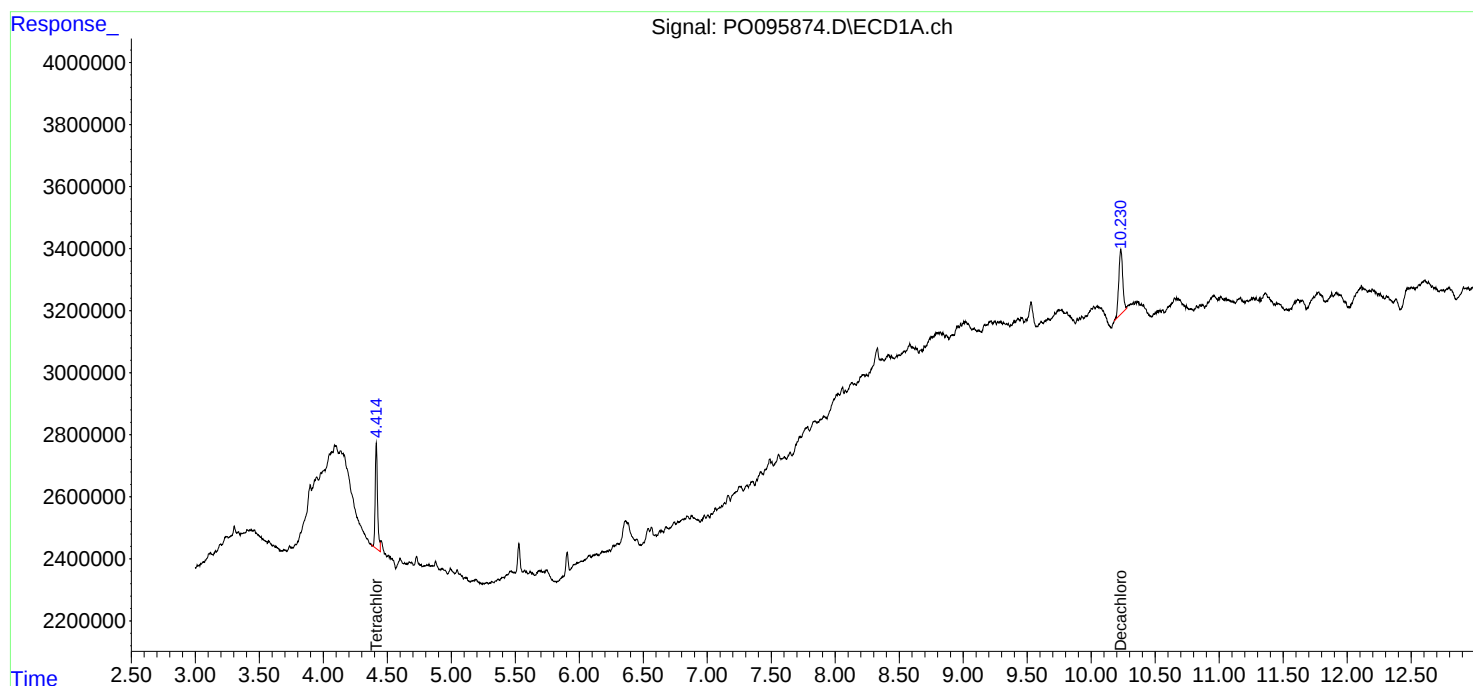

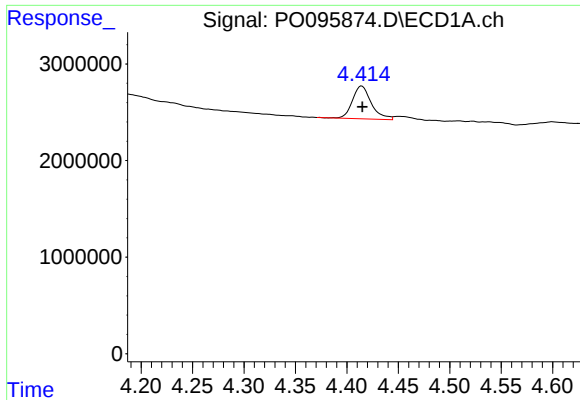


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: 0.000 min
Response: 4333415
Conc: 1.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC260371-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

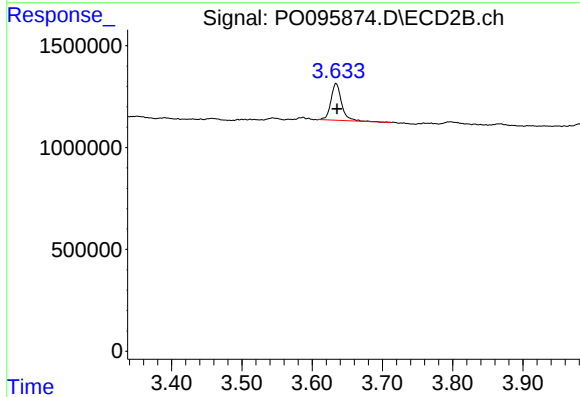


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.001 min
Response: 1916504
Conc: 1.41 ng/ml

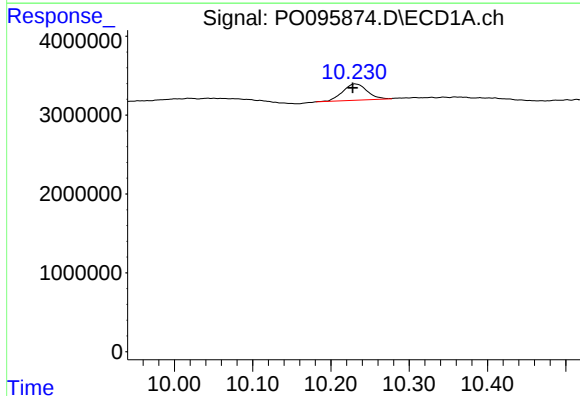

#2 Decachlorobiphenyl

R.T.: 10.231 min
Delta R.T.: 0.003 min
Response: 4499847
Conc: 2.17 ng/ml

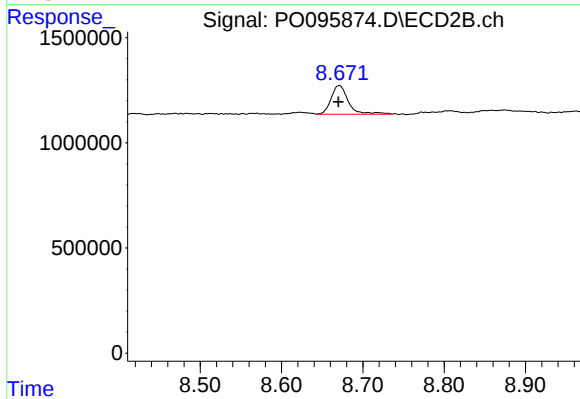

#2 Decachlorobiphenyl

R.T.: 8.671 min
Delta R.T.: 0.001 min
Response: 1994596
Conc: 1.63 ng/ml m