

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079046.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 10:05
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:23:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.332	3.603	1802670	656655	22.841	22.094
2)	SA Decachlor...	9.935	8.783	1350944	672019	21.631	22.552
Target Compounds							
9)	L2 AR-1221-2	4.673	0.000	25520	0	41.896	N.D. #
15)	L3 AR-1232-5	5.924	0.000	37770	0	73.120	N.D. #
22)	L5 AR-1248-2	5.924	0.000	37770	0	17.073	N.D. #
28)	L6 AR-1254-3	7.139f	0.000	25923	0	5.821	N.D. #
32)	L7 AR-1260-2	7.542	0.000	40474	0	10.413	N.D. #
40)	L8 AR-1262-5	9.356	0.000	109428	0	45.165	N.D. #
44)	L9 AR-1268-4	9.356	0.000	109428	0	42.515	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079046.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 10:05
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:23:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

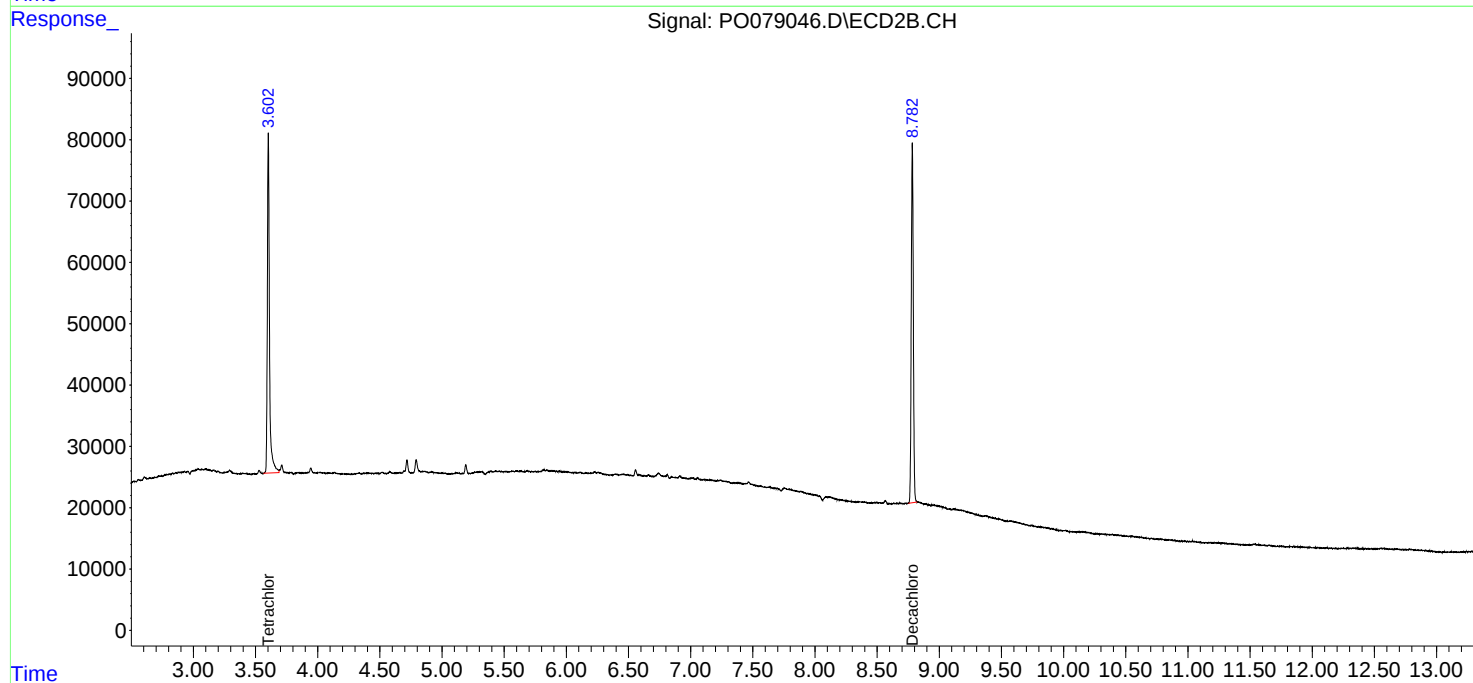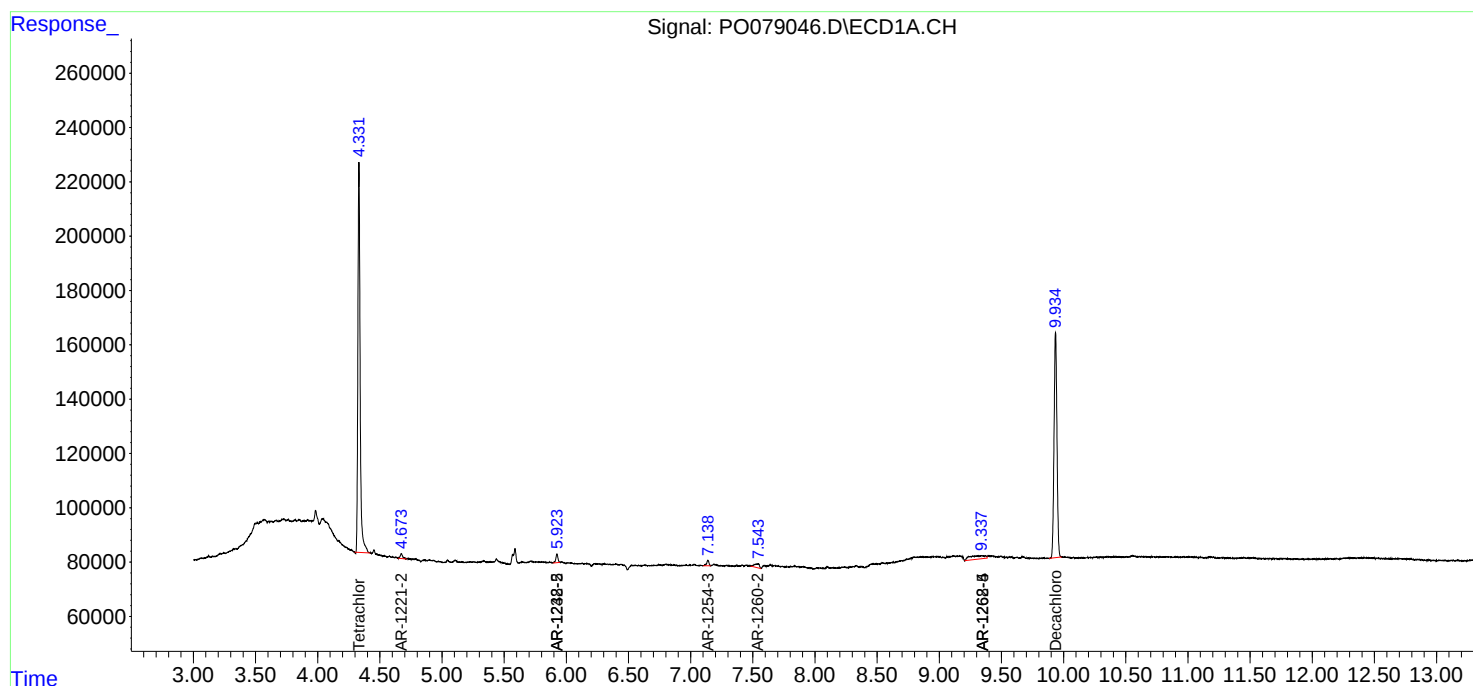


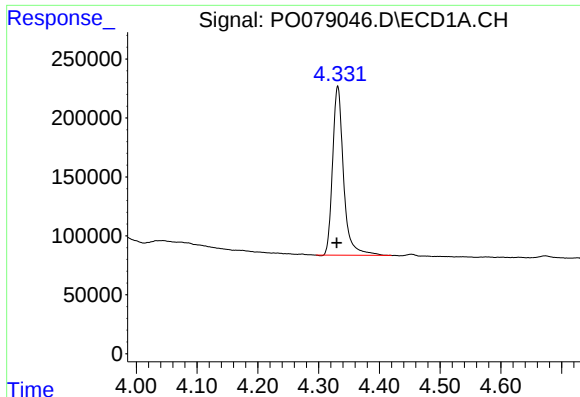

#1 Tetrachloro-m-xylene


R.T.: 4.332 min
Delta R.T.: 0.002 min
Response: 1802670
Conc: 22.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

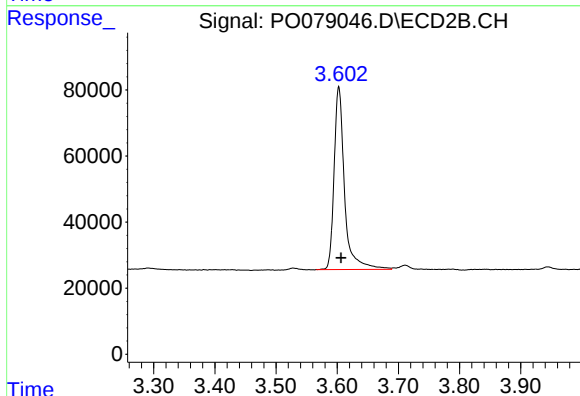


#1 Tetrachloro-m-xylene

R.T.: 3.603 min
Delta R.T.: -0.003 min
Response: 656655
Conc: 22.09 ng/ml

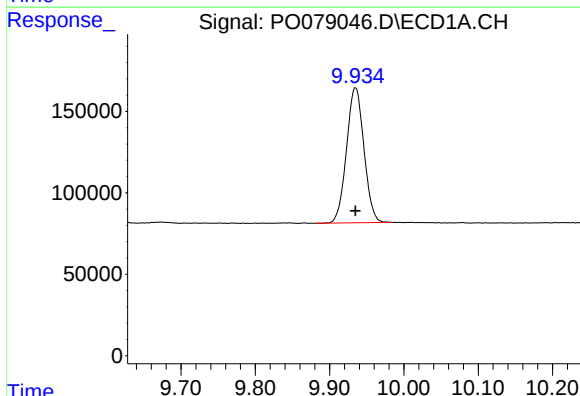


#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: 0.000 min
Response: 1350944
Conc: 21.63 ng/ml

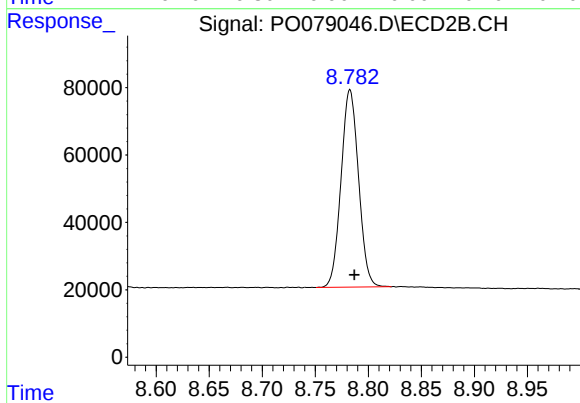

#2 Decachlorobiphenyl


R.T.: 8.783 min
Delta R.T.: -0.004 min
Response: 672019
Conc: 22.55 ng/ml

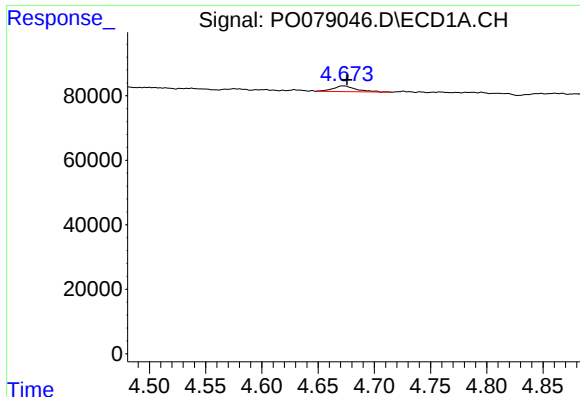

#9 AR-1221-2


R.T.: 4.673 min
Delta R.T.: -0.003 min
Response: 25520
Conc: 41.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

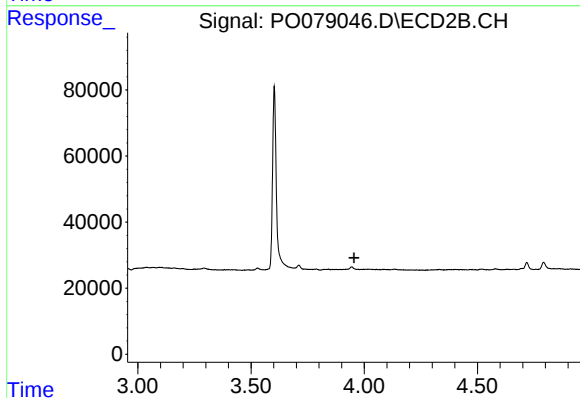


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.955 min
Response: 0
Conc: N.D.

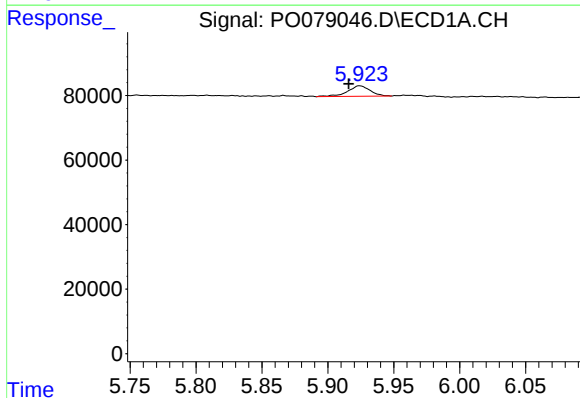


#15 AR-1232-5

R.T.: 5.924 min
Delta R.T.: 0.009 min
Response: 37770
Conc: 73.12 ng/ml

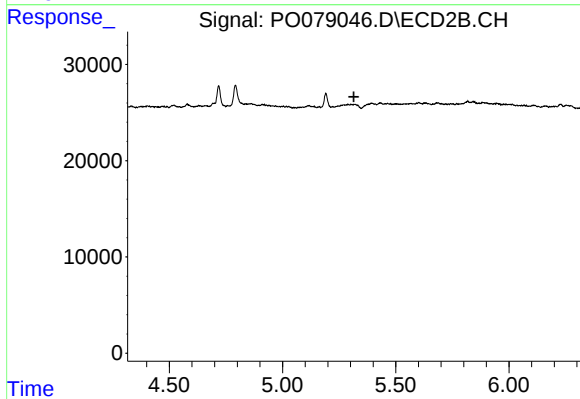

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.315 min
Response: 0
Conc: N.D.

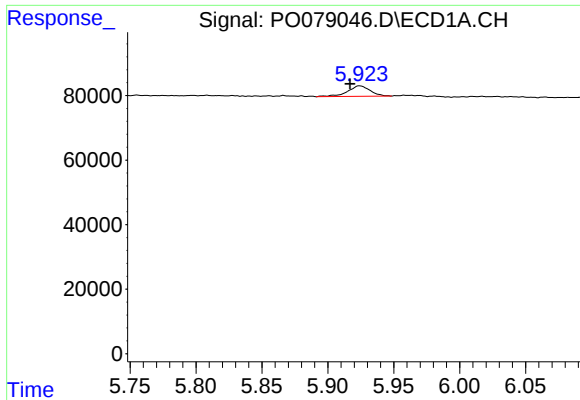

#22 AR-1248-2


R.T.: 5.924 min
Delta R.T.: 0.008 min
Response: 37770
Conc: 17.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

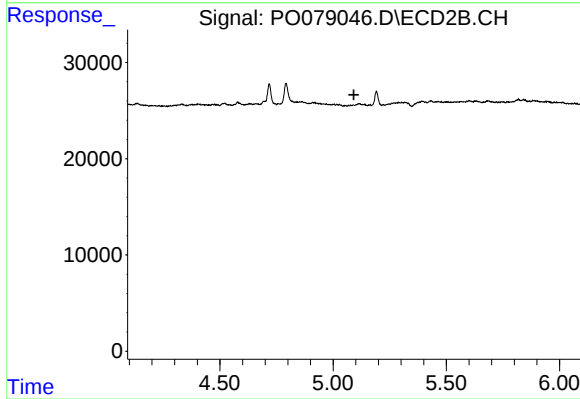


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.092 min
Response: 0
Conc: N.D.

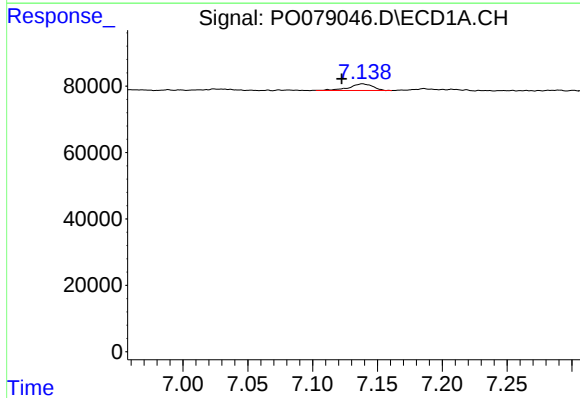


#28 AR-1254-3

R.T.: 7.139 min
Delta R.T.: 0.016 min
Response: 25923
Conc: 5.82 ng/ml

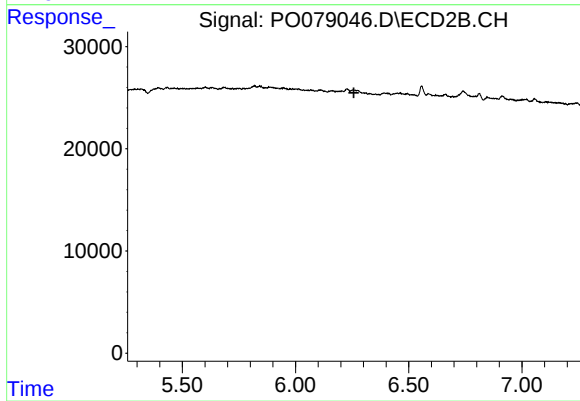

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.

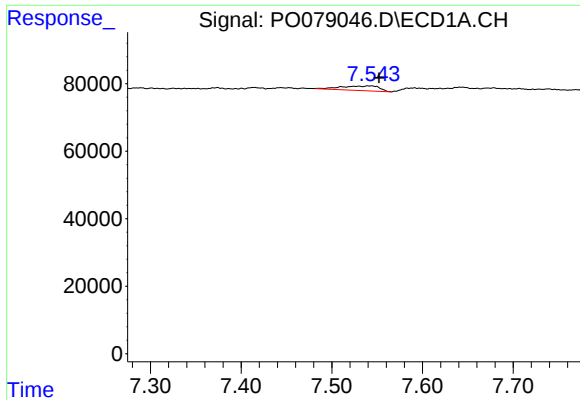

#32 AR-1260-2


R.T.: 7.542 min
Delta R.T.: -0.010 min
Response: 40474
Conc: 10.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

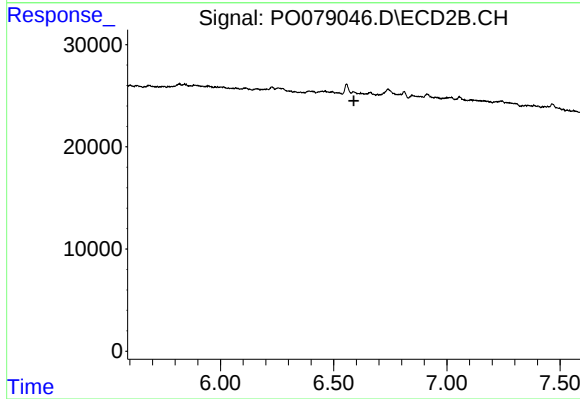


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.590 min
Response: 0
Conc: N.D.

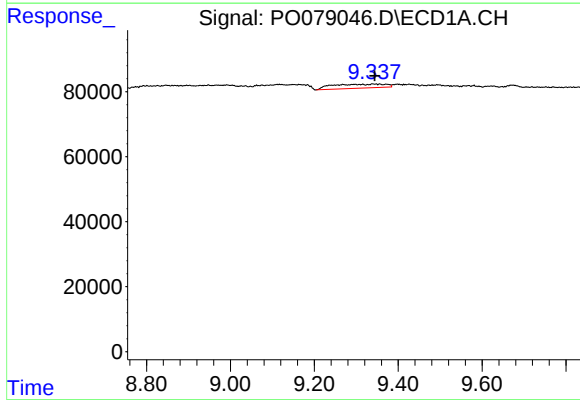


#40 AR-1262-5

R.T.: 9.356 min
Delta R.T.: 0.011 min
Response: 109428
Conc: 45.16 ng/ml

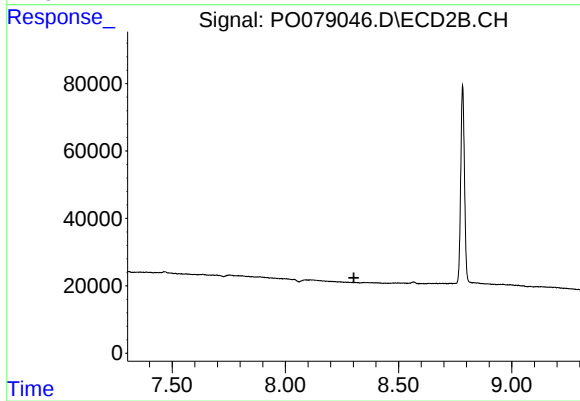

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.303 min
Response: 0
Conc: N.D.

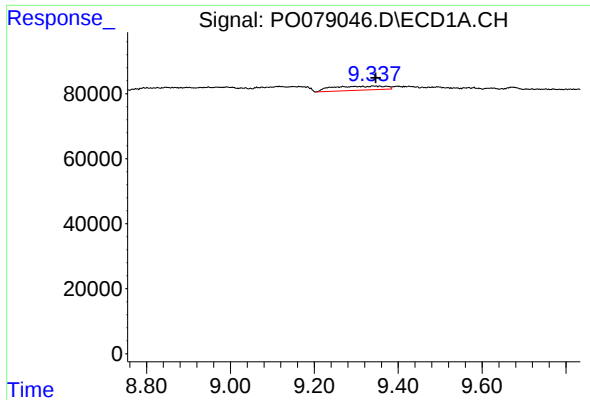

#44 AR-1268-4

R.T.: 9.356 min
Delta R.T.: 0.009 min
Response: 109428
Conc: 42.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

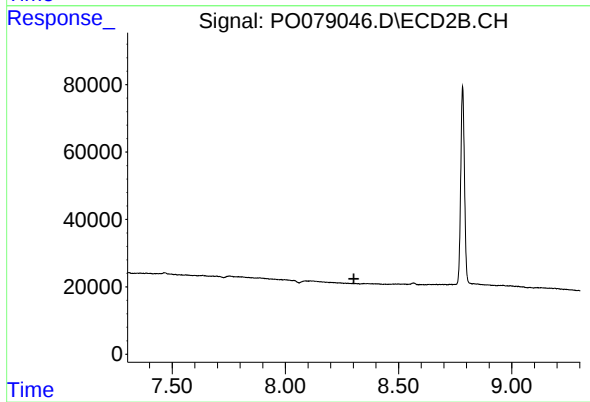

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.303 min
Response: 0
Conc: N.D.