

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079058.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 13:32
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:32:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.324	3.601	1808300	663925	22.912	22.339
2)	SA Decachlor...	9.927	8.780	1313214	654628	21.027	21.968
Target Compounds							
9)	L2 AR-1221-2	4.666	0.000	22195	0	36.438	N.D. #
15)	L3 AR-1232-5	5.918	0.000	36208	0	70.097	N.D. #
22)	L5 AR-1248-2	5.918	0.000	36208	0	16.367	N.D. #
24)	L5 AR-1248-4	6.546	0.000	61800	0	22.297	N.D. #
26)	L6 AR-1254-1	6.546f	0.000	61800	0	22.944	N.D. #
28)	L6 AR-1254-3	7.133	0.000	21278	0	4.778	N.D. #
45)	L9 AR-1268-5	9.666	0.000	17403	0	0.869	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079058.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 13:32
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:32:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

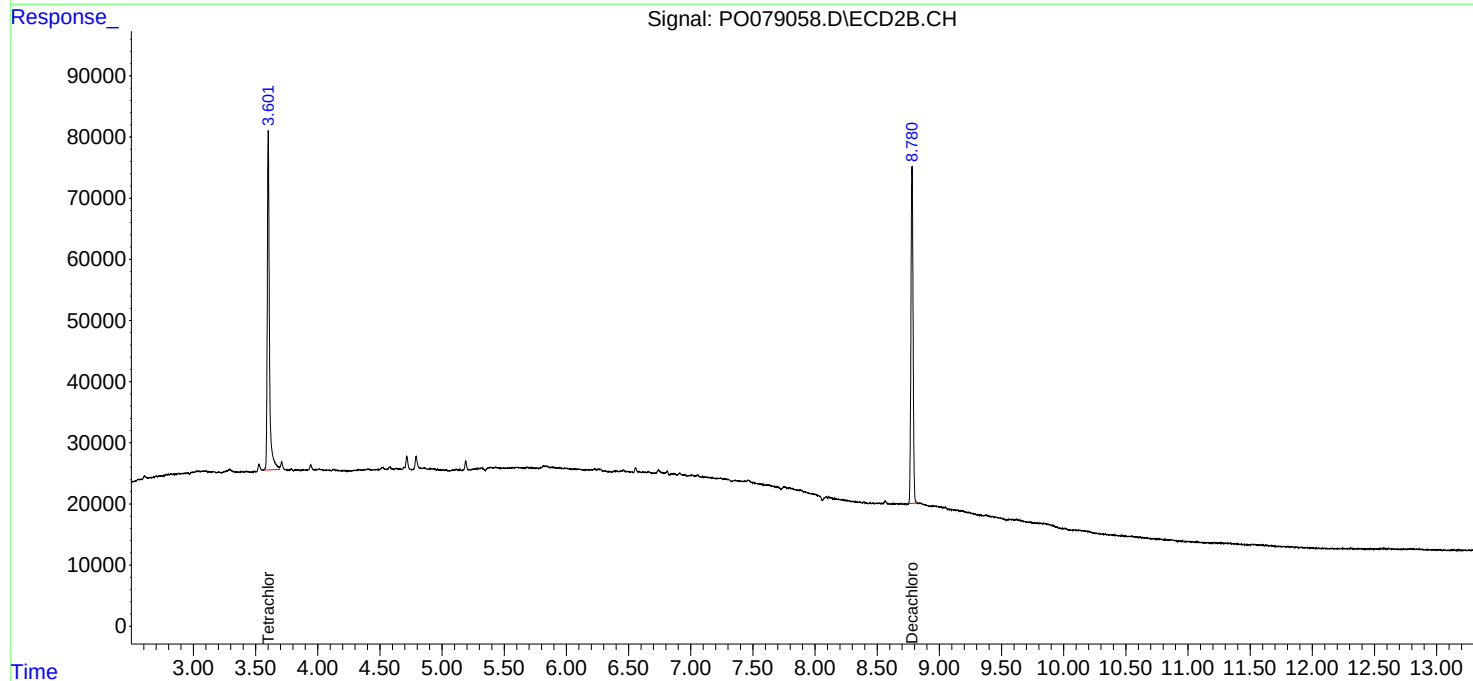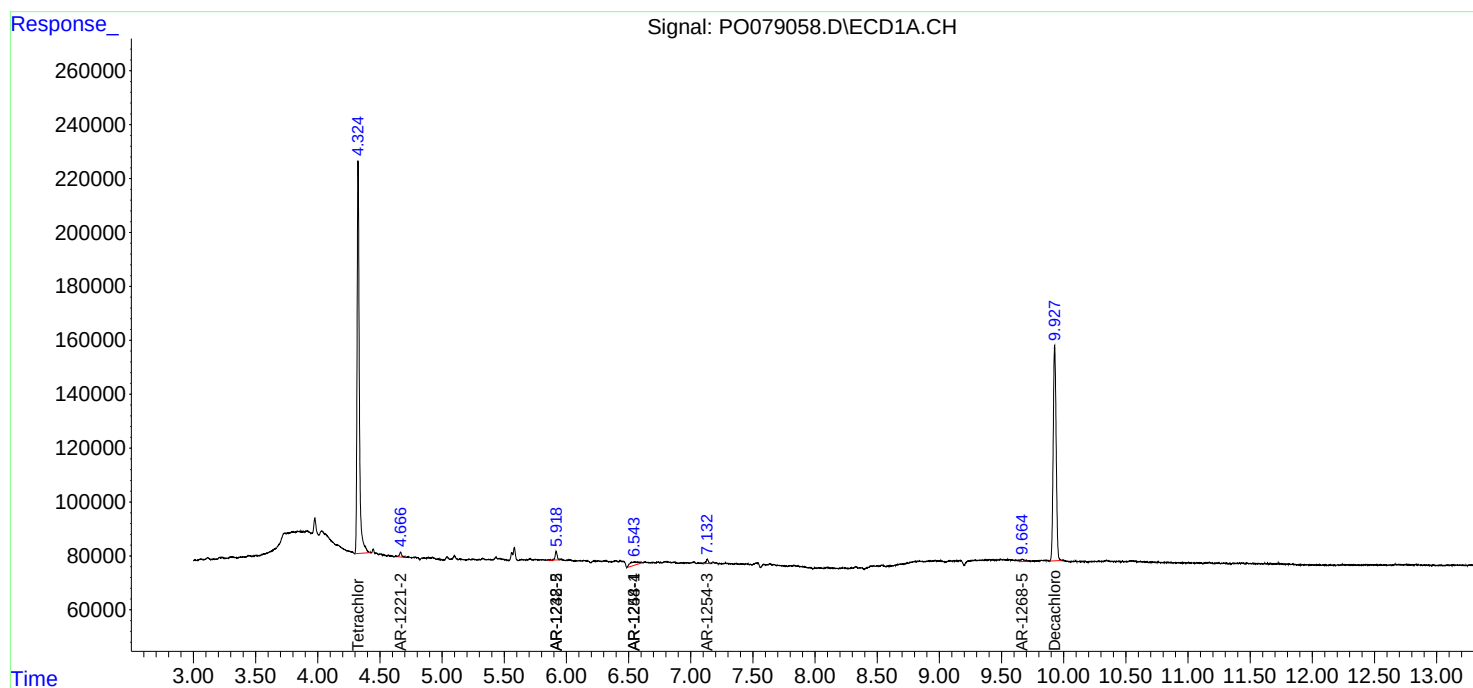


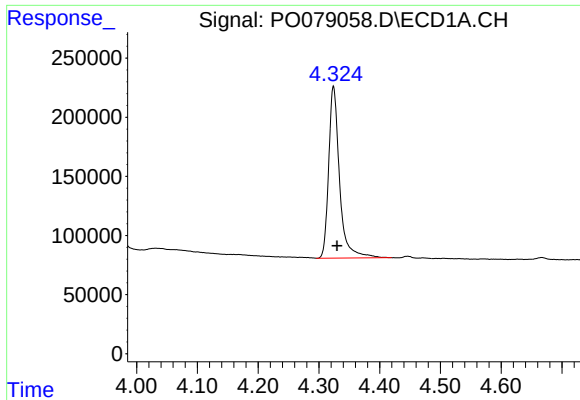

#1 Tetrachloro-m-xylene


R.T.: 4.324 min
Delta R.T.: -0.006 min
Response: 1808300
Conc: 22.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

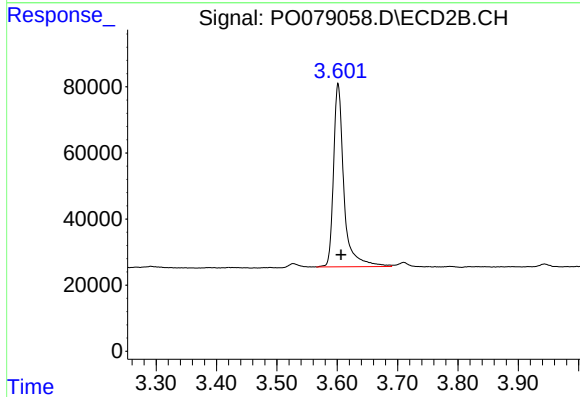


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.005 min
Response: 663925
Conc: 22.34 ng/ml

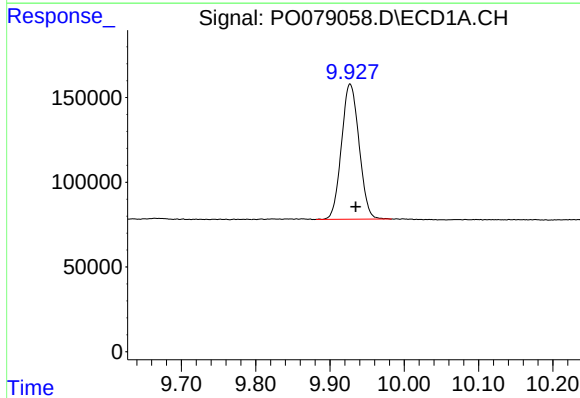


#2 Decachlorobiphenyl

R.T.: 9.927 min
Delta R.T.: -0.007 min
Response: 1313214
Conc: 21.03 ng/ml

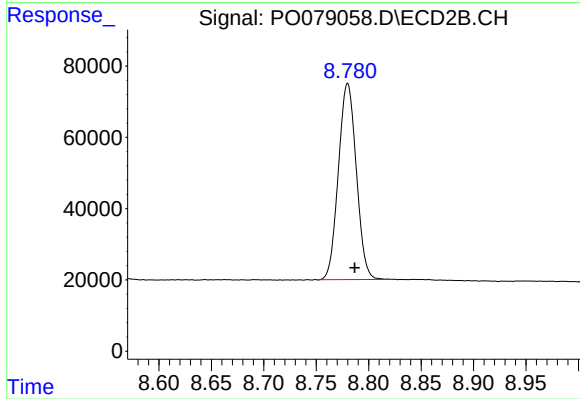

#2 Decachlorobiphenyl


R.T.: 8.780 min
Delta R.T.: -0.007 min
Response: 654628
Conc: 21.97 ng/ml

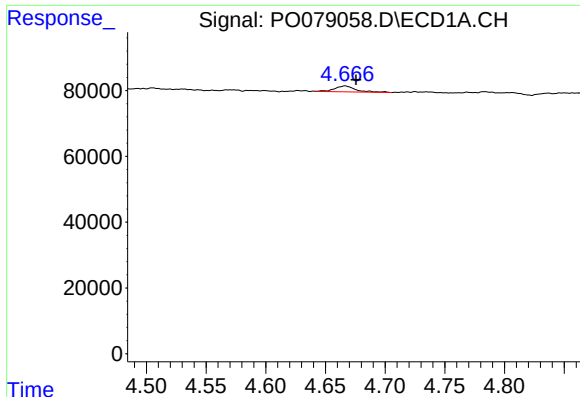

#9 AR-1221-2


R.T.: 4.666 min
Delta R.T.: -0.009 min
Response: 22195
Conc: 36.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

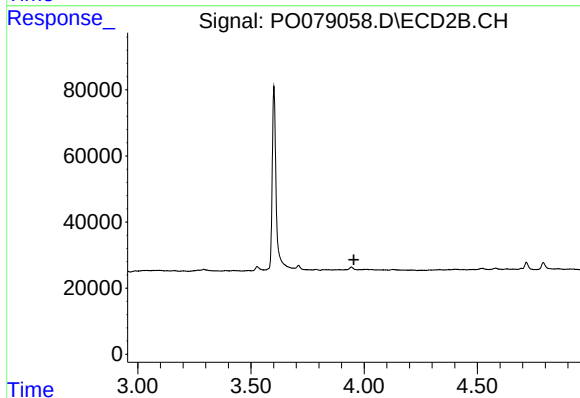


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.955 min
Response: 0
Conc: N.D.

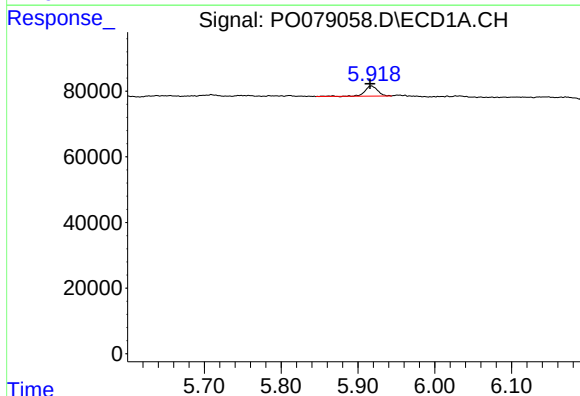


#15 AR-1232-5

R.T.: 5.918 min
Delta R.T.: 0.002 min
Response: 36208
Conc: 70.10 ng/ml

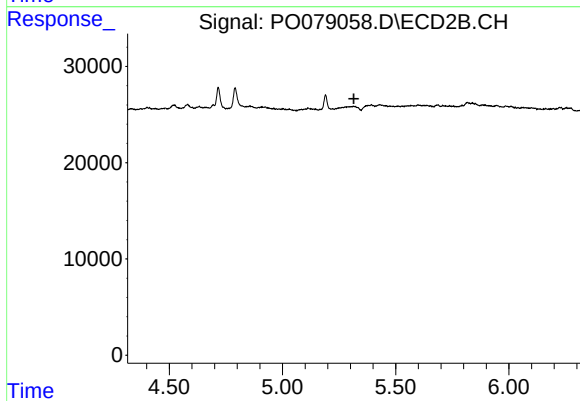

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.315 min
Response: 0
Conc: N.D.

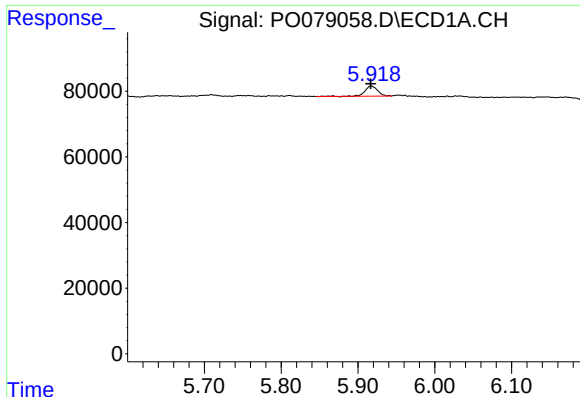

#22 AR-1248-2


R.T.: 5.918 min
Delta R.T.: 0.000 min
Response: 36208
Conc: 16.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

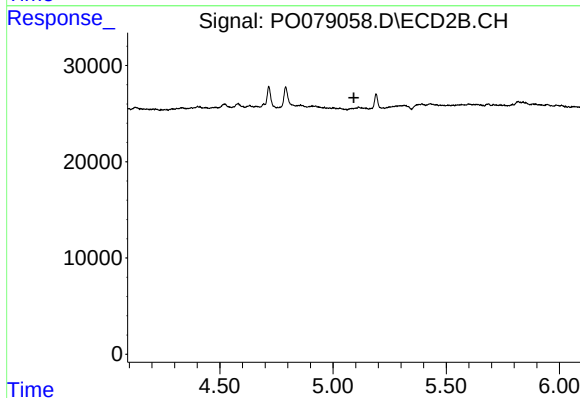


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.092 min
Response: 0
Conc: N.D.

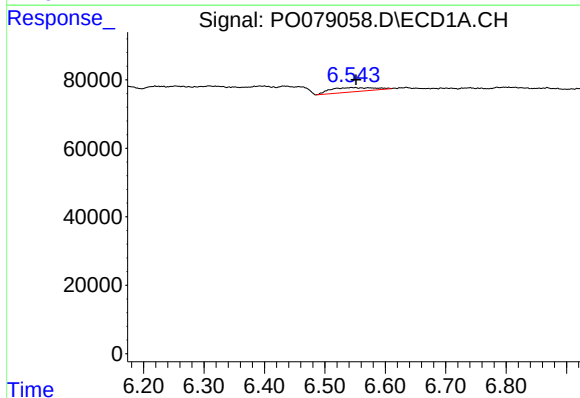


#24 AR-1248-4

R.T.: 6.546 min
Delta R.T.: -0.006 min
Response: 61800
Conc: 22.30 ng/ml

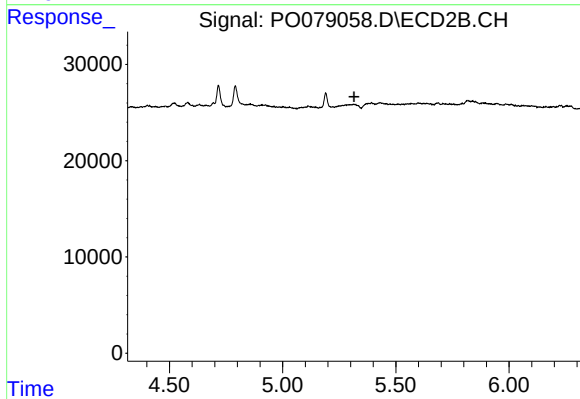

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.315 min
Response: 0
Conc: N.D.

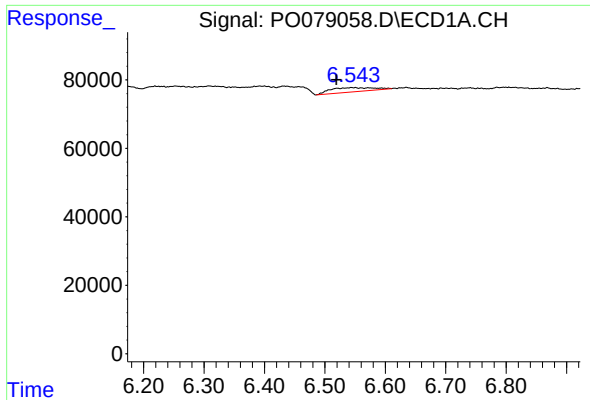

#26 AR-1254-1


R.T.: 6.546 min
Delta R.T.: 0.027 min
Response: 61800
Conc: 22.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

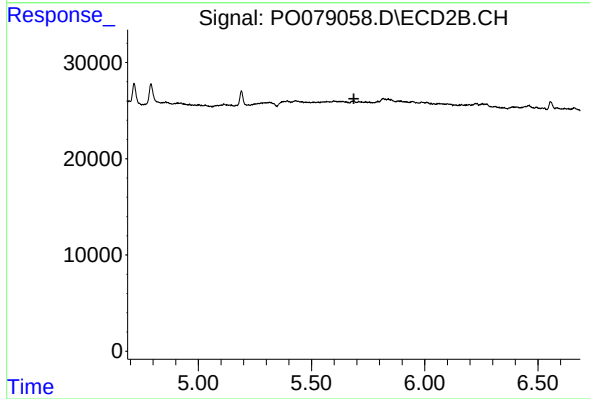


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.687 min
Response: 0
Conc: N.D.

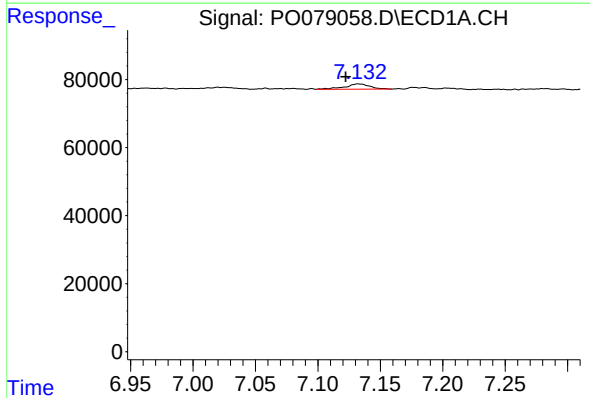


#28 AR-1254-3

R.T.: 7.133 min
Delta R.T.: 0.010 min
Response: 21278
Conc: 4.78 ng/ml

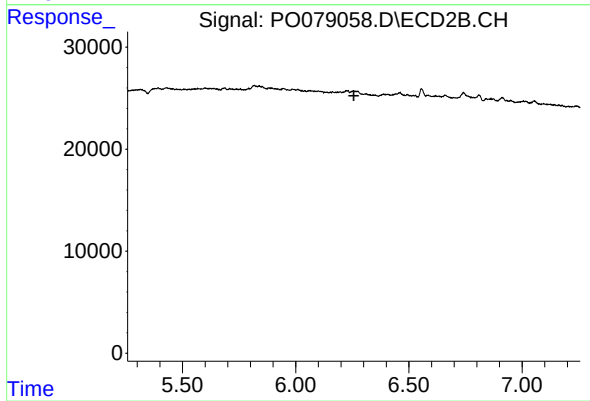

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.257 min
Response: 0
Conc: N.D.

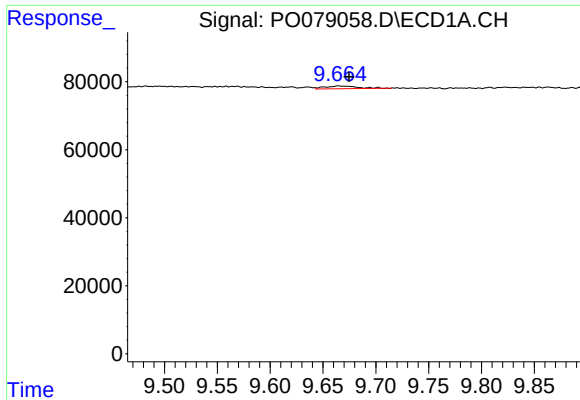

#45 AR-1268-5

R.T.: 9.666 min
Delta R.T.: -0.009 min
Response: 17403
Conc: 0.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

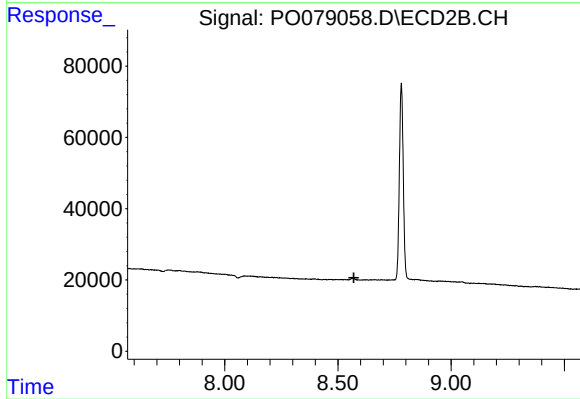

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.571 min
Response: 0
Conc: N.D.