

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062321\
 Data File : P0079050.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 11:14
 Operator : DD\AJ
 Sample : M2789-27
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 2ND-WALLS

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:22:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:26:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.602	1150175	420536	14.573	14.150
2) SA Decachlor...	9.931	8.782	761688	382439	12.196	12.834
Target Compounds						
26) L6 AR-1254-1	6.515	5.683	49792	52040	18.486m	31.323 #
27) L6 AR-1254-2	6.742	5.841	129688	46452	30.919	31.520
28) L6 AR-1254-3	7.118	6.253	157812	75438	35.435	33.916
29) L6 AR-1254-4	7.410	6.491	101027	39056	32.833	28.725
30) L6 AR-1254-5	7.833	6.913	111393	75330	34.124	37.832

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079050.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 11:14
Operator : DD\AJ
Sample : M2789-27
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
2ND-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:26:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

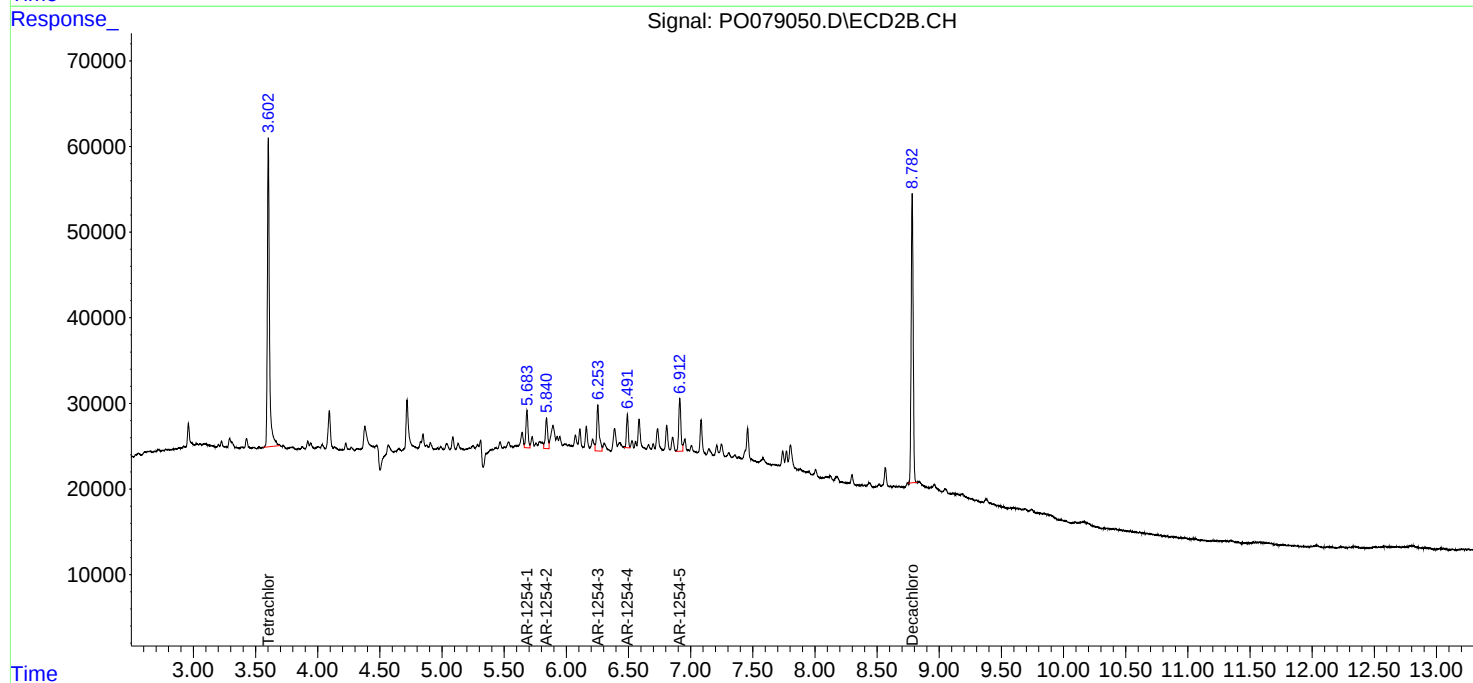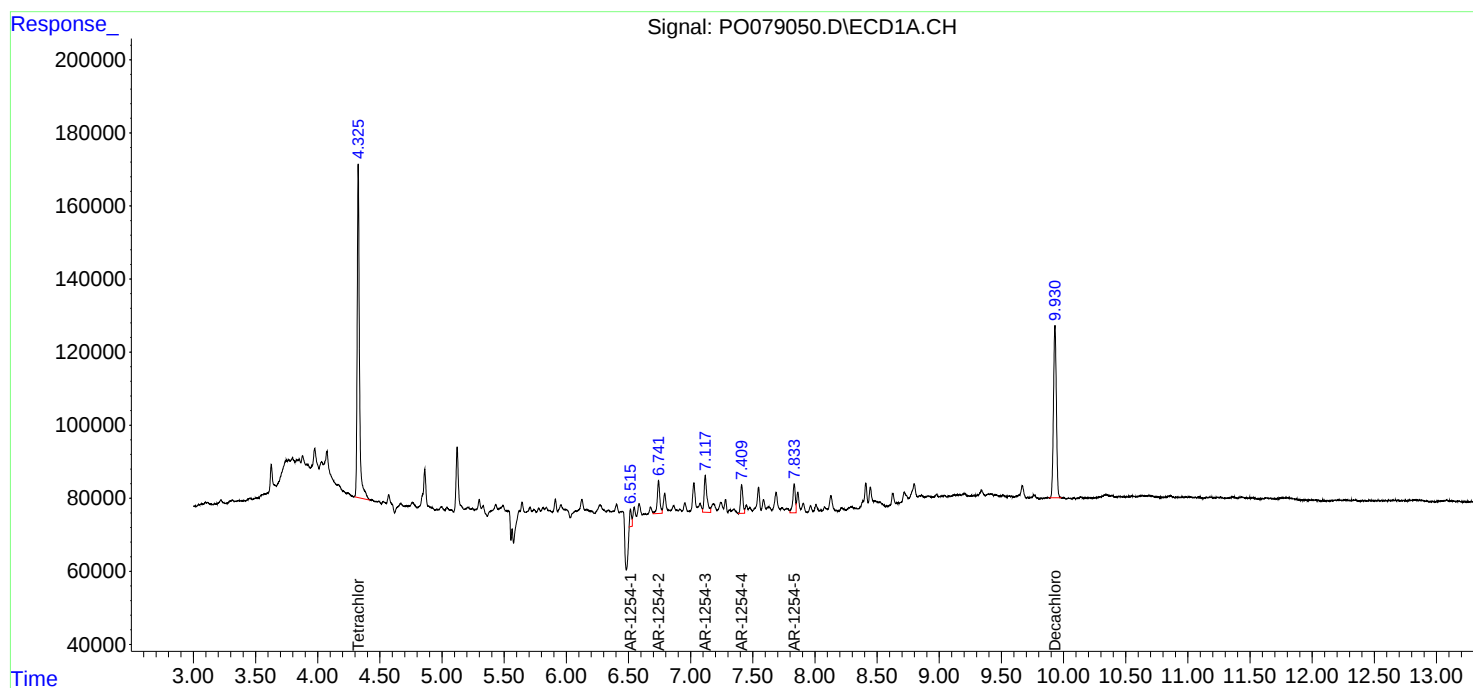

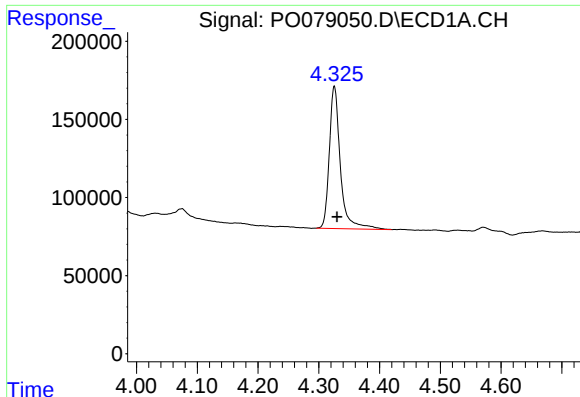


#1 Tetrachloro-m-xylene

R.T.: 4.326 min
Delta R.T.: -0.004 min
Response: 1150175
Conc: 14.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
2ND-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:08 PM

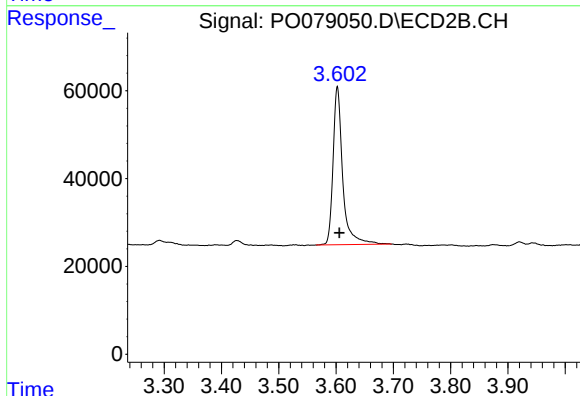


#1 Tetrachloro-m-xylene

R.T.: 3.602 min
Delta R.T.: -0.004 min
Response: 420536
Conc: 14.15 ng/ml

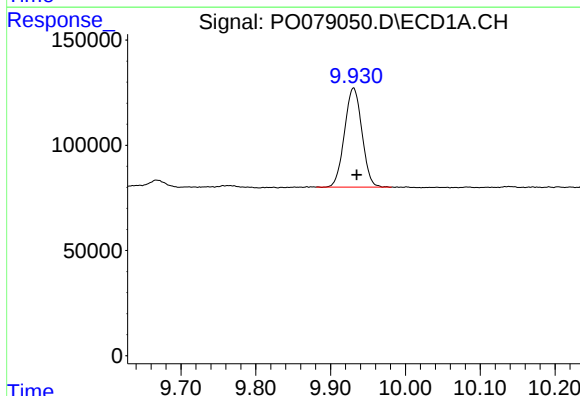


#2 Decachlorobiphenyl

R.T.: 9.931 min
Delta R.T.: -0.004 min
Response: 761688
Conc: 12.20 ng/ml

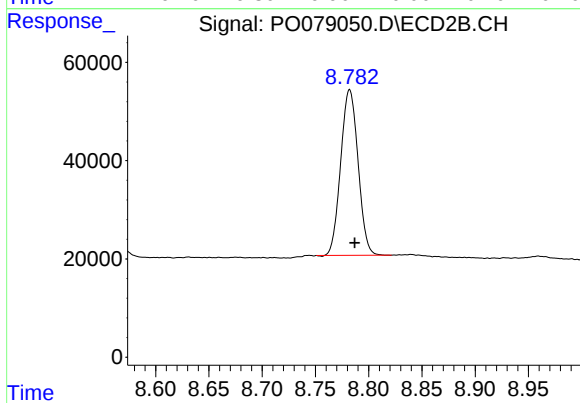

#2 Decachlorobiphenyl

R.T.: 8.782 min
Delta R.T.: -0.005 min
Response: 382439
Conc: 12.83 ng/ml

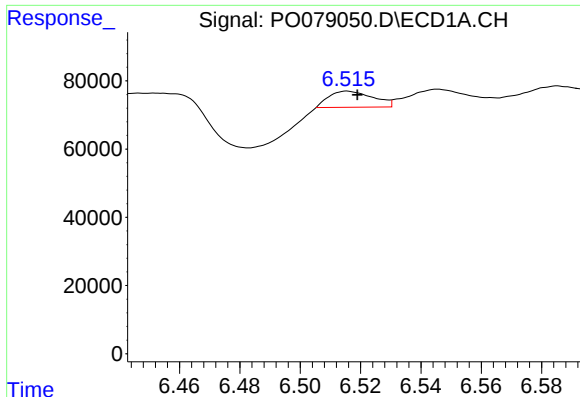


#26 AR-1254-1

R.T.: 6.515 min
Delta R.T.: -0.004 min
Response: 49792
Conc: 18.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
2ND-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:08 PM

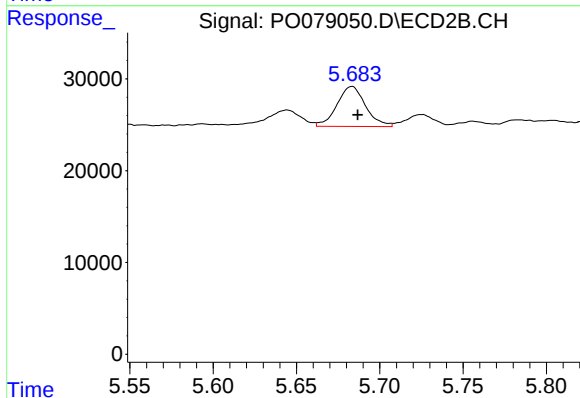


#26 AR-1254-1

R.T.: 5.683 min
Delta R.T.: -0.004 min
Response: 52040
Conc: 31.32 ng/ml

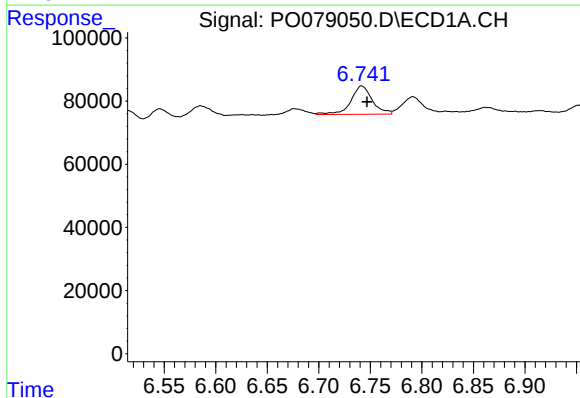


#27 AR-1254-2

R.T.: 6.742 min
Delta R.T.: -0.005 min
Response: 129688
Conc: 30.92 ng/ml

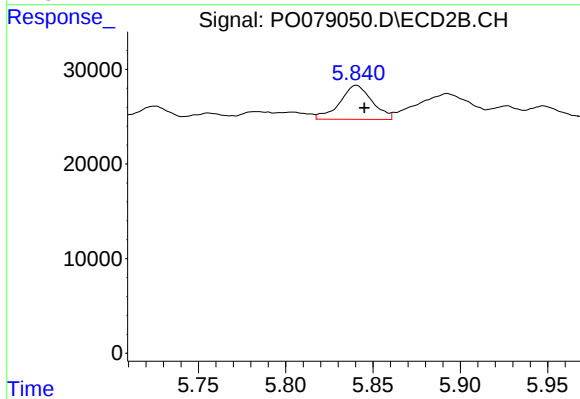

#27 AR-1254-2

R.T.: 5.841 min
Delta R.T.: -0.004 min
Response: 46452
Conc: 31.52 ng/ml

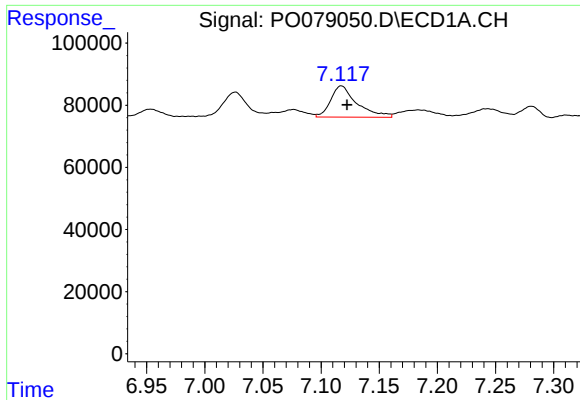


#28 AR-1254-3

R.T.: 7.118 min
Delta R.T.: -0.005 min
Response: 157812
Conc: 35.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
2ND-WALLS


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:08 PM

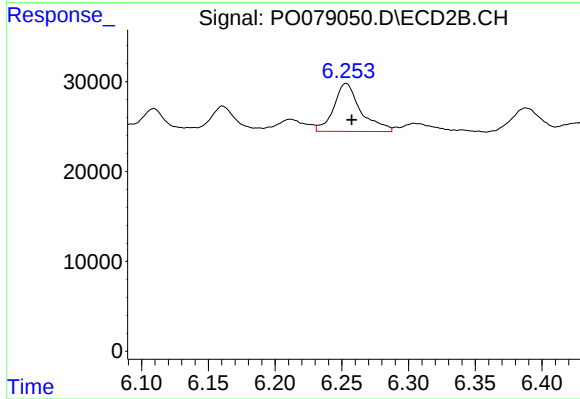


#28 AR-1254-3

R.T.: 6.253 min
Delta R.T.: -0.004 min
Response: 75438
Conc: 33.92 ng/ml

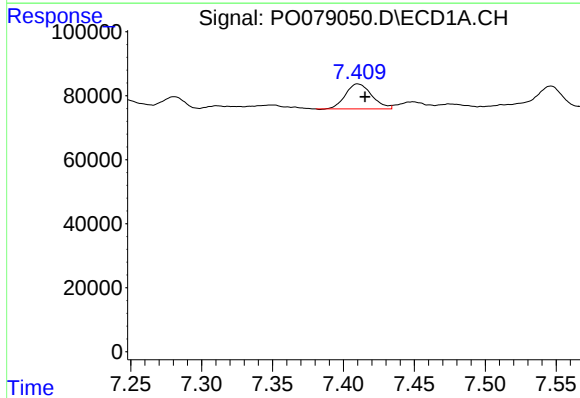


#29 AR-1254-4

R.T.: 7.410 min
Delta R.T.: -0.005 min
Response: 101027
Conc: 32.83 ng/ml

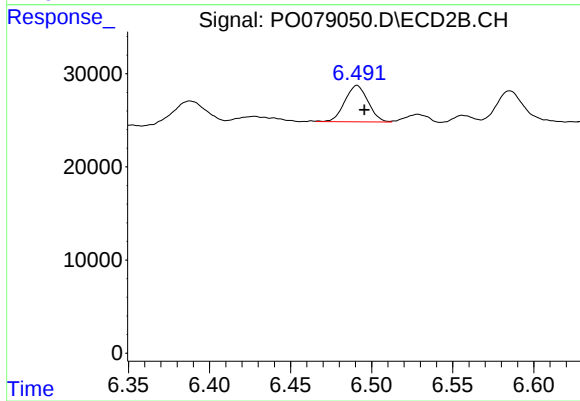

#29 AR-1254-4

R.T.: 6.491 min
Delta R.T.: -0.005 min
Response: 39056
Conc: 28.72 ng/ml

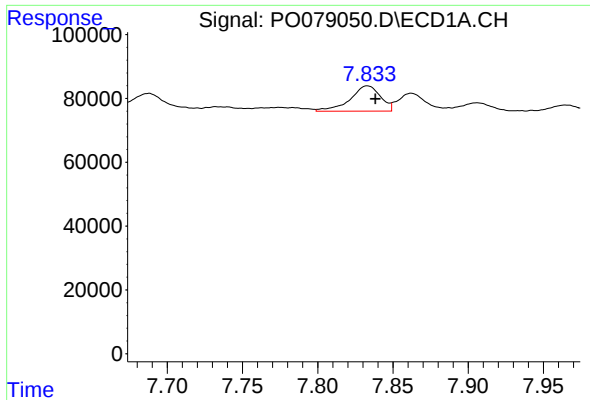


#30 AR-1254-5

R.T.: 7.833 min
Delta R.T.: -0.005 min
Response: 111393
Conc: 34.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
2ND-WALLS

Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:08 PM

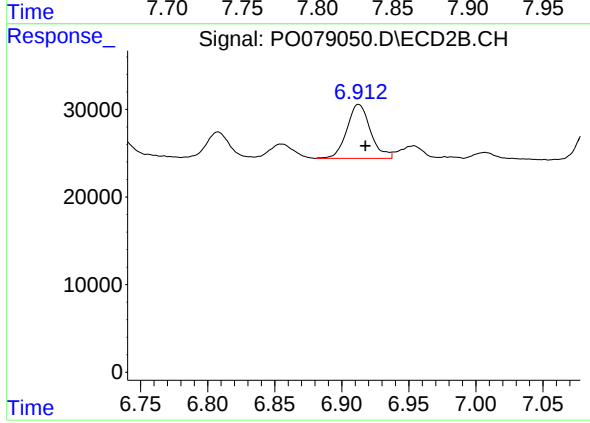

#30 AR-1254-5

R.T.: 6.913 min
Delta R.T.: -0.005 min
Response: 75330
Conc: 37.83 ng/ml