

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079065.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 15:32
 Operator : DD\AJ
 Sample : M2816-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-062221

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:22:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:36:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.602	1304799	504653	16.533m	16.980
2) SA Decachlor...	9.929	8.781	857871	419710	13.736	14.085
Target Compounds						
26) L6 AR-1254-1	6.514	5.683	262560	146690	97.478	88.294
27) L6 AR-1254-2	6.742	5.840	408182	139427	97.316	94.610
28) L6 AR-1254-3	7.117	6.253	443270	205873	99.531	92.560
29) L6 AR-1254-4	7.410	6.490	275201	112225	89.439	82.538
30) L6 AR-1254-5	7.833	6.913	350465	211826	107.362	106.383

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079065.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 15:32
Operator : DD\AJ
Sample : M2816-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:36:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

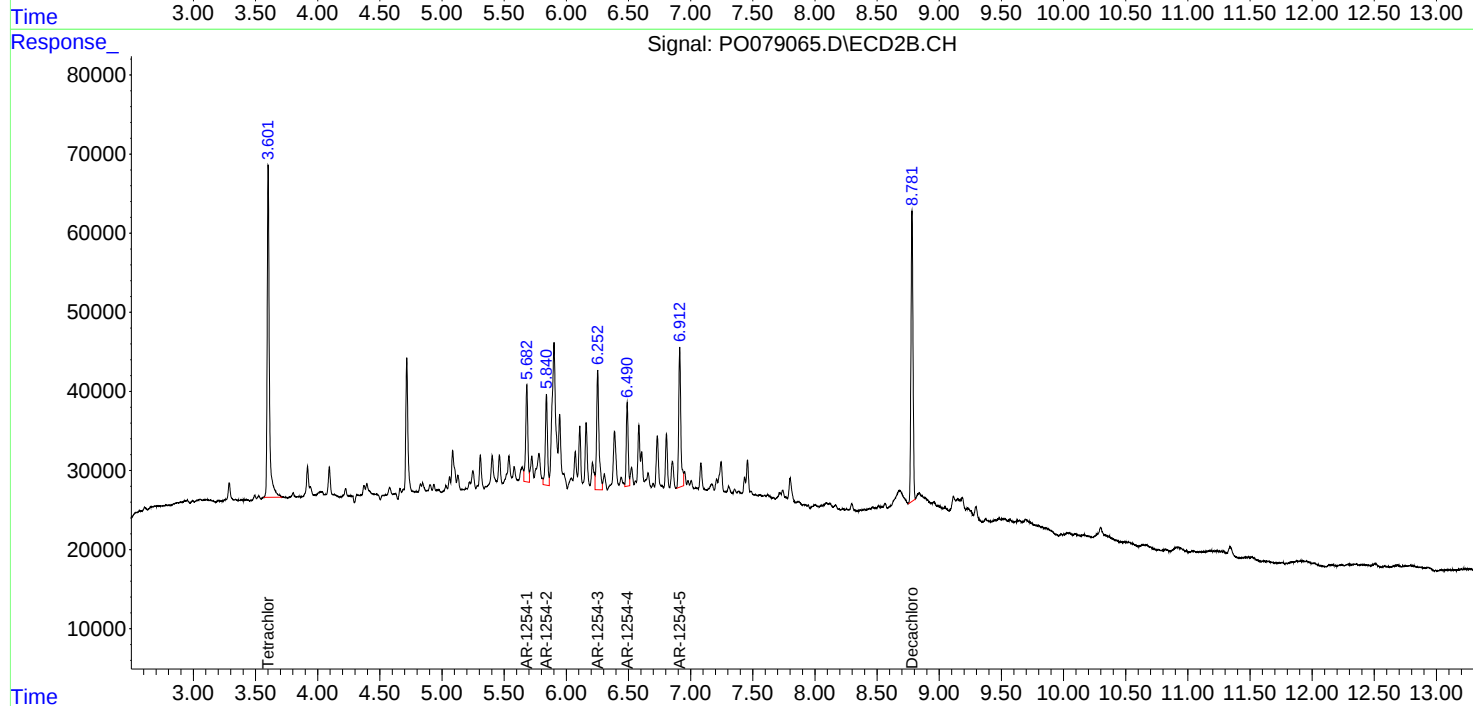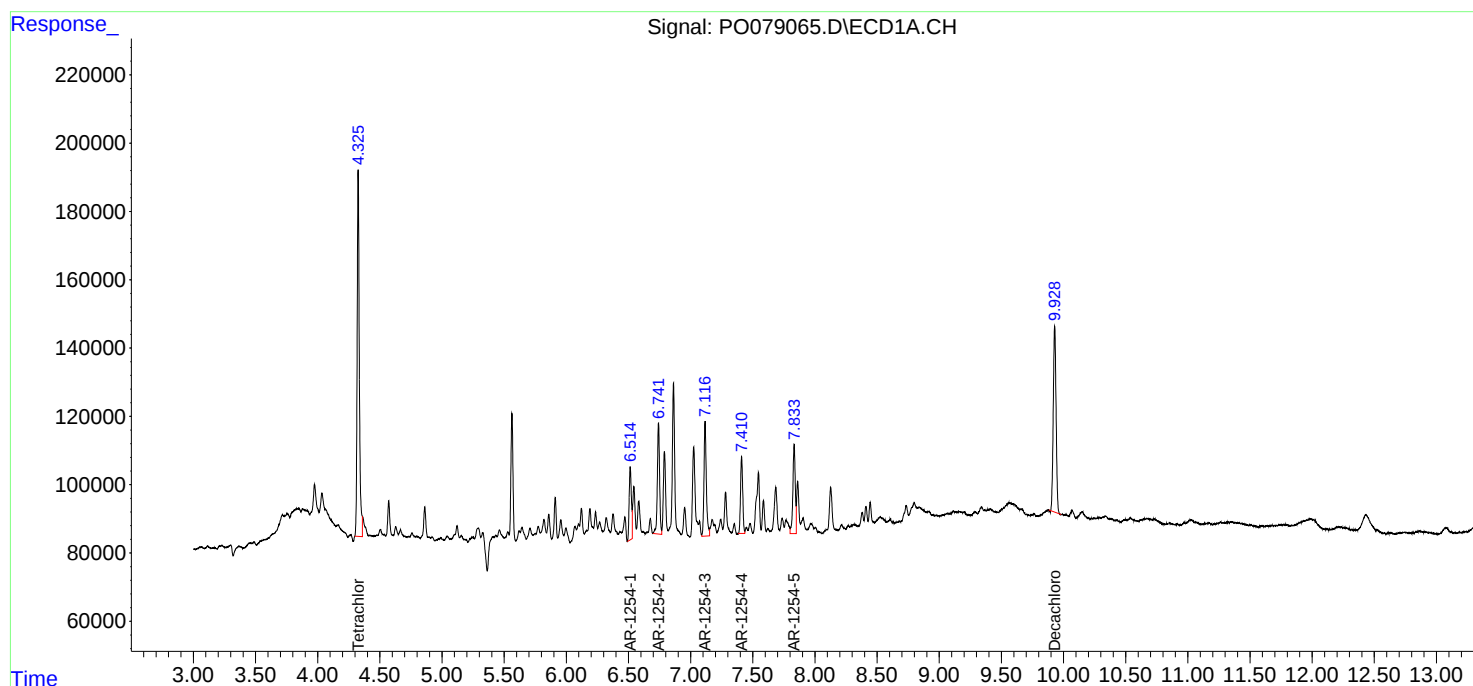

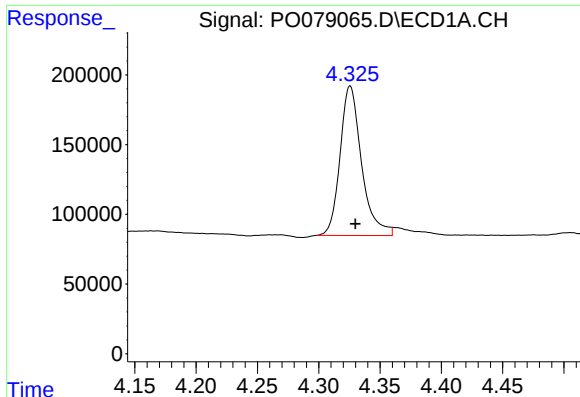


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.005 min
Response: 1304799
Conc: 16.53 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:29 PM

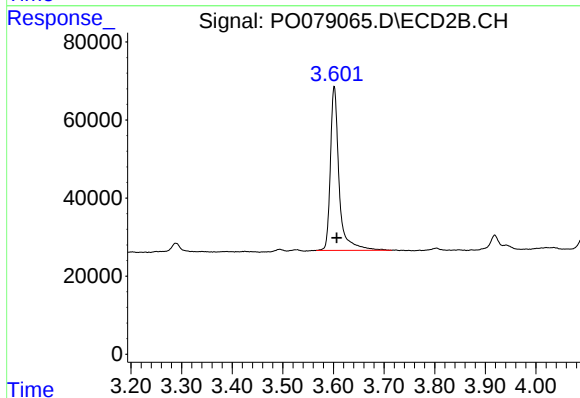


#1 Tetrachloro-m-xylene

R.T.: 3.602 min
Delta R.T.: -0.005 min
Response: 504653
Conc: 16.98 ng/ml

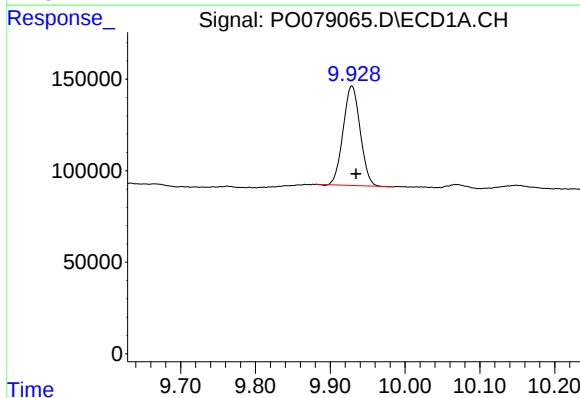


#2 Decachlorobiphenyl

R.T.: 9.929 min
Delta R.T.: -0.006 min
Response: 857871
Conc: 13.74 ng/ml

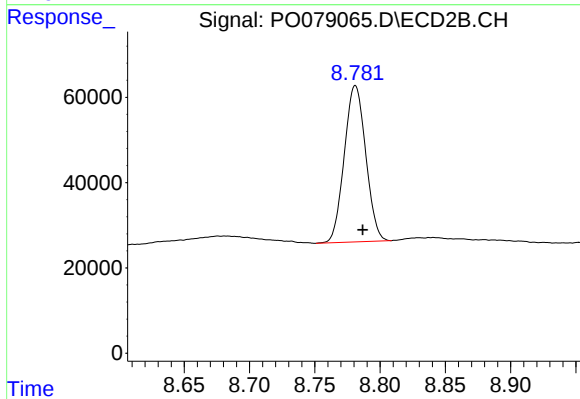

#2 Decachlorobiphenyl

R.T.: 8.781 min
Delta R.T.: -0.006 min
Response: 419710
Conc: 14.08 ng/ml

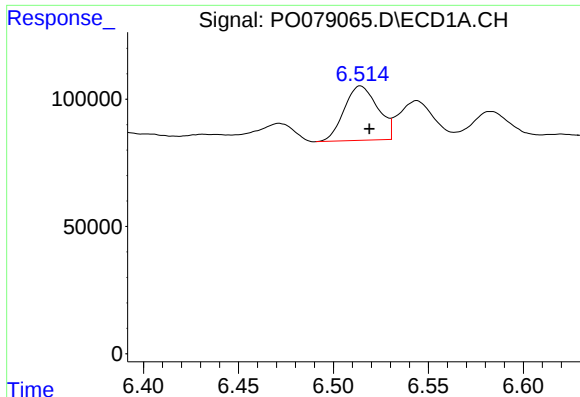


#26 AR-1254-1

R.T.: 6.514 min
Delta R.T.: -0.005 min
Response: 262560
Conc: 97.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:29 PM

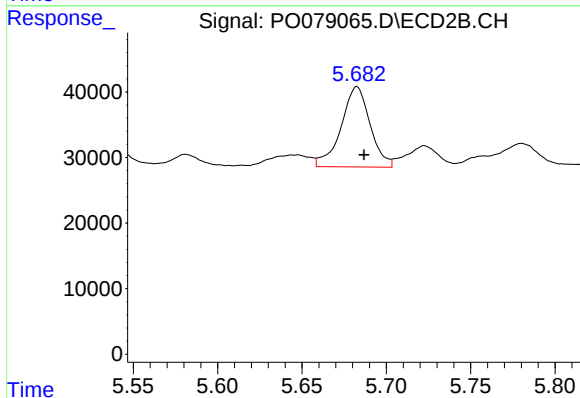


#26 AR-1254-1

R.T.: 5.683 min
Delta R.T.: -0.004 min
Response: 146690
Conc: 88.29 ng/ml

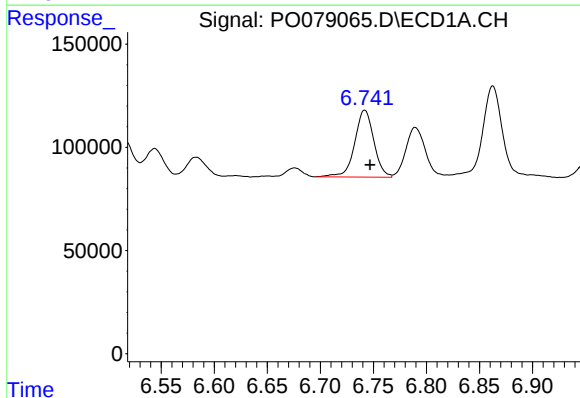


#27 AR-1254-2

R.T.: 6.742 min
Delta R.T.: -0.005 min
Response: 408182
Conc: 97.32 ng/ml

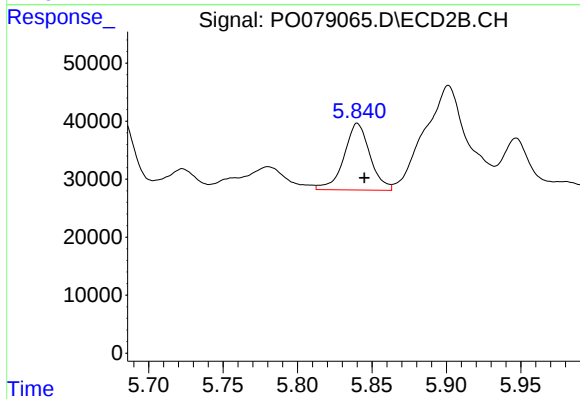

#27 AR-1254-2

R.T.: 5.840 min
Delta R.T.: -0.005 min
Response: 139427
Conc: 94.61 ng/ml

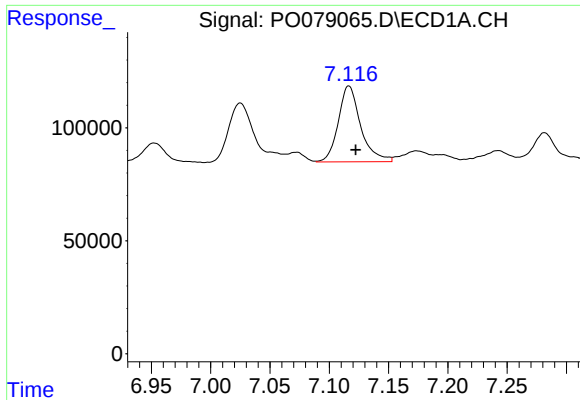


#28 AR-1254-3

R.T.: 7.117 min
Delta R.T.: -0.006 min
Response: 443270
Conc: 99.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-062221


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:29 PM

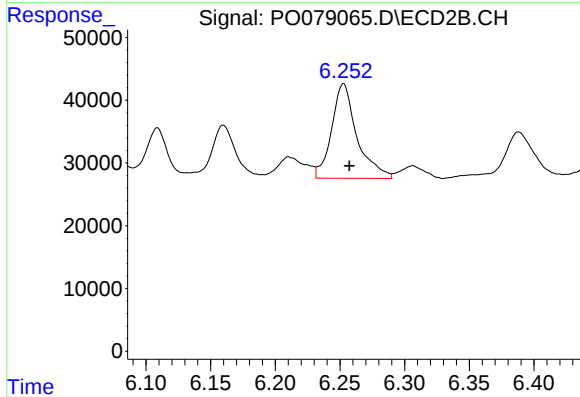


#28 AR-1254-3

R.T.: 6.253 min
Delta R.T.: -0.005 min
Response: 205873
Conc: 92.56 ng/ml

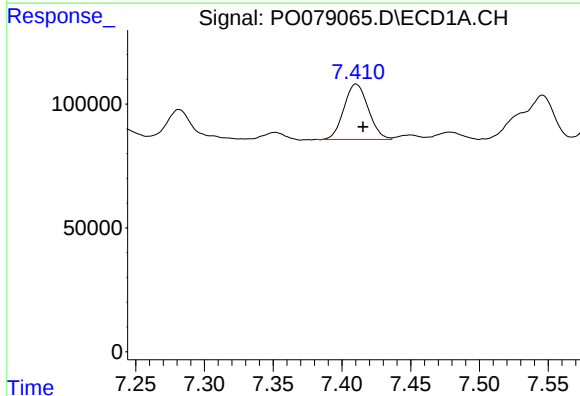


#29 AR-1254-4

R.T.: 7.410 min
Delta R.T.: -0.005 min
Response: 275201
Conc: 89.44 ng/ml

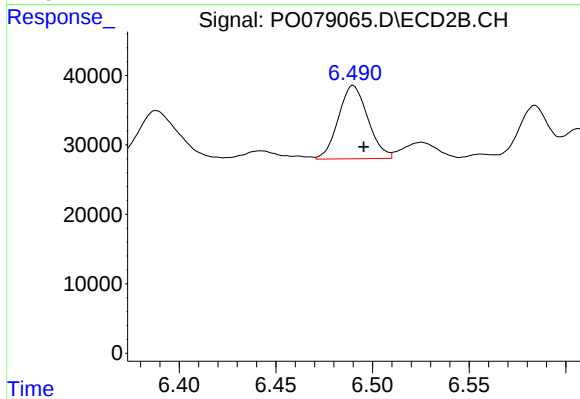

#29 AR-1254-4

R.T.: 6.490 min
Delta R.T.: -0.005 min
Response: 112225
Conc: 82.54 ng/ml

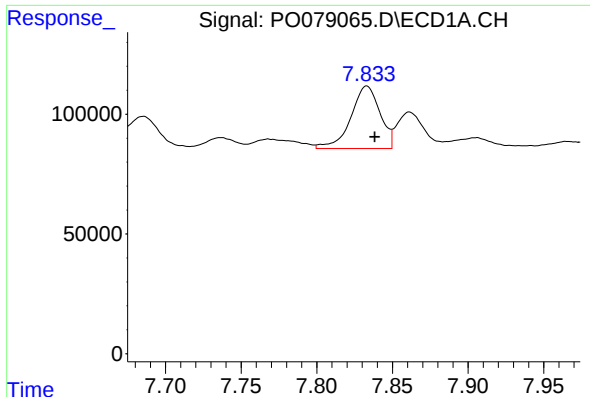


#30 AR-1254-5

R.T.: 7.833 min
Delta R.T.: -0.005 min
Response: 350465
Conc: 107.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-062221

Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:29 PM

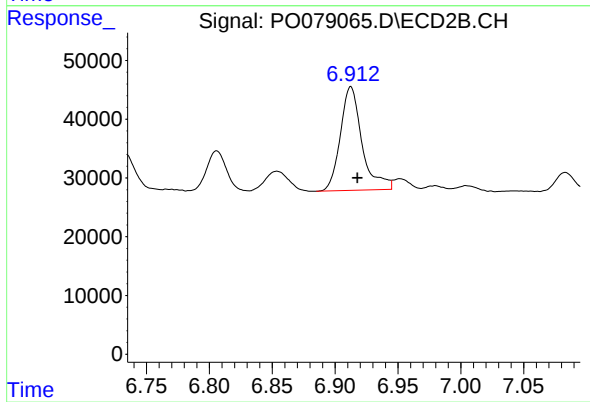

#30 AR-1254-5

R.T.: 6.913 min
Delta R.T.: -0.005 min
Response: 211826
Conc: 106.38 ng/ml