

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079068.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 16:24
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:22:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:38:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.325	3.601	4147395	1519652	52.550	51.131
2) SA Decachlor...	9.926	8.780	2779673	1287093	44.507	43.193
Target Compounds						
21) L5 AR-1248-1	5.620	4.827	780288	292739	494.008	459.794
22) L5 AR-1248-2	5.911	5.086	1076504	442213	486.607	447.956
23) L5 AR-1248-3	6.121	5.128	1281134	449417	494.055	452.687
24) L5 AR-1248-4	6.543	5.309	1358775	484185	490.244m	412.353
25) L5 AR-1248-5	6.582	5.724	1344549	508302	492.133m	472.059

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079068.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 16:24
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:38:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

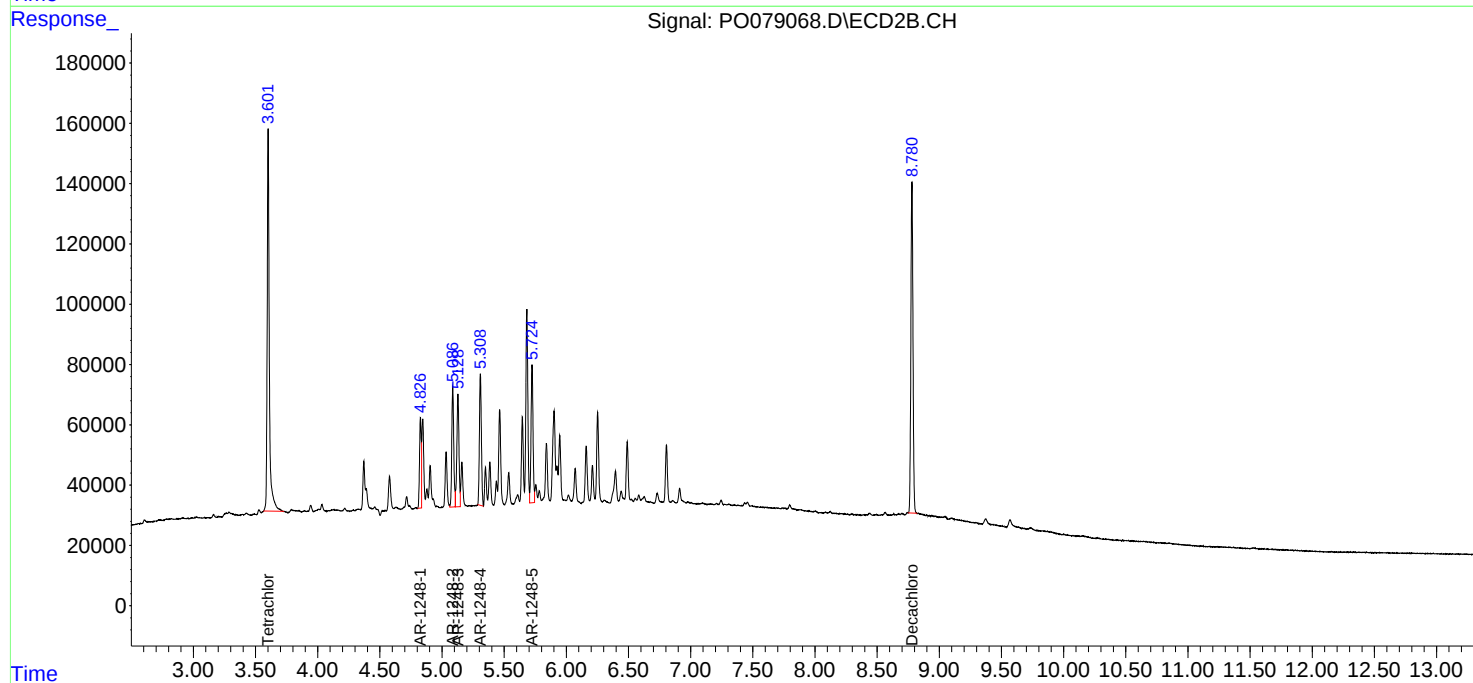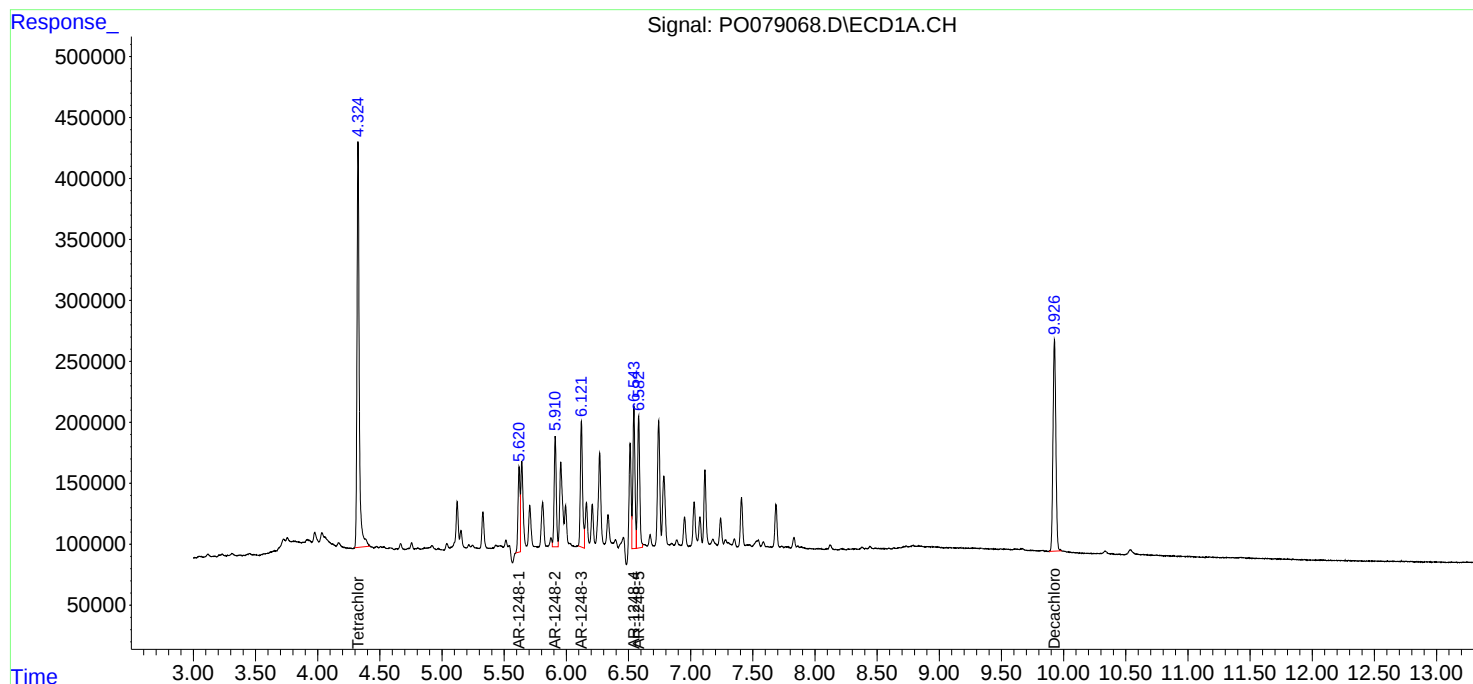

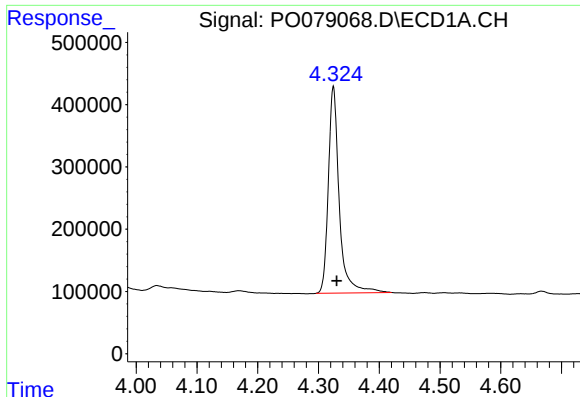


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: -0.005 min
Response: 4147395
Conc: 52.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:31 PM

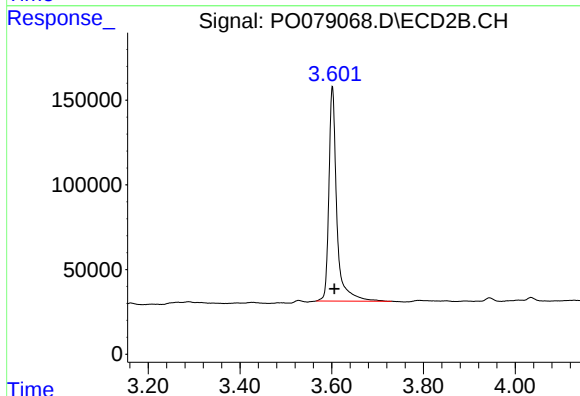


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.005 min
Response: 1519652
Conc: 51.13 ng/ml

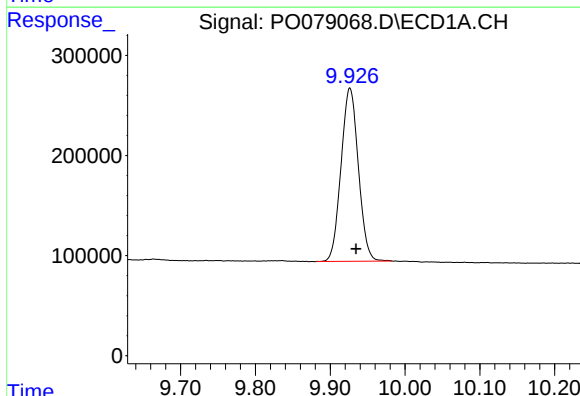


#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.008 min
Response: 2779673
Conc: 44.51 ng/ml

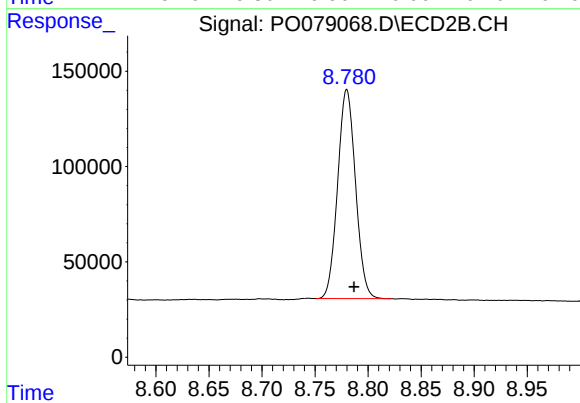

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.007 min
Response: 1287093
Conc: 43.19 ng/ml

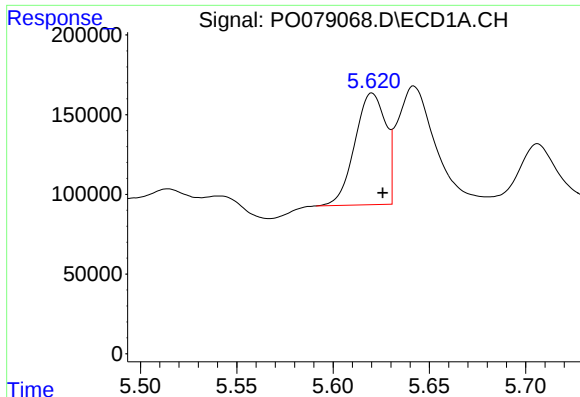


#21 AR-1248-1

R.T.: 5.620 min
Delta R.T.: -0.005 min
Response: 780288
Conc: 494.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:31 PM

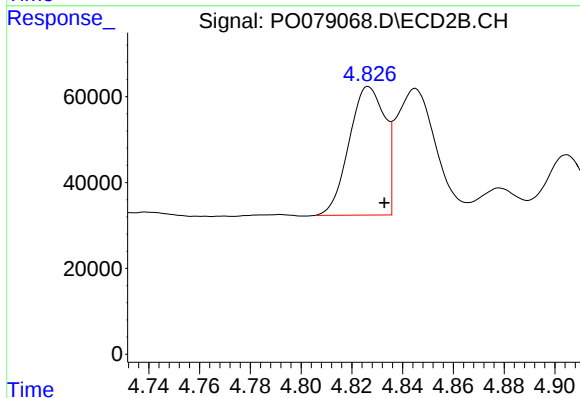


#21 AR-1248-1

R.T.: 4.827 min
Delta R.T.: -0.006 min
Response: 292739
Conc: 459.79 ng/ml

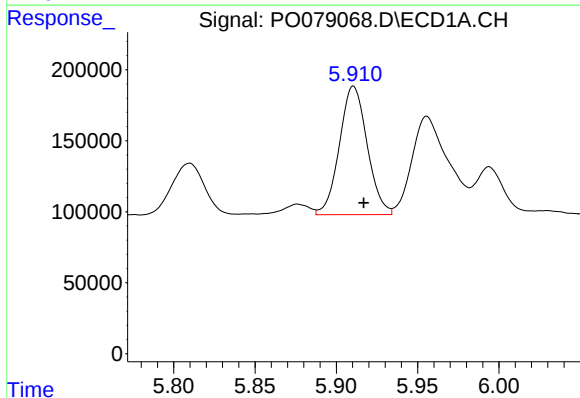


#22 AR-1248-2

R.T.: 5.911 min
Delta R.T.: -0.006 min
Response: 1076504
Conc: 486.61 ng/ml

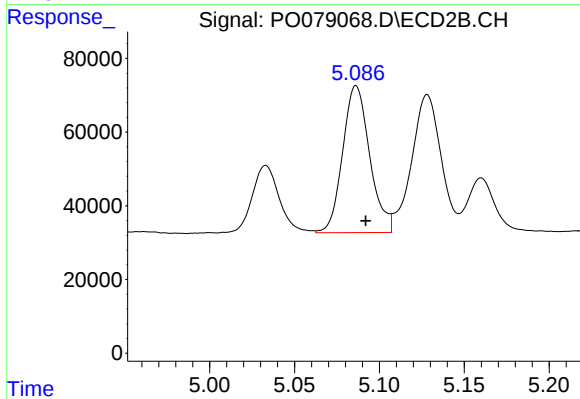

#22 AR-1248-2

R.T.: 5.086 min
Delta R.T.: -0.006 min
Response: 442213
Conc: 447.96 ng/ml

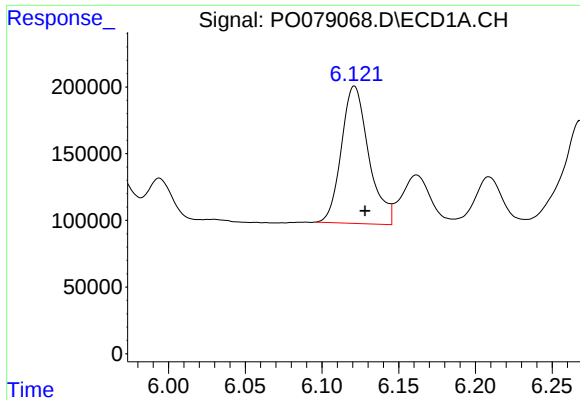


#23 AR-1248-3

R.T.: 6.121 min
Delta R.T.: -0.007 min
Response: 1281134
Conc: 494.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:31 PM

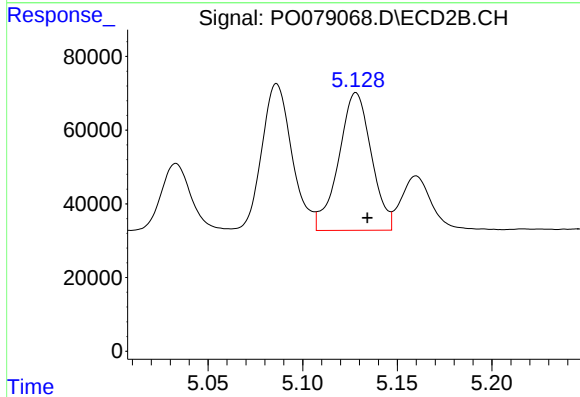


#23 AR-1248-3

R.T.: 5.128 min
Delta R.T.: -0.006 min
Response: 449417
Conc: 452.69 ng/ml

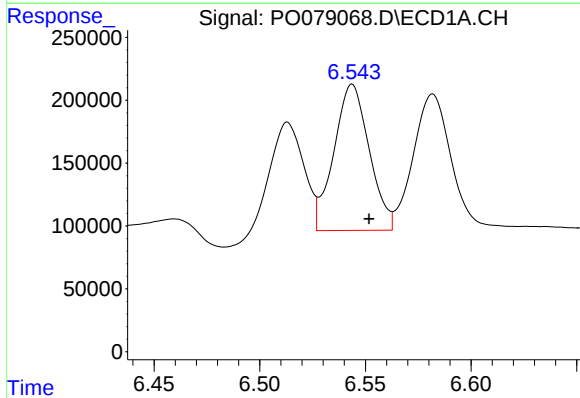


#24 AR-1248-4

R.T.: 6.543 min
Delta R.T.: -0.008 min
Response: 1358775
Conc: 490.24 ng/ml m

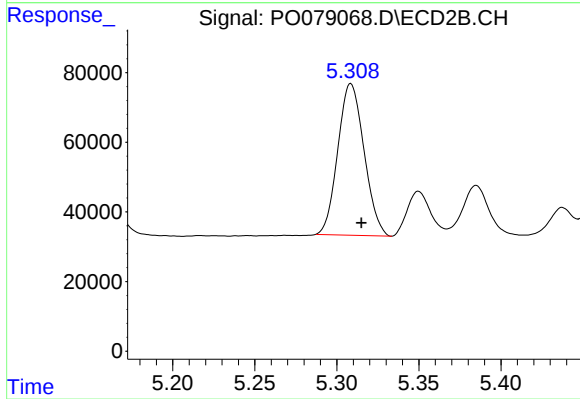

#24 AR-1248-4

R.T.: 5.309 min
Delta R.T.: -0.006 min
Response: 484185
Conc: 412.35 ng/ml

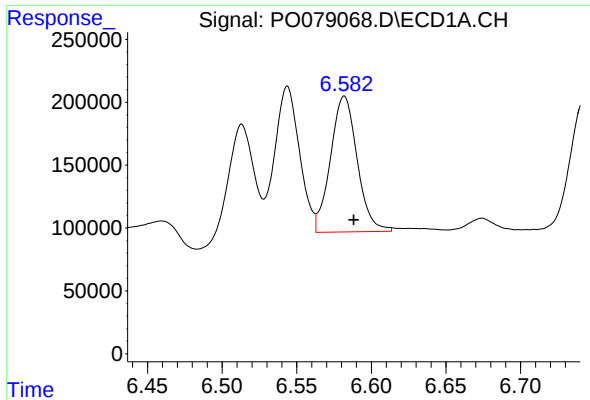


#25 AR-1248-5

R.T.: 6.582 min
Delta R.T.: -0.007 min
Response: 1344549
Conc: 492.13 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:31 PM

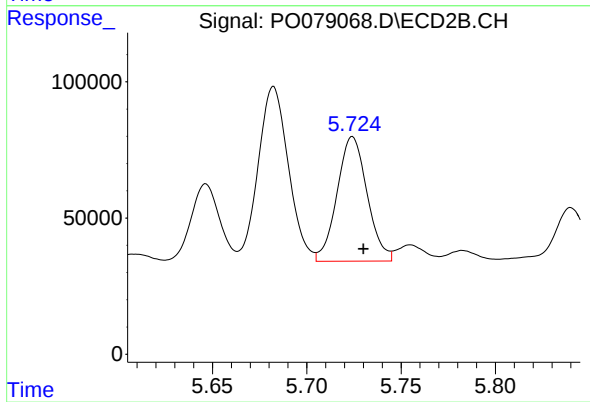

#25 AR-1248-5

R.T.: 5.724 min
Delta R.T.: -0.006 min
Response: 508302
Conc: 472.06 ng/ml