

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079075.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 18:25
 Operator : DD\AJ
 Sample : M2800-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BORING-ADDITION

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:43:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.326	3.602	1827509	692887	23.156	23.313
2) SA Decachlor...	9.927	8.780	1242614	598374	19.896	20.081

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079075.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 18:25
Operator : DD\AJ
Sample : M2800-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BORING-ADDITION

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:43:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

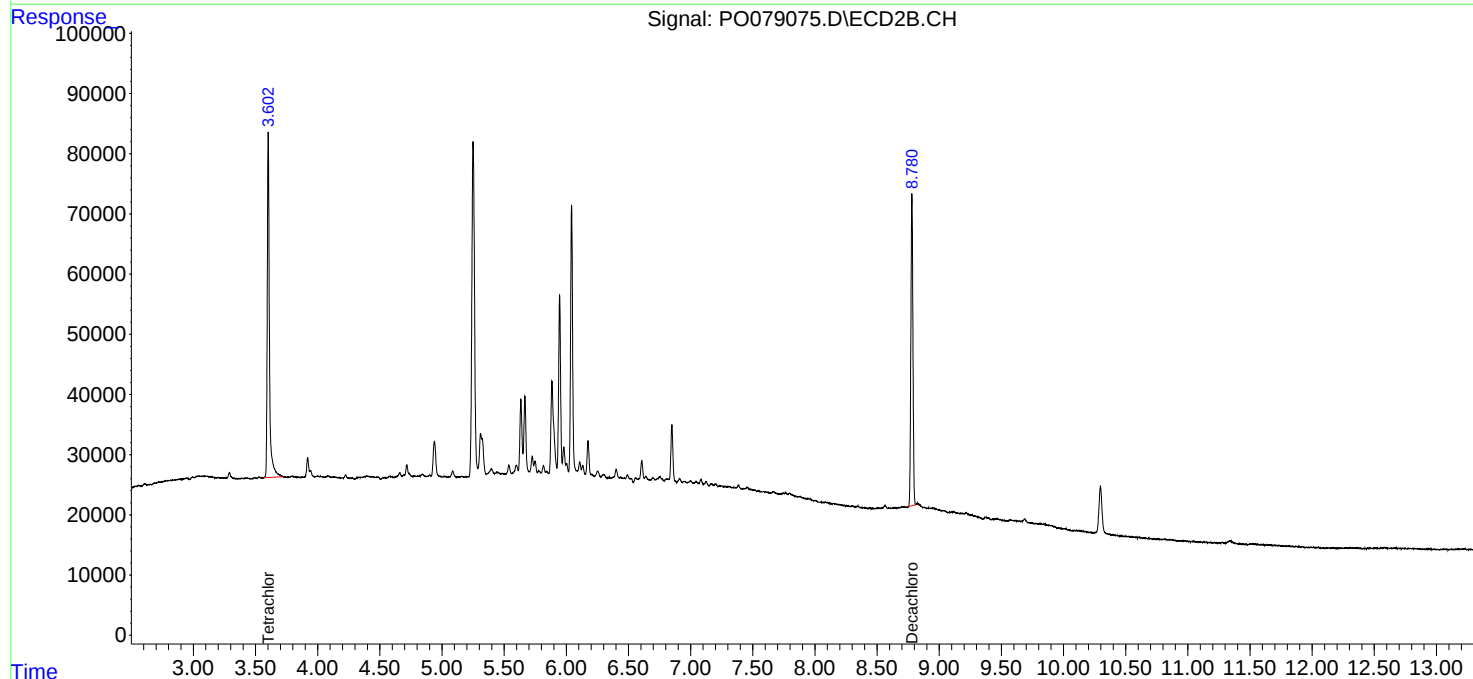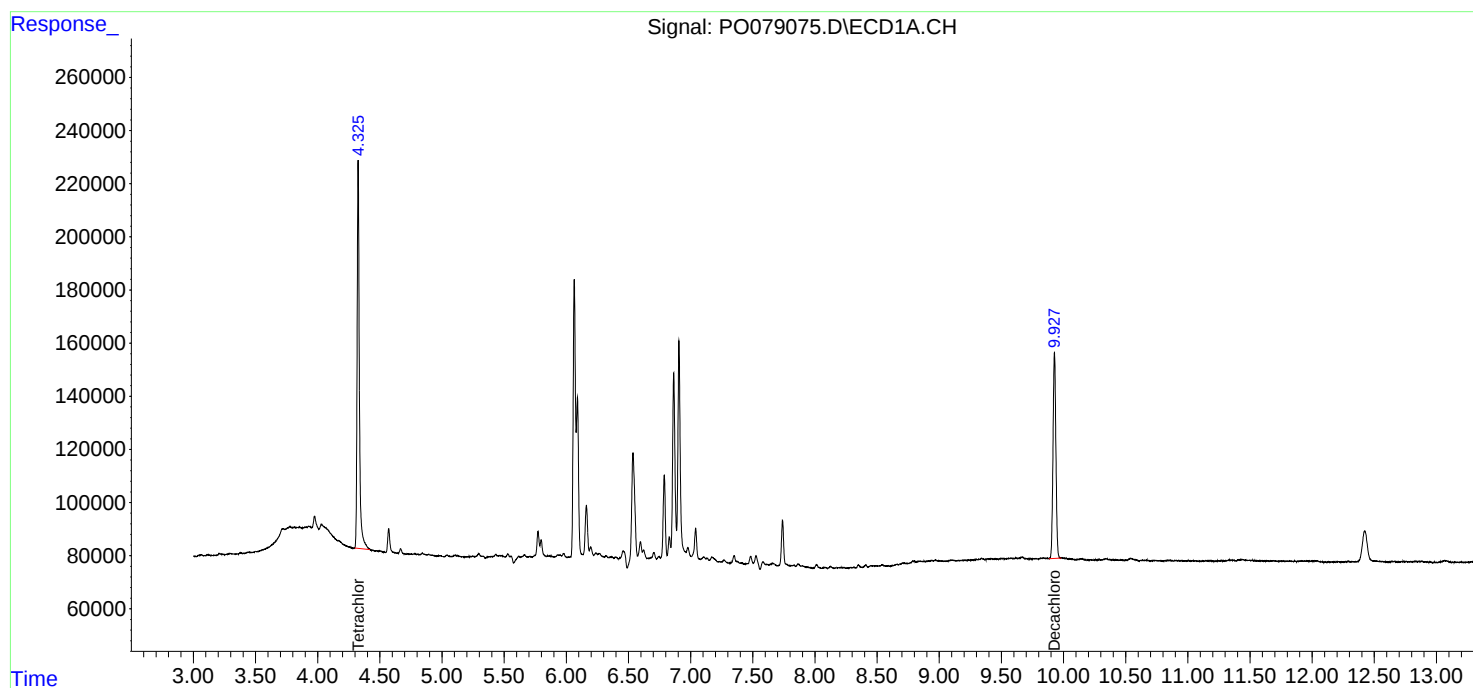


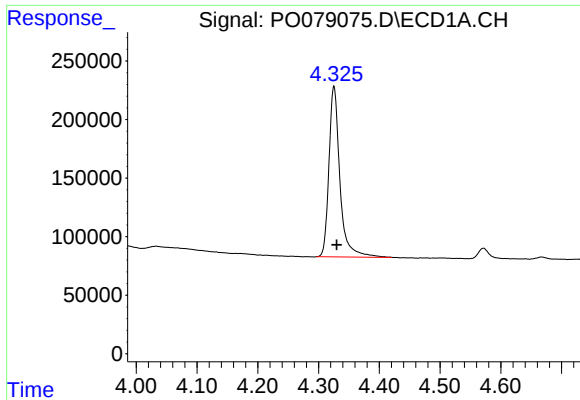

#1 Tetrachloro-m-xylene


R.T.: 4.326 min
Delta R.T.: -0.004 min
Response: 1827509
Conc: 23.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
BORING-ADDITION

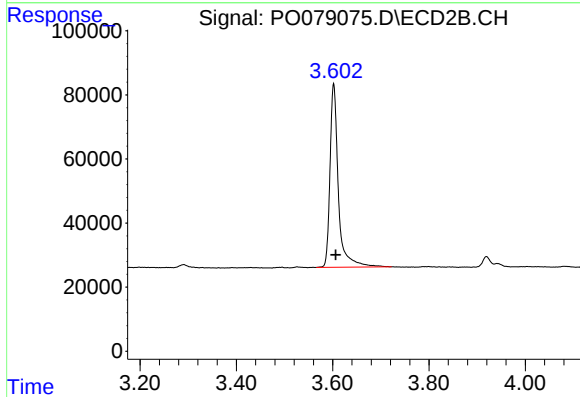


#1 Tetrachloro-m-xylene

R.T.: 3.602 min
Delta R.T.: -0.004 min
Response: 692887
Conc: 23.31 ng/ml

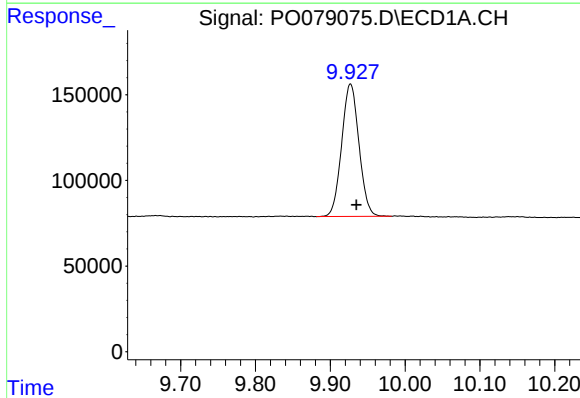

#2 Decachlorobiphenyl

R.T.: 9.927 min
Delta R.T.: -0.008 min
Response: 1242614
Conc: 19.90 ng/ml

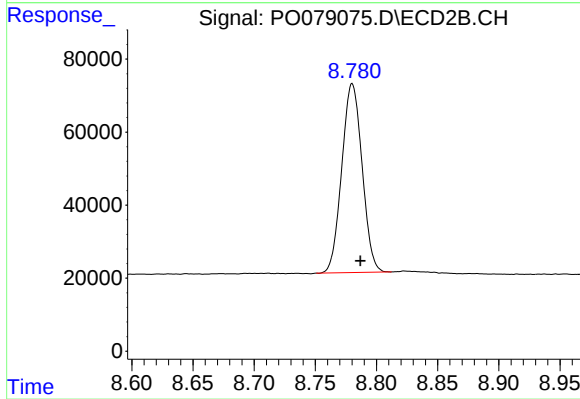

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: -0.007 min
Response: 598374
Conc: 20.08 ng/ml