

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079085.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 21:36
 Operator : DD\AJ
 Sample : M2812-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KG-WATER

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:22:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:50:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.323	3.601	1510961	493411	19.145m	16.601
2) SA Decachlor...	9.925	8.778	848512	418487	13.586	14.044

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079085.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 21:36
Operator : DD\AJ
Sample : M2812-07
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KG-WATER


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:50:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

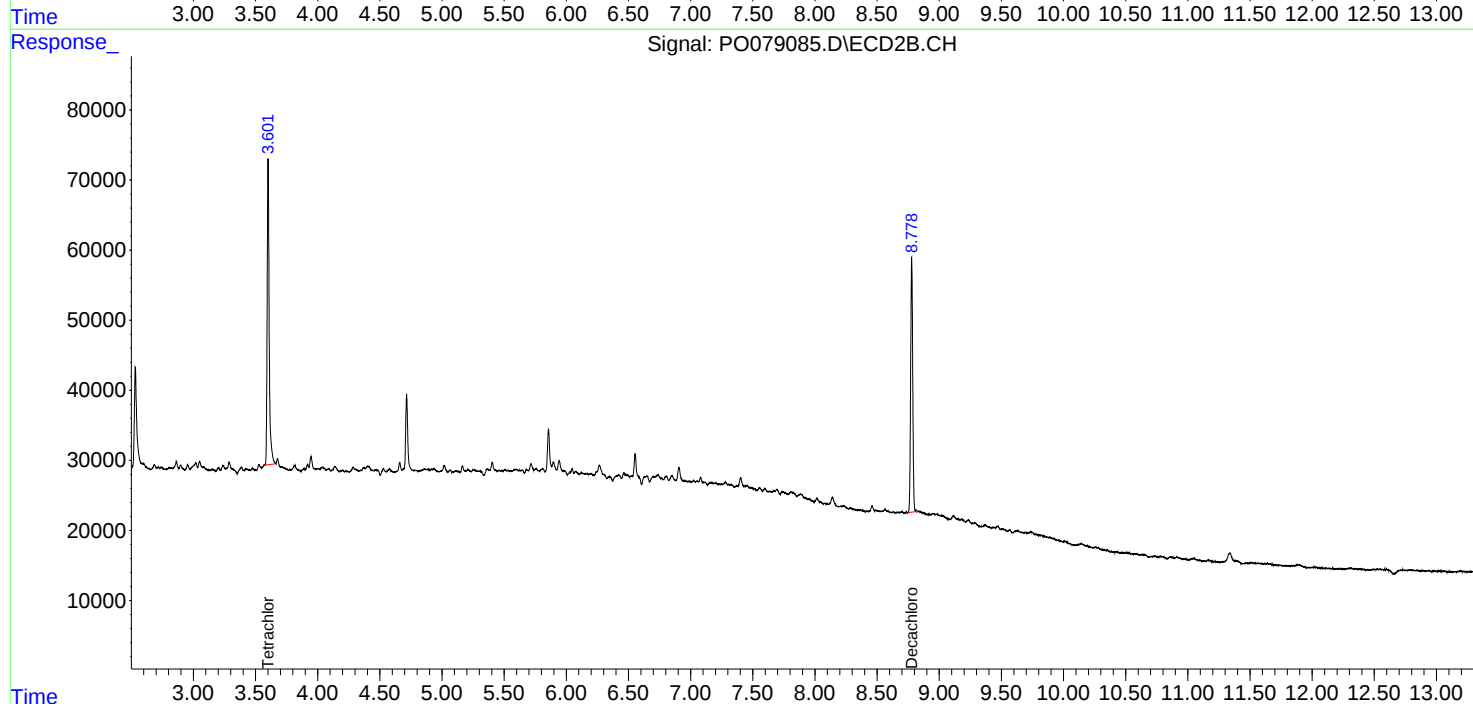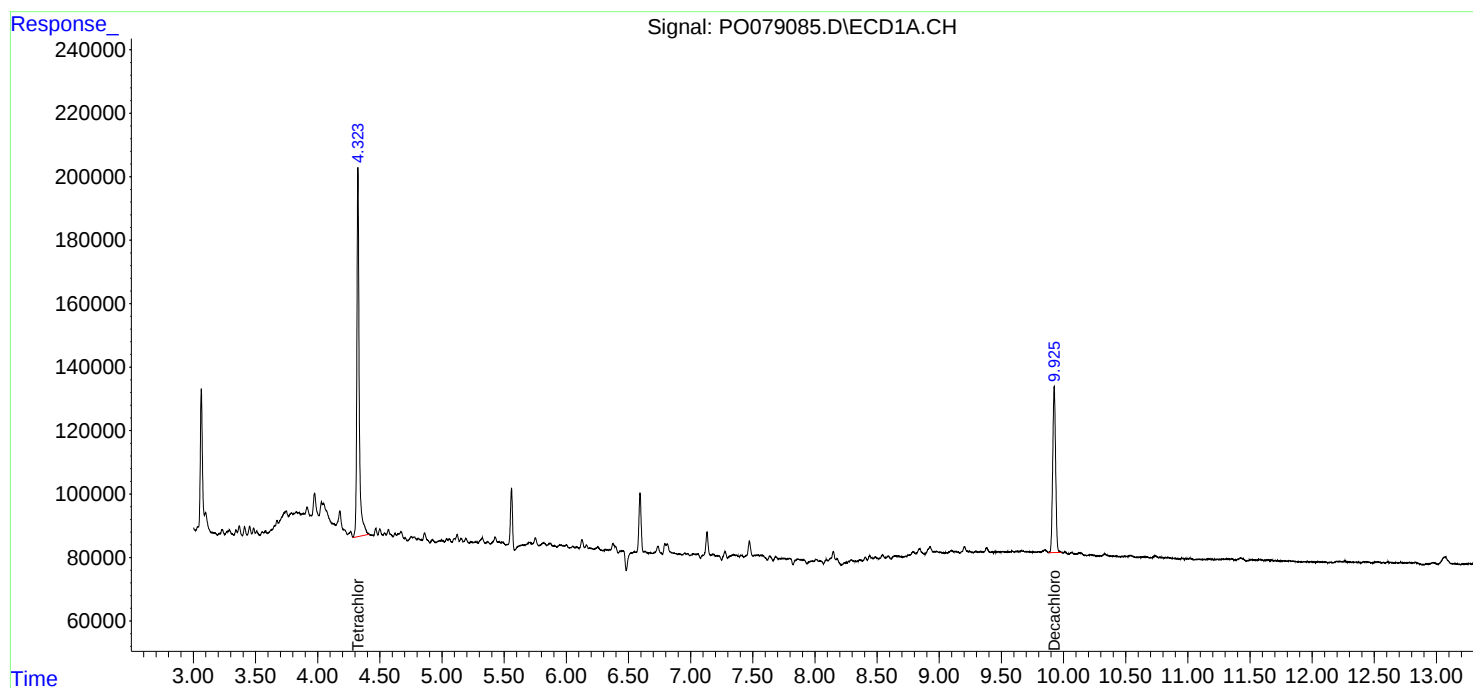

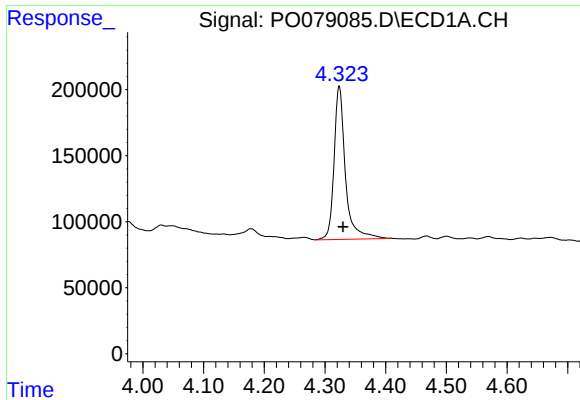


#1 Tetrachloro-m-xylene

R.T.: 4.323 min
Delta R.T.: -0.007 min
Response: 1510961
Conc: 19.14 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KG-WATER


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:43 PM

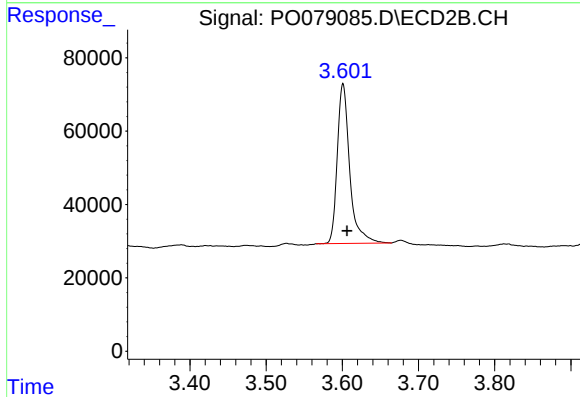


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.005 min
Response: 493411
Conc: 16.60 ng/ml

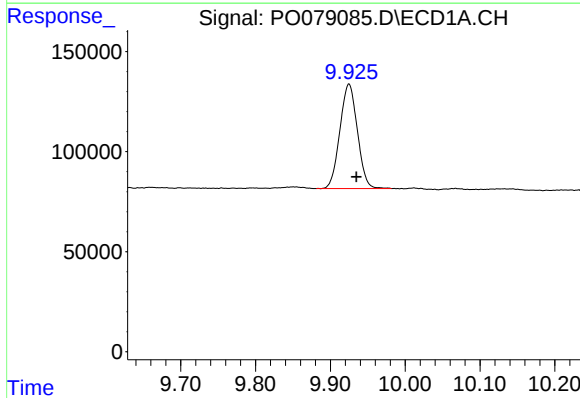

#2 Decachlorobiphenyl

R.T.: 9.925 min
Delta R.T.: -0.010 min
Response: 848512
Conc: 13.59 ng/ml

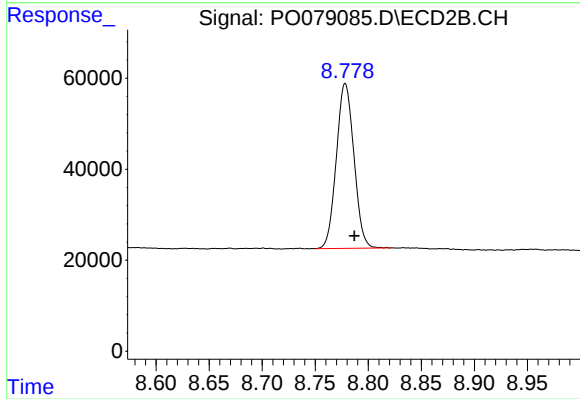

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.009 min
Response: 418487
Conc: 14.04 ng/ml