

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079088.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 22:28
 Operator : DD\AJ
 Sample : M2802-03
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41175

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:22:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:52:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.601	1129702	496206	14.314m	16.696m
2) SA Decachlor...	9.924	8.778	780188	404514	12.492	13.575

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079088.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 22:28
Operator : DD\AJ
Sample : M2802-03
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
41175


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:52:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

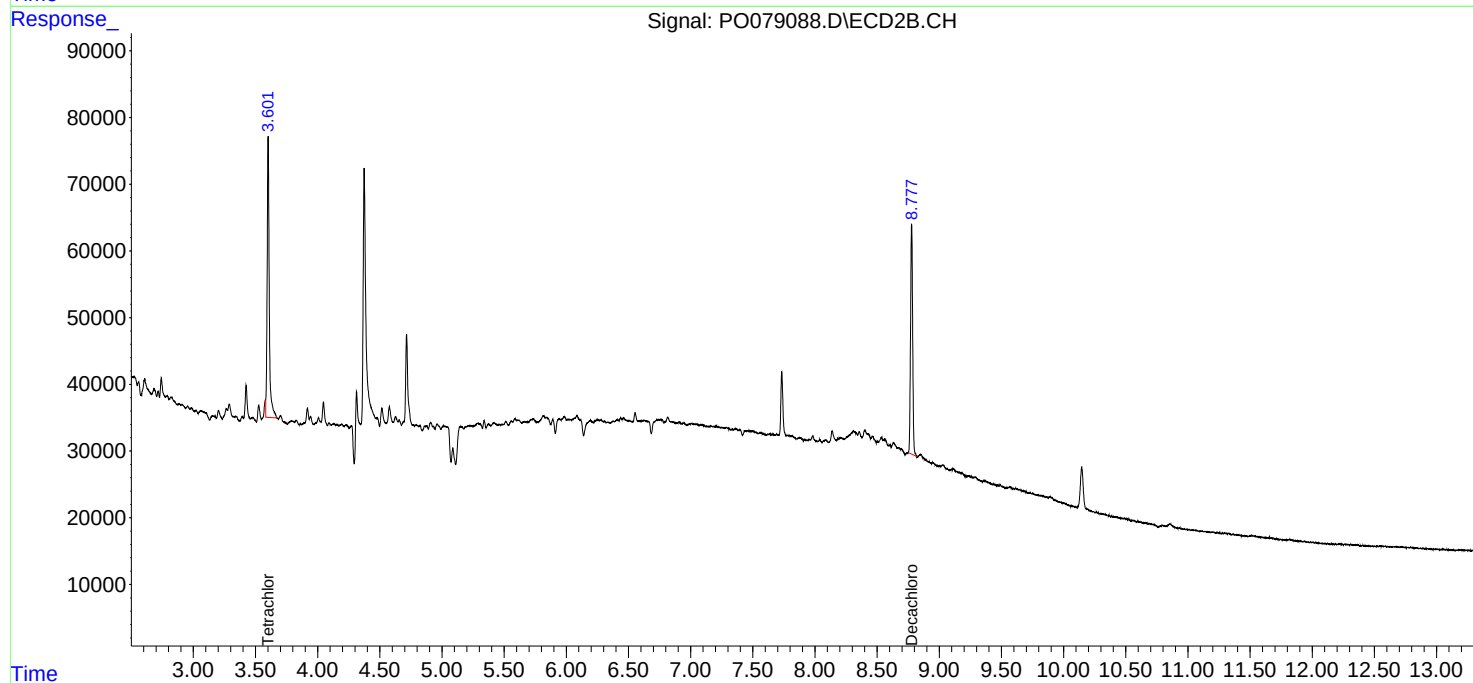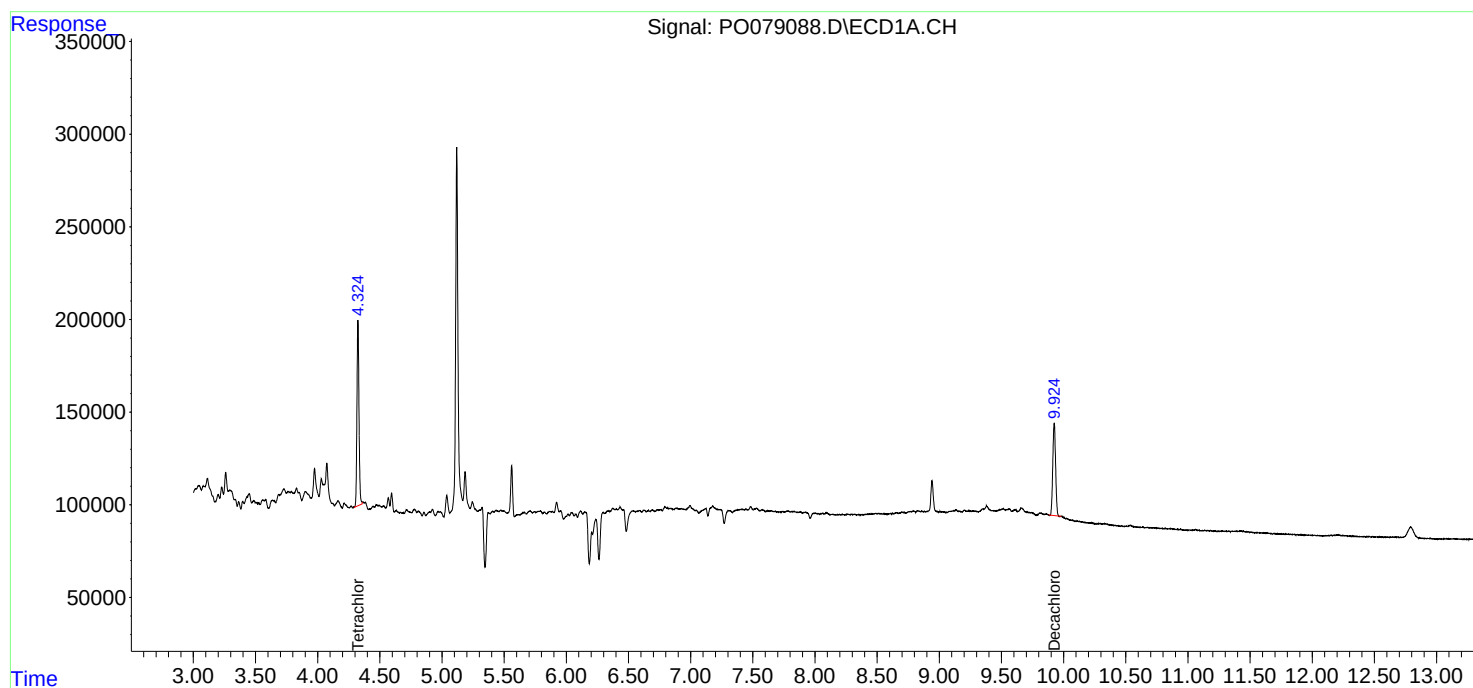

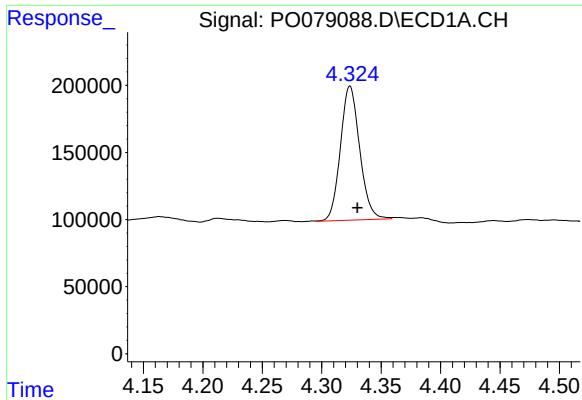


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.006 min
Response: 1129702
Conc: 14.31 ng/ml m

Instrument :
ECD_O
ClientSampleId :
41175


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:51 PM

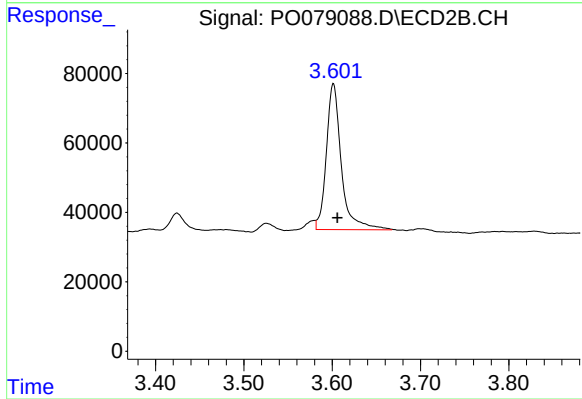


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.005 min
Response: 496206
Conc: 16.70 ng/ml m

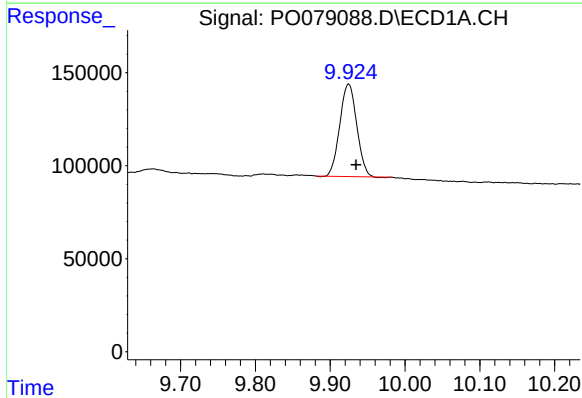

#2 Decachlorobiphenyl

R.T.: 9.924 min
Delta R.T.: -0.010 min
Response: 780188
Conc: 12.49 ng/ml

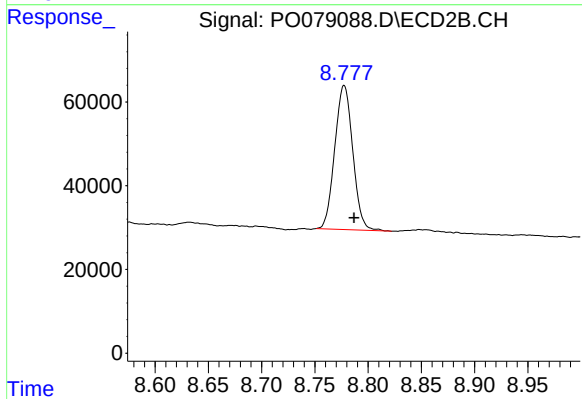

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.009 min
Response: 404514
Conc: 13.57 ng/ml