

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
 Data File : P0079092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jun 2021 23:54
 Operator : DD\AJ
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Ankita
 6/24/2021 1:22:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 00:55:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Jun 20 03:02:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.601	4351601	1591934	55.138	53.563
2) SA Decachlor...	9.926	8.778	3080389	1439865	49.322	48.320
Target Compounds						
26) L6 AR-1254-1	6.512	5.681	1412534	851897	524.416	512.763
27) L6 AR-1254-2	6.739	5.839	2228040	759240	531.192	515.189
28) L6 AR-1254-3	7.115	6.251	2358024	1151215	529.466	517.582
29) L6 AR-1254-4	7.409	6.489	1642643	714252	533.851	525.307
30) L6 AR-1254-5	7.831	6.910	1744296	1027238	534.350m	515.899

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062321\
Data File : P0079092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jun 2021 23:54
Operator : DD\AJ
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 00:55:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061921.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Jun 20 03:02:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

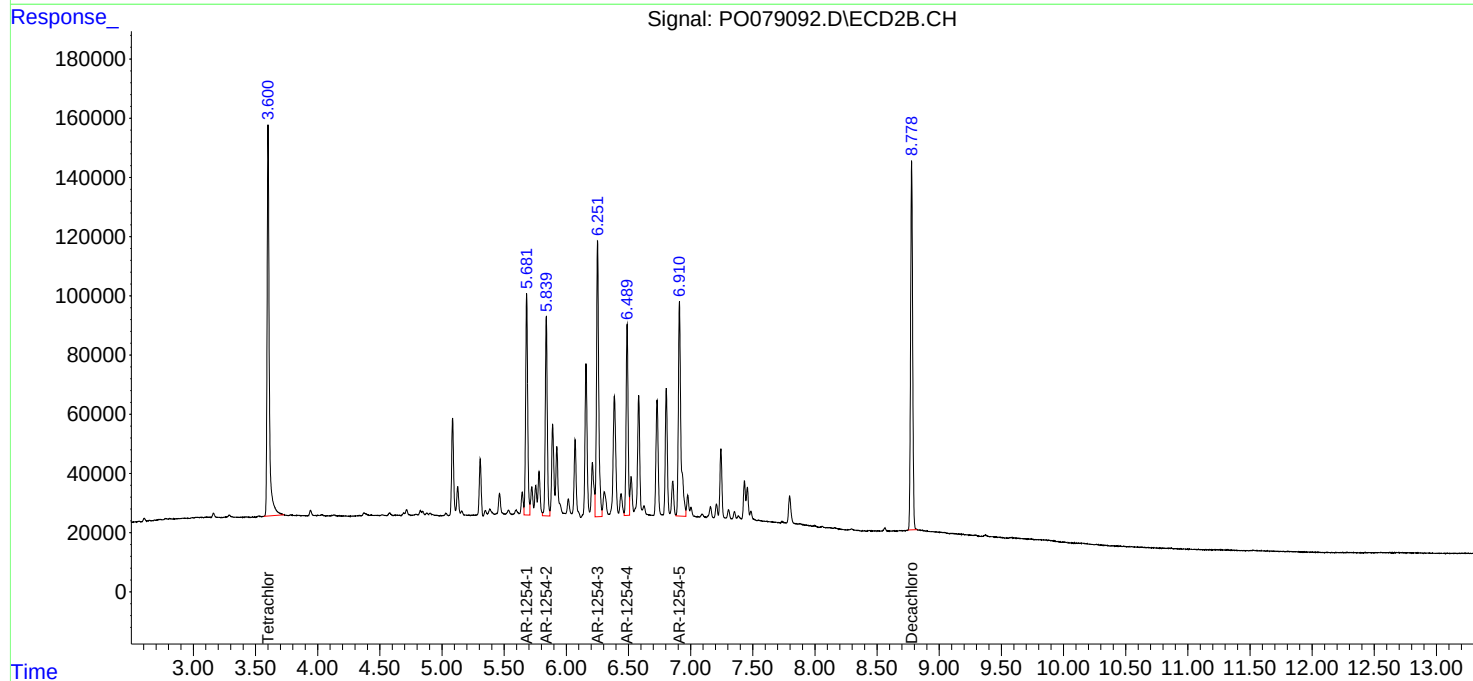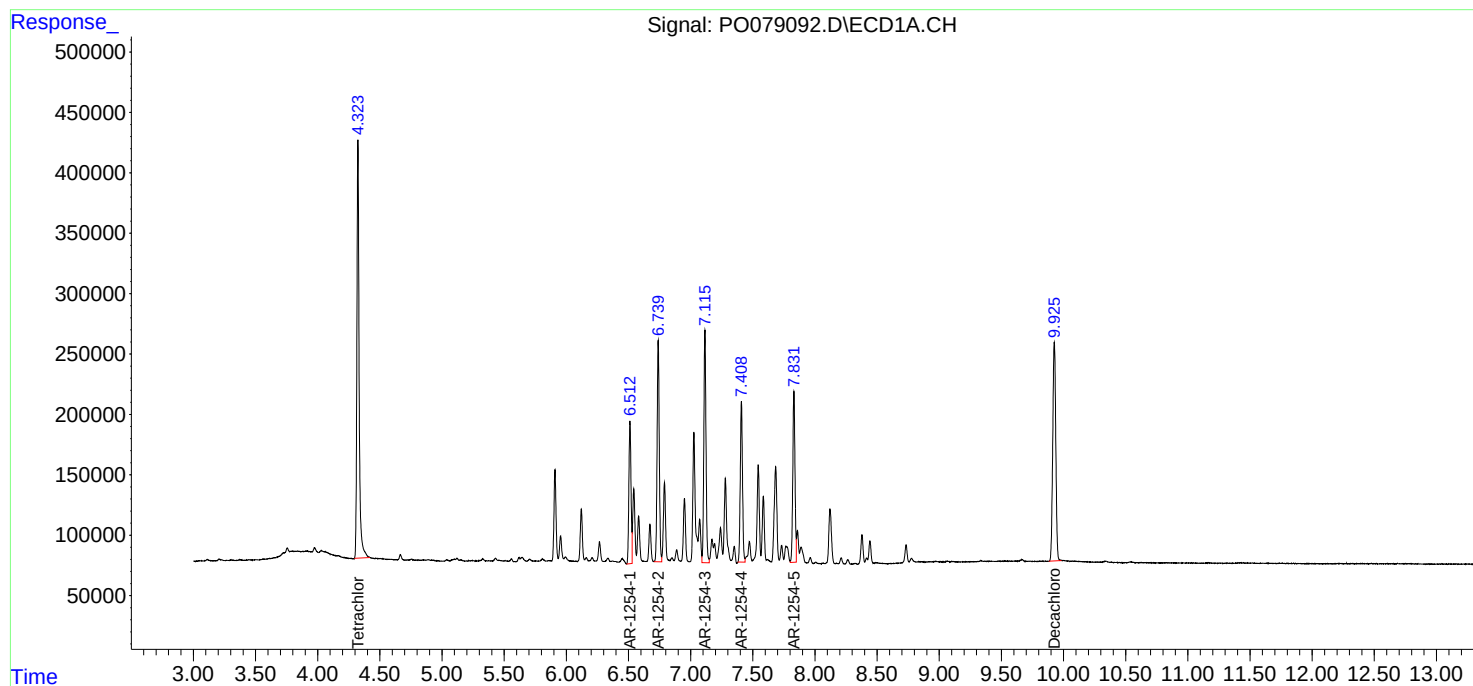

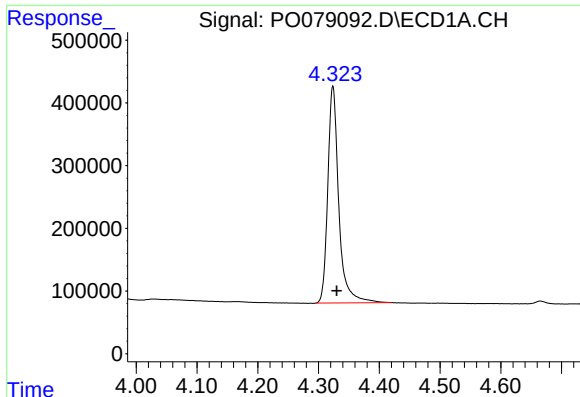


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: -0.006 min
Response: 4351601
Conc: 55.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:53 PM

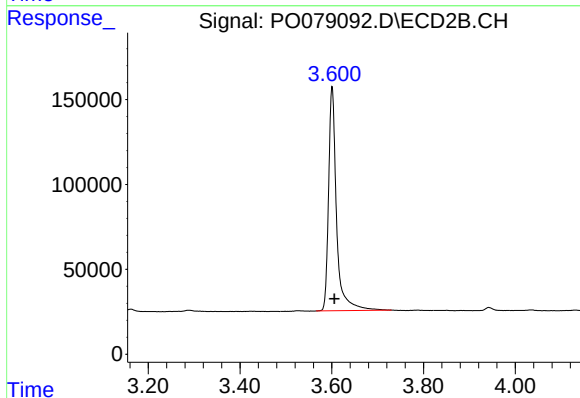


#1 Tetrachloro-m-xylene

R.T.: 3.601 min
Delta R.T.: -0.005 min
Response: 1591934
Conc: 53.56 ng/ml

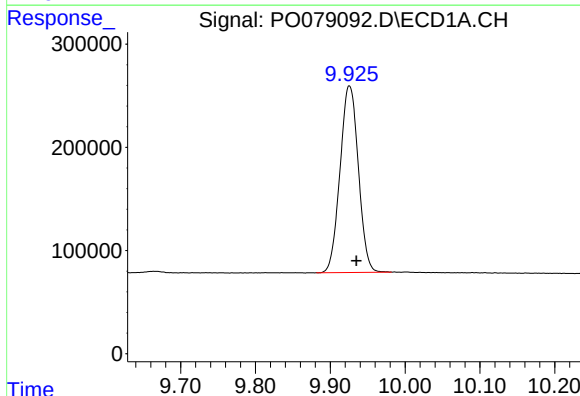


#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.009 min
Response: 3080389
Conc: 49.32 ng/ml

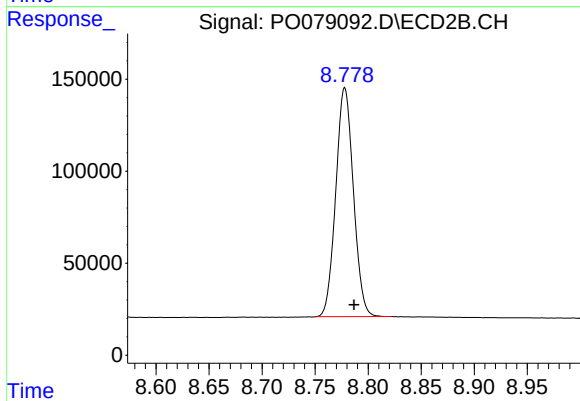

#2 Decachlorobiphenyl

R.T.: 8.778 min
Delta R.T.: -0.009 min
Response: 1439865
Conc: 48.32 ng/ml

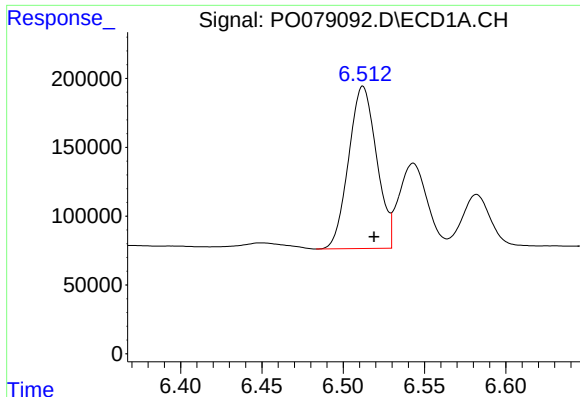


#26 AR-1254-1

R.T.: 6.512 min
Delta R.T.: -0.007 min
Response: 1412534
Conc: 524.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:53 PM

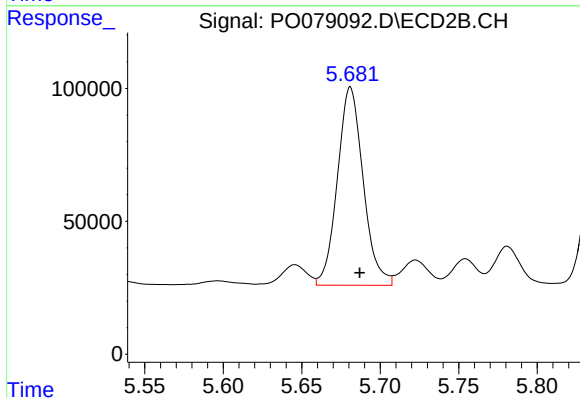


#26 AR-1254-1

R.T.: 5.681 min
Delta R.T.: -0.006 min
Response: 851897
Conc: 512.76 ng/ml

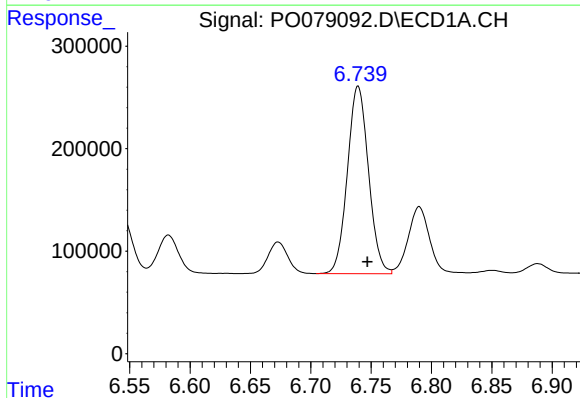


#27 AR-1254-2

R.T.: 6.739 min
Delta R.T.: -0.008 min
Response: 2228040
Conc: 531.19 ng/ml

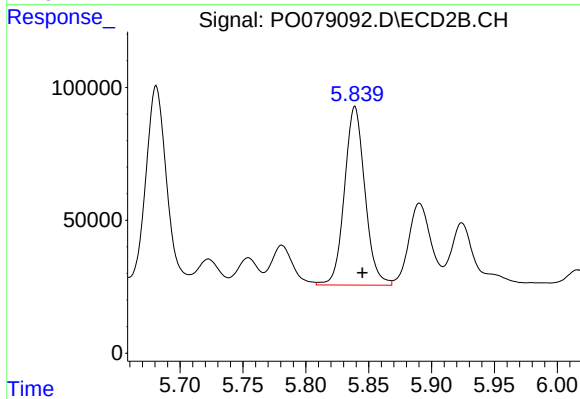

#27 AR-1254-2

R.T.: 5.839 min
Delta R.T.: -0.006 min
Response: 759240
Conc: 515.19 ng/ml

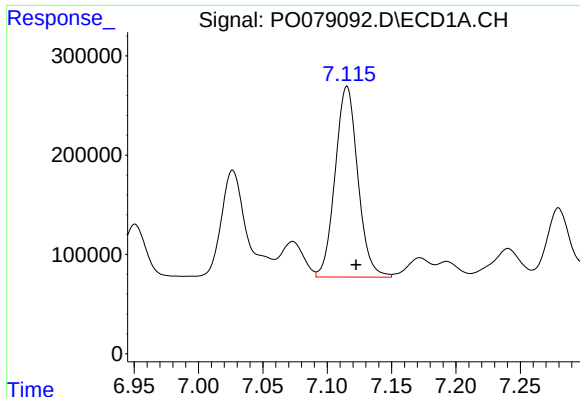


#28 AR-1254-3

R.T.: 7.115 min
Delta R.T.: -0.007 min
Response: 2358024
Conc: 529.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:53 PM

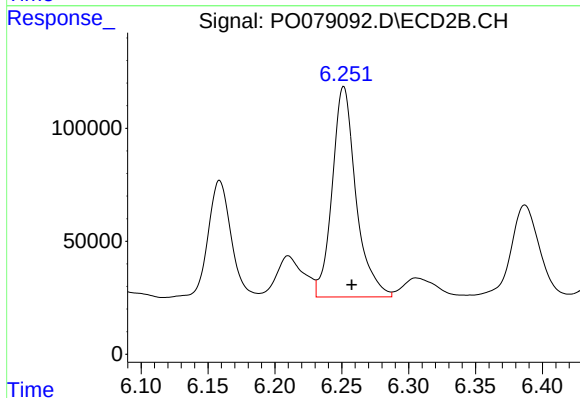


#28 AR-1254-3

R.T.: 6.251 min
Delta R.T.: -0.006 min
Response: 1151215
Conc: 517.58 ng/ml

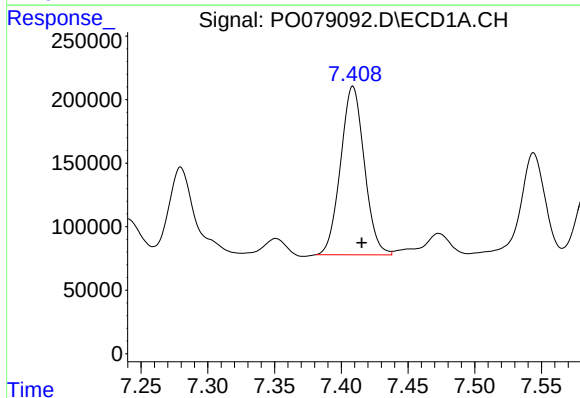


#29 AR-1254-4

R.T.: 7.409 min
Delta R.T.: -0.007 min
Response: 1642643
Conc: 533.85 ng/ml

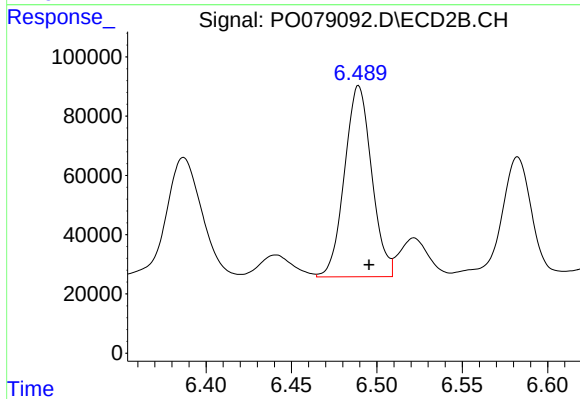

#29 AR-1254-4

R.T.: 6.489 min
Delta R.T.: -0.006 min
Response: 714252
Conc: 525.31 ng/ml

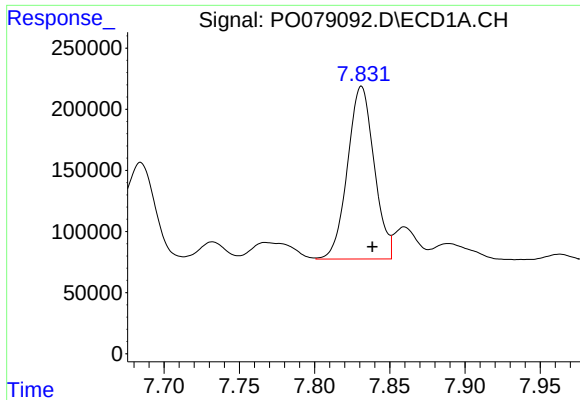


#30 AR-1254-5

R.T.: 7.831 min
Delta R.T.: -0.008 min
Response: 1744296
Conc: 534.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Ankita
6/24/2021 1:22:53 PM

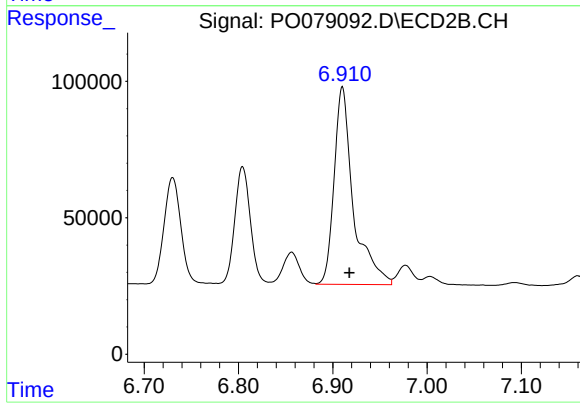

#30 AR-1254-5

R.T.: 6.910 min
Delta R.T.: -0.008 min
Response: 1027238
Conc: 515.90 ng/ml