

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062322\
 Data File : P0087323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 14:27
 Operator : YP/AJ
 Sample : N3438-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FRAC-TANK-N47935

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 15:18:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.492	3.639	37446666	19804408	16.023	17.589
2) SA Decachlor...	10.347	8.640	22890254	9731214	12.438	12.377

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062322\
Data File : PO087323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 14:27
Operator : YP/AJ
Sample : N3438-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FRAC-TANK-N47935

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 15:18:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

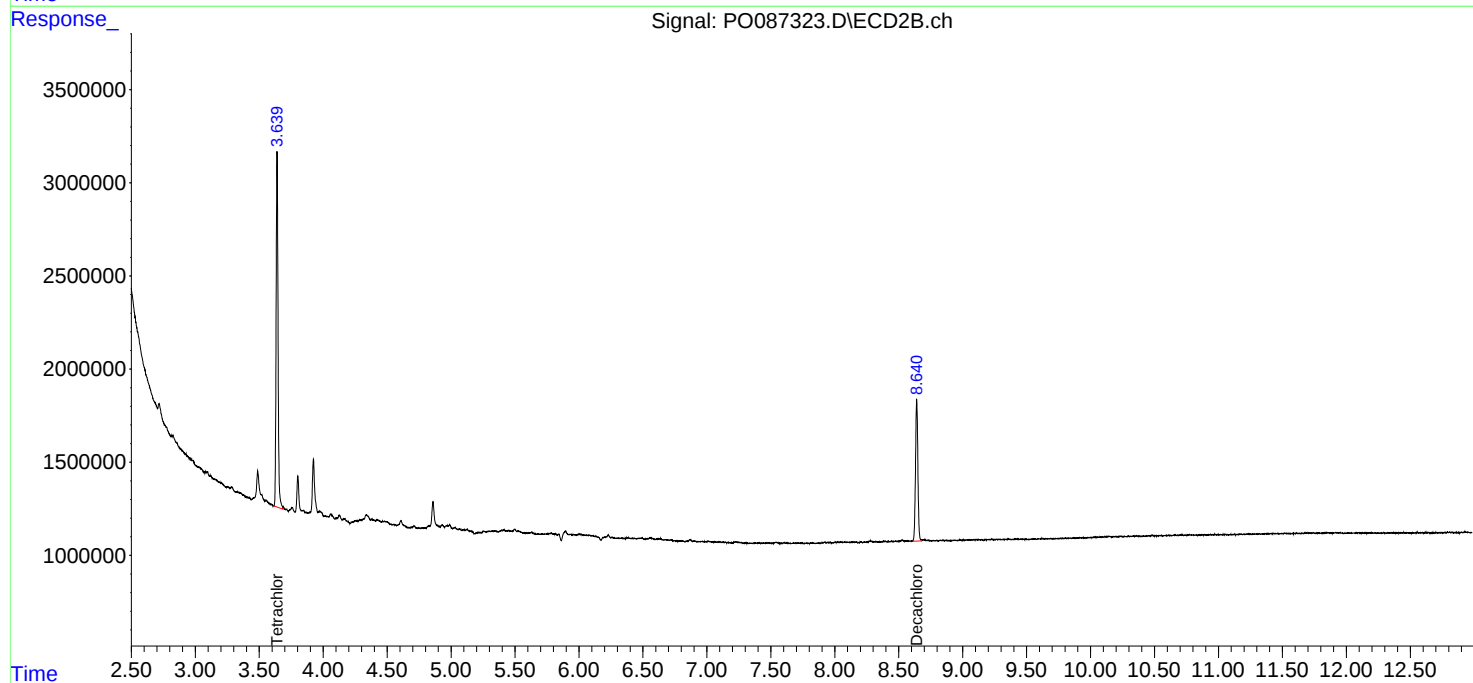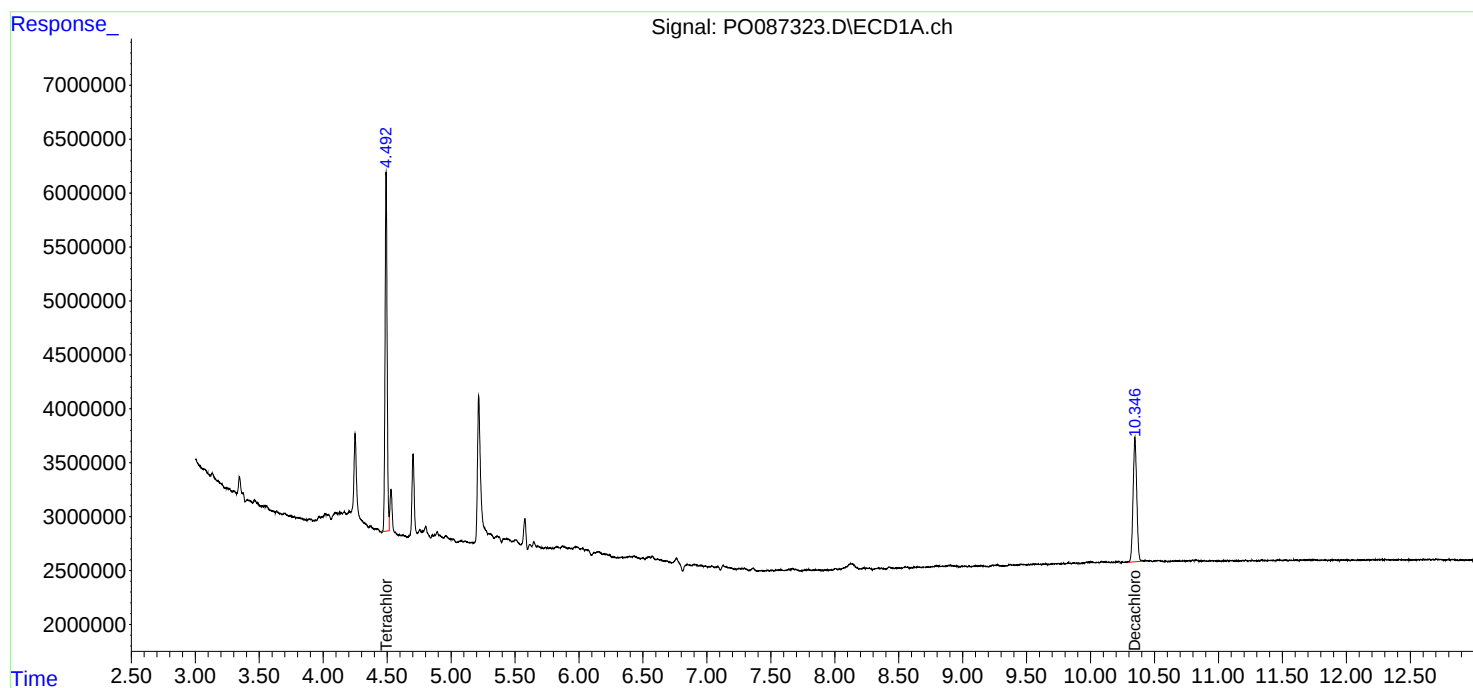


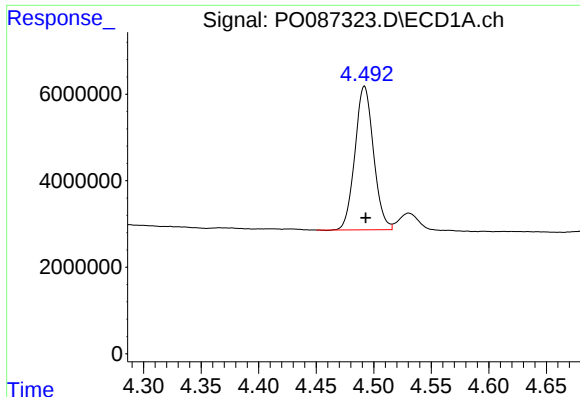

#1 Tetrachloro-m-xylene


R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 37446666
Conc: 16.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
FRAC-TANK-N47935

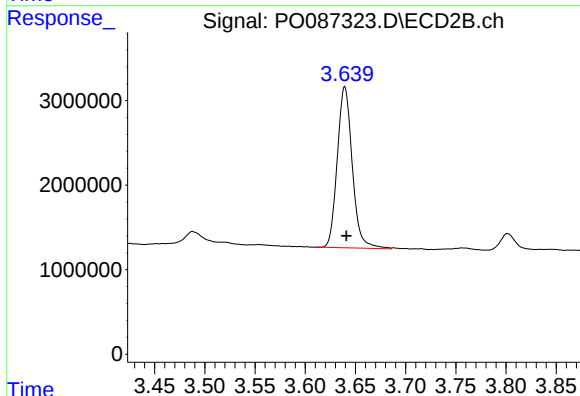


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.002 min
Response: 19804408
Conc: 17.59 ng/ml

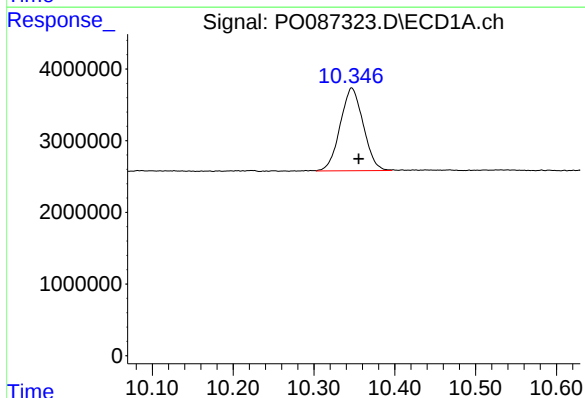

#2 Decachlorobiphenyl

R.T.: 10.347 min
Delta R.T.: -0.009 min
Response: 22890254
Conc: 12.44 ng/ml

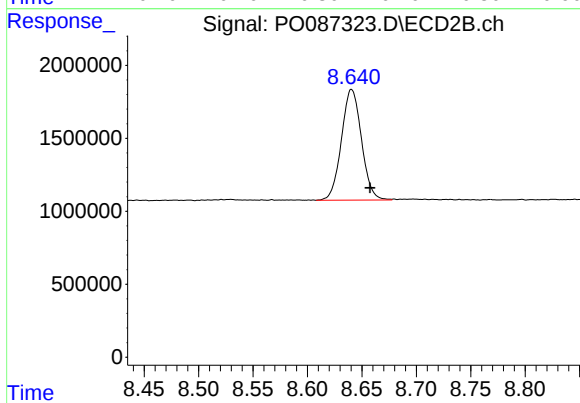

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.017 min
Response: 9731214
Conc: 12.38 ng/ml