

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062322\
 Data File : P0087324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 14:43
 Operator : YP/AJ
 Sample : N3447-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D2342

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/24/2022
 Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 15:18:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.498	3.650	25747606	15202344	11.017m	13.502m
2) SA Decachlor...	10.354	8.650	34358565	10332789	18.670	13.142 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062322\
Data File : PO087324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 14:43
Operator : YP/AJ
Sample : N3447-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
D2342


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 15:18:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

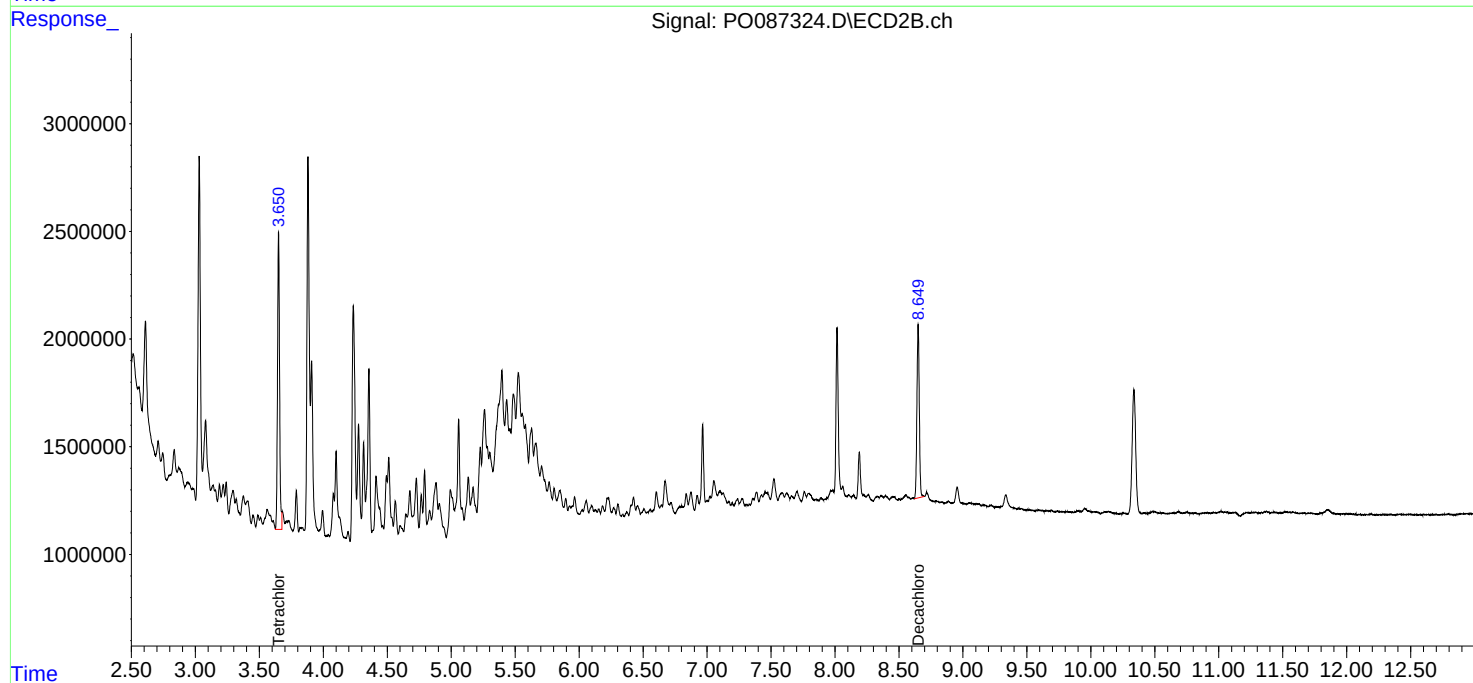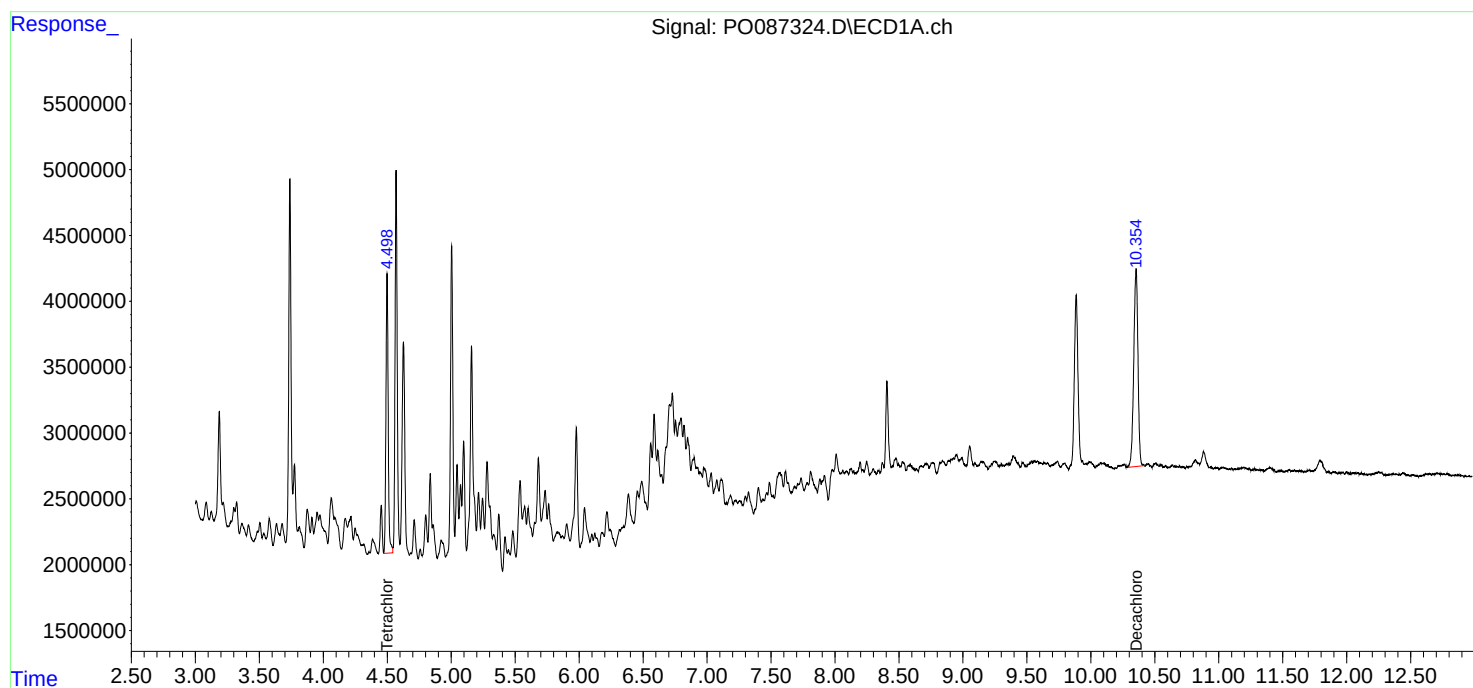

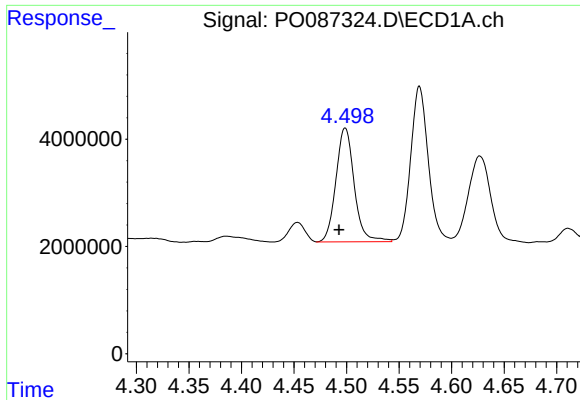


#1 Tetrachloro-m-xylene

R.T.: 4.498 min
Delta R.T.: 0.005 min
Response: 25747606
Conc: 11.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
D2342


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

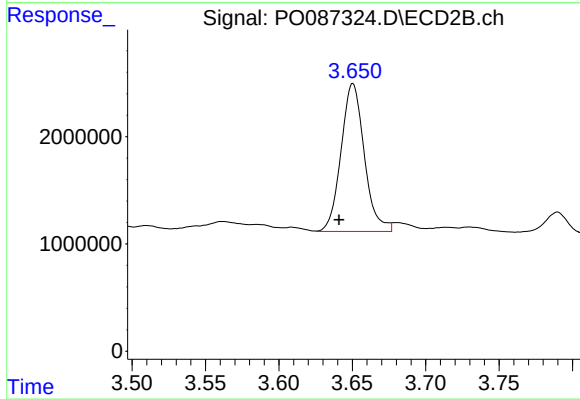


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.009 min
Response: 15202344
Conc: 13.50 ng/ml m

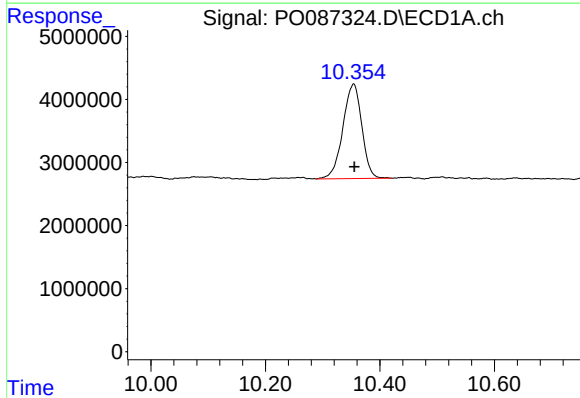

#2 Decachlorobiphenyl

R.T.: 10.354 min
Delta R.T.: -0.002 min
Response: 34358565
Conc: 18.67 ng/ml

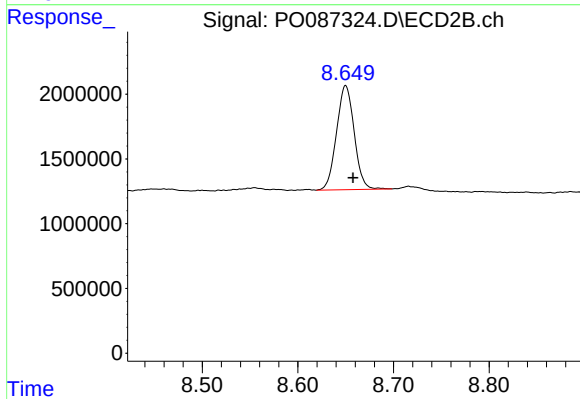

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.008 min
Response: 10332789
Conc: 13.14 ng/ml