

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062322\
 Data File : P0087340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 19:19
 Operator : YP/AJ
 Sample : N3462-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-6-0-2-20220622

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/24/2022
 Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 02:57:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.638	36985597	20393094	15.826m	18.112
2) SA Decachlor...	10.351	8.642	58217559	24372677	31.634	30.999

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062322\
Data File : PO087340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 19:19
Operator : YP/AJ
Sample : N3462-04
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-6-0-2-20220622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 02:57:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

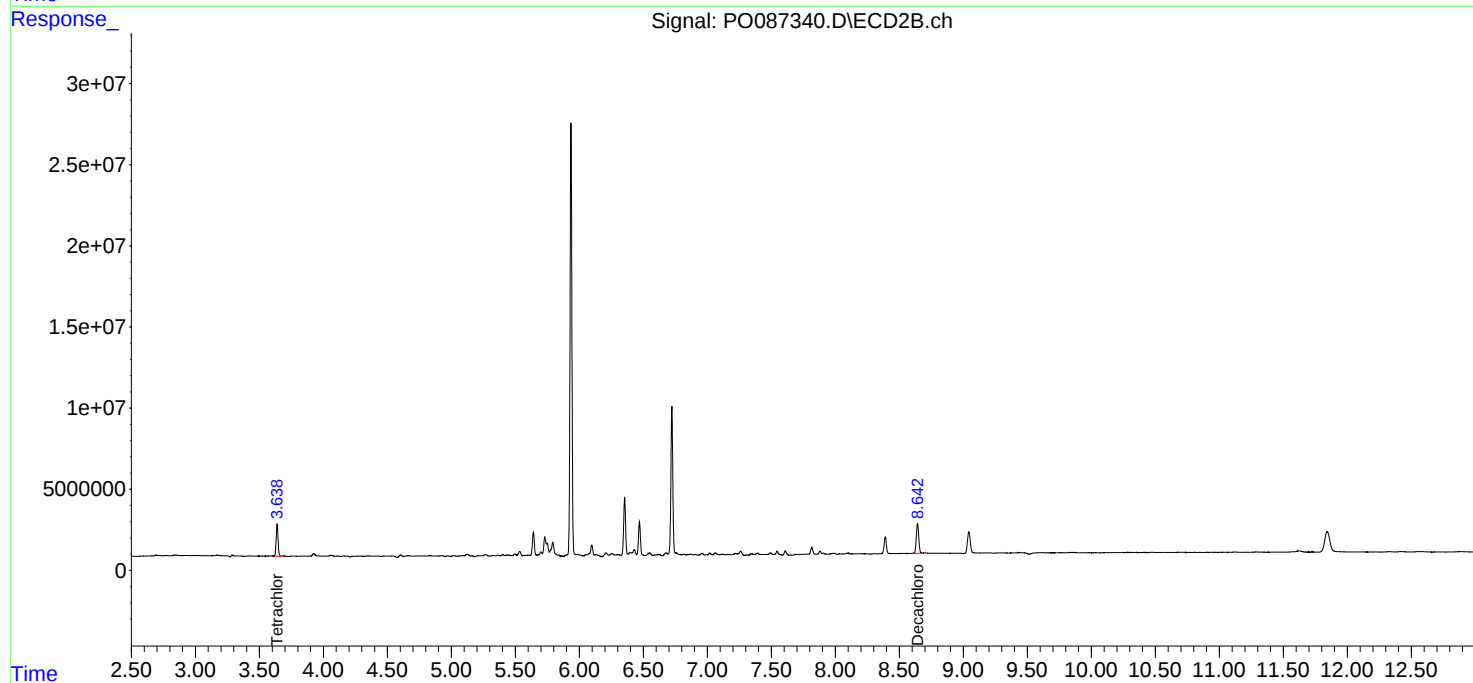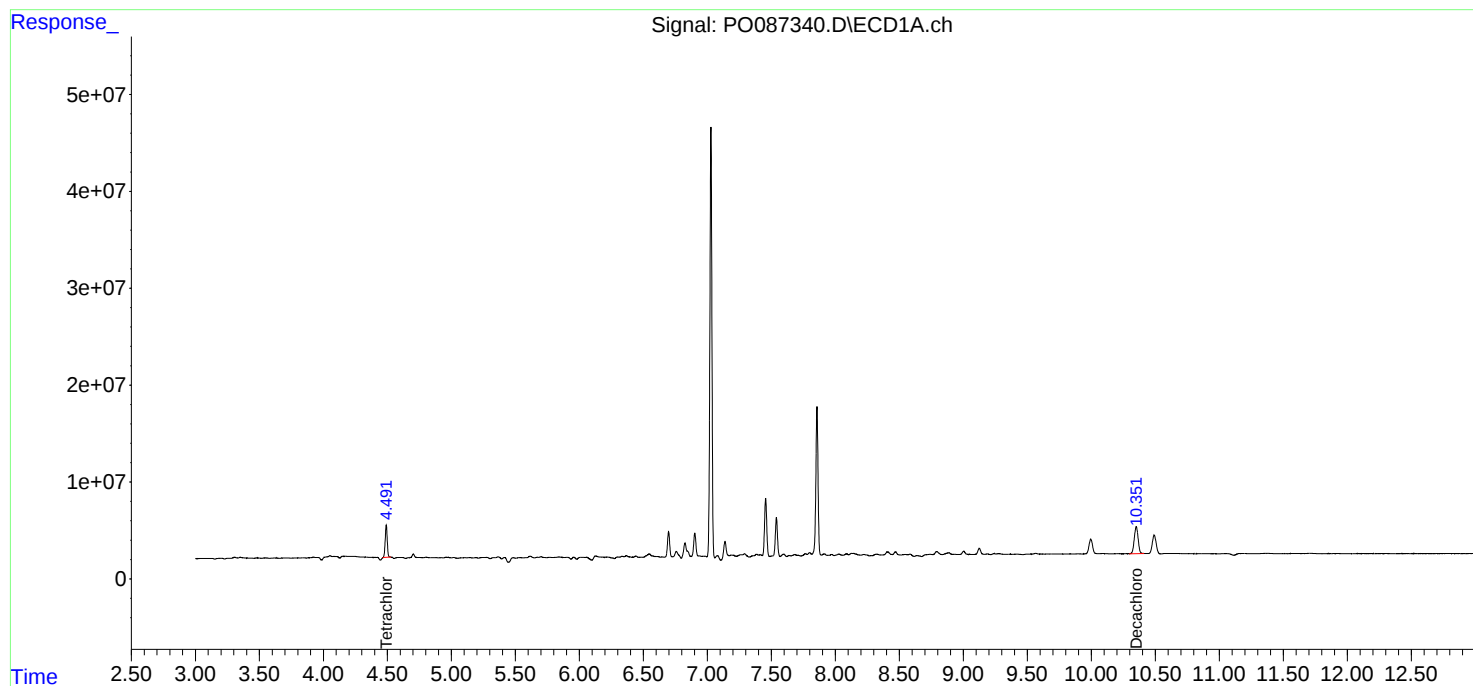

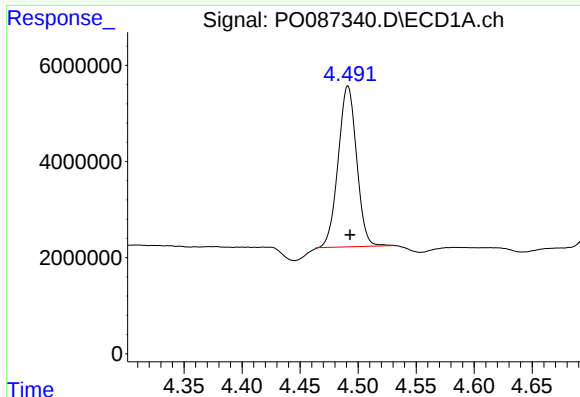


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: -0.002 min
Response: 36985597
Conc: 15.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-6-0-2-20220622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

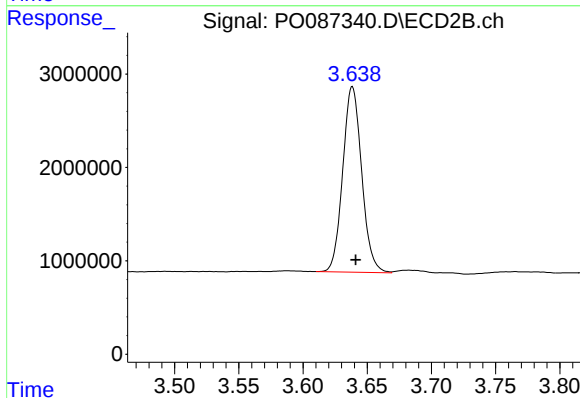


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 20393094
Conc: 18.11 ng/ml

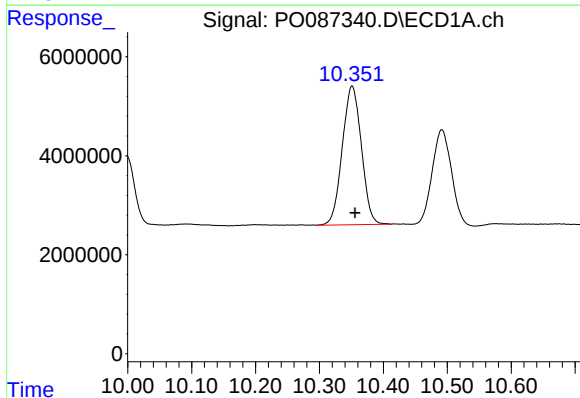

#2 Decachlorobiphenyl

R.T.: 10.351 min
Delta R.T.: -0.005 min
Response: 58217559
Conc: 31.63 ng/ml

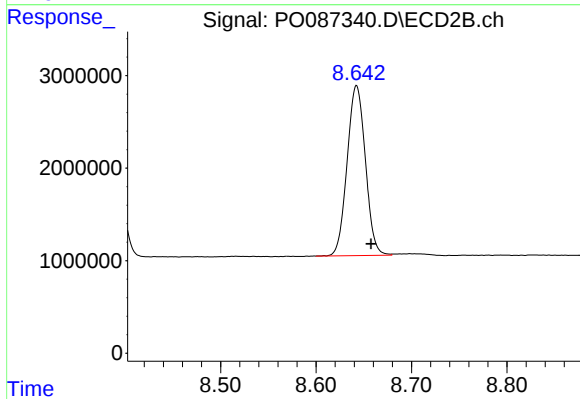

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.015 min
Response: 24372677
Conc: 31.00 ng/ml