

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062322\
 Data File : P0087346.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 20:57
 Operator : YP/AJ
 Sample : N3468-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 XRDS-SCREENFILL-CLEAN-FILL-SP-A-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/24/2022
 Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 03:00:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.496	3.641	53755260	23695994	23.002	21.046
2)	SA Decachlor...	10.360	8.648	44986547	18559886	24.445	23.606
Target Compounds							
26)	L6 AR-1254-1	6.544	5.535	24933241	12312147	285.976m	254.394
27)	L6 AR-1254-2	6.765	5.679	28038681	6150751	214.701	144.209 #
28)	L6 AR-1254-3	7.138	6.082	43909176	10711002	336.543	156.727 #
29)	L6 AR-1254-4	7.419	6.310	12109375	6691529	126.741m	158.612 #
30)	L6 AR-1254-5	7.848	6.727	21206223	29808807	202.977m	490.843 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062322\
Data File : PO087346.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 20:57
Operator : YP/AJ
Sample : N3468-01
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
XRDS-SCREENFILL-CLEAN-FILL-SP-A-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 03:00:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

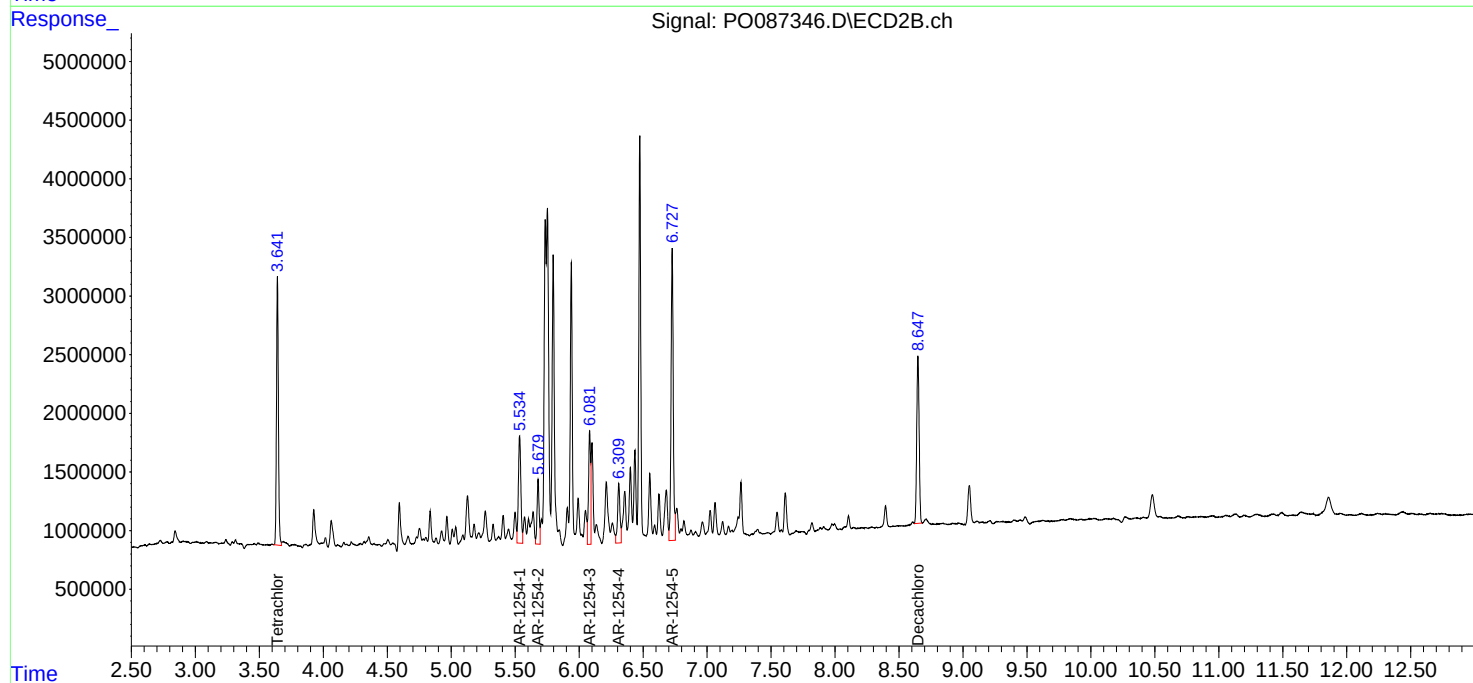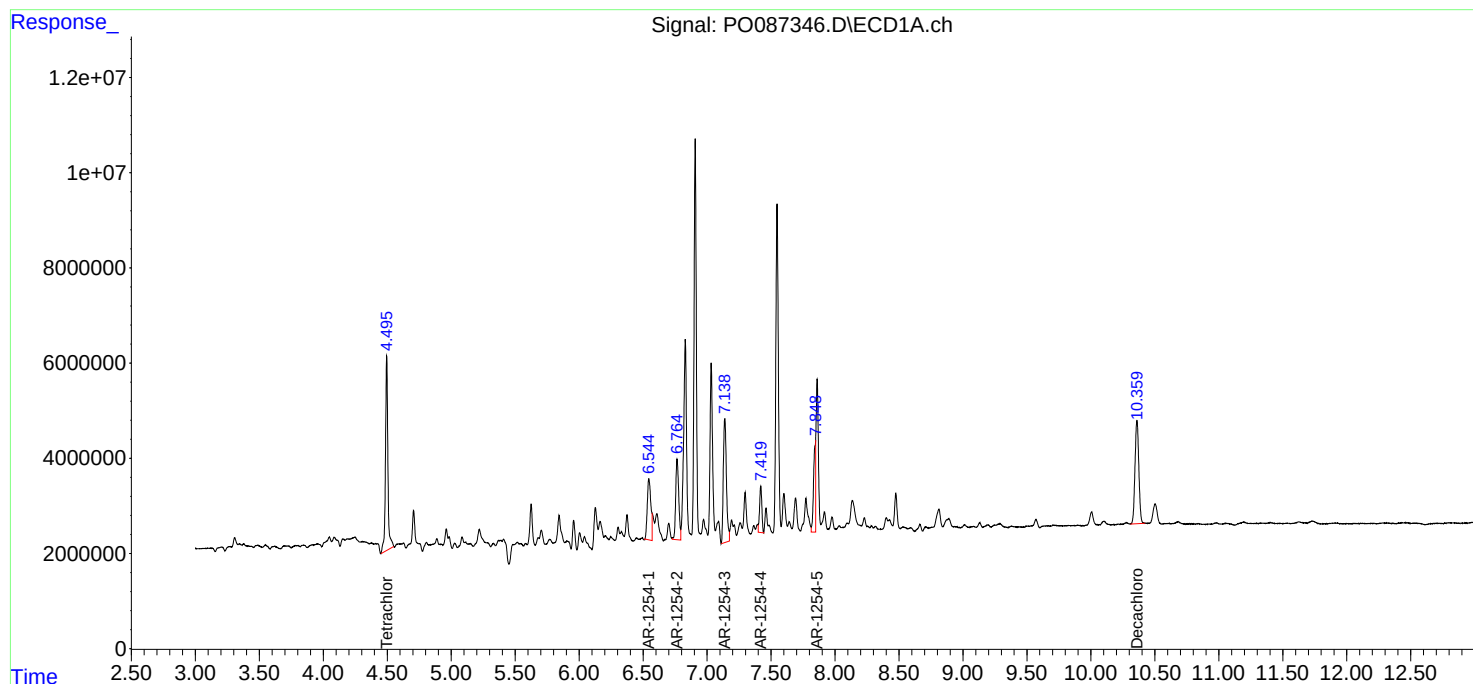

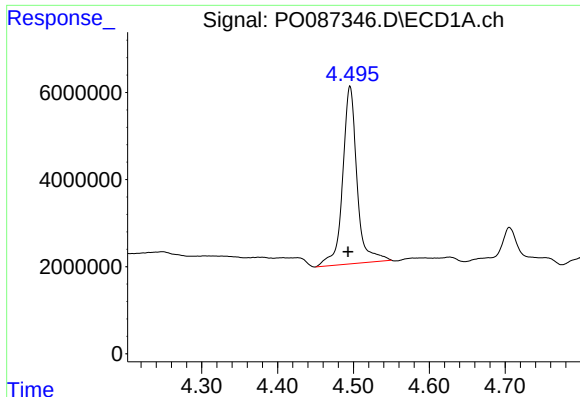


#1 Tetrachloro-m-xylene

R.T.: 4.496 min
Delta R.T.: 0.003 min
Response: 53755260
Conc: 23.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
XRDS-SCREENFILL-CLEAN-FILL-SP-A-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

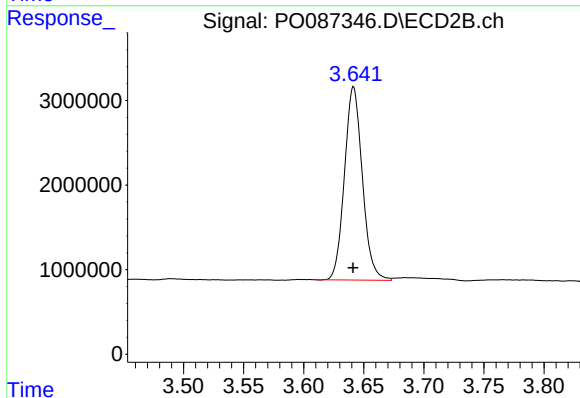


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: 0.000 min
Response: 23695994
Conc: 21.05 ng/ml

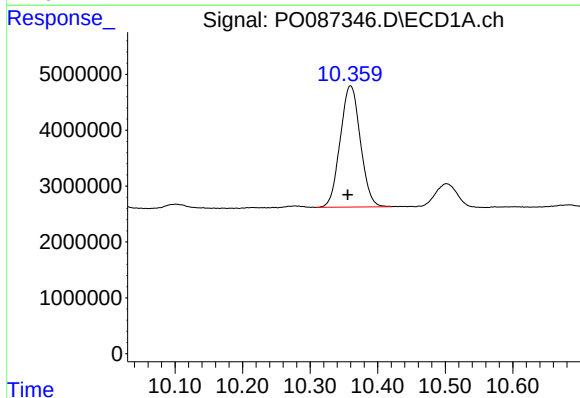


#2 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: 0.004 min
Response: 44986547
Conc: 24.44 ng/ml

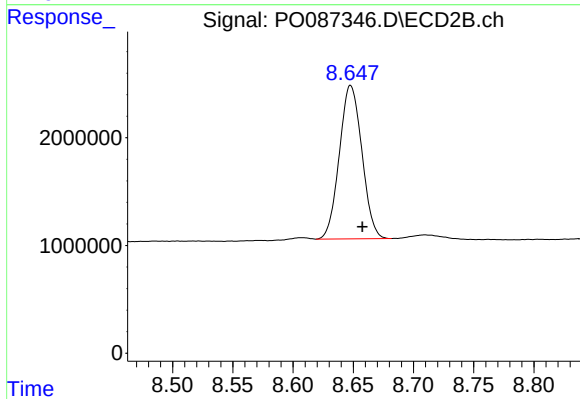

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.010 min
Response: 18559886
Conc: 23.61 ng/ml

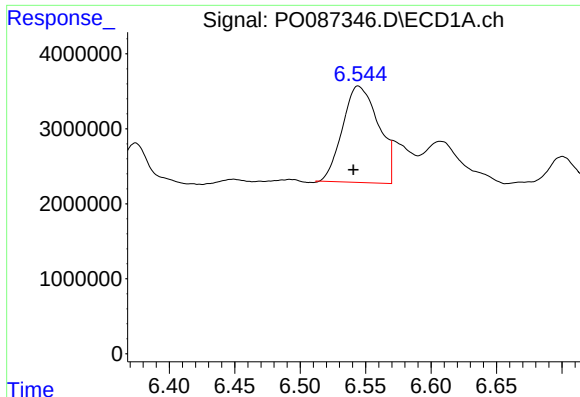


#26 AR-1254-1

R.T.: 6.544 min
Delta R.T.: 0.003 min
Response: 24933241
Conc: 285.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
XRDS-SCREENFILL-CLEAN-FILL-SP-A-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

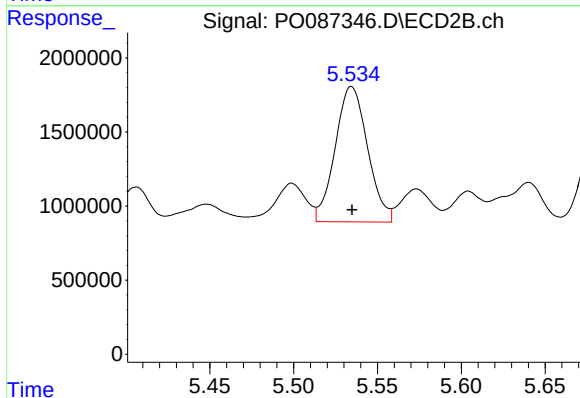


#26 AR-1254-1

R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 12312147
Conc: 254.39 ng/ml

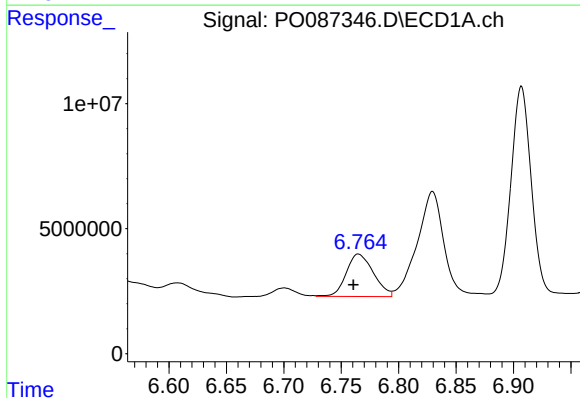


#27 AR-1254-2

R.T.: 6.765 min
Delta R.T.: 0.004 min
Response: 28038681
Conc: 214.70 ng/ml

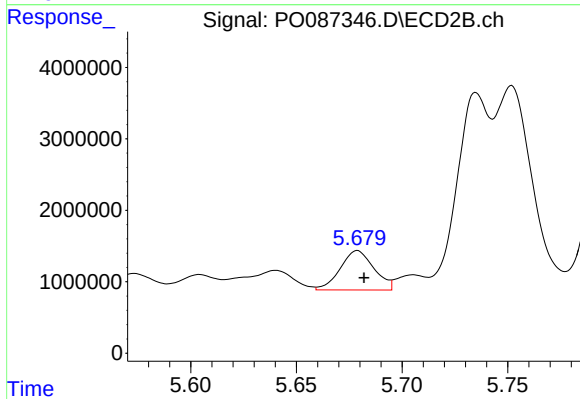

#27 AR-1254-2

R.T.: 5.679 min
Delta R.T.: -0.003 min
Response: 6150751
Conc: 144.21 ng/ml

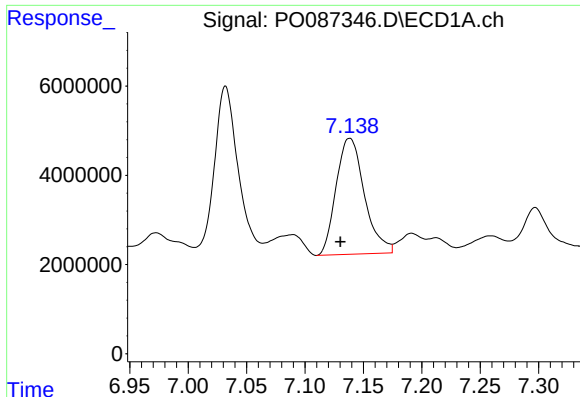

#28 AR-1254-3

R.T.: 7.138 min
Delta R.T.: 0.008 min
Response: 43909176
Conc: 336.54 ng/ml

Instrument :

ECD_O


ClientSampleId :

XRDS-SCREENFILL-CLEAN-FILL-SP-A-COMP

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

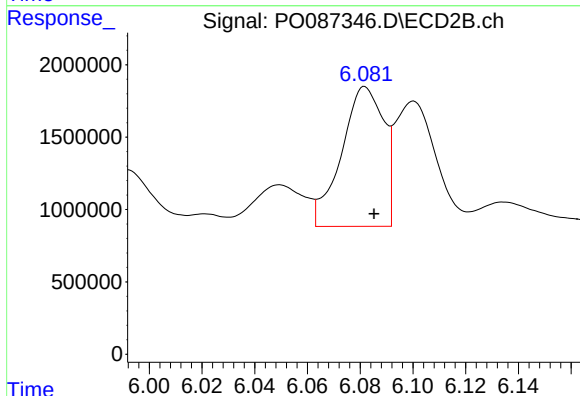


#28 AR-1254-3

R.T.: 6.082 min
Delta R.T.: -0.003 min
Response: 10711002
Conc: 156.73 ng/ml

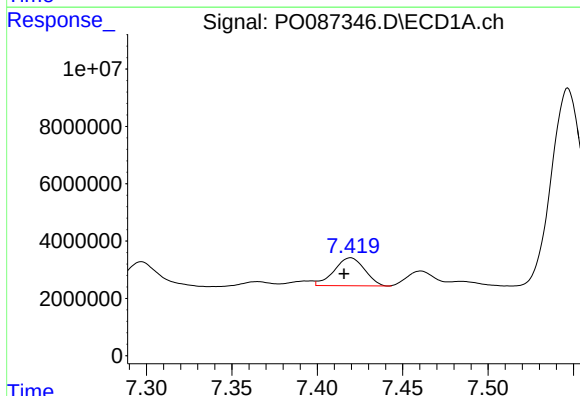


#29 AR-1254-4

R.T.: 7.419 min
Delta R.T.: 0.004 min
Response: 12109375
Conc: 126.74 ng/ml m

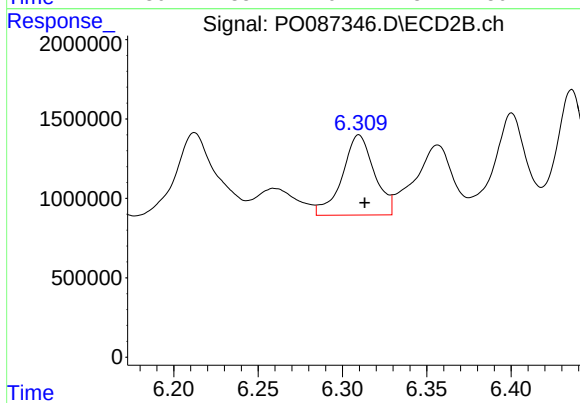

#29 AR-1254-4

R.T.: 6.310 min
Delta R.T.: -0.003 min
Response: 6691529
Conc: 158.61 ng/ml

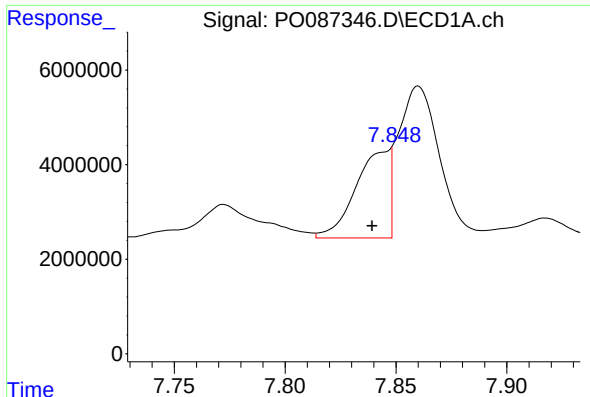

#30 AR-1254-5

R.T.: 7.848 min
Delta R.T.: 0.009 min
Response: 21206223
Conc: 202.98 ng/ml

Instrument :

ECD_O


ClientSampleId :

XRDS-SCREENFILL-CLEAN-FILL-SP-A-COMP

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/24/2022
Supervised By :Ankita Jodhani 06/24/2022

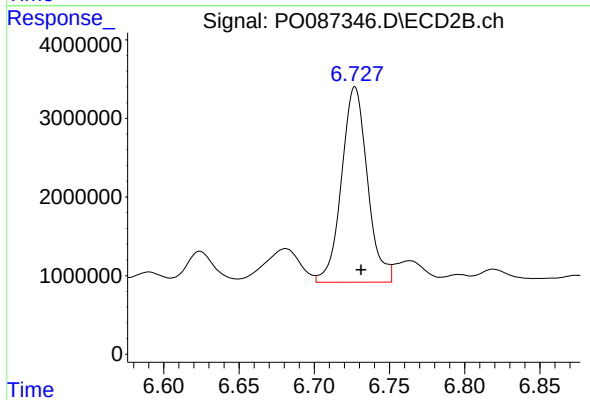

#30 AR-1254-5

R.T.: 6.727 min
Delta R.T.: -0.004 min
Response: 29808807
Conc: 490.84 ng/ml