

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062322\
 Data File : P0087347.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2022 21:14
 Operator : YP/AJ
 Sample : N3469-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 XRDS-SCREENED-CLEAN-FILL-SP-1-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 03:00:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 10 04:33:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.495	3.642	44252670	22723647	18.936	20.182
2) SA Decachlor...	10.358	8.649	38151220	14947319	20.731	19.011

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062322\
Data File : PO087347.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2022 21:14
Operator : YP/AJ
Sample : N3469-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
XRDS-SCREENED-CLEAN-FILL-SP-1-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 03:00:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060922.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 10 04:33:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

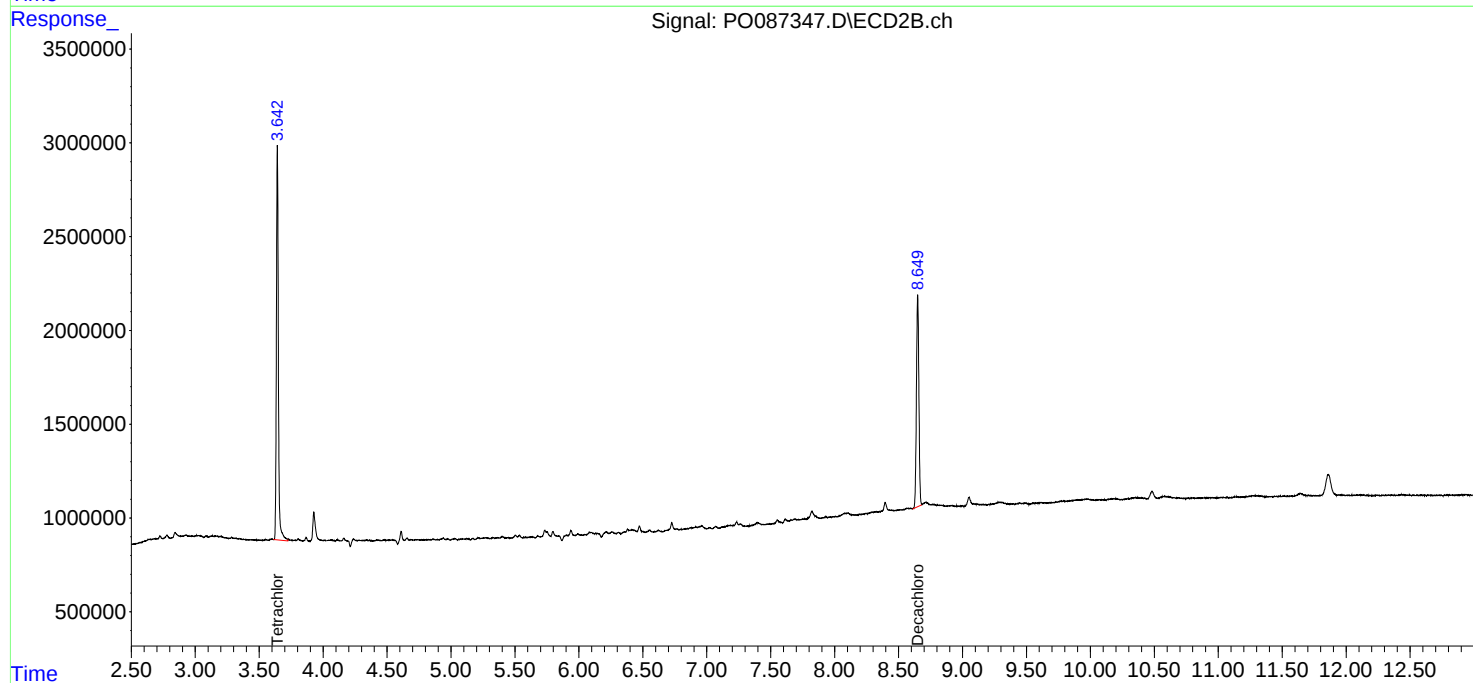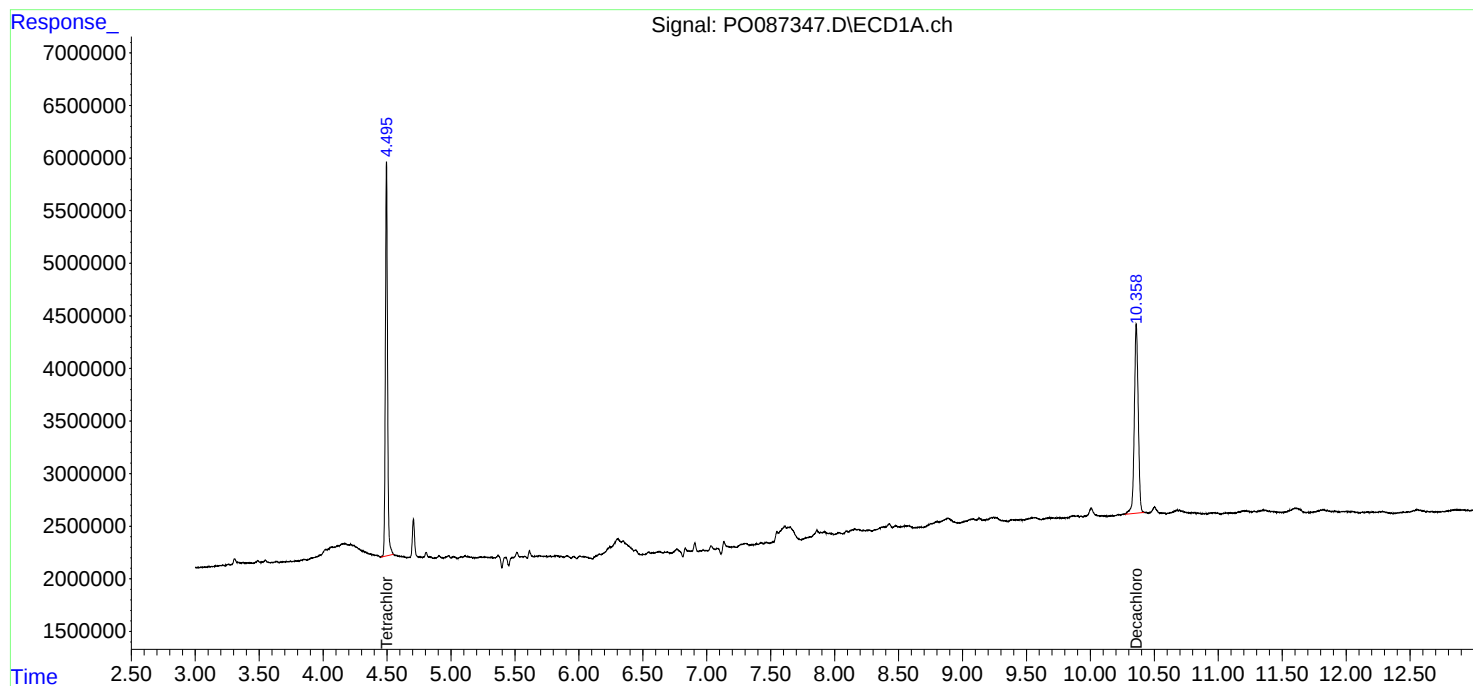

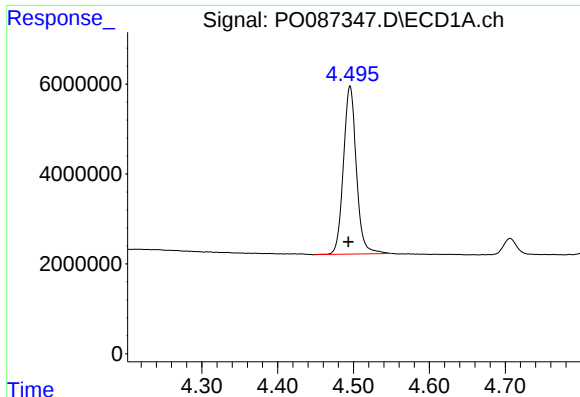

#1 Tetrachloro-m-xylene


R.T.: 4.495 min
Delta R.T.: 0.002 min
Response: 44252670
Conc: 18.94 ng/ml

Instrument :

ECD_O


ClientSampleId :

XRDS-SCREENED-CLEAN-FILL-SP-1-COMP

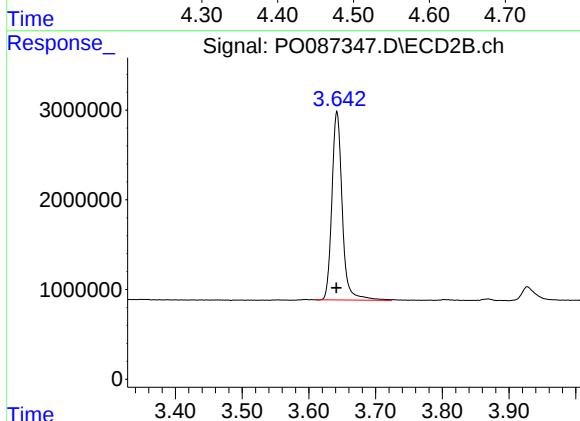


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: 0.001 min
Response: 22723647
Conc: 20.18 ng/ml

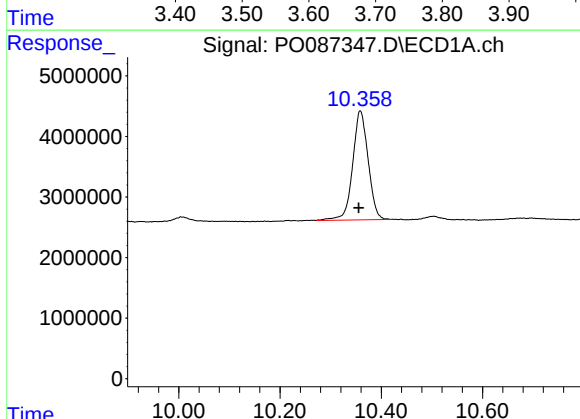

#2 Decachlorobiphenyl

R.T.: 10.358 min
Delta R.T.: 0.003 min
Response: 38151220
Conc: 20.73 ng/ml

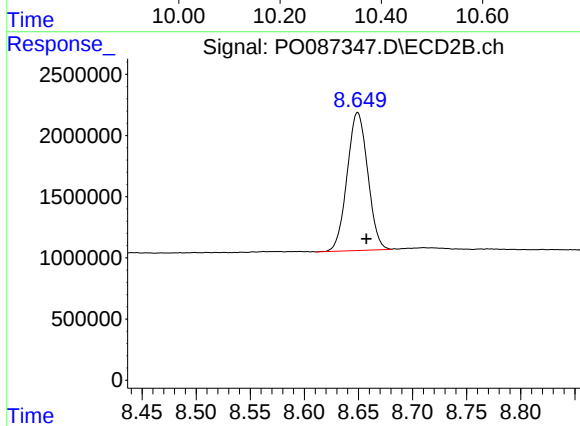

#2 Decachlorobiphenyl

R.T.: 8.649 min
Delta R.T.: -0.008 min
Response: 14947319
Conc: 19.01 ng/ml