

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062323\
 Data File : P0095914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 13:39
 Operator : YP/AJ
 Sample : 03345-03 (Sig #1); 03345-04 10X (Sig #2)
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2-0620

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 15:54:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.418	3.635	49442442	22584495	16.993	16.641
2) SA Decachlor...	10.239	8.672	20190396	11467697	9.746	9.352

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO062323\
Data File : PO095914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 13:39
Operator : YP/AJ
Sample : 03345-03 (Sig #1); 03345-04 10X (Sig #2)
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-2-0620

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 15:54:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

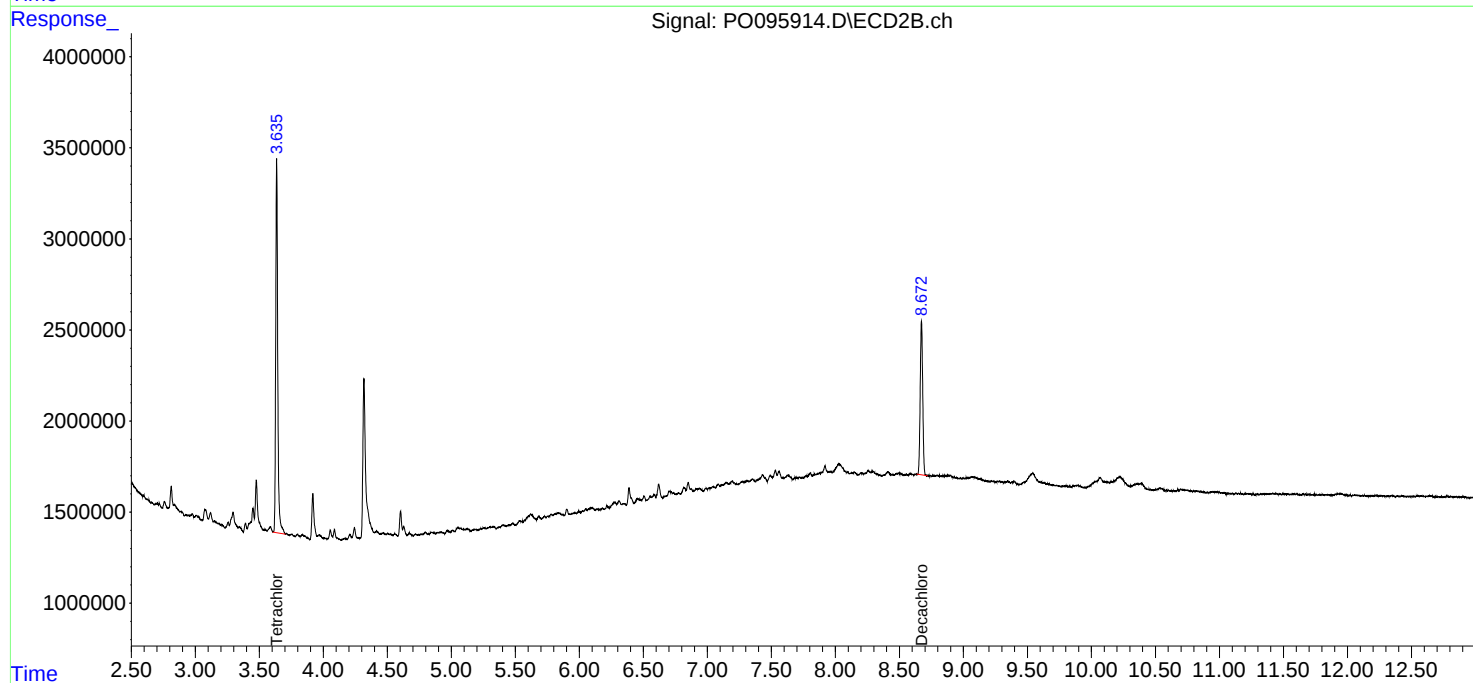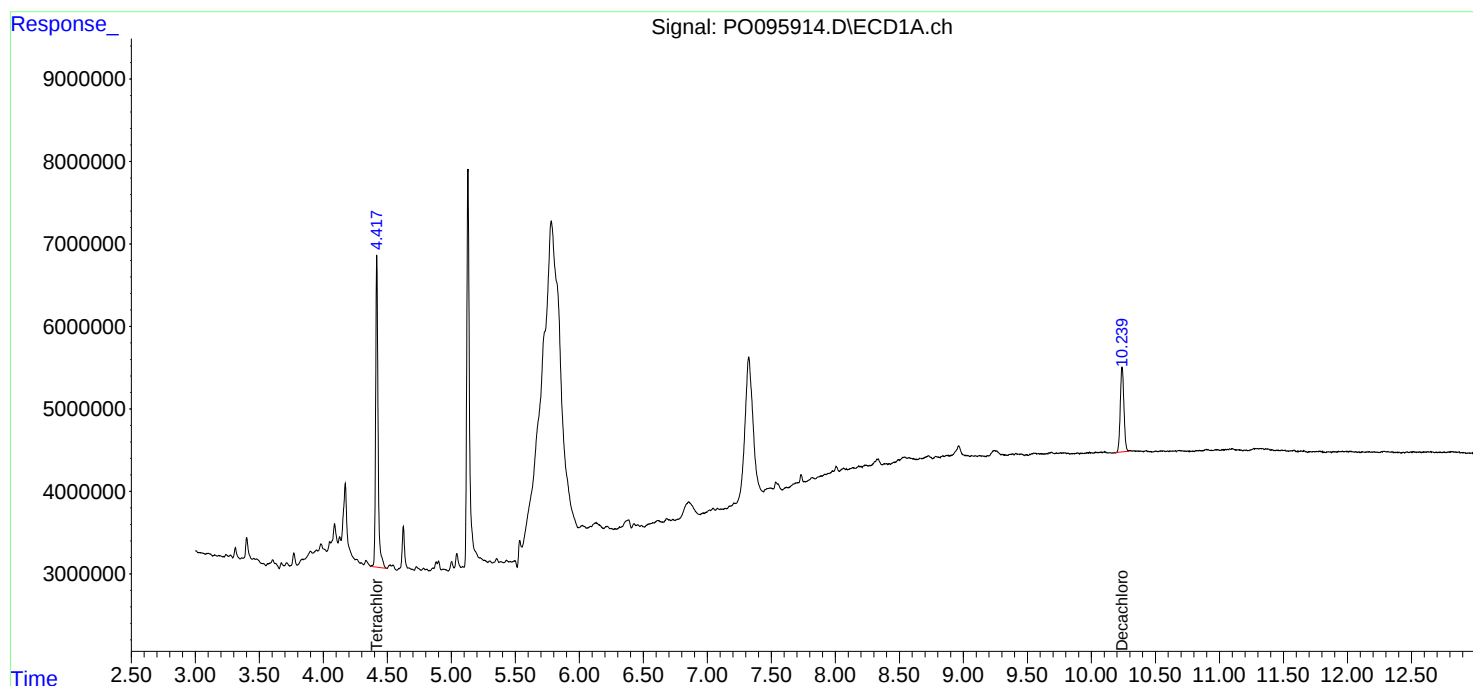


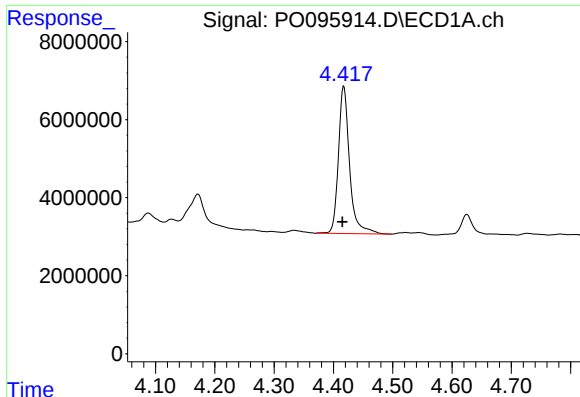

#1 Tetrachloro-m-xylene


R.T.: 4.418 min
Delta R.T.: 0.003 min
Response: 49442442
Conc: 16.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2-0620

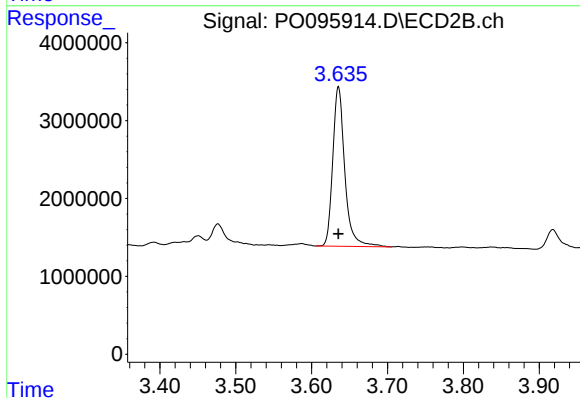


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 22584495
Conc: 16.64 ng/ml

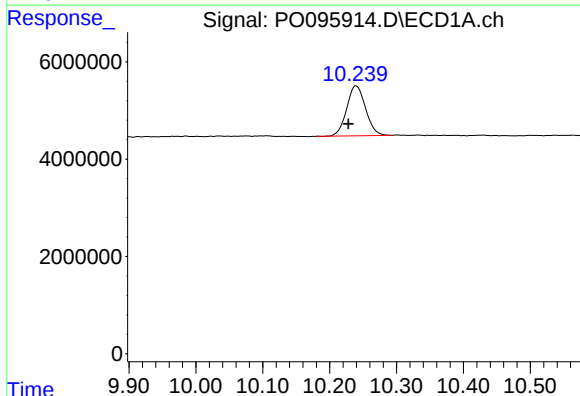

#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: 0.011 min
Response: 20190396
Conc: 9.75 ng/ml

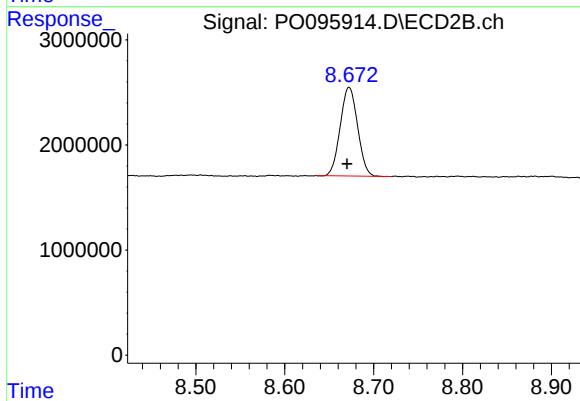

#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: 0.002 min
Response: 11467697
Conc: 9.35 ng/ml