

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062323\
 Data File : P0095917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 14:54
 Operator : YP/AJ
 Sample : 03342-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 50047

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 15:55:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.418	3.636	41821836	19397892	14.374	14.293
2) SA Decachlor...	10.241	8.672	24132338	14054932	11.648m	11.462

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062323\
Data File : PO095917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 14:54
Operator : YP/AJ
Sample : 03342-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
50047


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 15:55:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

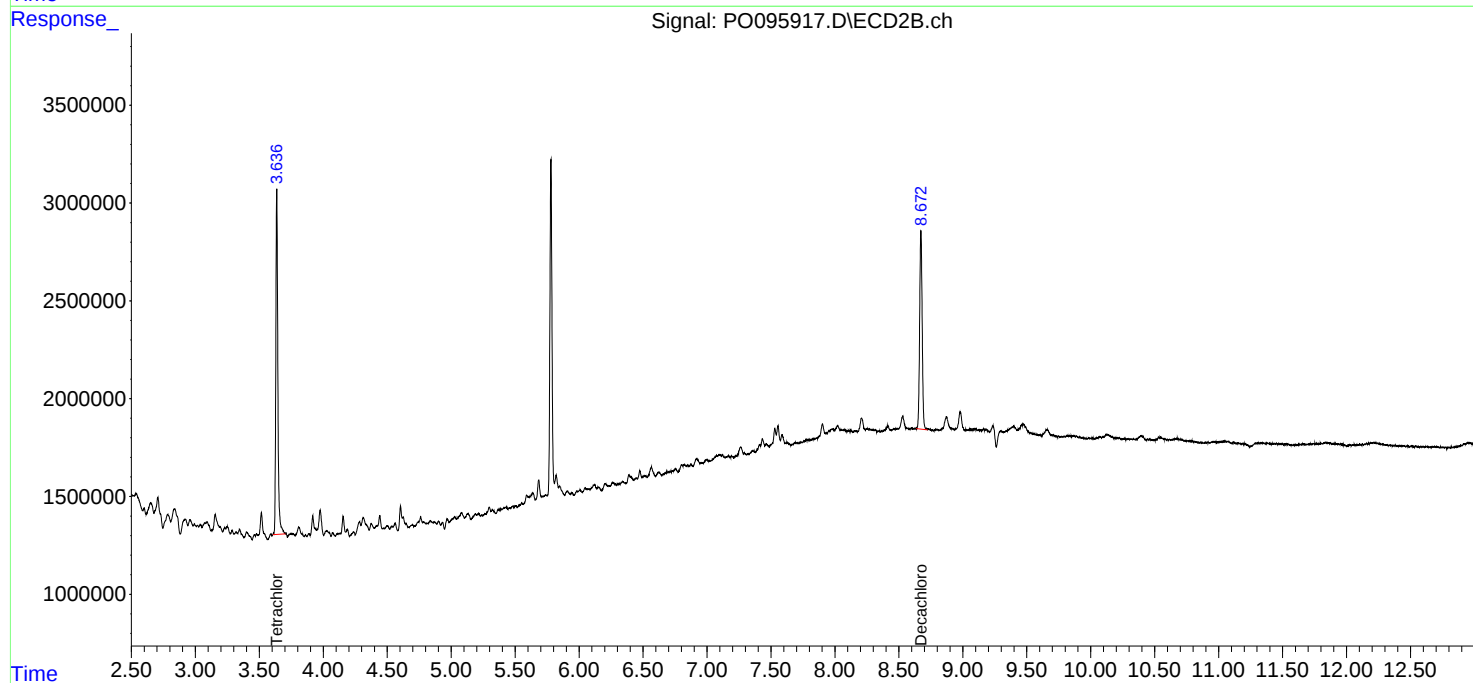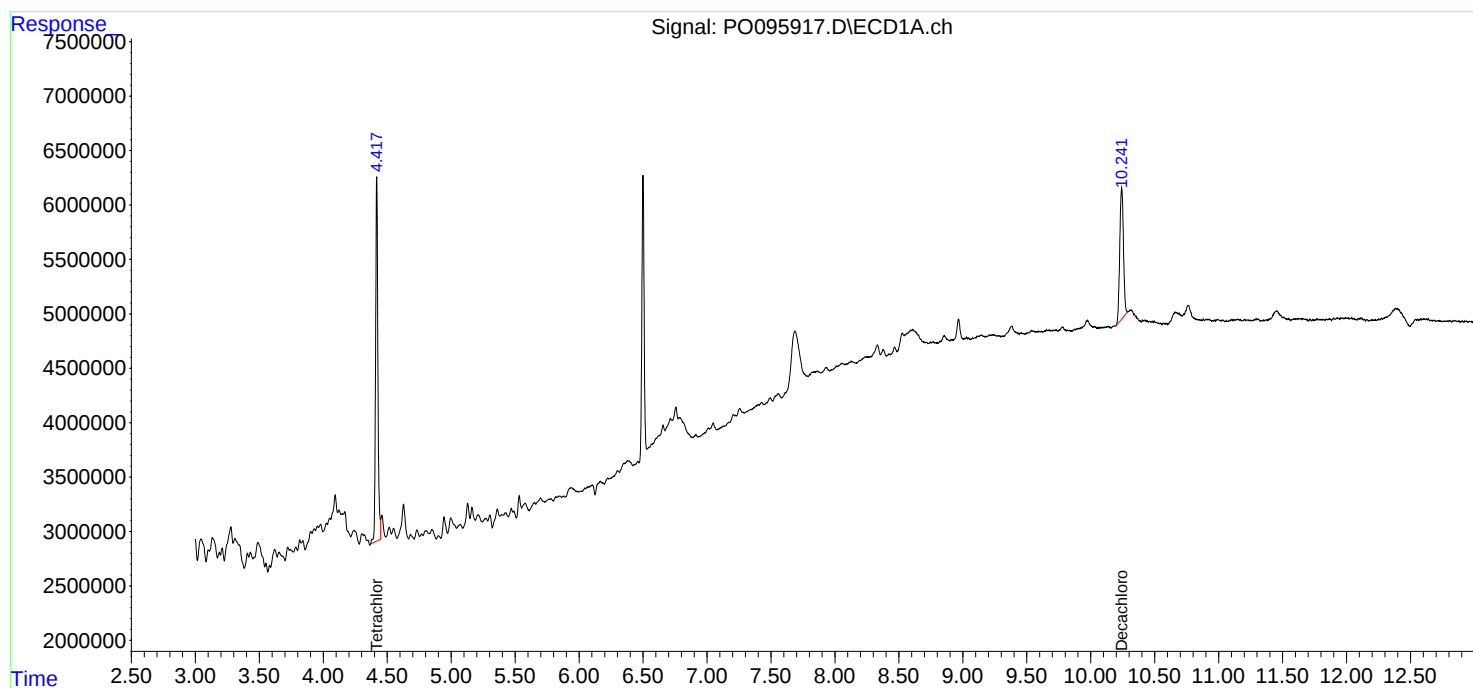

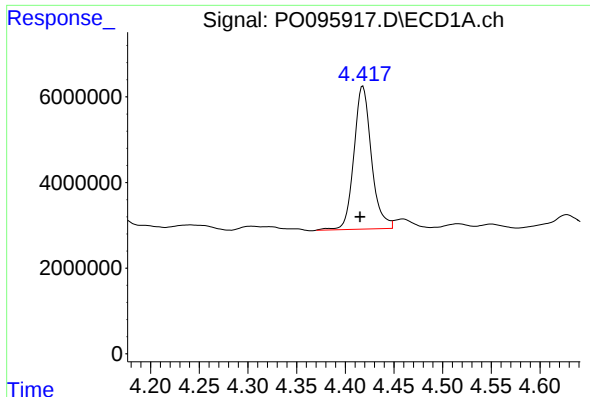


#1 Tetrachloro-m-xylene

R.T.: 4.418 min
Delta R.T.: 0.003 min
Response: 41821836
Conc: 14.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
50047


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

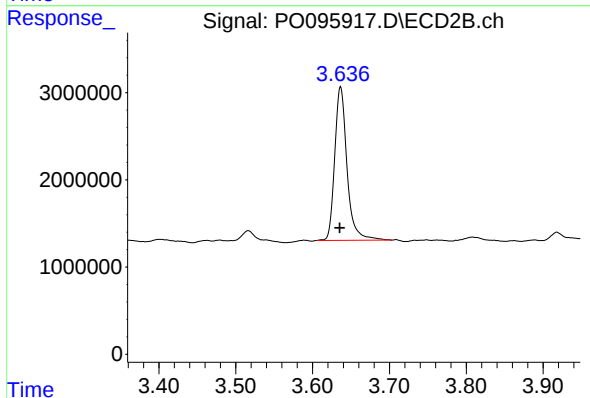


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: 0.001 min
Response: 19397892
Conc: 14.29 ng/ml

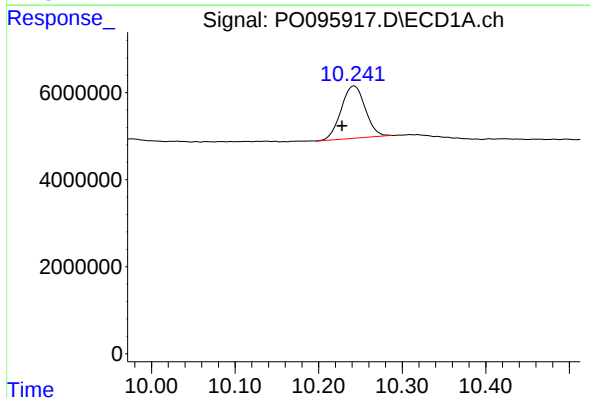

#2 Decachlorobiphenyl

R.T.: 10.241 min
Delta R.T.: 0.013 min
Response: 24132338
Conc: 11.65 ng/ml m

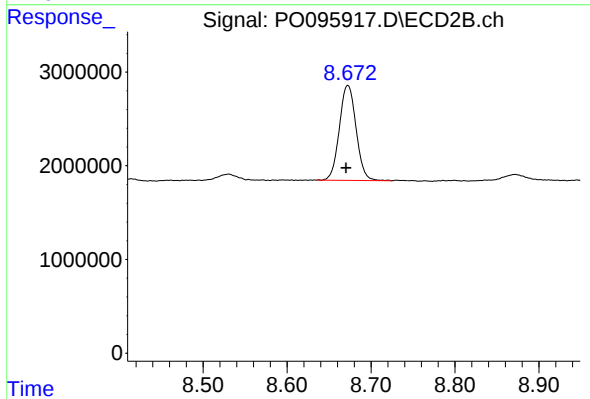

#2 Decachlorobiphenyl

R.T.: 8.672 min
Delta R.T.: 0.002 min
Response: 14054932
Conc: 11.46 ng/ml