

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062323\
 Data File : P0095930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 18:41
 Operator : YP/AJ
 Sample : 03355-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-01-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 22:47:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.634	56534083	25918576	19.431	19.097
2) SA Decachlor...	10.240	8.669	39559099	21824839	19.095	17.799
Target Compounds						
31) L7 AR-1260-1	7.212	6.214	7129073	6594632	62.701	91.884m#
32) L7 AR-1260-2	7.467	6.403	20159355	4854973	166.025	58.282 #
33) L7 AR-1260-3	7.756	6.557	11068383	4439629	79.838	57.633 #
34) L7 AR-1260-4	8.056	7.032	6155185	3306682	64.377	57.970
35) L7 AR-1260-5	8.384	7.273	7476961	7248300	44.785	56.465 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062323\
Data File : PO095930.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 18:41
Operator : YP/AJ
Sample : 03355-02
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 22:47:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

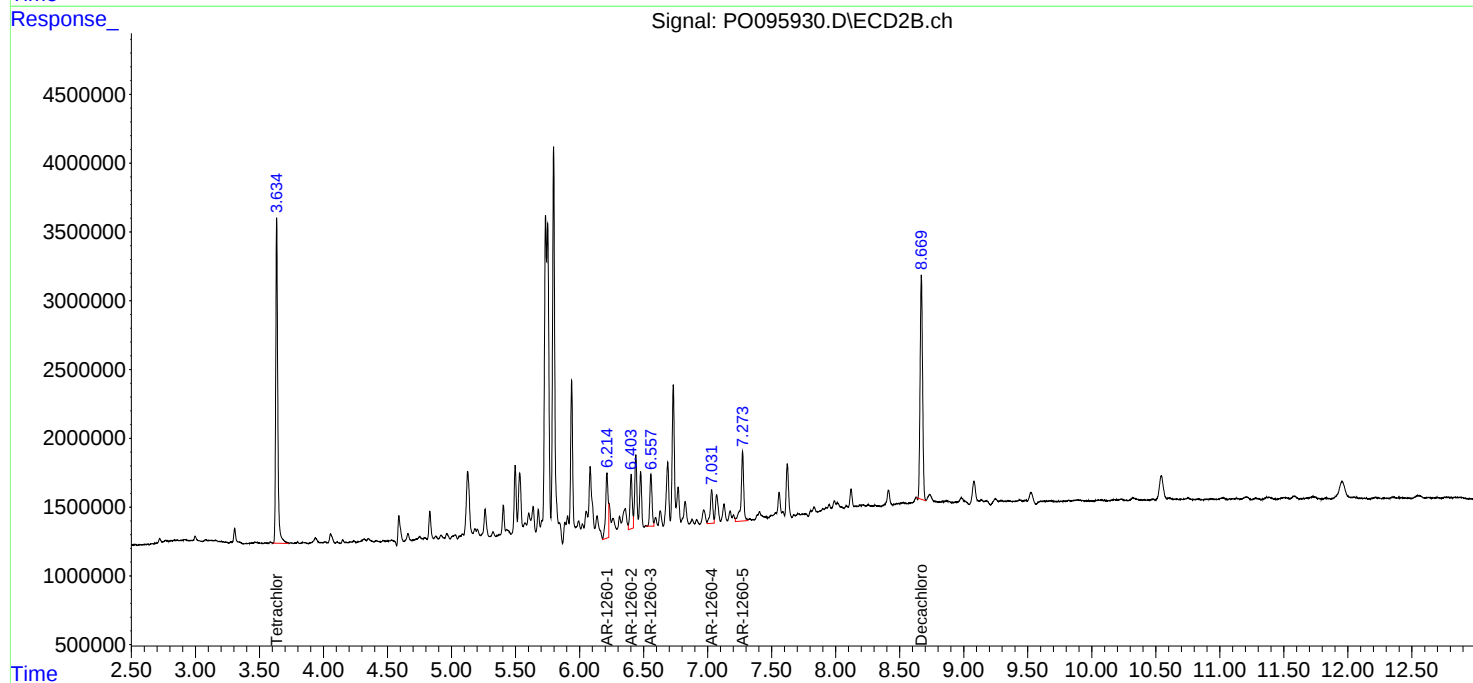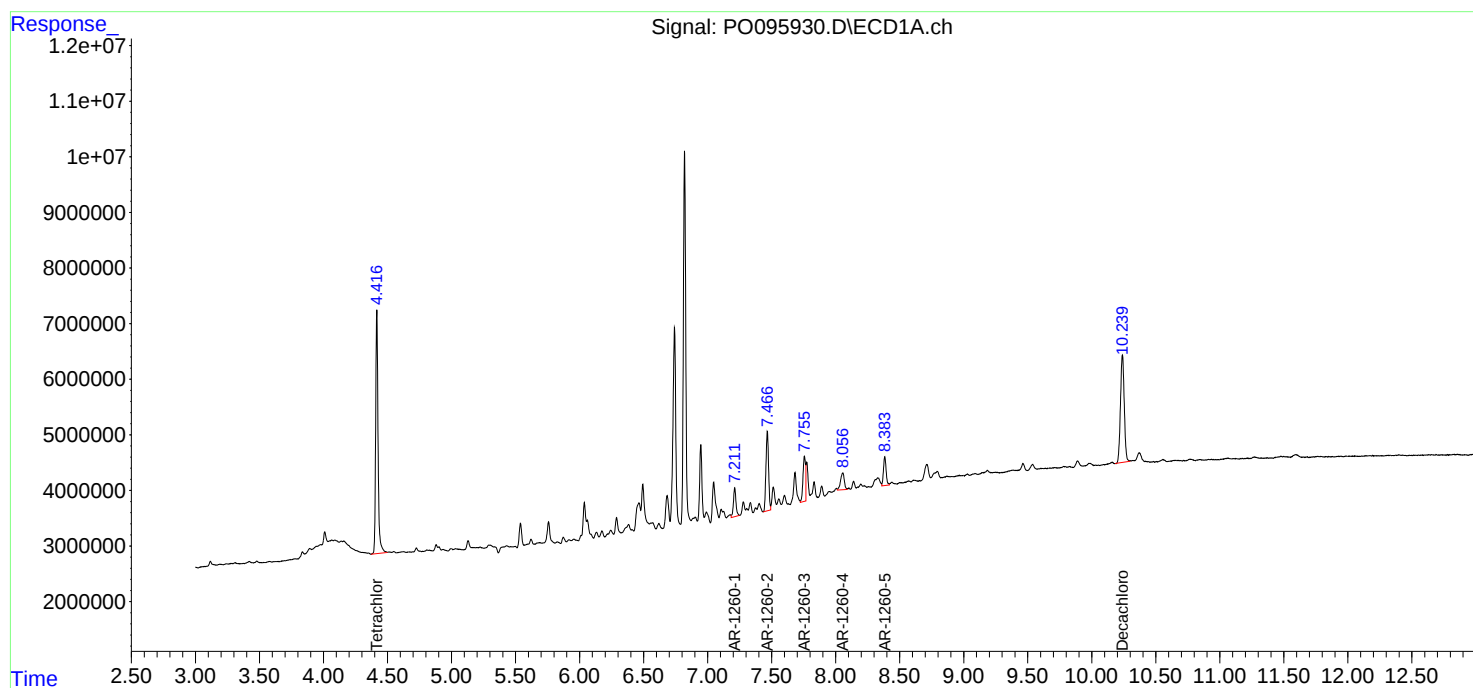

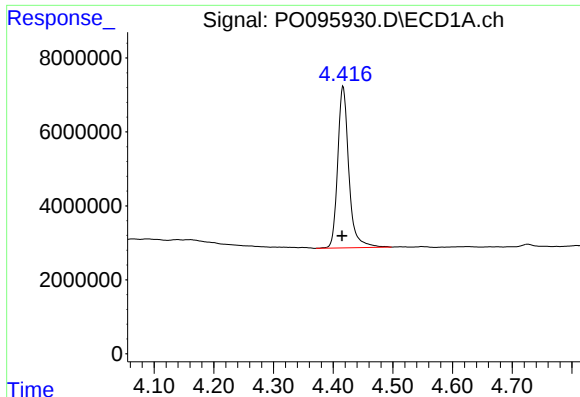


#1 Tetrachloro-m-xylene

R.T.: 4.417 min
Delta R.T.: 0.002 min
Response: 56534083
Conc: 19.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

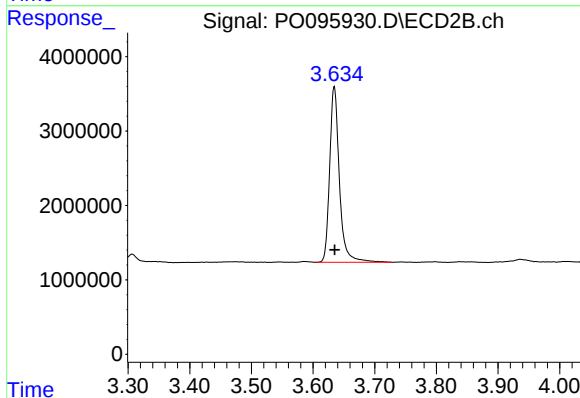


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 25918576
Conc: 19.10 ng/ml

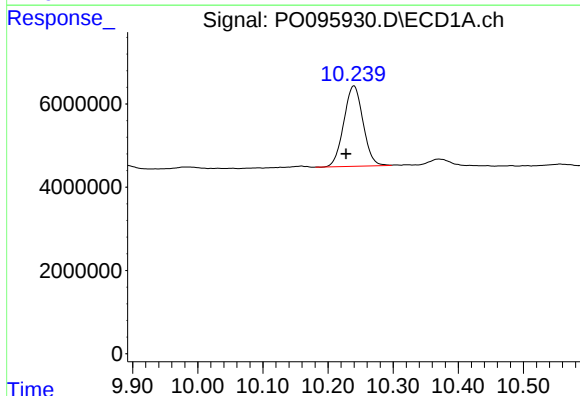


#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.012 min
Response: 39559099
Conc: 19.09 ng/ml

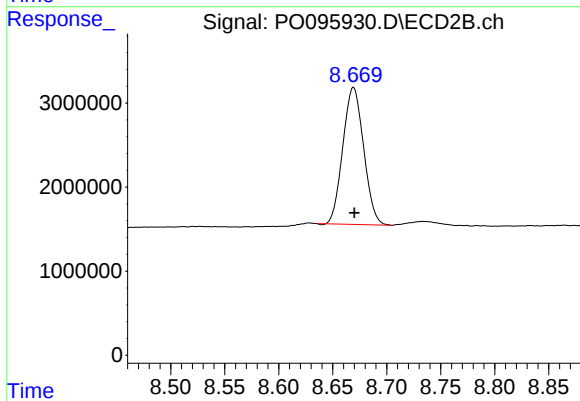

#2 Decachlorobiphenyl

R.T.: 8.669 min
Delta R.T.: 0.000 min
Response: 21824839
Conc: 17.80 ng/ml

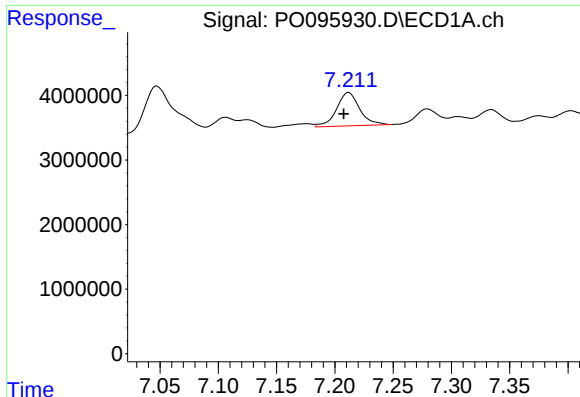


#31 AR-1260-1

R.T.: 7.212 min
Delta R.T.: 0.004 min
Response: 7129073
Conc: 62.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

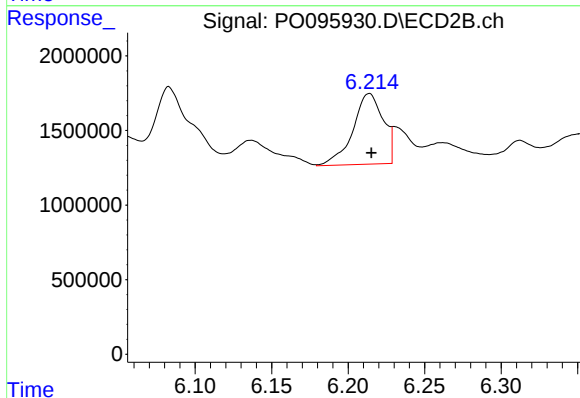


#31 AR-1260-1

R.T.: 6.214 min
Delta R.T.: -0.001 min
Response: 6594632
Conc: 91.88 ng/ml m

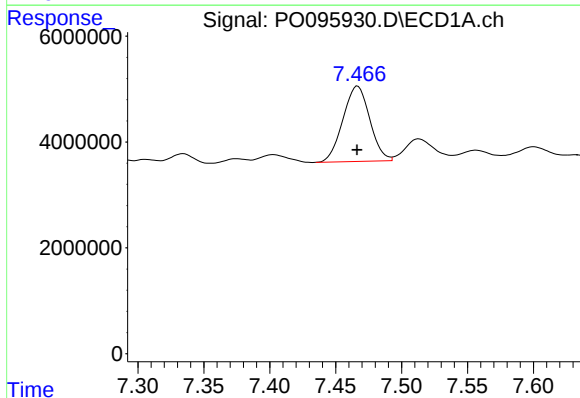


#32 AR-1260-2

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 20159355
Conc: 166.02 ng/ml

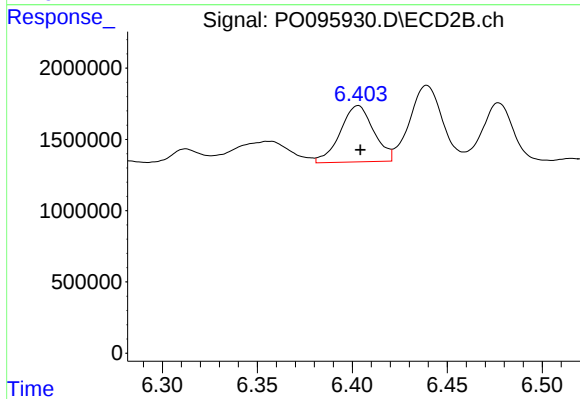

#32 AR-1260-2

R.T.: 6.403 min
Delta R.T.: -0.001 min
Response: 4854973
Conc: 58.28 ng/ml

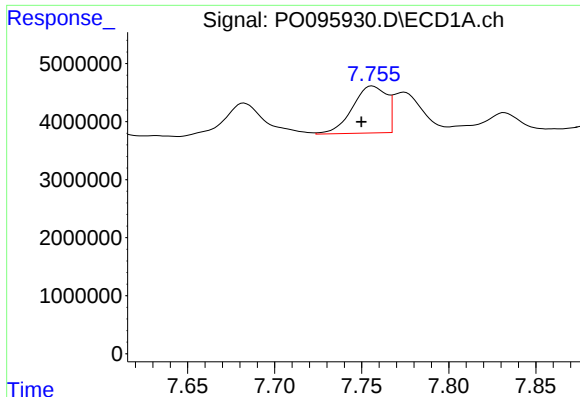


#33 AR-1260-3

R.T.: 7.756 min
Delta R.T.: 0.006 min
Response: 11068383
Conc: 79.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

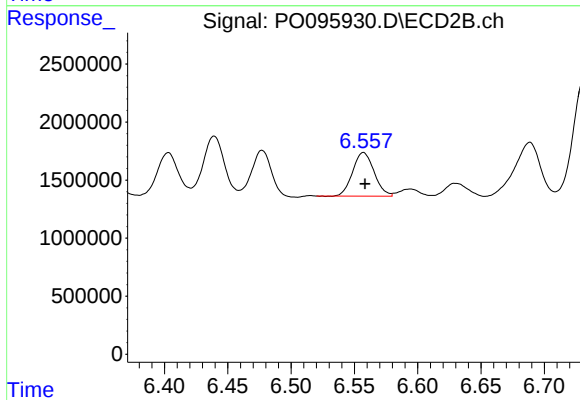


#33 AR-1260-3

R.T.: 6.557 min
Delta R.T.: -0.001 min
Response: 4439629
Conc: 57.63 ng/ml

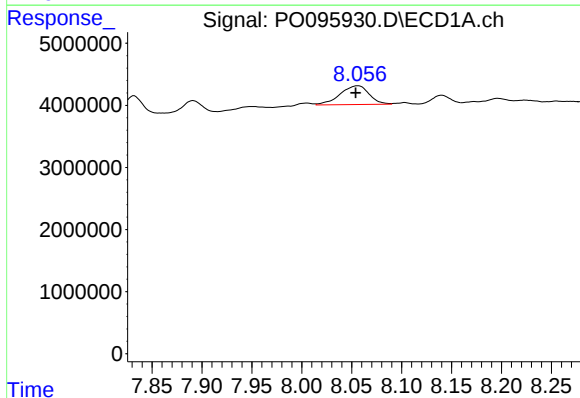


#34 AR-1260-4

R.T.: 8.056 min
Delta R.T.: 0.002 min
Response: 6155185
Conc: 64.38 ng/ml

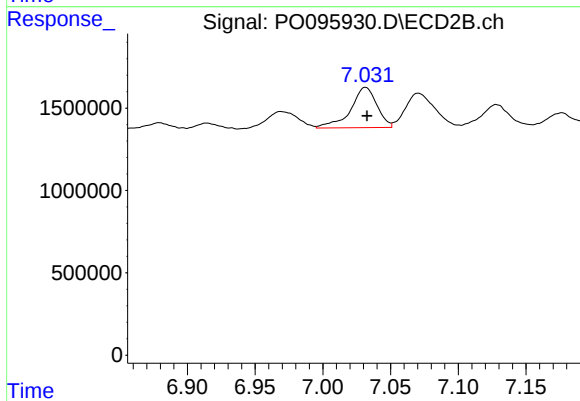

#34 AR-1260-4

R.T.: 7.032 min
Delta R.T.: -0.001 min
Response: 3306682
Conc: 57.97 ng/ml

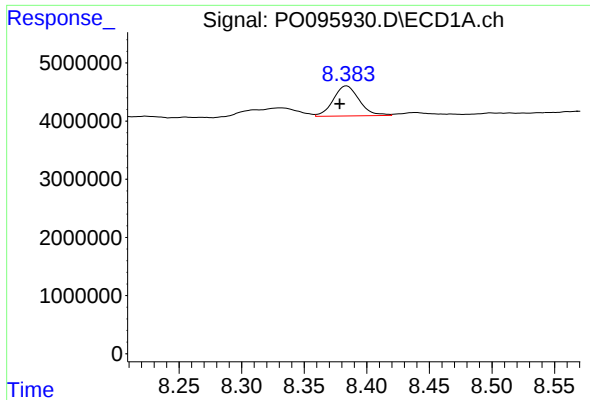


#35 AR-1260-5

R.T.: 8.384 min
Delta R.T.: 0.006 min
Response: 7476961
Conc: 44.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-01-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

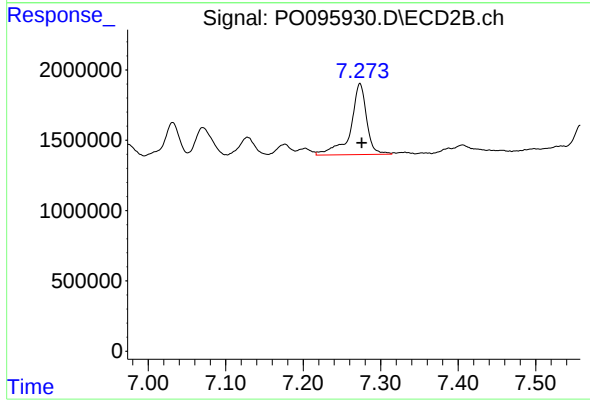

#35 AR-1260-5

R.T.: 7.273 min
Delta R.T.: -0.002 min
Response: 7248300
Conc: 56.47 ng/ml