

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062323\
 Data File : P0095937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 20:39
 Operator : YP/AJ
 Sample : 03355-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-07-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 22:54:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.634	66666346	27463249	22.913	20.235
2) SA Decachlor...	10.238	8.668	52385772	26272122	25.286	21.426m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062323\
Data File : P0095937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 20:39
Operator : YP/AJ
Sample : 03355-14
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-07-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 22:54:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

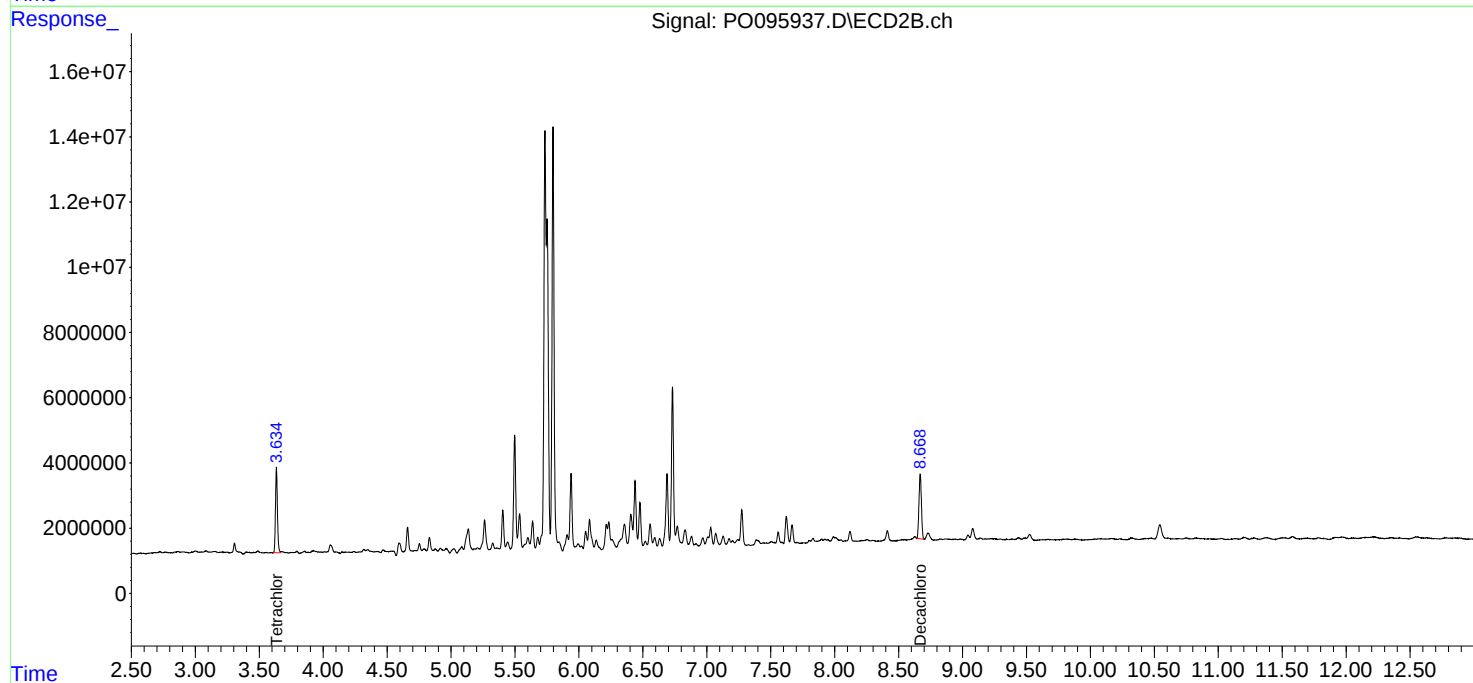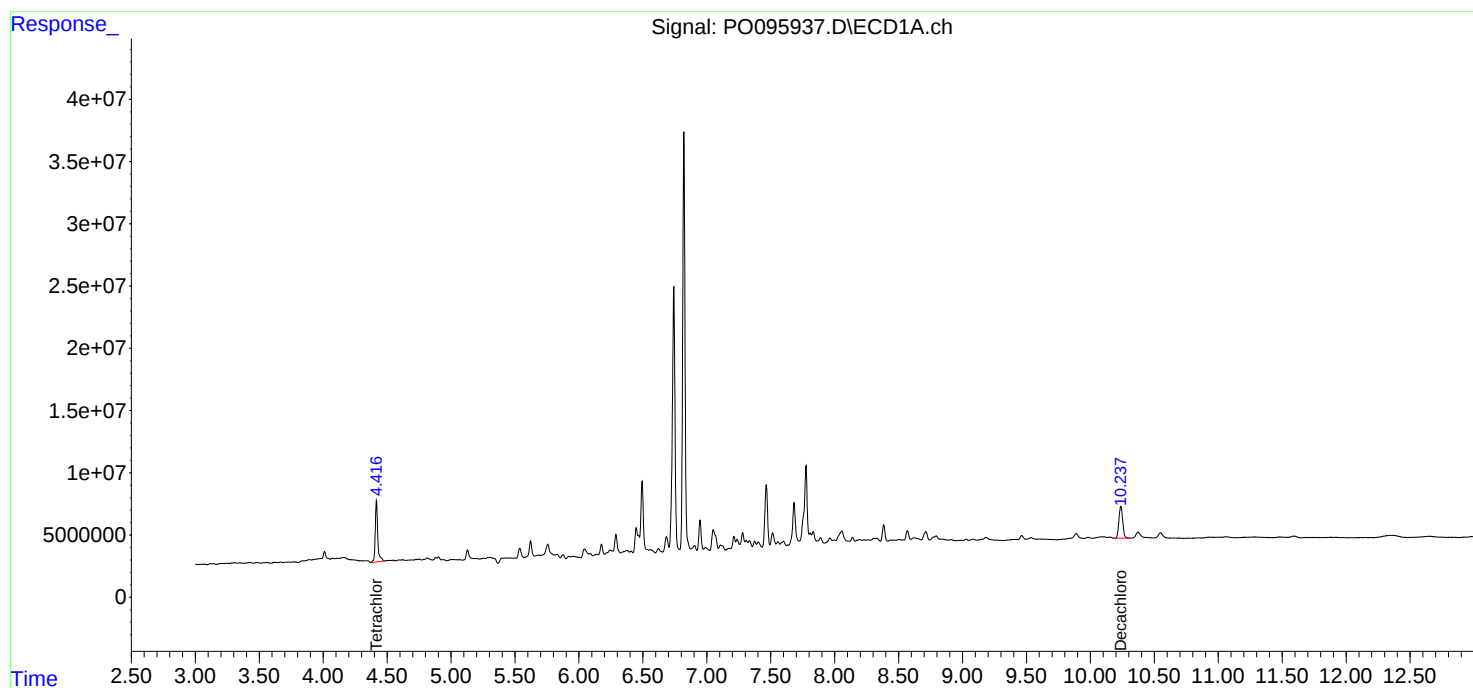

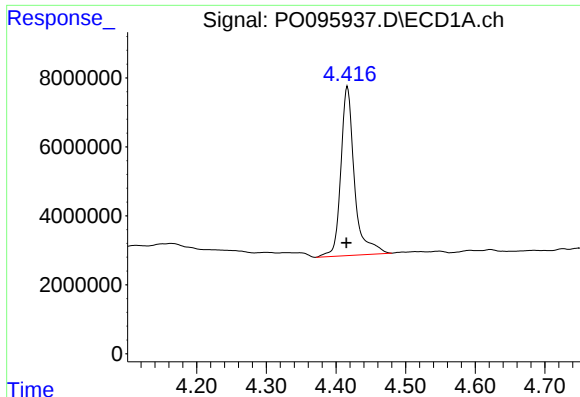


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: 0.001 min
Response: 66666346
Conc: 22.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-07-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

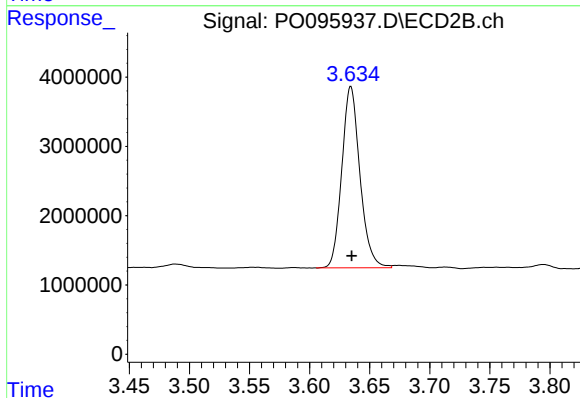


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 27463249
Conc: 20.24 ng/ml

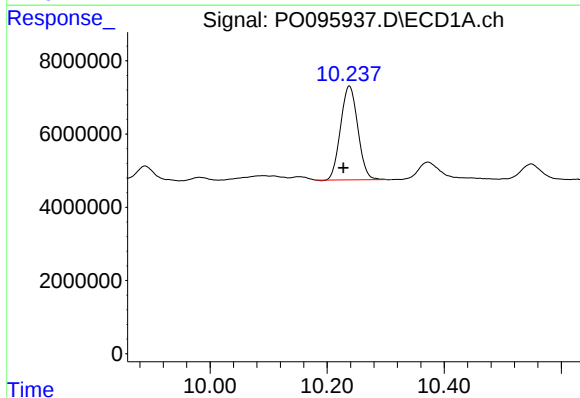

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: 0.010 min
Response: 52385772
Conc: 25.29 ng/ml

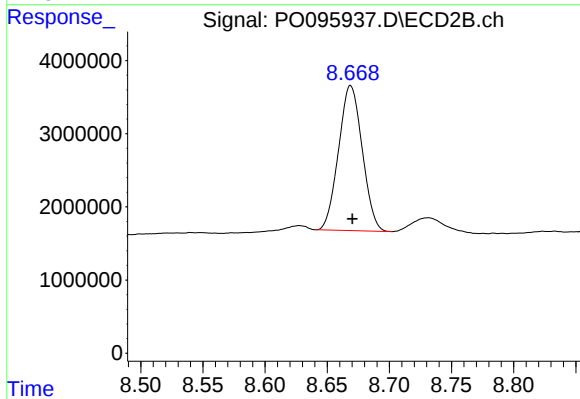

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.002 min
Response: 26272122
Conc: 21.43 ng/ml m