

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062323\
 Data File : P0095943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 23:32
 Operator : YP/AJ
 Sample : 03357-16 10X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-SCAN-04

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 06:20:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.633	5252713	2640297	1.805	1.945
2) SA Decachlor...	10.237	8.668	5298285	3158726	2.557	2.576
Target Compounds						
26) L6 AR-1254-1	6.457	5.530	3742487	2028986	39.305m	27.395 #
27) L6 AR-1254-2	6.679	5.679	4636452	1878626	33.385	27.529
28) L6 AR-1254-3	7.046	6.083	7247624	3127259	53.646	31.405 #
29) L6 AR-1254-4	7.333	6.313	2122082	1430961	23.666	24.245
30) L6 AR-1254-5	7.756	6.732	3026926	2285856	29.426	25.635

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062323\
Data File : PO095943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 23:32
Operator : YP/AJ
Sample : 03357-16 10X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-SCAN-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:20:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

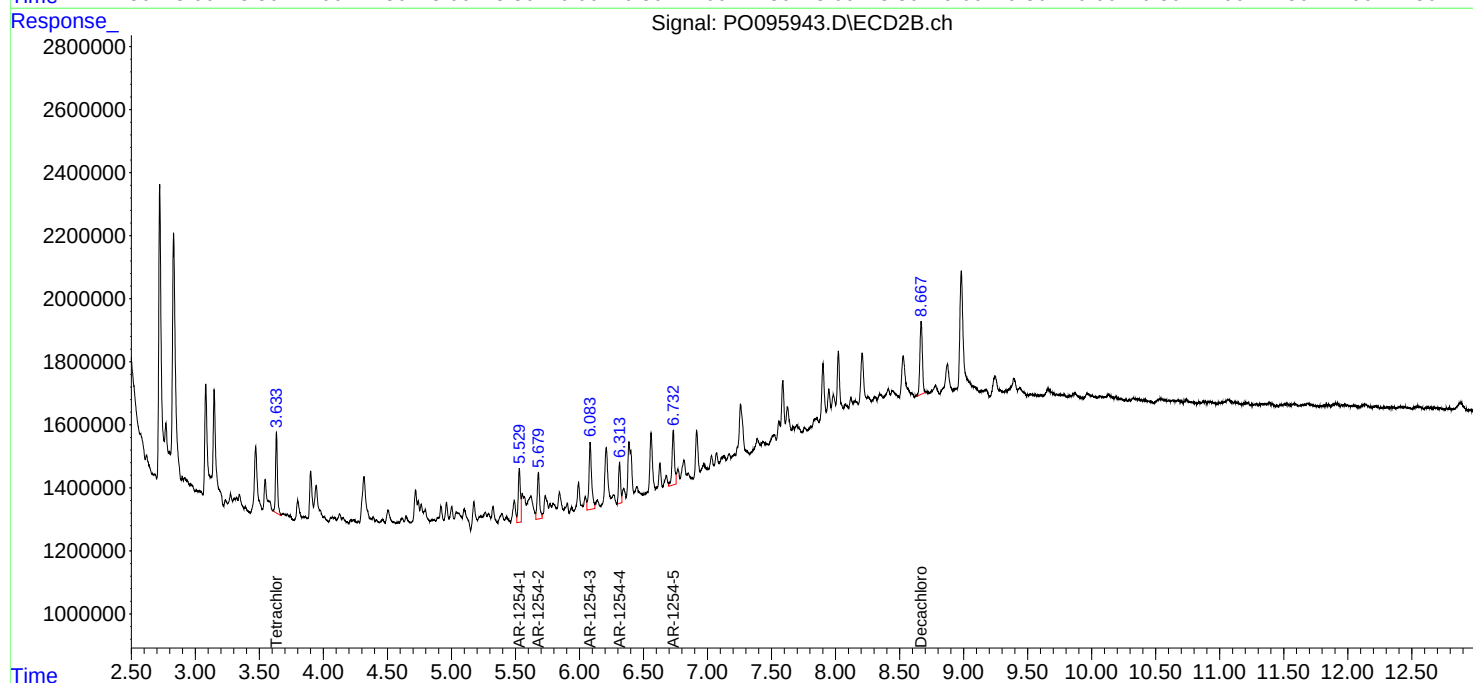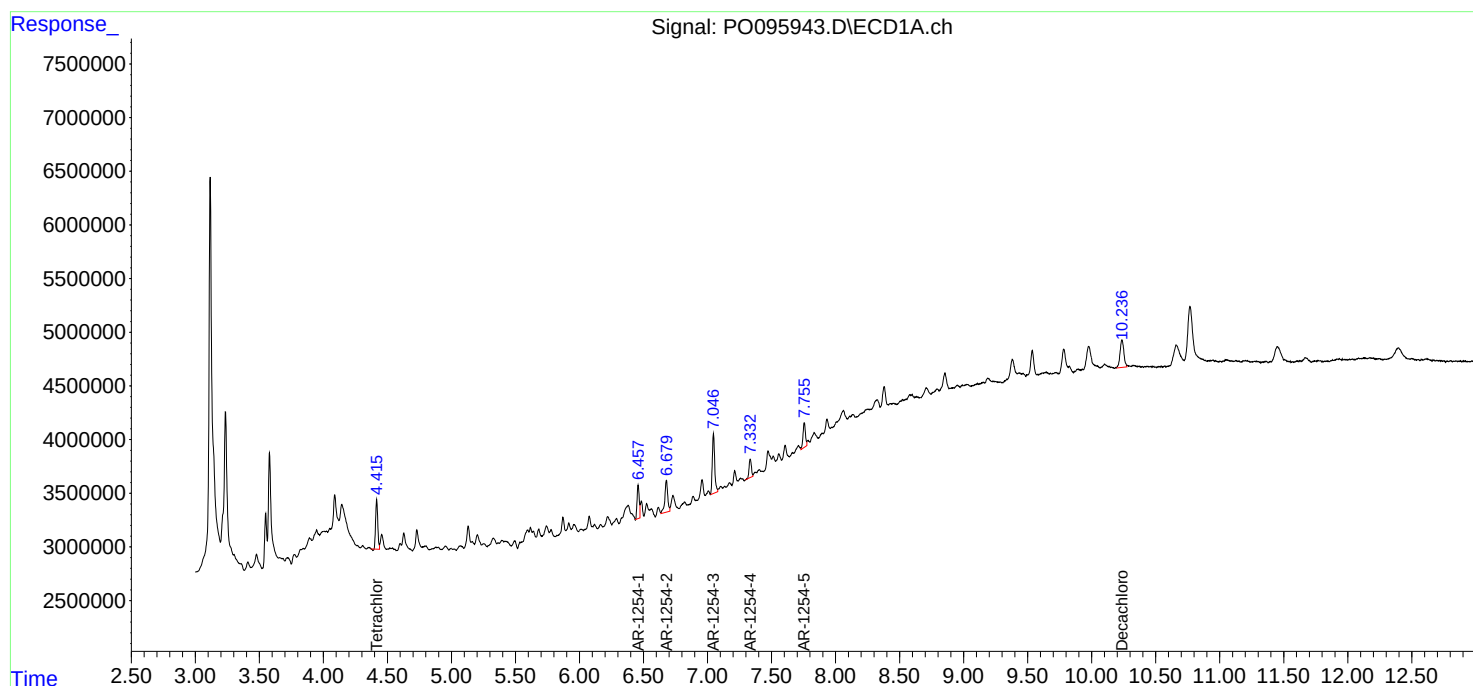

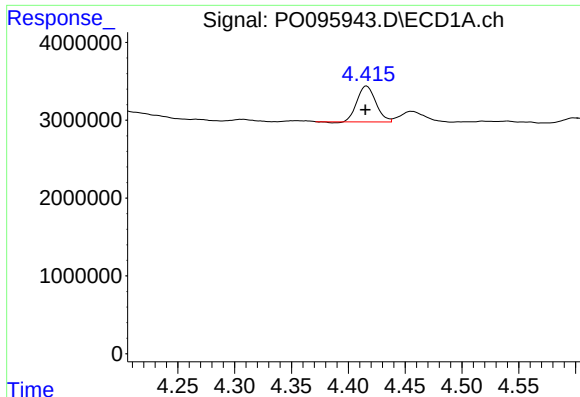


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: 0.001 min
Response: 5252713
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-SCAN-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

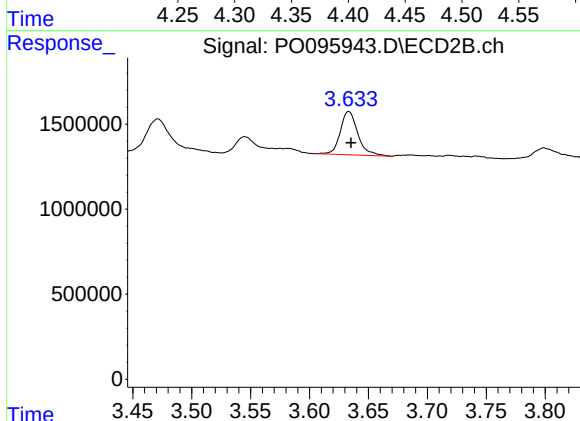


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.002 min
Response: 2640297
Conc: 1.95 ng/ml

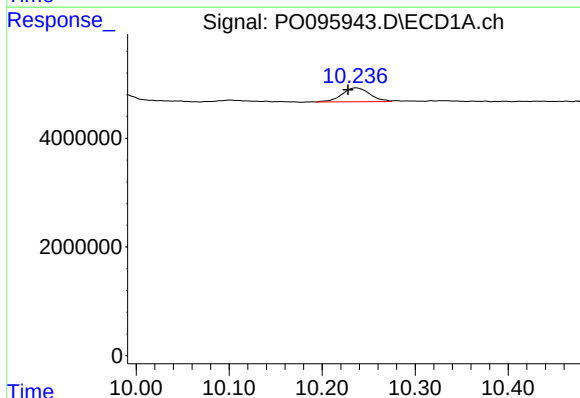


#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: 0.009 min
Response: 5298285
Conc: 2.56 ng/ml

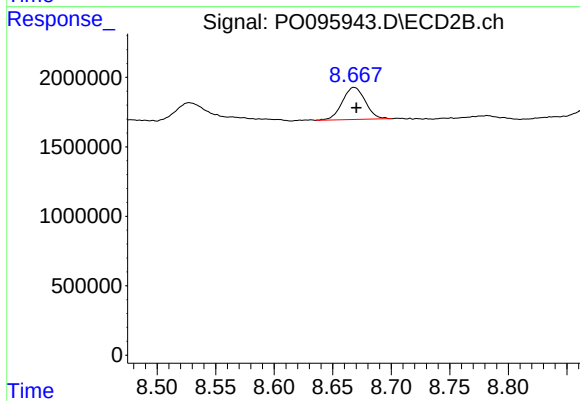

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.002 min
Response: 3158726
Conc: 2.58 ng/ml

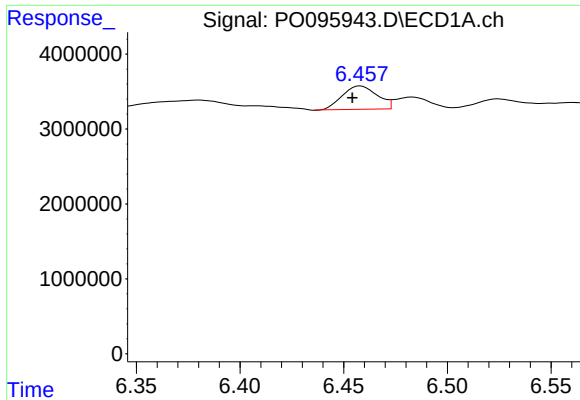


#26 AR-1254-1

R.T.: 6.457 min
Delta R.T.: 0.003 min
Response: 3742487
Conc: 39.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-SCAN-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

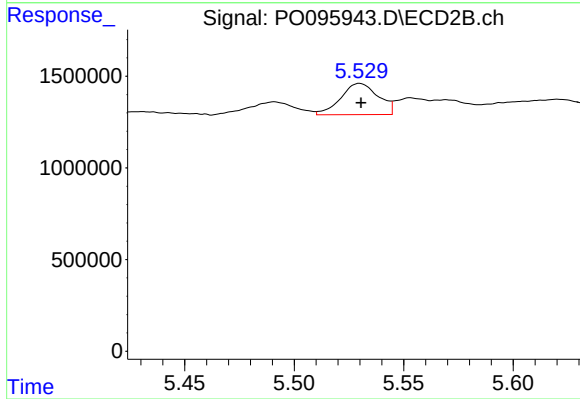


#26 AR-1254-1

R.T.: 5.530 min
Delta R.T.: 0.000 min
Response: 2028986
Conc: 27.40 ng/ml

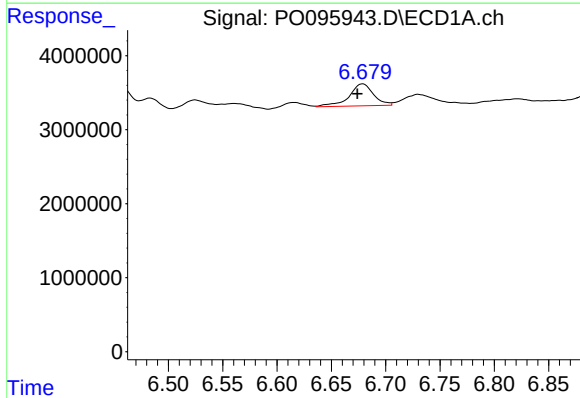


#27 AR-1254-2

R.T.: 6.679 min
Delta R.T.: 0.005 min
Response: 4636452
Conc: 33.38 ng/ml

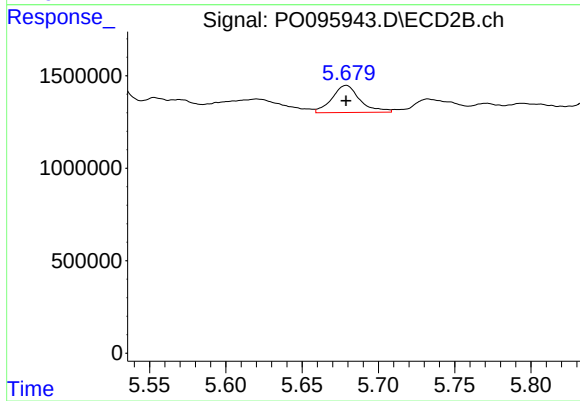

#27 AR-1254-2

R.T.: 5.679 min
Delta R.T.: 0.000 min
Response: 1878626
Conc: 27.53 ng/ml

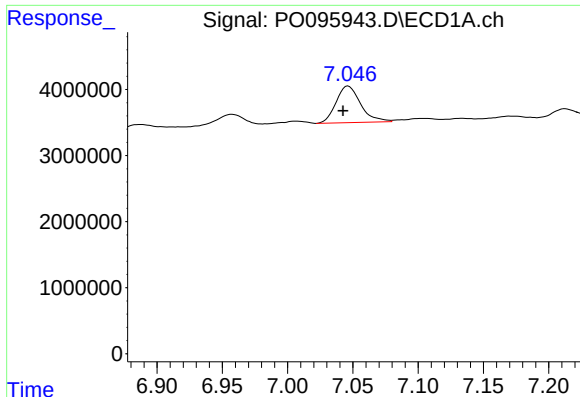


#28 AR-1254-3

R.T.: 7.046 min
Delta R.T.: 0.004 min
Response: 7247624
Conc: 53.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-SCAN-04


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

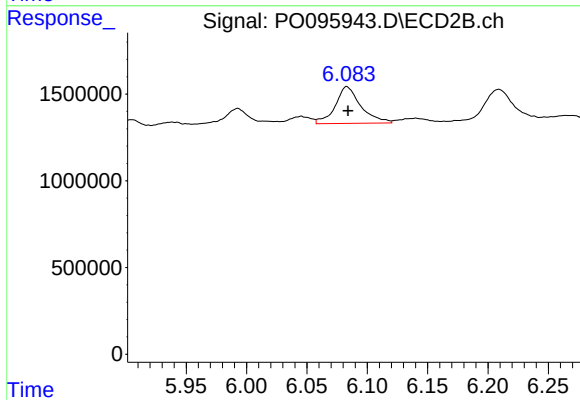


#28 AR-1254-3

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 3127259
Conc: 31.40 ng/ml

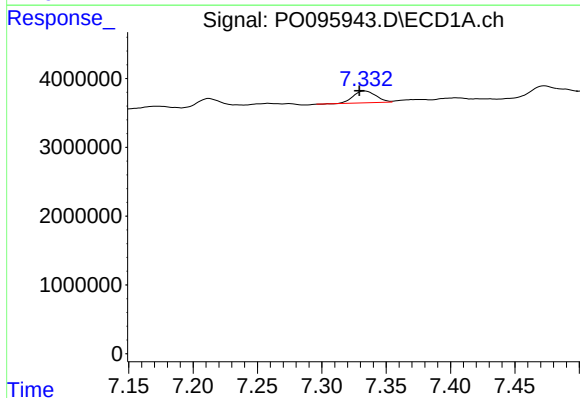


#29 AR-1254-4

R.T.: 7.333 min
Delta R.T.: 0.004 min
Response: 2122082
Conc: 23.67 ng/ml

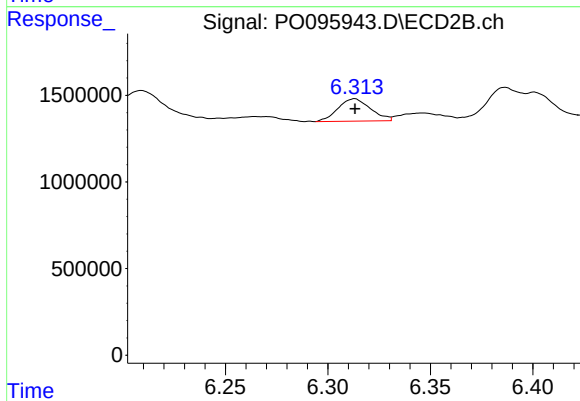

#29 AR-1254-4

R.T.: 6.313 min
Delta R.T.: 0.000 min
Response: 1430961
Conc: 24.25 ng/ml

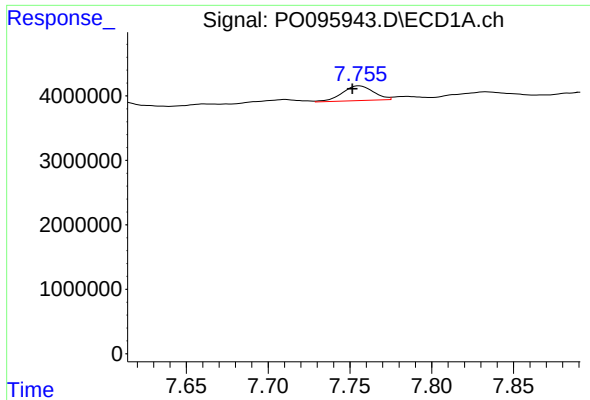


#30 AR-1254-5

R.T.: 7.756 min
Delta R.T.: 0.004 min
Response: 3026926
Conc: 29.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-SCAN-04

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

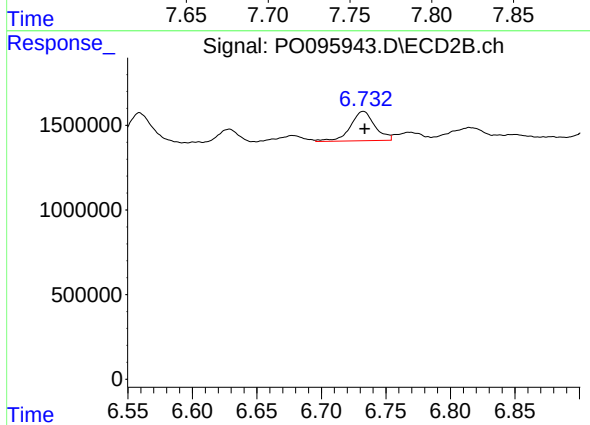

#30 AR-1254-5

R.T.: 6.732 min
Delta R.T.: -0.001 min
Response: 2285856
Conc: 25.64 ng/ml