

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0062323\
 Data File : P0095944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 23:49
 Operator : YP/AJ
 Sample : 03355-08 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SB-04-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/26/2023
 Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 06:20:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0062023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 21 13:08:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.634	5697743	2162728	1.958	1.594
2) SA Decachlor...	10.239	8.668	4664306	2764780	2.251	2.255m
Target Compounds						
26) L6 AR-1254-1	6.459	5.531	14795923	8117743	155.393	109.605m#
27) L6 AR-1254-2	6.679	5.677	14983135	5503190	107.885	80.642m#
28) L6 AR-1254-3	7.050	6.084	23087903	10025399	170.893	100.677m#
29) L6 AR-1254-4	7.333	6.312	4517740	2743647	50.383	46.487
30) L6 AR-1254-5	7.755	6.732	19977737	12869473	194.209	144.329 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062323\
Data File : PO095944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 23:49
Operator : YP/AJ
Sample : 03355-08 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-04-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:20:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 21 13:08:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

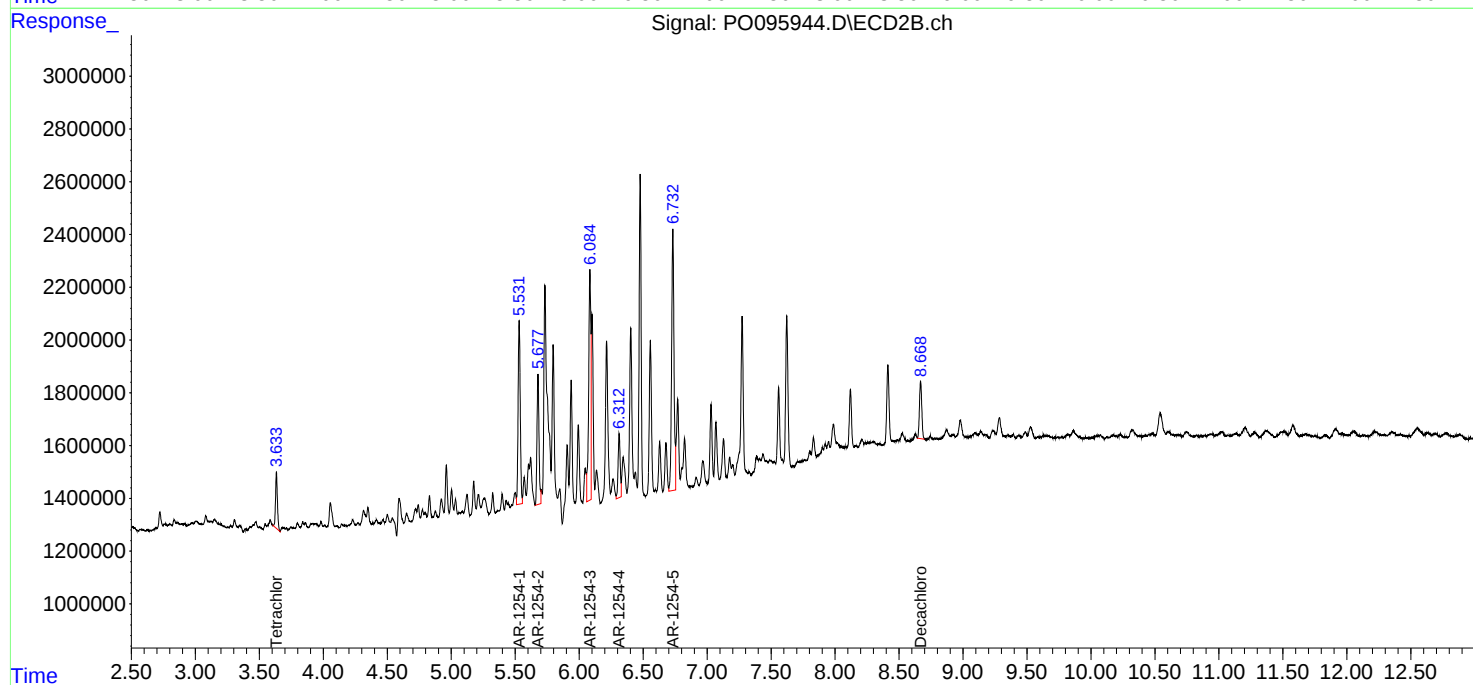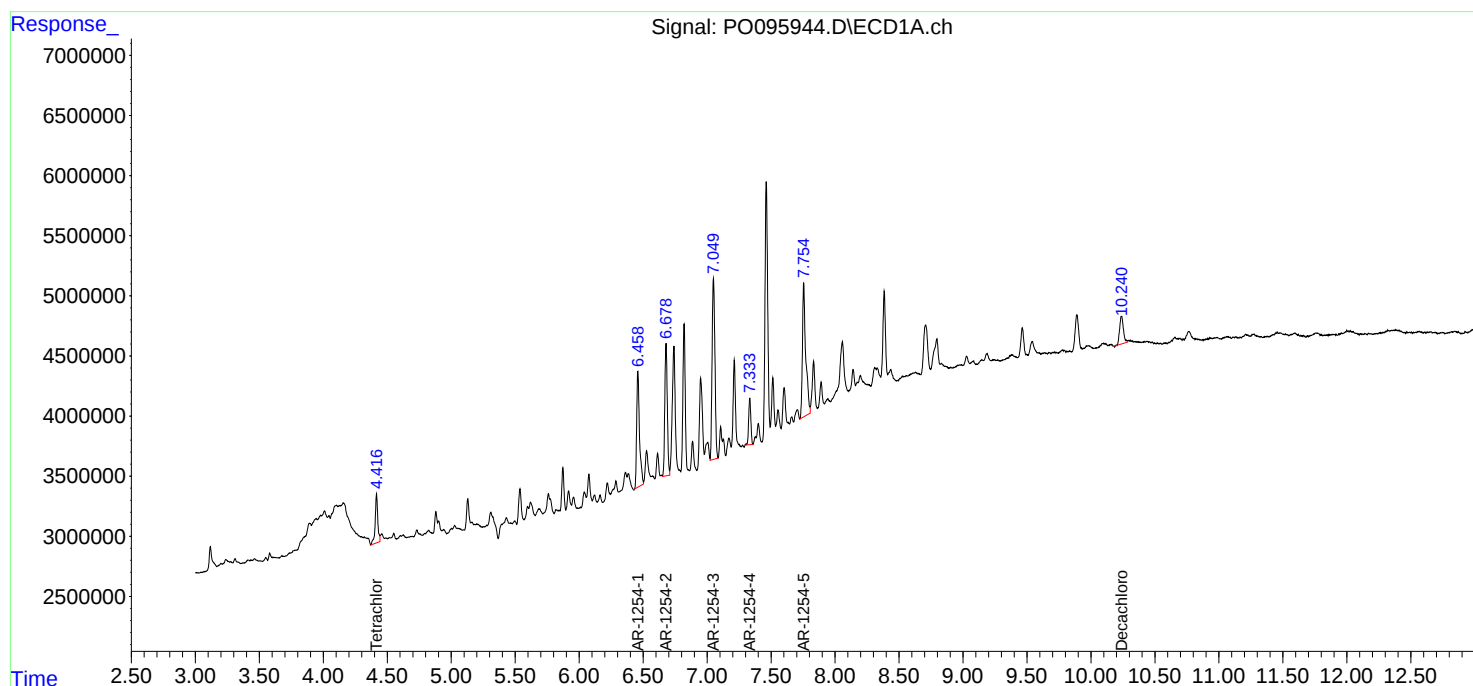

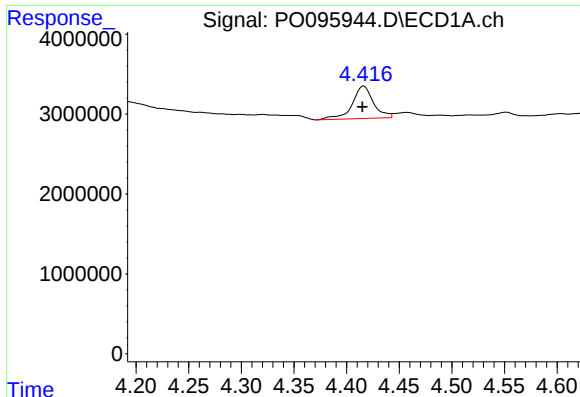


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: 0.001 min
Response: 5697743
Conc: 1.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

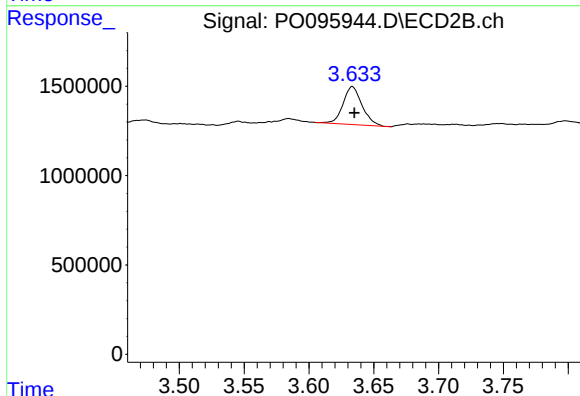


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.002 min
Response: 2162728
Conc: 1.59 ng/ml

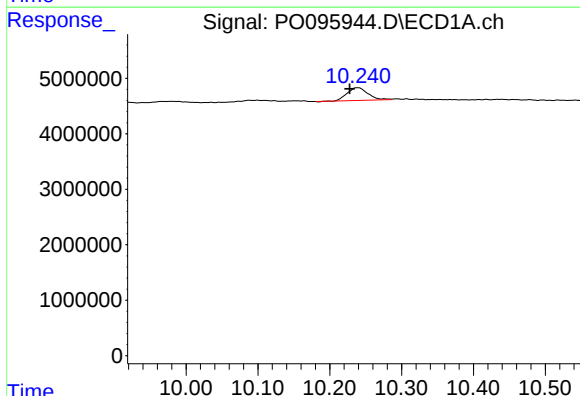


#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: 0.011 min
Response: 4664306
Conc: 2.25 ng/ml

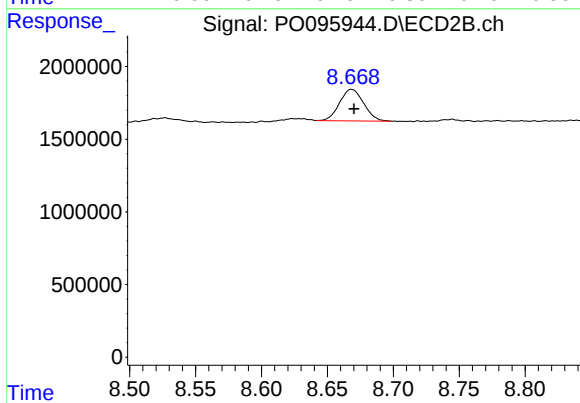

#2 Decachlorobiphenyl

R.T.: 8.668 min
Delta R.T.: -0.003 min
Response: 2764780
Conc: 2.25 ng/ml m

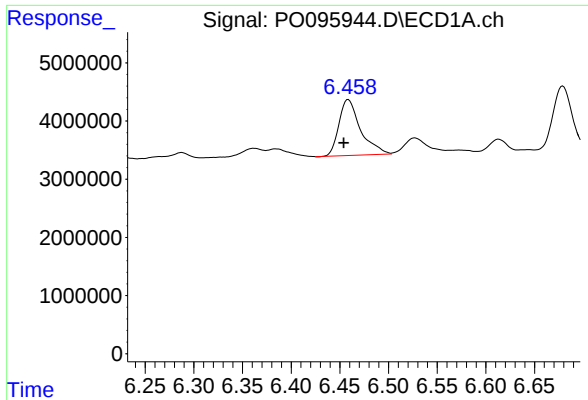


#26 AR-1254-1

R.T.: 6.459 min
Delta R.T.: 0.005 min
Response: 14795923
Conc: 155.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

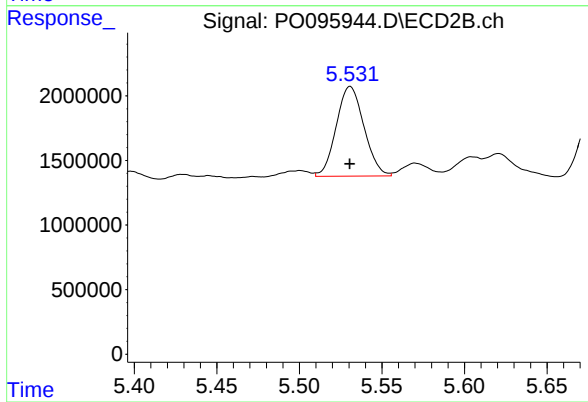


#26 AR-1254-1

R.T.: 5.531 min
Delta R.T.: 0.000 min
Response: 8117743
Conc: 109.60 ng/ml m

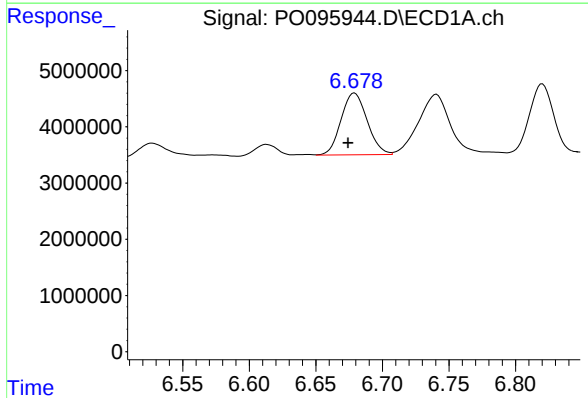


#27 AR-1254-2

R.T.: 6.679 min
Delta R.T.: 0.005 min
Response: 14983135
Conc: 107.89 ng/ml

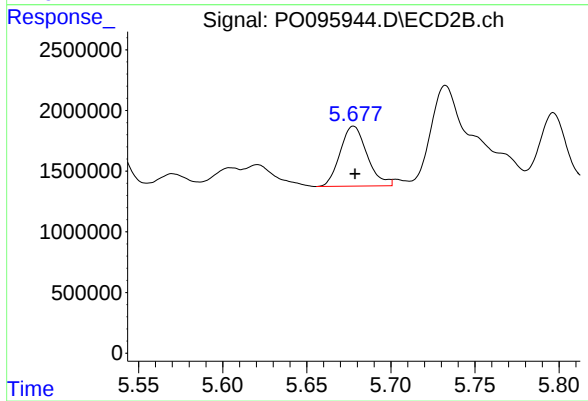

#27 AR-1254-2

R.T.: 5.677 min
Delta R.T.: -0.001 min
Response: 5503190
Conc: 80.64 ng/ml m

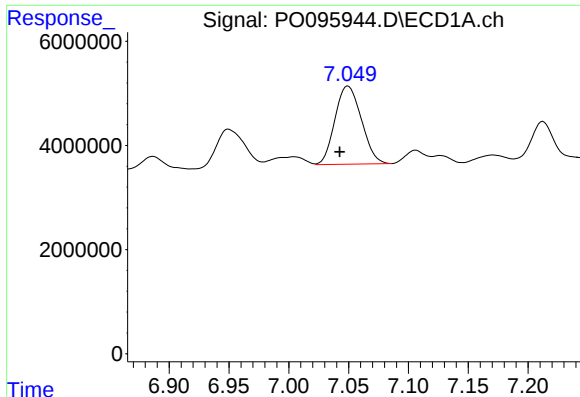


#28 AR-1254-3

R.T.: 7.050 min
Delta R.T.: 0.007 min
Response: 23087903
Conc: 170.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

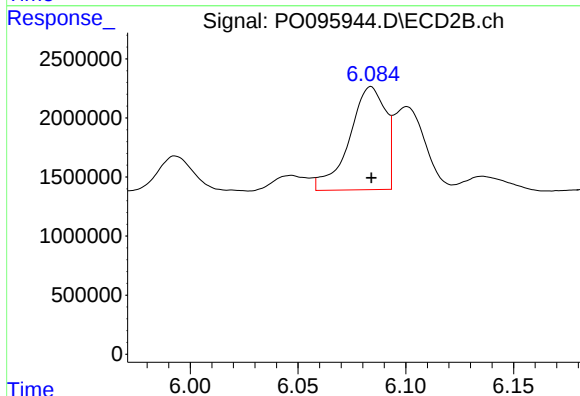


#28 AR-1254-3

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 10025399
Conc: 100.68 ng/ml m

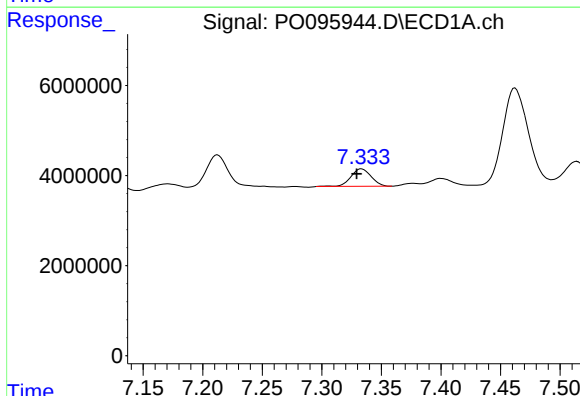


#29 AR-1254-4

R.T.: 7.333 min
Delta R.T.: 0.004 min
Response: 4517740
Conc: 50.38 ng/ml

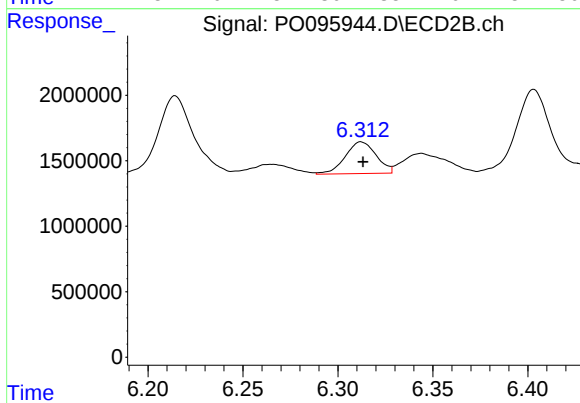

#29 AR-1254-4

R.T.: 6.312 min
Delta R.T.: 0.000 min
Response: 2743647
Conc: 46.49 ng/ml

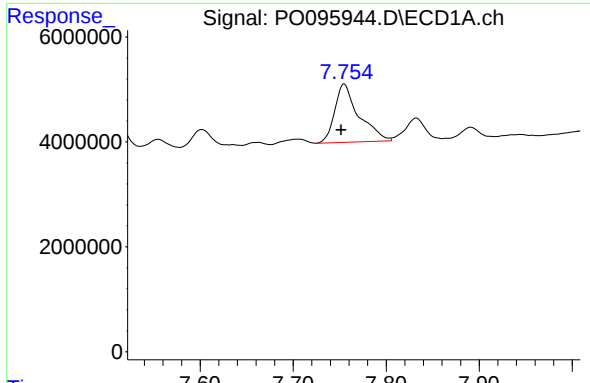


#30 AR-1254-5

R.T.: 7.755 min
Delta R.T.: 0.004 min
Response: 19977737
Conc: 194.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-04-COMP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

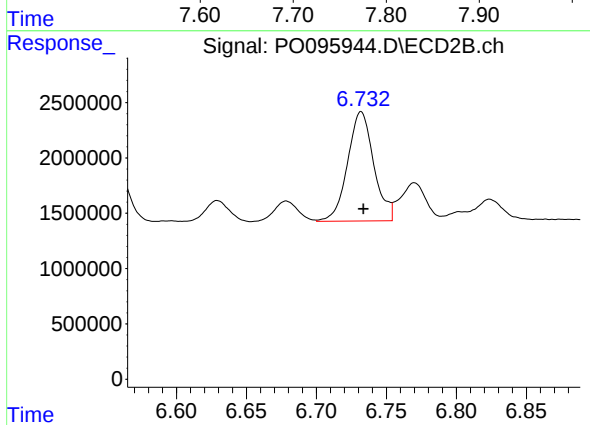

#30 AR-1254-5

R.T.: 6.732 min
Delta R.T.: -0.002 min
Response: 12869473
Conc: 144.33 ng/ml