

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0062325\
 Data File : P0111830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2025 17:04
 Operator : YP/AJ
 Sample : Q2126-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 07:13:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.677	3.672	114.6E6	103.9E6	19.897	18.502
2) SA Decachlor...	8.709	8.657	108.3E6	36555015	20.634	20.564
Target Compounds						
21) L5 AR-1248-1	4.765	4.748	4046755	3978274	25.094	29.848
22) L5 AR-1248-2	5.003	4.984	4944627	4664553	22.934	26.182
23) L5 AR-1248-3	5.217	5.027	6699791	4773962	24.838	25.201
24) L5 AR-1248-4	5.570	5.197	11335517	5490600	28.353	24.047
25) L5 AR-1248-5	5.612	5.588	7115506	5484536	25.339	25.186



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO062325\
Data File : PO111830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2025 17:04
Operator : YP/AJ
Sample : Q2126-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 07:13:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

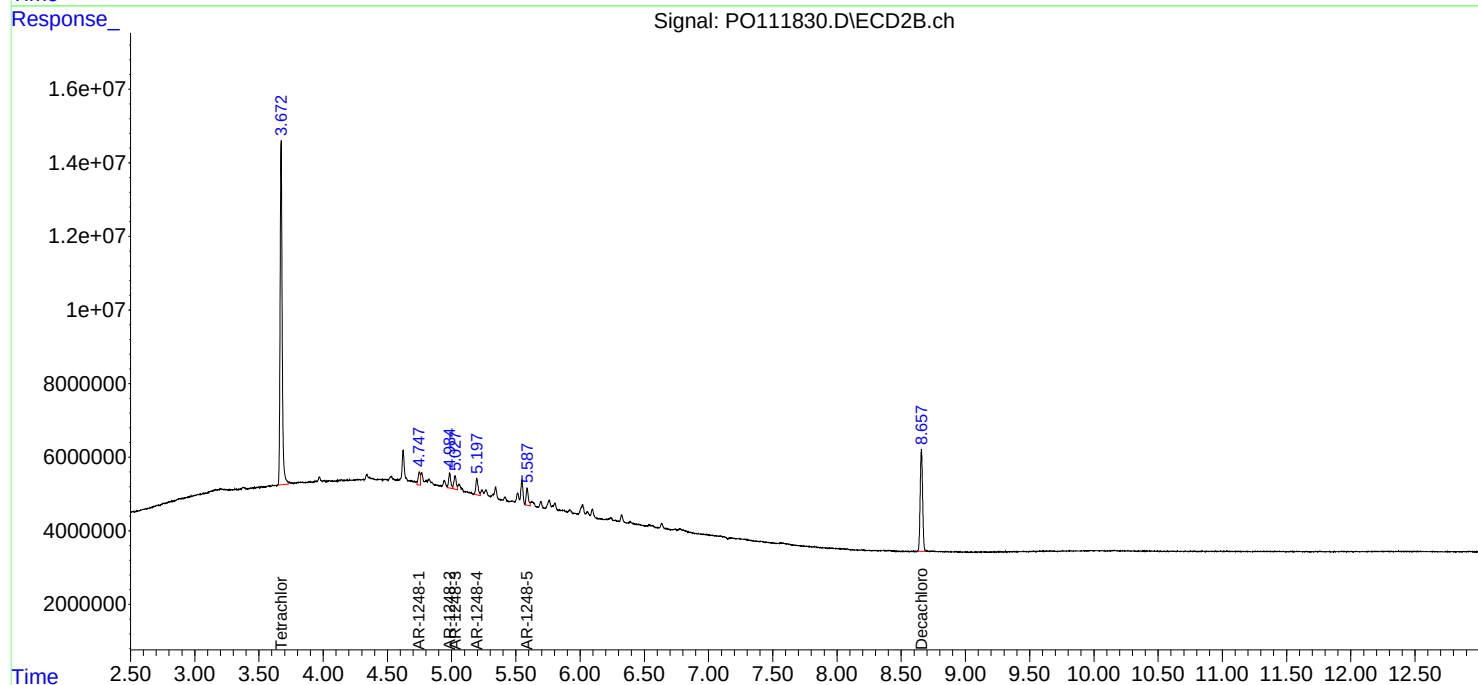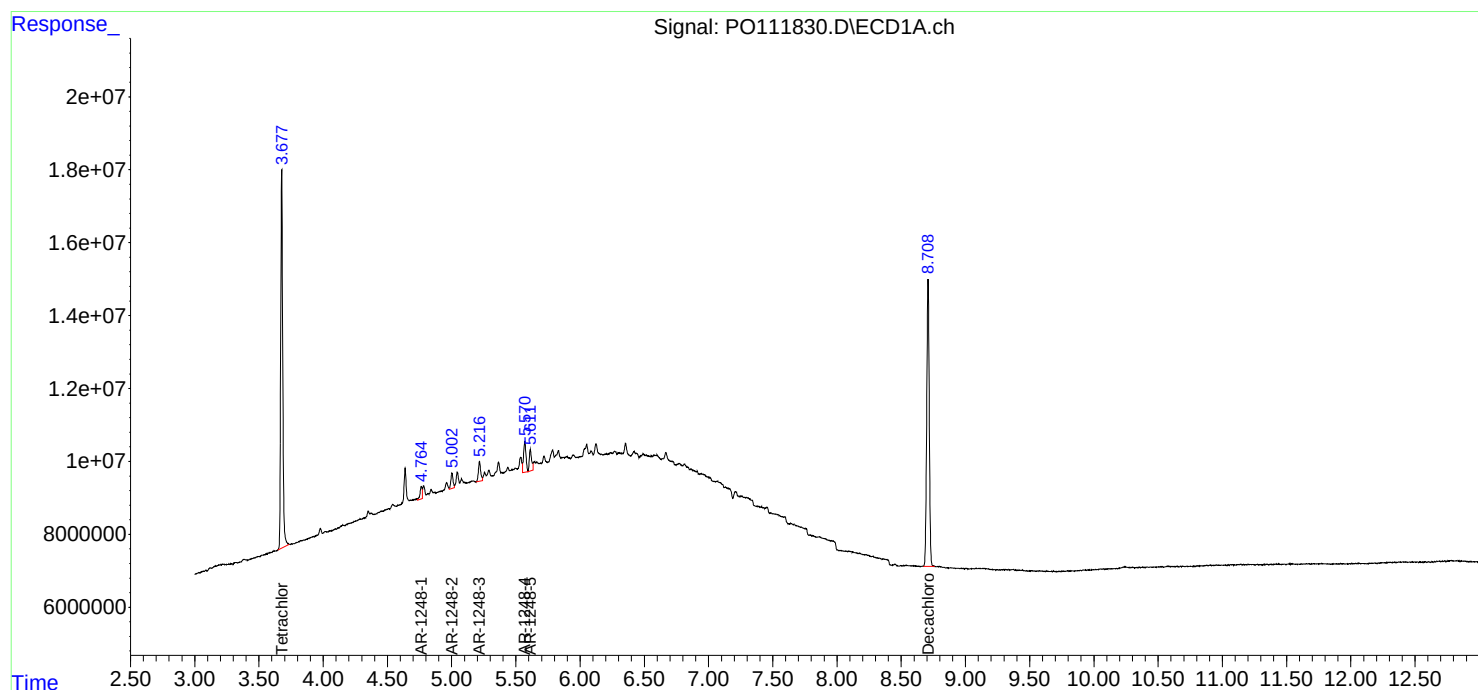


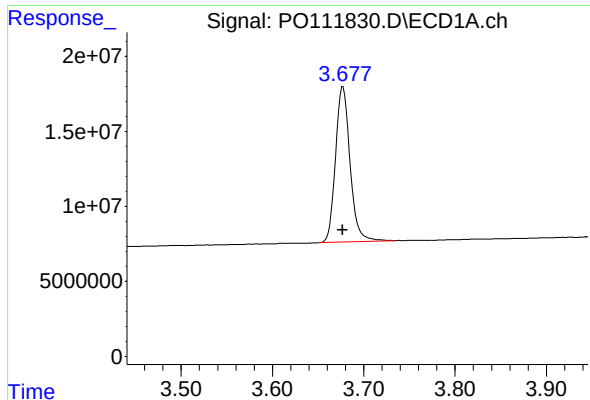

#1 Tetrachloro-m-xylene


R.T.: 3.677 min
Delta R.T.: 0.000 min
Response: 114594324
Conc: 19.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2025

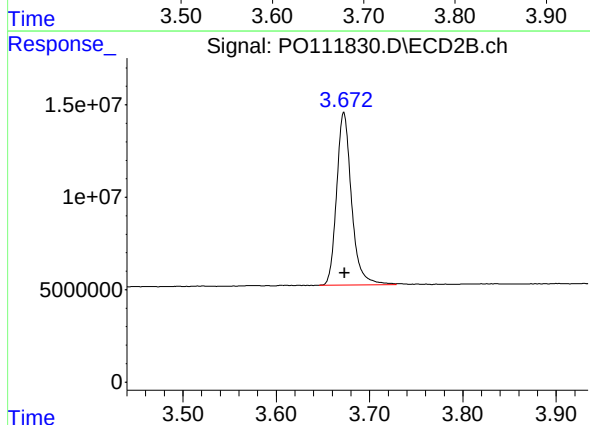


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 103930947
Conc: 18.50 ng/ml

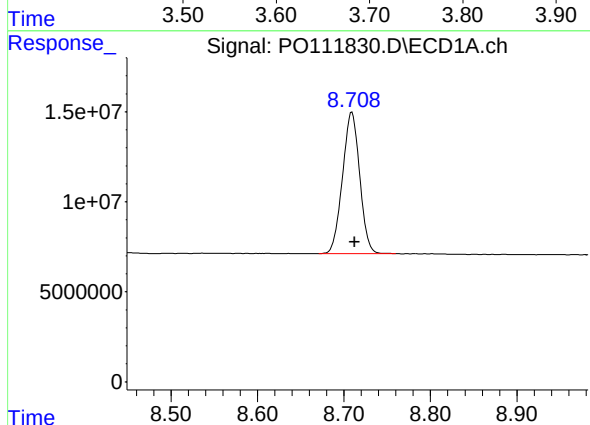


#2 Decachlorobiphenyl

R.T.: 8.709 min
Delta R.T.: -0.003 min
Response: 108311608
Conc: 20.63 ng/ml

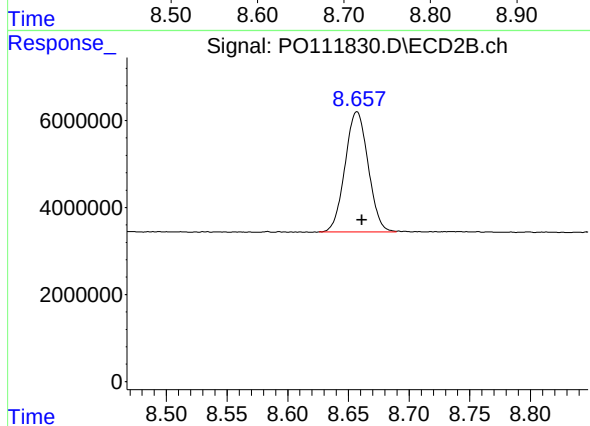

#2 Decachlorobiphenyl


R.T.: 8.657 min
Delta R.T.: -0.004 min
Response: 36555015
Conc: 20.56 ng/ml

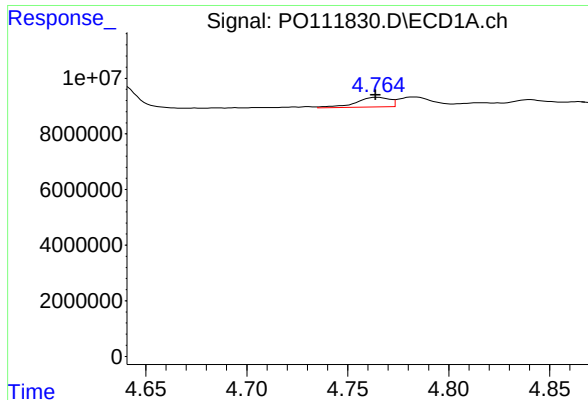

#21 AR-1248-1


R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 4046755
Conc: 25.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2025

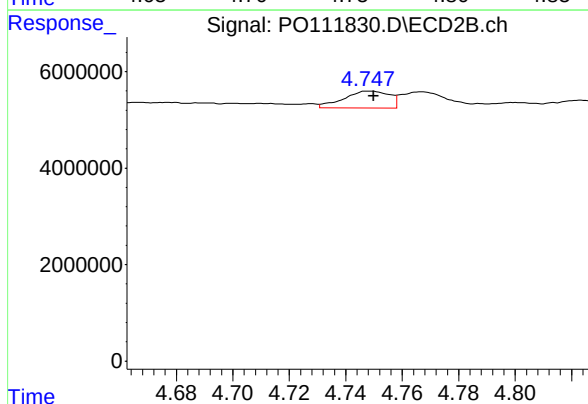


#21 AR-1248-1

R.T.: 4.748 min
Delta R.T.: -0.002 min
Response: 3978274
Conc: 29.85 ng/ml

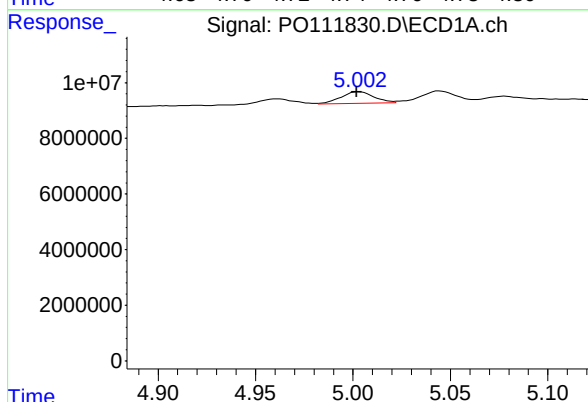


#22 AR-1248-2

R.T.: 5.003 min
Delta R.T.: 0.001 min
Response: 4944627
Conc: 22.93 ng/ml

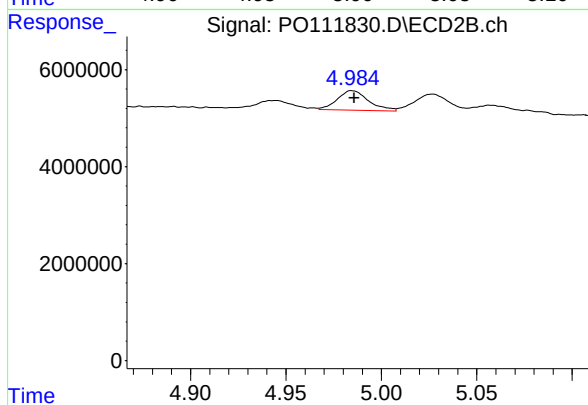

#22 AR-1248-2


R.T.: 4.984 min
Delta R.T.: -0.001 min
Response: 4664553
Conc: 26.18 ng/ml

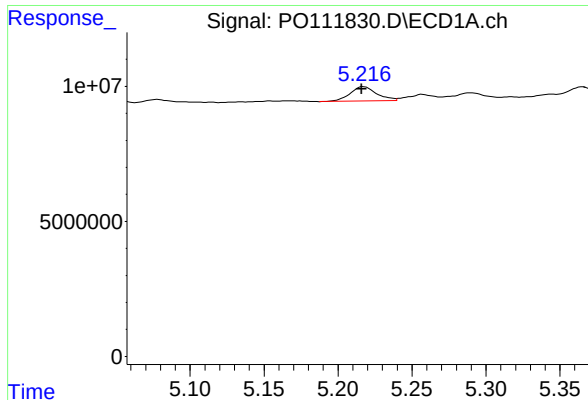

#23 AR-1248-3


R.T.: 5.217 min
Delta R.T.: 0.001 min
Response: 6699791
Conc: 24.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2025

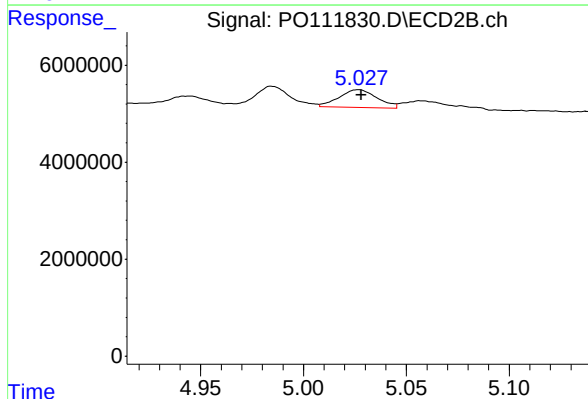


#23 AR-1248-3

R.T.: 5.027 min
Delta R.T.: 0.000 min
Response: 4773962
Conc: 25.20 ng/ml

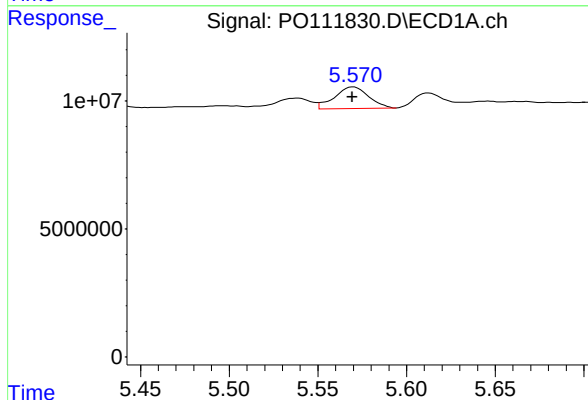


#24 AR-1248-4

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 11335517
Conc: 28.35 ng/ml

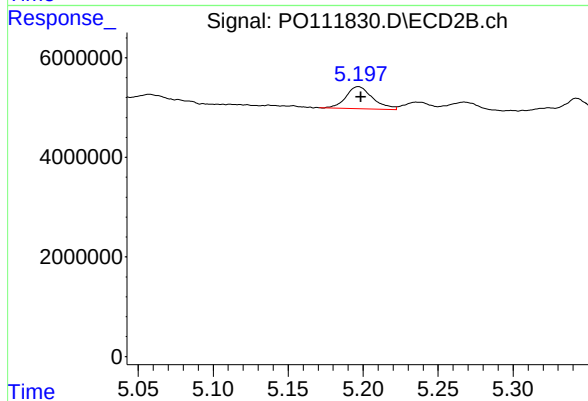

#24 AR-1248-4


R.T.: 5.197 min
Delta R.T.: -0.002 min
Response: 5490600
Conc: 24.05 ng/ml

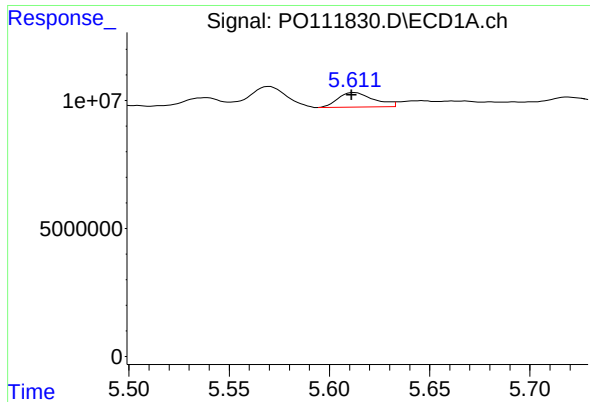

#25 AR-1248-5

R.T.: 5.612 min
Delta R.T.: 0.001 min
Response: 7115506
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2025

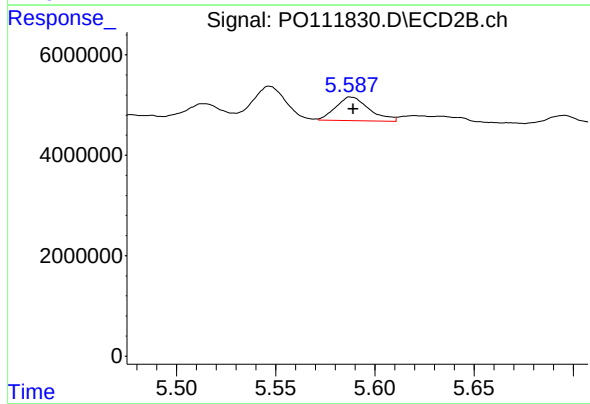

#25 AR-1248-5

R.T.: 5.588 min
Delta R.T.: -0.002 min
Response: 5484536
Conc: 25.19 ng/ml